

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010220\
 Data File : PL055486.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jan 2020 20:38
 Operator : SG\AJ
 Sample : L1001-05
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PAMT-COMP-1-12-31-19

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 02 22:10:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 21 05:21:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.534	4.048	175.1E6	51460821	16.645	19.476
28)	SA Decachlor...	8.313	9.149	143.5E6	34349324	15.464	15.561
Target Compounds							
6)	B beta-BHC	0.000	4.877f	0	1085529	N.D.	0.661 #
10)	B gamma-Chl...	0.000	6.168	0	1847706	N.D.	0.696 #
12)	B 4,4'-DDE	0.000	6.392	0	3240595	N.D.	1.329 #
15)	B Endosulfa...	6.389	6.985f	22248636	10849045	1.896	4.576 #
16)	A 4,4'-DDD	0.000	6.884	0	1233934	N.D.	0.649 #
21)	B Endrin ke...	0.000	7.786	0	2783785	N.D.	1.250 #
25)	Chlordane-3	0.000	6.168	0	1847706	N.D.	5.742 #
27)	Chlordane-5	6.389	0.000	22248636	0	57.096	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010220\
Data File : PL055486.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jan 2020 20:38
Operator : SG\AJ
Sample : L1001-05
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PAMT-COMP-1-12-31-19

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 02 22:10:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
Quant Title : GC Extractables
QLast Update : Sat Dec 21 05:21:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

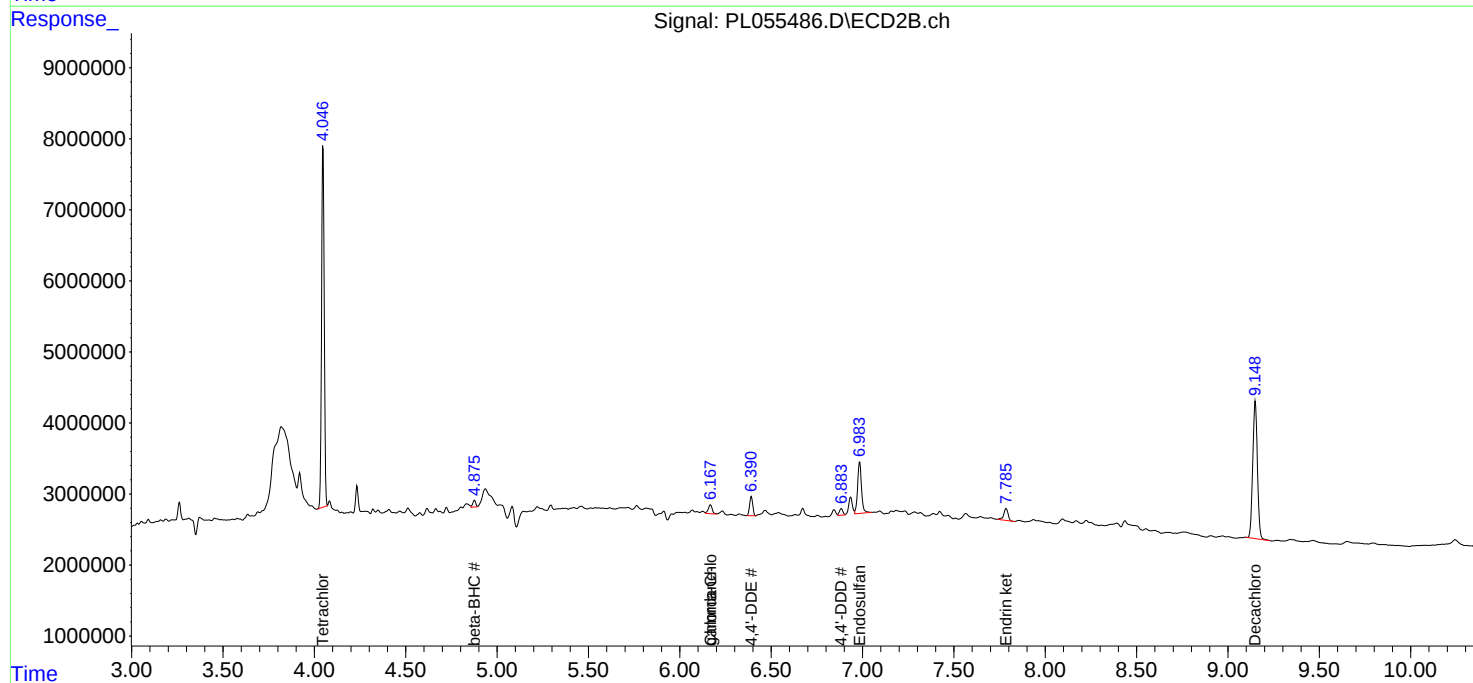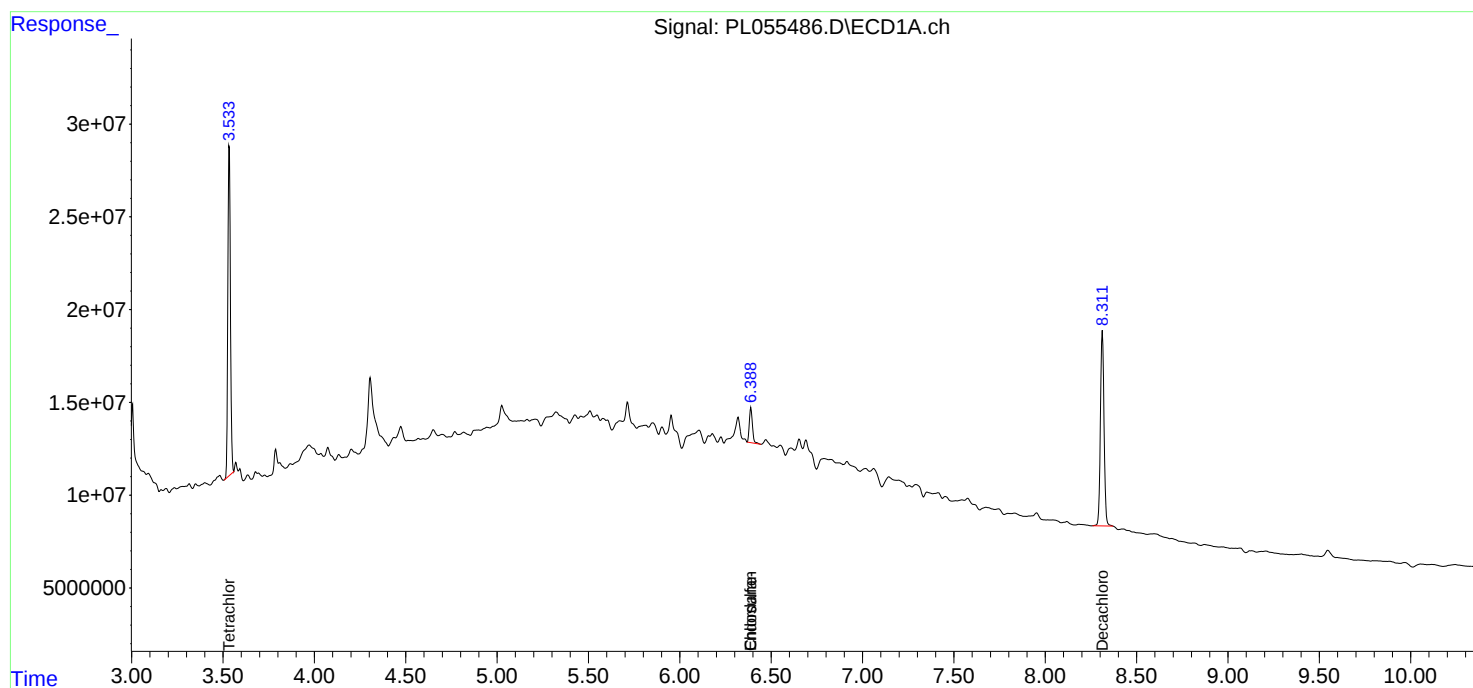


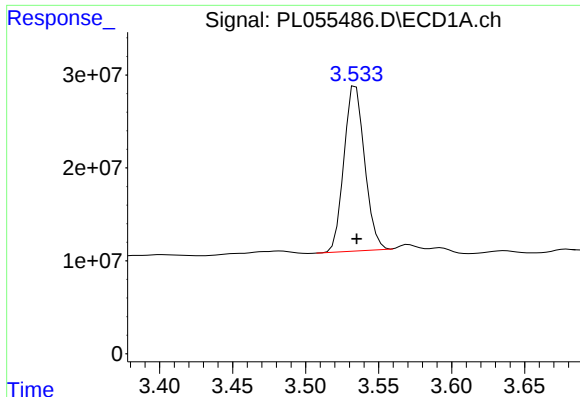

#1 Tetrachloro-m-xylene


R.T.: 3.534 min
Delta R.T.: 0.000 min
Response: 175050709
Conc: 16.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAMT-COMP-1-12-31-19

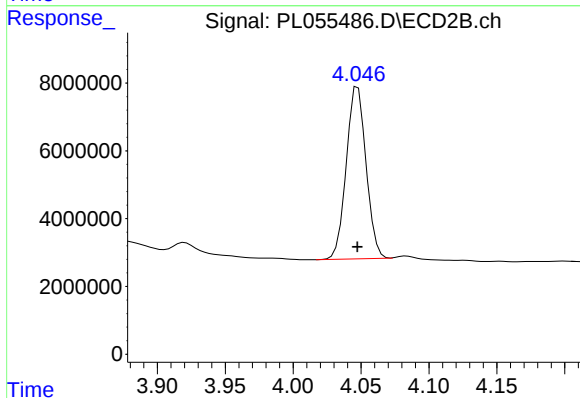


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.000 min
Response: 51460821
Conc: 19.48 ng/ml

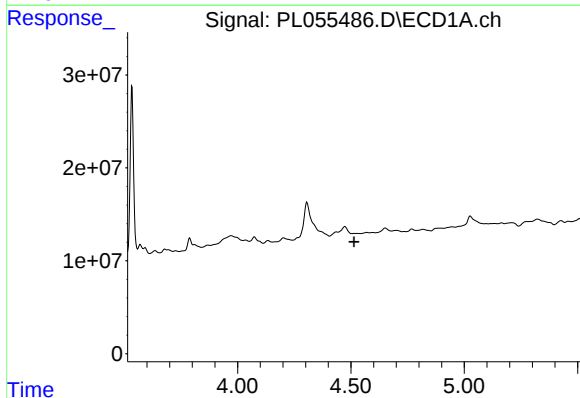


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.514 min
Response: 0
Conc: N.D.

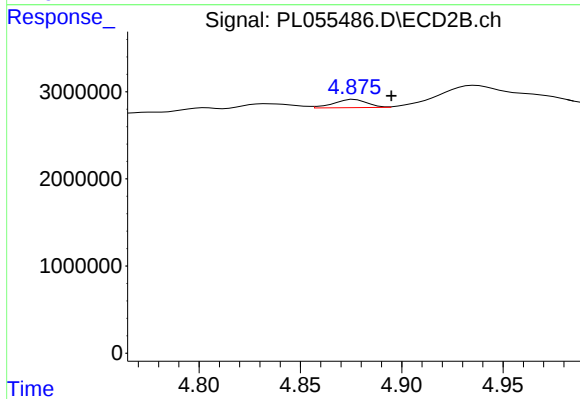

#6 beta-BHC


R.T.: 4.877 min
Delta R.T.: -0.018 min
Response: 1085529
Conc: 0.66 ng/ml

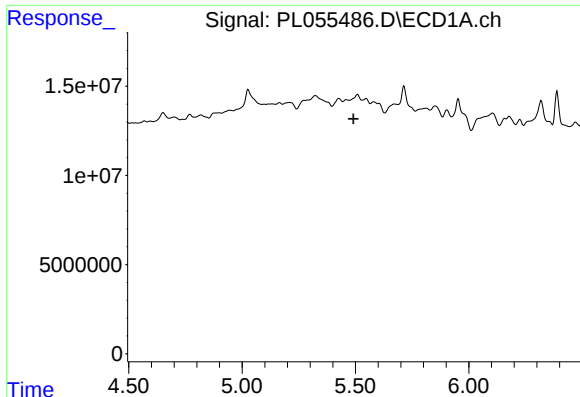

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.492 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PAMT-COMP-1-12-31-19

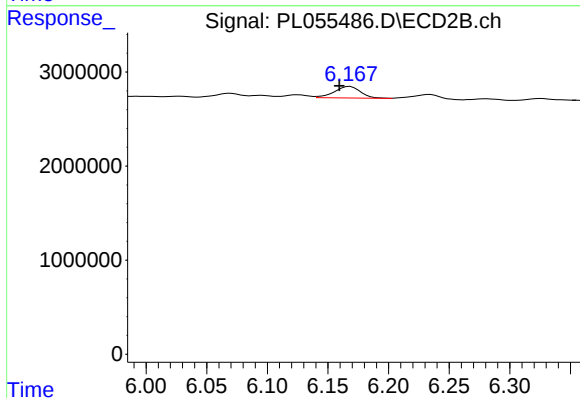


#10 gamma-Chlordane

R.T.: 6.168 min
Delta R.T.: 0.009 min
Response: 1847706
Conc: 0.70 ng/ml

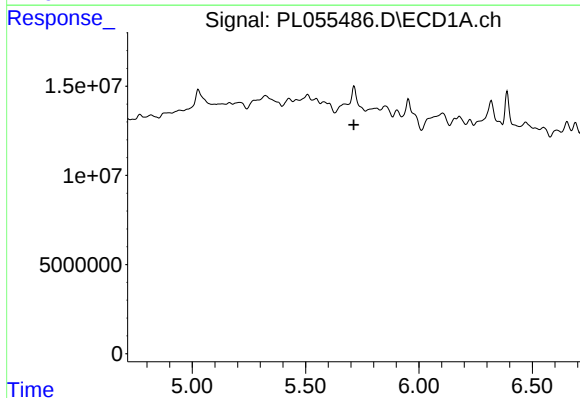


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.713 min
Response: 0
Conc: N.D.

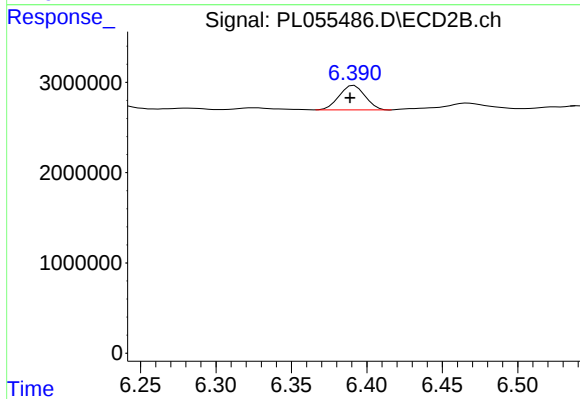

#12 4,4'-DDE


R.T.: 6.392 min
Delta R.T.: 0.003 min
Response: 3240595
Conc: 1.33 ng/ml

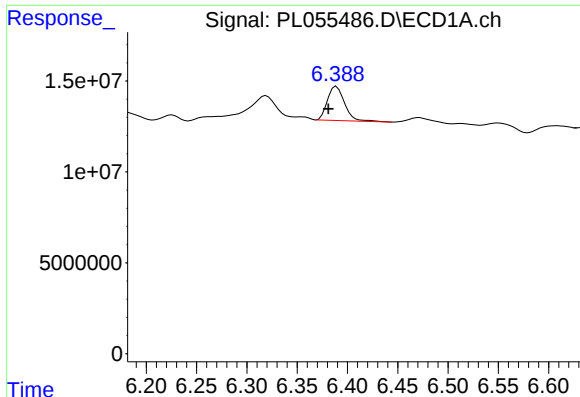

#15 Endosulfan II


R.T.: 6.389 min
Delta R.T.: 0.008 min
Response: 22248636
Conc: 1.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAMT-COMP-1-12-31-19

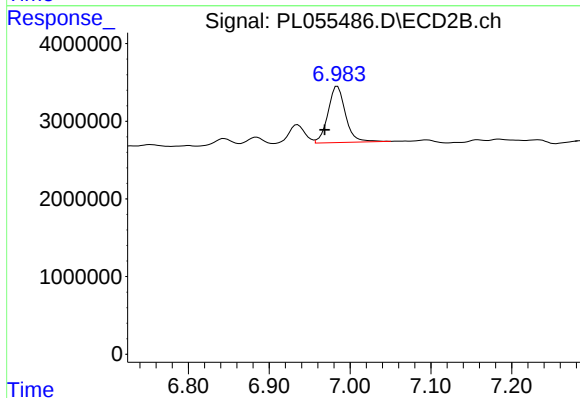


#15 Endosulfan II

R.T.: 6.985 min
Delta R.T.: 0.016 min
Response: 10849045
Conc: 4.58 ng/ml

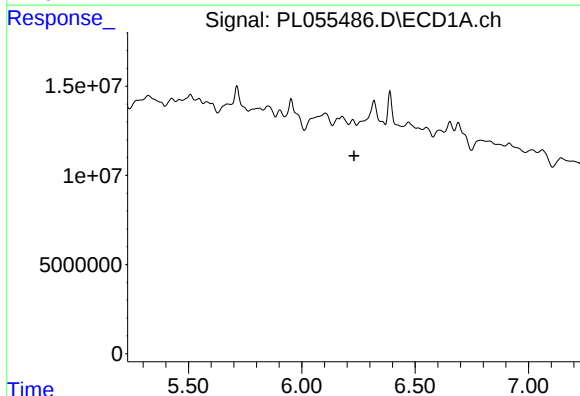


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.231 min
Response: 0
Conc: N.D.

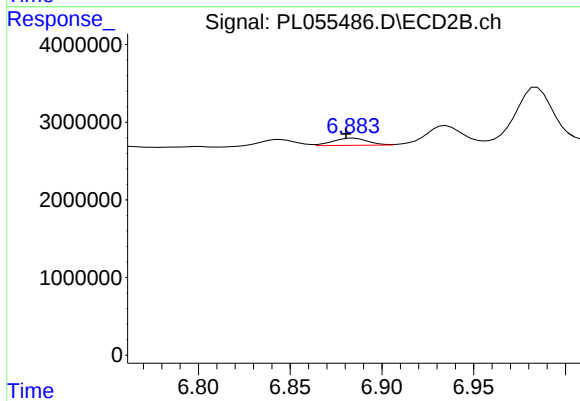

#16 4,4'-DDD


R.T.: 6.884 min
Delta R.T.: 0.004 min
Response: 1233934
Conc: 0.65 ng/ml

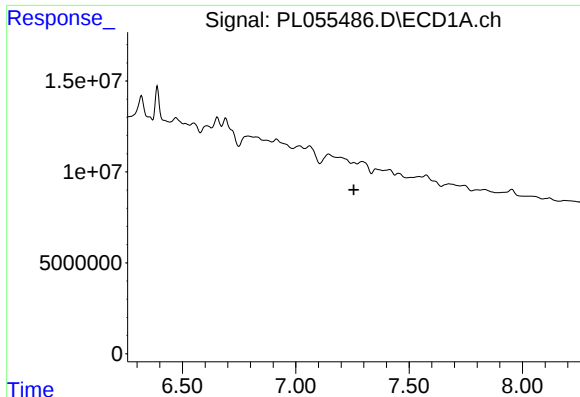

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.256 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PAMT-COMP-1-12-31-19

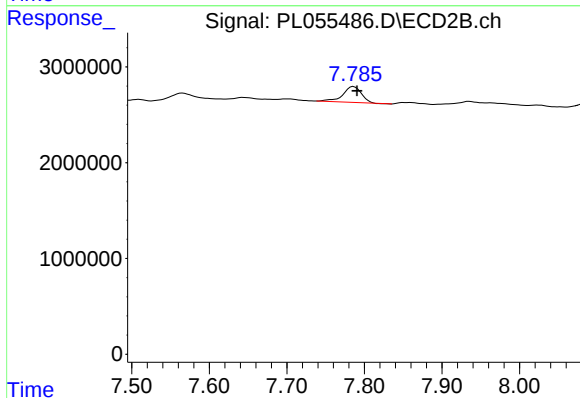


#21 Endrin ketone

R.T.: 7.786 min
Delta R.T.: -0.004 min
Response: 2783785
Conc: 1.25 ng/ml

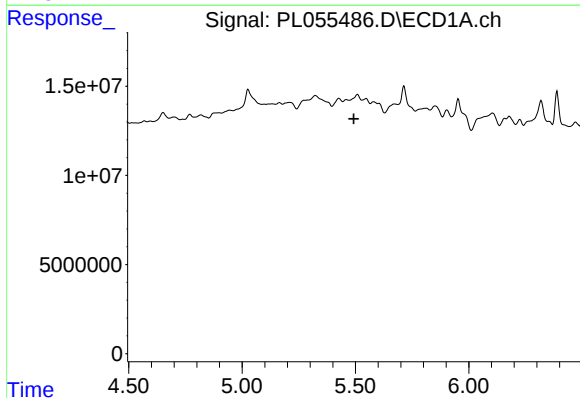


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.492 min
Response: 0
Conc: N.D.

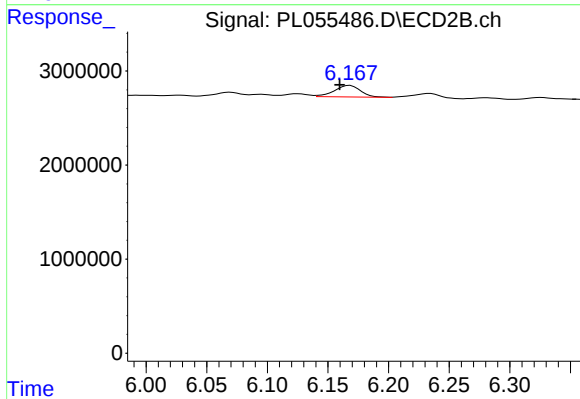

#25 Chlordane-3


R.T.: 6.168 min
Delta R.T.: 0.008 min
Response: 1847706
Conc: 5.74 ng/ml

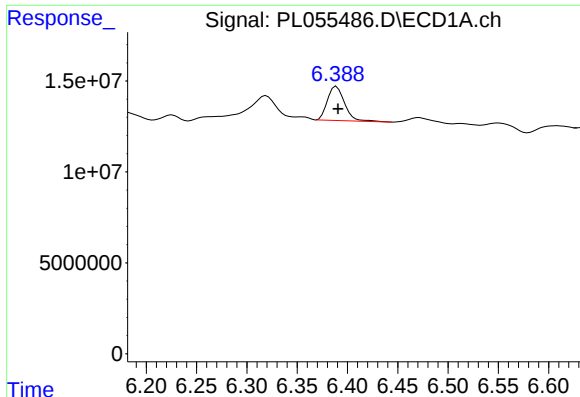

#27 Chlordane-5


R.T.: 6.389 min
Delta R.T.: -0.002 min
Response: 22248636
Conc: 57.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAMT-COMP-1-12-31-19

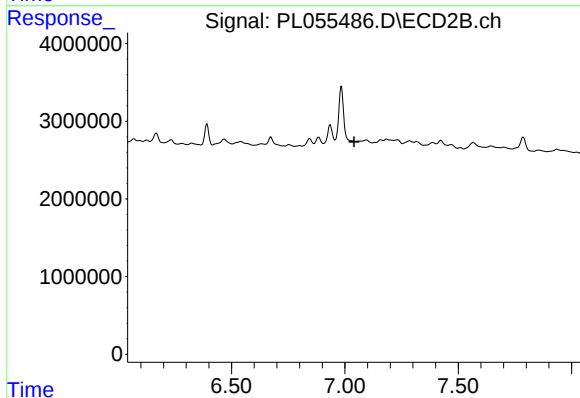


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.041 min
Response: 0
Conc: N.D.

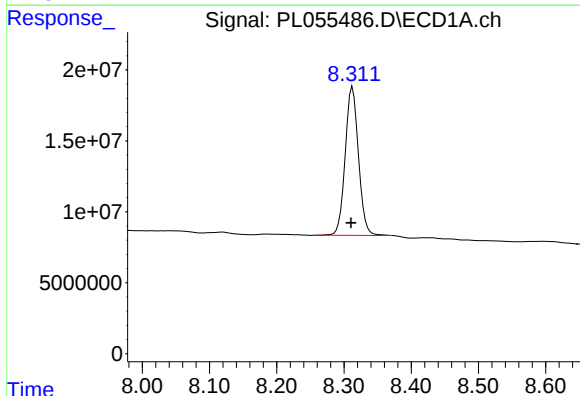

#28 Decachlorobiphenyl

R.T.: 8.313 min
Delta R.T.: 0.002 min
Response: 143488636
Conc: 15.46 ng/ml

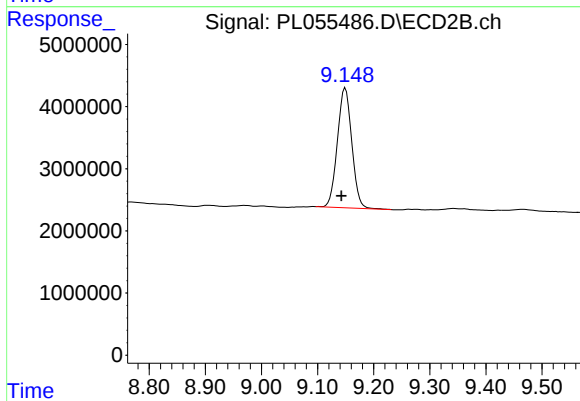

#28 Decachlorobiphenyl

R.T.: 9.149 min
Delta R.T.: 0.007 min
Response: 34349324
Conc: 15.56 ng/ml