

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010220\
 Data File : PL055485.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jan 2020 20:24
 Operator : SG\AJ
 Sample : L1001-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SC-1-12-31-19

Manual Integrations
 APPROVED

mohammad
 1/3/2020 10:18:08 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 02 22:10:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 21 05:21:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.534	4.048	144.4E6	39871893	13.730	15.090
28)	SA Decachlor...	8.313	9.149	94436118	23757592	10.178	10.762
Target Compounds							
12)	B 4,4'-DDE	5.713	6.391	13110887	2629800	0.984m	1.079

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010220\
Data File : PL055485.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jan 2020 20:24
Operator : SG\AJ
Sample : L1001-04
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
SC-1-12-31-19


Manual Integrations
APPROVED

mohammad
1/3/2020 10:18:08 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 02 22:10:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122119.M
Quant Title : GC Extractables
QLast Update : Sat Dec 21 05:21:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

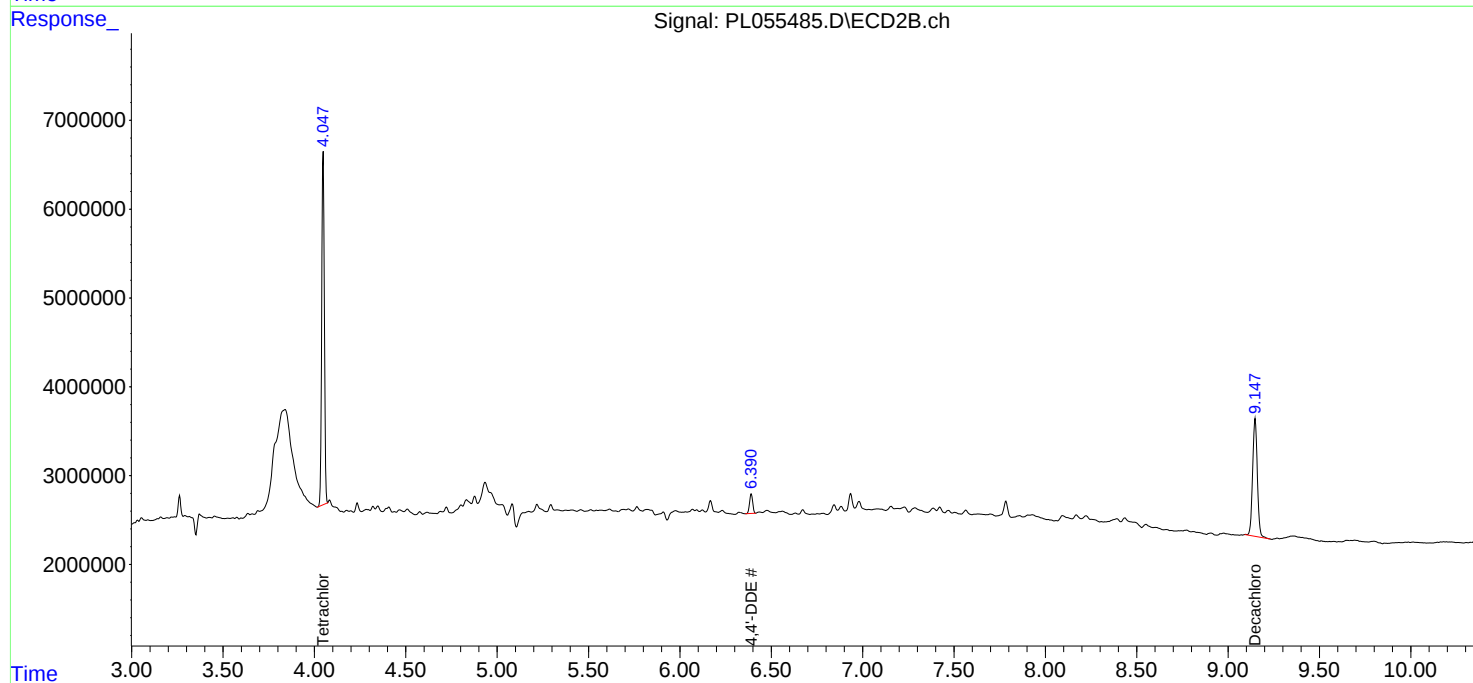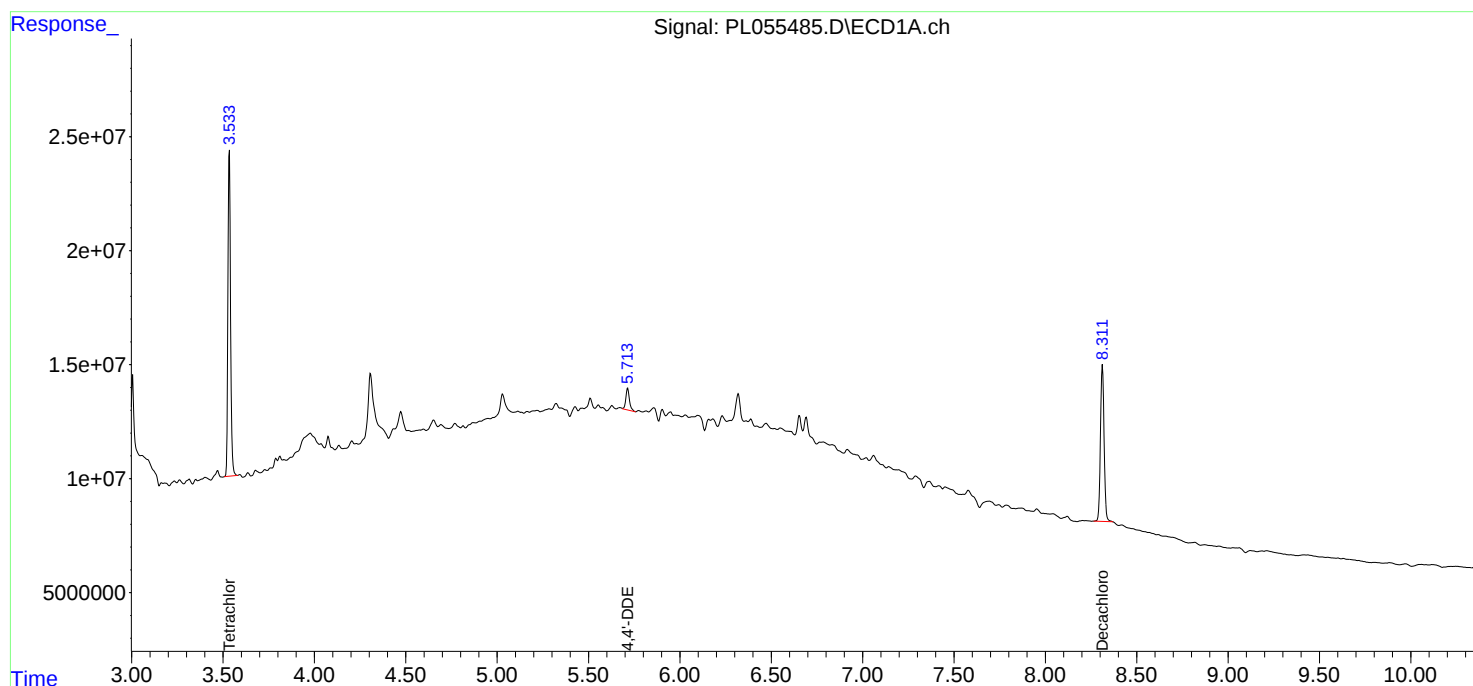

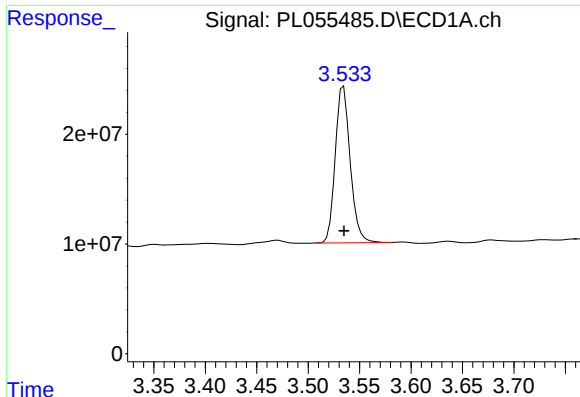


#1 Tetrachloro-m-xylene

R.T.: 3.534 min
Delta R.T.: 0.000 min
Response: 144392439
Conc: 13.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
SC-1-12-31-19


Manual Integrations
APPROVED

mohammad
1/3/2020 10:18:08 AM

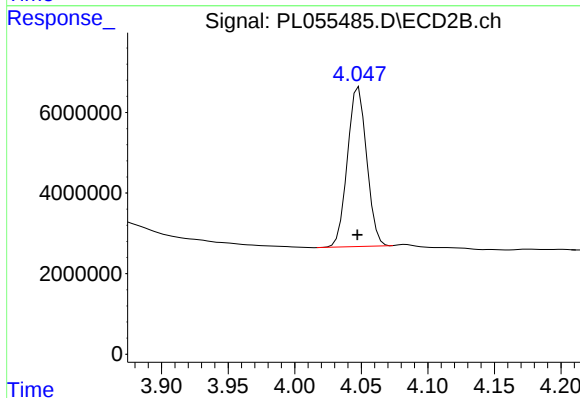


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.000 min
Response: 39871893
Conc: 15.09 ng/ml

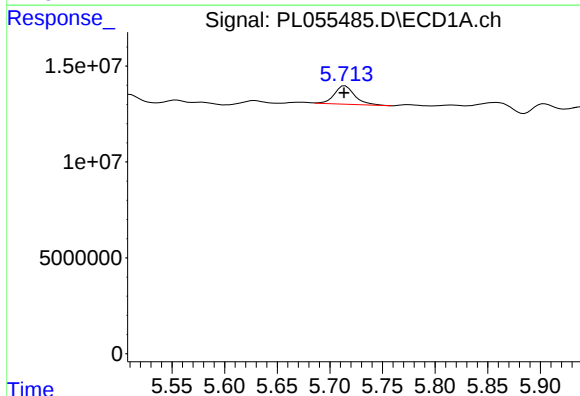


#12 4,4'-DDE

R.T.: 5.713 min
Delta R.T.: 0.000 min
Response: 13110887
Conc: 0.98 ng/ml m

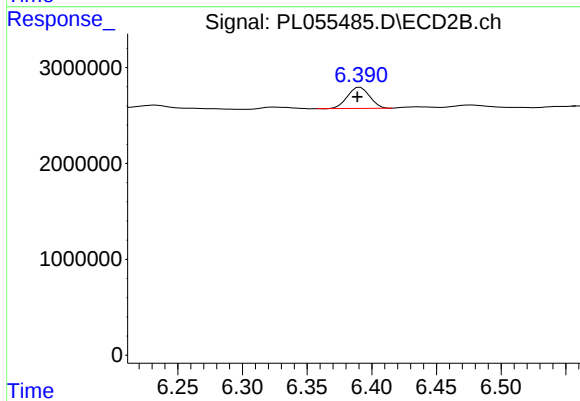

#12 4,4'-DDE

R.T.: 6.391 min
Delta R.T.: 0.002 min
Response: 2629800
Conc: 1.08 ng/ml

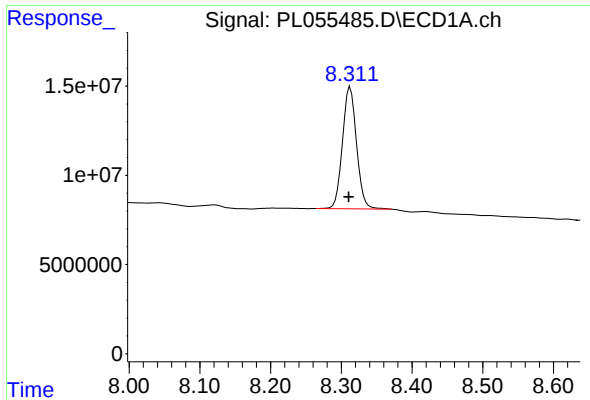


#28 Decachlorobiphenyl

R.T.: 8.313 min
Delta R.T.: 0.002 min
Response: 94436118
Conc: 10.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
SC-1-12-31-19

Manual Integrations
APPROVED

mohammad
1/3/2020 10:18:08 AM

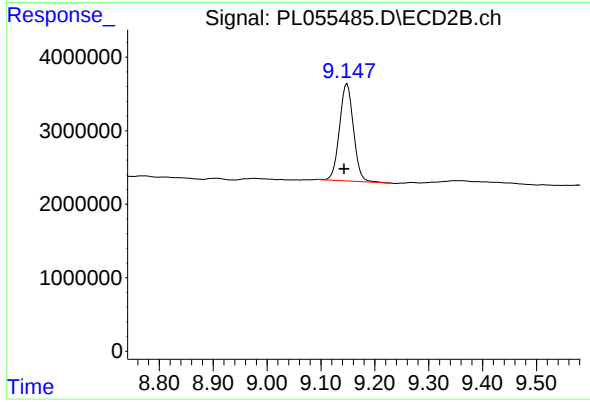

#28 Decachlorobiphenyl

R.T.: 9.149 min
Delta R.T.: 0.006 min
Response: 23757592
Conc: 10.76 ng/ml