

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010319\
 Data File : PL043556.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jan 2019 16:29
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 06:45:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 04 06:12:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.463	4.100	128.6E6	61328959	20.126	20.990
28)	SA Decachlor...	8.199	9.229	97087975	48259966	19.266	21.831
Target Compounds							
6)	B beta-BHC	4.393f	0.000	2341947	0	0.640	N.D. #
7)	B delta-BHC	0.000	5.164	0	11528058	N.D.	2.726 #
8)	B Heptachlo...	5.107f	5.996	1907239	19100181	0.248	5.225 #
23)	Chlordane-1	4.360	5.164	893740	11528058	3.320	86.175 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010319\
Data File : PL043556.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jan 2019 16:29
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 06:45:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
Quant Title : GC Extractables
QLast Update : Fri Jan 04 06:12:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

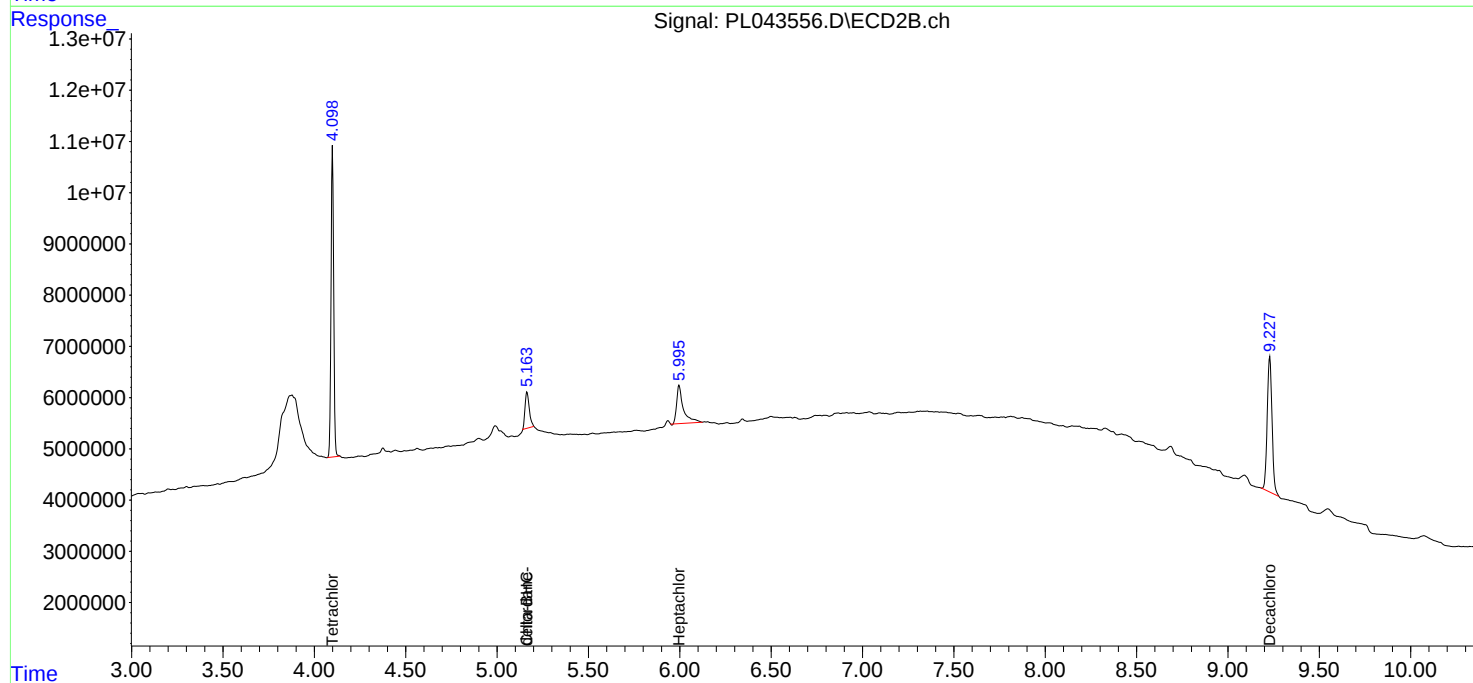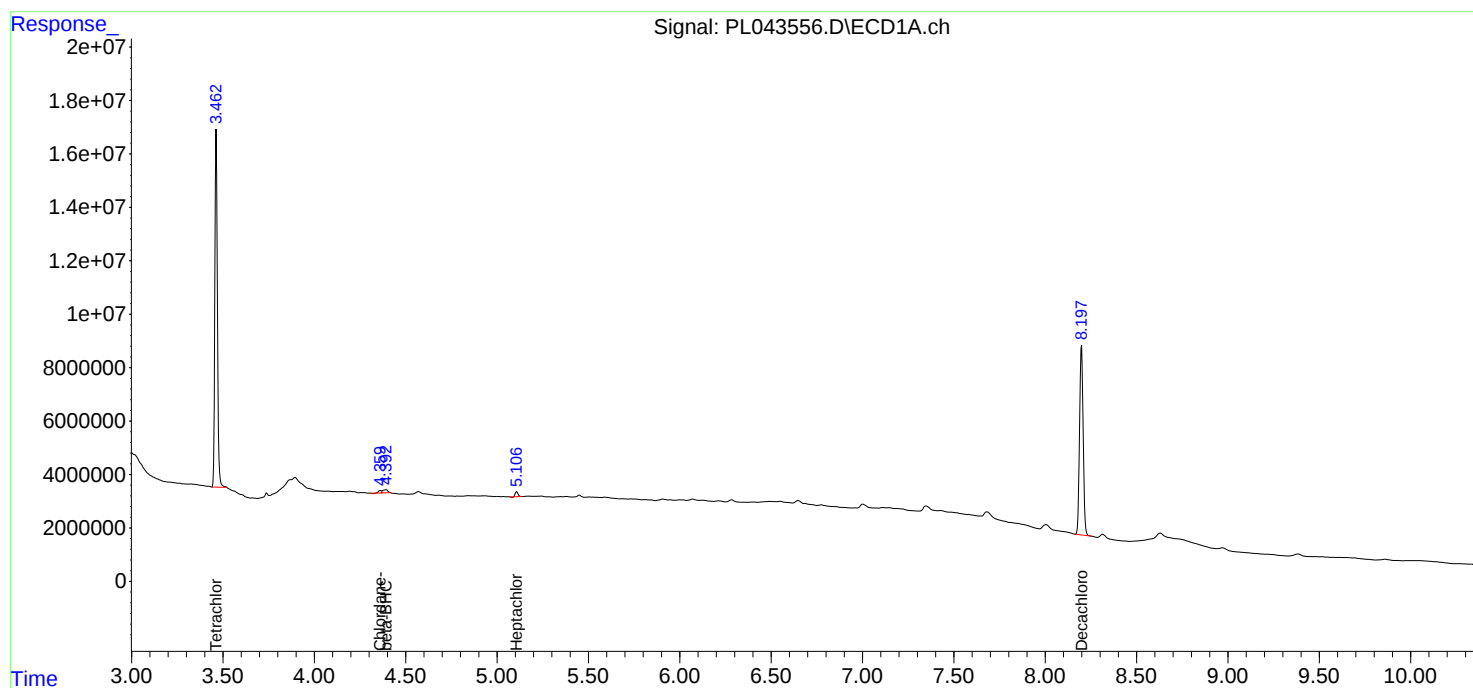


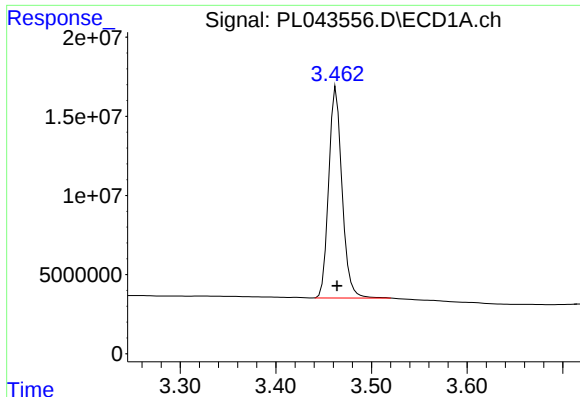

#1 Tetrachloro-m-xylene


R.T.: 3.463 min
Delta R.T.: 0.000 min
Response: 128590082
Conc: 20.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

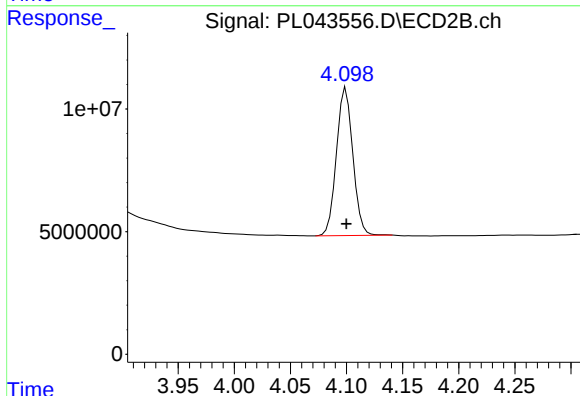


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: 0.000 min
Response: 61328959
Conc: 20.99 ng/ml

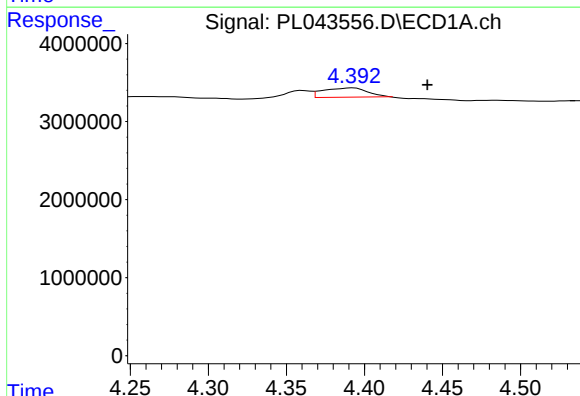


#6 beta-BHC

R.T.: 4.393 min
Delta R.T.: -0.047 min
Response: 2341947
Conc: 0.64 ng/ml

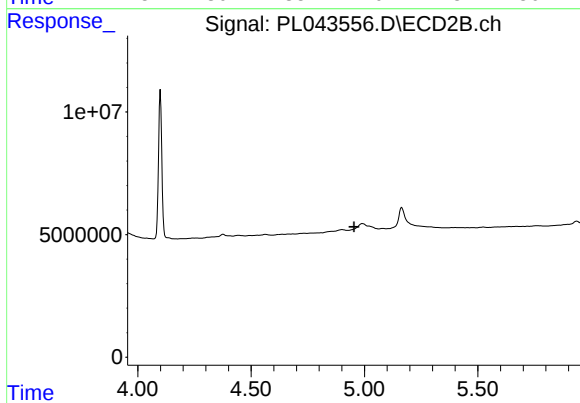

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

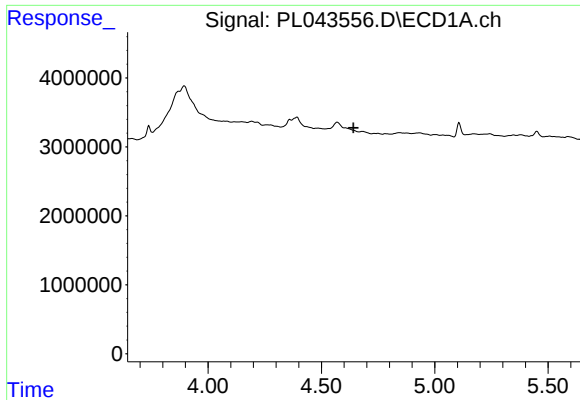

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.642 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

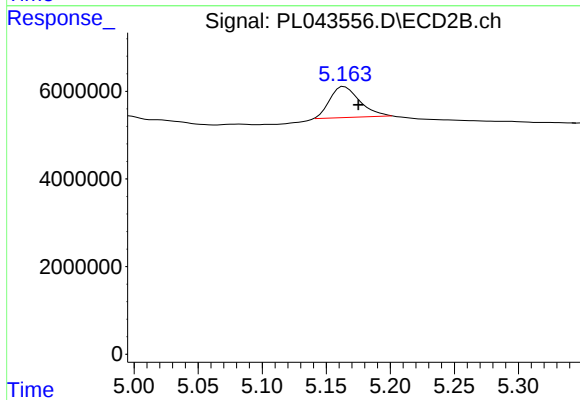


#7 delta-BHC

R.T.: 5.164 min
Delta R.T.: -0.011 min
Response: 11528058
Conc: 2.73 ng/ml

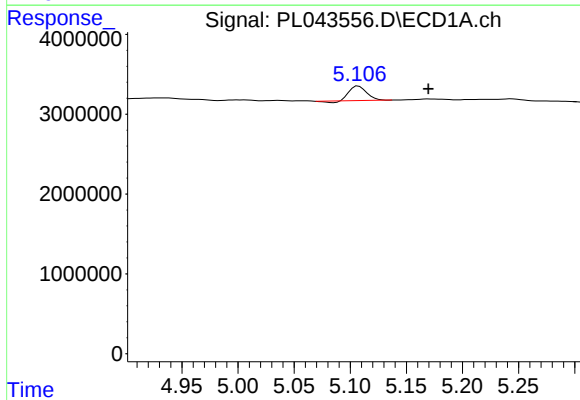


#8 Heptachlor epoxide

R.T.: 5.107 min
Delta R.T.: -0.062 min
Response: 1907239
Conc: 0.25 ng/ml

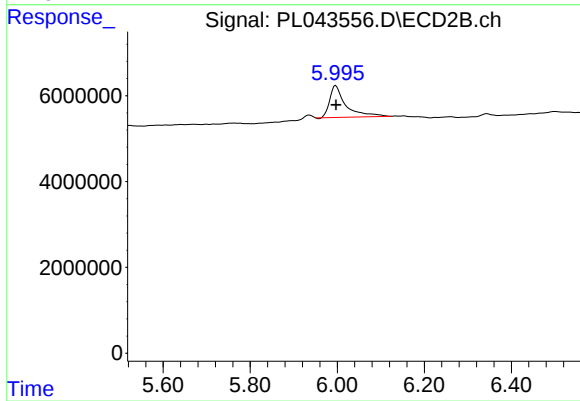

#8 Heptachlor epoxide


R.T.: 5.996 min
Delta R.T.: 0.000 min
Response: 19100181
Conc: 5.22 ng/ml

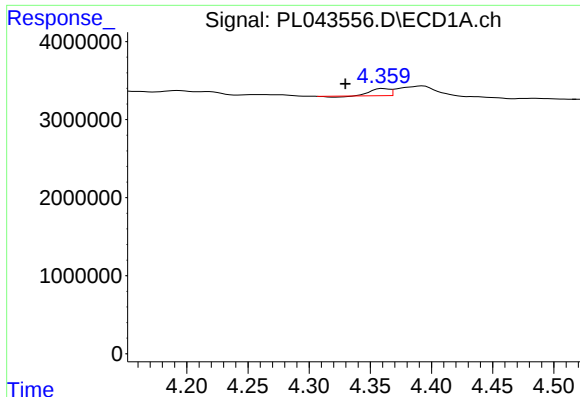

#23 Chlordane-1


R.T.: 4.360 min
Delta R.T.: 0.030 min
Response: 893740
Conc: 3.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

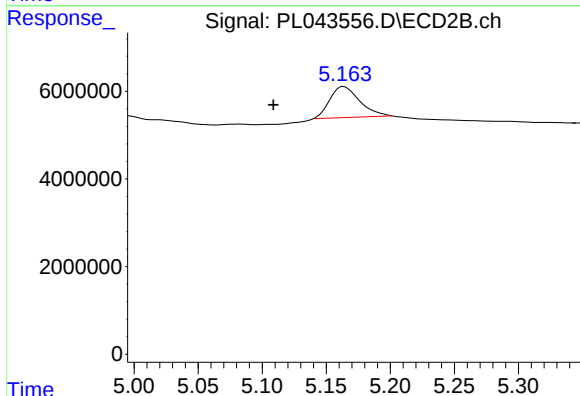


#23 Chlordane-1

R.T.: 5.164 min
Delta R.T.: 0.055 min
Response: 11528058
Conc: 86.18 ng/ml

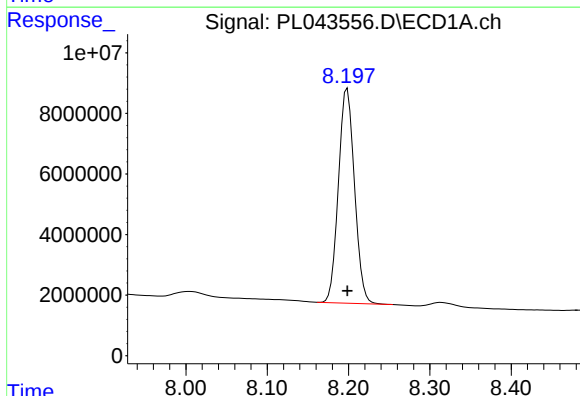

#28 Decachlorobiphenyl

R.T.: 8.199 min
Delta R.T.: 0.000 min
Response: 97087975
Conc: 19.27 ng/ml

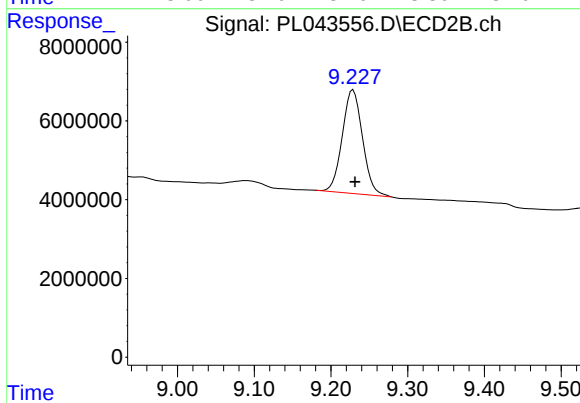

#28 Decachlorobiphenyl

R.T.: 9.229 min
Delta R.T.: -0.002 min
Response: 48259966
Conc: 21.83 ng/ml