

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010319\
 Data File : PL043581.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jan 2019 22:22
 Operator : AJ\SJ
 Sample : K1002-04
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 07:02:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 04 06:12:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.463	4.100	123.8E6	59565118	19.371	20.386
28)	SA Decachlor...	8.198	9.231	111.0E6	44561082	22.020	20.158
Target Compounds							
2)	A alpha-BHC	3.859f	0.000	353984	0	0.037	N.D. #
6)	B beta-BHC	4.396f	0.000	12423309	0	3.395	N.D. #
7)	B delta-BHC	0.000	5.162	0	14402972	N.D.	3.406 #
8)	B Heptachlo...	0.000	5.996	0	28463291	N.D.	7.786 #
14)	MA Endrin	5.993	0.000	3851840	0	0.631	N.D. #
15)	B Endosulfa...	6.284	0.000	2198426	0	0.376	N.D. #
19)	B Endosulfa...	0.000	7.458f	0	2039959	N.D.	0.812 #
23)	Chlordane-1	4.396	5.162	12423309	14402972	46.154	107.666 #
27)	Chlordane-5	6.284	0.000	2198426	0	10.367	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010319\
Data File : PL043581.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jan 2019 22:22
Operator : AJ\SJ
Sample : K1002-04
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 07:02:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
Quant Title : GC Extractables
QLast Update : Fri Jan 04 06:12:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

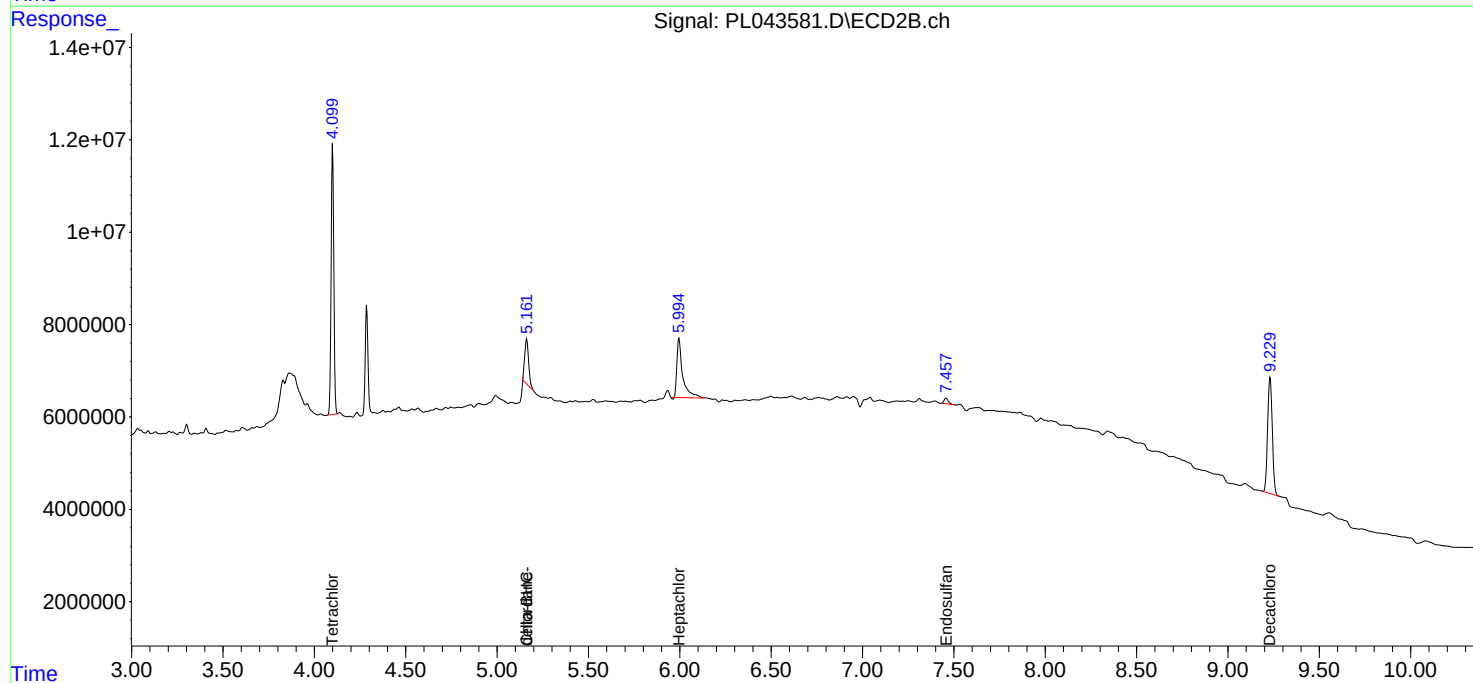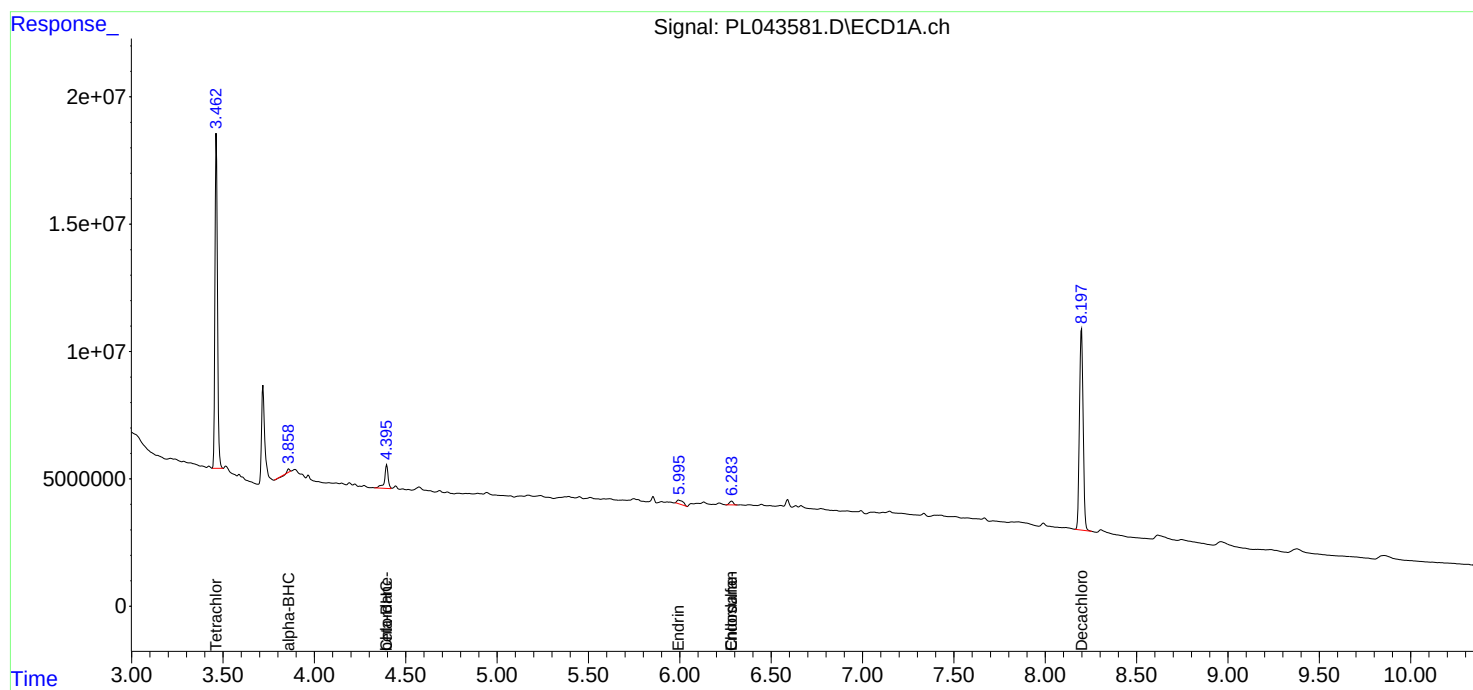


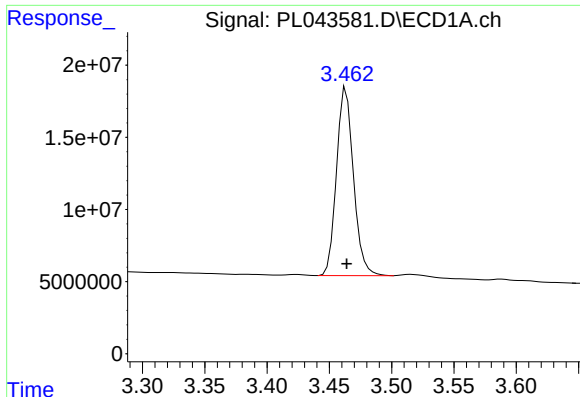

#1 Tetrachloro-m-xylene


R.T.: 3.463 min
Delta R.T.: 0.000 min
Response: 123761833
Conc: 19.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

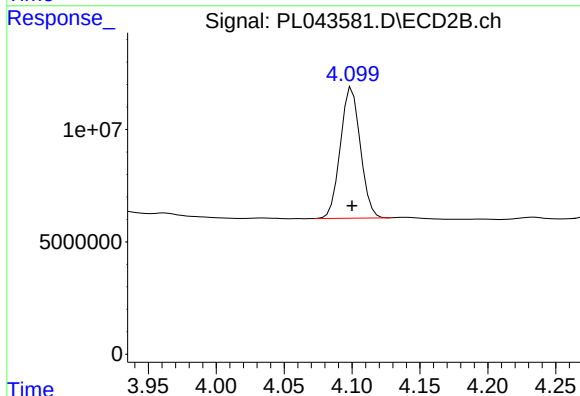


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: 0.000 min
Response: 59565118
Conc: 20.39 ng/ml

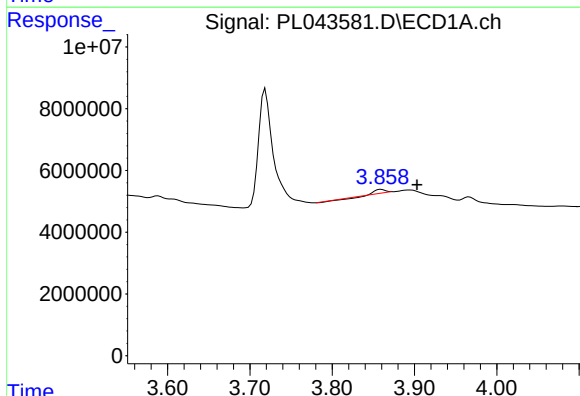


#2 alpha-BHC

R.T.: 3.859 min
Delta R.T.: -0.044 min
Response: 353984
Conc: 0.04 ng/ml

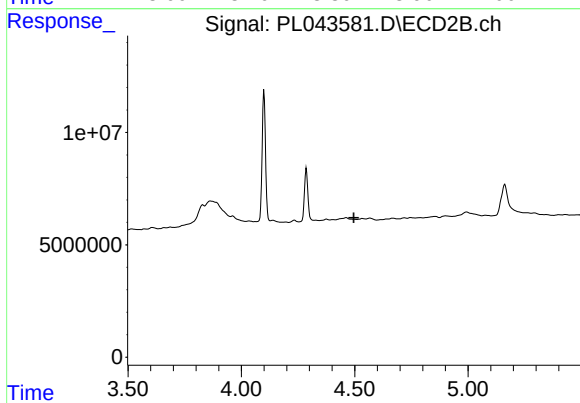

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.496 min
Response: 0
Conc: N.D.

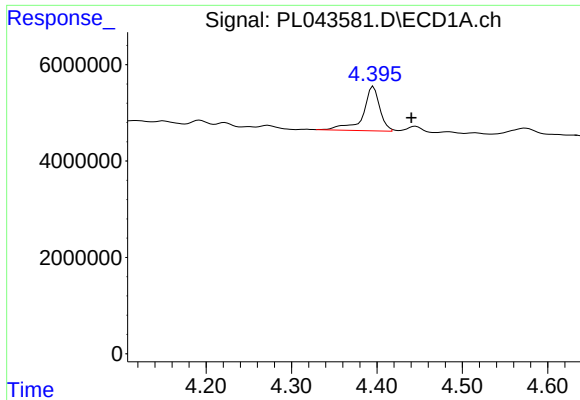

#6 beta-BHC


R.T.: 4.396 min
Delta R.T.: -0.044 min
Response: 12423309
Conc: 3.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

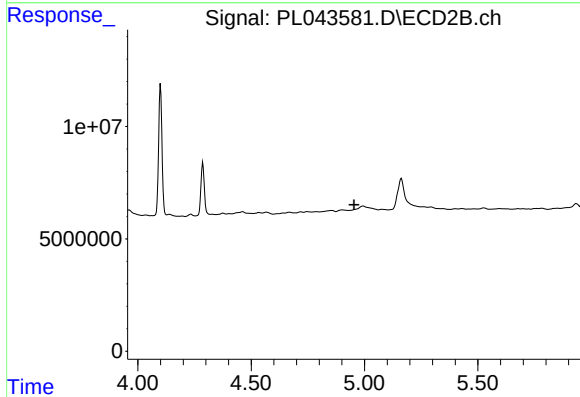


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

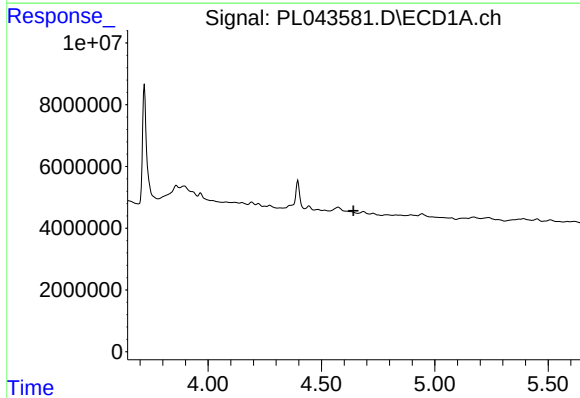


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.642 min
Response: 0
Conc: N.D.

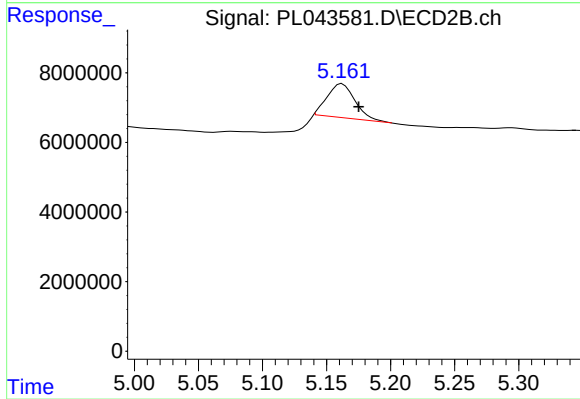

#7 delta-BHC


R.T.: 5.162 min
Delta R.T.: -0.013 min
Response: 14402972
Conc: 3.41 ng/ml

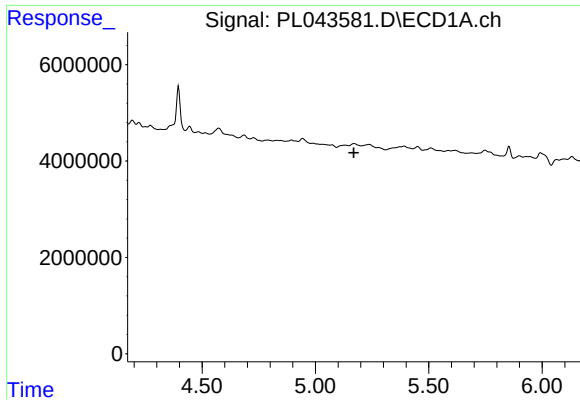

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.170 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

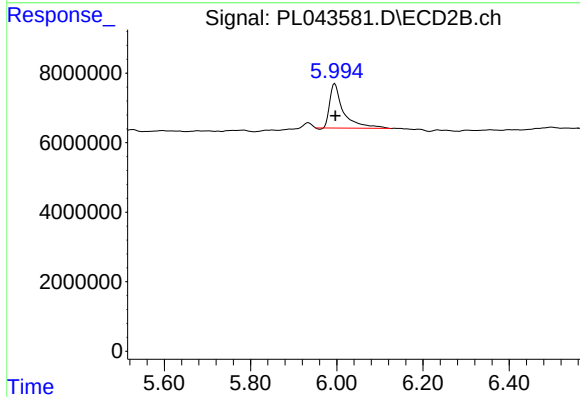


#8 Heptachlor epoxide

R.T.: 5.996 min
Delta R.T.: -0.001 min
Response: 28463291
Conc: 7.79 ng/ml

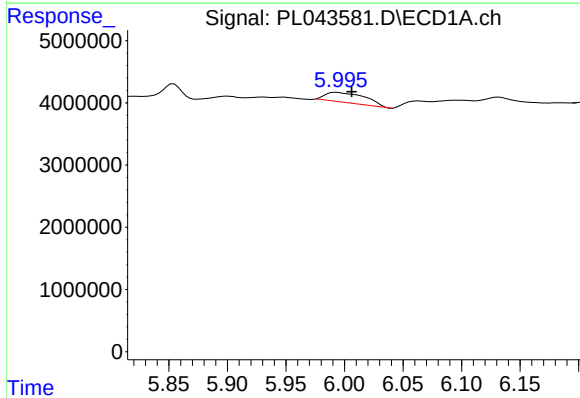


#14 Endrin

R.T.: 5.993 min
Delta R.T.: -0.013 min
Response: 3851840
Conc: 0.63 ng/ml

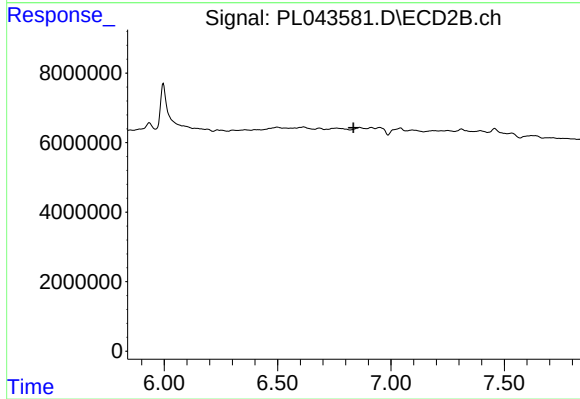

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.835 min
Response: 0
Conc: N.D.

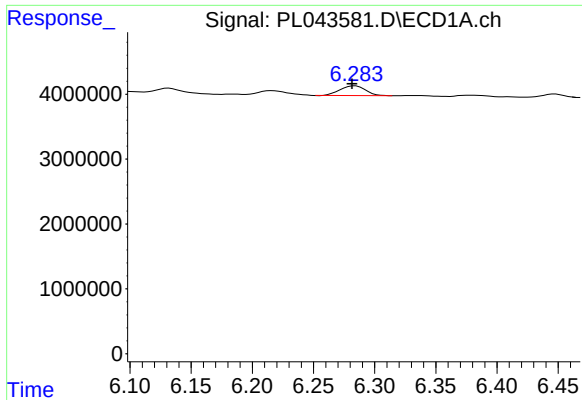

#15 Endosulfan II


R.T.: 6.284 min
Delta R.T.: 0.003 min
Response: 2198426
Conc: 0.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

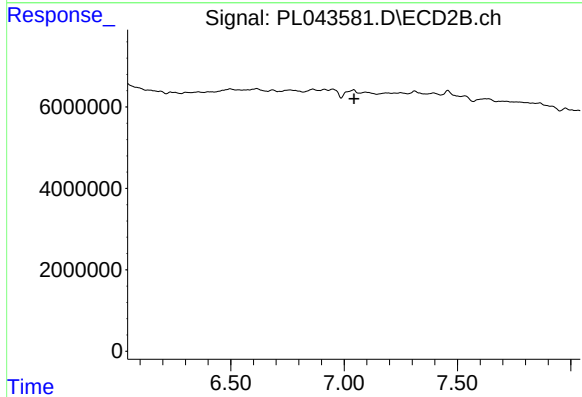


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.044 min
Response: 0
Conc: N.D.

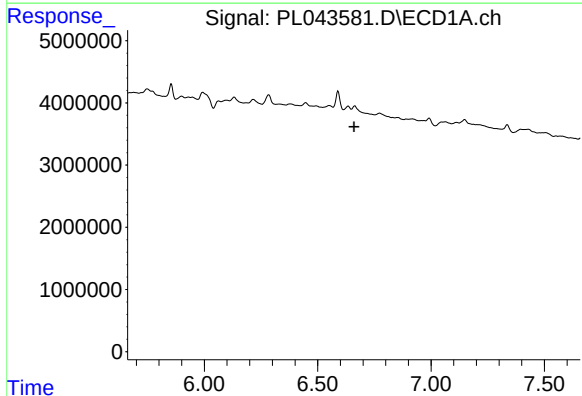


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.661 min
Response: 0
Conc: N.D.

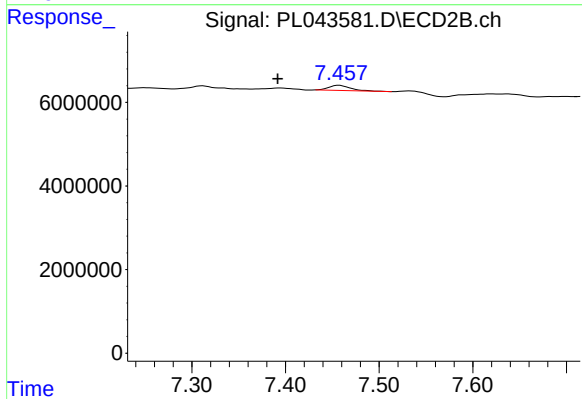

#19 Endosulfan Sulfate


R.T.: 7.458 min
Delta R.T.: 0.066 min
Response: 2039959
Conc: 0.81 ng/ml

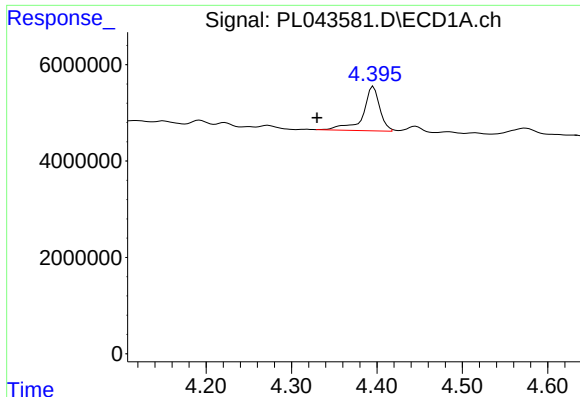

#23 Chlordane-1


R.T.: 4.396 min
Delta R.T.: 0.066 min
Response: 12423309
Conc: 46.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

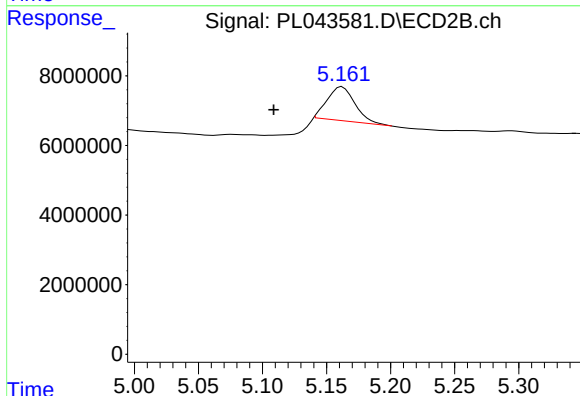


#23 Chlordane-1

R.T.: 5.162 min
Delta R.T.: 0.053 min
Response: 14402972
Conc: 107.67 ng/ml

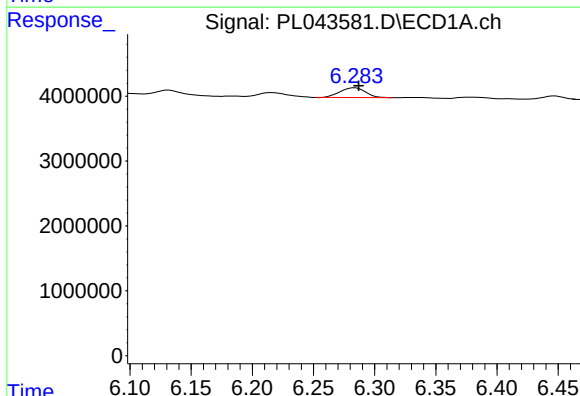


#27 Chlordane-5

R.T.: 6.284 min
Delta R.T.: -0.003 min
Response: 2198426
Conc: 10.37 ng/ml

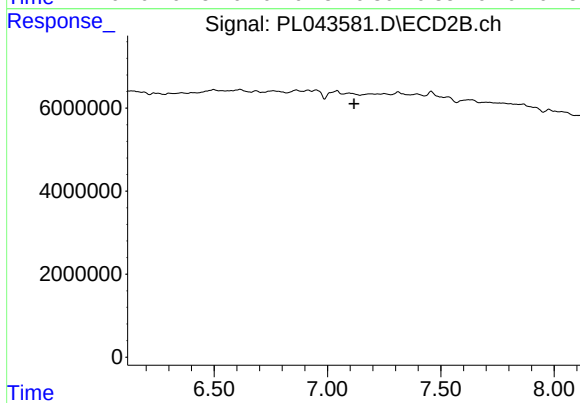

#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

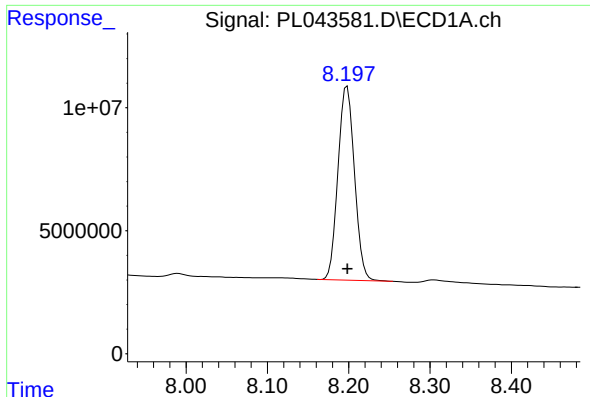

#28 Decachlorobiphenyl


R.T.: 8.198 min

Delta R.T.: 0.000 min

Response: 110964632

Conc: 22.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

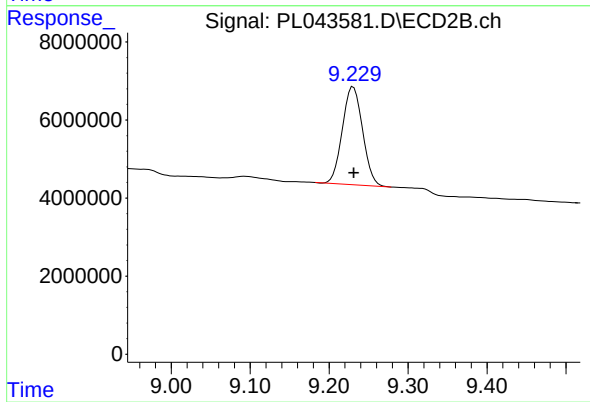

#28 Decachlorobiphenyl

R.T.: 9.231 min

Delta R.T.: 0.000 min

Response: 44561082

Conc: 20.16 ng/ml