

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010319\
 Data File : PL043589.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2019 00:15
 Operator : AJ\SJ
 Sample : K1017-20
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 07:05:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 04 06:12:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.463	4.101	118.5E6	58983099	18.550	20.187
28)	SA Decachlor...	8.198	9.230	87224743	29755827	17.309	13.460
Target Compounds							
2)	A alpha-BHC	3.900	0.000	4332403	0	0.448	N.D. #
6)	B beta-BHC	4.396f	0.000	13063922	0	3.570	N.D. #
8)	B Heptachlo...	0.000	5.999	0	7812410	N.D.	2.137 #
10)	B gamma-Chl...	5.418	0.000	1609771	0	0.205	N.D. #
11)	B alpha-Chl...	5.418	0.000	1609771	0	0.209	N.D. #
23)	Chlordane-1	4.396	0.000	13063922	0	48.533	N.D. #
25)	Chlordane-3	5.418	0.000	1609771	0	1.912	N.D. #
26)	Chlordane-4	5.418	0.000	1609771	0	2.162	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010319\
Data File : PL043589.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2019 00:15
Operator : AJ\SJ
Sample : K1017-20
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 07:05:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
Quant Title : GC Extractables
QLast Update : Fri Jan 04 06:12:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

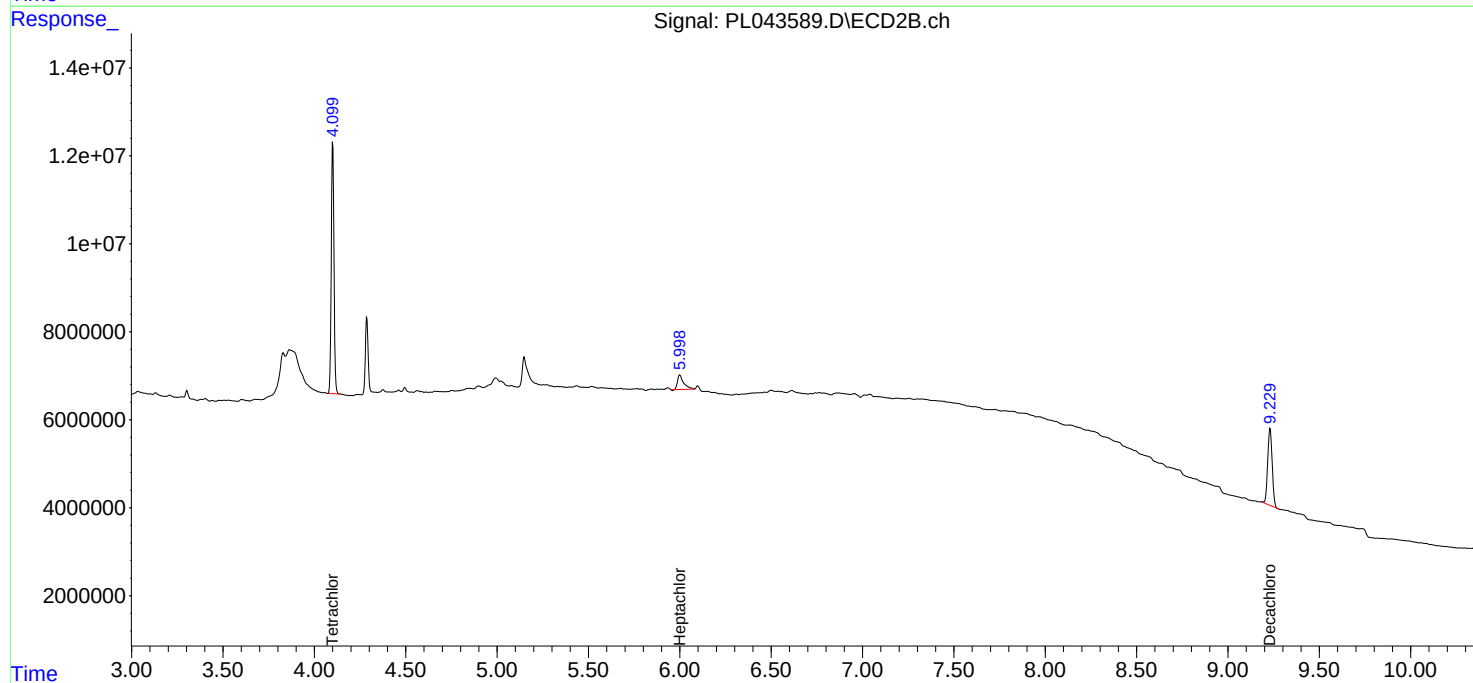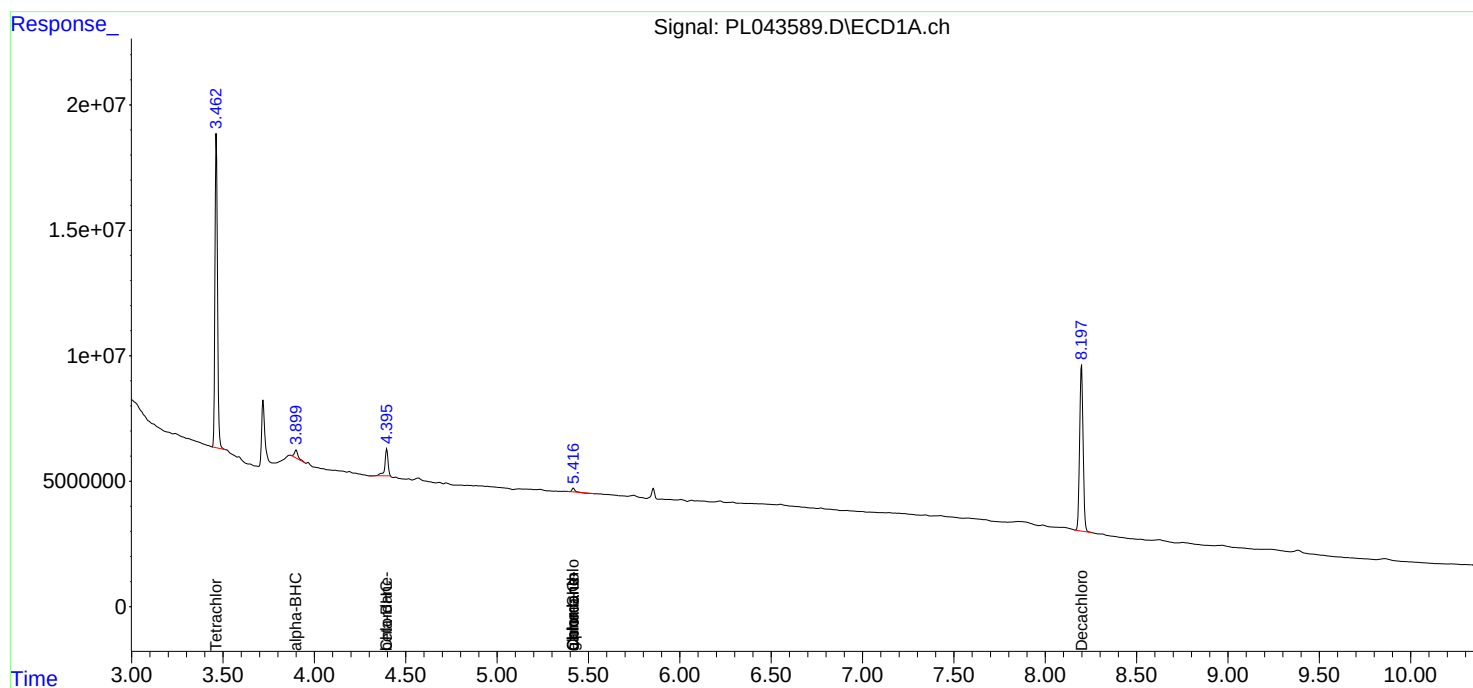


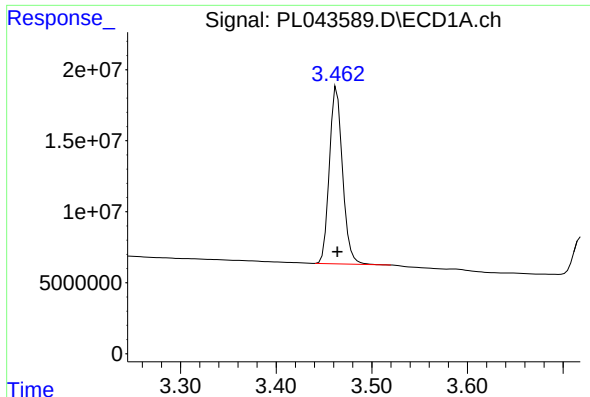

#1 Tetrachloro-m-xylene


R.T.: 3.463 min
Delta R.T.: 0.000 min
Response: 118521167
Conc: 18.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

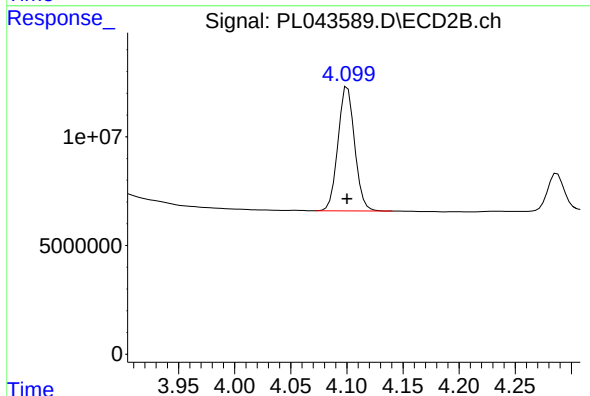


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 58983099
Conc: 20.19 ng/ml

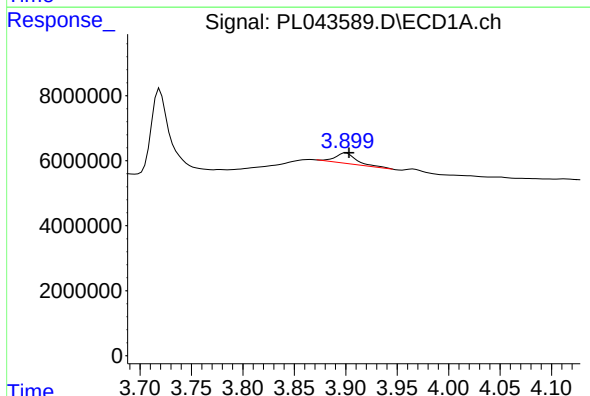


#2 alpha-BHC

R.T.: 3.900 min
Delta R.T.: -0.003 min
Response: 4332403
Conc: 0.45 ng/ml

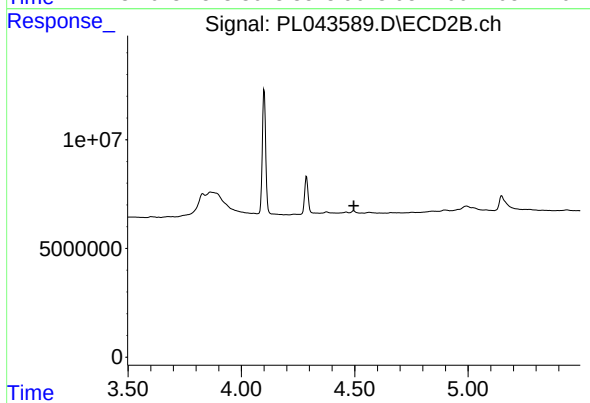

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.496 min
Response: 0
Conc: N.D.

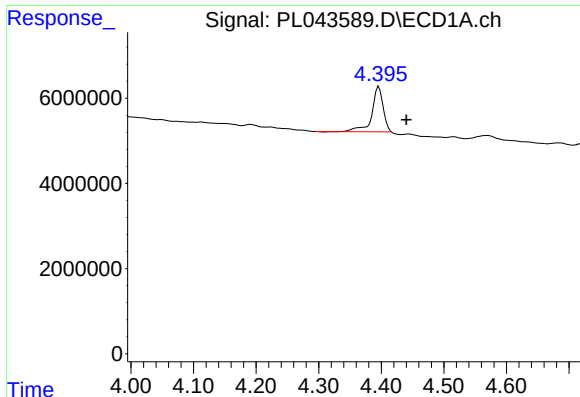

#6 beta-BHC


R.T.: 4.396 min
Delta R.T.: -0.044 min
Response: 13063922
Conc: 3.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

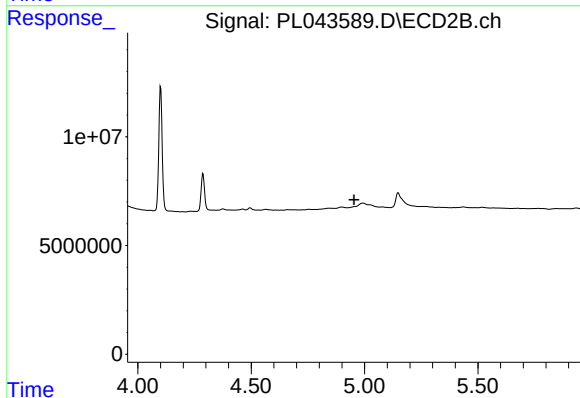


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

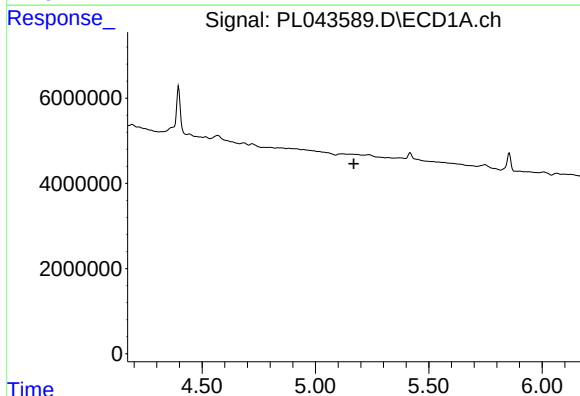


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.170 min
Response: 0
Conc: N.D.

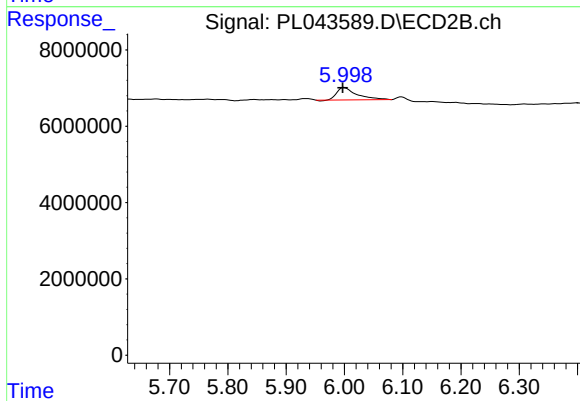

#8 Heptachlor epoxide


R.T.: 5.999 min
Delta R.T.: 0.002 min
Response: 7812410
Conc: 2.14 ng/ml

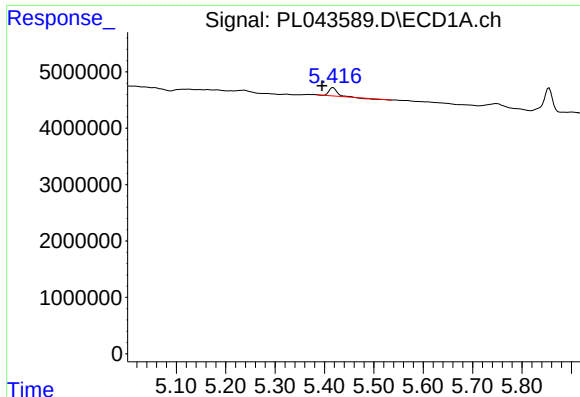

#10 gamma-Chlordane


R.T.: 5.418 min
Delta R.T.: 0.022 min
Response: 1609771
Conc: 0.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

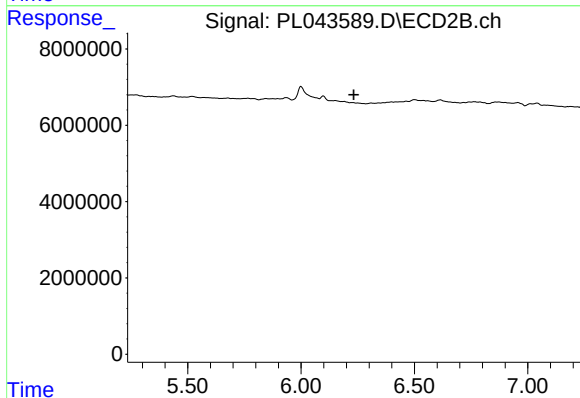


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.232 min
Response: 0
Conc: N.D.

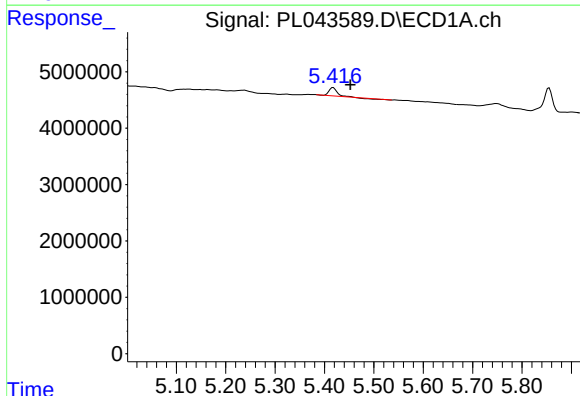


#11 alpha-Chlordane

R.T.: 5.418 min
Delta R.T.: -0.035 min
Response: 1609771
Conc: 0.21 ng/ml

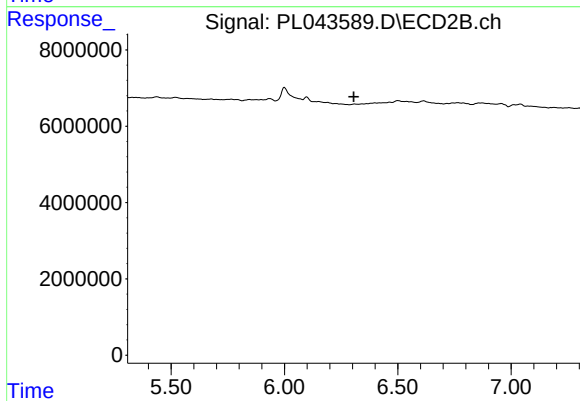

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.306 min
Response: 0
Conc: N.D.

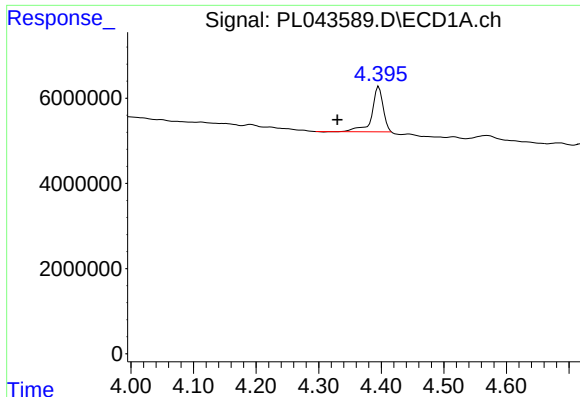

#23 Chlordane-1


R.T.: 4.396 min
Delta R.T.: 0.066 min
Response: 13063922
Conc: 48.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

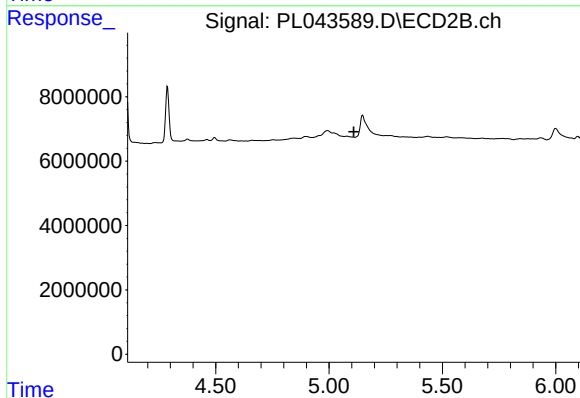


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.109 min
Response: 0
Conc: N.D.

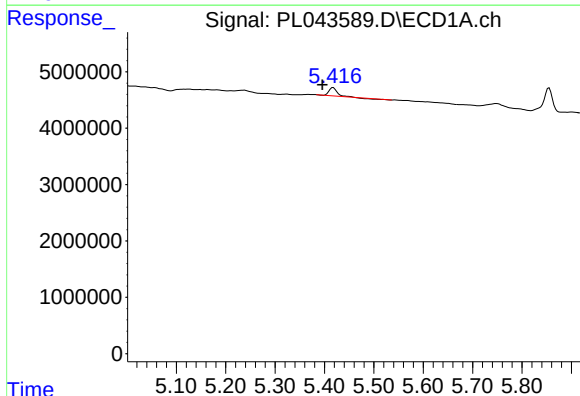


#25 Chlordane-3

R.T.: 5.418 min
Delta R.T.: 0.022 min
Response: 1609771
Conc: 1.91 ng/ml

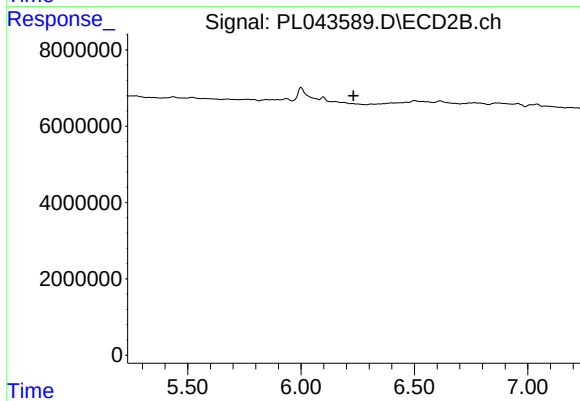

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.232 min
Response: 0
Conc: N.D.

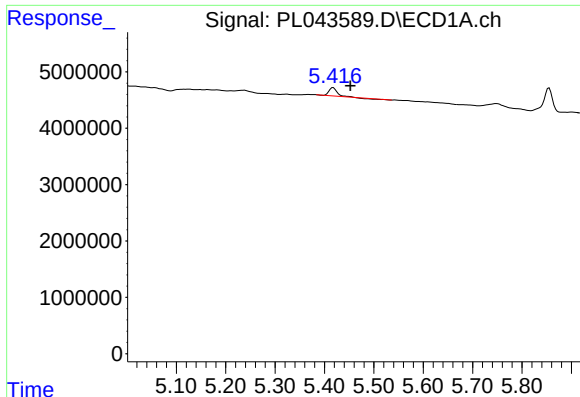

#26 Chlordane-4


R.T.: 5.418 min
Delta R.T.: -0.035 min
Response: 1609771
Conc: 2.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

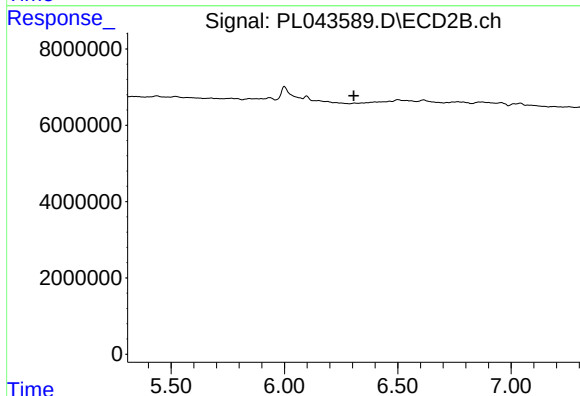


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.306 min
Response: 0
Conc: N.D.

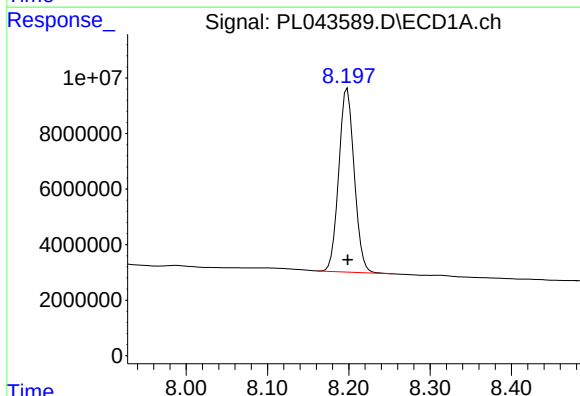

#28 Decachlorobiphenyl

R.T.: 8.198 min
Delta R.T.: 0.000 min
Response: 87224743
Conc: 17.31 ng/ml

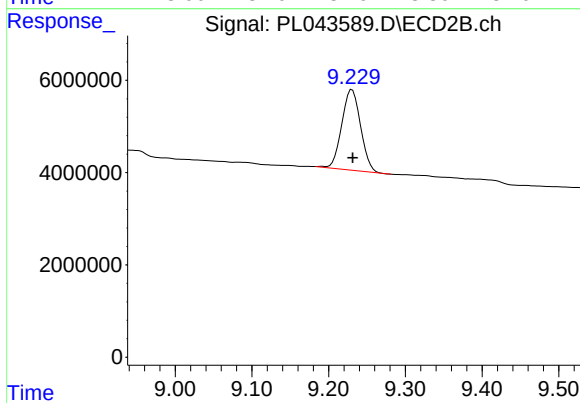

#28 Decachlorobiphenyl

R.T.: 9.230 min
Delta R.T.: 0.000 min
Response: 29755827
Conc: 13.46 ng/ml