

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010319\
 Data File : PL043593.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2019 01:11
 Operator : AJ\SJ
 Sample : K1019-06
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 07:07:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 04 06:12:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.463	4.101	127.7E6	64875080	19.992	22.203
28)	SA Decachlor...	8.198	9.230	127.3E6	47708037	25.253	21.581
Target Compounds							
2)	A alpha-BHC	0.000	4.456f	0	500259	N.D.	0.118 #
3)	MA gamma-BHC...	4.191	4.743f	6524081	1140480	0.747	0.287 #
4)	MA Heptachlor	4.495	0.000	66060539	0	7.394	N.D. #
6)	B beta-BHC	4.446	0.000	1819182	0	0.497	N.D. #
7)	B delta-BHC	0.000	5.149f	0	3044782	N.D.	0.720 #
8)	B Heptachlo...	0.000	5.996	0	12915366	N.D.	3.533 #
13)	MA Dieldrin	5.698f	0.000	1042818	0	0.147	N.D. #
14)	MA Endrin	6.013	0.000	3924764	0	0.643	N.D. #
16)	A 4,4'-DDD	6.067f	0.000	745402	0	0.141	N.D. #
23)	Chlordane-1	4.396	5.149	14123212	3044782	52.469	22.760 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010319\
Data File : PL043593.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2019 01:11
Operator : AJ\SJ
Sample : K1019-06
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 07:07:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
Quant Title : GC Extractables
QLast Update : Fri Jan 04 06:12:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

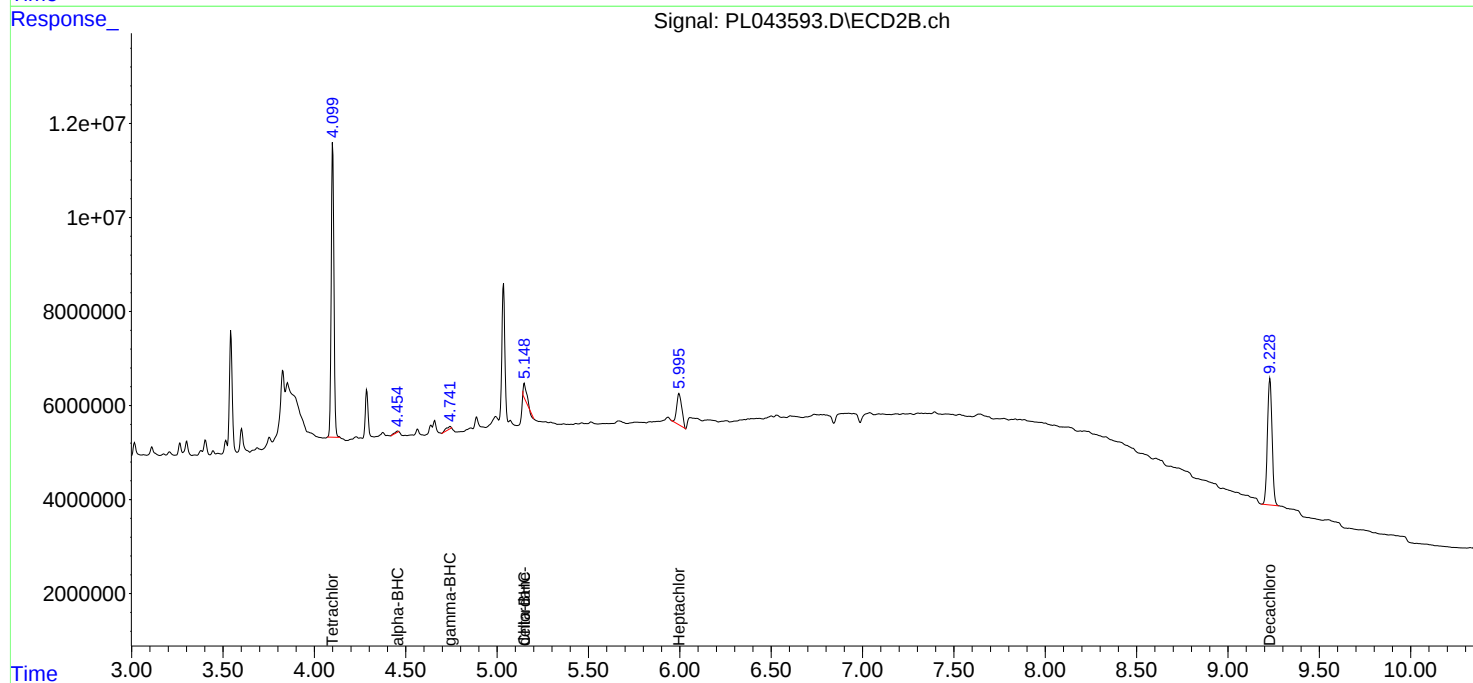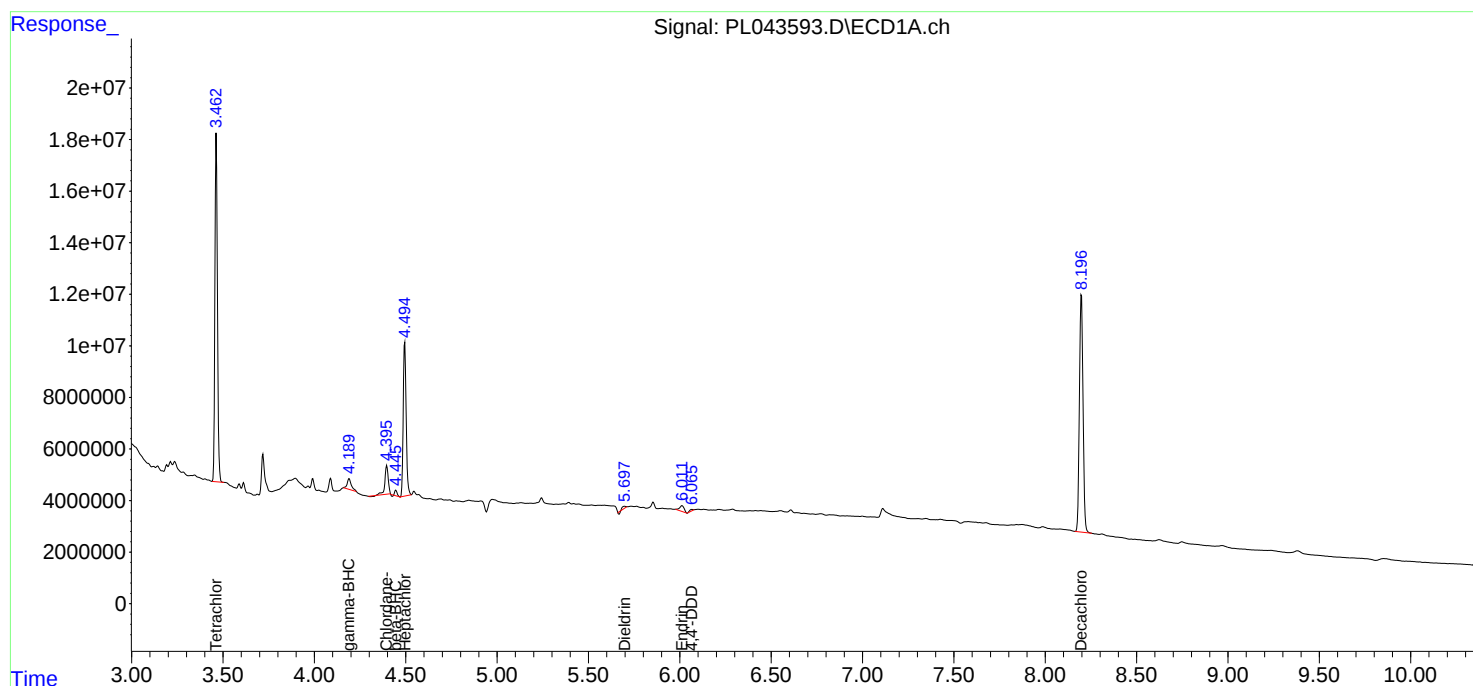


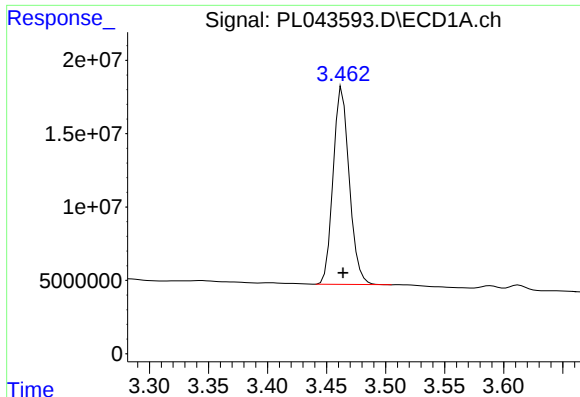

#1 Tetrachloro-m-xylene


R.T.: 3.463 min
Delta R.T.: 0.000 min
Response: 127733690
Conc: 19.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

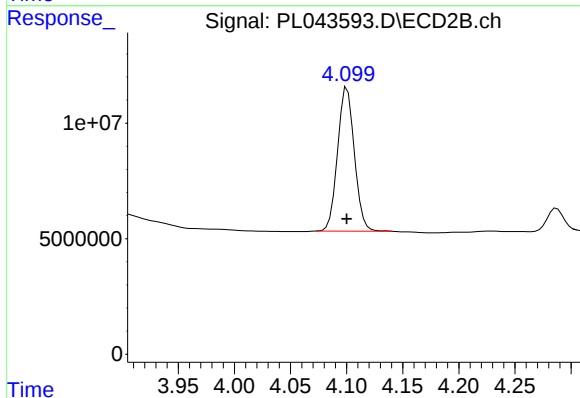


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 64875080
Conc: 22.20 ng/ml

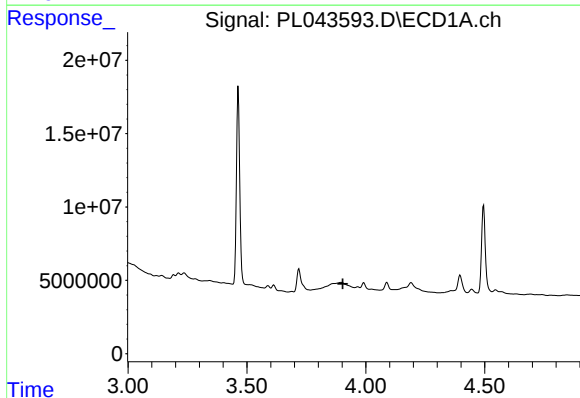


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.903 min
Response: 0
Conc: N.D.

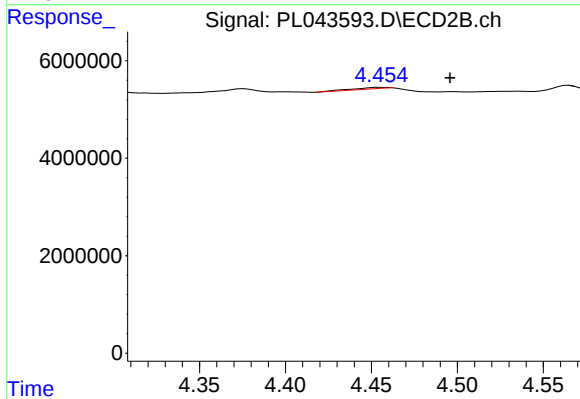

#2 alpha-BHC


R.T.: 4.456 min
Delta R.T.: -0.040 min
Response: 500259
Conc: 0.12 ng/ml

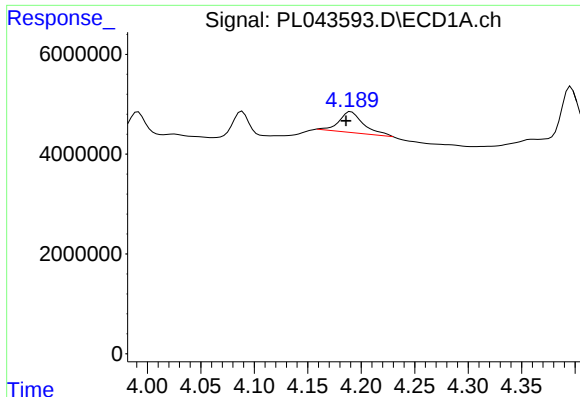

#3 gamma-BHC (Lindane)


R.T.: 4.191 min
Delta R.T.: 0.005 min
Response: 6524081
Conc: 0.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

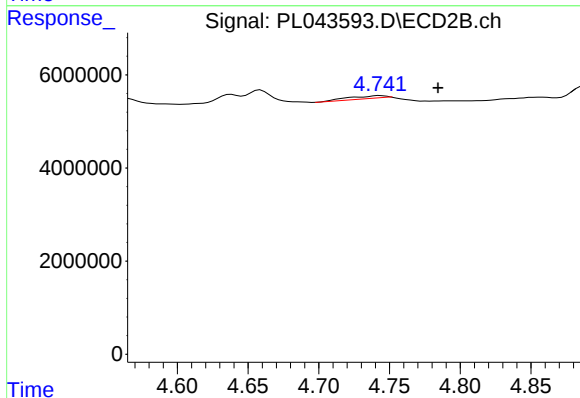


#3 gamma-BHC (Lindane)

R.T.: 4.743 min
Delta R.T.: -0.041 min
Response: 1140480
Conc: 0.29 ng/ml

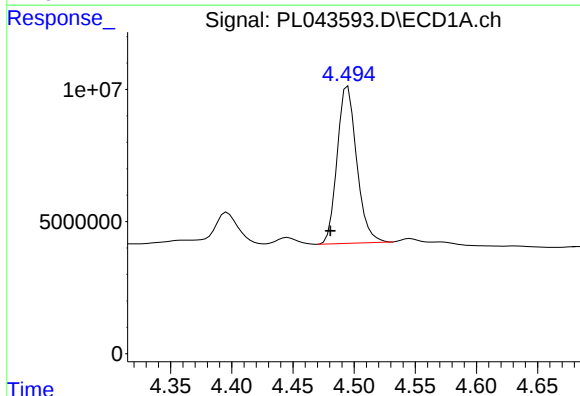


#4 Heptachlor

R.T.: 4.495 min
Delta R.T.: 0.014 min
Response: 66060539
Conc: 7.39 ng/ml

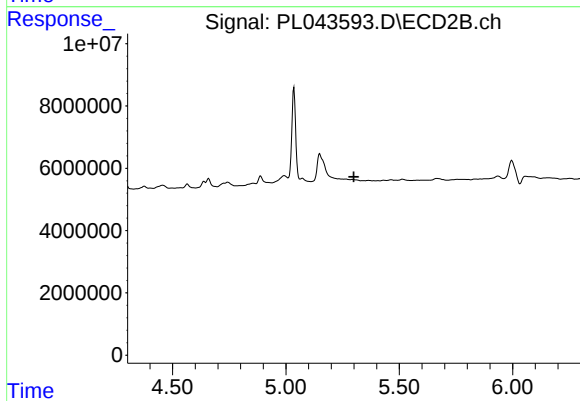

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.300 min
Response: 0
Conc: N.D.

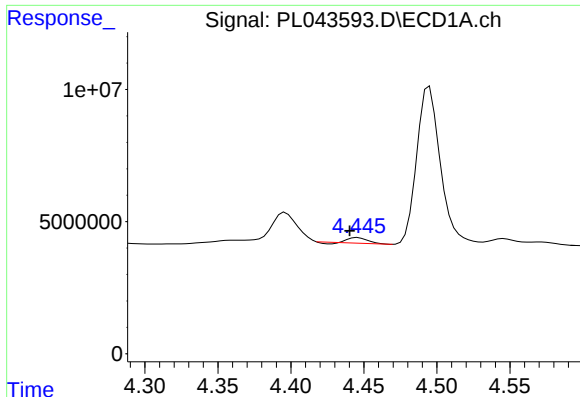

#6 beta-BHC


R.T.: 4.446 min
Delta R.T.: 0.005 min
Response: 1819182
Conc: 0.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

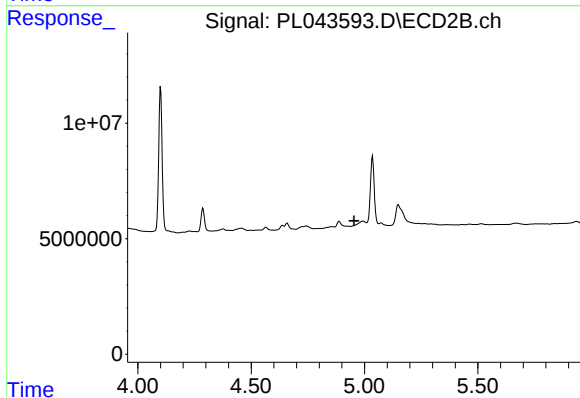


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

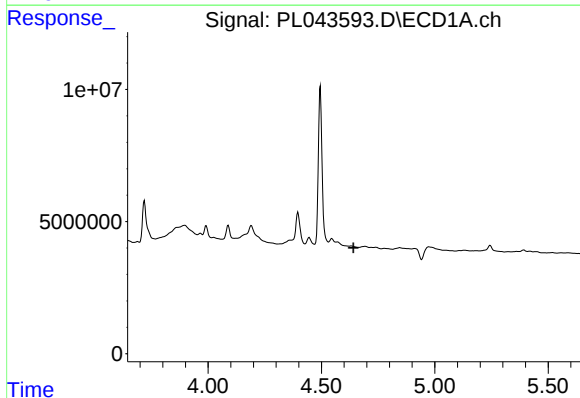


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.642 min
Response: 0
Conc: N.D.

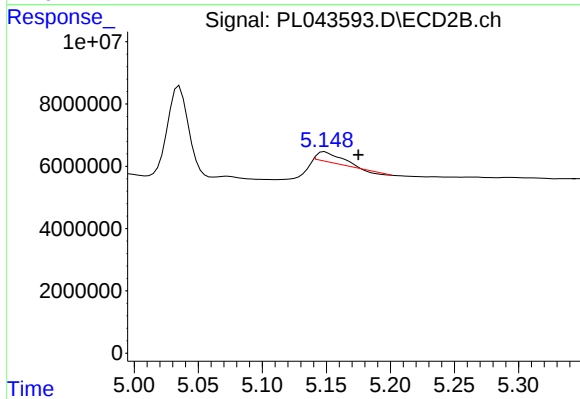

#7 delta-BHC


R.T.: 5.149 min
Delta R.T.: -0.026 min
Response: 3044782
Conc: 0.72 ng/ml

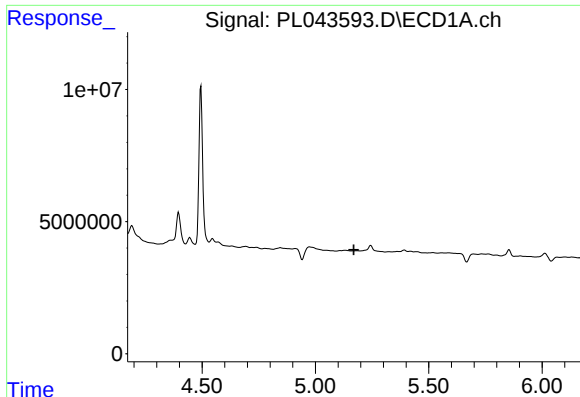

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.170 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

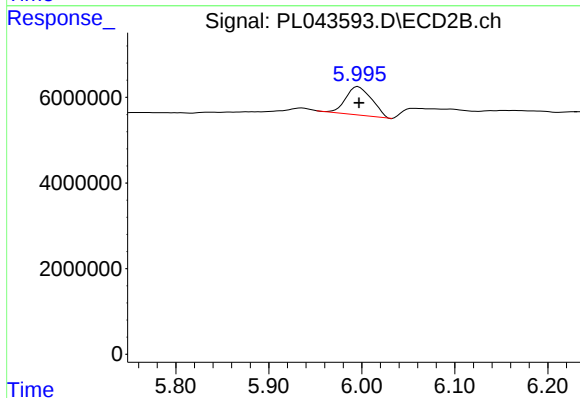


#8 Heptachlor epoxide

R.T.: 5.996 min
Delta R.T.: 0.000 min
Response: 12915366
Conc: 3.53 ng/ml

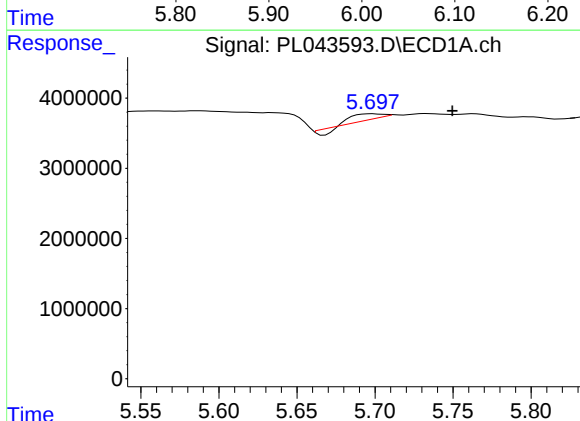


#13 Dieldrin

R.T.: 5.698 min
Delta R.T.: -0.051 min
Response: 1042818
Conc: 0.15 ng/ml

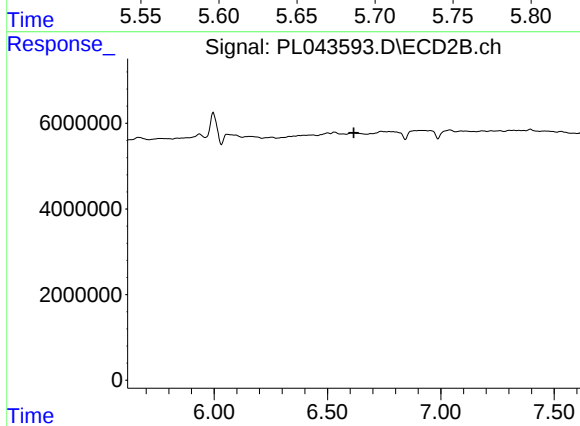

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.616 min
Response: 0
Conc: N.D.

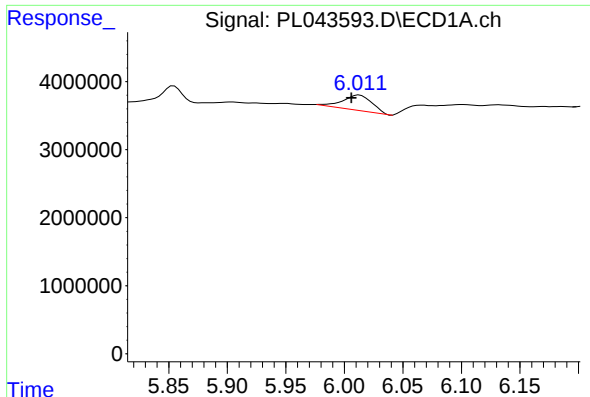

#14 Endrin


R.T.: 6.013 min
Delta R.T.: 0.007 min
Response: 3924764
Conc: 0.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

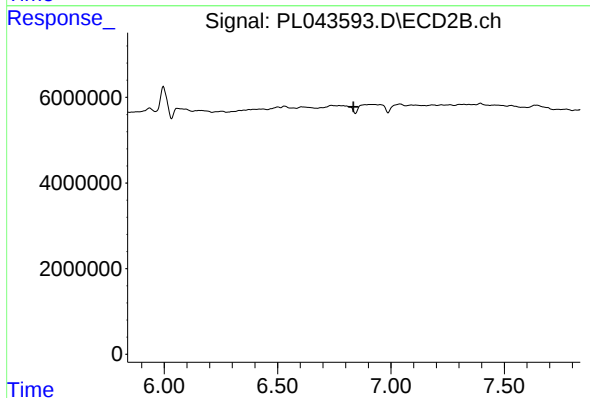


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.835 min
Response: 0
Conc: N.D.

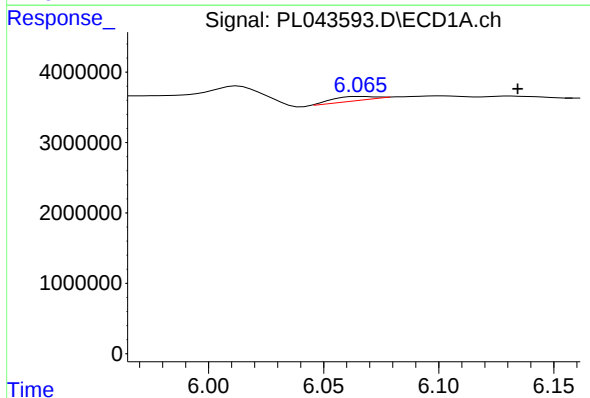


#16 4,4'-DDD

R.T.: 6.067 min
Delta R.T.: -0.068 min
Response: 745402
Conc: 0.14 ng/ml

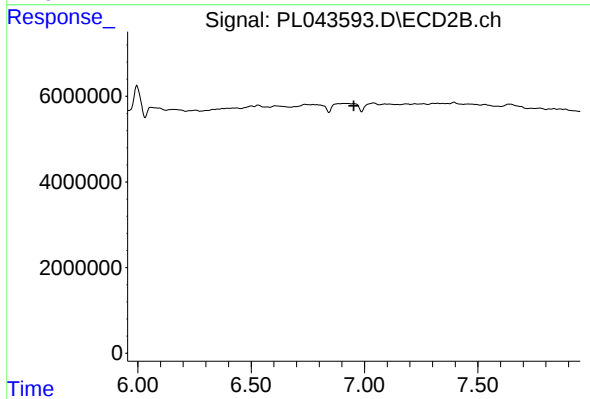

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.952 min
Response: 0
Conc: N.D.

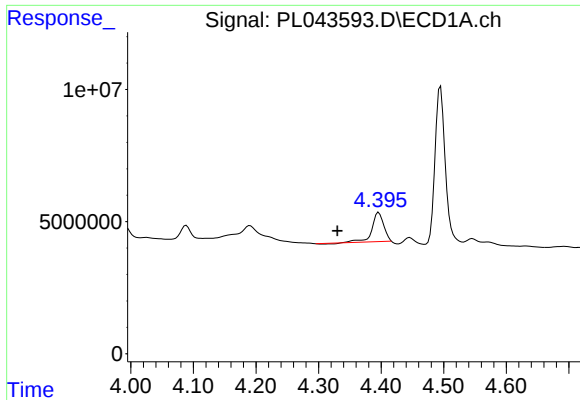

#23 Chlordane-1


R.T.: 4.396 min
Delta R.T.: 0.066 min
Response: 14123212
Conc: 52.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

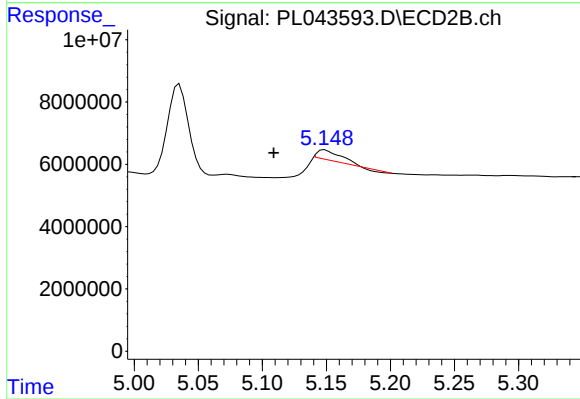


#23 Chlordane-1

R.T.: 5.149 min
Delta R.T.: 0.040 min
Response: 3044782
Conc: 22.76 ng/ml

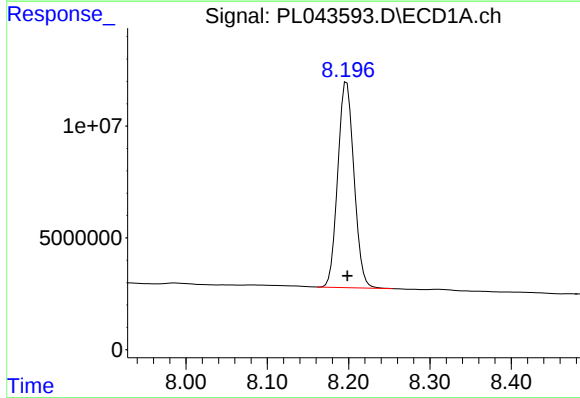

#28 Decachlorobiphenyl

R.T.: 8.198 min
Delta R.T.: 0.000 min
Response: 127255257
Conc: 25.25 ng/ml

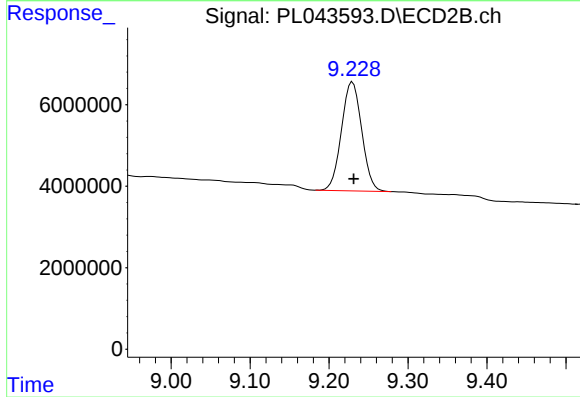

#28 Decachlorobiphenyl

R.T.: 9.230 min
Delta R.T.: -0.001 min
Response: 47708037
Conc: 21.58 ng/ml