

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010319\
 Data File : PL043595.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2019 01:39
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 07:08:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 04 06:12:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.100	125.8E6	61222595	19.690	20.953
28)	SA Decachlor...	8.198	9.231	129.2E6	49055252	25.647	22.191
Target Compounds							
7)	B delta-BHC	0.000	5.167	0	4257624	N.D.	1.007 #
8)	B Heptachlo...	5.108f	5.995	2688354	8714549	0.350	2.384 #
13)	MA Dieldrin	5.701f	0.000	609106	0	0.086	N.D. #
23)	Chlordane-1	0.000	5.167	0	4257624	N.D.	31.827 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010319\
Data File : PL043595.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2019 01:39
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 07:08:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
Quant Title : GC Extractables
QLast Update : Fri Jan 04 06:12:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

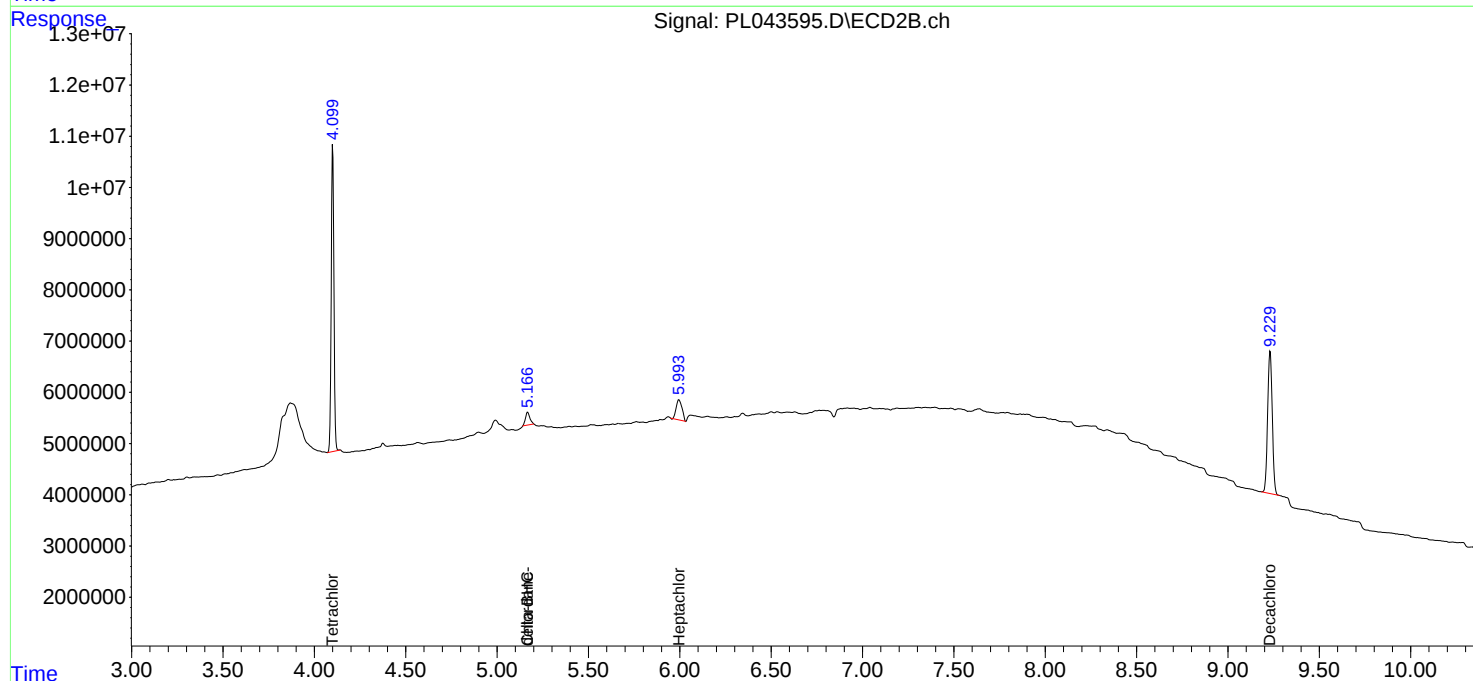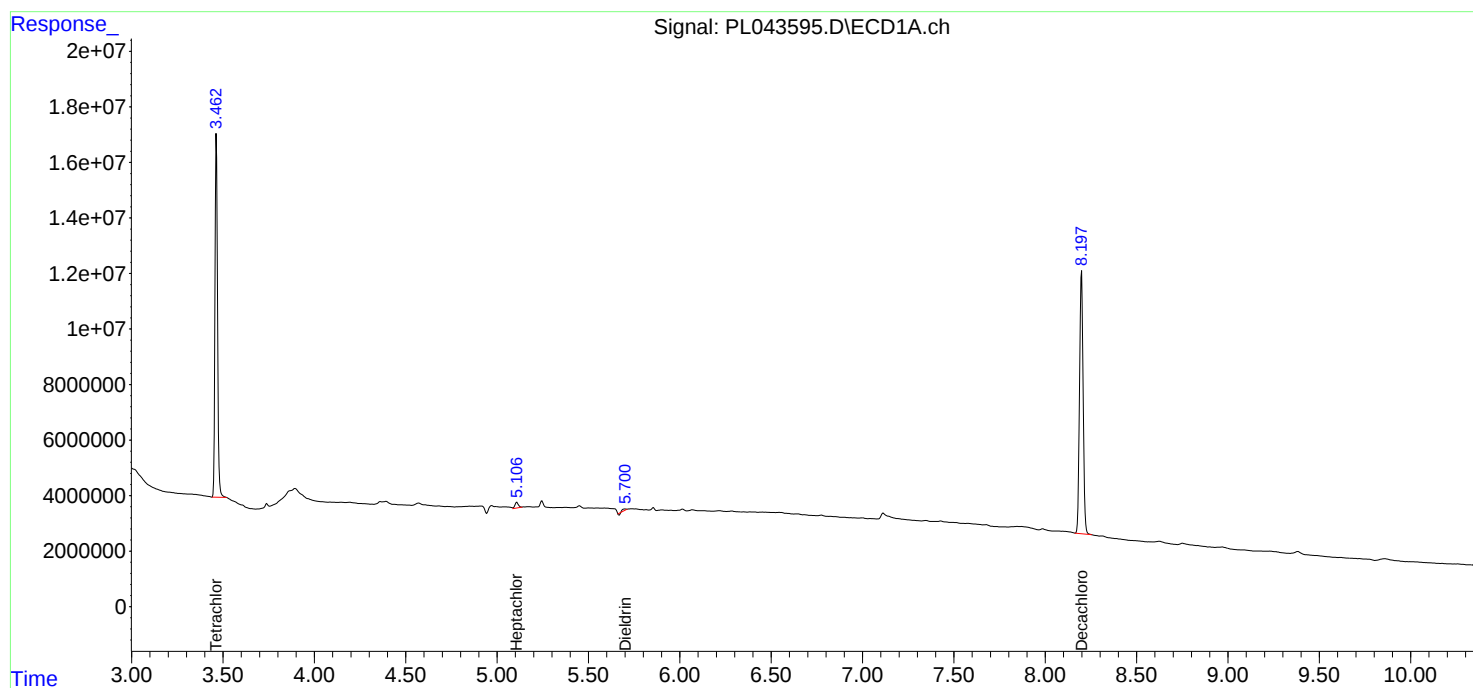


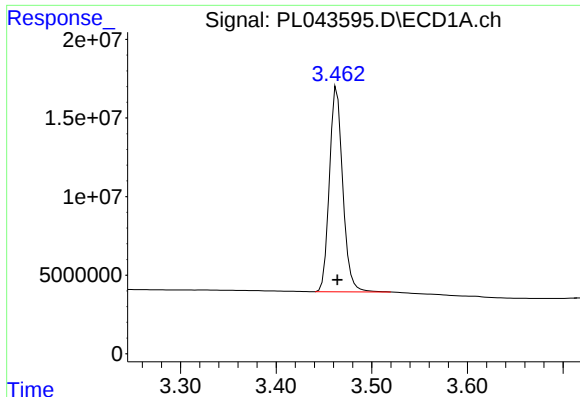

#1 Tetrachloro-m-xylene


R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 125800449
Conc: 19.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

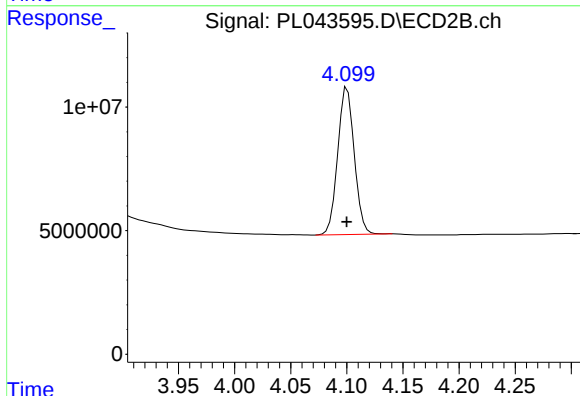


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: 0.000 min
Response: 61222595
Conc: 20.95 ng/ml

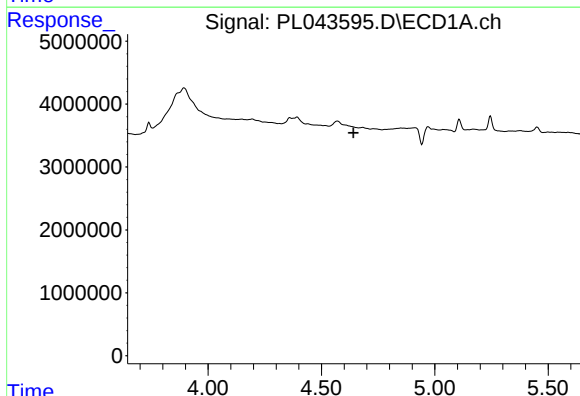


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.642 min
Response: 0
Conc: N.D.

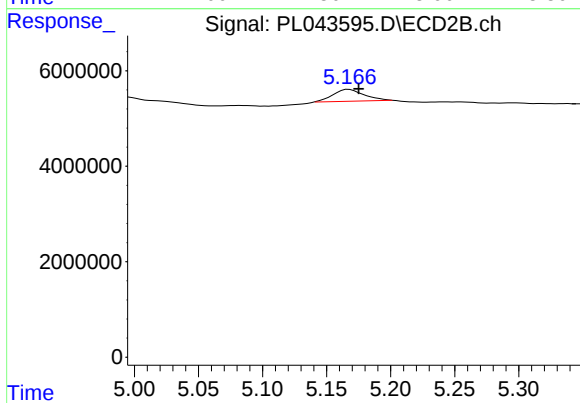

#7 delta-BHC


R.T.: 5.167 min
Delta R.T.: -0.008 min
Response: 4257624
Conc: 1.01 ng/ml

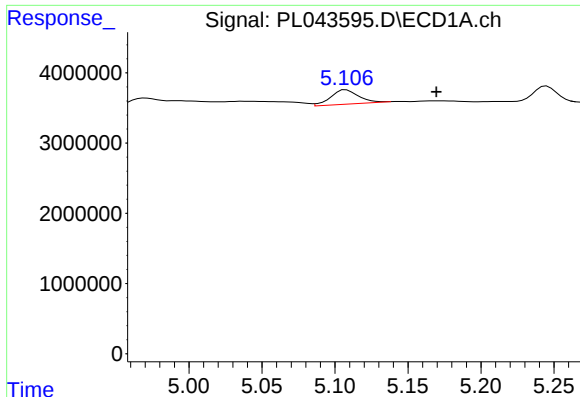

#8 Heptachlor epoxide


R.T.: 5.108 min
Delta R.T.: -0.062 min
Response: 2688354
Conc: 0.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

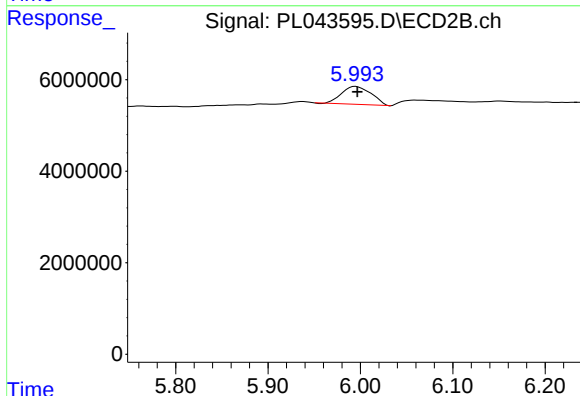


#8 Heptachlor epoxide

R.T.: 5.995 min
Delta R.T.: -0.002 min
Response: 8714549
Conc: 2.38 ng/ml

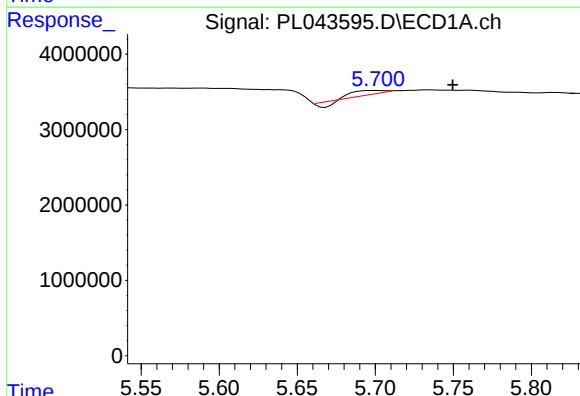


#13 Dieldrin

R.T.: 5.701 min
Delta R.T.: -0.048 min
Response: 609106
Conc: 0.09 ng/ml

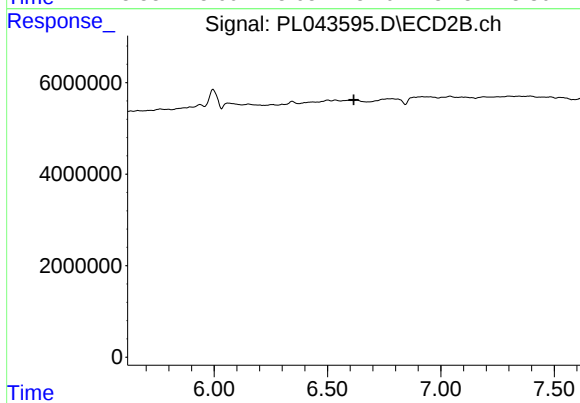

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.616 min
Response: 0
Conc: N.D.

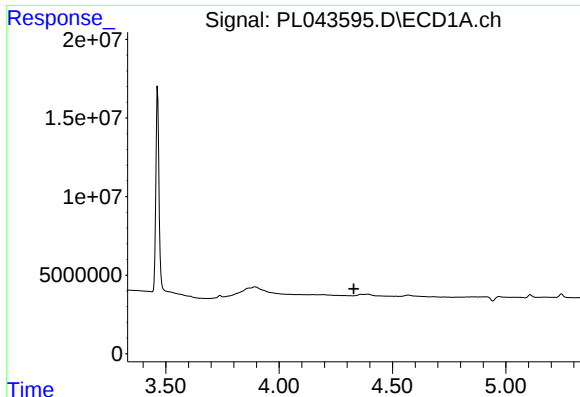

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.330 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

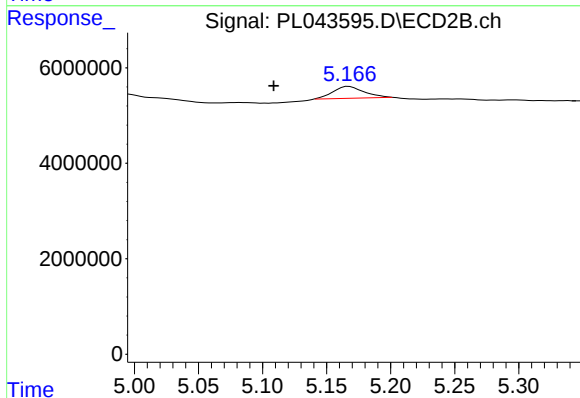


#23 Chlordane-1

R.T.: 5.167 min
Delta R.T.: 0.058 min
Response: 4257624
Conc: 31.83 ng/ml

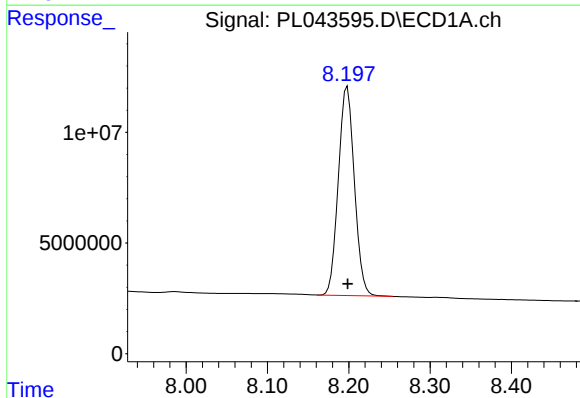

#28 Decachlorobiphenyl

R.T.: 8.198 min
Delta R.T.: 0.000 min
Response: 129242115
Conc: 25.65 ng/ml

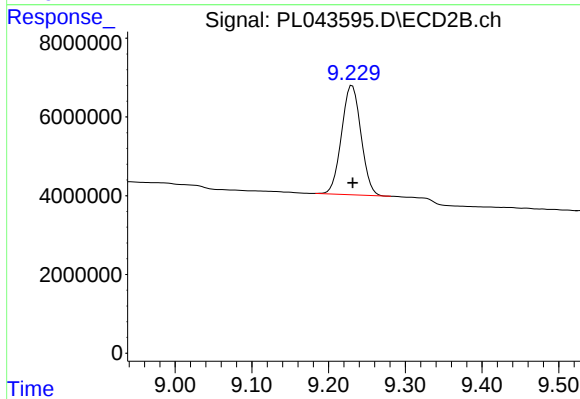

#28 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: 0.000 min
Response: 49055252
Conc: 22.19 ng/ml