

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010319\
 Data File : PL043609.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2019 04:57
 Operator : AJ\SJ
 Sample : K1017-21
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 07:14:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 04 06:12:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.101	67420026	32743789	10.552	11.207
28)	SA Decachlor...	8.198	9.230	74888147	30991060	14.861	14.019
Target Compounds							
6)	B beta-BHC	4.396f	0.000	7730402	0	2.113	N.D. #
7)	B delta-BHC	0.000	5.166	0	5861602	N.D.	1.386 #
8)	B Heptachlo...	0.000	6.000	0	9627680	N.D.	2.634 #
23)	Chlordane-1	4.396	5.166	7730402	5861602	28.719	43.817 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010319\
Data File : PL043609.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2019 04:57
Operator : AJ\SJ
Sample : K1017-21
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 07:14:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
Quant Title : GC Extractables
QLast Update : Fri Jan 04 06:12:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

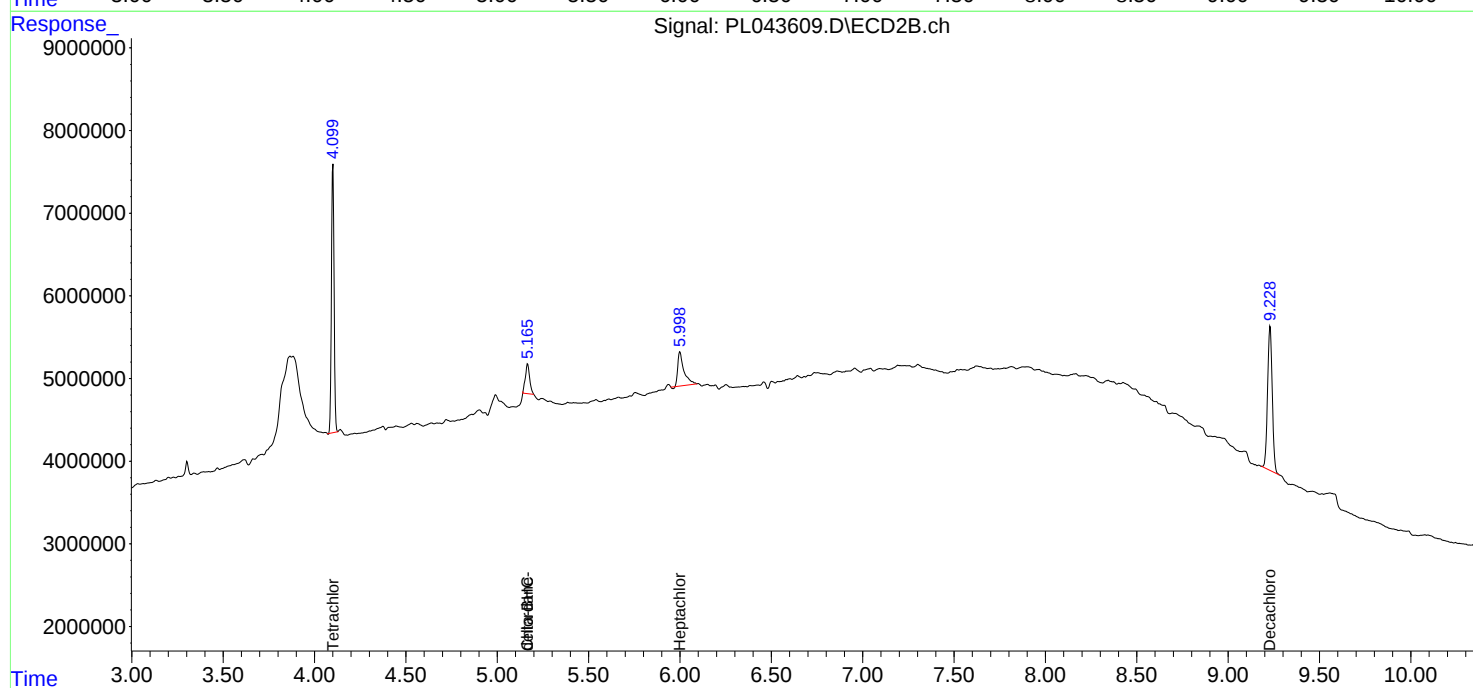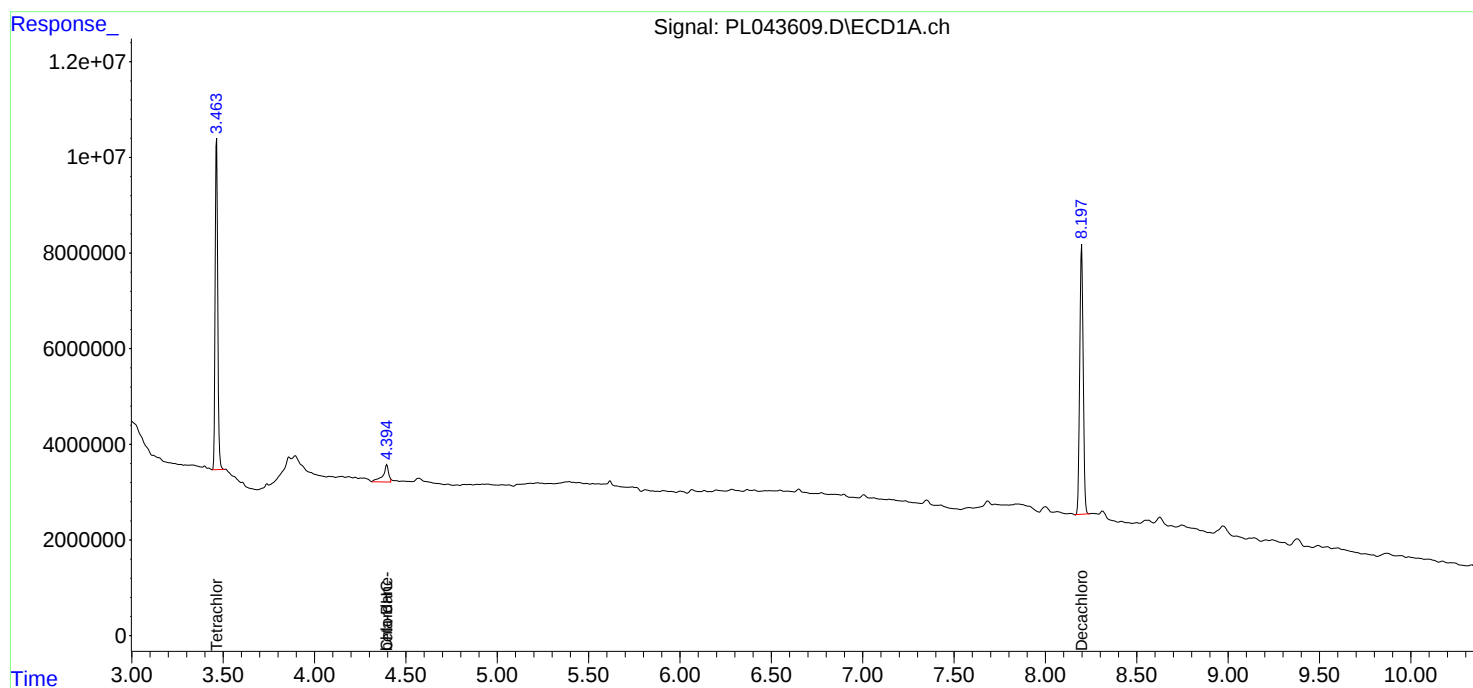


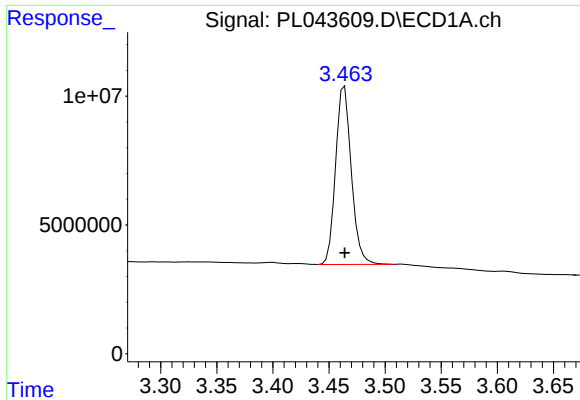

#1 Tetrachloro-m-xylene


R.T.: 3.464 min
Delta R.T.: 0.000 min
Response: 67420026
Conc: 10.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

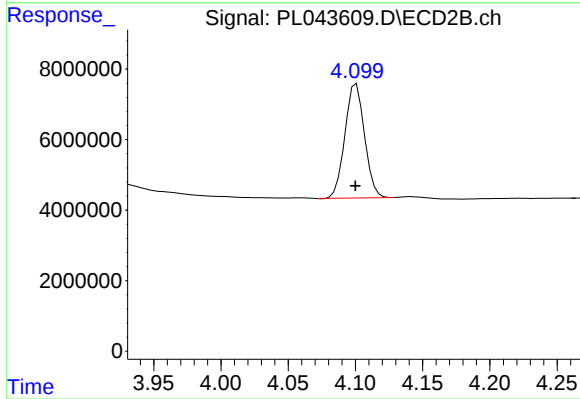


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 32743789
Conc: 11.21 ng/ml

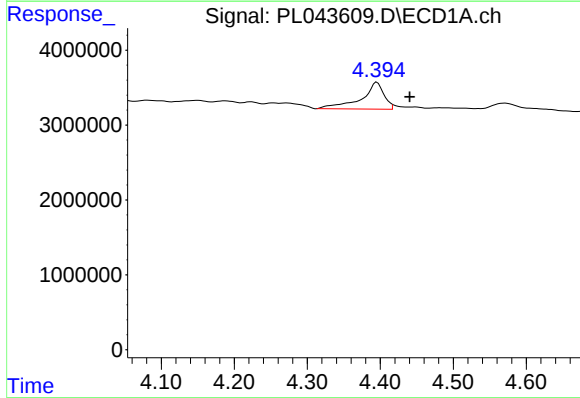


#6 beta-BHC

R.T.: 4.396 min
Delta R.T.: -0.045 min
Response: 7730402
Conc: 2.11 ng/ml

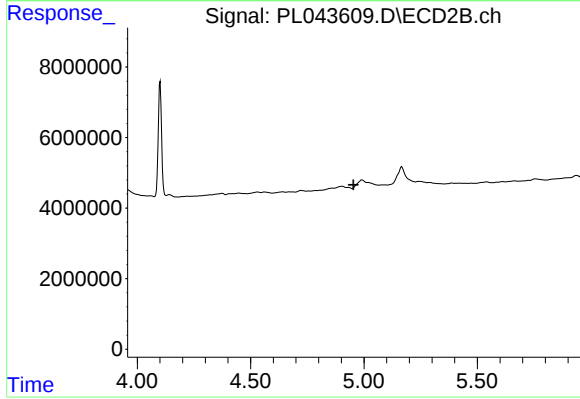

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

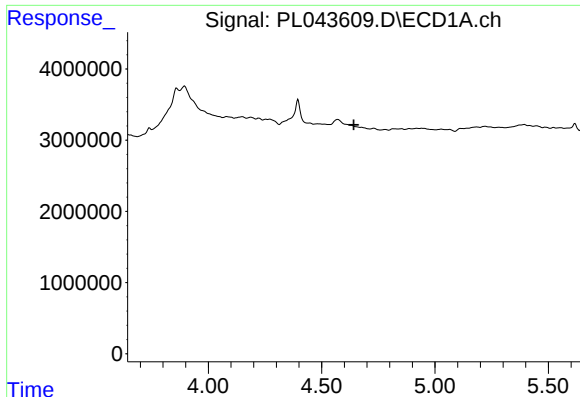

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.642 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

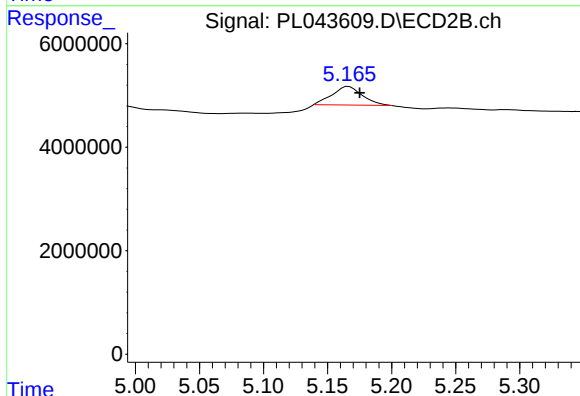


#7 delta-BHC

R.T.: 5.166 min
Delta R.T.: -0.009 min
Response: 5861602
Conc: 1.39 ng/ml

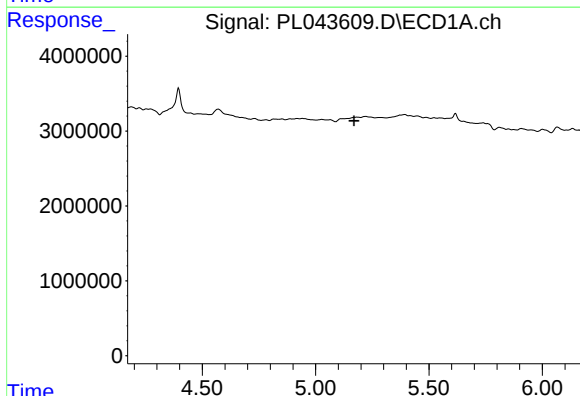


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.170 min
Response: 0
Conc: N.D.

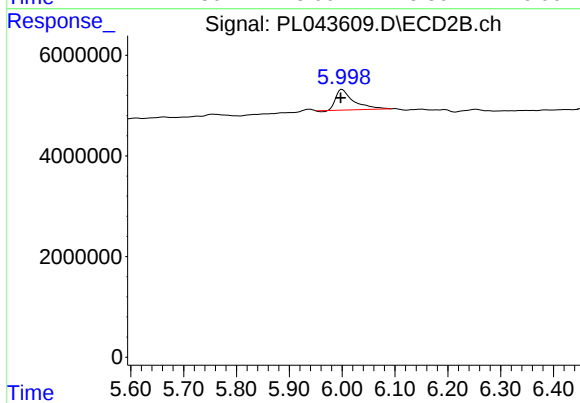

#8 Heptachlor epoxide


R.T.: 6.000 min
Delta R.T.: 0.003 min
Response: 9627680
Conc: 2.63 ng/ml

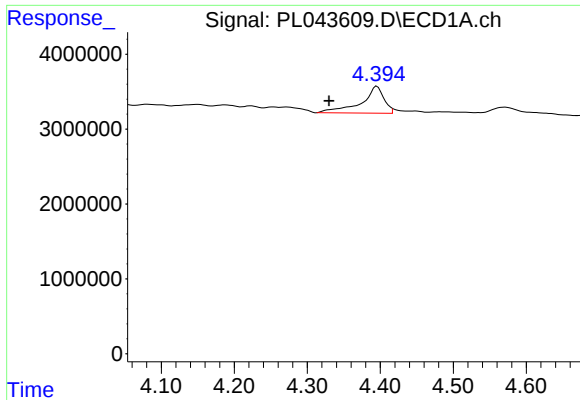

#23 Chlordane-1


R.T.: 4.396 min
Delta R.T.: 0.066 min
Response: 7730402
Conc: 28.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

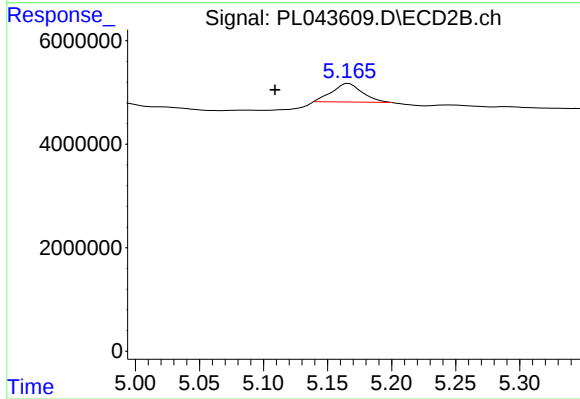


#23 Chlordane-1

R.T.: 5.166 min
Delta R.T.: 0.058 min
Response: 5861602
Conc: 43.82 ng/ml

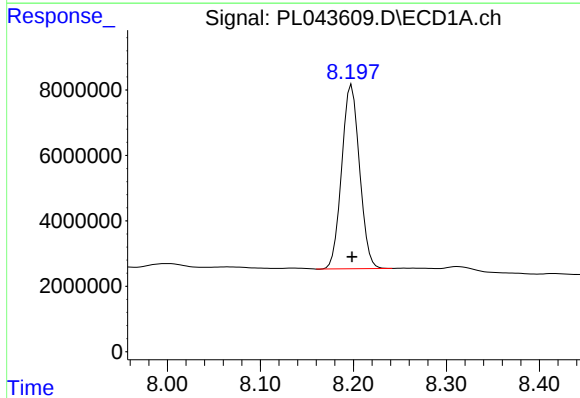

#28 Decachlorobiphenyl

R.T.: 8.198 min
Delta R.T.: 0.000 min
Response: 74888147
Conc: 14.86 ng/ml

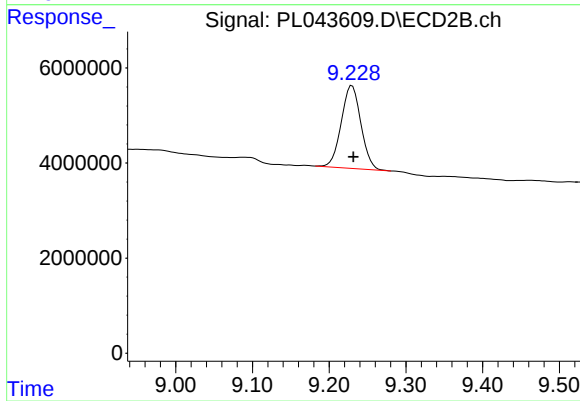

#28 Decachlorobiphenyl

R.T.: 9.230 min
Delta R.T.: -0.001 min
Response: 30991060
Conc: 14.02 ng/ml