

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010319\
 Data File : PL043613.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2019 05:54
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 07:16:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 04 06:12:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.463	4.100	127.9E6	61704516	20.023	21.118
28)	SA Decachlor...	8.199	9.232	118.1E6	43324892	23.439	19.598
Target Compounds							
7)	B delta-BHC	0.000	5.167	0	5182410	N.D.	1.226 #
8)	B Heptachlo...	5.107f	5.992	3961339	15004507	0.515	4.104 #
14)	MA Endrin	6.015	0.000	1987693	0	0.325	N.D. #
20)	A Methoxychlor	0.000	7.643f	0	4358181	N.D.	3.871 #
23)	Chlordane-1	0.000	5.167	0	5182410	N.D.	38.740 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010319\
Data File : PL043613.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2019 05:54
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 07:16:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
Quant Title : GC Extractables
QLast Update : Fri Jan 04 06:12:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

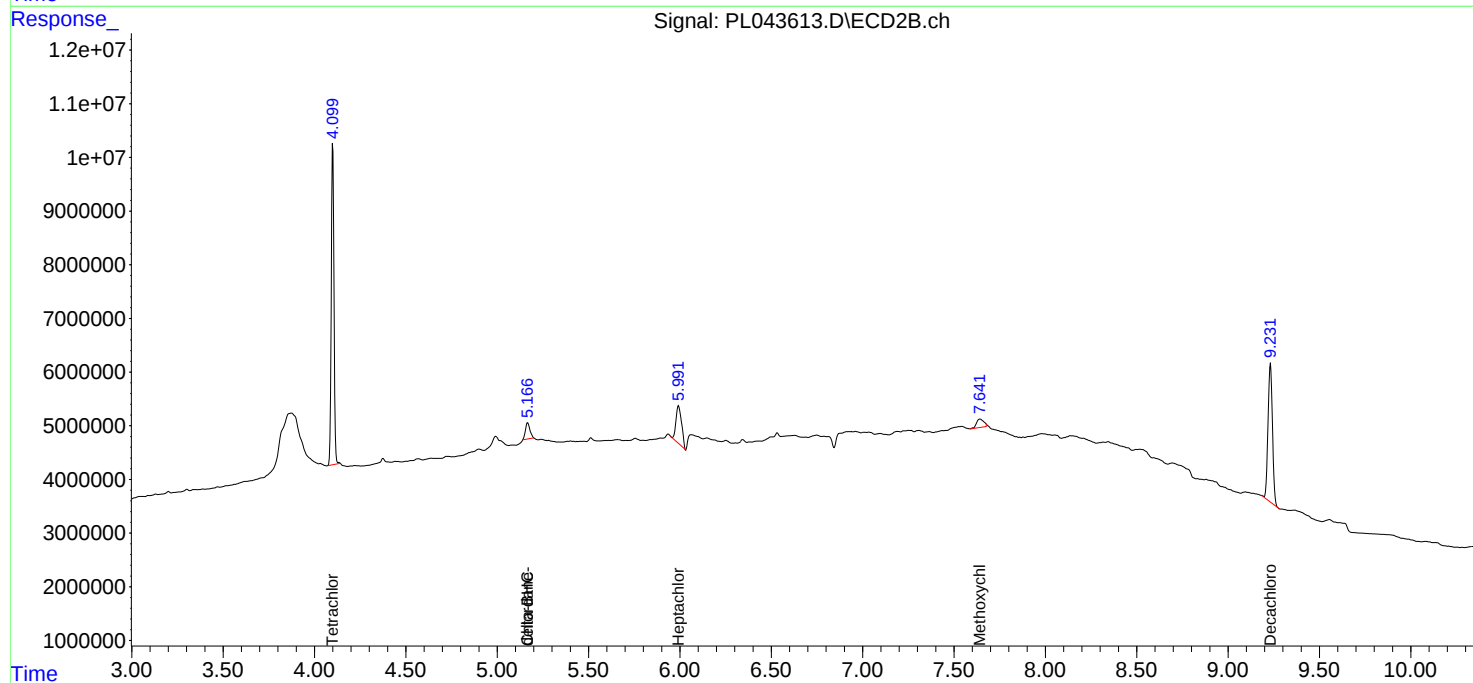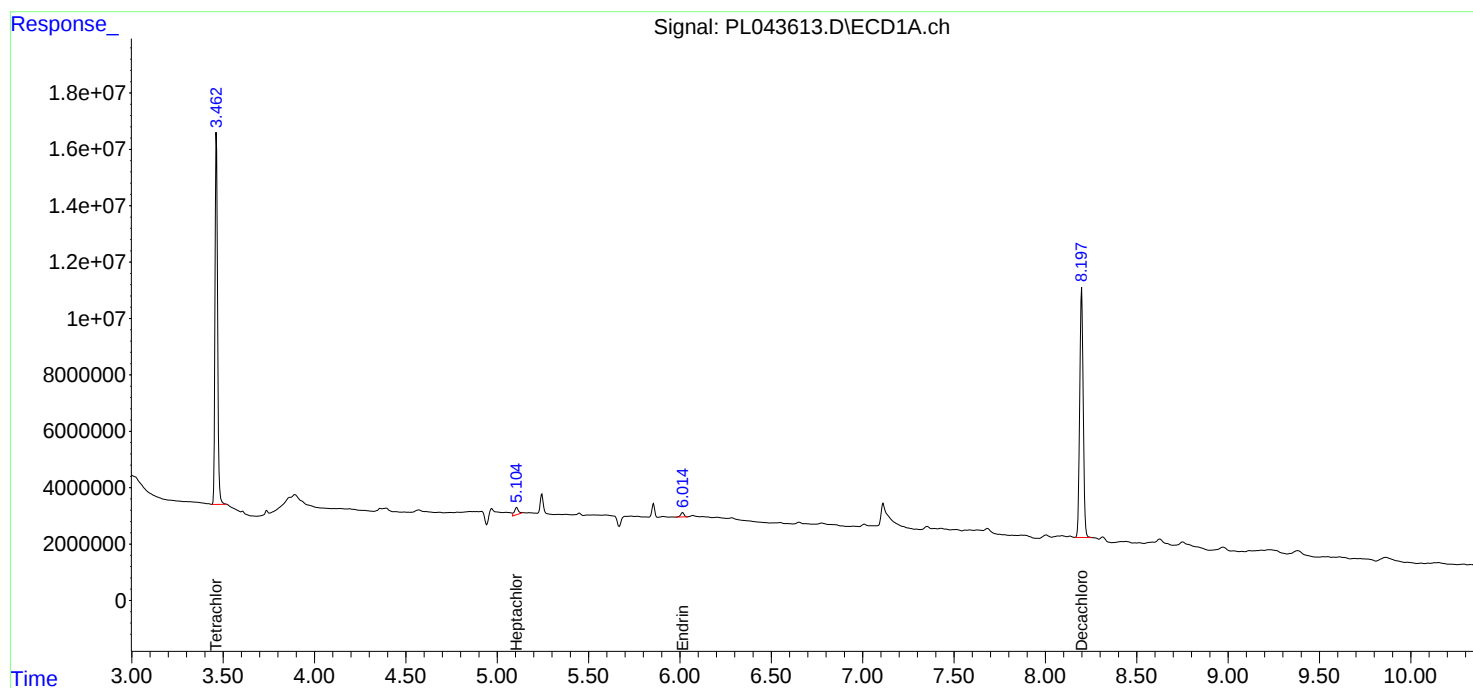


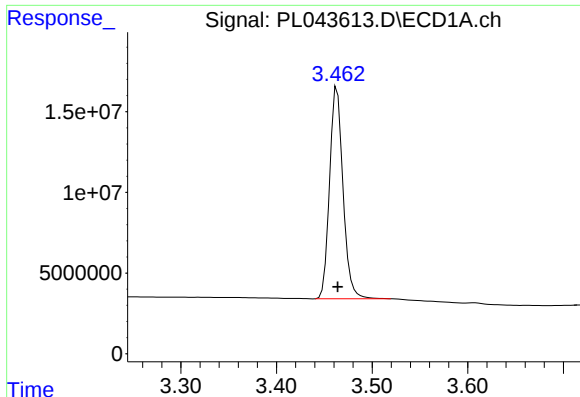

#1 Tetrachloro-m-xylene


R.T.: 3.463 min
Delta R.T.: 0.000 min
Response: 127933758
Conc: 20.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

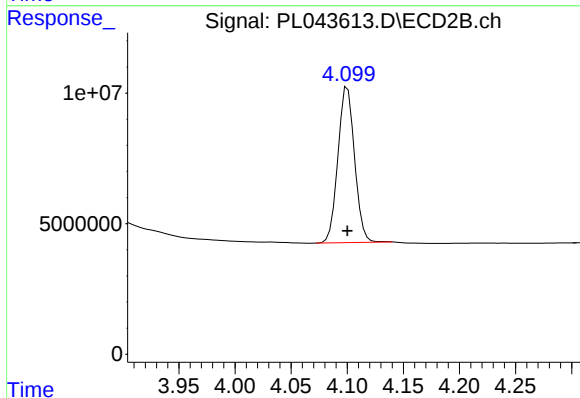


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: 0.000 min
Response: 61704516
Conc: 21.12 ng/ml

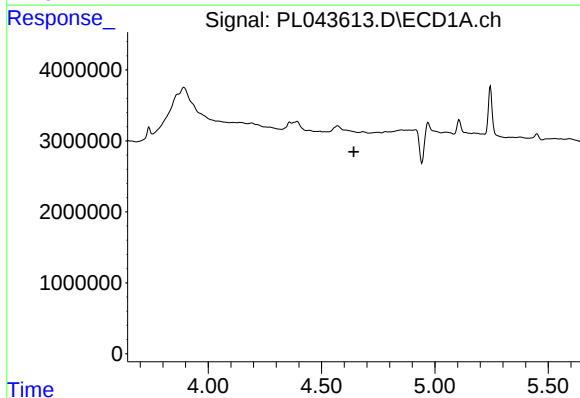


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.642 min
Response: 0
Conc: N.D.

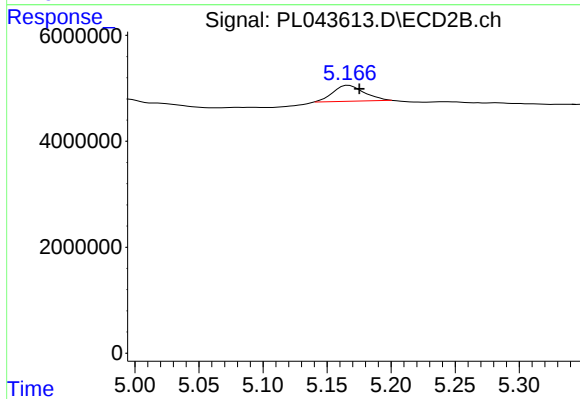

#7 delta-BHC


R.T.: 5.167 min
Delta R.T.: -0.008 min
Response: 5182410
Conc: 1.23 ng/ml

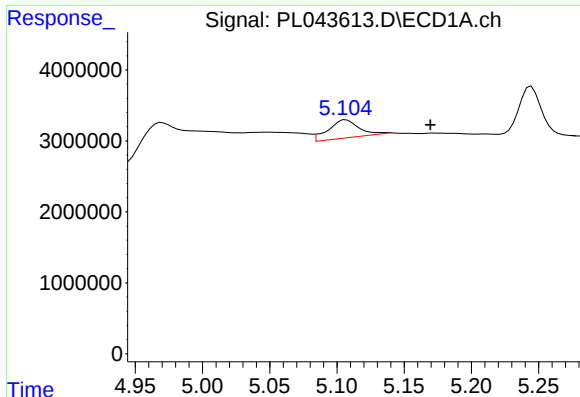

#8 Heptachlor epoxide


R.T.: 5.107 min
Delta R.T.: -0.063 min
Response: 3961339
Conc: 0.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

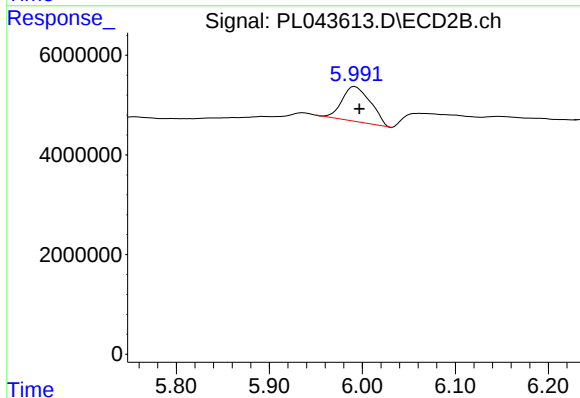


#8 Heptachlor epoxide

R.T.: 5.992 min
Delta R.T.: -0.005 min
Response: 15004507
Conc: 4.10 ng/ml

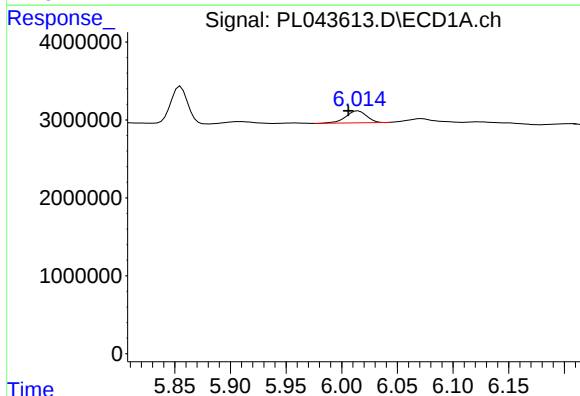


#14 Endrin

R.T.: 6.015 min
Delta R.T.: 0.009 min
Response: 1987693
Conc: 0.33 ng/ml

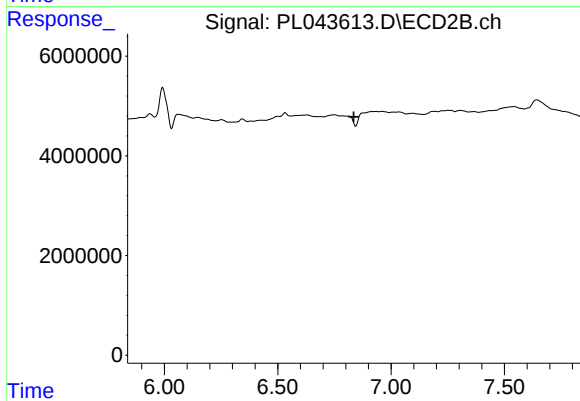

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.835 min
Response: 0
Conc: N.D.

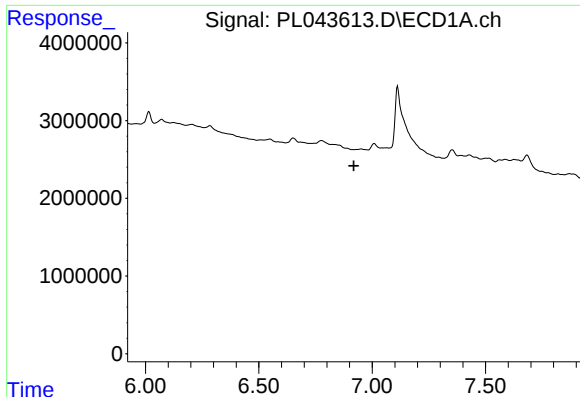

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.918 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

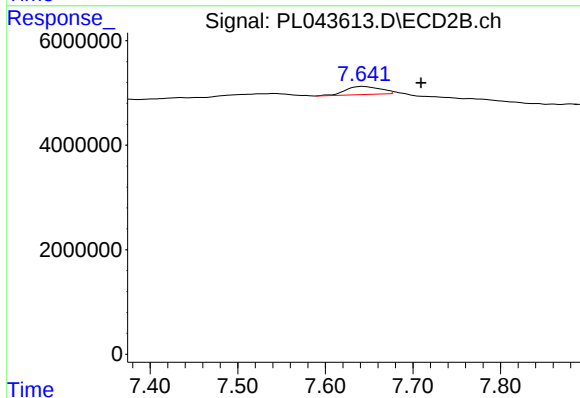


#20 Methoxychlor

R.T.: 7.643 min
Delta R.T.: -0.066 min
Response: 4358181
Conc: 3.87 ng/ml

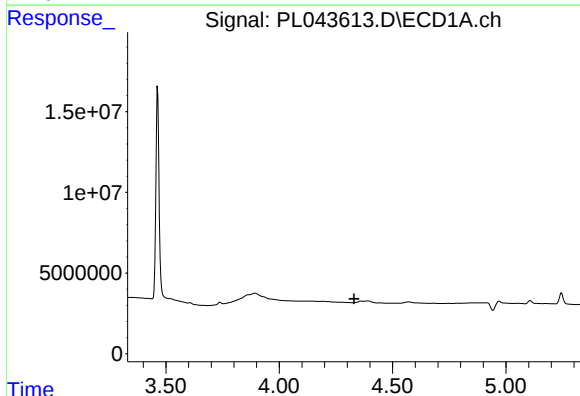


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.330 min
Response: 0
Conc: N.D.

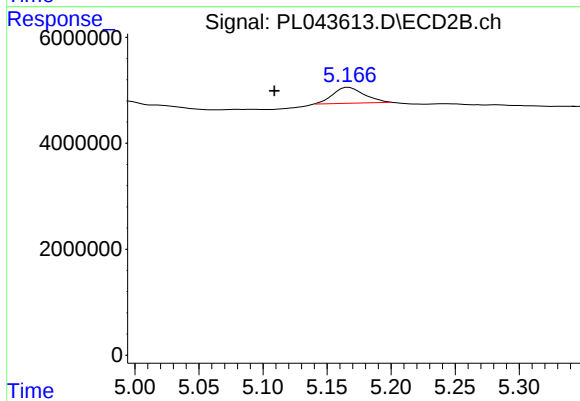

#23 Chlordane-1


R.T.: 5.167 min
Delta R.T.: 0.058 min
Response: 5182410
Conc: 38.74 ng/ml

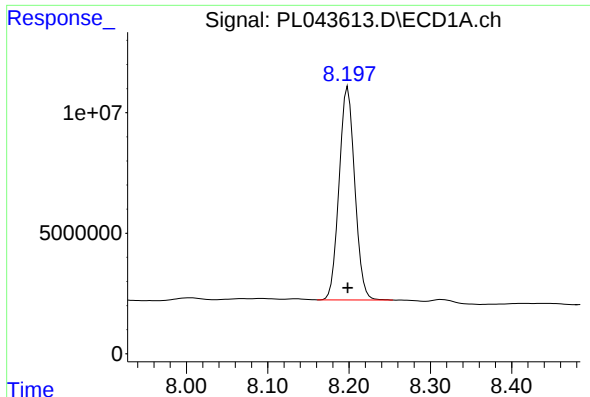

#28 Decachlorobiphenyl

R.T.: 8.199 min
Delta R.T.: 0.000 min
Response: 118118460
Conc: 23.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

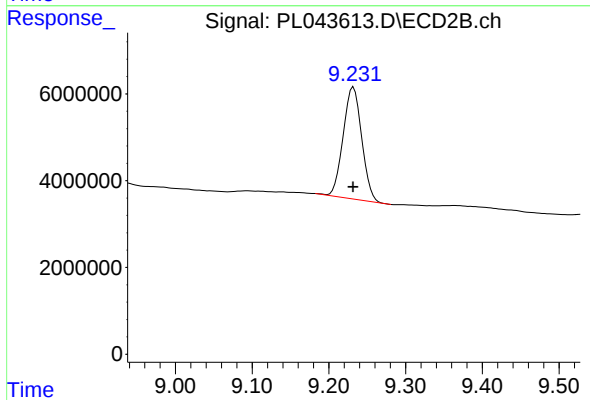

#28 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: 0.000 min
Response: 43324892
Conc: 19.60 ng/ml