

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010319\
 Data File : PL043543.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jan 2019 10:46
 Operator : AJ\SJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 06:09:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 04 06:09:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.463	4.100	319.7E6	138.4E6	50.000	50.000
28)	SA Decachlor...	8.199	9.231	240.4E6	107.3E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.330	5.109	134.6E6	66887462	500.000	500.000
24)	Chlordane-2	4.829	5.581	137.9E6	61741357	500.000	500.000
25)	Chlordane-3	5.396	6.232	421.1E6	216.5E6	500.000	500.000
26)	Chlordane-4	5.453	6.306	372.2E6	250.9E6	500.000	500.000
27)	Chlordane-5	6.287	7.117	106.0E6	46048710	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010319\
Data File : PL043543.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jan 2019 10:46
Operator : AJ\SJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 06:09:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
Quant Title : GC Extractables
QLast Update : Fri Jan 04 06:09:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

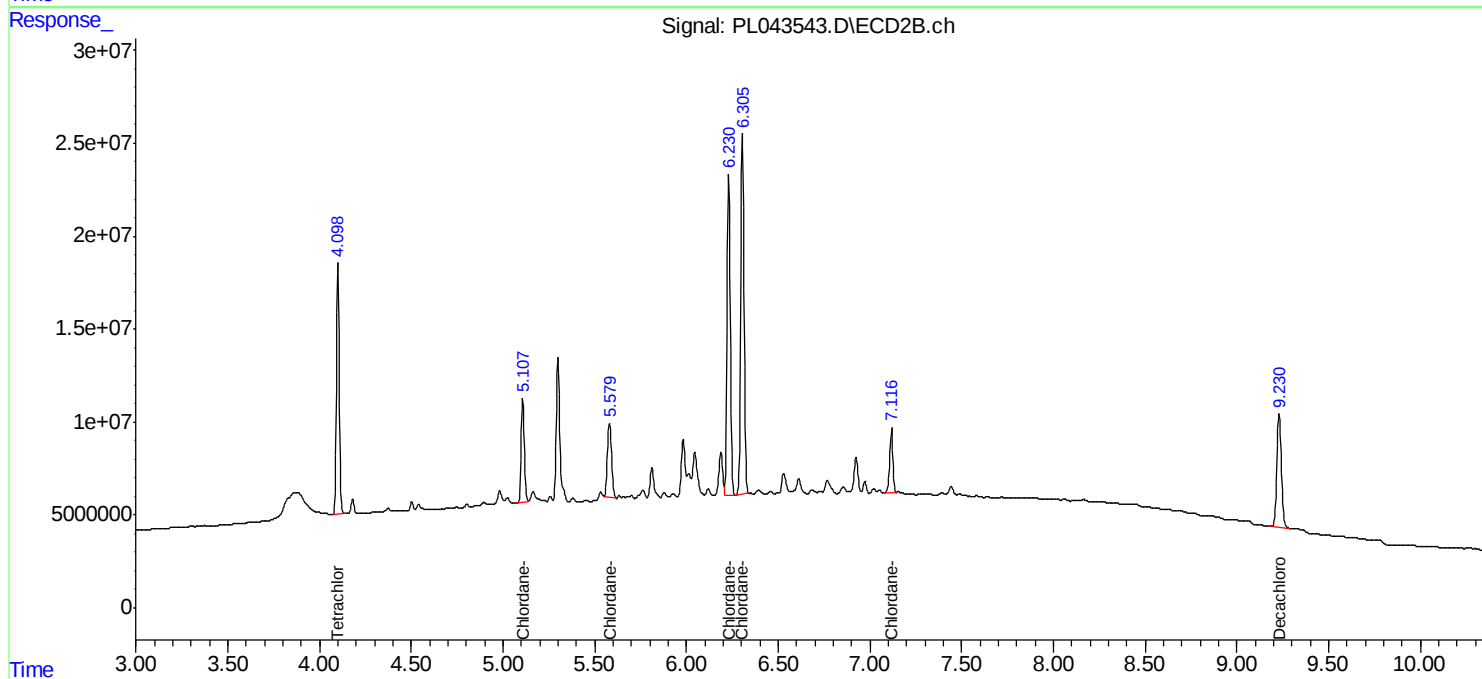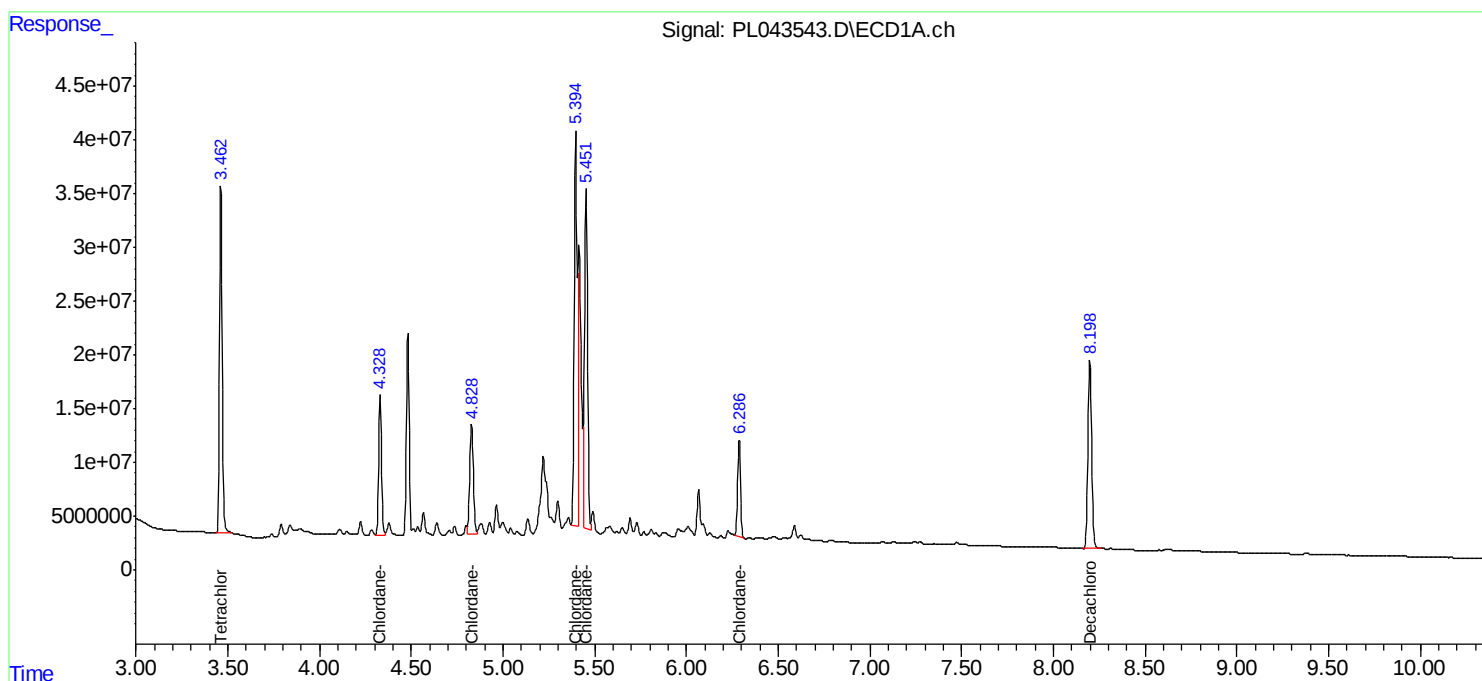


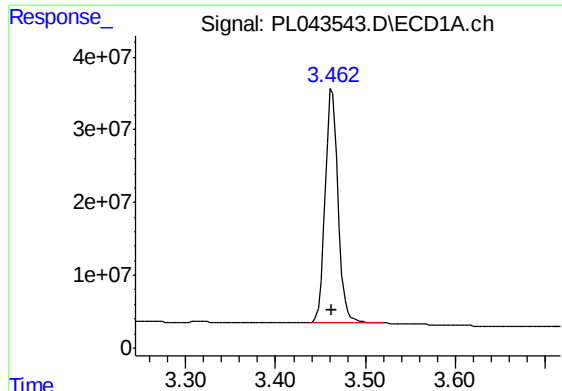

#1 Tetrachloro-m-xylene


R.T.: 3.463 min
Delta R.T.: 0.000 min
Response: 319712254
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

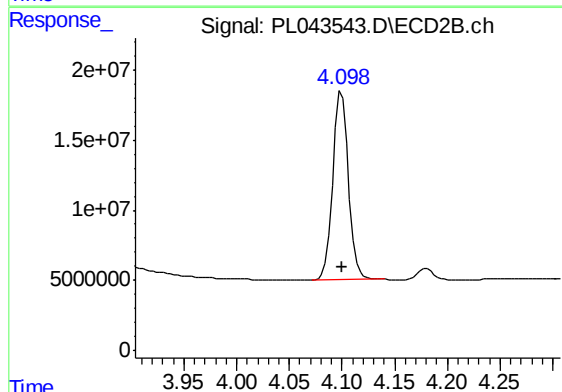


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: 0.000 min
Response: 138386094
Conc: 50.00 ng/ml

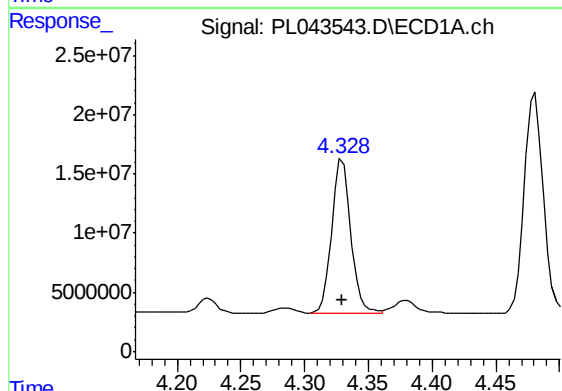


#23 Chlordane-1

R.T.: 4.330 min
Delta R.T.: 0.000 min
Response: 134586751
Conc: 500.00 ng/ml

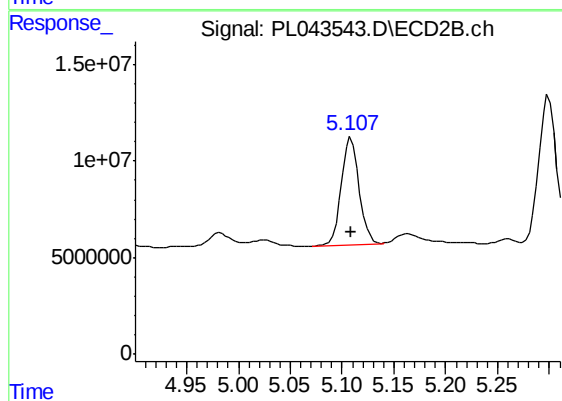

#23 Chlordane-1


R.T.: 5.109 min
Delta R.T.: 0.000 min
Response: 66887462
Conc: 500.00 ng/ml

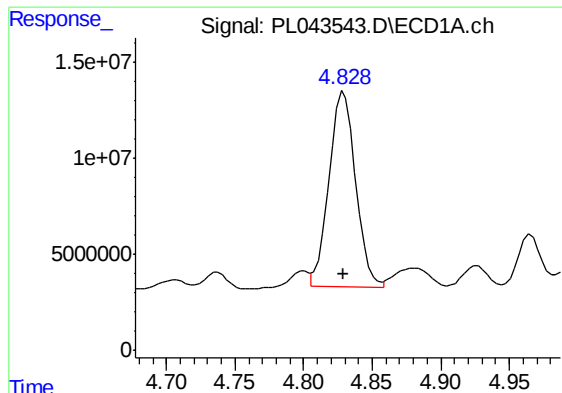

#24 Chlordane-2


R.T.: 4.829 min
Delta R.T.: 0.000 min
Response: 137874744
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

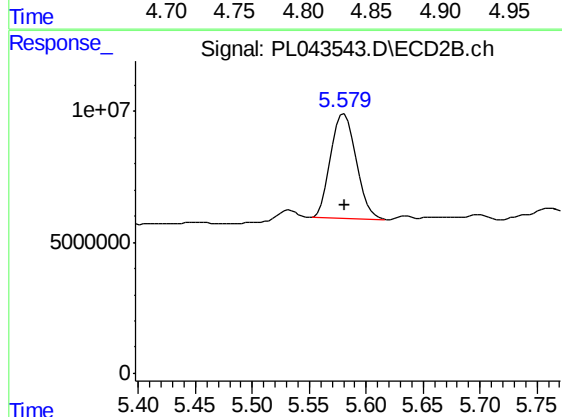


#24 Chlordane-2

R.T.: 5.581 min
Delta R.T.: 0.000 min
Response: 61741357
Conc: 500.00 ng/ml

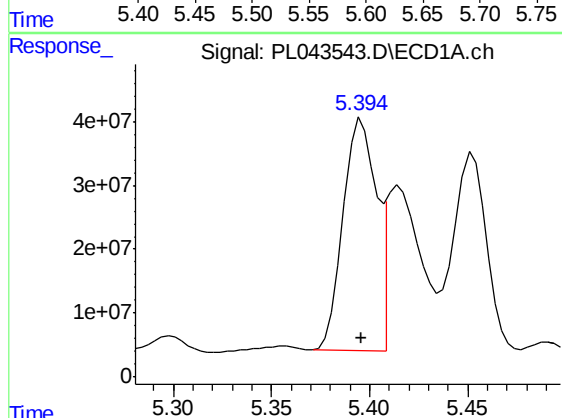


#25 Chlordane-3

R.T.: 5.396 min
Delta R.T.: 0.000 min
Response: 421060240
Conc: 500.00 ng/ml

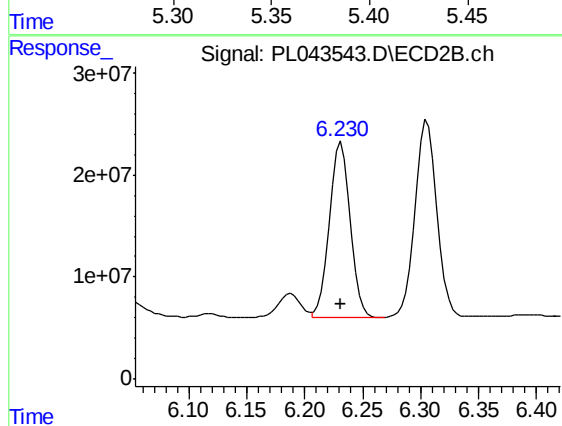

#25 Chlordane-3


R.T.: 6.232 min
Delta R.T.: 0.000 min
Response: 216504404
Conc: 500.00 ng/ml

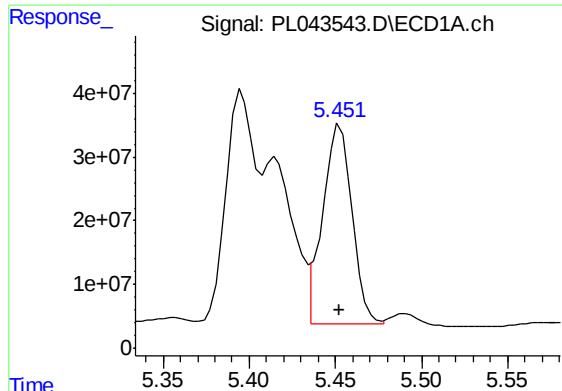

#26 Chlordane-4


R.T.: 5.453 min
Delta R.T.: 0.000 min
Response: 372241464
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

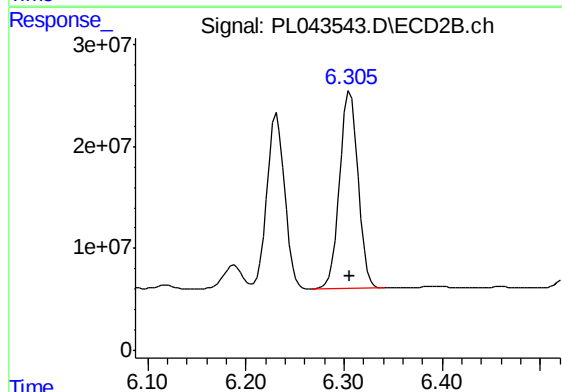


#26 Chlordane-4

R.T.: 6.306 min
Delta R.T.: 0.000 min
Response: 250937736
Conc: 500.00 ng/ml

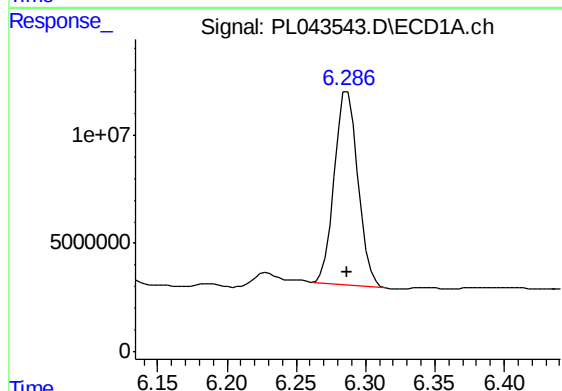


#27 Chlordane-5

R.T.: 6.287 min
Delta R.T.: 0.000 min
Response: 106032289
Conc: 500.00 ng/ml

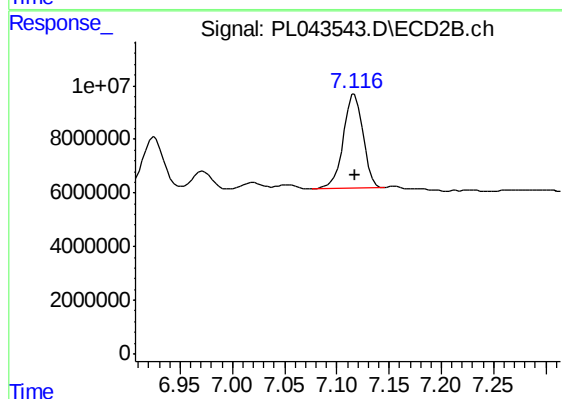

#27 Chlordane-5


R.T.: 7.117 min
Delta R.T.: 0.000 min
Response: 46048710
Conc: 500.00 ng/ml

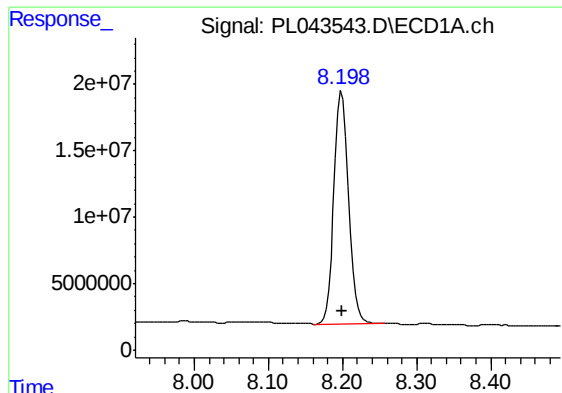

#28 Decachlorobiphenyl

R.T.: 8.199 min
Delta R.T.: 0.000 min
Response: 240429406
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

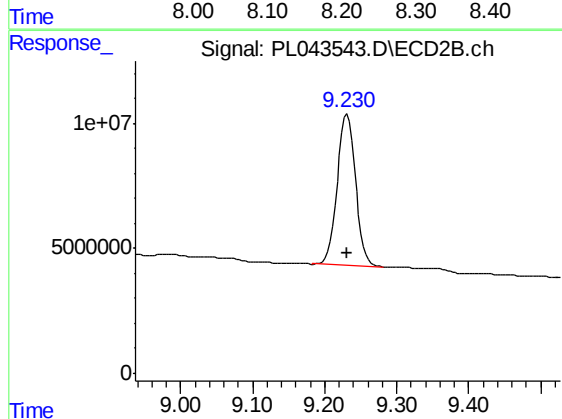

#28 Decachlorobiphenyl

R.T.: 9.231 min
Delta R.T.: 0.000 min
Response: 107315027
Conc: 50.00 ng/ml