

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010319\
 Data File : PL043570.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jan 2019 19:46
 Operator : AJ\SJ
 Sample : K1018-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TEST-PIT-D11-12

Manual Integrations
 APPROVED

Sohil
 1/4/2019 9:25:46 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 06:54:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 04 06:12:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.462	4.099	106.1E6	47417456	16.607m	16.229m
28)	SA Decachlor...	8.199	9.228	70720606	29739485	14.034	13.453m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010319\
Data File : PL043570.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jan 2019 19:46
Operator : AJ\SJ
Sample : K1018-02
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TEST-PIT-D11-12


Manual Integrations
APPROVED

Sohil
1/4/2019 9:25:46 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 06:54:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
Quant Title : GC Extractables
QLast Update : Fri Jan 04 06:12:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

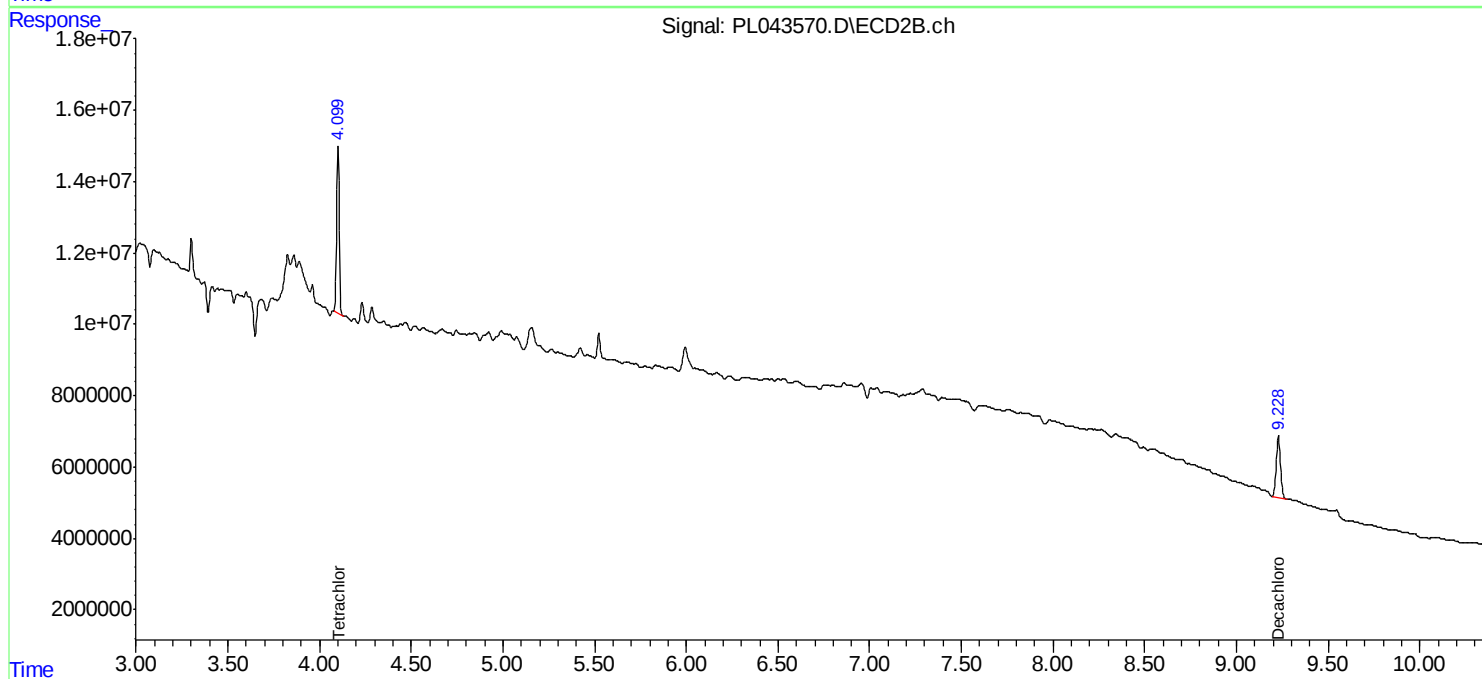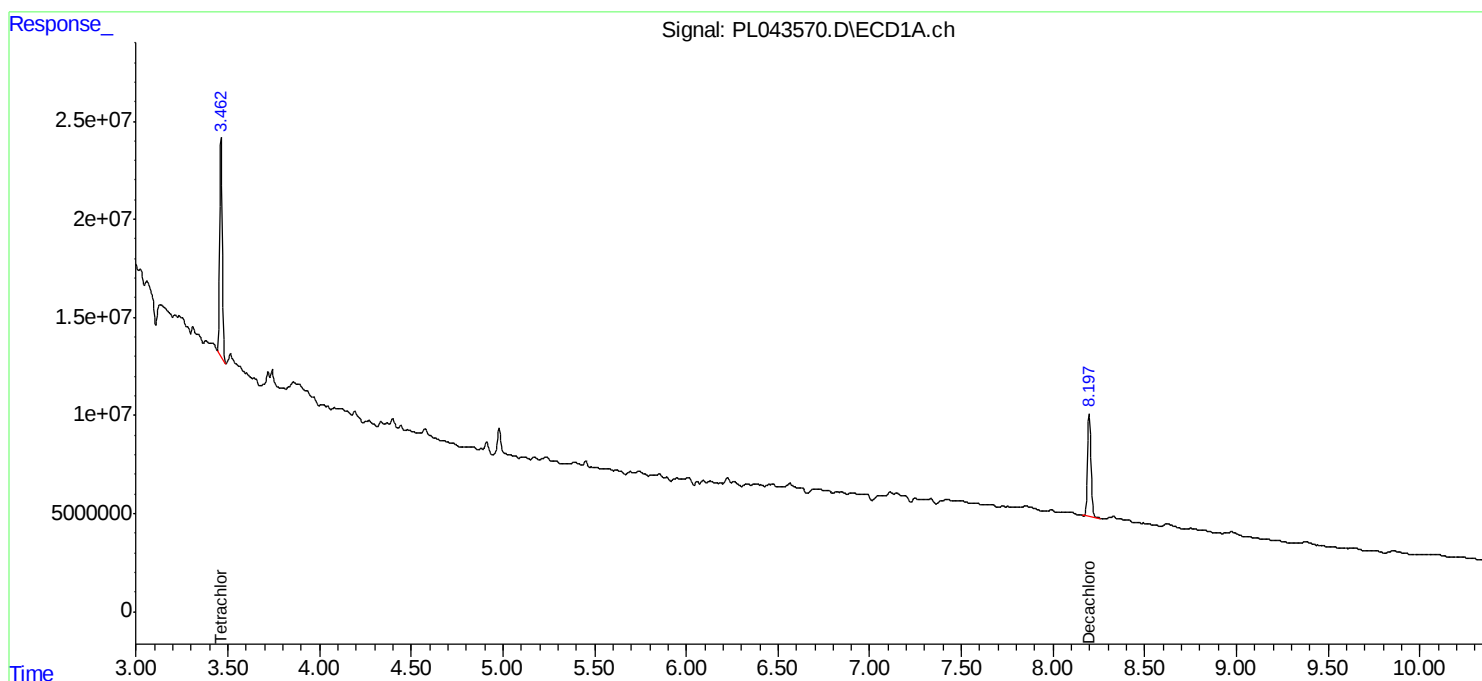

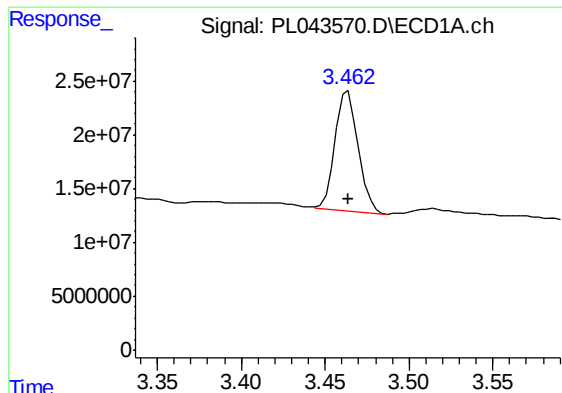


#1 Tetrachloro-m-xylene

R.T.: 3.462 min
Delta R.T.: -0.002 min
Response: 106103633
Conc: 16.61 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TEST-PIT-D11-12


Manual Integrations
APPROVED

Sohil
1/4/2019 9:25:46 AM

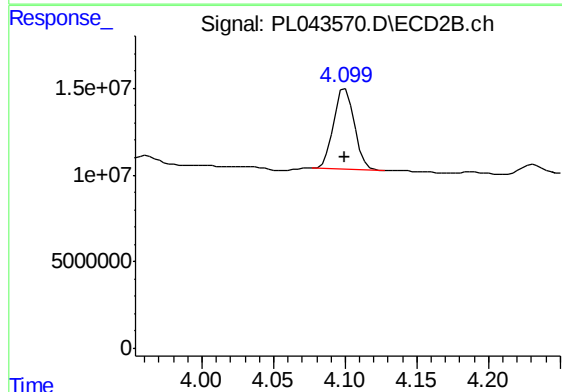


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: -0.001 min
Response: 47417456
Conc: 16.23 ng/ml m

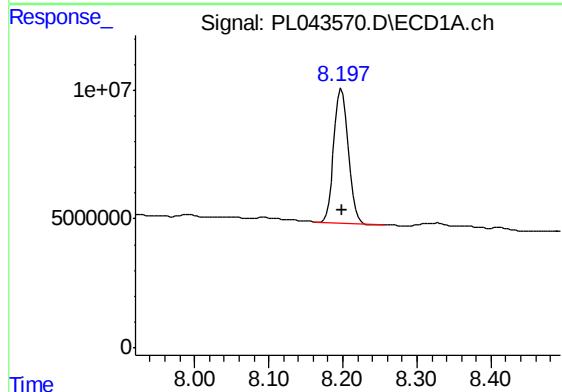

#28 Decachlorobiphenyl

R.T.: 8.199 min
Delta R.T.: 0.000 min
Response: 70720606
Conc: 14.03 ng/ml

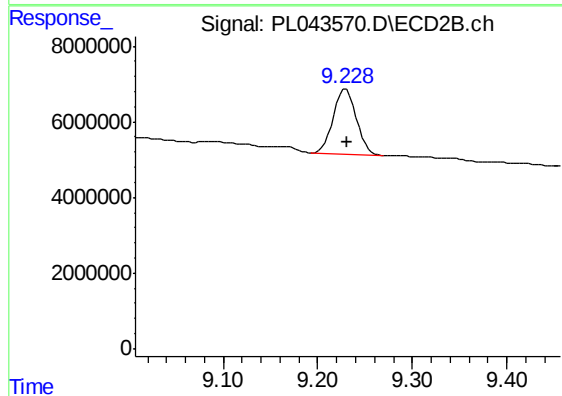

#28 Decachlorobiphenyl

R.T.: 9.228 min
Delta R.T.: -0.003 min
Response: 29739485
Conc: 13.45 ng/ml m