

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010319\
 Data File : PL043571.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jan 2019 20:01
 Operator : AJ\SJ
 Sample : K1023-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PURGE-WATER

Manual Integrations
 APPROVED

Sohil
 1/10/2019 8:38:23 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 06:55:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 04 06:12:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.465	4.120	9980623	2256660	1.562m	0.772m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010319\
Data File : PL043571.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jan 2019 20:01
Operator : AJ\SJ
Sample : K1023-01
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PURGE-WATER


Manual Integrations
APPROVED

Sohil
1/10/2019 8:38:23 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 06:55:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
Quant Title : GC Extractables
QLast Update : Fri Jan 04 06:12:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

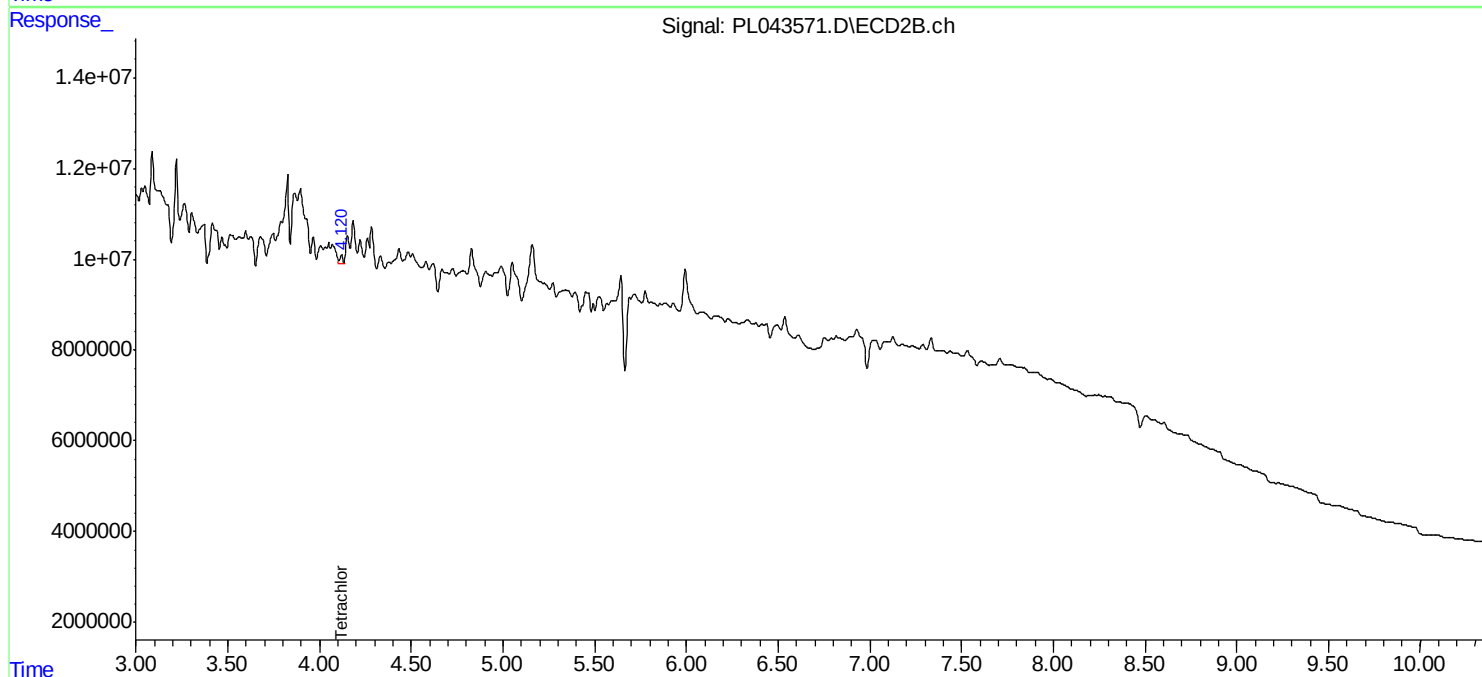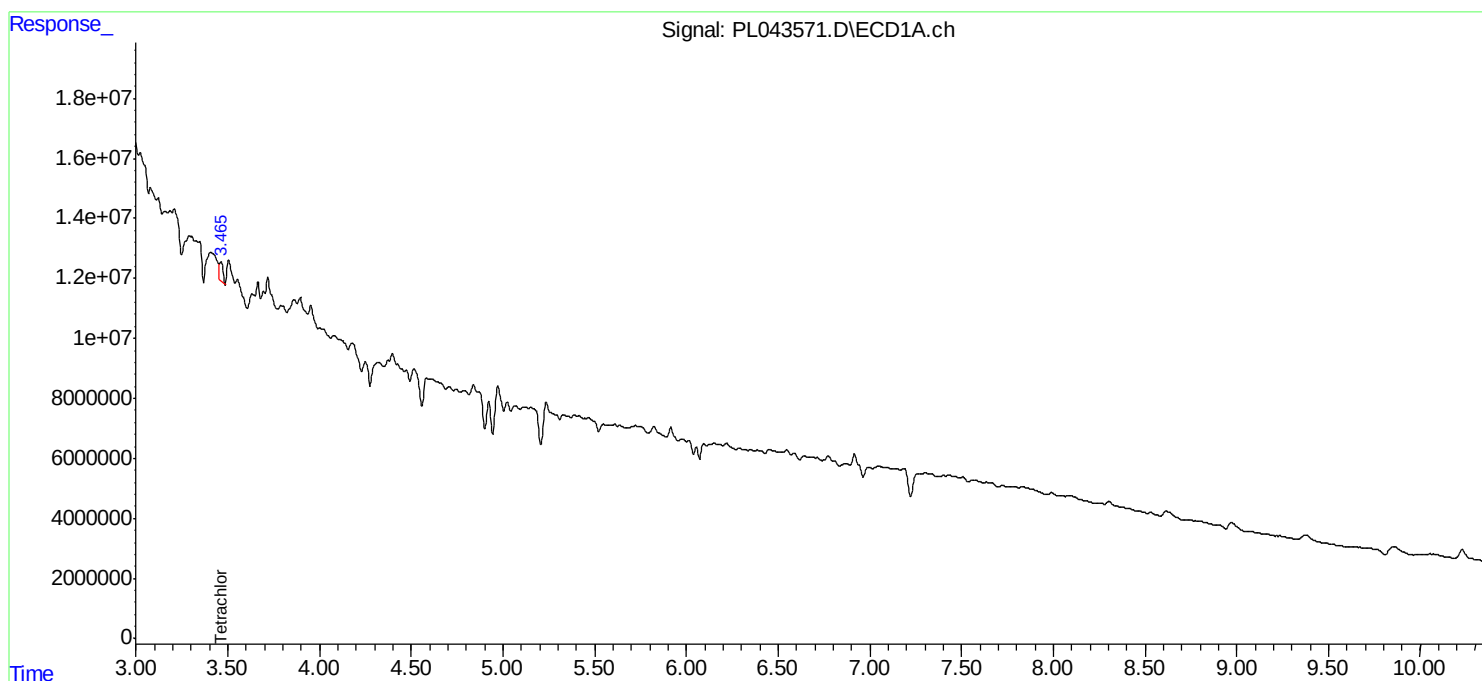

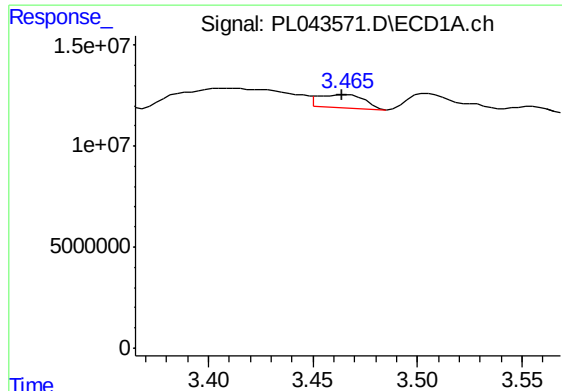


#1 Tetrachloro-m-xylene

R.T.: 3.465 min
Delta R.T.: 0.001 min
Response: 9980623
Conc: 1.56 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PURGE-WATER


Manual Integrations
APPROVED

Sohil
1/10/2019 8:38:23 AM

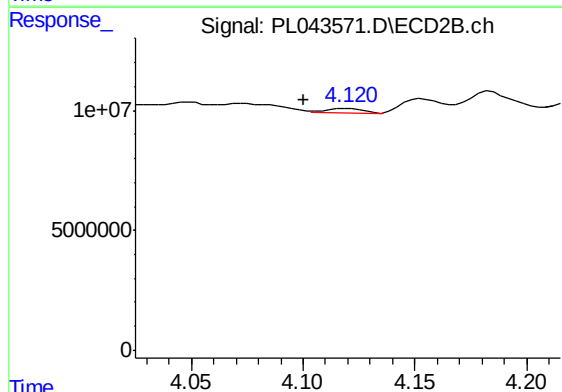


#1 Tetrachloro-m-xylene

R.T.: 4.120 min
Delta R.T.: 0.020 min
Response: 2256660
Conc: 0.77 ng/ml m

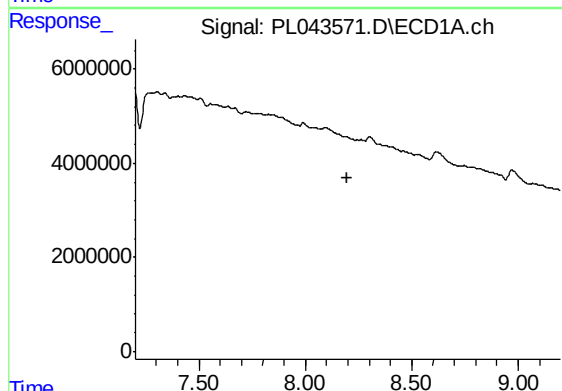

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.199 min
Response: 0
Conc: N.D.

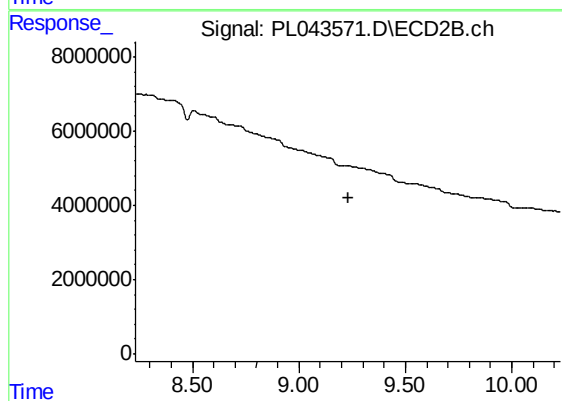

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.231 min
Response: 0
Conc: N.D.