

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010320\
 Data File : PL055501.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jan 2020 19:26
 Operator : AJ\MA
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 00:41:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010320.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 04 00:40:56 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.501	4.012	540.6E6	130.4E6	50.000	50.000
28)	SA Decachlor...	8.265	9.084	401.6E6	102.6E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.377	5.004	167.0E6	48053732	500.000	500.000
24)	Chlordane-2	4.879	5.470	178.9E6	51596596	500.000	500.000
25)	Chlordane-3	5.450	6.116	561.2E6	174.1E6	500.000	500.000
26)	Chlordane-4	5.508	6.190	467.2E6	207.6E6	500.000	500.000
27)	Chlordane-5	6.346	6.996	154.7E6	36237008	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010320\
Data File : PL055501.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jan 2020 19:26
Operator : AJ\MA
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 00:41:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010320.M
Quant Title : GC Extractables
QLast Update : Sat Jan 04 00:40:56 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

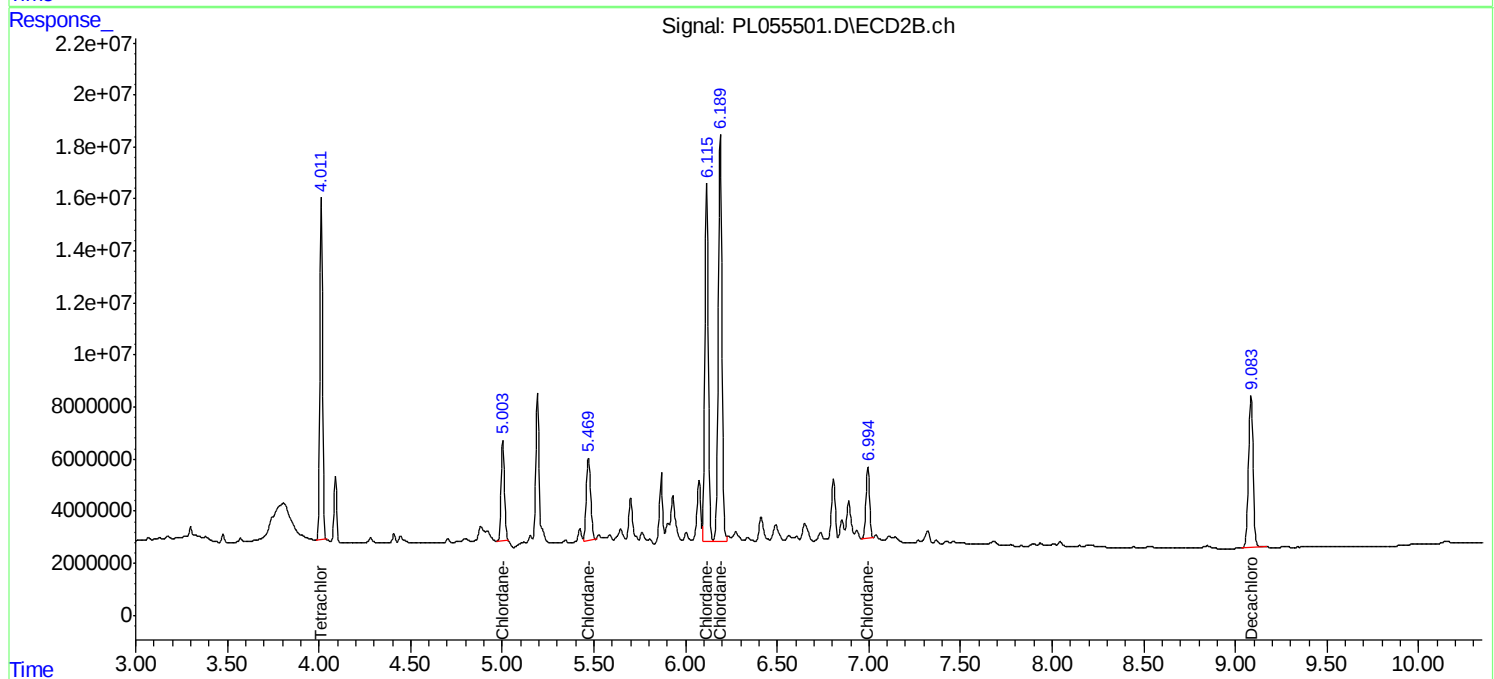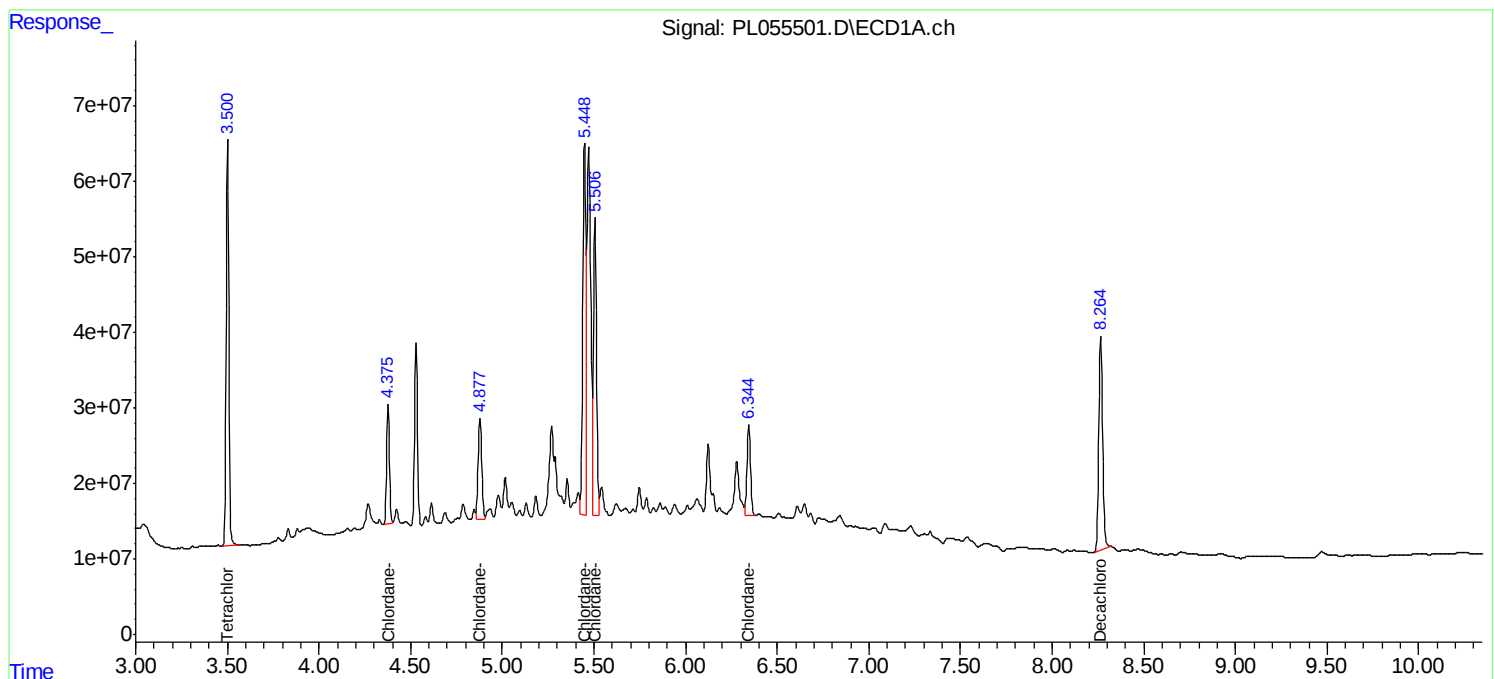


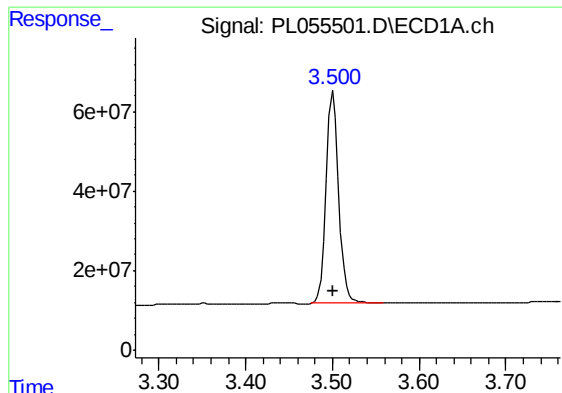

#1 Tetrachloro-m-xylene


R.T.: 3.501 min
Delta R.T.: 0.000 min
Response: 540633254
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

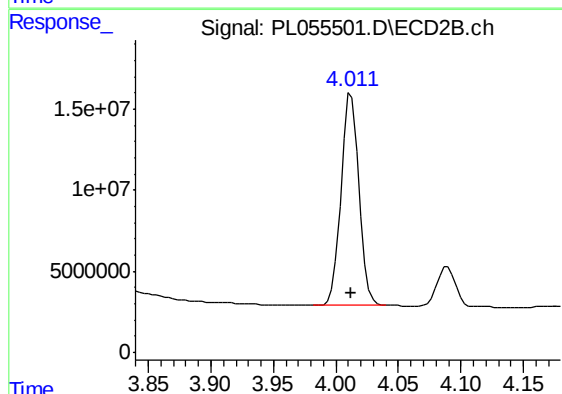


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 130440893
Conc: 50.00 ng/ml

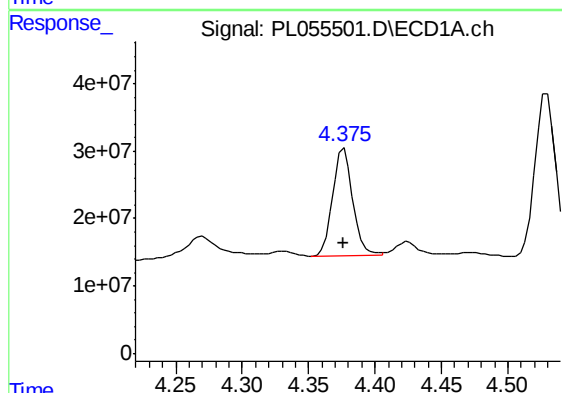


#23 Chlordane-1

R.T.: 4.377 min
Delta R.T.: 0.000 min
Response: 166974432
Conc: 500.00 ng/ml

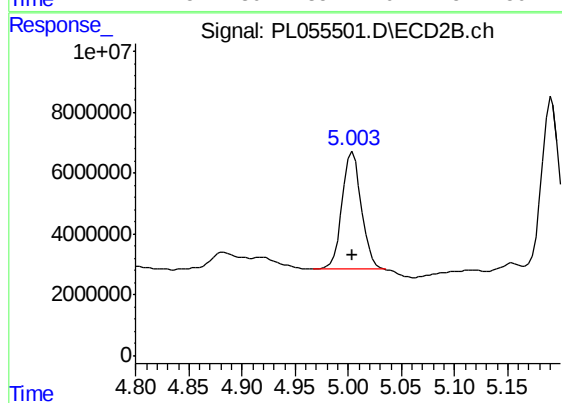

#23 Chlordane-1


R.T.: 5.004 min
Delta R.T.: 0.000 min
Response: 48053732
Conc: 500.00 ng/ml

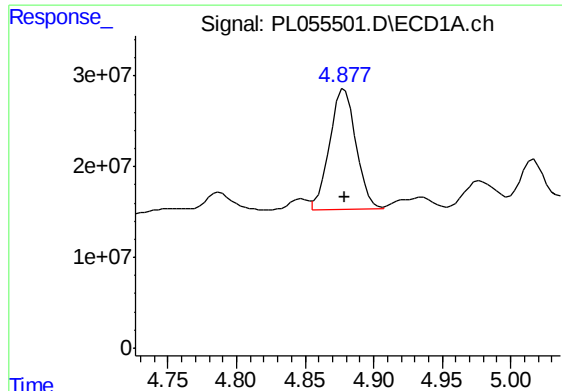

#24 Chlordane-2


R.T.: 4.879 min
Delta R.T.: 0.000 min
Response: 178942250
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

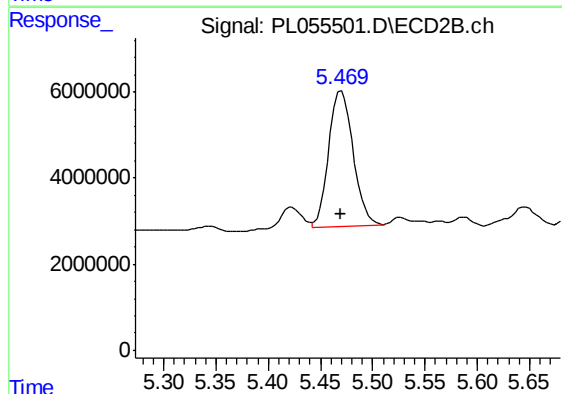


#24 Chlordane-2

R.T.: 5.470 min
Delta R.T.: 0.000 min
Response: 51596596
Conc: 500.00 ng/ml

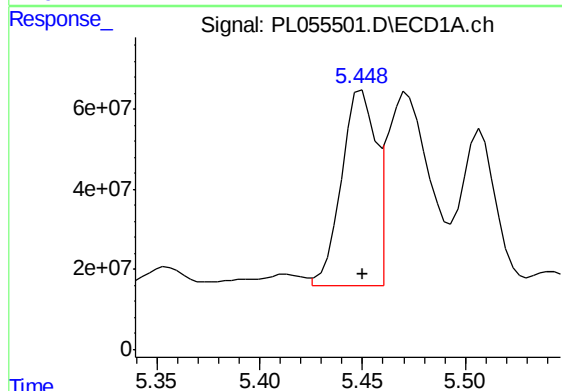


#25 Chlordane-3

R.T.: 5.450 min
Delta R.T.: 0.000 min
Response: 561195746
Conc: 500.00 ng/ml

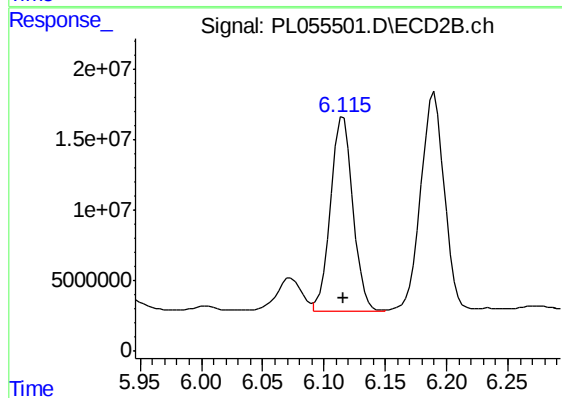

#25 Chlordane-3


R.T.: 6.116 min
Delta R.T.: 0.000 min
Response: 174065076
Conc: 500.00 ng/ml

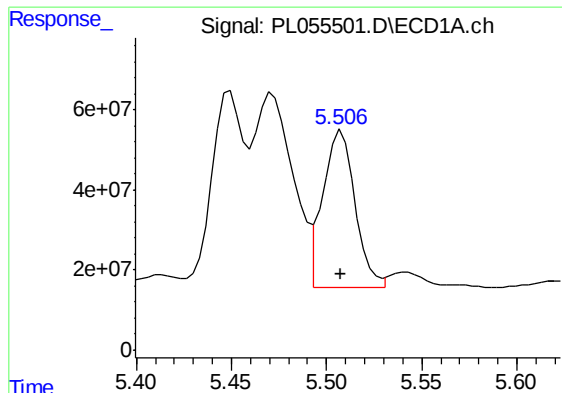

#26 Chlordane-4


R.T.: 5.508 min
Delta R.T.: 0.000 min
Response: 467200887
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

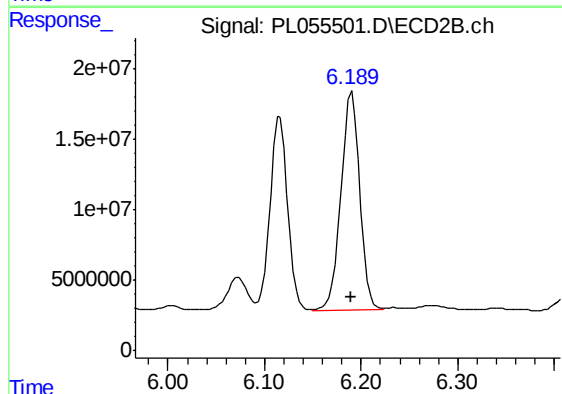


#26 Chlordane-4

R.T.: 6.190 min
Delta R.T.: 0.000 min
Response: 207600348
Conc: 500.00 ng/ml

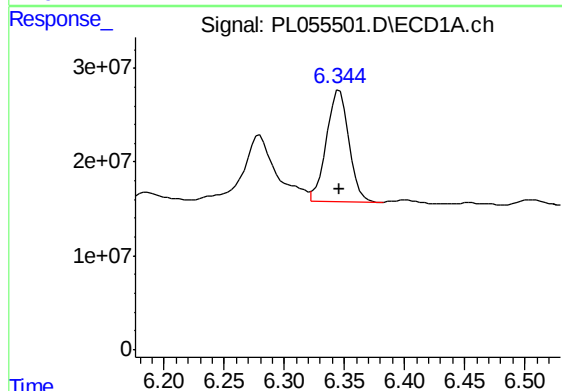


#27 Chlordane-5

R.T.: 6.346 min
Delta R.T.: 0.000 min
Response: 154721159
Conc: 500.00 ng/ml

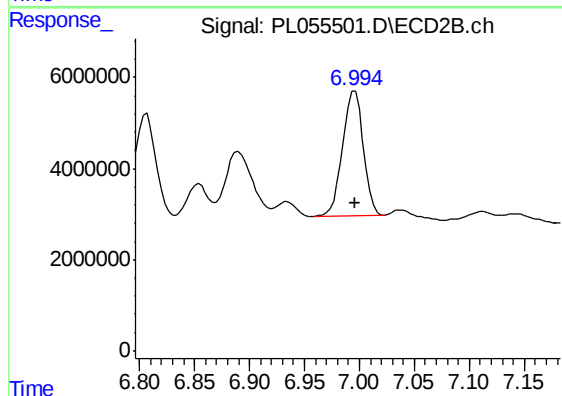

#27 Chlordane-5


R.T.: 6.996 min
Delta R.T.: 0.000 min
Response: 36237008
Conc: 500.00 ng/ml

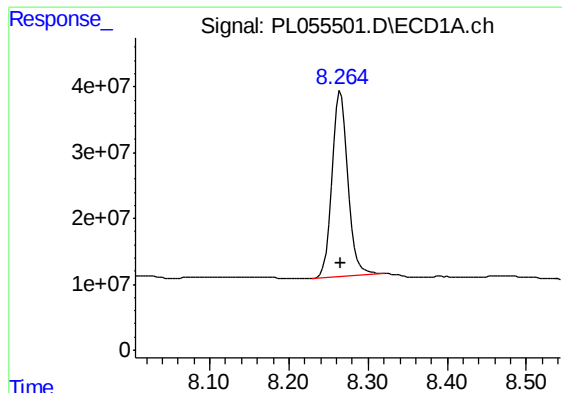

#28 Decachlorobiphenyl

R.T.: 8.265 min
Delta R.T.: 0.000 min
Response: 401594885
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

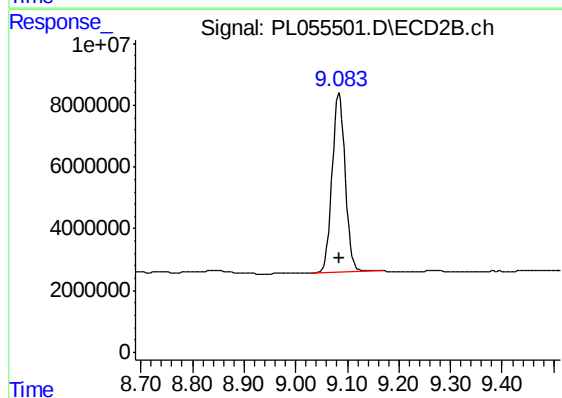

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.000 min
Response: 102612723
Conc: 50.00 ng/ml