

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010320\
 Data File : PL055516.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jan 2020 23:26
 Operator : AJ\MA
 Sample : L1010-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-01-010220

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 01:15:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010320.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 04 01:07:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.502	4.013	173.1E6	55473405	17.965	19.614
28)	SA Decachlor...	8.265	9.086	201.0E6	51326309	23.764	23.175
Target Compounds							
7)	B delta-BHC	0.000	5.048f	0	3070603	N.D.	1.054 #
27)	Chlordane-5	6.374f	0.000	14033166	0	45.350	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010320\
Data File : PL055516.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jan 2020 23:26
Operator : AJ\MA
Sample : L1010-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OK-01-010220

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 01:15:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010320.M
Quant Title : GC Extractables
QLast Update : Sat Jan 04 01:07:28 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

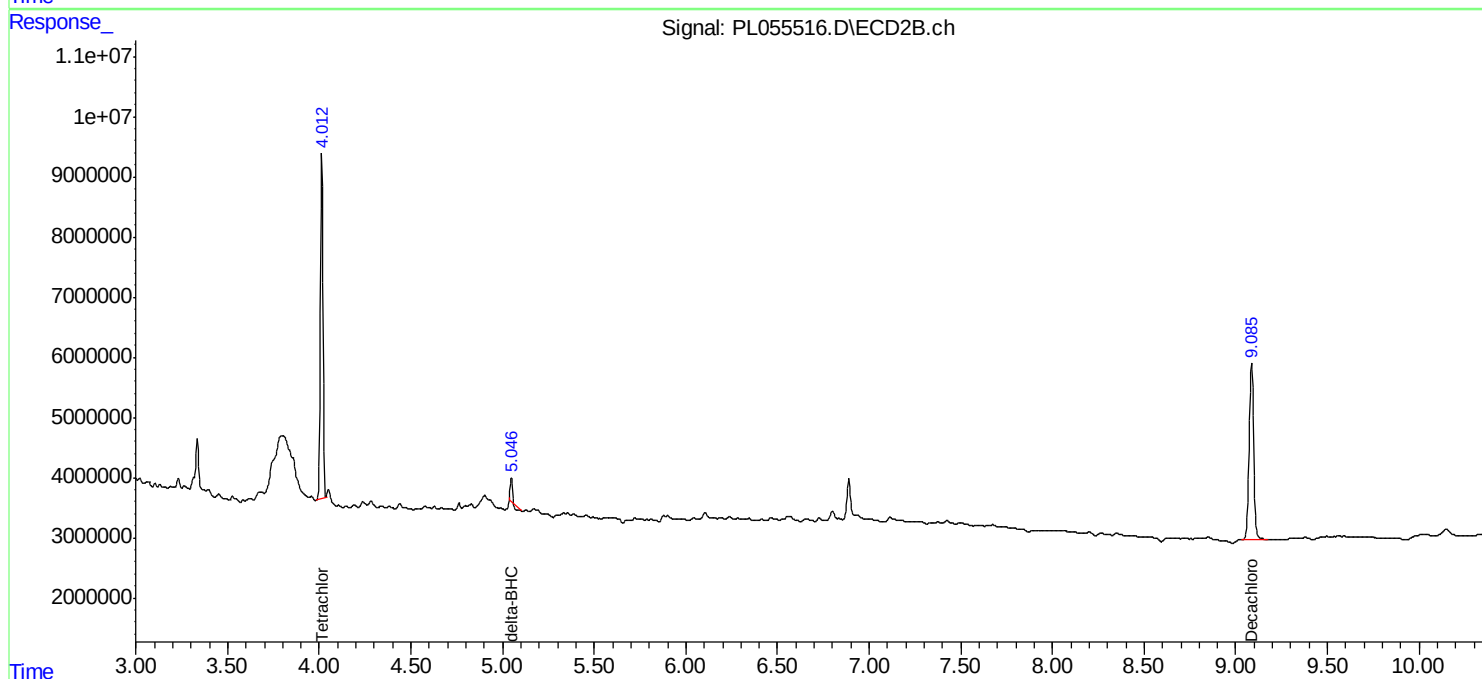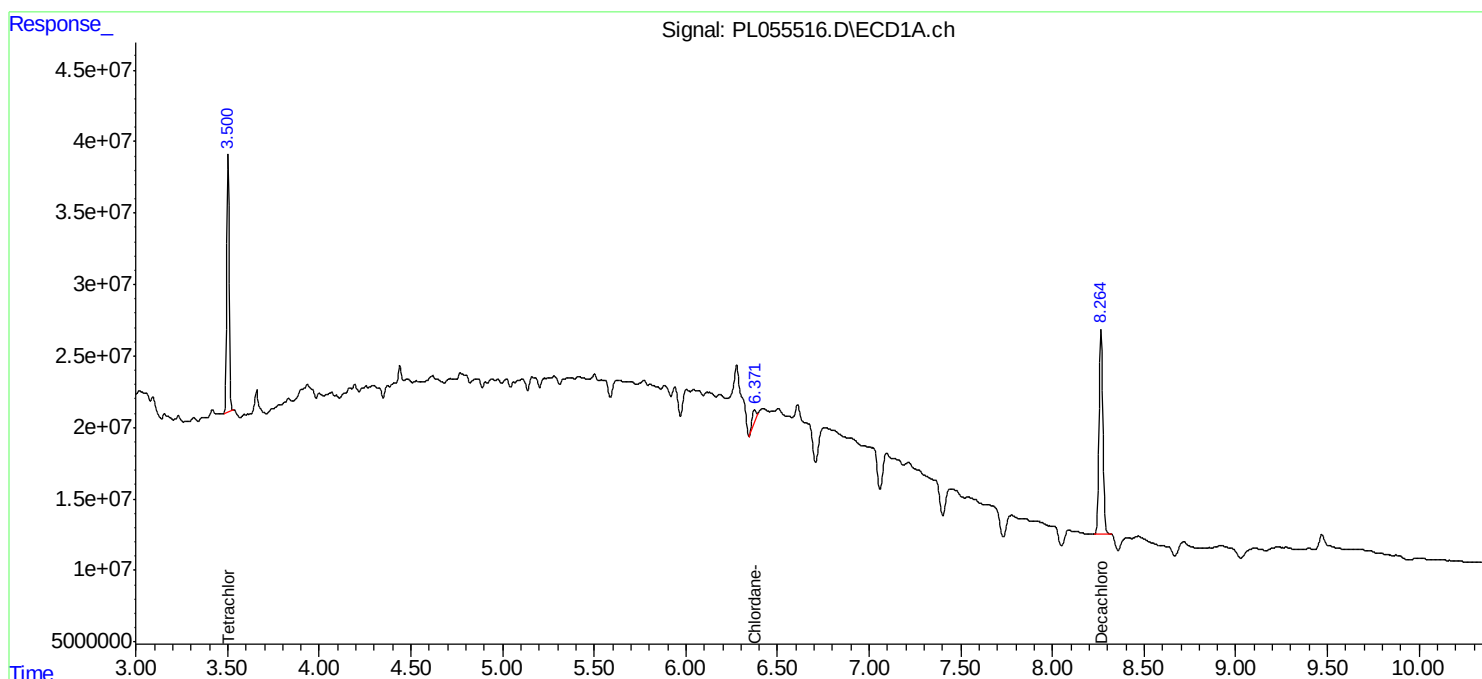


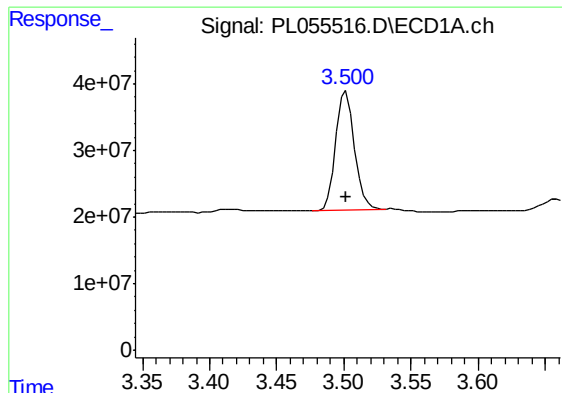

#1 Tetrachloro-m-xylene


R.T.: 3.502 min
Delta R.T.: 0.000 min
Response: 173050846
Conc: 17.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-01-010220

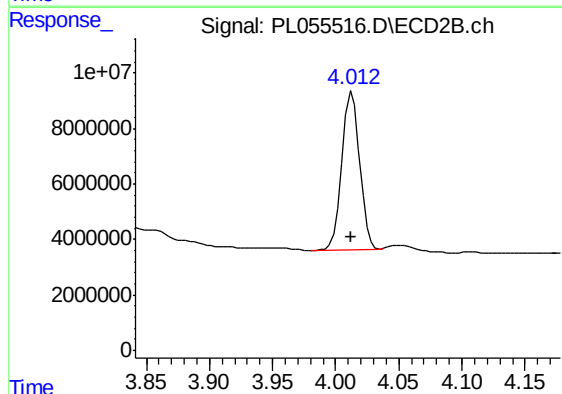


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 55473405
Conc: 19.61 ng/ml

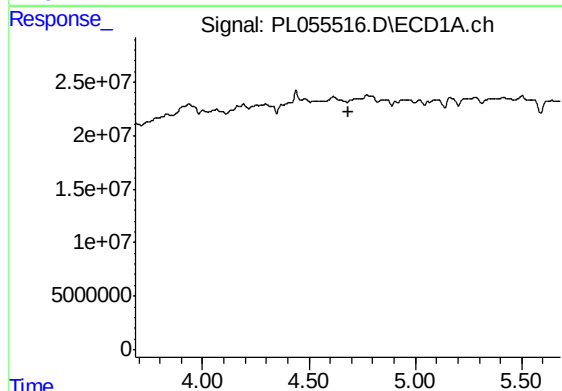


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.683 min
Response: 0
Conc: N.D.

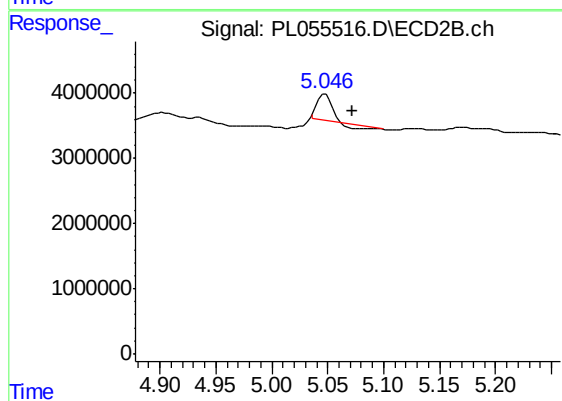

#7 delta-BHC


R.T.: 5.048 min
Delta R.T.: -0.025 min
Response: 3070603
Conc: 1.05 ng/ml

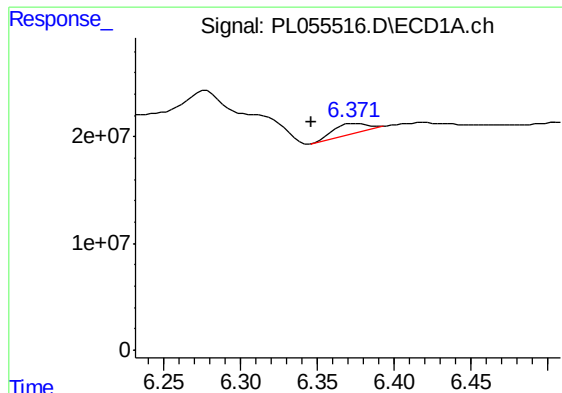

#27 Chlordane-5


R.T.: 6.374 min
Delta R.T.: 0.029 min
Response: 14033166
Conc: 45.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-01-010220

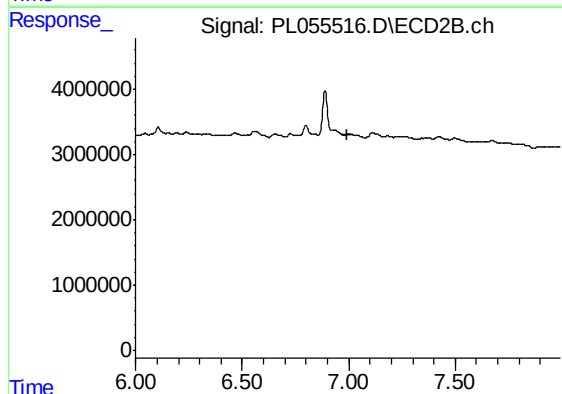


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.996 min
Response: 0
Conc: N.D.

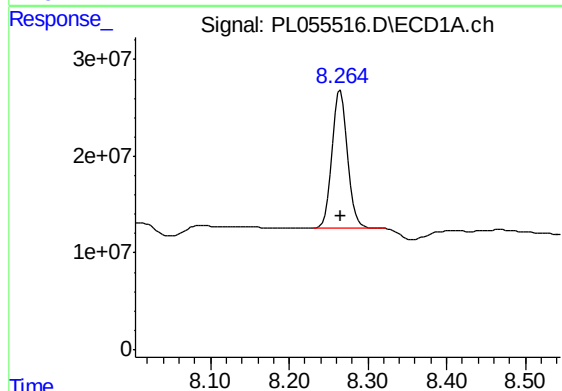

#28 Decachlorobiphenyl

R.T.: 8.265 min
Delta R.T.: -0.001 min
Response: 201006972
Conc: 23.76 ng/ml

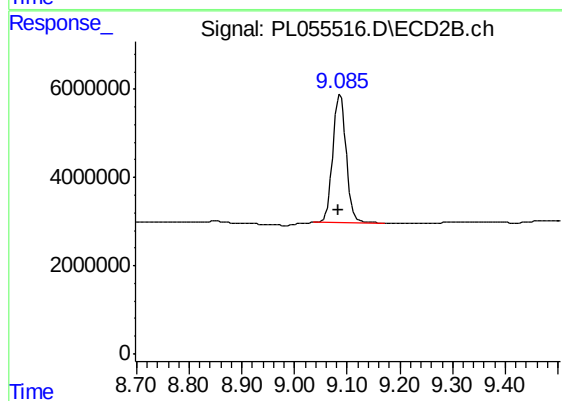

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: 0.002 min
Response: 51326309
Conc: 23.18 ng/ml