

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010320\
 Data File : PL055529.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2020 02:43
 Operator : AJ\MA
 Sample : L1009-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NB-08-010220

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 03:12:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010320.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 04 01:07:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.502	4.013	128.0E6	33860731	13.288	11.972
28)	SA Decachlor...	8.265	9.088	110.6E6	30452987	13.078	13.750
Target Compounds							
11)	B alpha-Chl...	0.000	6.191	0	5592299	N.D.	1.933 #
26)	Chlordane-4	0.000	6.191	0	5592299	N.D.	13.469 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010320\
Data File : PL055529.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2020 02:43
Operator : AJ\MA
Sample : L1009-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
NB-08-010220

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 03:12:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010320.M
Quant Title : GC Extractables
QLast Update : Sat Jan 04 01:07:28 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

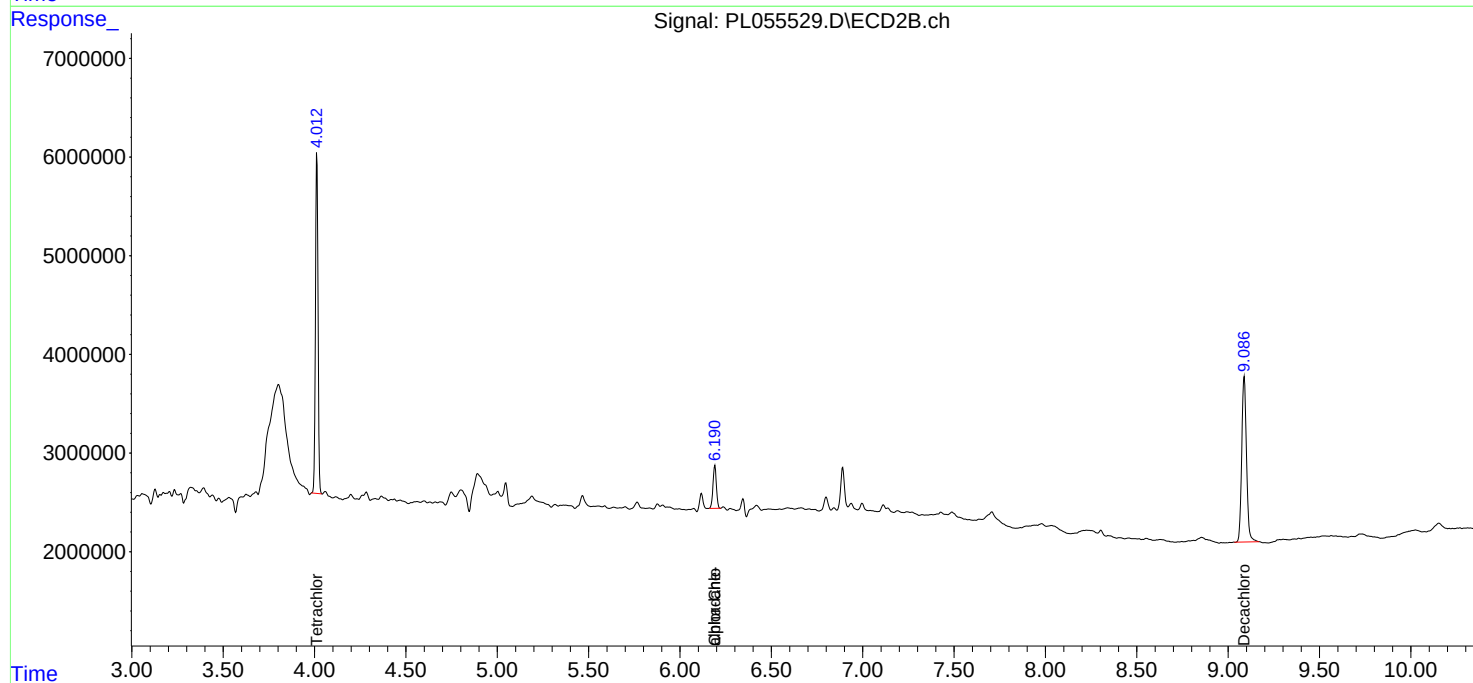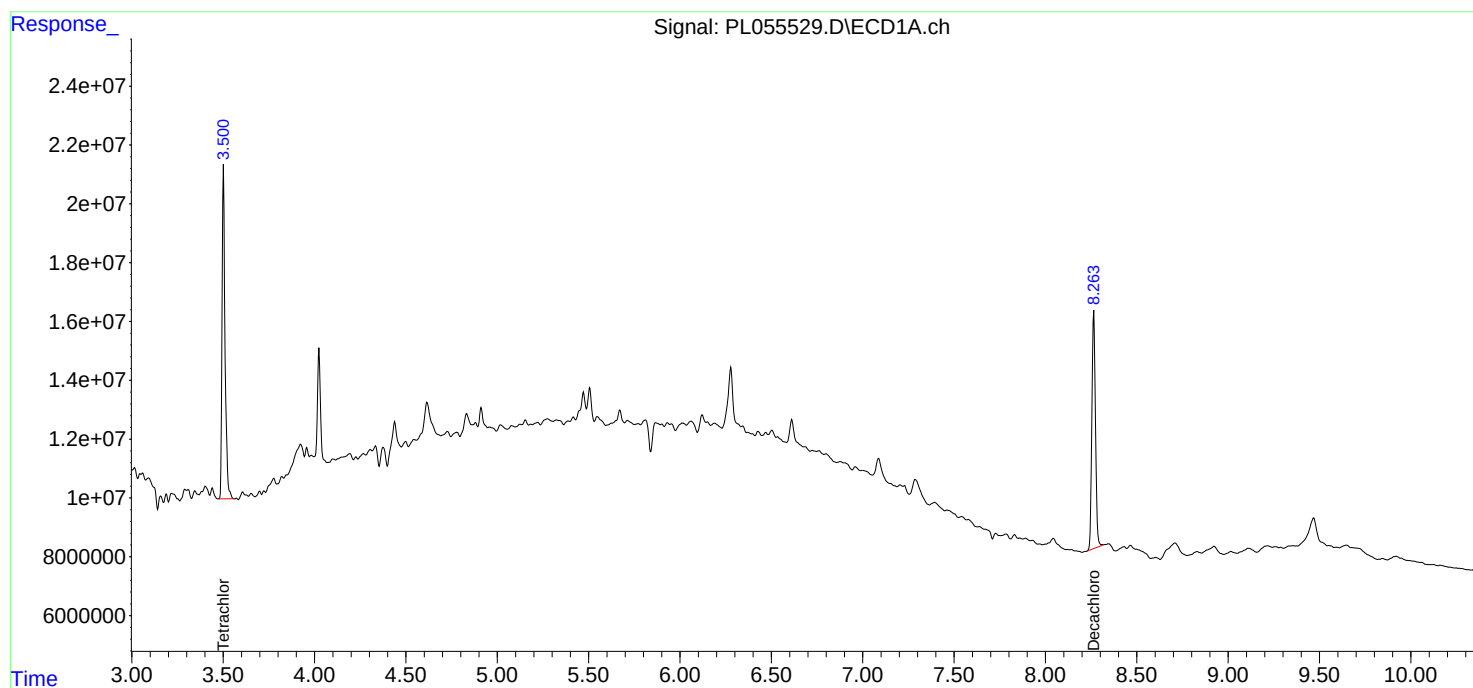


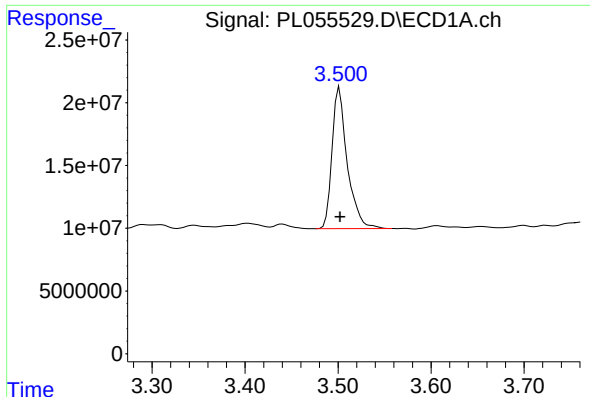

#1 Tetrachloro-m-xylene


R.T.: 3.502 min
Delta R.T.: 0.000 min
Response: 128001991
Conc: 13.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
NB-08-010220

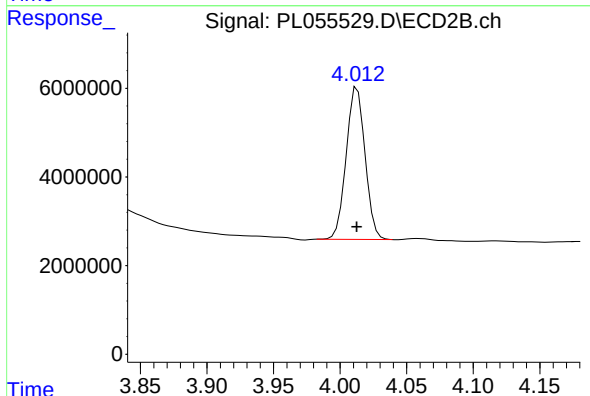


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 33860731
Conc: 11.97 ng/ml

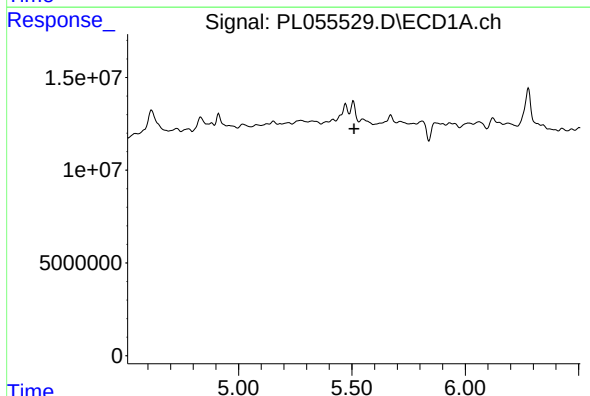


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.509 min
Response: 0
Conc: N.D.

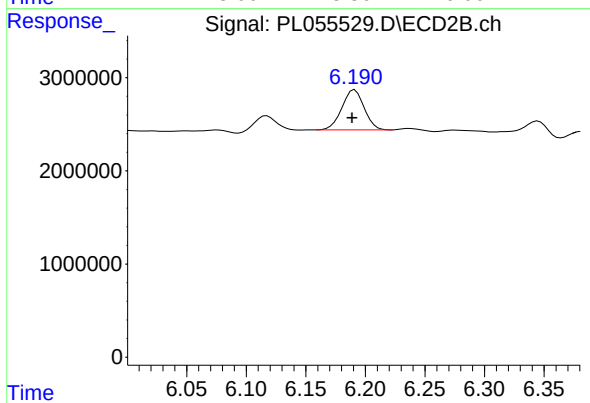

#11 alpha-Chlordane


R.T.: 6.191 min
Delta R.T.: 0.002 min
Response: 5592299
Conc: 1.93 ng/ml

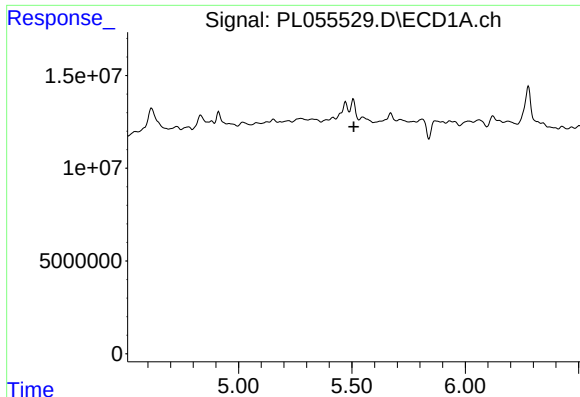

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.508 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
NB-08-010220

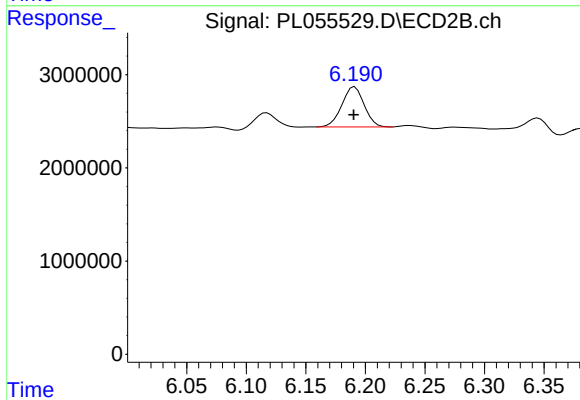


#26 Chlordane-4

R.T.: 6.191 min
Delta R.T.: 0.000 min
Response: 5592299
Conc: 13.47 ng/ml

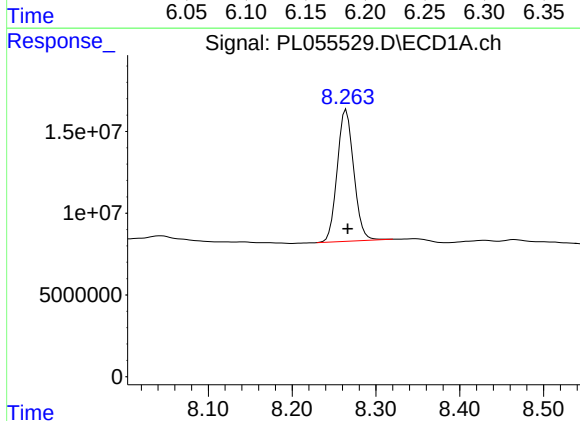

#28 Decachlorobiphenyl

R.T.: 8.265 min
Delta R.T.: -0.002 min
Response: 110618498
Conc: 13.08 ng/ml

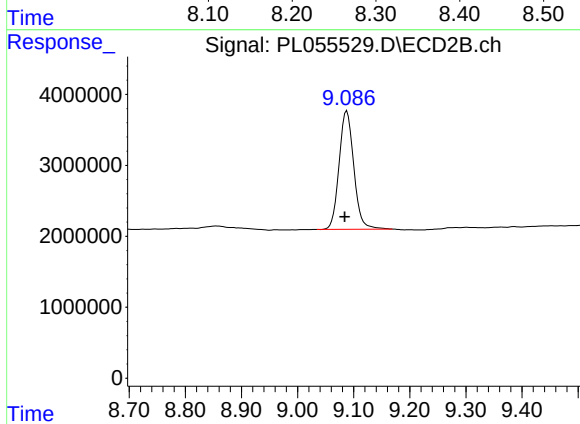

#28 Decachlorobiphenyl

R.T.: 9.088 min
Delta R.T.: 0.004 min
Response: 30452987
Conc: 13.75 ng/ml