

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010320\
 Data File : PL055531.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2020 03:11
 Operator : AJ\MA
 Sample : L1011-02
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MC-010220-0-2-COMP-B3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 03:35:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010320.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 04 01:07:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.502	4.013	99989952	31461207	10.380	11.124
28)	SA Decachlor...	8.264	9.086	86142628	23901155	10.184	10.792
Target Compounds							
10)	B gamma-Chl...	5.445	6.088f	17517542	8485378	1.366	2.969 #
11)	B alpha-Chl...	0.000	6.189	0	10367642	N.D.	3.583 #
12)	B 4,4'-DDE	5.671	6.347	2203.4E6	511.6E6	189.808	187.712
14)	MA Endrin	6.062	6.742f	48317121	12439563	4.159	5.162
16)	A 4,4'-DDD	6.187	6.840	22008339	9626888	2.645	4.482 #
17)	MA 4,4'-DDT	6.427	7.138	179.9E6	48002550	20.752	19.866
25)	Chlordane-3	5.445	6.088f	17517542	8485378	15.607	24.374 #
26)	Chlordane-4	0.000	6.189	0	10367642	N.D.	24.970 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010320\
Data File : PL055531.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2020 03:11
Operator : AJ\MA
Sample : L1011-02
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MC-010220-0-2-COMP-B3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 03:35:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010320.M
Quant Title : GC Extractables
QLast Update : Sat Jan 04 01:07:28 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

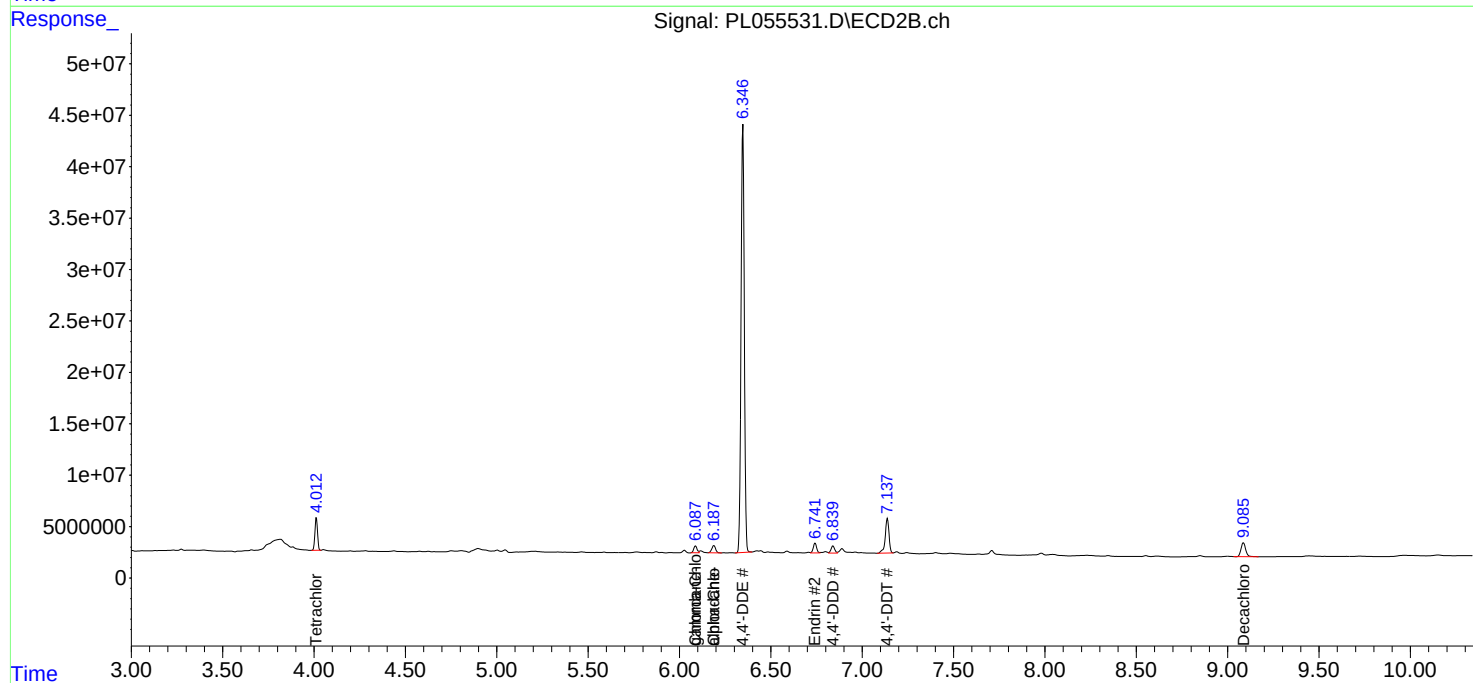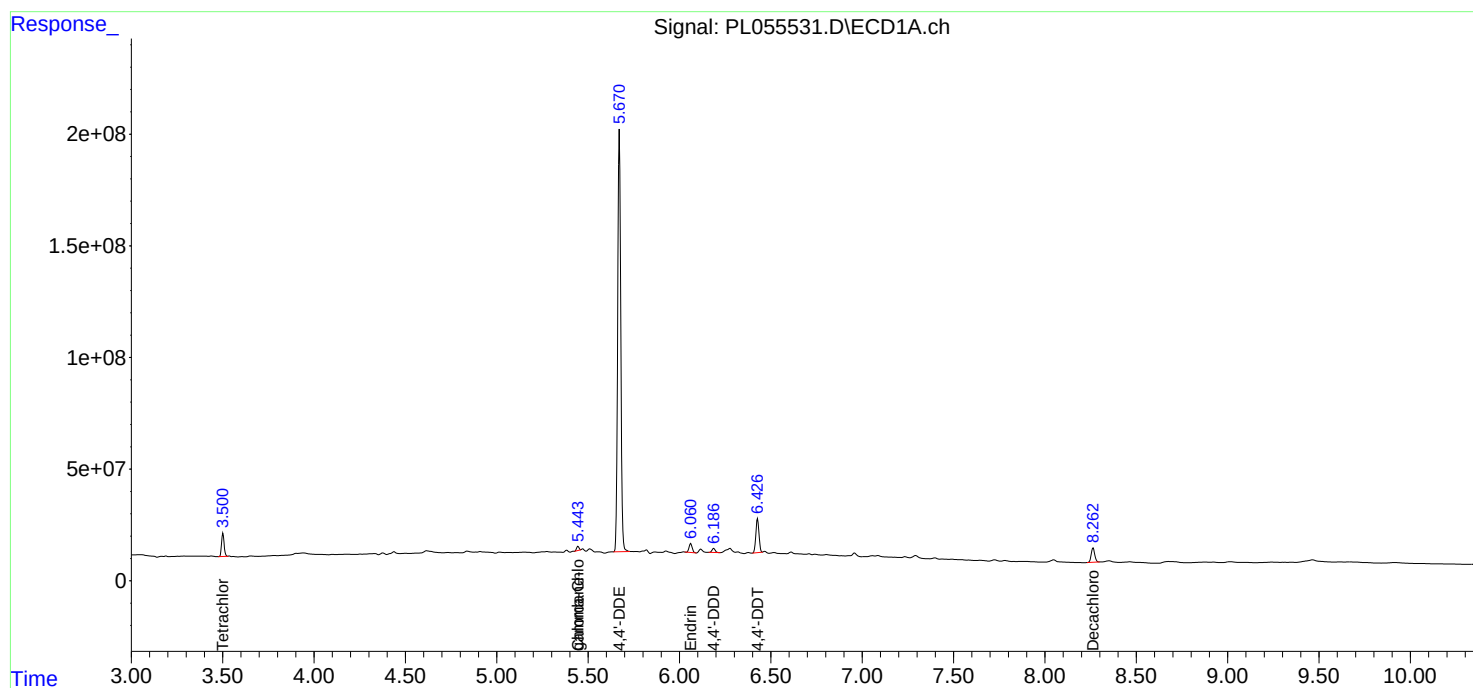


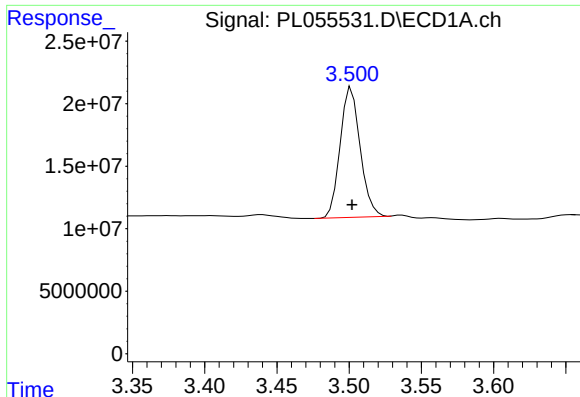

#1 Tetrachloro-m-xylene


R.T.: 3.502 min
Delta R.T.: 0.000 min
Response: 99989952
Conc: 10.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
MC-010220-0-2-COMP-B3

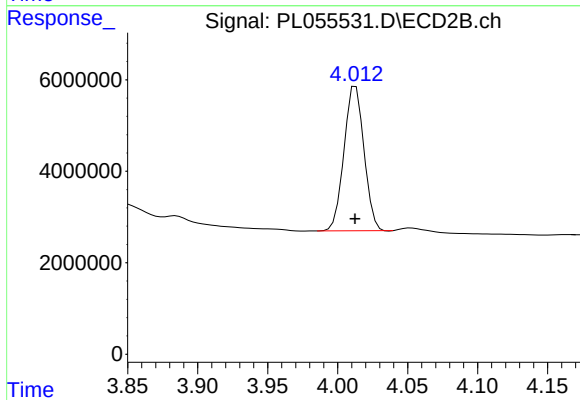


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 31461207
Conc: 11.12 ng/ml

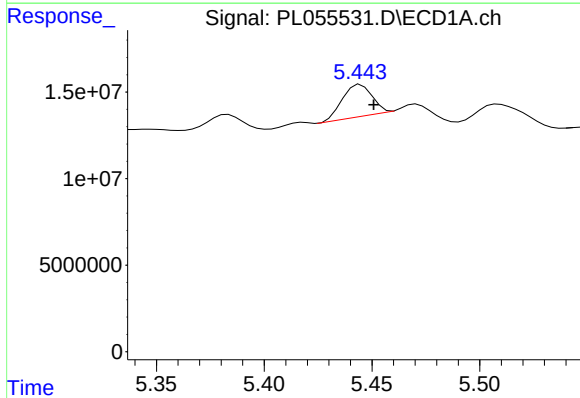


#10 gamma-Chlordane

R.T.: 5.445 min
Delta R.T.: -0.006 min
Response: 17517542
Conc: 1.37 ng/ml

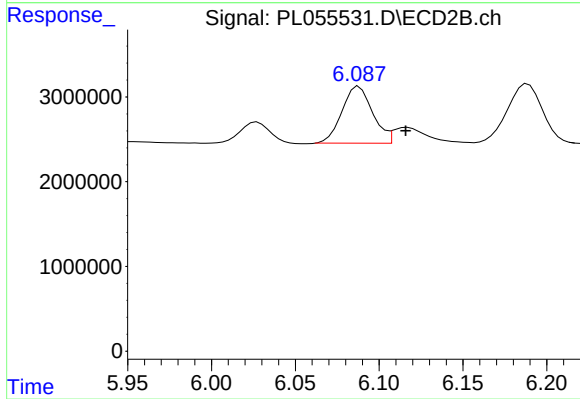

#10 gamma-Chlordane


R.T.: 6.088 min
Delta R.T.: -0.028 min
Response: 8485378
Conc: 2.97 ng/ml

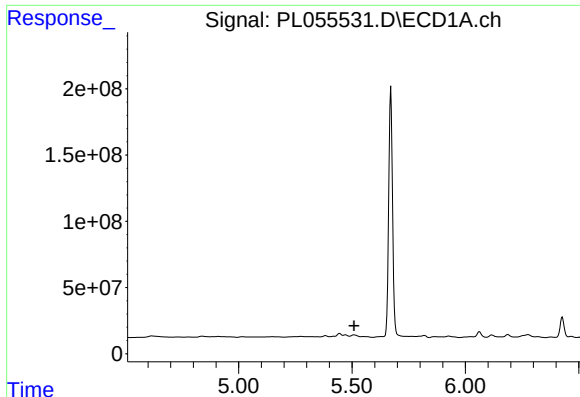

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
MC-010220-0-2-COMP-B3

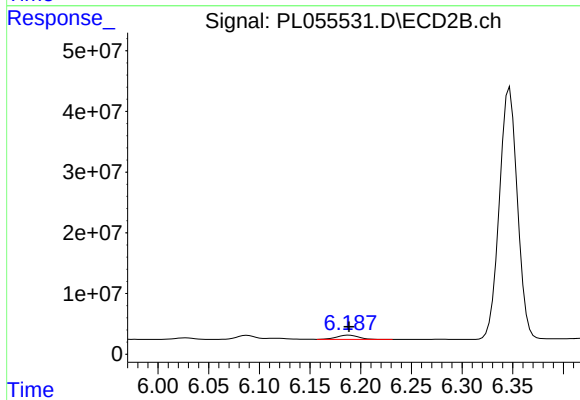


#11 alpha-Chlordane

R.T.: 6.189 min
Delta R.T.: 0.000 min
Response: 10367642
Conc: 3.58 ng/ml

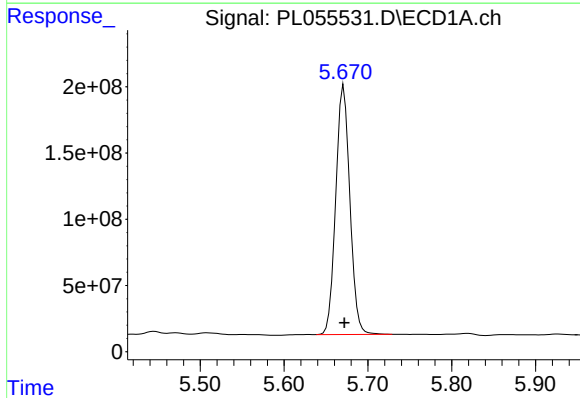


#12 4,4'-DDE

R.T.: 5.671 min
Delta R.T.: 0.000 min
Response: 2203446337
Conc: 189.81 ng/ml

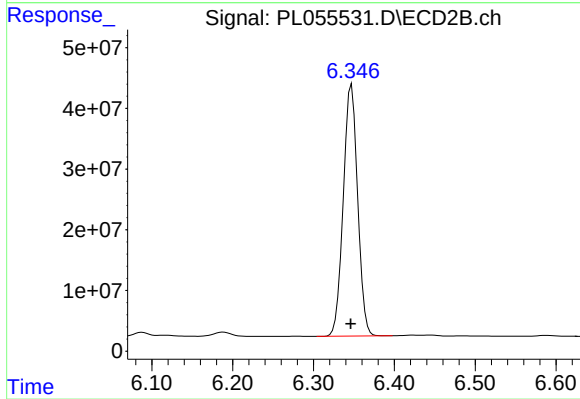

#12 4,4'-DDE


R.T.: 6.347 min
Delta R.T.: 0.001 min
Response: 511570061
Conc: 187.71 ng/ml

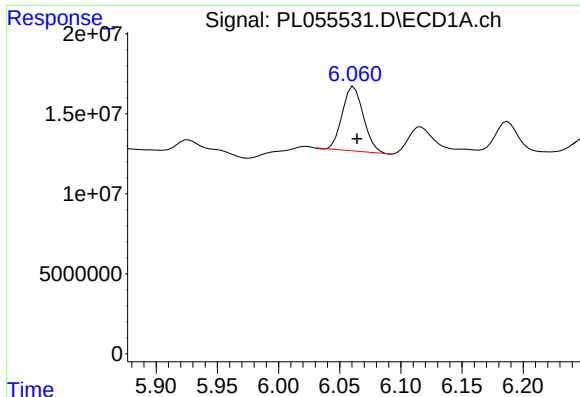

#14 Endrin


R.T.: 6.062 min
Delta R.T.: -0.002 min
Response: 48317121
Conc: 4.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
MC-010220-0-2-COMP-B3

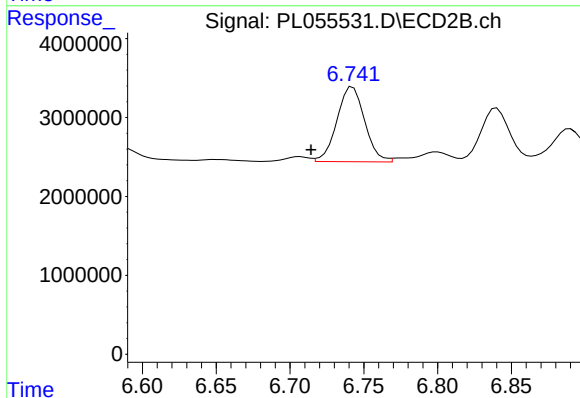


#14 Endrin

R.T.: 6.742 min
Delta R.T.: 0.028 min
Response: 12439563
Conc: 5.16 ng/ml

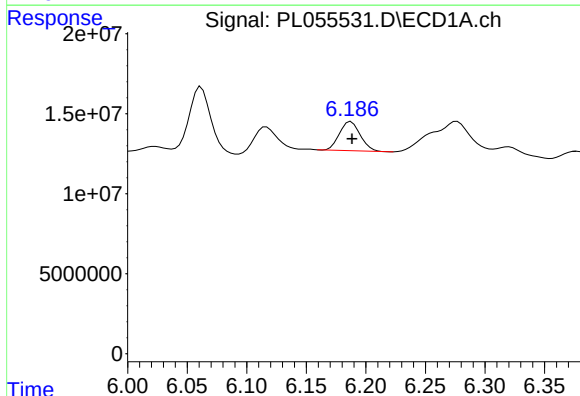


#16 4,4'-DDD

R.T.: 6.187 min
Delta R.T.: 0.000 min
Response: 22008339
Conc: 2.64 ng/ml

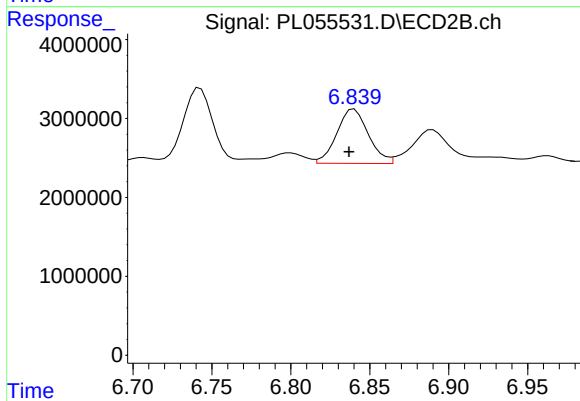

#16 4,4'-DDD


R.T.: 6.840 min
Delta R.T.: 0.003 min
Response: 9626888
Conc: 4.48 ng/ml

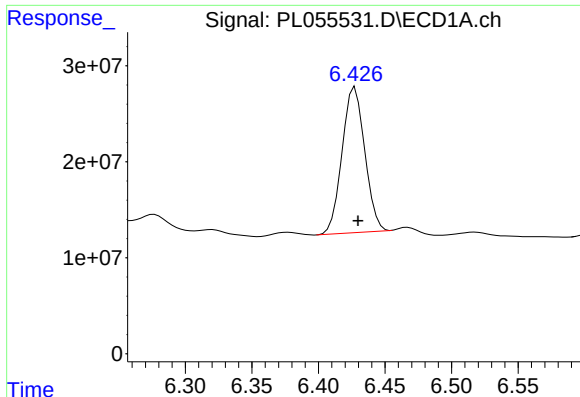

#17 4,4'-DDT


R.T.: 6.427 min
Delta R.T.: -0.002 min
Response: 179888750
Conc: 20.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
MC-010220-0-2-COMP-B3

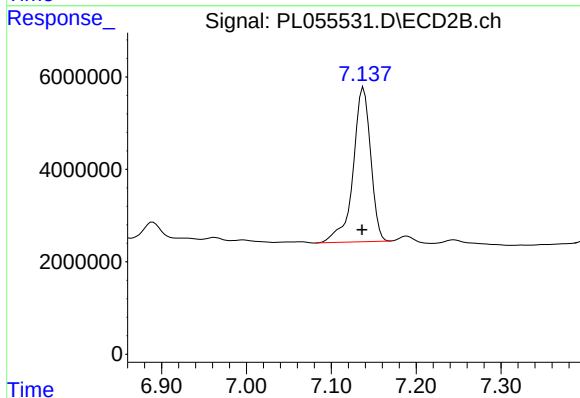


#17 4,4'-DDT

R.T.: 7.138 min
Delta R.T.: 0.002 min
Response: 48002550
Conc: 19.87 ng/ml

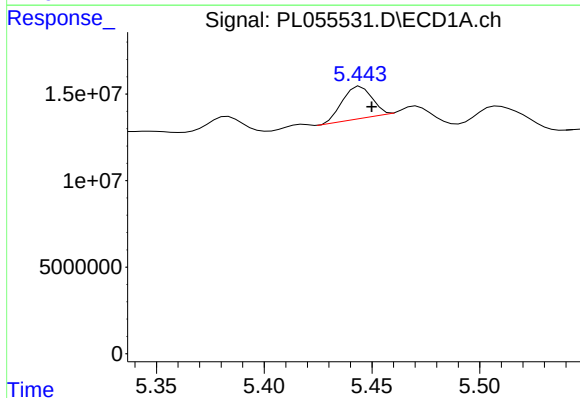


#25 Chlordane-3

R.T.: 5.445 min
Delta R.T.: -0.005 min
Response: 17517542
Conc: 15.61 ng/ml

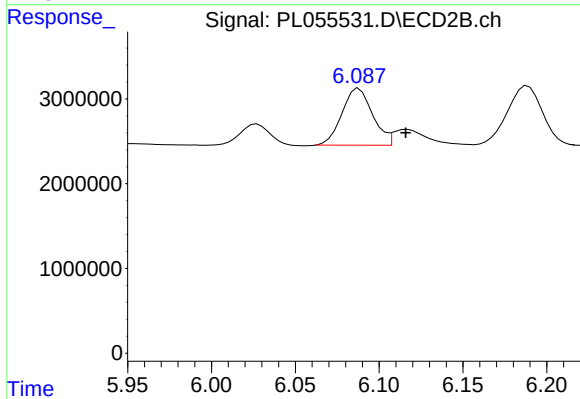

#25 Chlordane-3


R.T.: 6.088 min
Delta R.T.: -0.028 min
Response: 8485378
Conc: 24.37 ng/ml

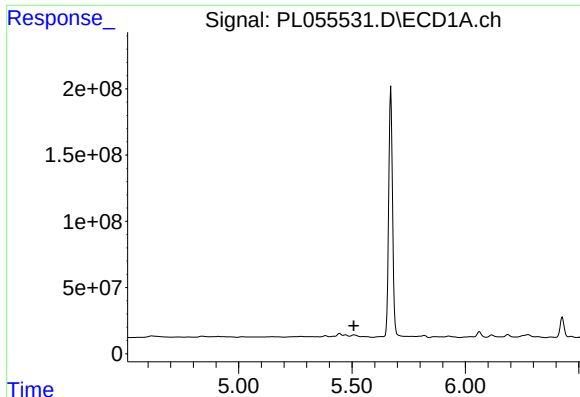

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.508 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
MC-010220-0-2-COMP-B3

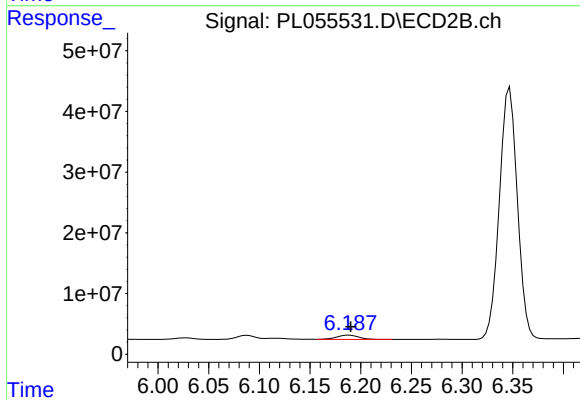


#26 Chlordane-4

R.T.: 6.189 min
Delta R.T.: -0.002 min
Response: 10367642
Conc: 24.97 ng/ml

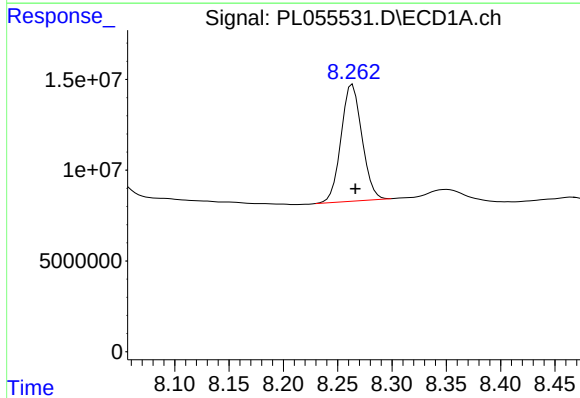

#28 Decachlorobiphenyl

R.T.: 8.264 min
Delta R.T.: -0.003 min
Response: 86142628
Conc: 10.18 ng/ml

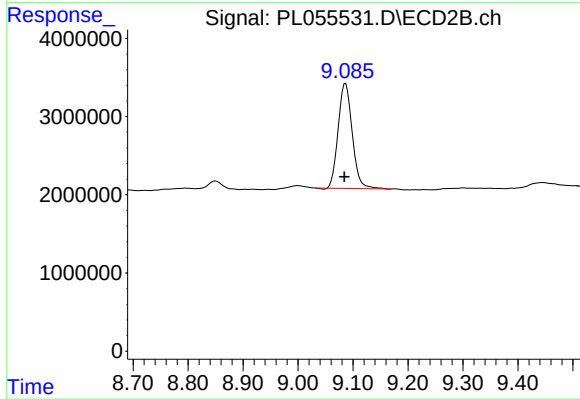

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: 0.002 min
Response: 23901155
Conc: 10.79 ng/ml