

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010320\
 Data File : PL055536.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2020 04:22
 Operator : AJ\MA
 Sample : L1011-08
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MC-010220-2-5-COMP-B7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 05:16:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010320.M
 Quant Title : GC Extractables
 QLast Update : Sat Jan 04 01:07:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.503	4.013	179.7E6	28851214	18.658	10.201 #
28)	SA Decachlor...	8.264	9.087	88127322	23853599	10.419	10.771
Target Compounds							
6)	B beta-BHC	0.000	4.882f	0	3219033	N.D.	1.840 #
9)	A Endosulfan I	0.000	6.234	0	9352982	N.D.	3.395 #
10)	B gamma-Chl...	0.000	6.124	0	1512444	N.D.	0.529 #
11)	B alpha-Chl...	0.000	6.191	0	12683052	N.D.	4.383 #
12)	B 4,4'-DDE	5.670	6.342	15030946	11262768	1.295	4.133 #
13)	MA Dieldrin	5.810	0.000	34452782	0	2.729	N.D. #
17)	MA 4,4'-DDT	0.000	7.137	0	6296650	N.D.	2.606 #
23)	Chlordane-1	4.376	0.000	17959006	0	53.778	N.D. #
25)	Chlordane-3	0.000	6.124	0	1512444	N.D.	4.344 #
26)	Chlordane-4	0.000	6.191	0	12683052	N.D.	30.547 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010320\
Data File : PL055536.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2020 04:22
Operator : AJ\MA
Sample : L1011-08
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MC-010220-2-5-COMP-B7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 05:16:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010320.M
Quant Title : GC Extractables
QLast Update : Sat Jan 04 01:07:28 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

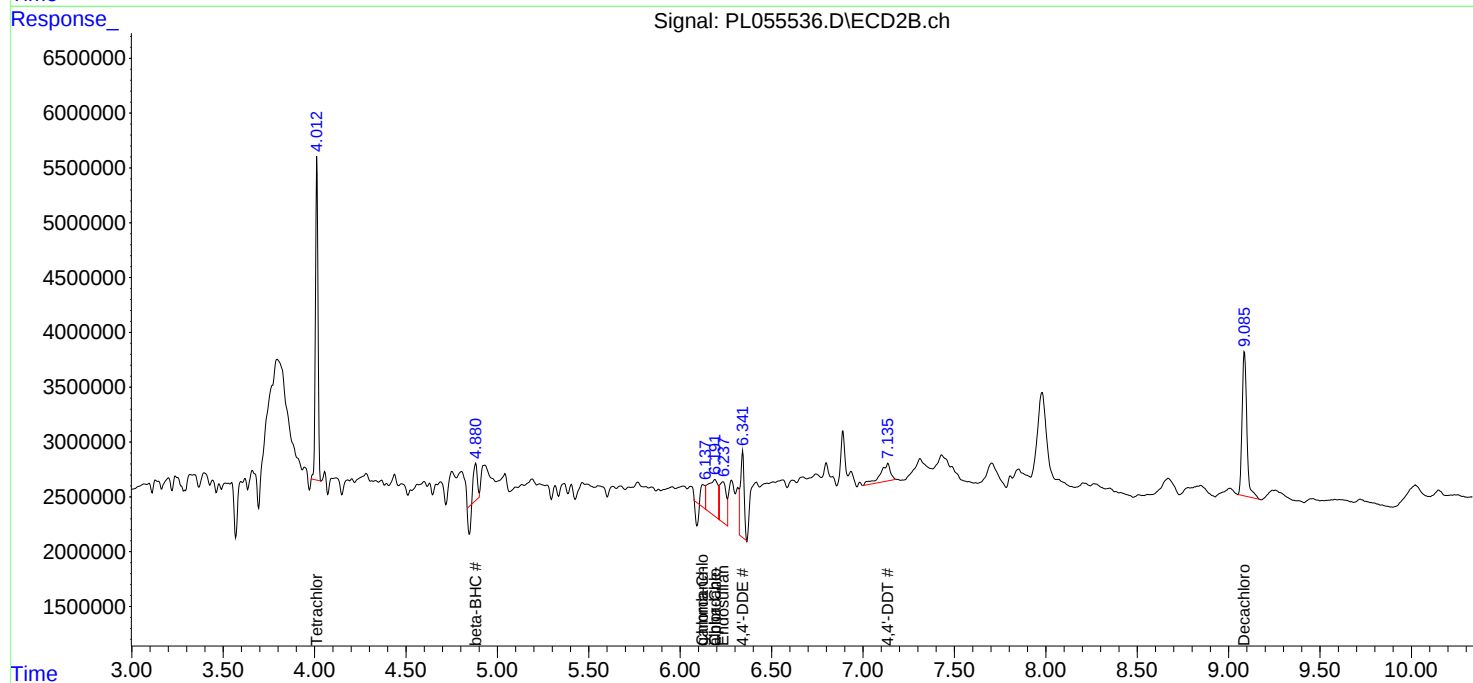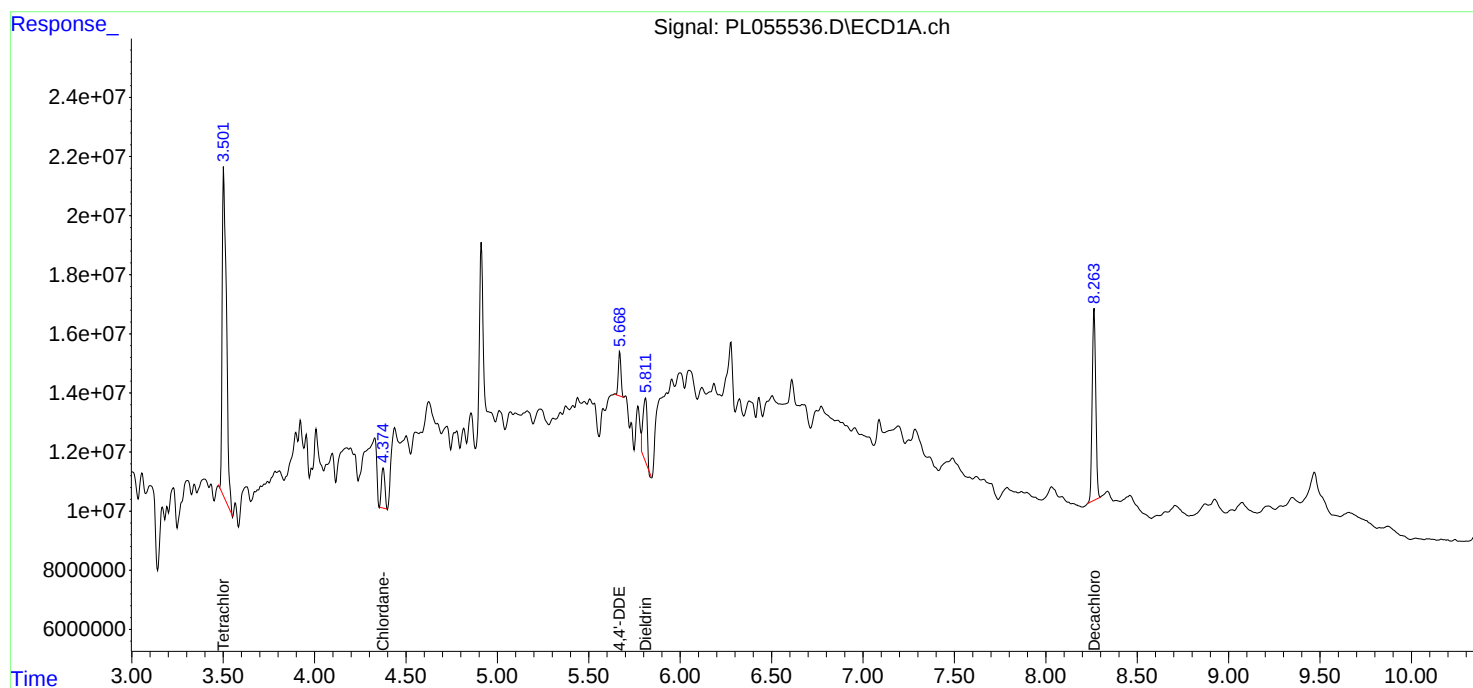


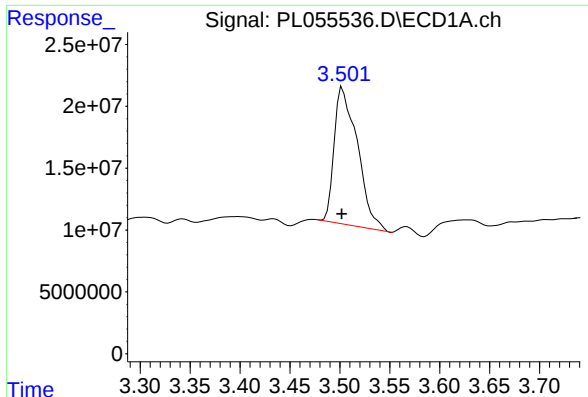

#1 Tetrachloro-m-xylene


R.T.: 3.503 min
Delta R.T.: 0.000 min
Response: 179720449
Conc: 18.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
MC-010220-2-5-COMP-B7

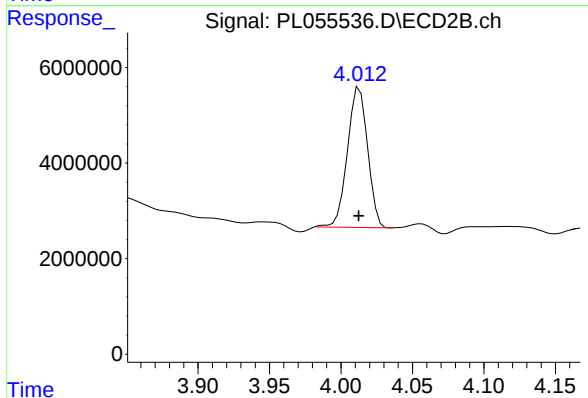


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 28851214
Conc: 10.20 ng/ml

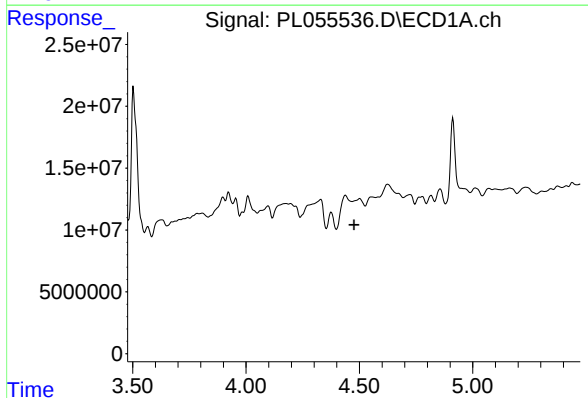


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.477 min
Response: 0
Conc: N.D.

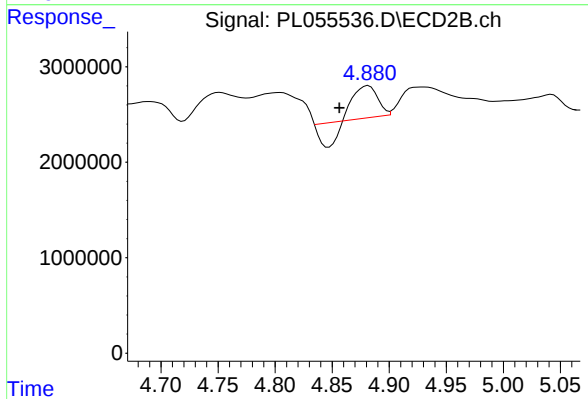

#6 beta-BHC


R.T.: 4.882 min
Delta R.T.: 0.025 min
Response: 3219033
Conc: 1.84 ng/ml

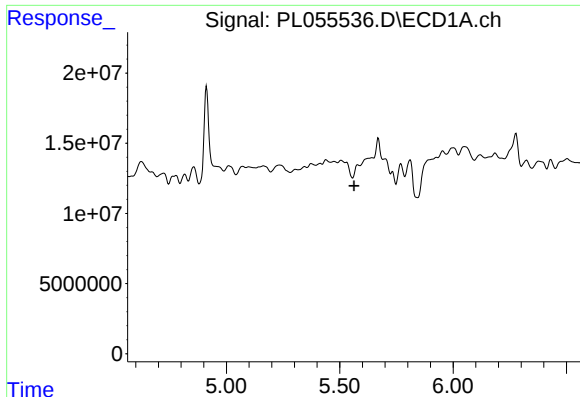

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.563 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
MC-010220-2-5-COMP-B7

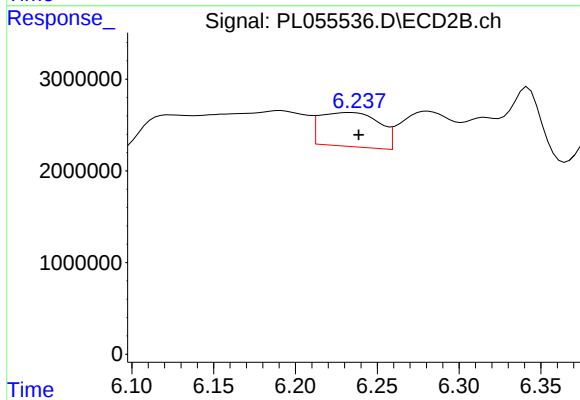


#9 Endosulfan I

R.T.: 6.234 min
Delta R.T.: -0.004 min
Response: 9352982
Conc: 3.40 ng/ml

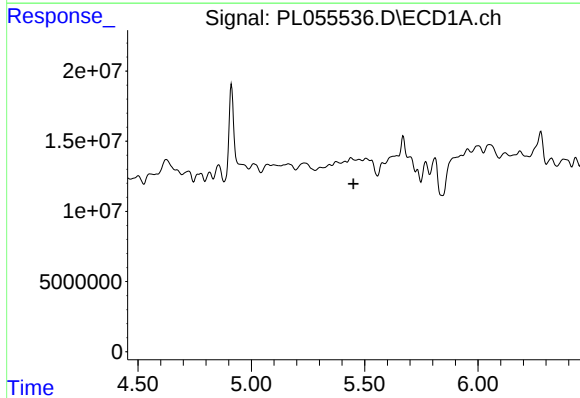


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.451 min
Response: 0
Conc: N.D.

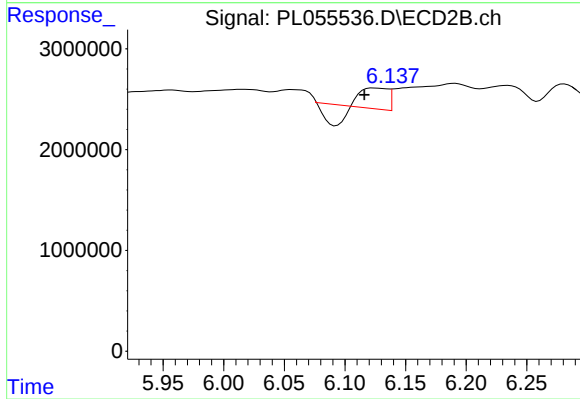

#10 gamma-Chlordane


R.T.: 6.124 min
Delta R.T.: 0.008 min
Response: 1512444
Conc: 0.53 ng/ml

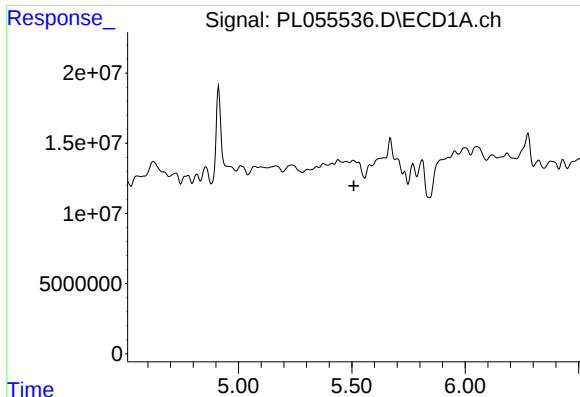

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
MC-010220-2-5-COMP-B7

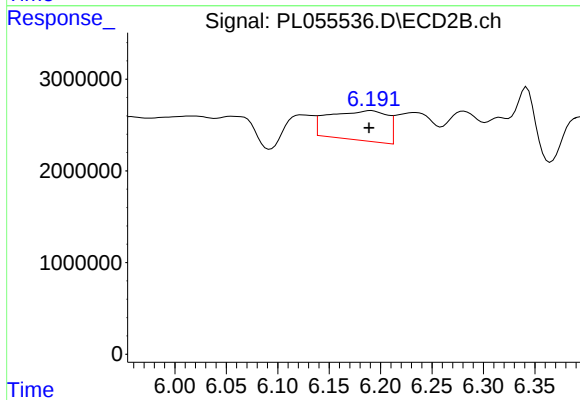


#11 alpha-Chlordane

R.T.: 6.191 min
Delta R.T.: 0.002 min
Response: 12683052
Conc: 4.38 ng/ml

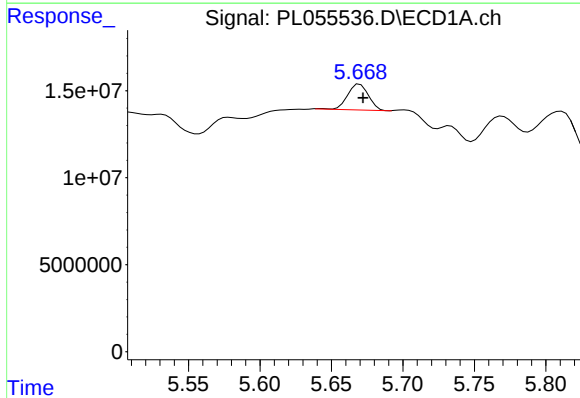


#12 4,4'-DDE

R.T.: 5.670 min
Delta R.T.: -0.002 min
Response: 15030946
Conc: 1.29 ng/ml

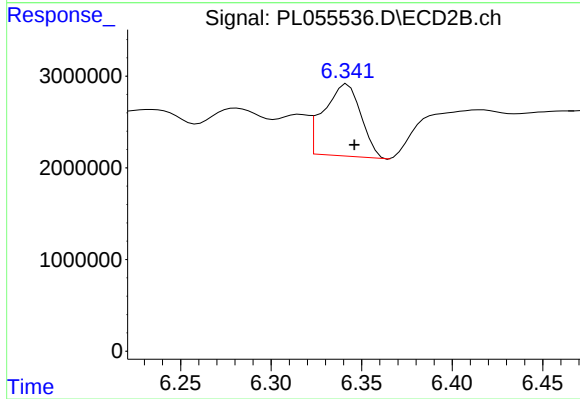

#12 4,4'-DDE


R.T.: 6.342 min
Delta R.T.: -0.004 min
Response: 11262768
Conc: 4.13 ng/ml

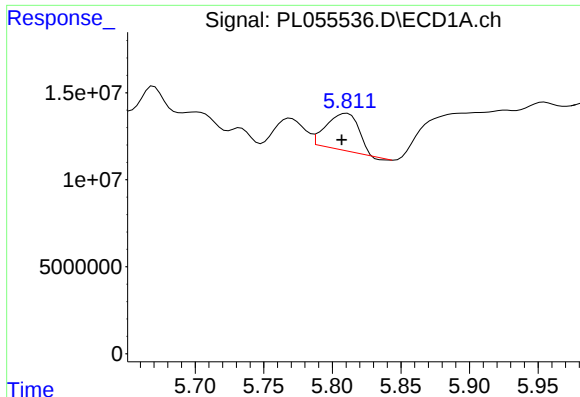

#13 Dieldrin


R.T.: 5.810 min
Delta R.T.: 0.003 min
Response: 34452782
Conc: 2.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
MC-010220-2-5-COMP-B7

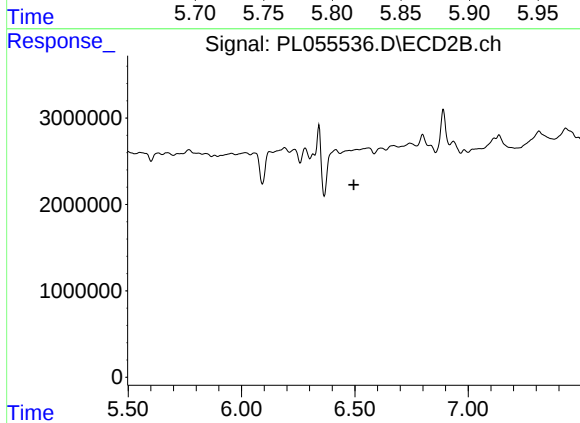


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.496 min
Response: 0
Conc: N.D.

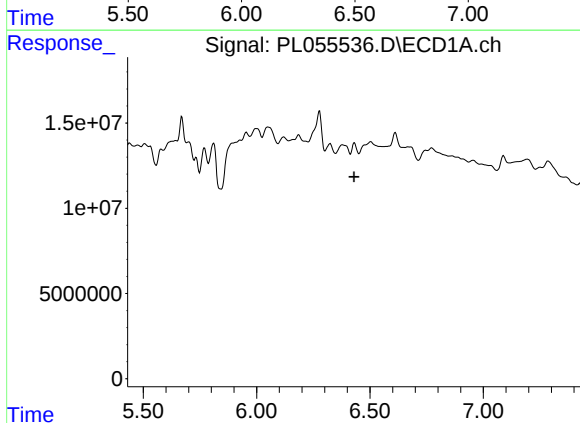


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.430 min
Response: 0
Conc: N.D.

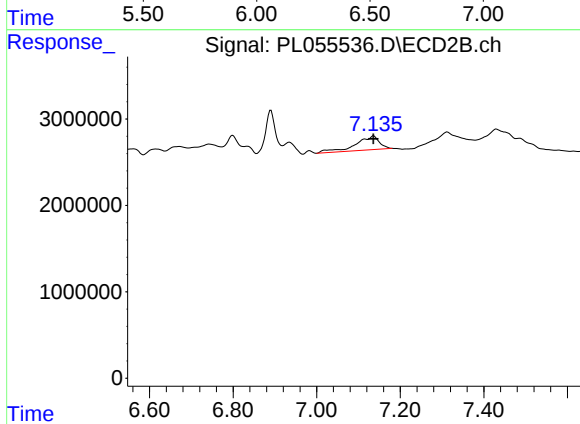

#17 4,4'-DDT


R.T.: 7.137 min
Delta R.T.: 0.000 min
Response: 6296650
Conc: 2.61 ng/ml

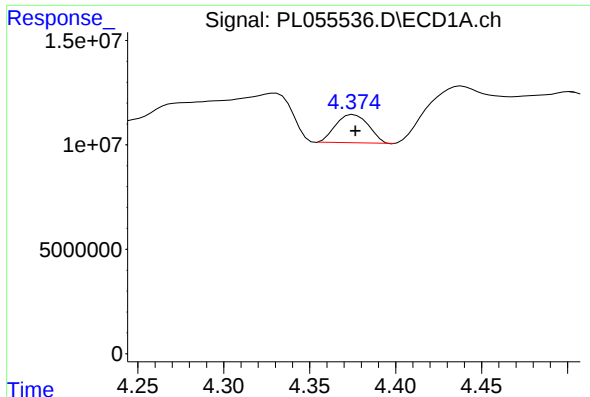

#23 Chlordane-1


R.T.: 4.376 min
Delta R.T.: 0.000 min
Response: 17959006
Conc: 53.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
MC-010220-2-5-COMP-B7

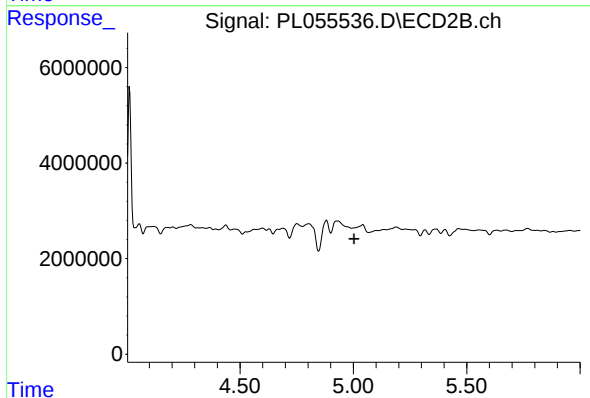


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.004 min
Response: 0
Conc: N.D.

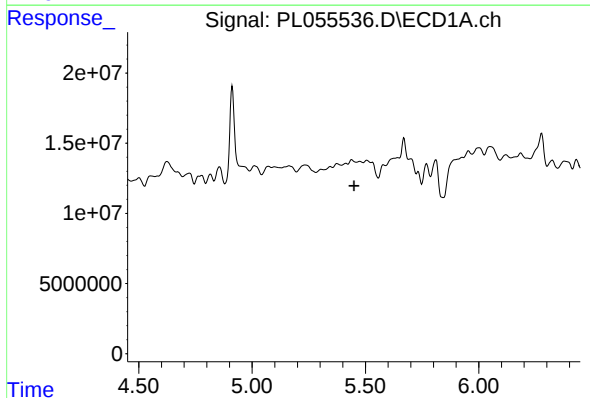


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.450 min
Response: 0
Conc: N.D.

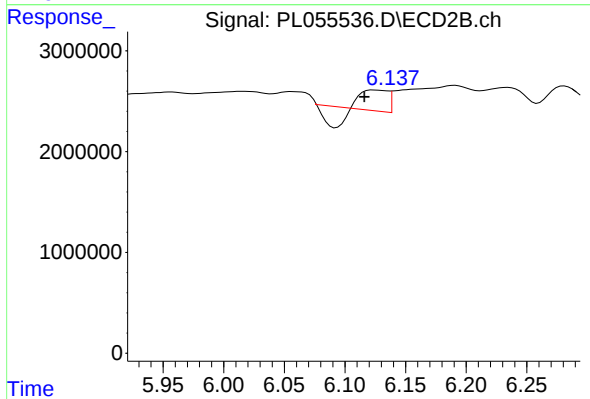

#25 Chlordane-3


R.T.: 6.124 min
Delta R.T.: 0.008 min
Response: 1512444
Conc: 4.34 ng/ml

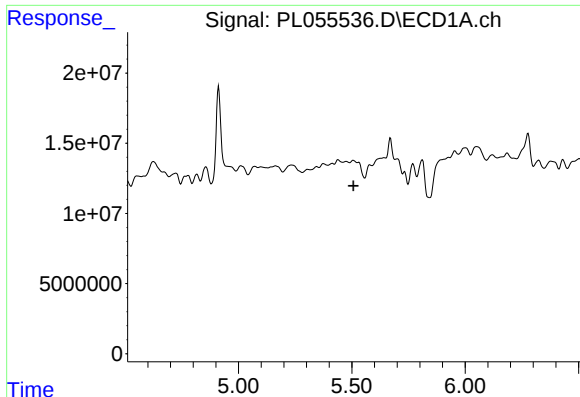

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.508 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
MC-010220-2-5-COMP-B7

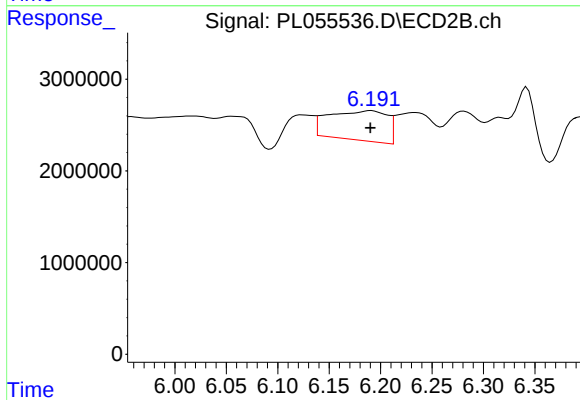


#26 Chlordane-4

R.T.: 6.191 min
Delta R.T.: 0.000 min
Response: 12683052
Conc: 30.55 ng/ml

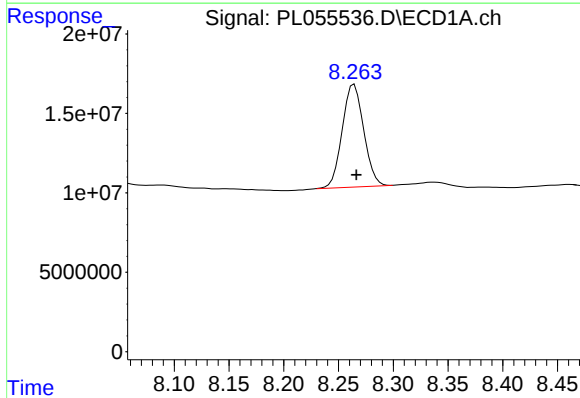

#28 Decachlorobiphenyl

R.T.: 8.264 min
Delta R.T.: -0.002 min
Response: 88127322
Conc: 10.42 ng/ml

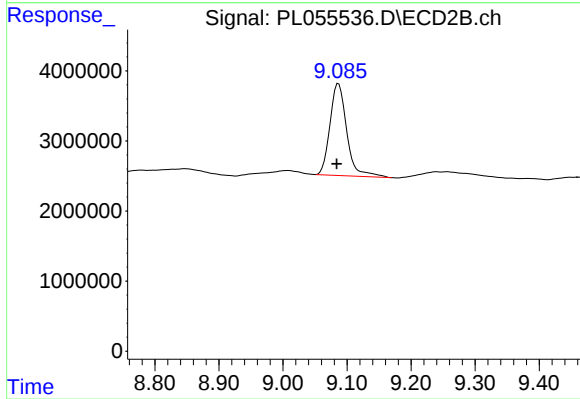

#28 Decachlorobiphenyl

R.T.: 9.087 min
Delta R.T.: 0.003 min
Response: 23853599
Conc: 10.77 ng/ml