

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010324\
 Data File : PL087617.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jan 2024 14:15
 Operator : AR\AJ
 Sample : P1004-01 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SU-04-01022024

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/04/2024
 Supervised By :Ankita Jodhani 01/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 21:40:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 29 03:17:47 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.420	2.675	5843179	2561883	1.952m	2.115
2) SA Decachlor...	8.986	7.863	6147395	2425020	2.158	1.914m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010324\
Data File : PL087617.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jan 2024 14:15
Operator : AR\AJ
Sample : P1004-01 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
SU-04-01022024


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/04/2024
Supervised By : Ankita Jodhani 01/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 21:40:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 03:17:47 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

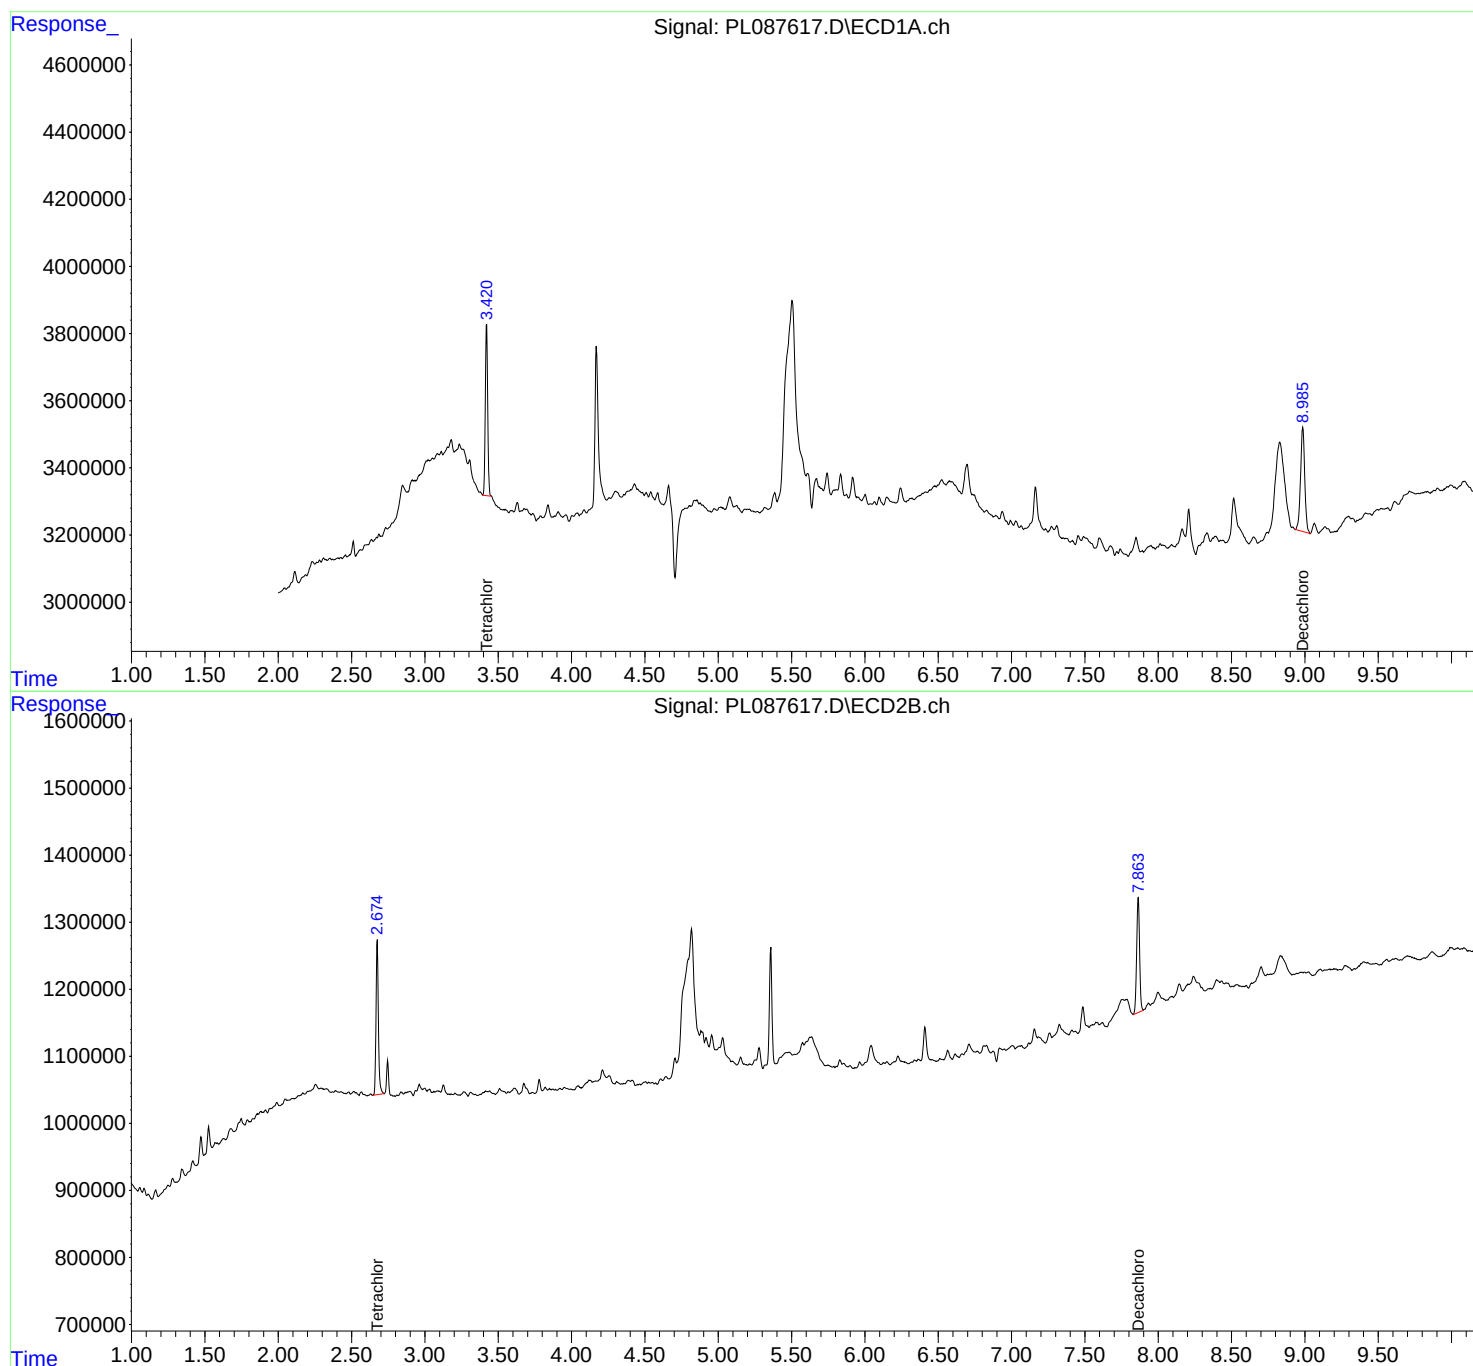

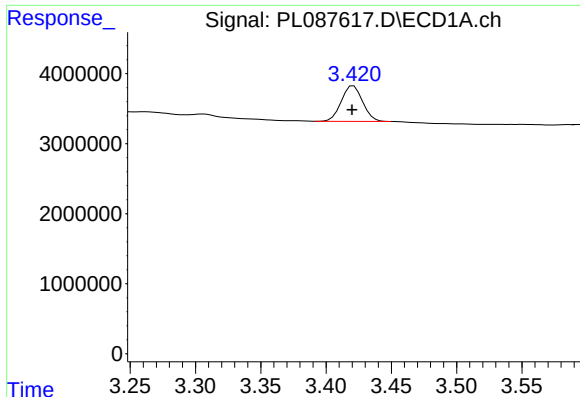


#1 Tetrachloro-m-xylene

R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 5843179
Conc: 1.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-04-01022024


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/04/2024
Supervised By :Ankita Jodhani 01/04/2024

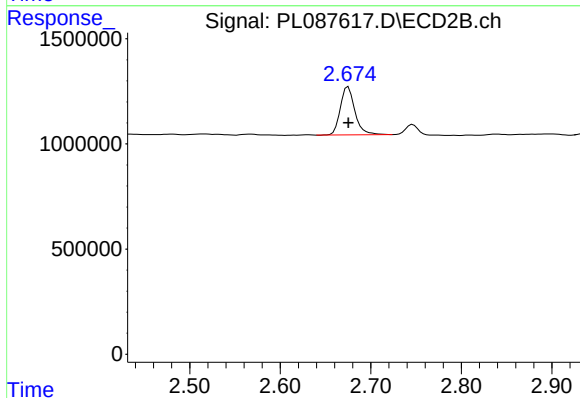


#1 Tetrachloro-m-xylene

R.T.: 2.675 min
Delta R.T.: 0.000 min
Response: 2561883
Conc: 2.11 ng/ml

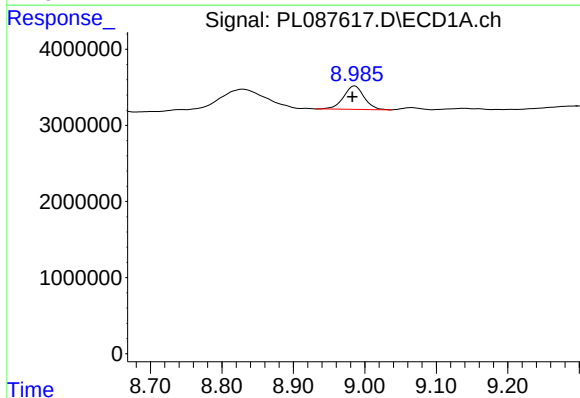

#28 Decachlorobiphenyl

R.T.: 8.986 min
Delta R.T.: 0.004 min
Response: 6147395
Conc: 2.16 ng/ml

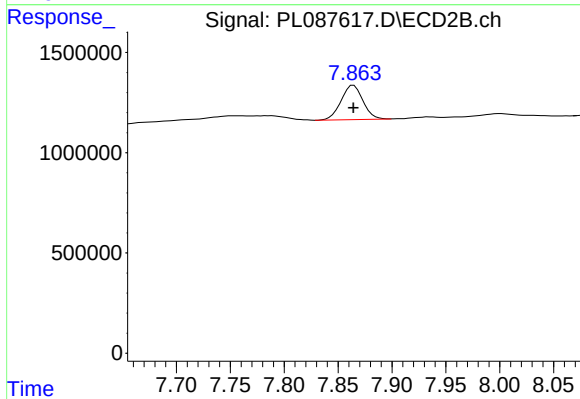

#28 Decachlorobiphenyl

R.T.: 7.863 min
Delta R.T.: -0.001 min
Response: 2425020
Conc: 1.91 ng/ml m