

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010419\
 Data File : PL043615.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2019 13:04
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 23:03:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 04 06:12:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.427f	0.000	714218	0	0.112	N.D. #
Target Compounds							
4)	MA Heptachlor	0.000	5.261f	0	1372578	N.D.	0.351 #
7)	B delta-BHC	0.000	5.166	0	1860912	N.D.	0.440 #
8)	B Heptachlo...	5.119f	5.984	1669848	7412121	0.217	2.028 #
14)	MA Endrin	5.946f	6.772f	1334877	944072	0.219	0.374 #
17)	MA 4,4'-DDT	0.000	7.186f	0	3293549	N.D.	1.474 #
18)	B Endrin al...	0.000	7.186	0	3293549	N.D.	1.548 #
20)	A Methoxychlor	0.000	7.728	0	879880	N.D.	0.781 #
23)	Chlordane-1	4.312	5.166	424901	1860912	1.579	13.911 #
24)	Chlordane-2	4.870	0.000	1961445	0	7.113	N.D. #
27)	Chlordane-5	0.000	7.186	0	3293549	N.D.	35.762 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010419\
Data File : PL043615.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2019 13:04
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 23:03:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
Quant Title : GC Extractables
QLast Update : Fri Jan 04 06:12:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

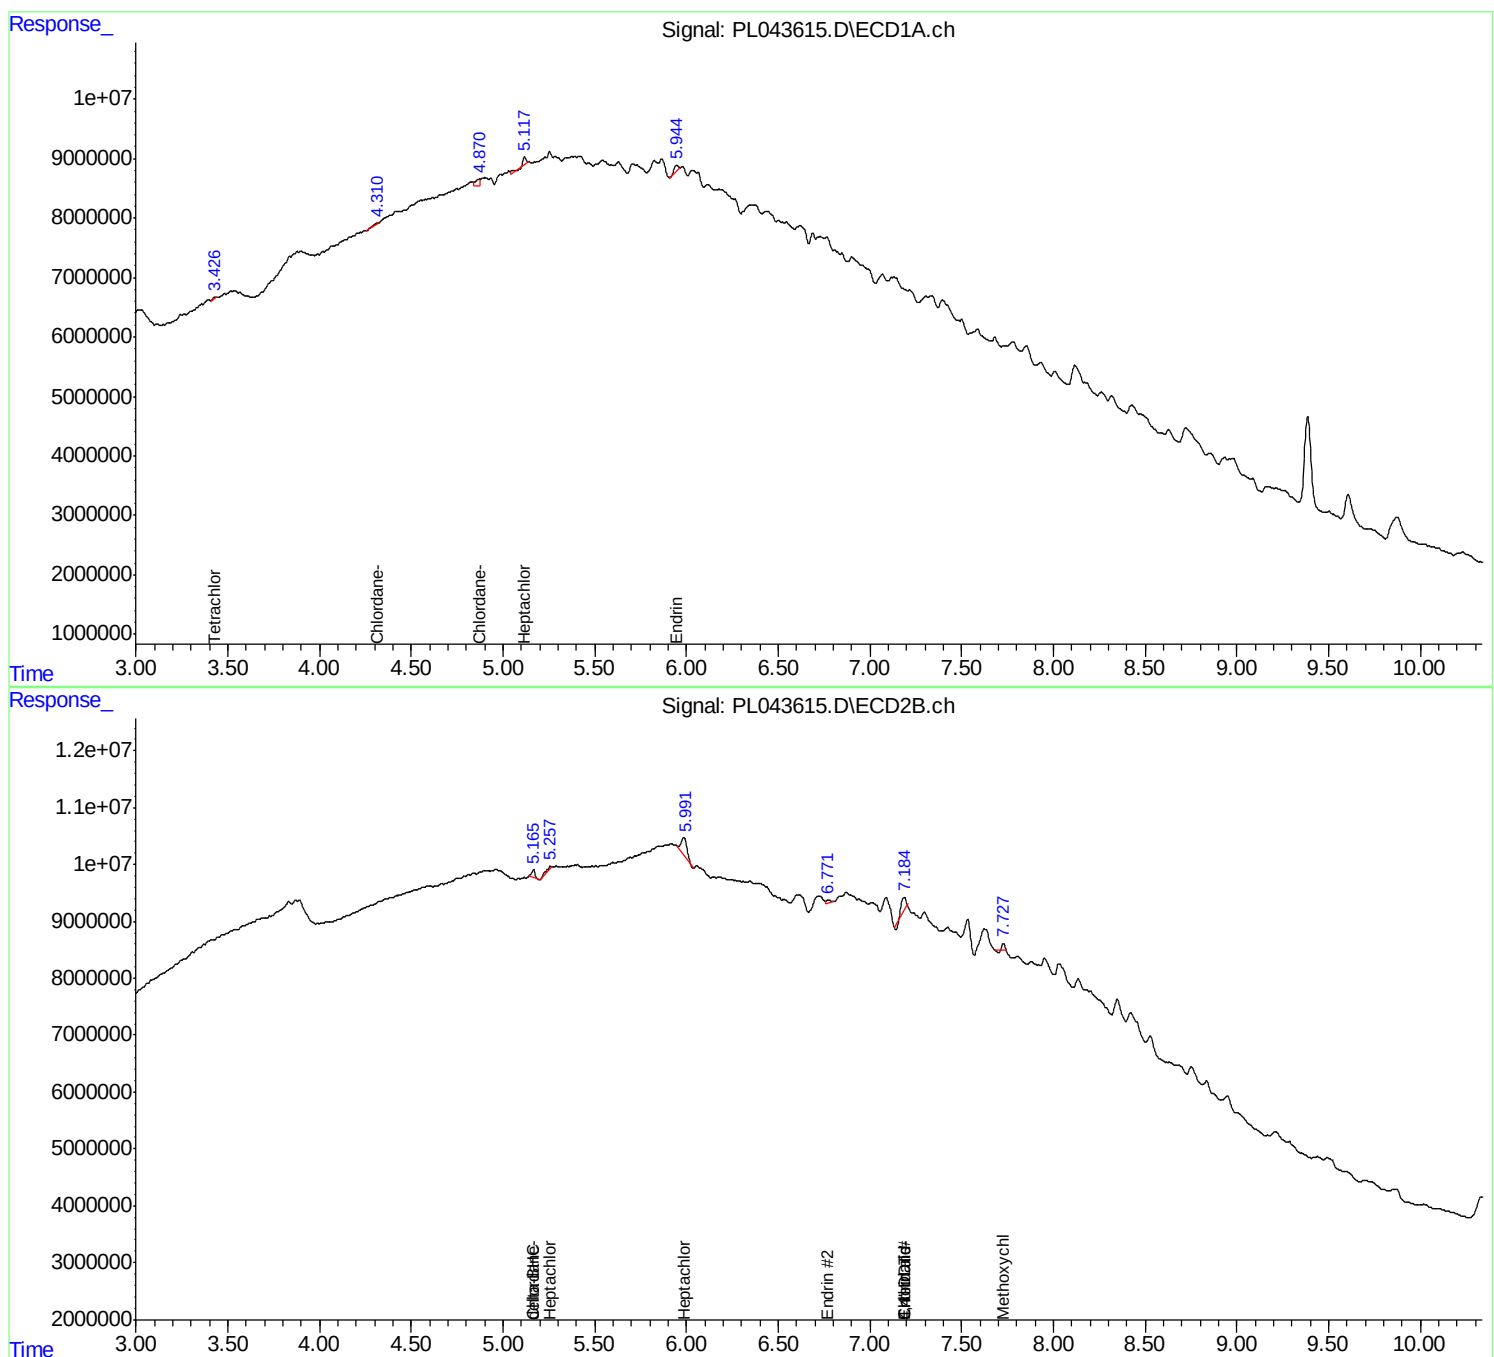


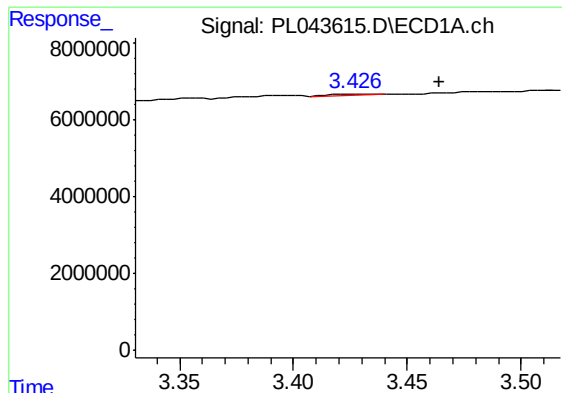

#1 Tetrachloro-m-xylene


R.T.: 3.427 min
Delta R.T.: -0.037 min
Response: 714218
Conc: 0.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

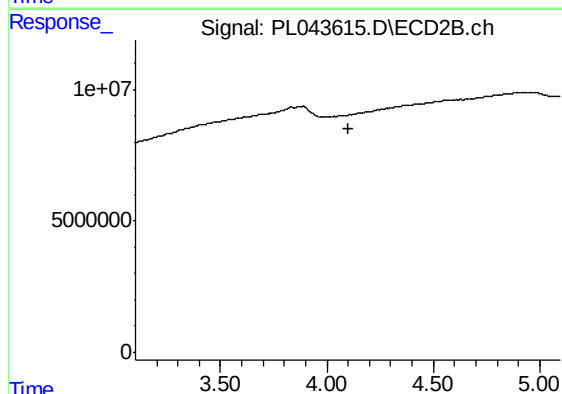


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.100 min
Response: 0
Conc: N.D.

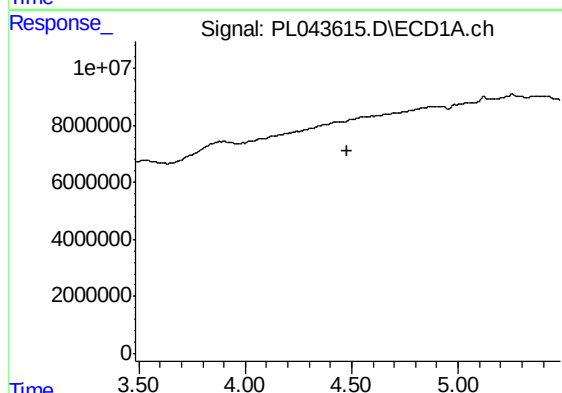


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.481 min
Response: 0
Conc: N.D.

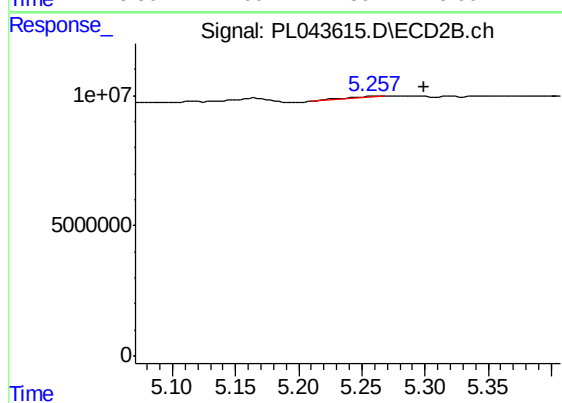

#4 Heptachlor


R.T.: 5.261 min
Delta R.T.: -0.039 min
Response: 1372578
Conc: 0.35 ng/ml

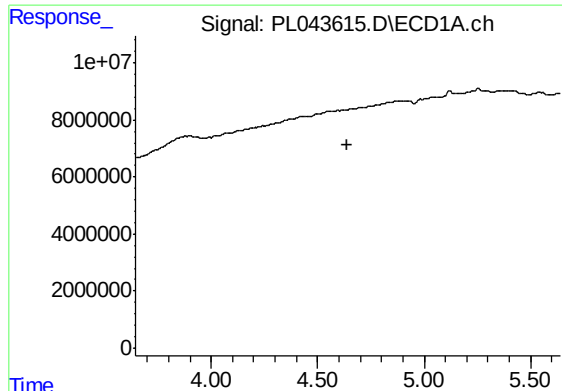

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.642 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

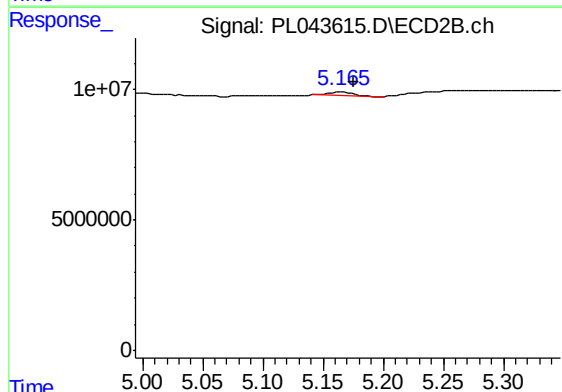


#7 delta-BHC

R.T.: 5.166 min
Delta R.T.: -0.009 min
Response: 1860912
Conc: 0.44 ng/ml

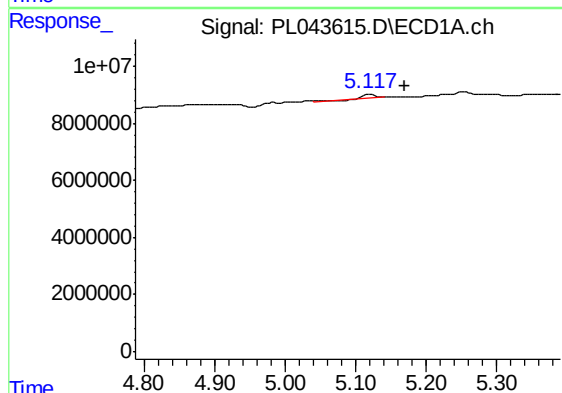


#8 Heptachlor epoxide

R.T.: 5.119 min
Delta R.T.: -0.050 min
Response: 1669848
Conc: 0.22 ng/ml

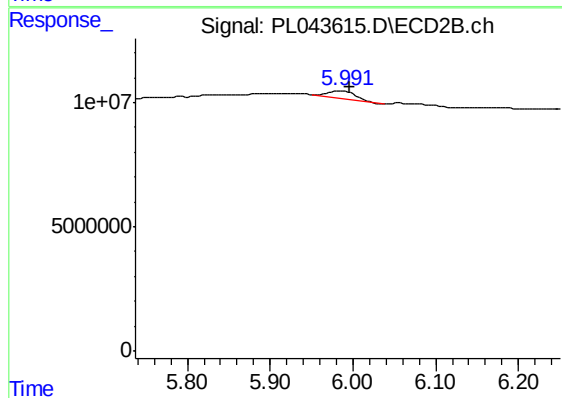

#8 Heptachlor epoxide


R.T.: 5.984 min
Delta R.T.: -0.013 min
Response: 7412121
Conc: 2.03 ng/ml

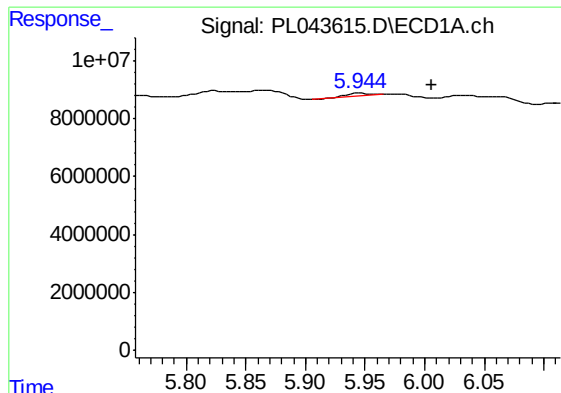

#14 Endrin


R.T.: 5.946 min
Delta R.T.: -0.061 min
Response: 1334877
Conc: 0.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

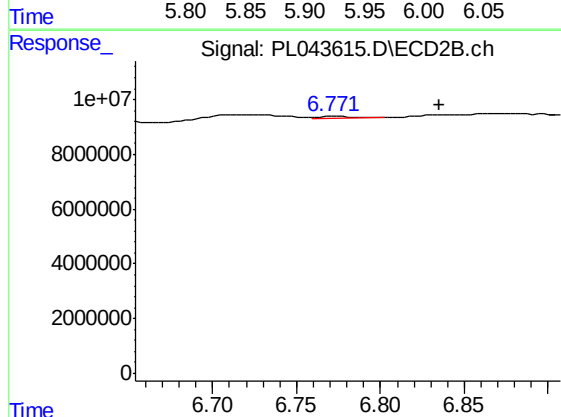


#14 Endrin

R.T.: 6.772 min
Delta R.T.: -0.063 min
Response: 944072
Conc: 0.37 ng/ml

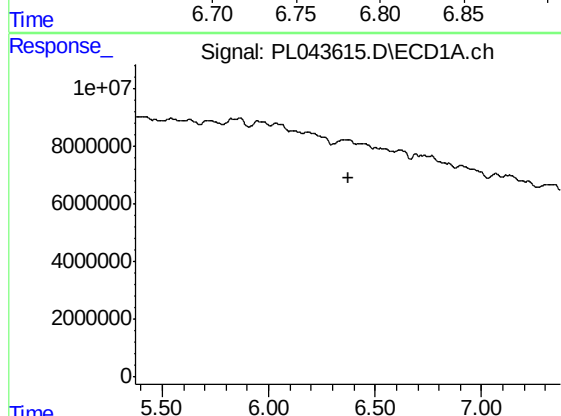


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.373 min
Response: 0
Conc: N.D.

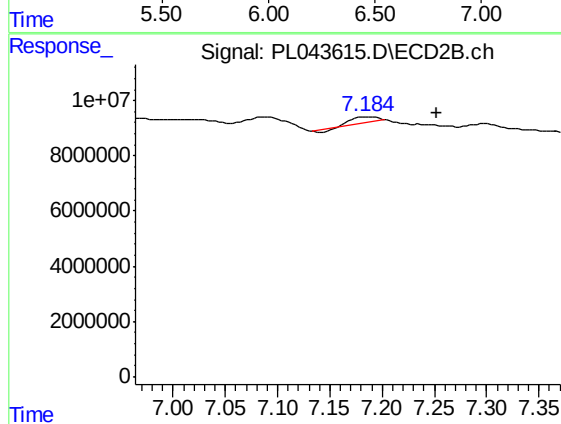

#17 4,4'-DDT


R.T.: 7.186 min
Delta R.T.: -0.067 min
Response: 3293549
Conc: 1.47 ng/ml

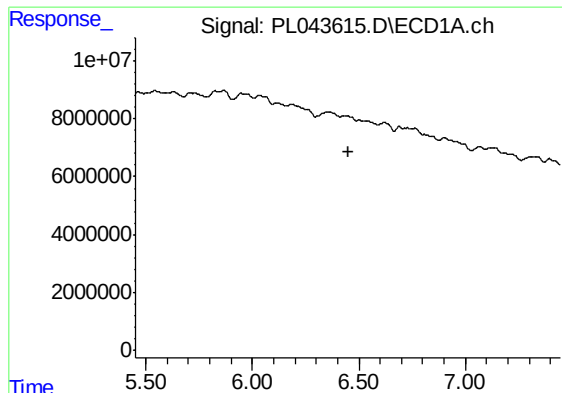

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.449 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

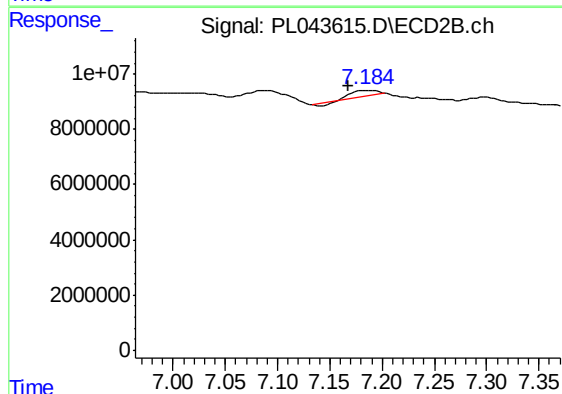


#18 Endrin aldehyde

R.T.: 7.186 min
Delta R.T.: 0.018 min
Response: 3293549
Conc: 1.55 ng/ml

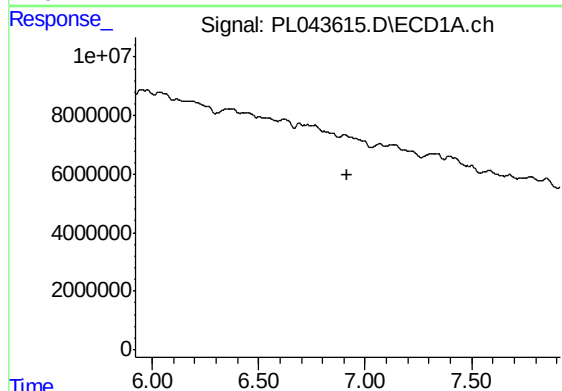


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.918 min
Response: 0
Conc: N.D.

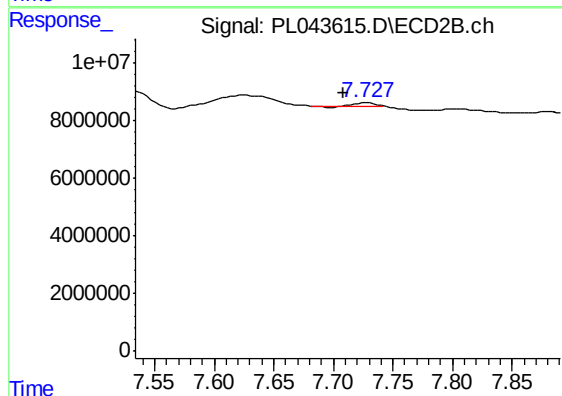

#20 Methoxychlor


R.T.: 7.728 min
Delta R.T.: 0.019 min
Response: 879880
Conc: 0.78 ng/ml

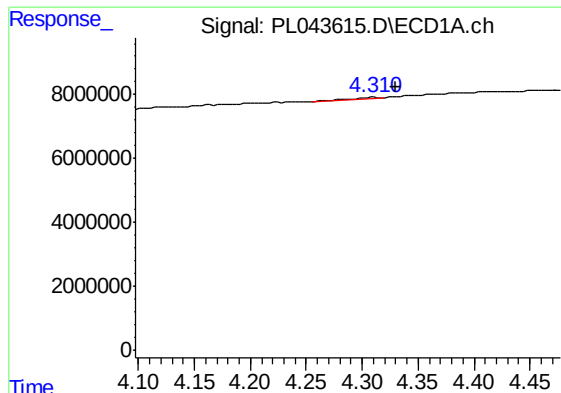

#23 Chlordane-1


R.T.: 4.312 min
Delta R.T.: -0.018 min
Response: 424901
Conc: 1.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

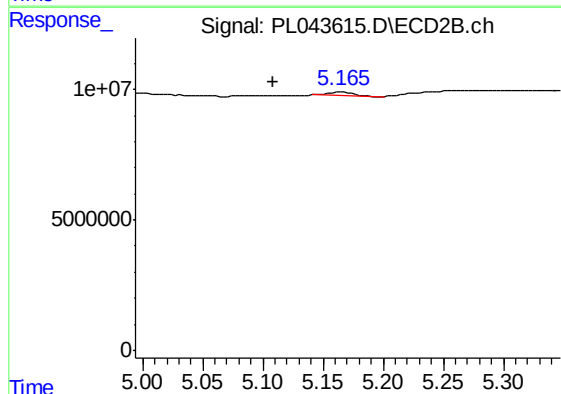


#23 Chlordane-1

R.T.: 5.166 min
Delta R.T.: 0.057 min
Response: 1860912
Conc: 13.91 ng/ml

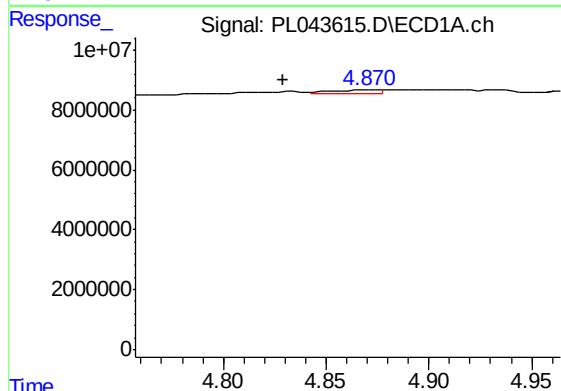


#24 Chlordane-2

R.T.: 4.870 min
Delta R.T.: 0.041 min
Response: 1961445
Conc: 7.11 ng/ml

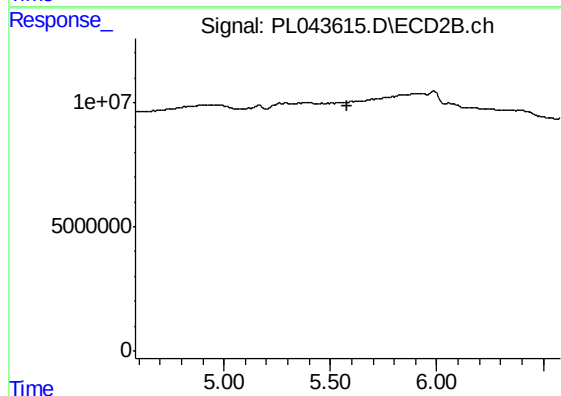

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.581 min
Response: 0
Conc: N.D.

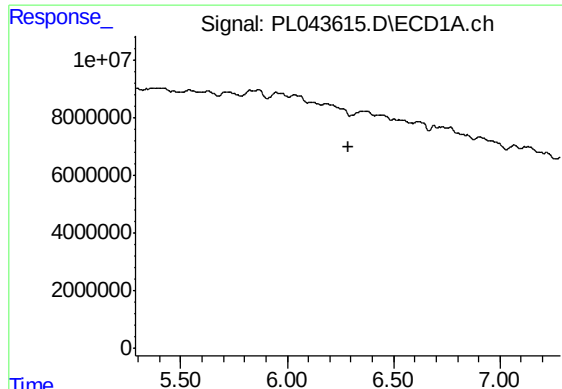

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.287 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

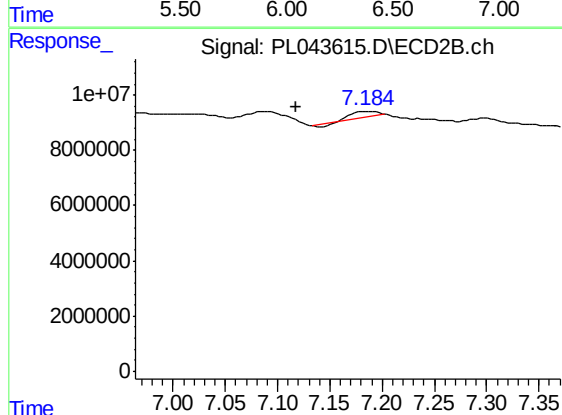


#27 Chlordane-5

R.T.: 7.186 min
Delta R.T.: 0.069 min
Response: 3293549
Conc: 35.76 ng/ml

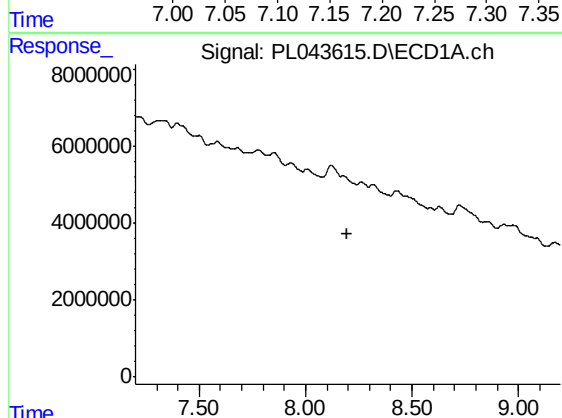

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.199 min
Response: 0
Conc: N.D.

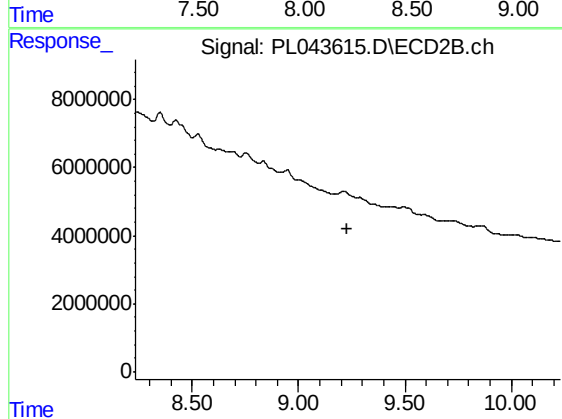

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.231 min
Response: 0
Conc: N.D.