

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010419\
 Data File : PL043627.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2019 18:18
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 23:06:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 04 06:12:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.463	4.099	111.3E6	55940638	17.425	19.146
28)	SA Decachlor...	8.198	9.230	113.8E6	46347192	22.587	20.966
Target Compounds							
2)	A alpha-BHC	0.000	4.448f	0	636196	N.D.	0.151 #
7)	B delta-BHC	0.000	5.166	0	4355157	N.D.	1.030 #
8)	B Heptachlo...	5.107f	5.991	3336650	16255168	0.434	4.446 #
14)	MA Endrin	6.015	0.000	1763663	0	0.289	N.D. #
23)	Chlordane-1	0.000	5.166	0	4355157	N.D.	32.556 #
24)	Chlordane-2	0.000	5.511	0	1731098	N.D.	14.019 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010419\
Data File : PL043627.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2019 18:18
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 23:06:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010319.M
Quant Title : GC Extractables
QLast Update : Fri Jan 04 06:12:42 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

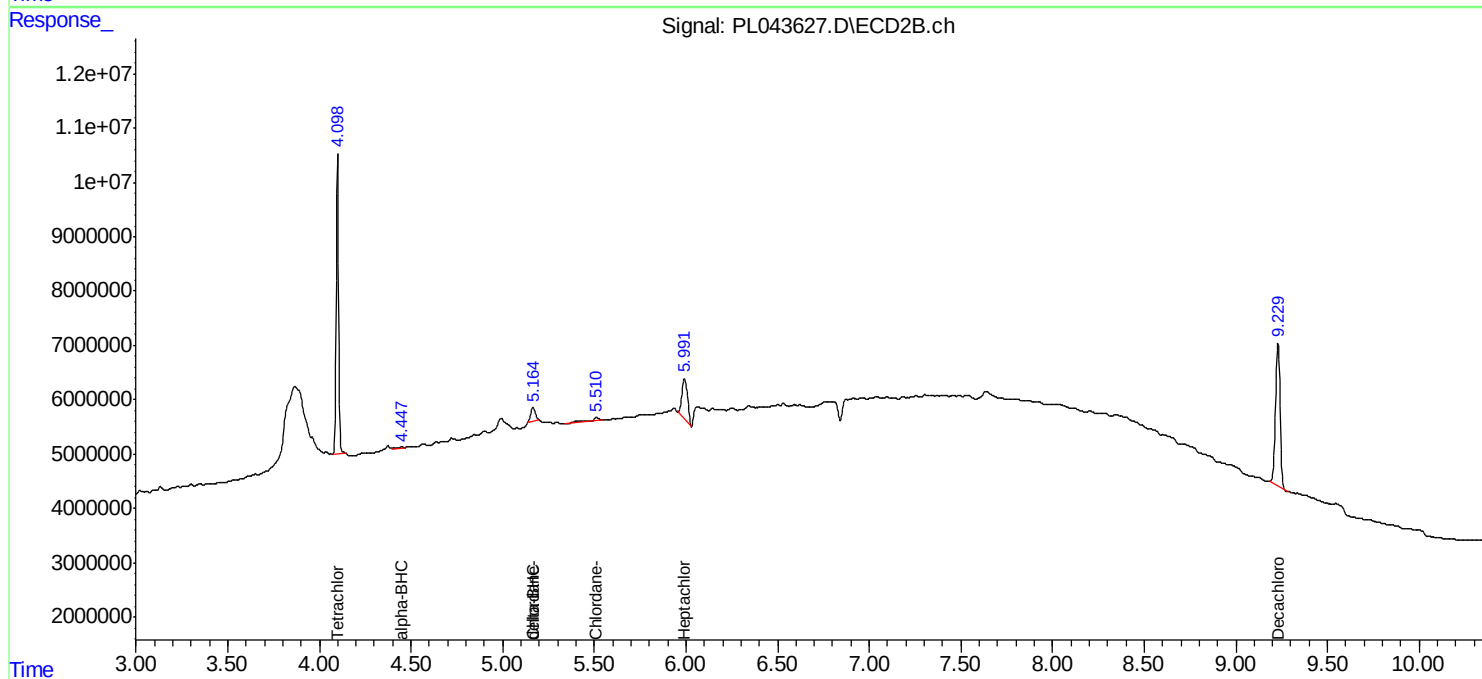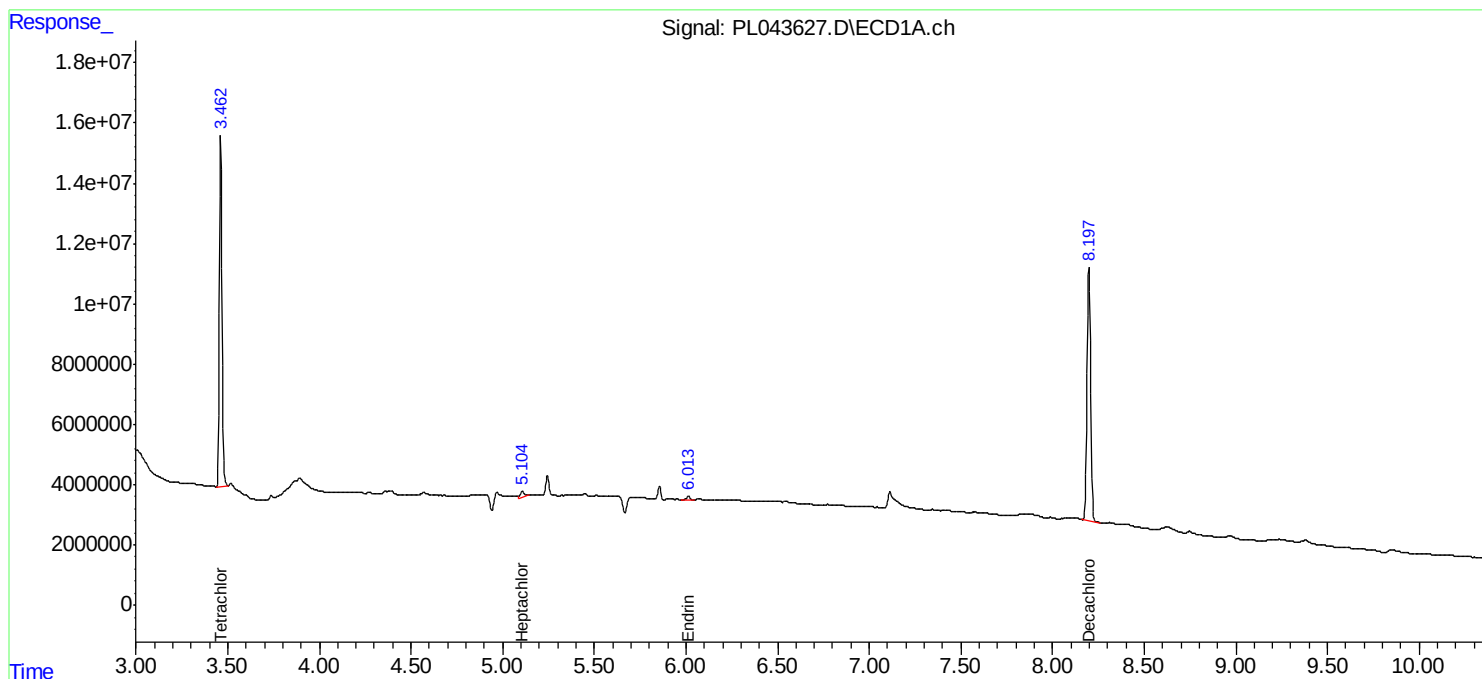


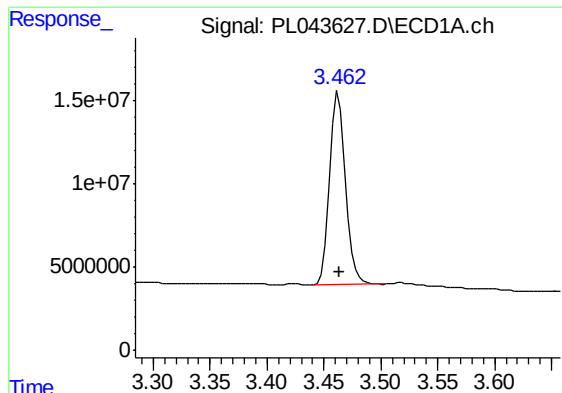

#1 Tetrachloro-m-xylene


R.T.: 3.463 min
Delta R.T.: -0.001 min
Response: 111330250
Conc: 17.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

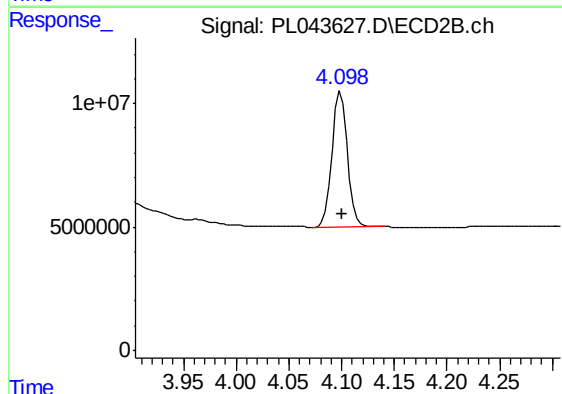


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: 0.000 min
Response: 55940638
Conc: 19.15 ng/ml

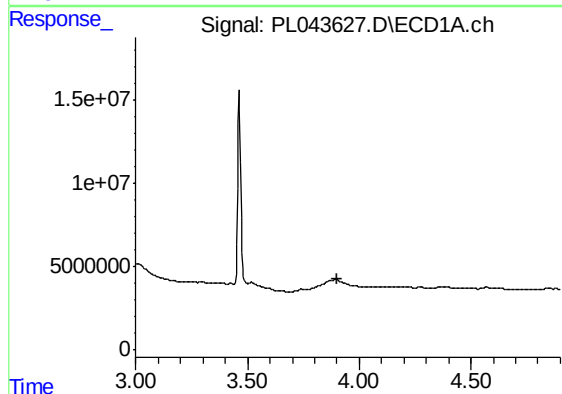


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.903 min
Response: 0
Conc: N.D.

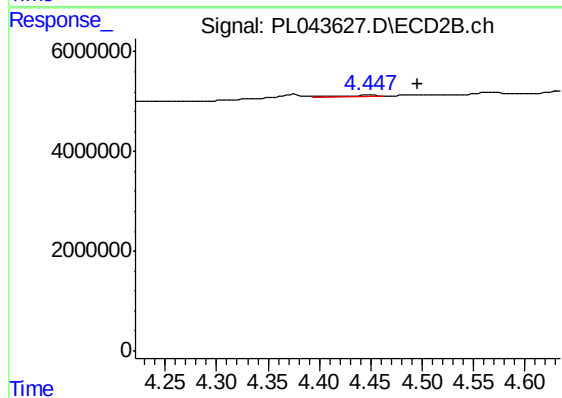

#2 alpha-BHC


R.T.: 4.448 min
Delta R.T.: -0.047 min
Response: 636196
Conc: 0.15 ng/ml

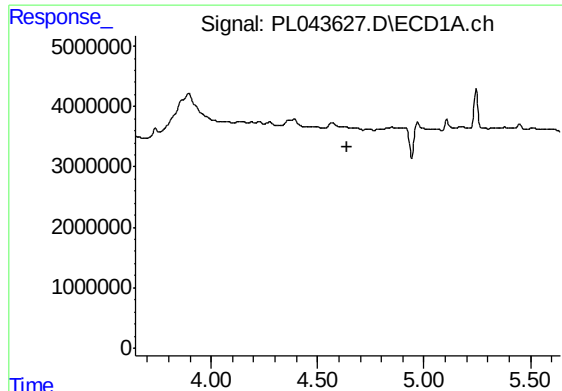

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.642 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

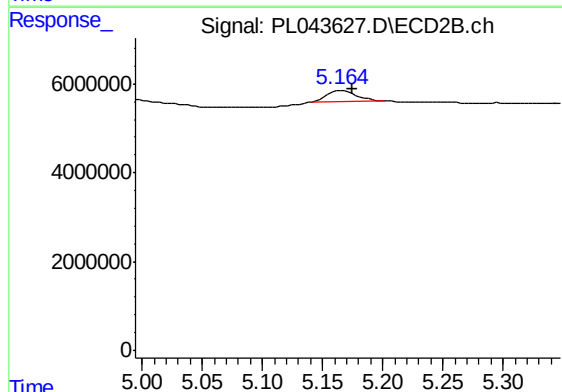


#7 delta-BHC

R.T.: 5.166 min
Delta R.T.: -0.009 min
Response: 4355157
Conc: 1.03 ng/ml

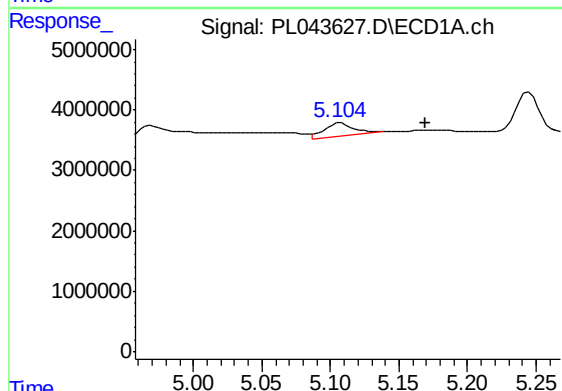


#8 Heptachlor epoxide

R.T.: 5.107 min
Delta R.T.: -0.062 min
Response: 3336650
Conc: 0.43 ng/ml

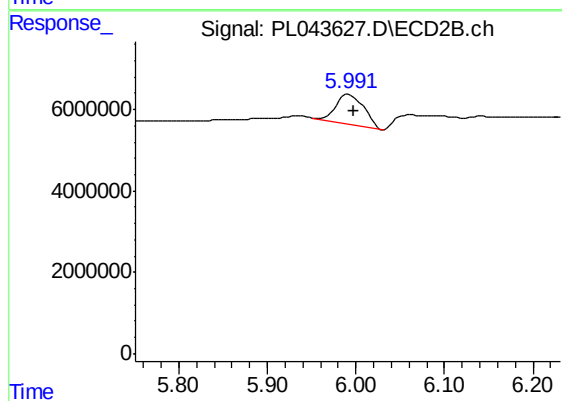

#8 Heptachlor epoxide


R.T.: 5.991 min
Delta R.T.: -0.005 min
Response: 16255168
Conc: 4.45 ng/ml

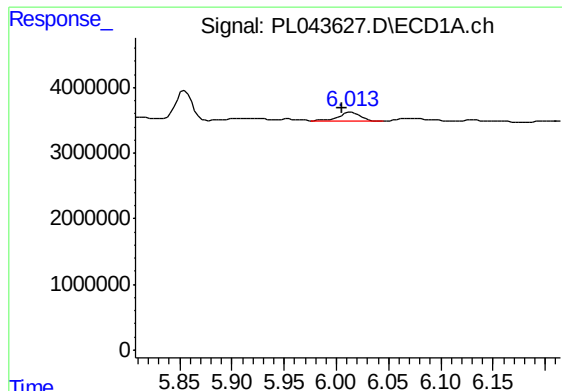

#14 Endrin


R.T.: 6.015 min
Delta R.T.: 0.009 min
Response: 1763663
Conc: 0.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

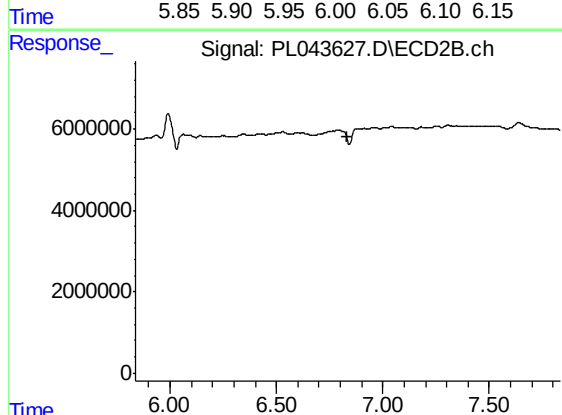


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.835 min
Response: 0
Conc: N.D.

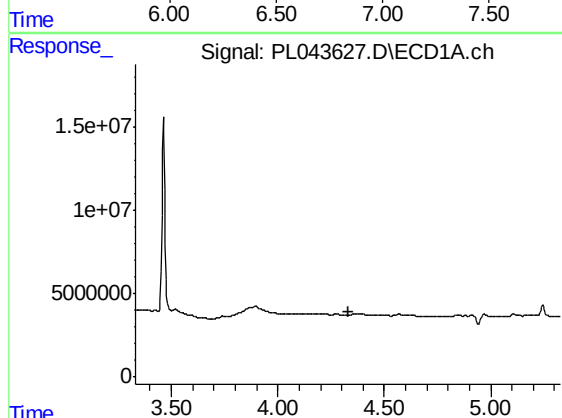


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.330 min
Response: 0
Conc: N.D.

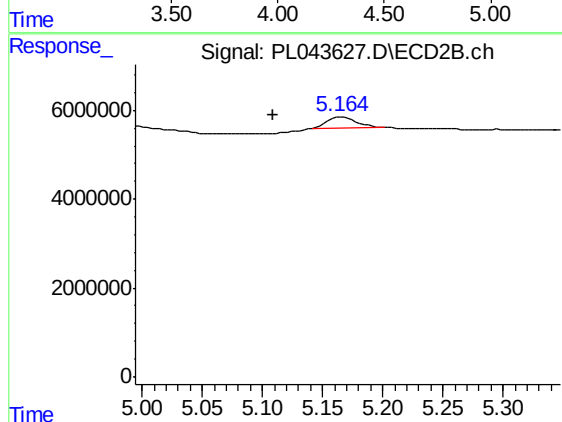

#23 Chlordane-1


R.T.: 5.166 min
Delta R.T.: 0.057 min
Response: 4355157
Conc: 32.56 ng/ml

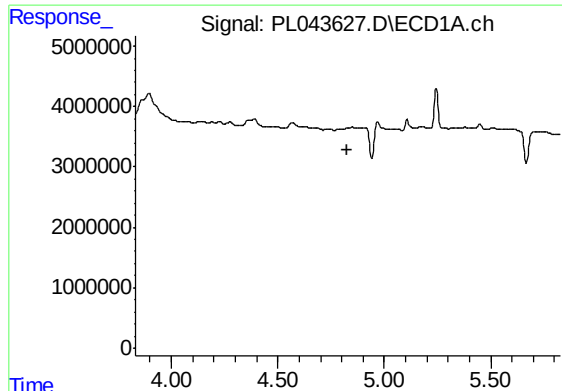

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.829 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

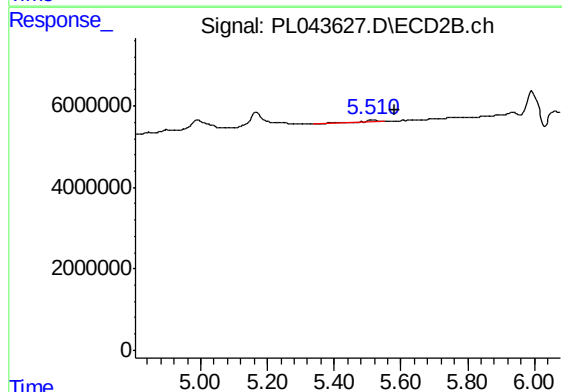


#24 Chlordane-2

R.T.: 5.511 min
Delta R.T.: -0.069 min
Response: 1731098
Conc: 14.02 ng/ml

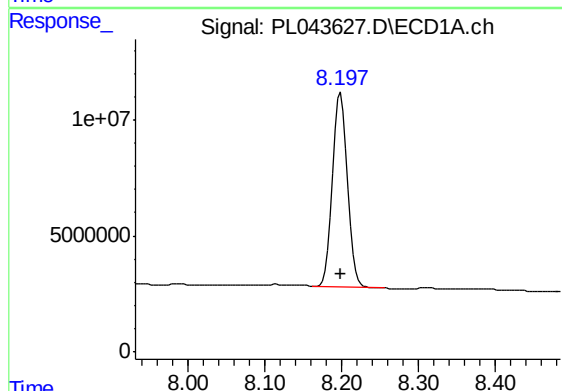

#28 Decachlorobiphenyl

R.T.: 8.198 min
Delta R.T.: 0.000 min
Response: 113821939
Conc: 22.59 ng/ml

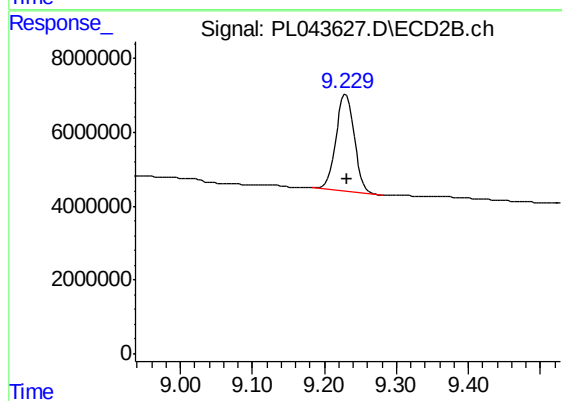

#28 Decachlorobiphenyl

R.T.: 9.230 min
Delta R.T.: -0.001 min
Response: 46347192
Conc: 20.97 ng/ml