

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010421\
 Data File : PL063913.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2021 13:36
 Operator : AR\AJ
 Sample : L5249-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 15:08:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.112	64917431	52809210	21.654	20.685
28)	SA Decachlor...	8.185	9.273	54493624	34921764	19.779	17.712
Target Compounds							
9)	A Endosulfan I	5.503f	0.000	5203847	0	1.503	N.D. #
10)	B gamma-Chl...	0.000	6.257	0	2848844	N.D.	1.030 #
13)	MA Dieldrin	5.727	6.644	4647701	2635701	1.282	1.012
24)	Chlordane-2	4.818	0.000	5298849	0	45.158	N.D. #
25)	Chlordane-3	0.000	6.257	0	2848844	N.D.	8.314 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010421\
Data File : PL063913.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2021 13:36
Operator : AR\AJ
Sample : L5249-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 15:08:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

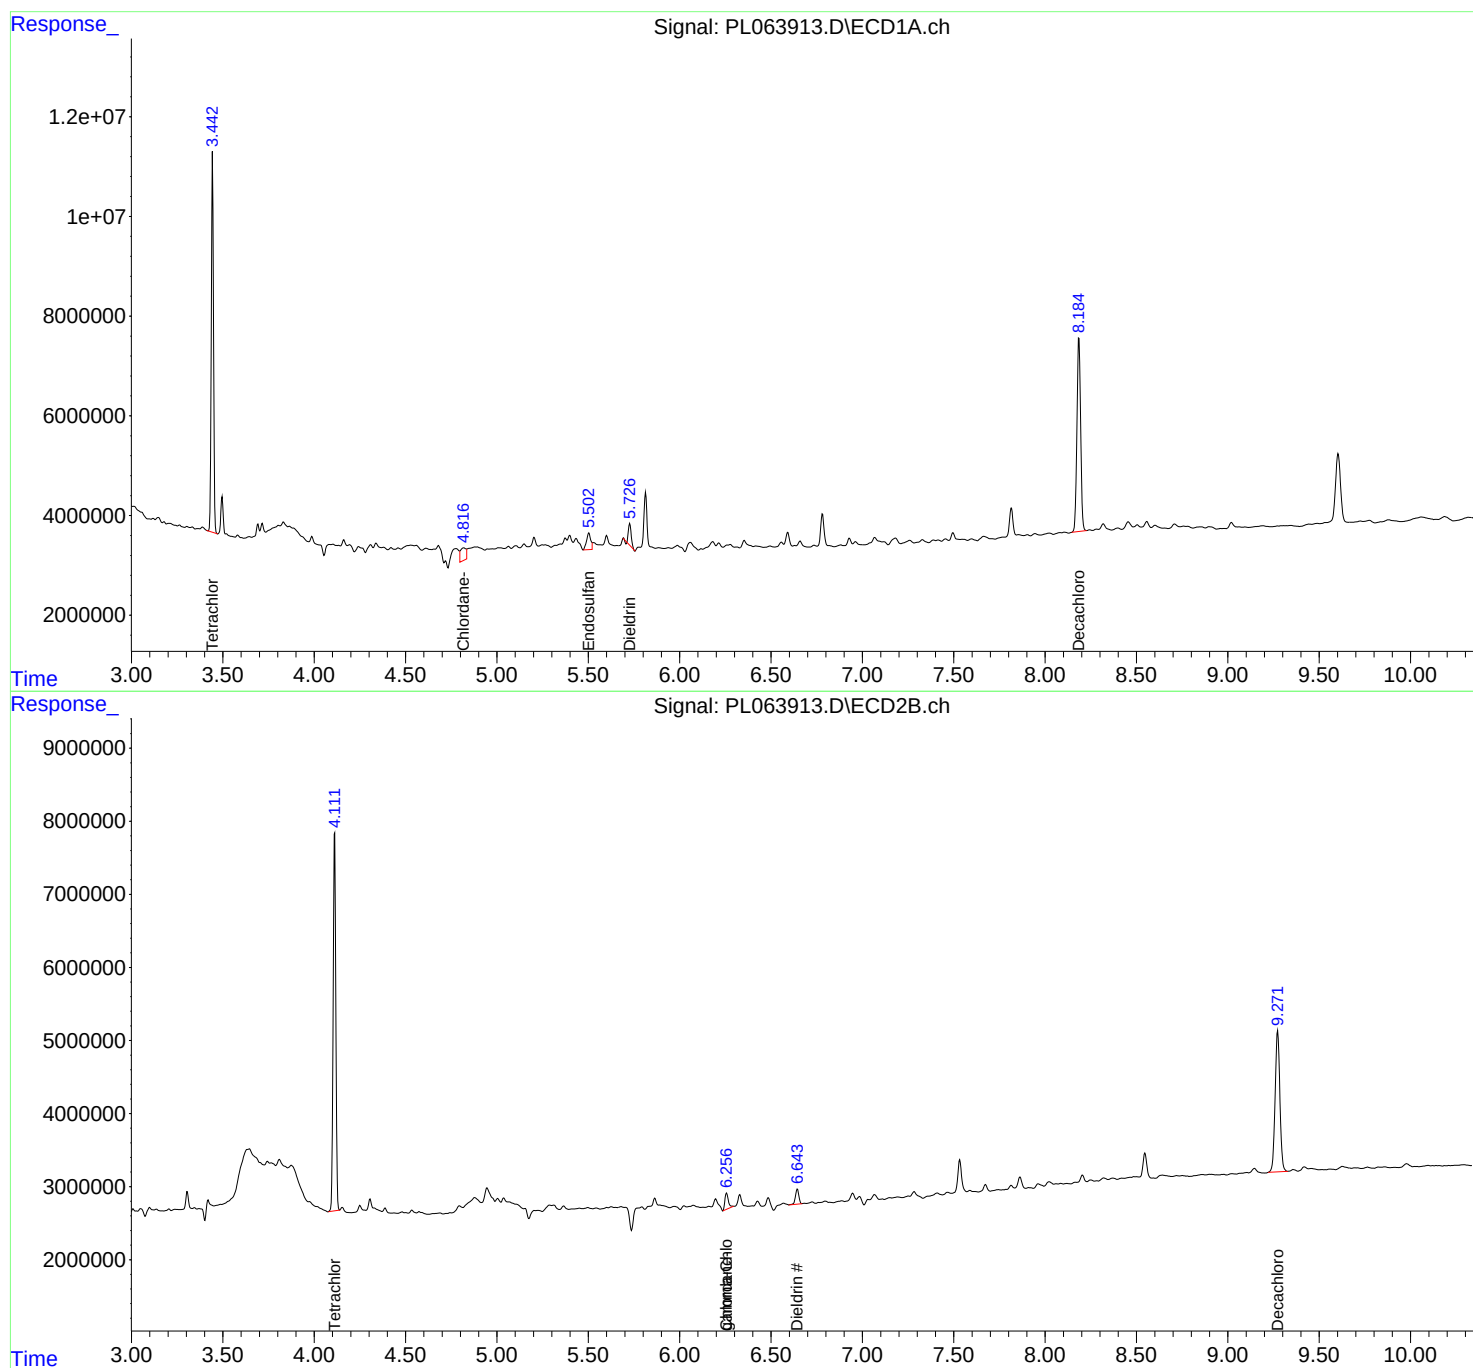


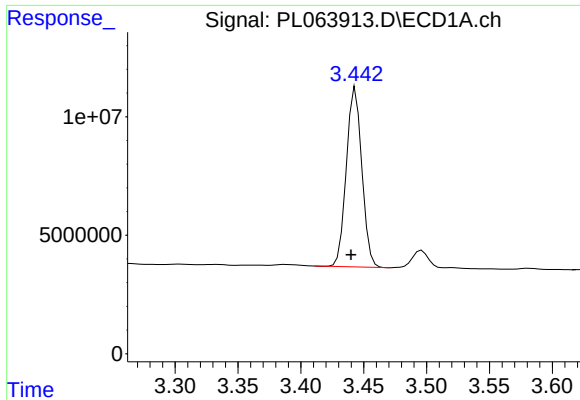

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: 0.004 min
Response: 64917431
Conc: 21.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

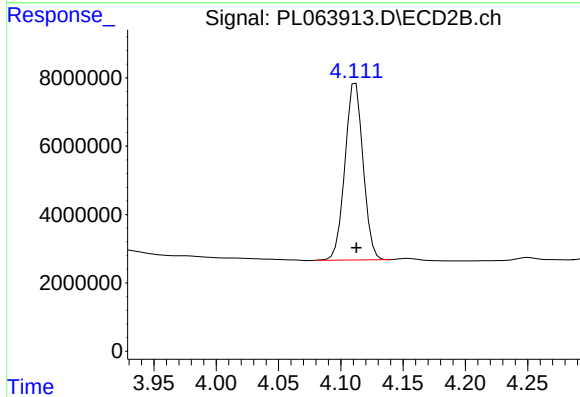


#1 Tetrachloro-m-xylene

R.T.: 4.112 min
Delta R.T.: 0.000 min
Response: 52809210
Conc: 20.68 ng/ml

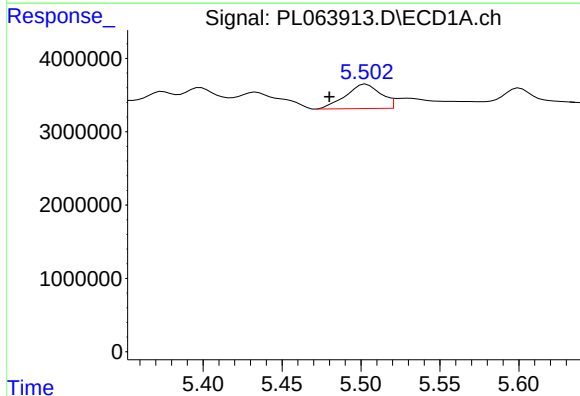


#9 Endosulfan I

R.T.: 5.503 min
Delta R.T.: 0.023 min
Response: 5203847
Conc: 1.50 ng/ml

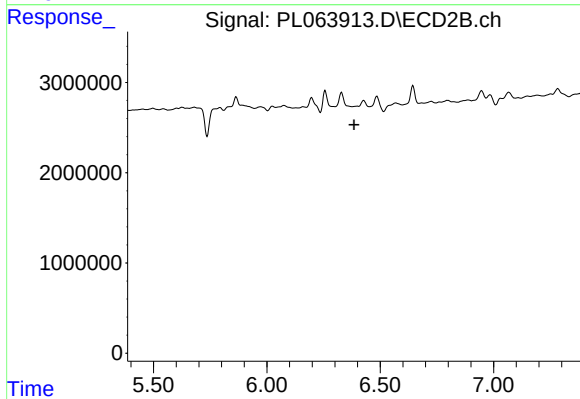

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.385 min
Response: 0
Conc: N.D.

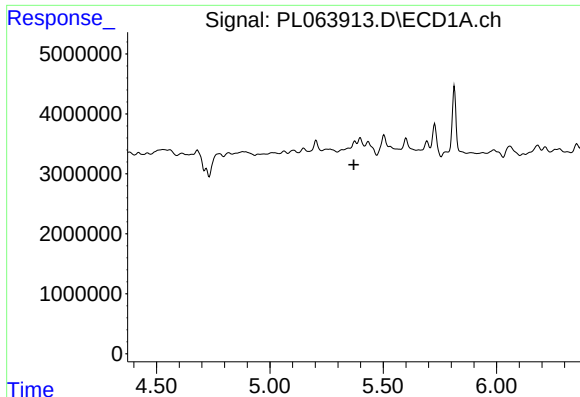

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.370 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

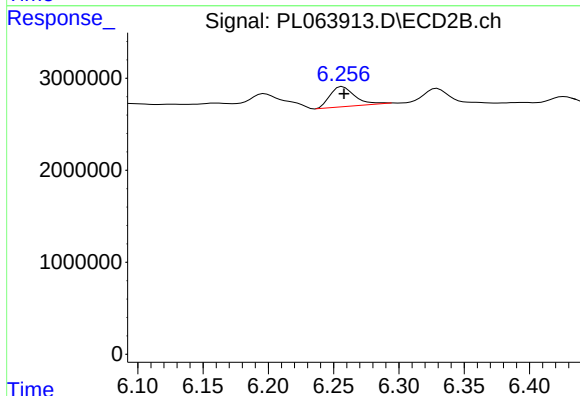


#10 gamma-Chlordane

R.T.: 6.257 min
Delta R.T.: 0.000 min
Response: 2848844
Conc: 1.03 ng/ml

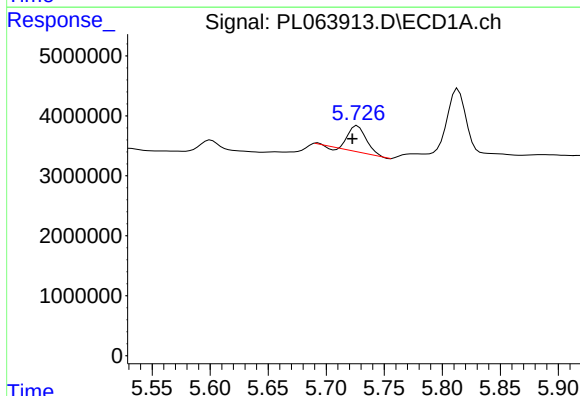


#13 Dieldrin

R.T.: 5.727 min
Delta R.T.: 0.004 min
Response: 4647701
Conc: 1.28 ng/ml

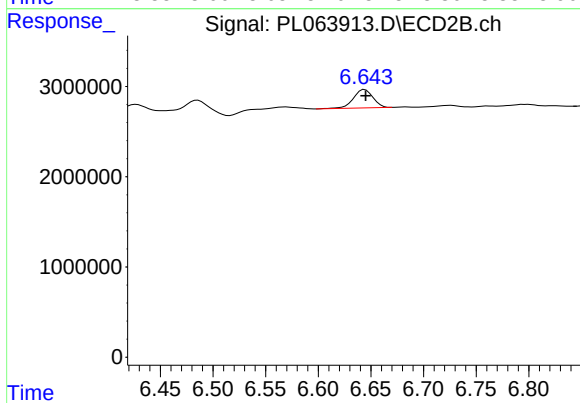

#13 Dieldrin


R.T.: 6.644 min
Delta R.T.: 0.000 min
Response: 2635701
Conc: 1.01 ng/ml

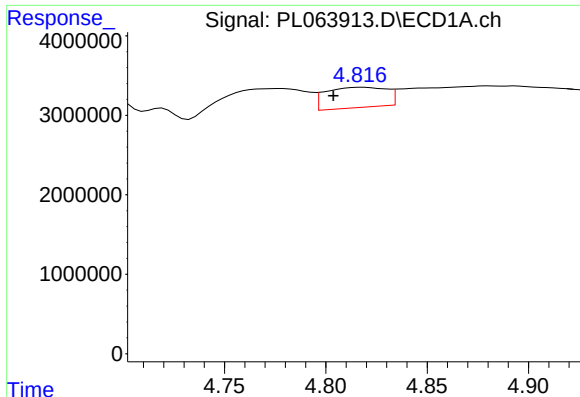

#24 Chlordane-2


R.T.: 4.818 min
Delta R.T.: 0.014 min
Response: 5298849
Conc: 45.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

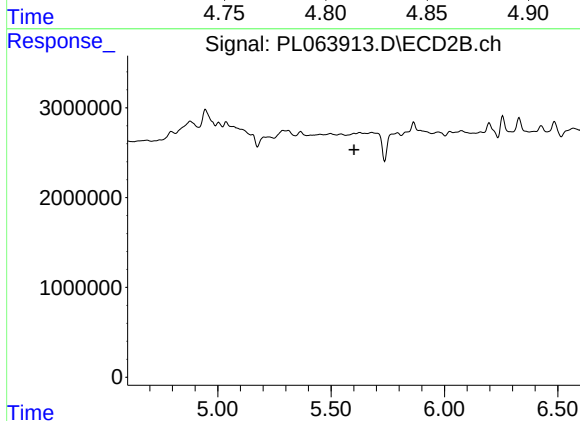


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.601 min
Response: 0
Conc: N.D.

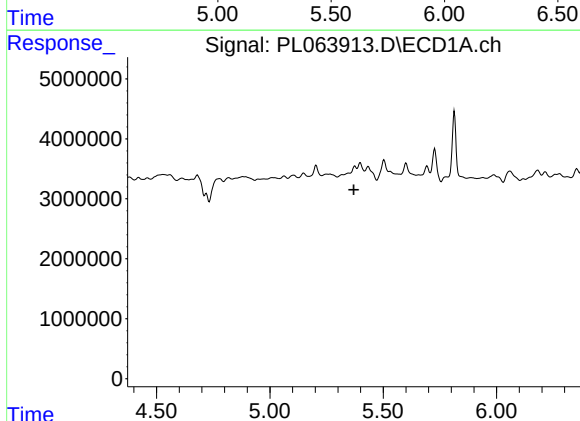


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.370 min
Response: 0
Conc: N.D.

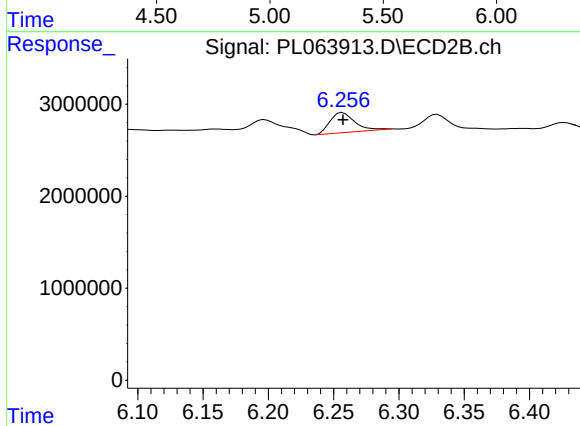

#25 Chlordane-3


R.T.: 6.257 min
Delta R.T.: 0.000 min
Response: 2848844
Conc: 8.31 ng/ml

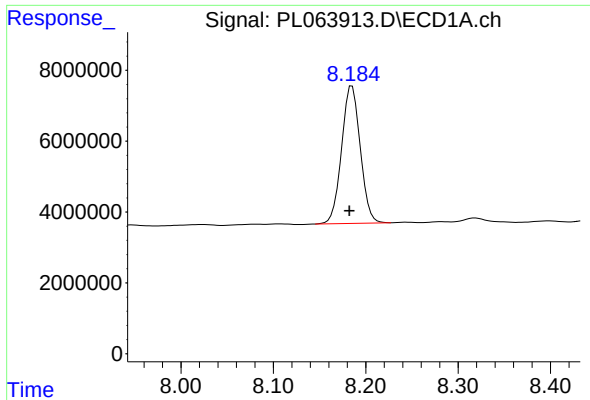

#28 Decachlorobiphenyl

R.T.: 8.185 min
Delta R.T.: 0.003 min
Response: 54493624
Conc: 19.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

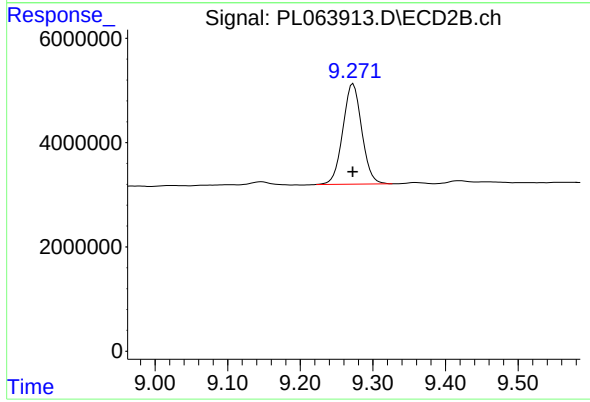

#28 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: 0.000 min
Response: 34921764
Conc: 17.71 ng/ml