

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010421\
 Data File : PL063913.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2021 13:36
 Operator : AR\AJ
 Sample : L5249-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BU-03-123120

Manual Integrations
 APPROVED

Ankita
 1/5/2021 9:50:16 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 04 15:08:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.112	64917431	52809210	21.654	20.685
28)	SA Decachlor...	8.185	9.273	54493624	34921764	19.779	17.712
Target Compounds							
13)	MA Dieldrin	5.726	6.644	6141446	2635701	1.694m	1.012 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010421\
Data File : PL063913.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2021 13:36
Operator : AR\AJ
Sample : L5249-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BU-03-123120


Manual Integrations
APPROVED

Ankita
1/5/2021 9:50:16 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 04 15:08:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

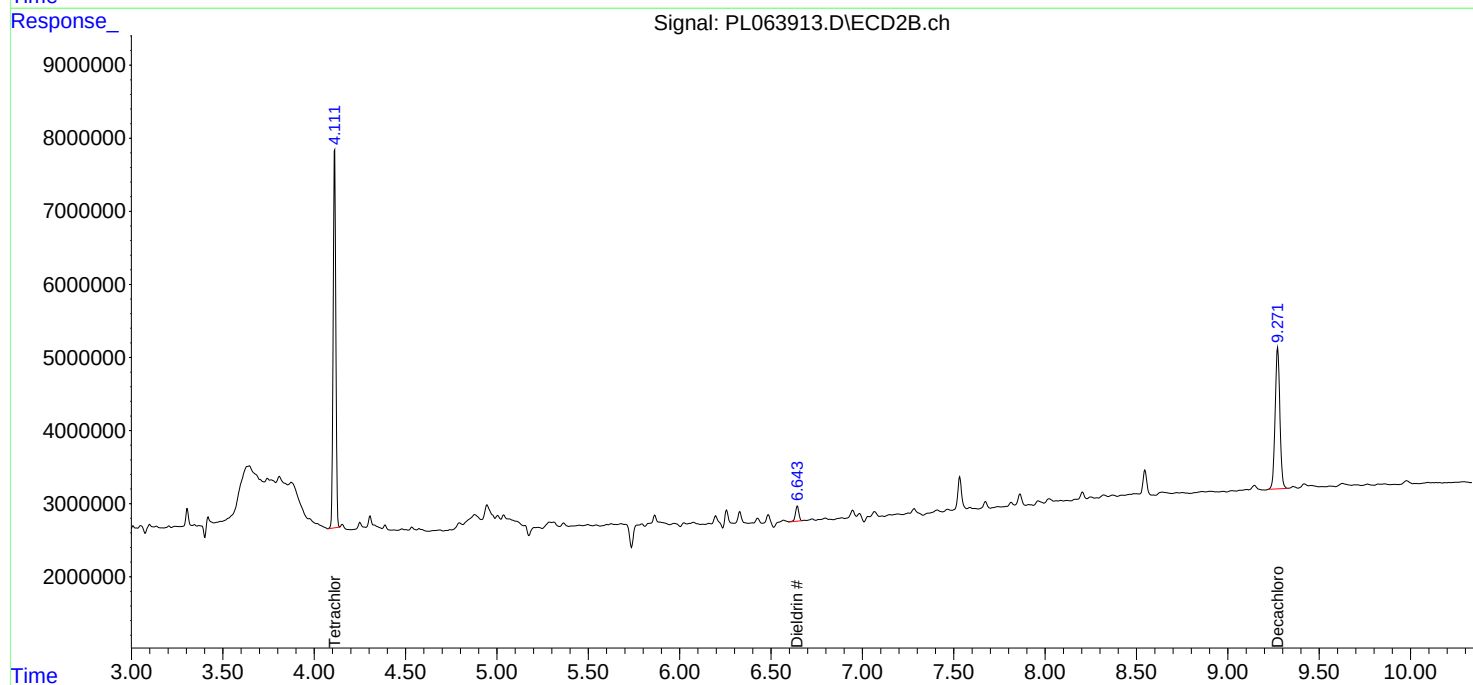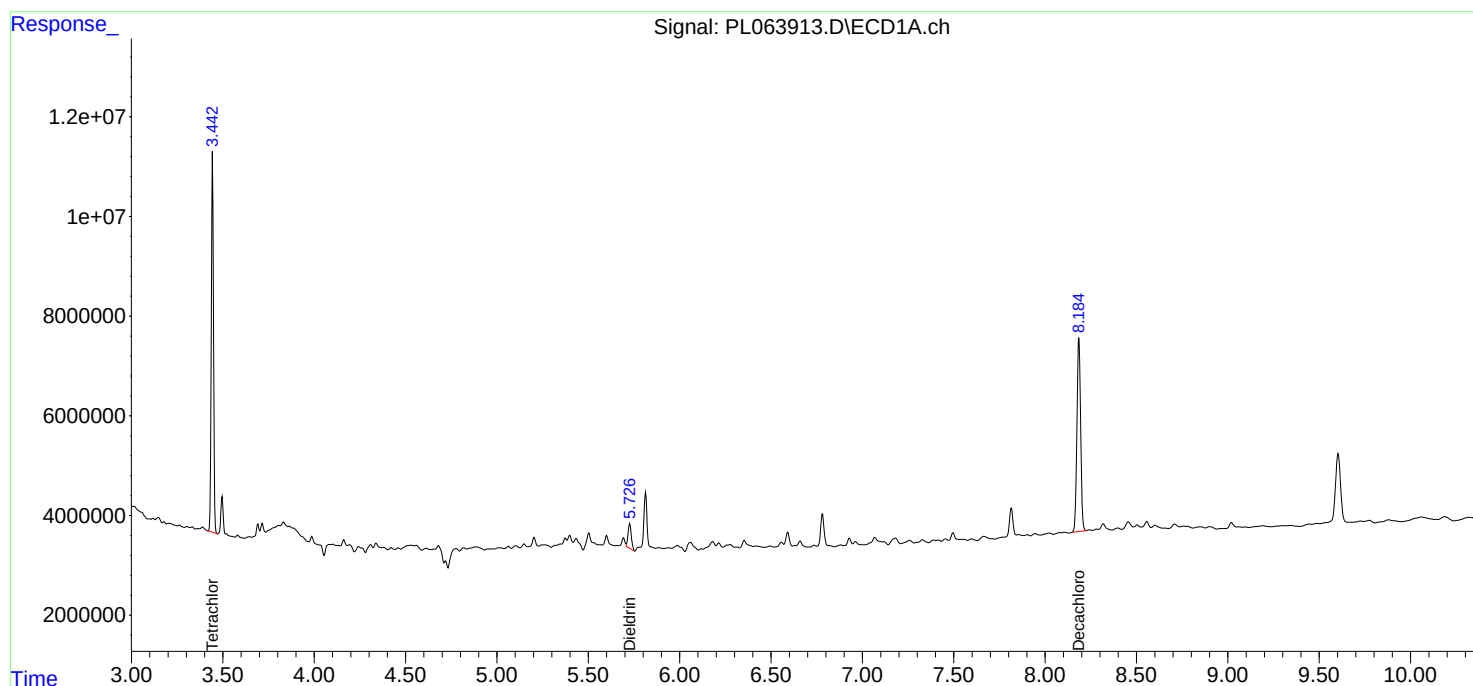

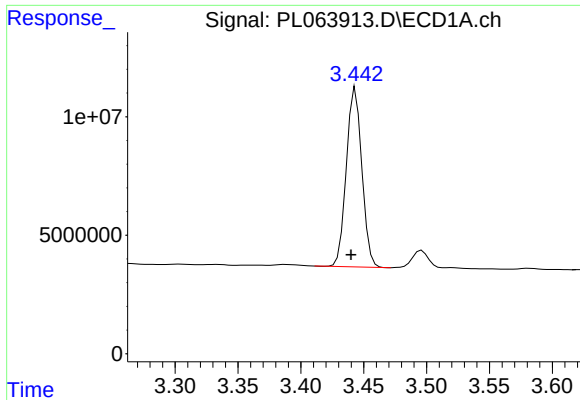


#1 Tetrachloro-m-xylene

R.T.: 3.444 min
Delta R.T.: 0.004 min
Response: 64917431
Conc: 21.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
BU-03-123120


Manual Integrations
APPROVED

Ankita
1/5/2021 9:50:16 AM

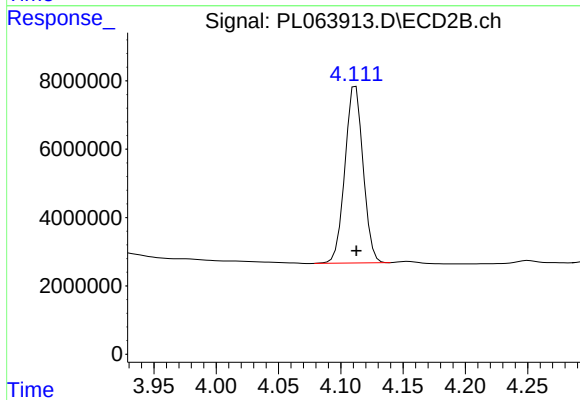


#1 Tetrachloro-m-xylene

R.T.: 4.112 min
Delta R.T.: 0.000 min
Response: 52809210
Conc: 20.68 ng/ml

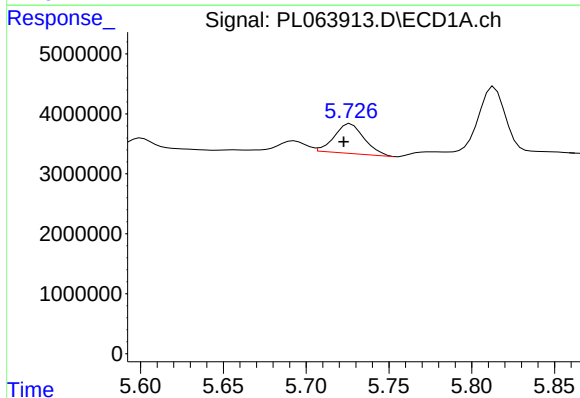


#13 Dieldrin

R.T.: 5.726 min
Delta R.T.: 0.003 min
Response: 6141446
Conc: 1.69 ng/ml m

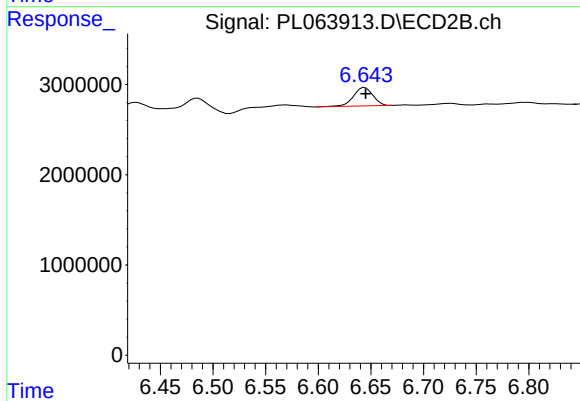

#13 Dieldrin

R.T.: 6.644 min
Delta R.T.: 0.000 min
Response: 2635701
Conc: 1.01 ng/ml

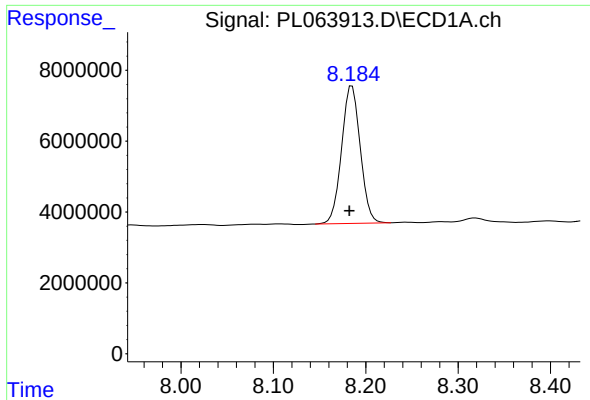


#28 Decachlorobiphenyl

R.T.: 8.185 min
Delta R.T.: 0.003 min
Response: 54493624
Conc: 19.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
BU-03-123120

Manual Integrations
APPROVED

Ankita
1/5/2021 9:50:16 AM

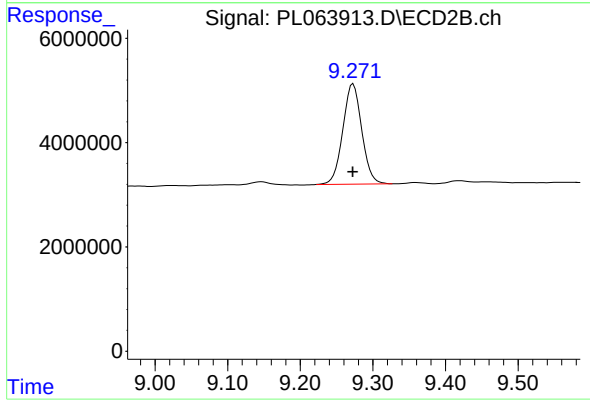

#28 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: 0.000 min
Response: 34921764
Conc: 17.71 ng/ml