

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010422\
 Data File : PL071783.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2022 16:07
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 01:51:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 05 01:51:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	10.339f	11.389	95113	46125	0.132	0.039 #
Target Compounds							
7)	B delta-BHC	0.000	7.019f	0	790916	N.D.	0.515 #
8)	B Heptachlo...	0.000	7.962	0	4755823	N.D.	3.403 #
10)	B gamma-Chl...	0.000	8.215	0	1139720	N.D.	0.833 #
11)	B alpha-Chl...	0.000	8.302	0	2191460	N.D.	1.647 #
13)	MA Dieldrin	7.690	0.000	1282889	0	2.127	N.D. #
14)	MA Endrin	7.999f	0.000	200147	0	0.379	N.D. #
15)	B Endosulfa...	0.000	9.145f	0	292301	N.D.	0.260 #
19)	B Endosulfa...	0.000	9.508	0	49546	N.D.	0.048 #
25)	Chlordane-3	0.000	8.215	0	1139720	N.D.	5.584 #
26)	Chlordane-4	0.000	8.302	0	2191460	N.D.	9.003 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010422\
Data File : PL071783.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2022 16:07
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 01:51:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Wed Jan 05 01:51:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

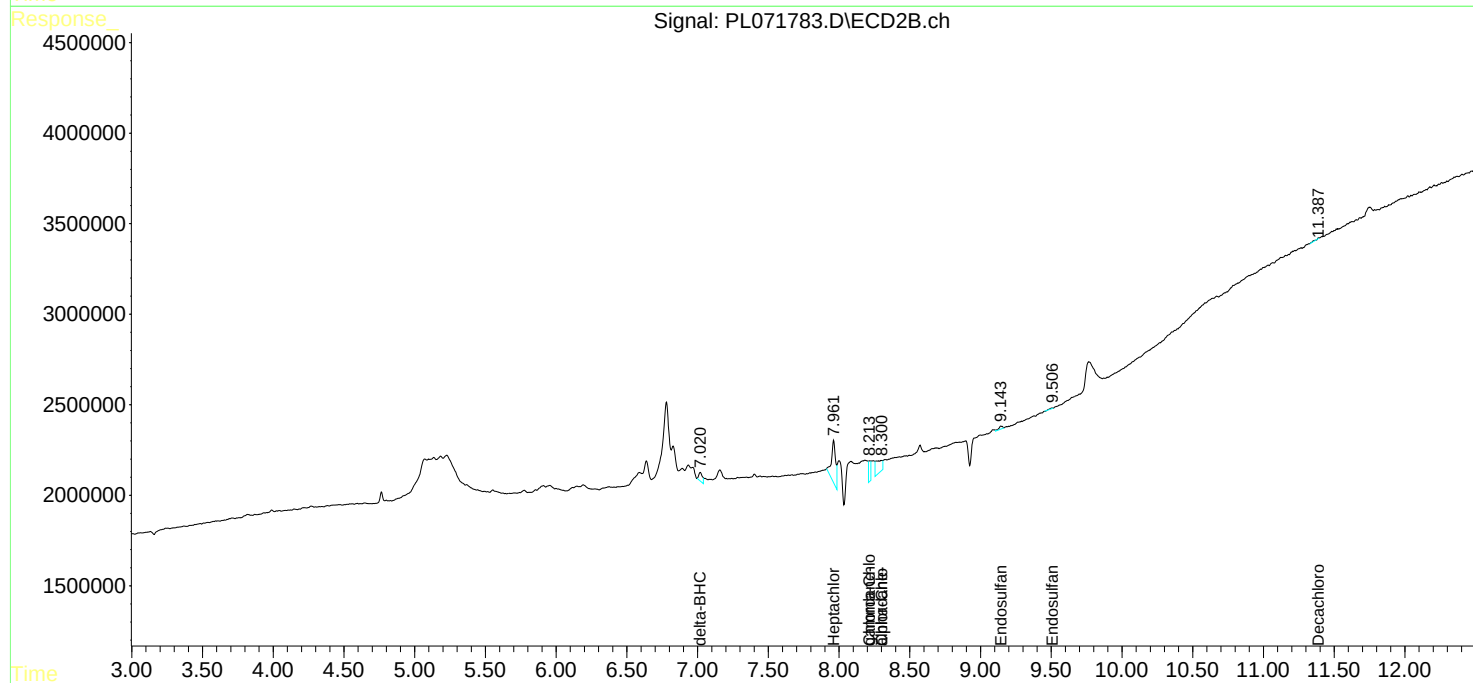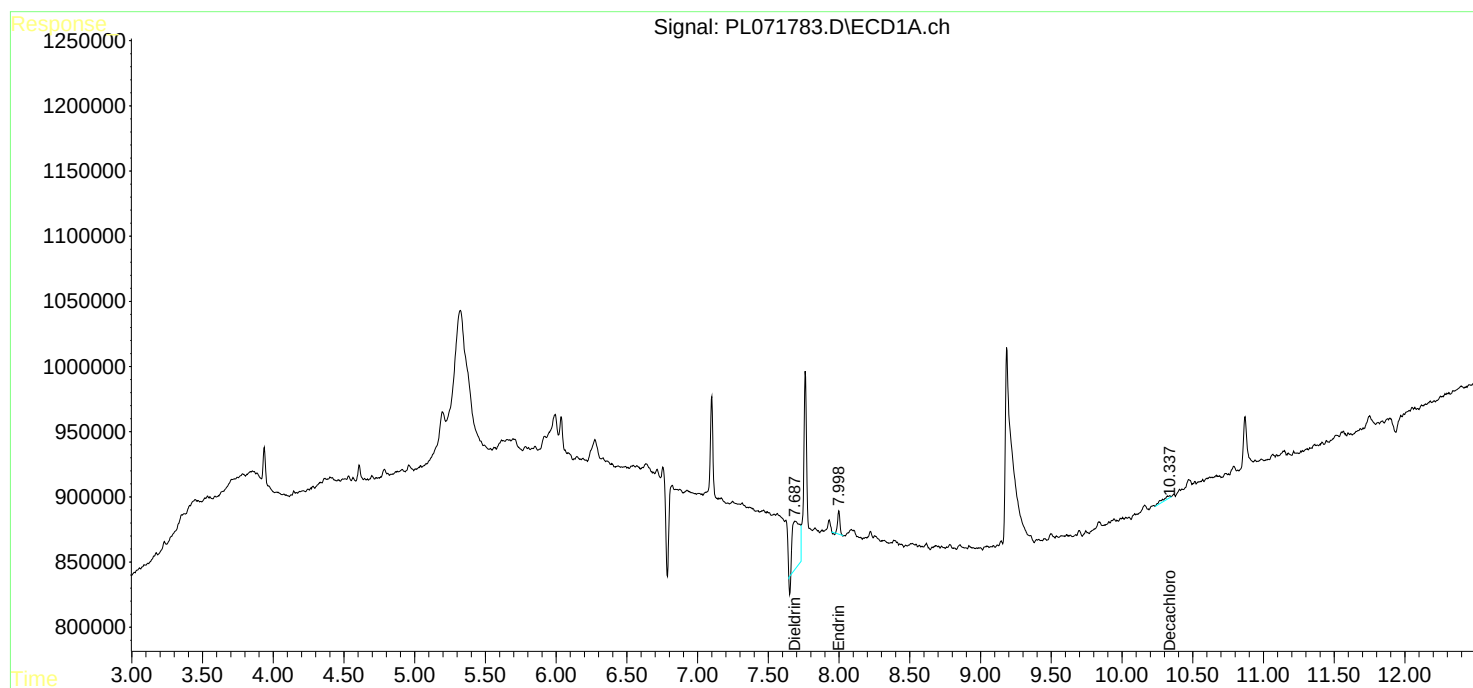


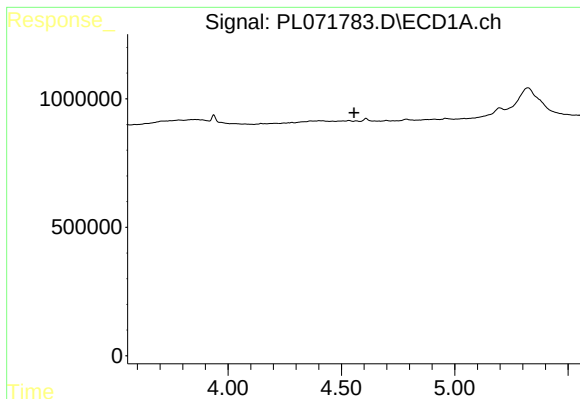

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.556 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

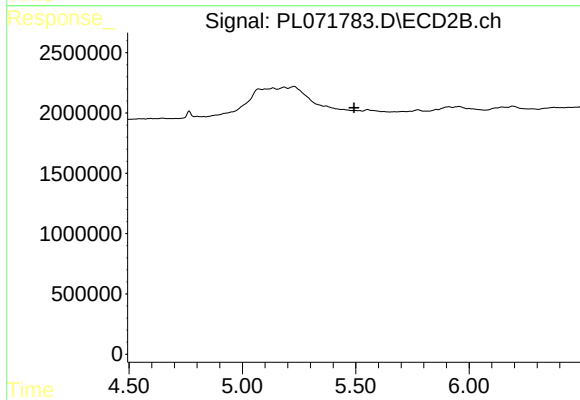


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.493 min
Response: 0
Conc: N.D.

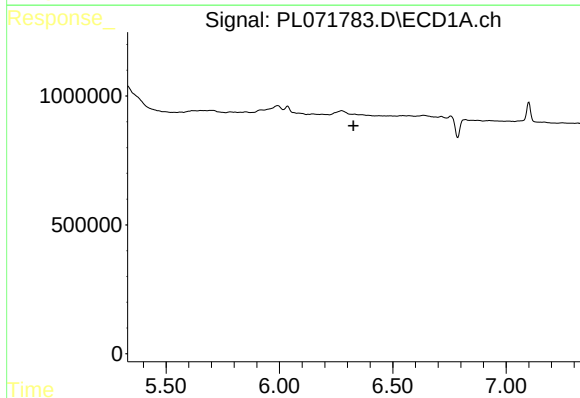


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.327 min
Response: 0
Conc: N.D.

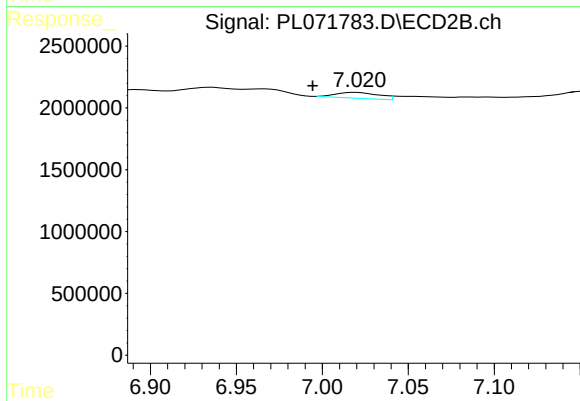

#7 delta-BHC


R.T.: 7.019 min
Delta R.T.: 0.025 min
Response: 790916
Conc: 0.52 ng/ml

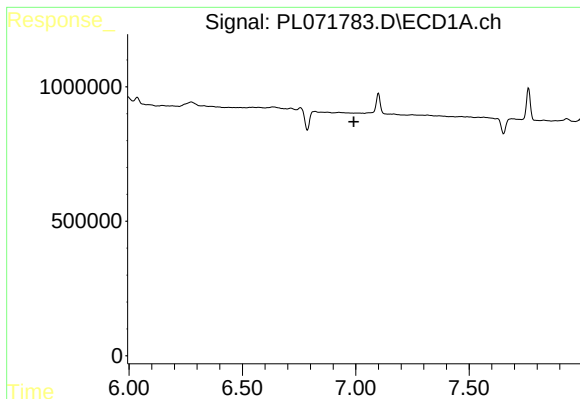

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.992 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

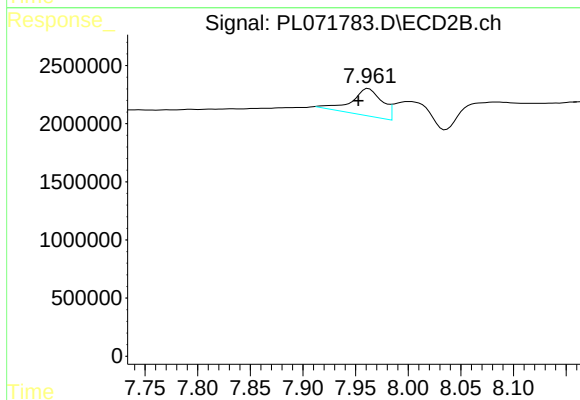


#8 Heptachlor epoxide

R.T.: 7.962 min
Delta R.T.: 0.010 min
Response: 4755823
Conc: 3.40 ng/ml

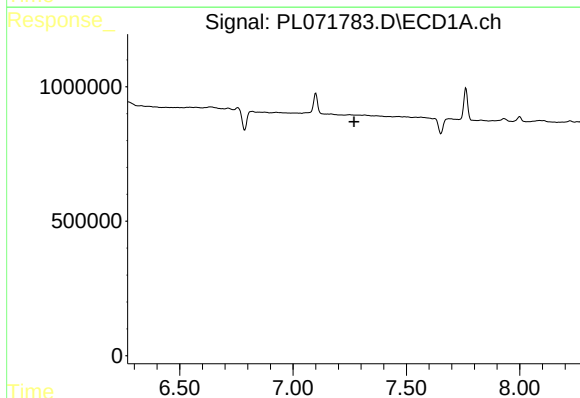


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

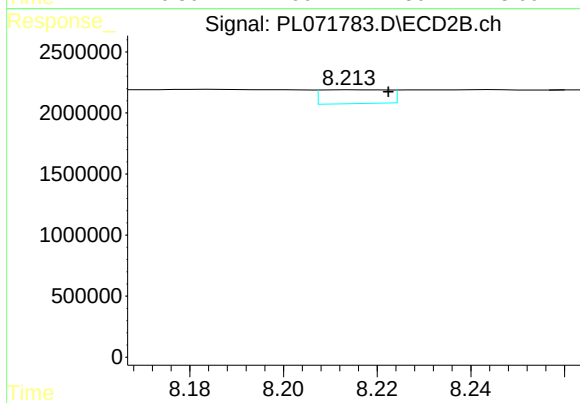

#10 gamma-Chlordane


R.T.: 8.215 min
Delta R.T.: -0.007 min
Response: 1139720
Conc: 0.83 ng/ml

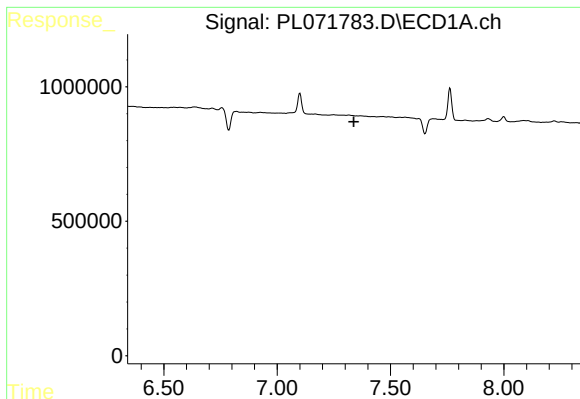

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.338 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

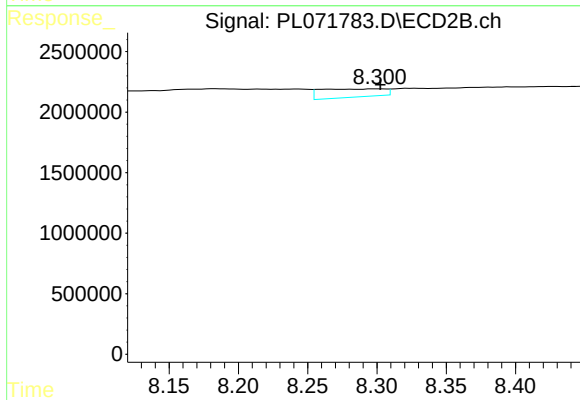


#11 alpha-Chlordane

R.T.: 8.302 min
Delta R.T.: 0.000 min
Response: 2191460
Conc: 1.65 ng/ml

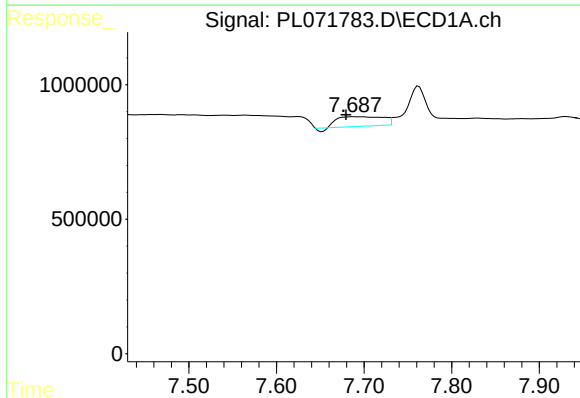


#13 Dieldrin

R.T.: 7.690 min
Delta R.T.: 0.010 min
Response: 1282889
Conc: 2.13 ng/ml

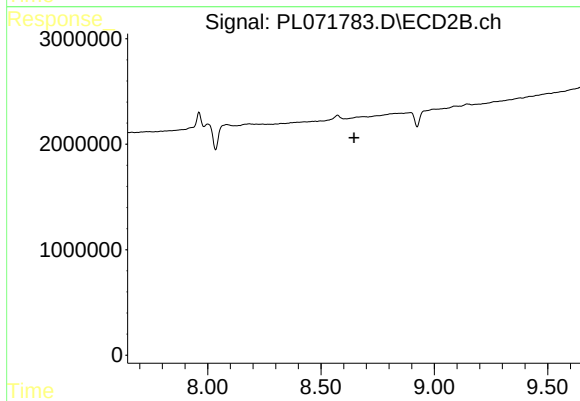

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.646 min
Response: 0
Conc: N.D.

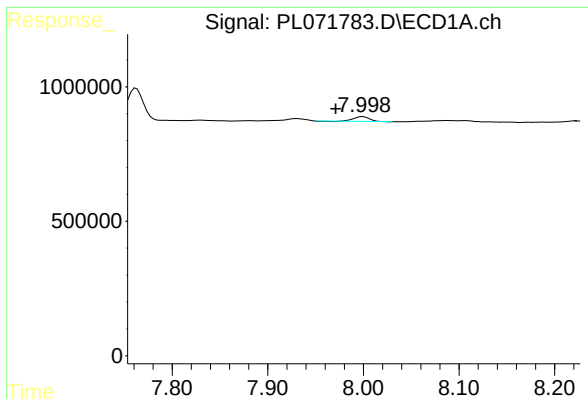

#14 Endrin


R.T.: 7.999 min
Delta R.T.: 0.028 min
Response: 200147
Conc: 0.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

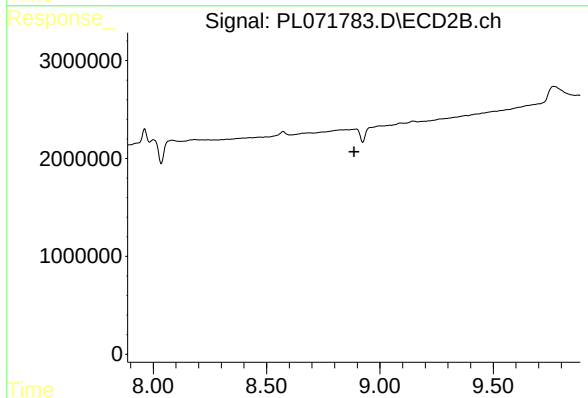


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.886 min
Response: 0
Conc: N.D.

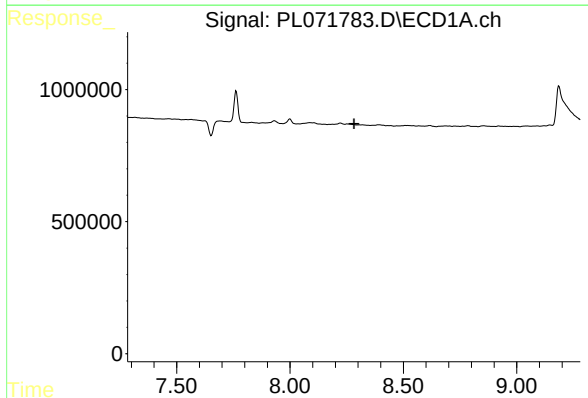


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.283 min
Response: 0
Conc: N.D.

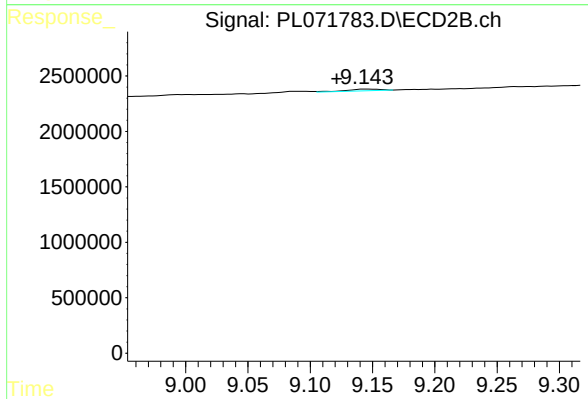

#15 Endosulfan II


R.T.: 9.145 min
Delta R.T.: 0.024 min
Response: 292301
Conc: 0.26 ng/ml

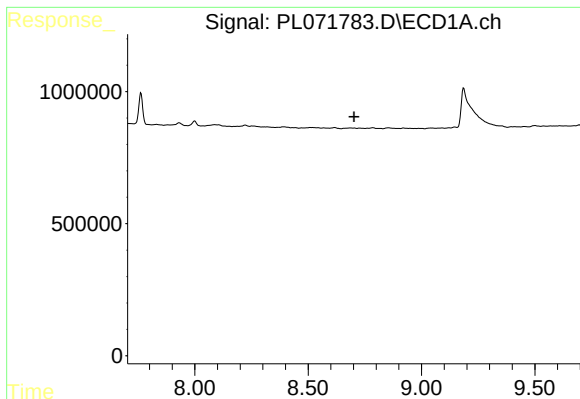

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 8.703 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

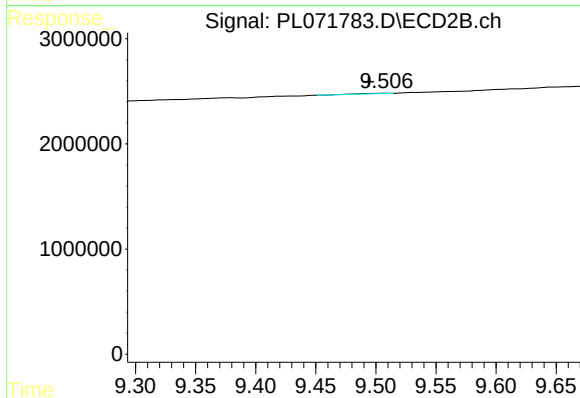


#19 Endosulfan Sulfate

R.T.: 9.508 min
Delta R.T.: 0.014 min
Response: 49546
Conc: 0.05 ng/ml

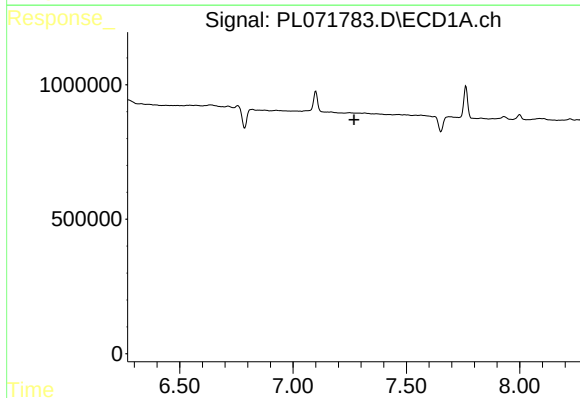


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

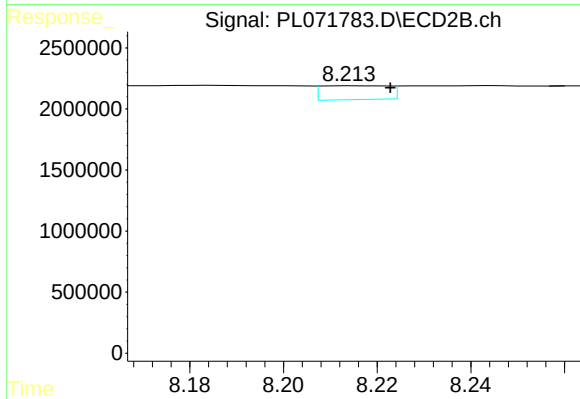

#25 Chlordane-3


R.T.: 8.215 min
Delta R.T.: -0.007 min
Response: 1139720
Conc: 5.58 ng/ml

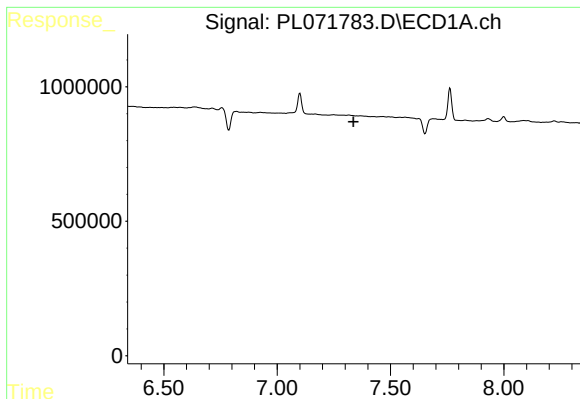

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.337 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

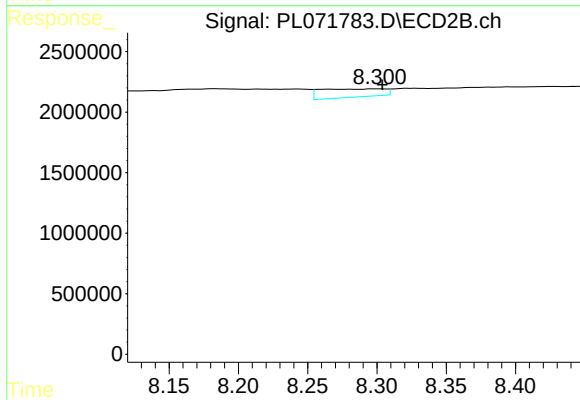


#26 Chlordane-4

R.T.: 8.302 min
Delta R.T.: -0.002 min
Response: 2191460
Conc: 9.00 ng/ml

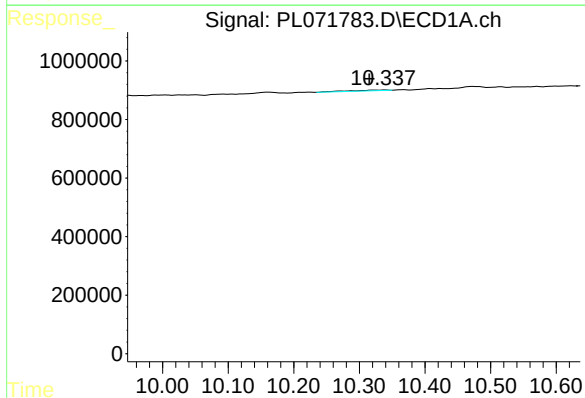

#28 Decachlorobiphenyl

R.T.: 10.339 min
Delta R.T.: 0.023 min
Response: 95113
Conc: 0.13 ng/ml

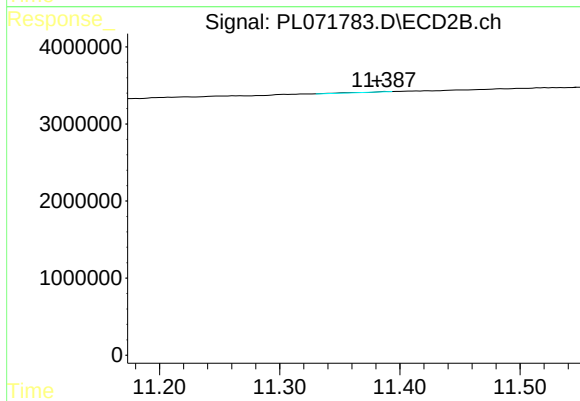

#28 Decachlorobiphenyl

R.T.: 11.389 min
Delta R.T.: 0.008 min
Response: 46125
Conc: 0.04 ng/ml