

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010422\
 Data File : PL071784.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2022 16:24
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 01:51:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 05 01:51:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.557	5.493	8403514	22321356	18.191	18.167
28)	SA Decachlor...	10.316	11.382	14055141	22128164	19.439	18.673
Target Compounds							
8)	B Heptachlo...	0.000	7.962	0	1183120	N.D.	0.847 #
9)	A Endosulfan I	0.000	8.381f	0	542160	N.D.	0.438 #
10)	B gamma-Chl...	0.000	8.223	0	565629	N.D.	0.414 #
13)	MA Dieldrin	7.684	8.672f	148349	111401	0.246	0.085 #
25)	Chlordane-3	0.000	8.223	0	565629	N.D.	2.771 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010422\
Data File : PL071784.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2022 16:24
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 01:51:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Wed Jan 05 01:51:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

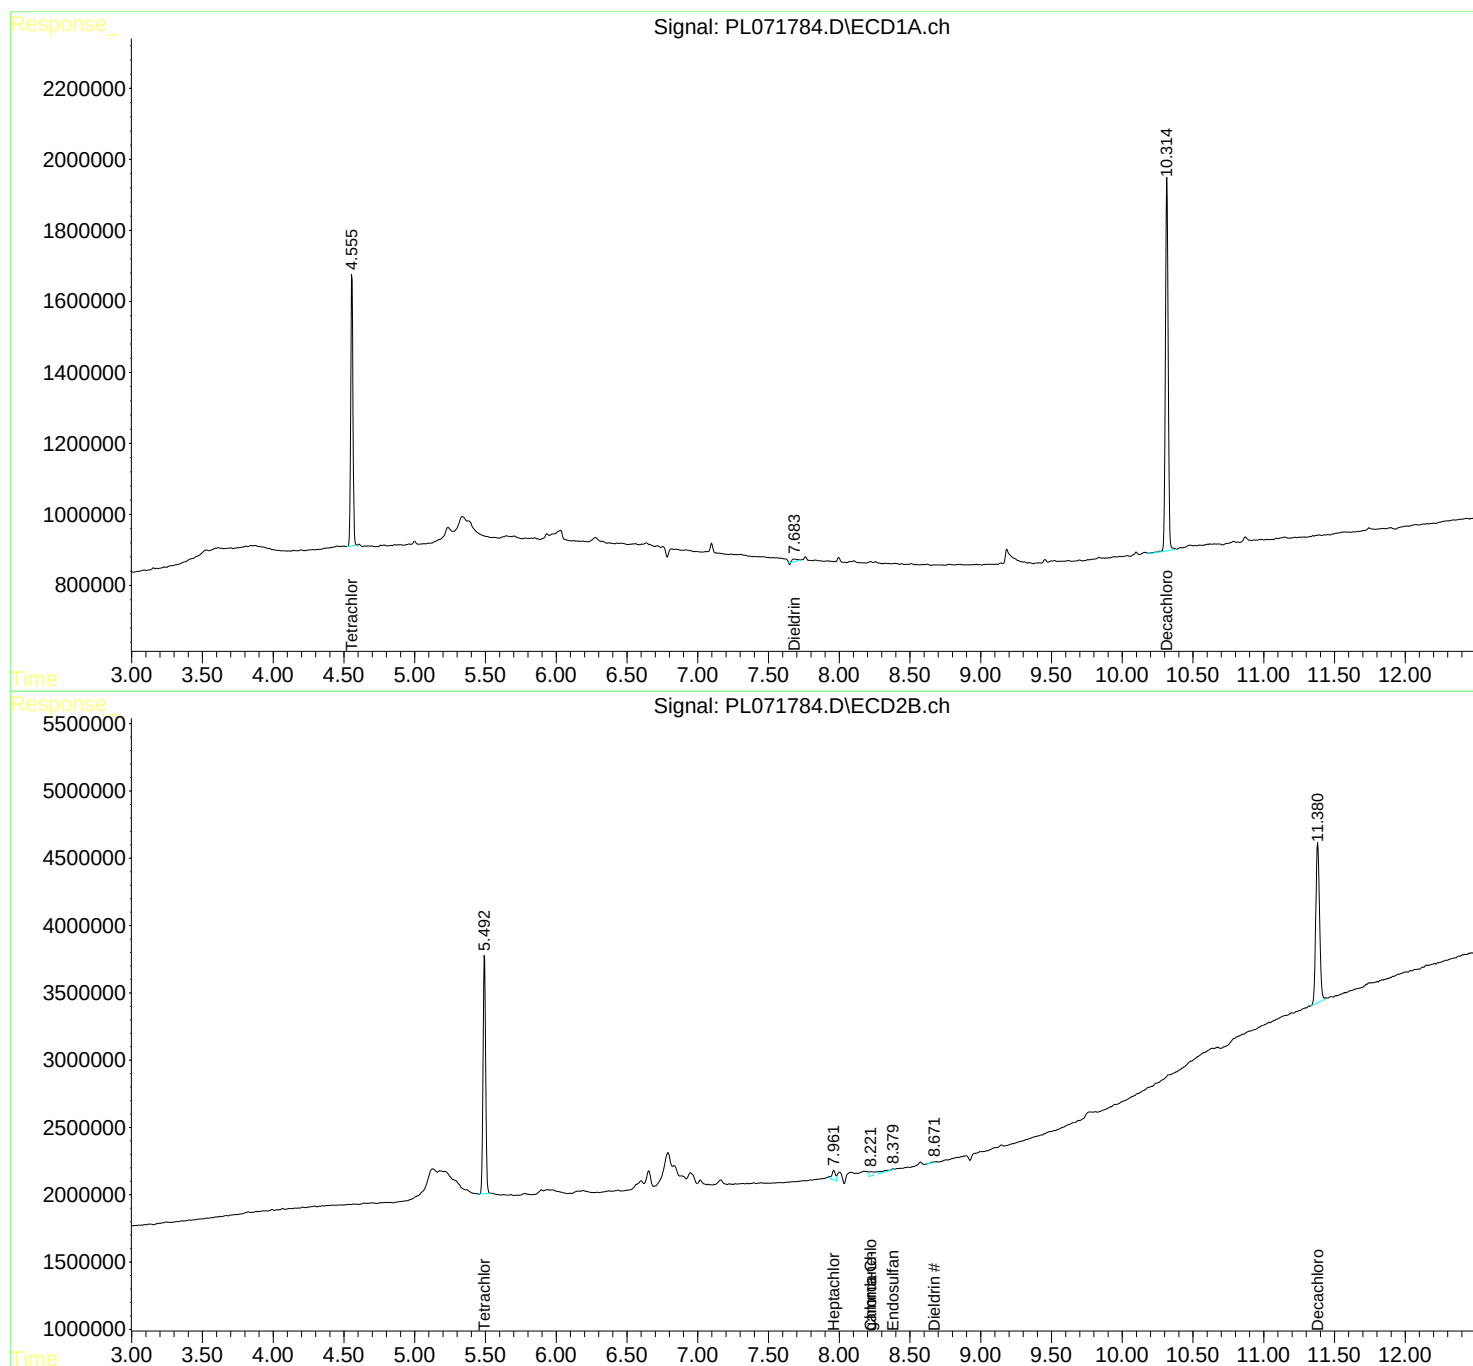


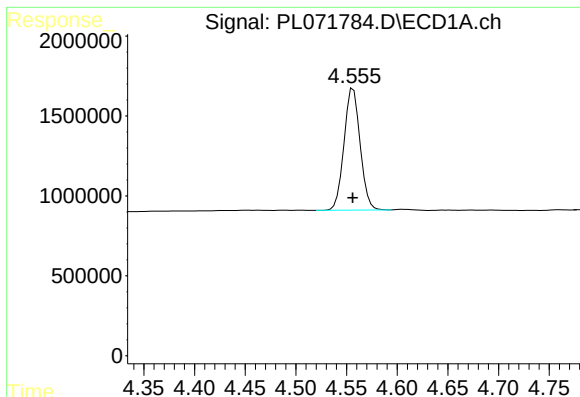

#1 Tetrachloro-m-xylene


R.T.: 4.557 min
Delta R.T.: 0.000 min
Response: 8403514
Conc: 18.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

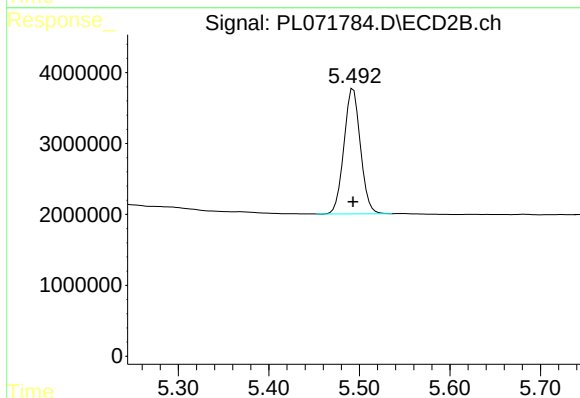


#1 Tetrachloro-m-xylene

R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 22321356
Conc: 18.17 ng/ml

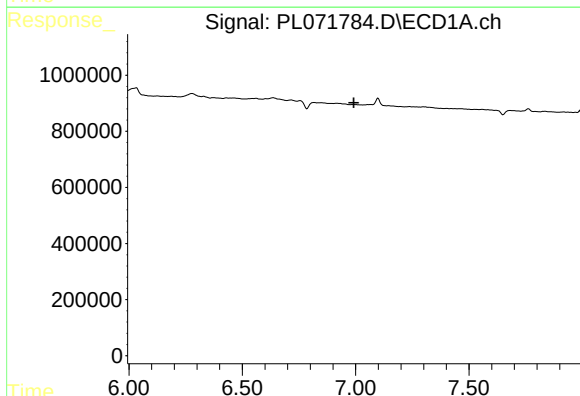


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 6.992 min
Response: 0
Conc: N.D.

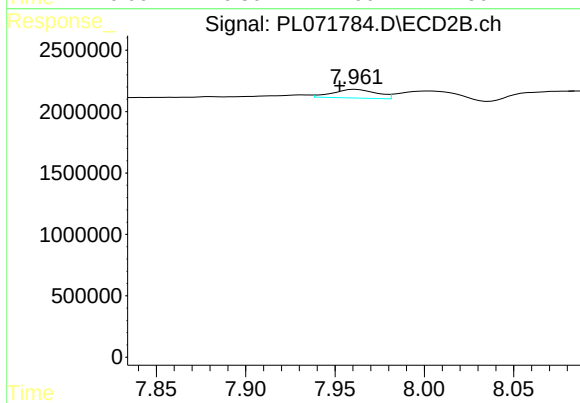

#8 Heptachlor epoxide


R.T.: 7.962 min
Delta R.T.: 0.009 min
Response: 1183120
Conc: 0.85 ng/ml

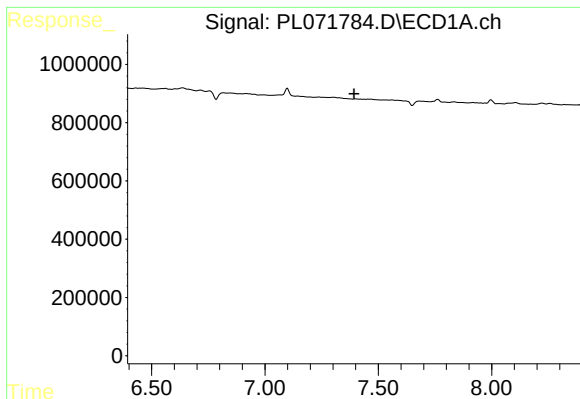

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.394 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

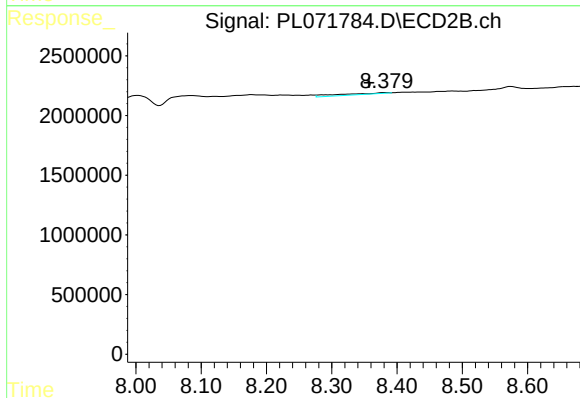


#9 Endosulfan I

R.T.: 8.381 min
Delta R.T.: 0.023 min
Response: 542160
Conc: 0.44 ng/ml

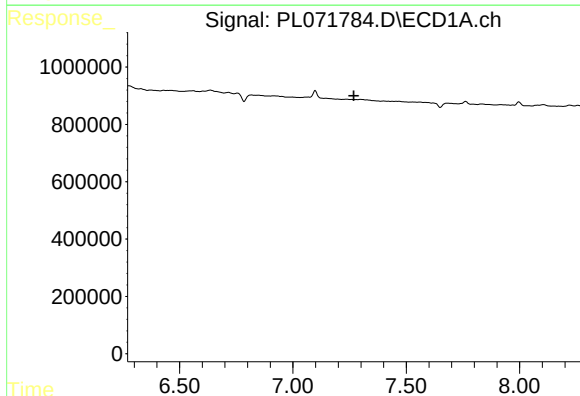


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

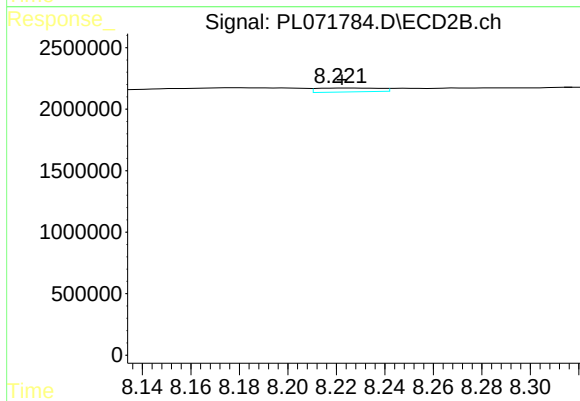

#10 gamma-Chlordane


R.T.: 8.223 min
Delta R.T.: 0.000 min
Response: 565629
Conc: 0.41 ng/ml

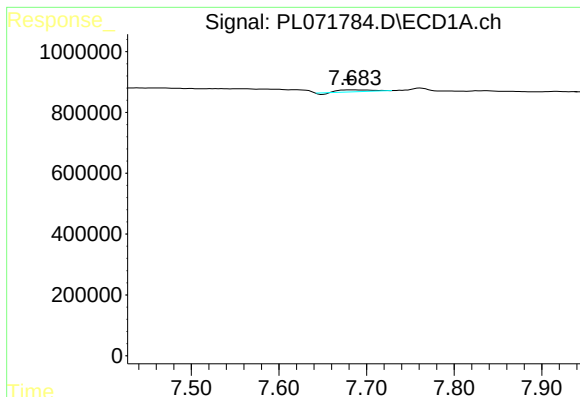

#13 Dieldrin


R.T.: 7.684 min
Delta R.T.: 0.004 min
Response: 148349
Conc: 0.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

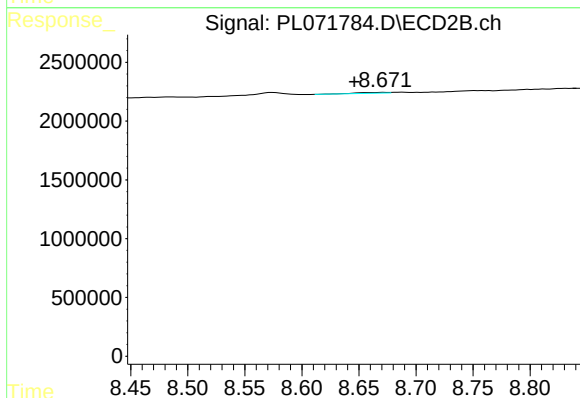


#13 Dieldrin

R.T.: 8.672 min
Delta R.T.: 0.026 min
Response: 111401
Conc: 0.08 ng/ml

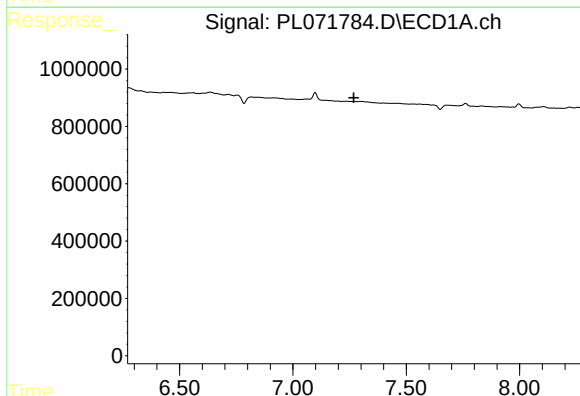


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.269 min
Response: 0
Conc: N.D.

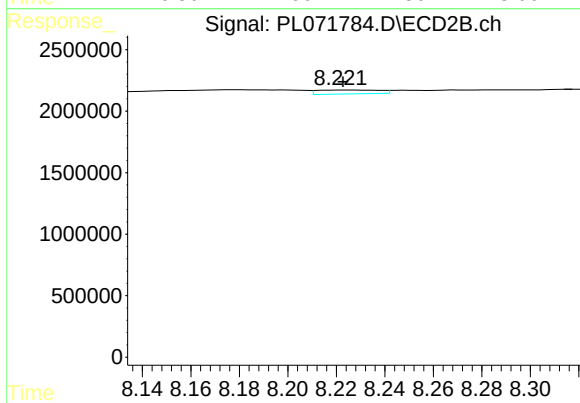

#25 Chlordane-3


R.T.: 8.223 min
Delta R.T.: 0.000 min
Response: 565629
Conc: 2.77 ng/ml

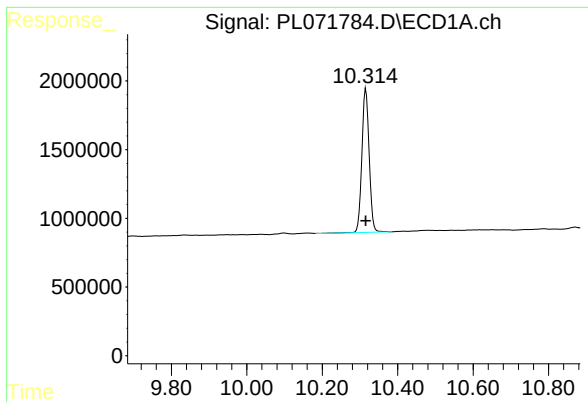

#28 Decachlorobiphenyl

R.T.: 10.316 min
Delta R.T.: 0.000 min
Response: 14055141
Conc: 19.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

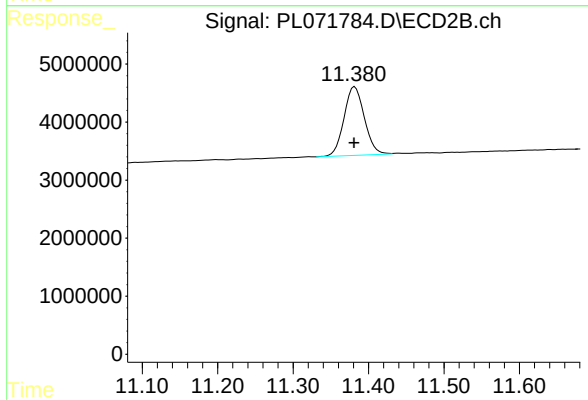

#28 Decachlorobiphenyl

R.T.: 11.382 min
Delta R.T.: 0.000 min
Response: 22128164
Conc: 18.67 ng/ml