

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010422\
 Data File : PL071794.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2022 19:10
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 01:02:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 05 00:57:02 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.492	24504448	63724380	50.000	50.000
28)	SA Decachlor...	10.315	11.381	36552746	60372132	50.000	50.000
Target Compounds							
23)	Chlordane-1	5.880	6.873	9036170	25642302	500.000	500.000
24)	Chlordane-2	6.569	7.465	12179626	27100813	500.000	500.000
25)	Chlordane-3	7.269	8.223	33503998	104.2E6	500.000	500.000
26)	Chlordane-4	7.336	8.304	35836268	124.4E6	500.000	500.000
27)	Chlordane-5	8.286	9.190	12170724	20524326	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010422\
Data File : PL071794.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2022 19:10
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 01:02:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Wed Jan 05 00:57:02 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

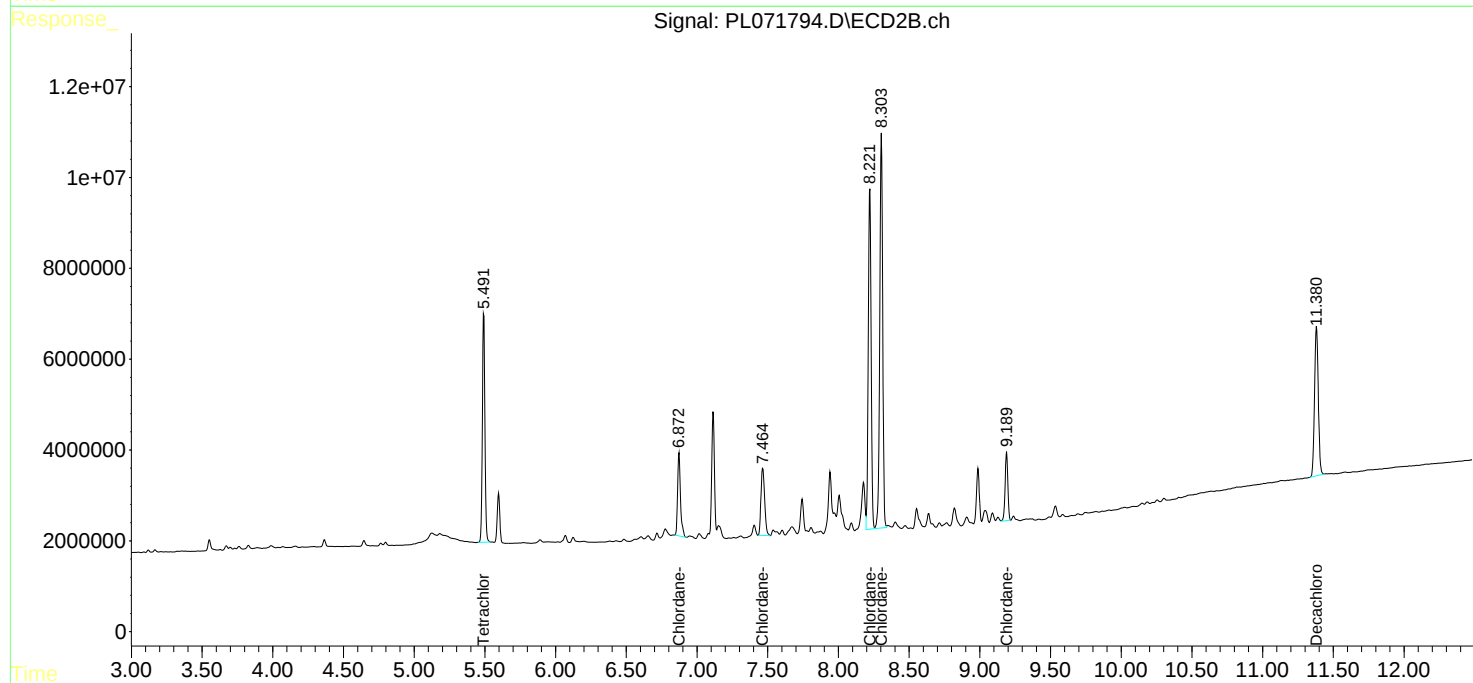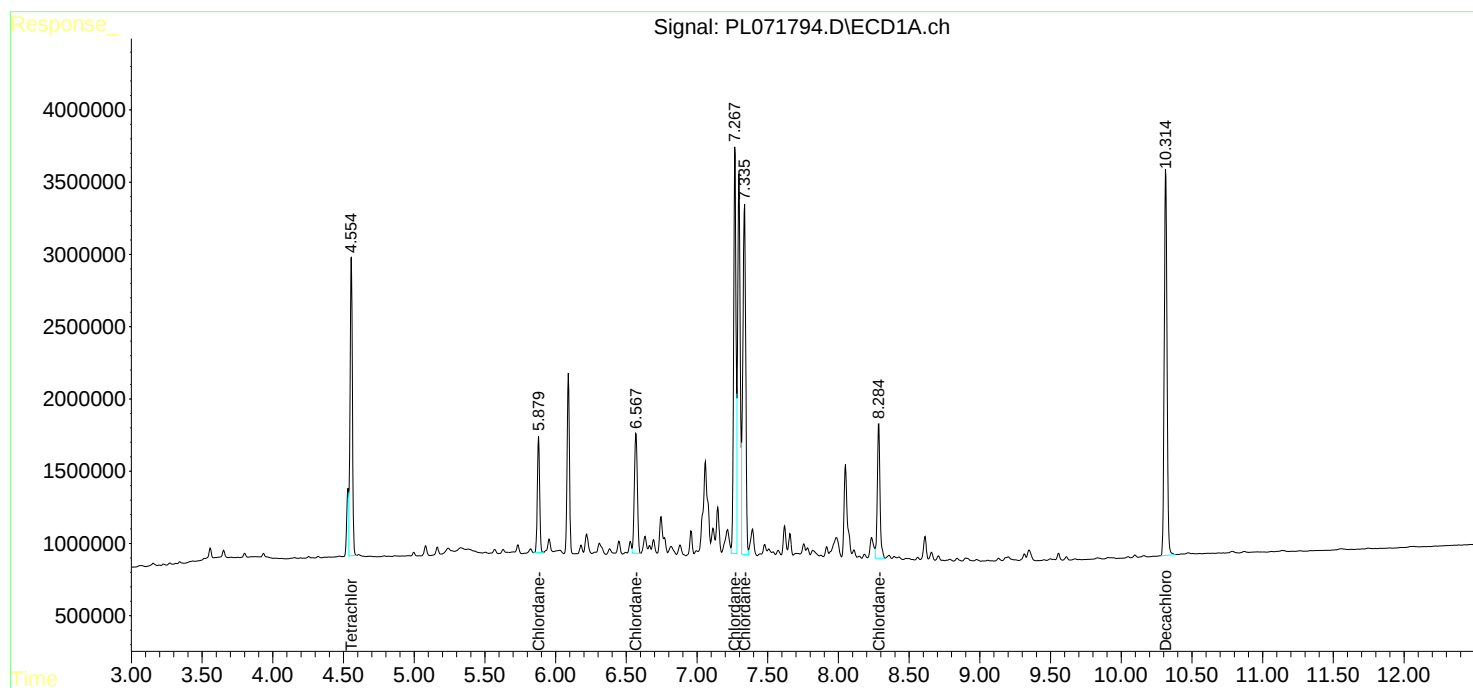


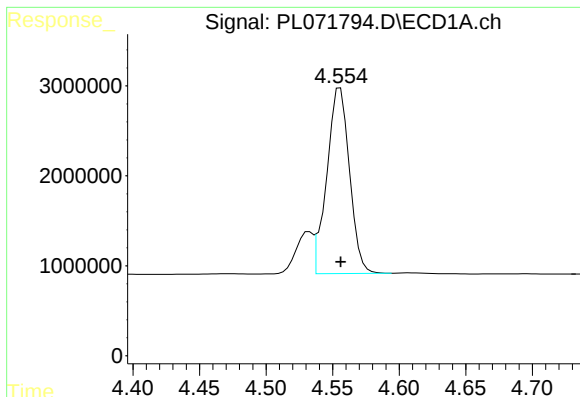

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: 0.000 min
Response: 24504448
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

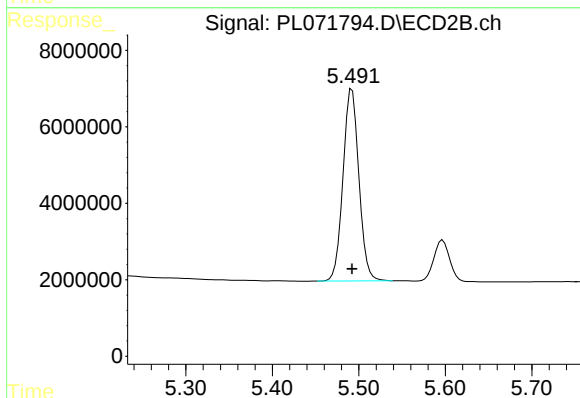


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: 0.000 min
Response: 63724380
Conc: 50.00 ng/ml

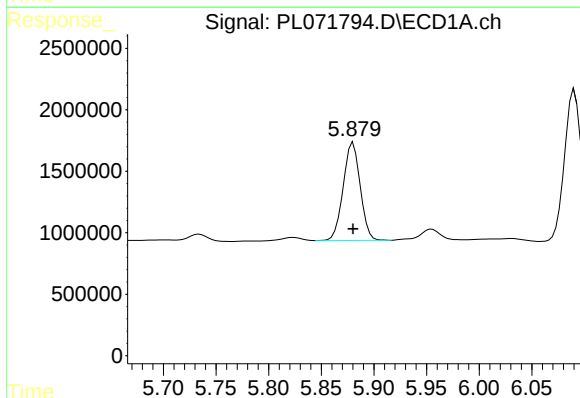


#23 Chlordane-1

R.T.: 5.880 min
Delta R.T.: 0.000 min
Response: 9036170
Conc: 500.00 ng/ml

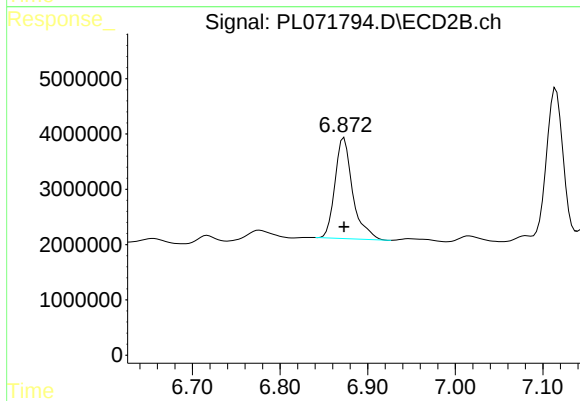

#23 Chlordane-1


R.T.: 6.873 min
Delta R.T.: 0.000 min
Response: 25642302
Conc: 500.00 ng/ml

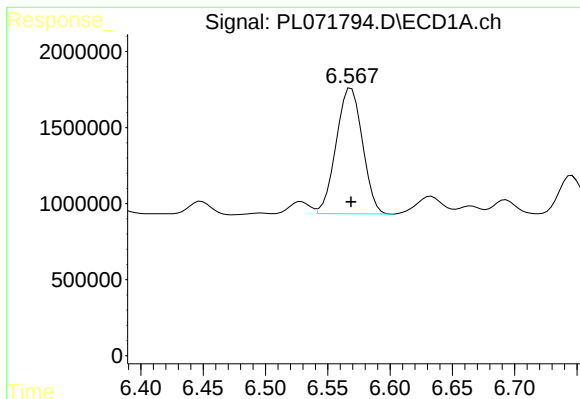

#24 Chlordane-2


R.T.: 6.569 min
Delta R.T.: 0.000 min
Response: 12179626
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

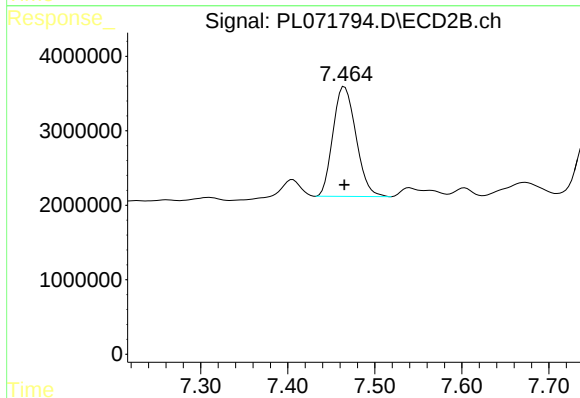


#24 Chlordane-2

R.T.: 7.465 min
Delta R.T.: 0.000 min
Response: 27100813
Conc: 500.00 ng/ml

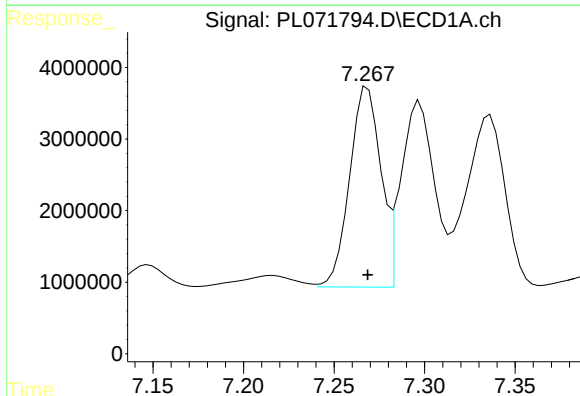


#25 Chlordane-3

R.T.: 7.269 min
Delta R.T.: 0.000 min
Response: 33503998
Conc: 500.00 ng/ml

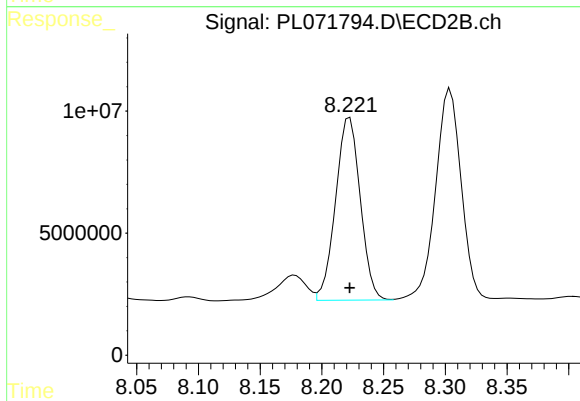

#25 Chlordane-3


R.T.: 8.223 min
Delta R.T.: 0.000 min
Response: 104172029
Conc: 500.00 ng/ml

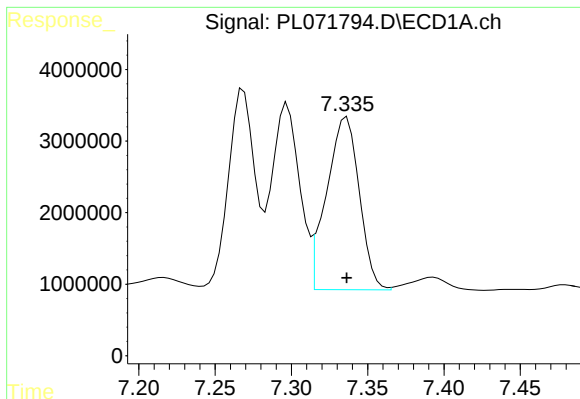

#26 Chlordane-4


R.T.: 7.336 min
Delta R.T.: 0.000 min
Response: 35836268
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

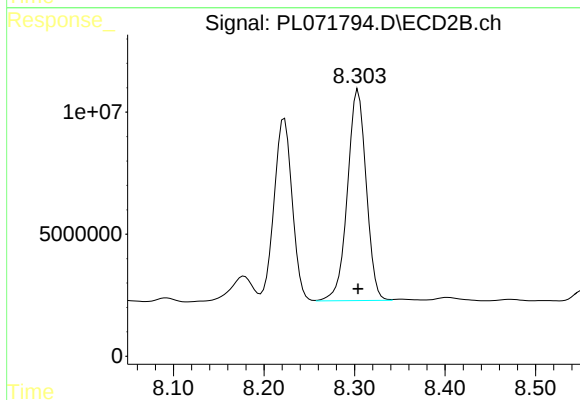


#26 Chlordane-4

R.T.: 8.304 min
Delta R.T.: 0.000 min
Response: 124381048
Conc: 500.00 ng/ml

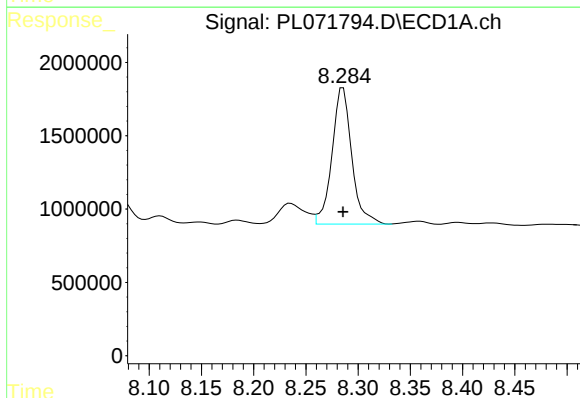


#27 Chlordane-5

R.T.: 8.286 min
Delta R.T.: 0.000 min
Response: 12170724
Conc: 500.00 ng/ml

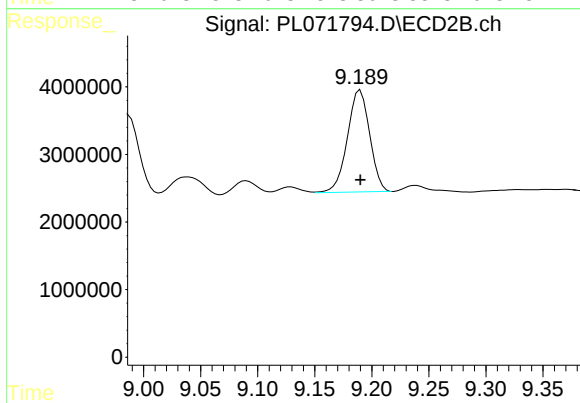

#27 Chlordane-5


R.T.: 9.190 min
Delta R.T.: 0.000 min
Response: 20524326
Conc: 500.00 ng/ml

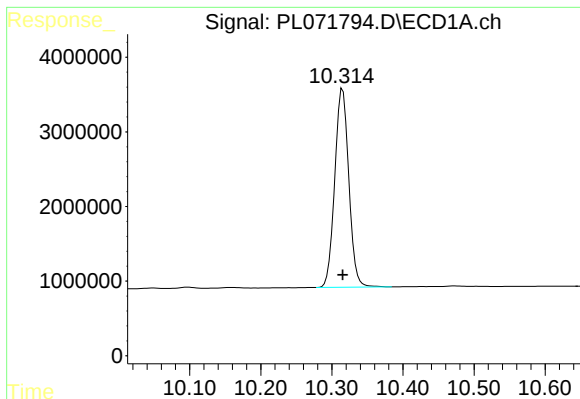

#28 Decachlorobiphenyl

R.T.: 10.315 min
Delta R.T.: 0.000 min
Response: 36552746
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

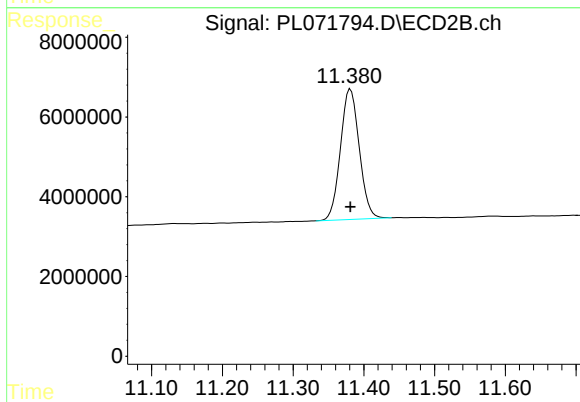

#28 Decachlorobiphenyl

R.T.: 11.381 min
Delta R.T.: 0.000 min
Response: 60372132
Conc: 50.00 ng/ml