

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010422\
 Data File : PL071792.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2022 18:37
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 01:05:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 05 00:57:02 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.492	48940282	125.7E6	99.930	99.299
28)	SA Decachlor...	10.315	11.382	67254100	116.2E6	95.831	98.071
Target Compounds							
23)	Chlordane-1	5.881	6.873	18094442	51378922	1000.611	1000.919
24)	Chlordane-2	6.569	7.466	23236246	52288186	976.405	982.032
25)	Chlordane-3	7.269	8.223	67102305	210.1E6	1000.703	1004.296
26)	Chlordane-4	7.337	8.304	72288436	247.4E6	1004.278	997.340
27)	Chlordane-5	8.286	9.190	23965671	40633863	992.221	994.922



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010422\
Data File : PL071792.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2022 18:37
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 01:05:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Wed Jan 05 00:57:02 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

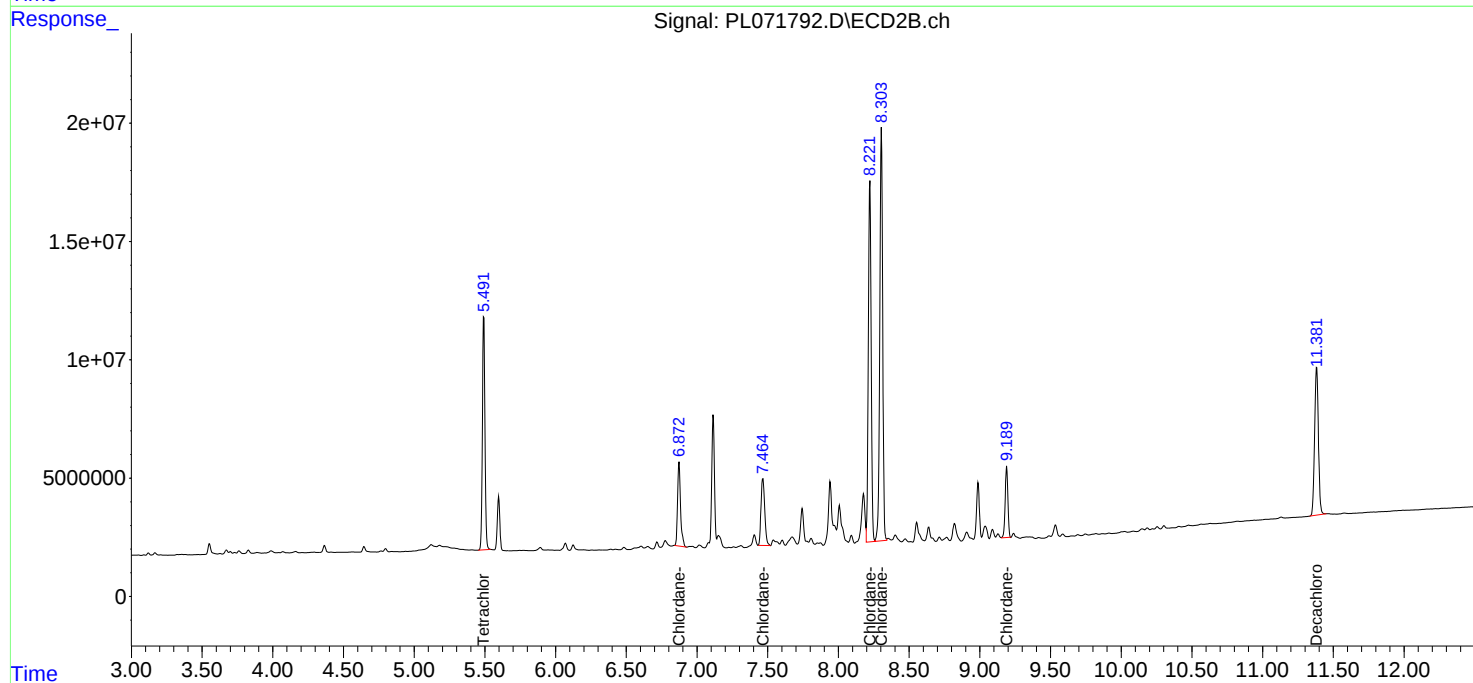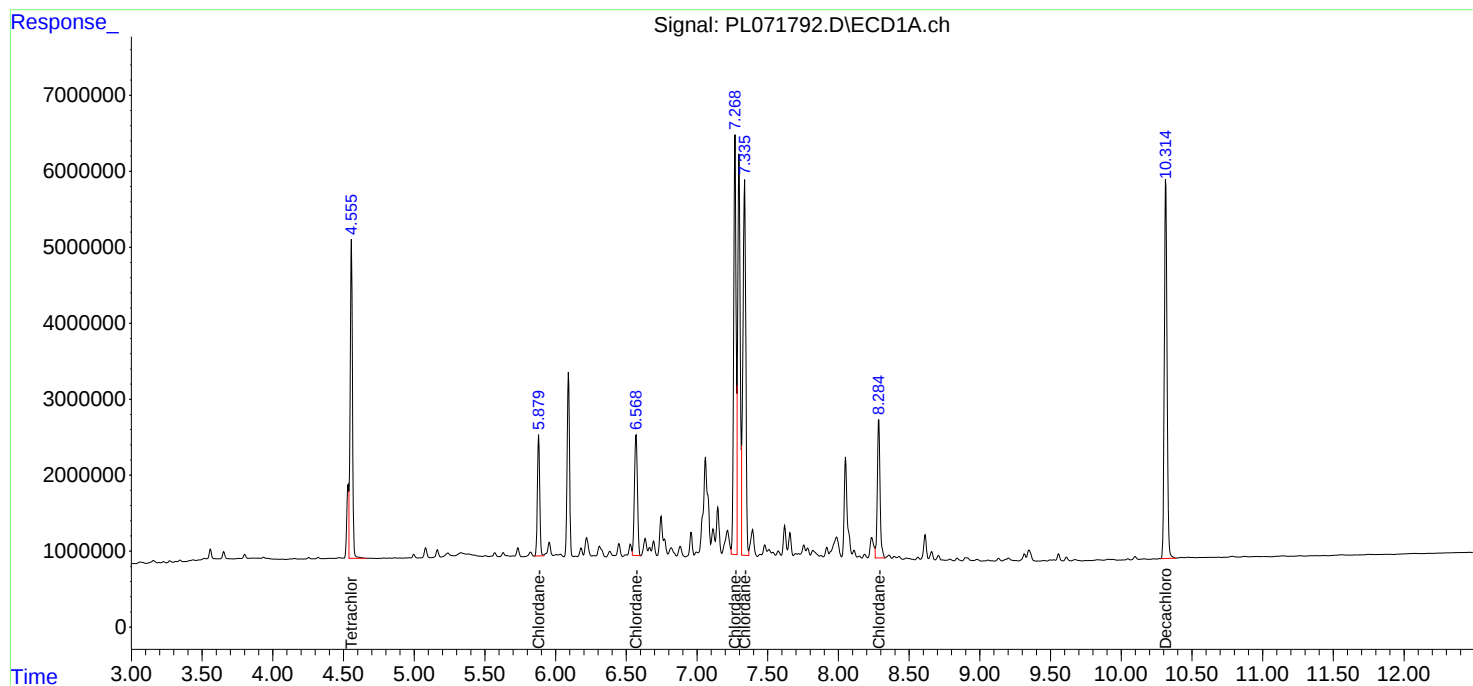


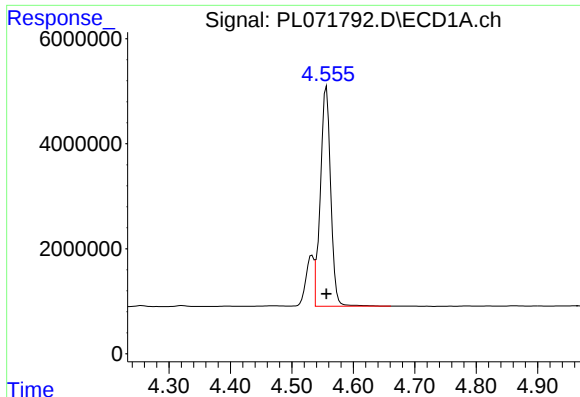

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: 0.000 min
Response: 48940282
Conc: 99.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

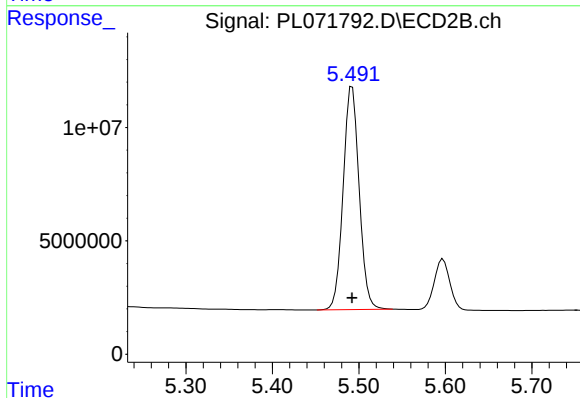


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: 0.000 min
Response: 125673760
Conc: 99.30 ng/ml

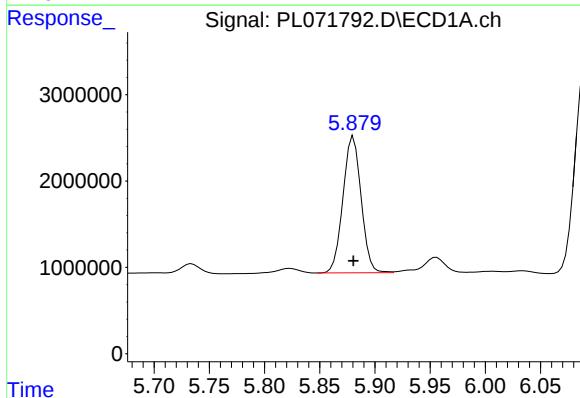


#23 Chlordane-1

R.T.: 5.881 min
Delta R.T.: 0.000 min
Response: 18094442
Conc: 1000.61 ng/ml

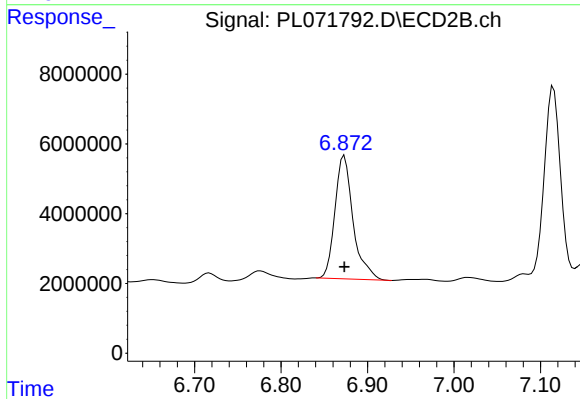

#23 Chlordane-1


R.T.: 6.873 min
Delta R.T.: 0.000 min
Response: 51378922
Conc: 1000.92 ng/ml

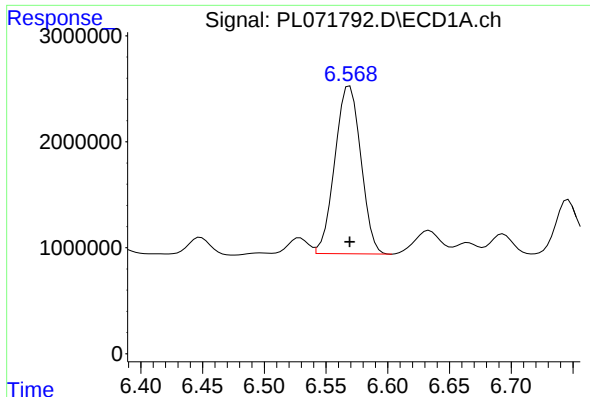

#24 Chlordane-2


R.T.: 6.569 min
Delta R.T.: 0.000 min
Response: 23236246
Conc: 976.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

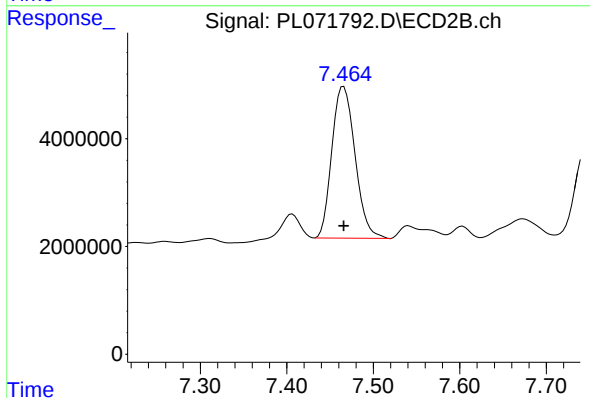


#24 Chlordane-2

R.T.: 7.466 min
Delta R.T.: 0.000 min
Response: 52288186
Conc: 982.03 ng/ml

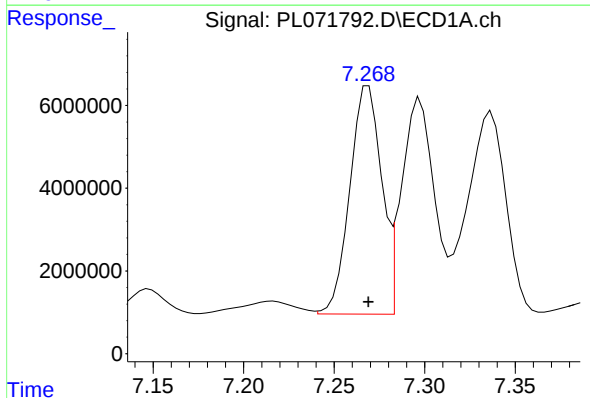


#25 Chlordane-3

R.T.: 7.269 min
Delta R.T.: 0.000 min
Response: 67102305
Conc: 1000.70 ng/ml

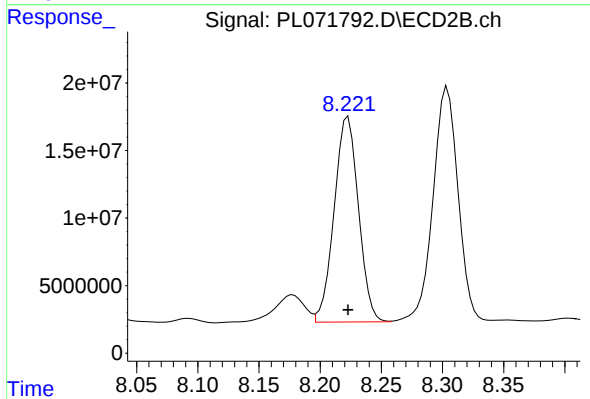

#25 Chlordane-3


R.T.: 8.223 min
Delta R.T.: 0.000 min
Response: 210142032
Conc: 1004.30 ng/ml

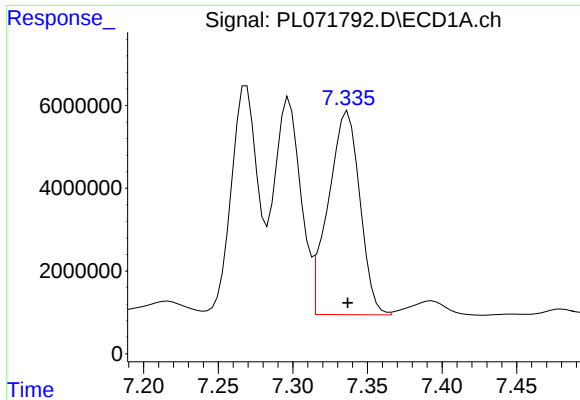

#26 Chlordane-4


R.T.: 7.337 min
Delta R.T.: 0.000 min
Response: 72288436
Conc: 1004.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

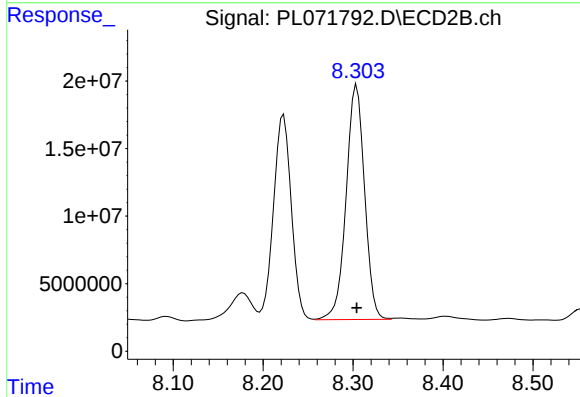


#26 Chlordane-4

R.T.: 8.304 min
Delta R.T.: 0.000 min
Response: 247442036
Conc: 997.34 ng/ml

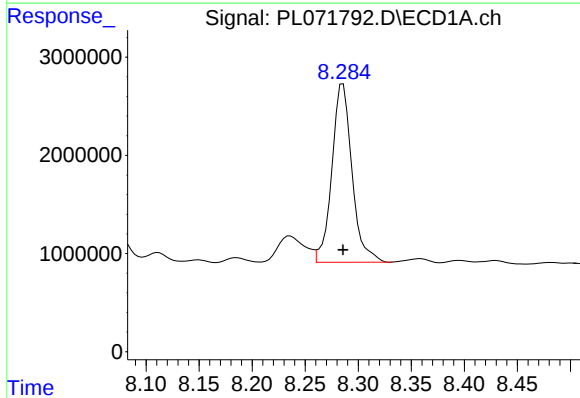


#27 Chlordane-5

R.T.: 8.286 min
Delta R.T.: 0.000 min
Response: 23965671
Conc: 992.22 ng/ml

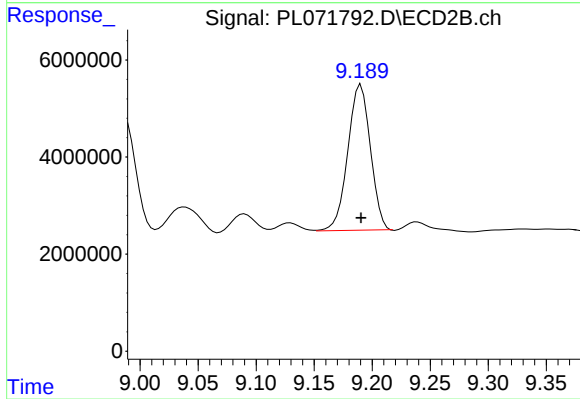

#27 Chlordane-5


R.T.: 9.190 min
Delta R.T.: 0.000 min
Response: 40633863
Conc: 994.92 ng/ml

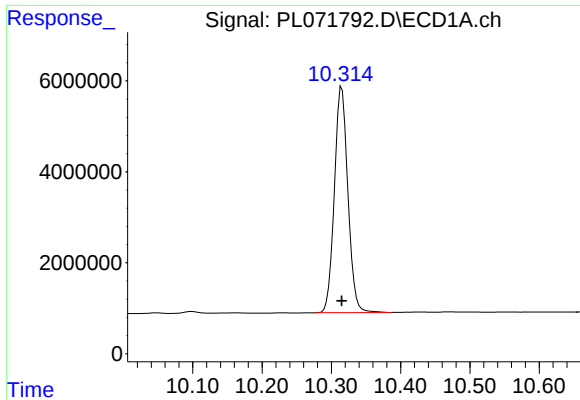

#28 Decachlorobiphenyl

R.T.: 10.315 min
Delta R.T.: 0.000 min
Response: 67254100
Conc: 95.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

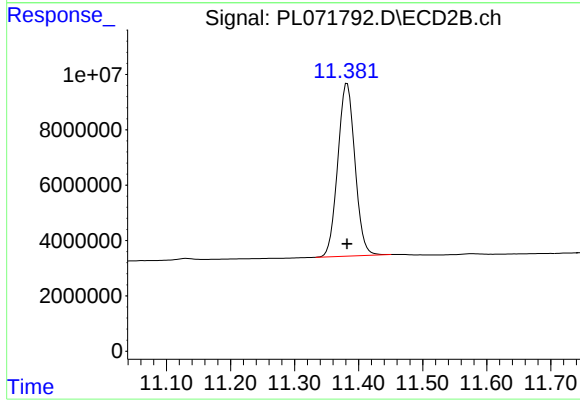

#28 Decachlorobiphenyl

R.T.: 11.382 min
Delta R.T.: 0.000 min
Response: 116175201
Conc: 98.07 ng/ml