

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010422\
 Data File : PL071793.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2022 18:54
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 01:07:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 05 00:57:02 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.492	36599219	95208559	74.820	75.151
28)	SA Decachlor...	10.315	11.382	52215448	88792027	74.601	74.970
Target Compounds							
23)	Chlordane-1	5.880	6.873	13658032	38240929	753.512	746.643
24)	Chlordane-2	6.569	7.466	17941598	40266390	752.609	754.154
25)	Chlordane-3	7.269	8.223	50513013	158.7E6	752.200	755.517
26)	Chlordane-4	7.337	8.305	54082267	187.4E6	750.897	753.473
27)	Chlordane-5	8.286	9.190	18230113	30498905	753.166	747.842



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010422\
Data File : PL071793.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2022 18:54
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 01:07:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Wed Jan 05 00:57:02 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

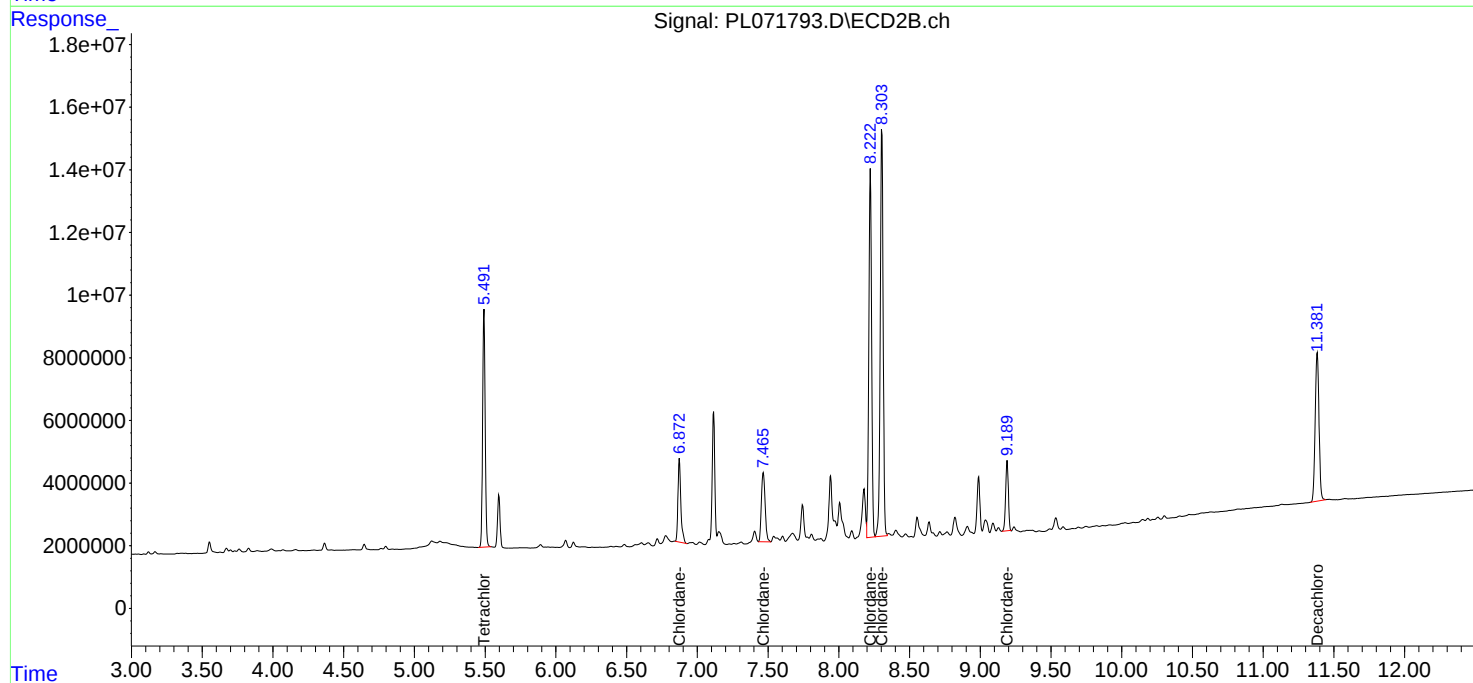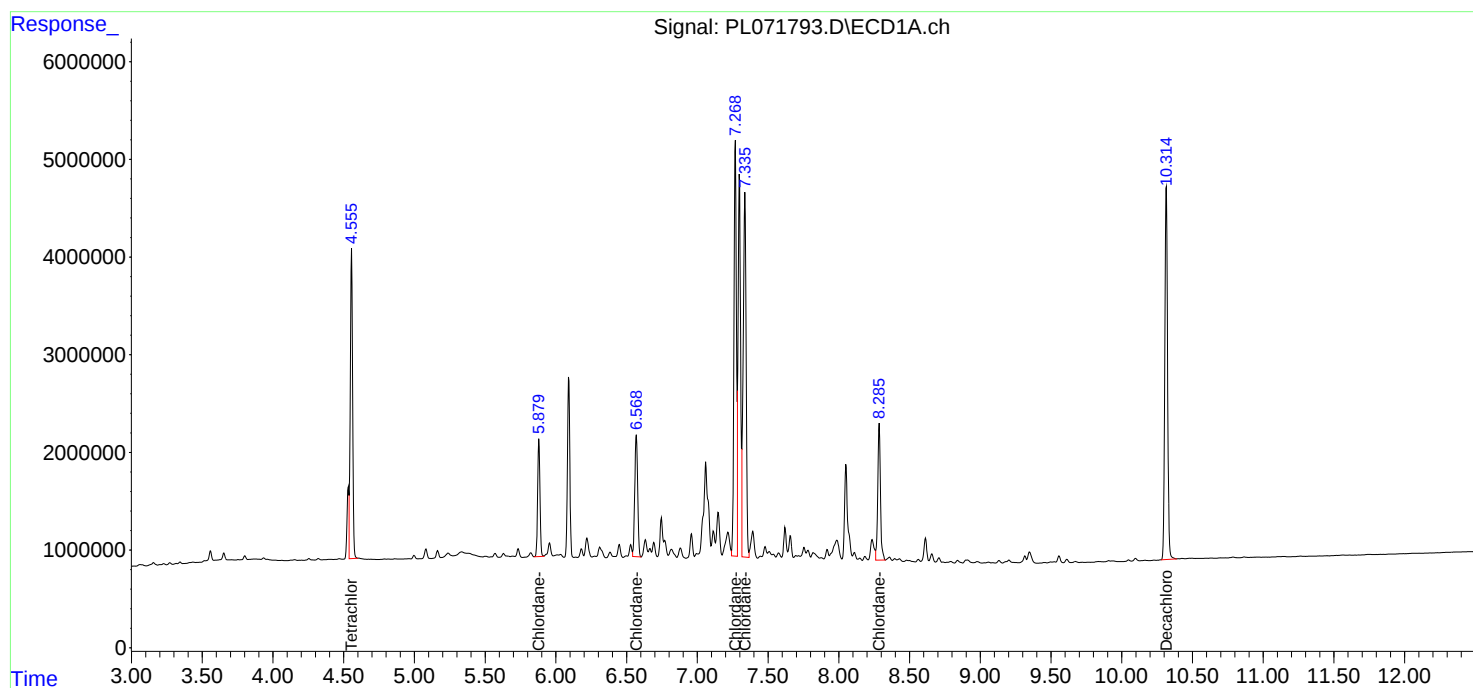


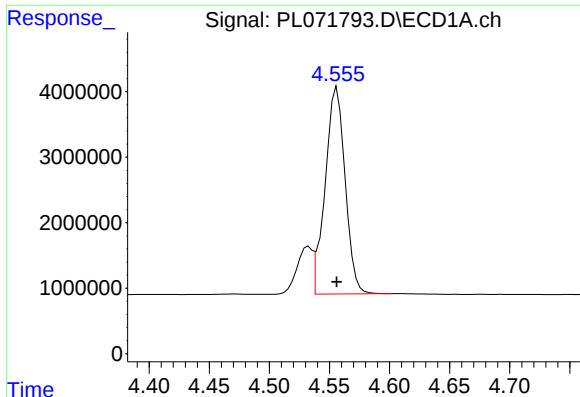

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: 0.000 min
Response: 36599219
Conc: 74.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

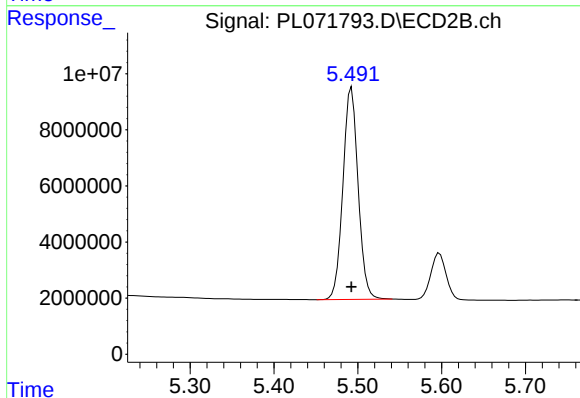


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: 0.000 min
Response: 95208559
Conc: 75.15 ng/ml

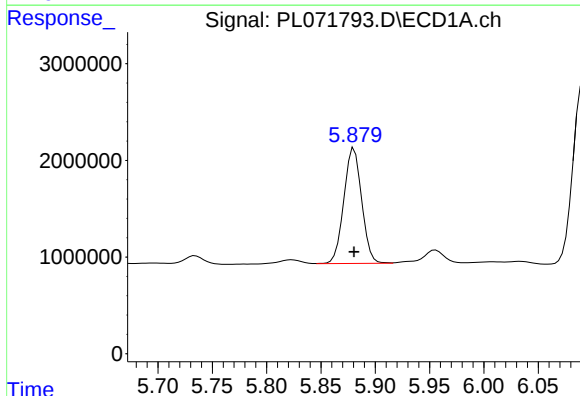


#23 Chlordane-1

R.T.: 5.880 min
Delta R.T.: 0.000 min
Response: 13658032
Conc: 753.51 ng/ml

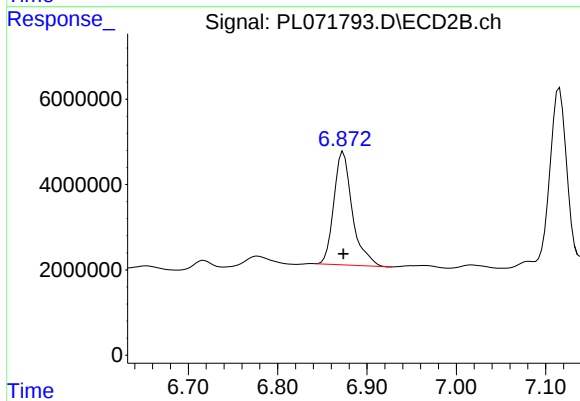

#23 Chlordane-1


R.T.: 6.873 min
Delta R.T.: 0.000 min
Response: 38240929
Conc: 746.64 ng/ml

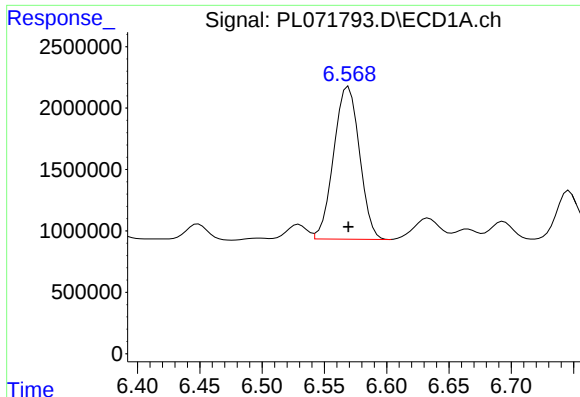

#24 Chlordane-2


R.T.: 6.569 min
Delta R.T.: 0.000 min
Response: 17941598
Conc: 752.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

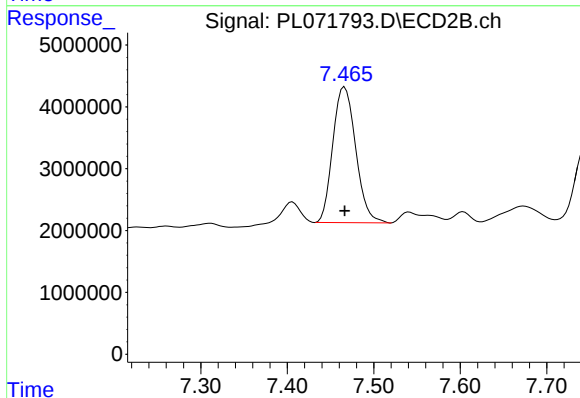


#24 Chlordane-2

R.T.: 7.466 min
Delta R.T.: 0.000 min
Response: 40266390
Conc: 754.15 ng/ml

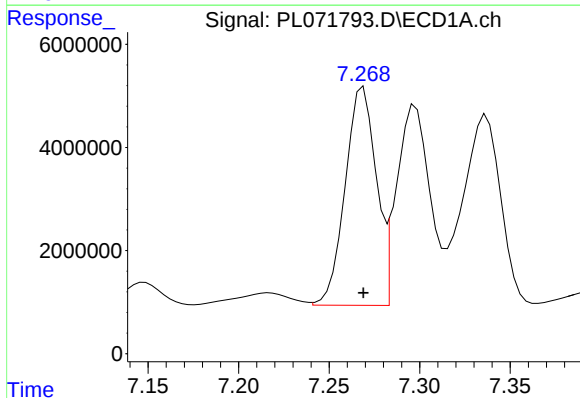


#25 Chlordane-3

R.T.: 7.269 min
Delta R.T.: 0.000 min
Response: 50513013
Conc: 752.20 ng/ml

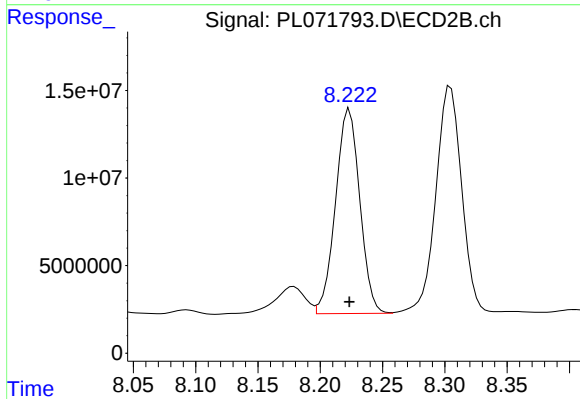

#25 Chlordane-3


R.T.: 8.223 min
Delta R.T.: 0.000 min
Response: 158670184
Conc: 755.52 ng/ml

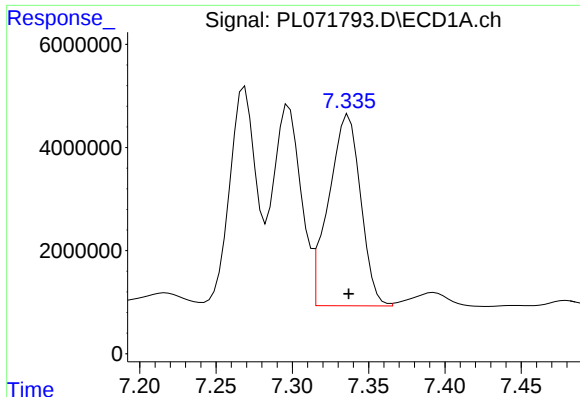

#26 Chlordane-4


R.T.: 7.337 min
Delta R.T.: 0.000 min
Response: 54082267
Conc: 750.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

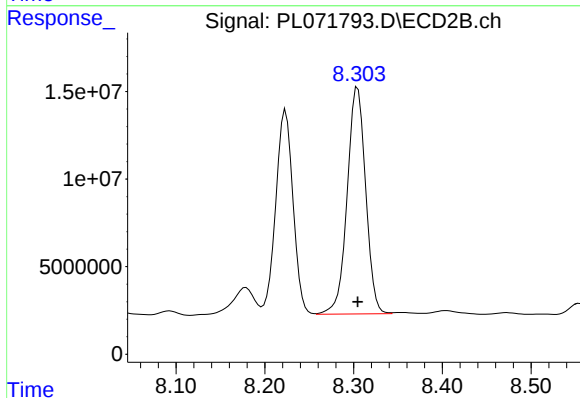


#26 Chlordane-4

R.T.: 8.305 min
Delta R.T.: 0.000 min
Response: 187371957
Conc: 753.47 ng/ml

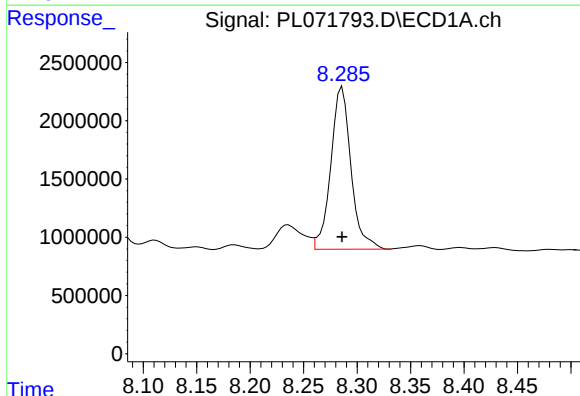


#27 Chlordane-5

R.T.: 8.286 min
Delta R.T.: 0.000 min
Response: 18230113
Conc: 753.17 ng/ml

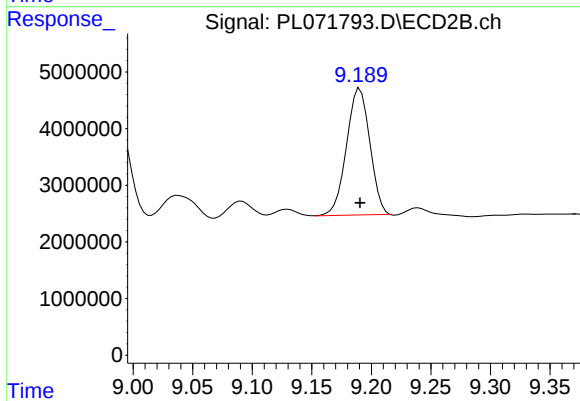

#27 Chlordane-5


R.T.: 9.190 min
Delta R.T.: 0.000 min
Response: 30498905
Conc: 747.84 ng/ml

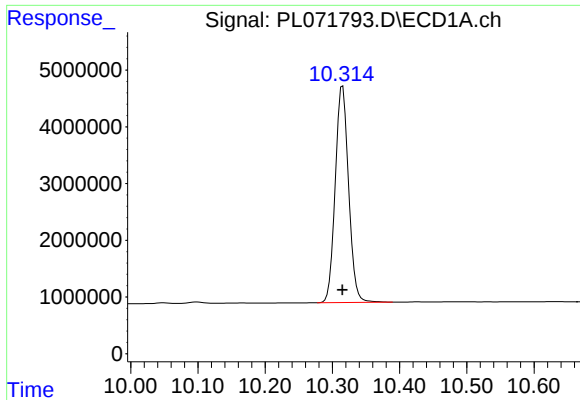

#28 Decachlorobiphenyl

R.T.: 10.315 min
Delta R.T.: 0.000 min
Response: 52215448
Conc: 74.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

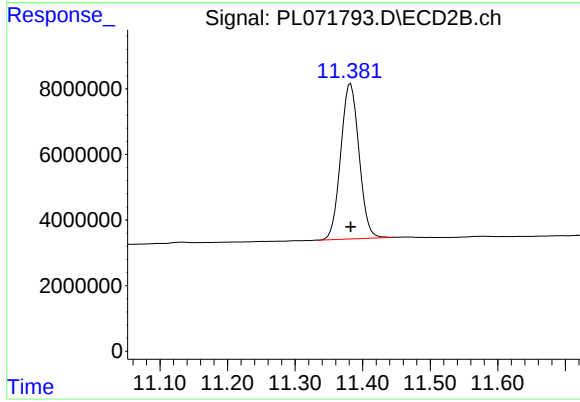

#28 Decachlorobiphenyl

R.T.: 11.382 min
Delta R.T.: 0.000 min
Response: 88792027
Conc: 74.97 ng/ml