

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010422\
 Data File : PL071795.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2022 19:27
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 01:09:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 05 00:57:02 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.493	12124463	31322249	24.839	24.792
28)	SA Decachlor...	10.315	11.382	19143746	30587562	26.723	25.615
Target Compounds							
23)	Chlordane-1	5.880	6.874	4347051	12338289	242.291	243.114
24)	Chlordane-2	6.570	7.466	6111499	13756955	254.742	255.698
25)	Chlordane-3	7.269	8.223	15980953	50166947	240.872	241.561
26)	Chlordane-4	7.337	8.305	17317629	60454529	242.764	244.792
27)	Chlordane-5	8.286	9.191	5912531	9882825	245.680	244.203



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010422\
Data File : PL071795.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2022 19:27
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 01:09:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Wed Jan 05 00:57:02 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

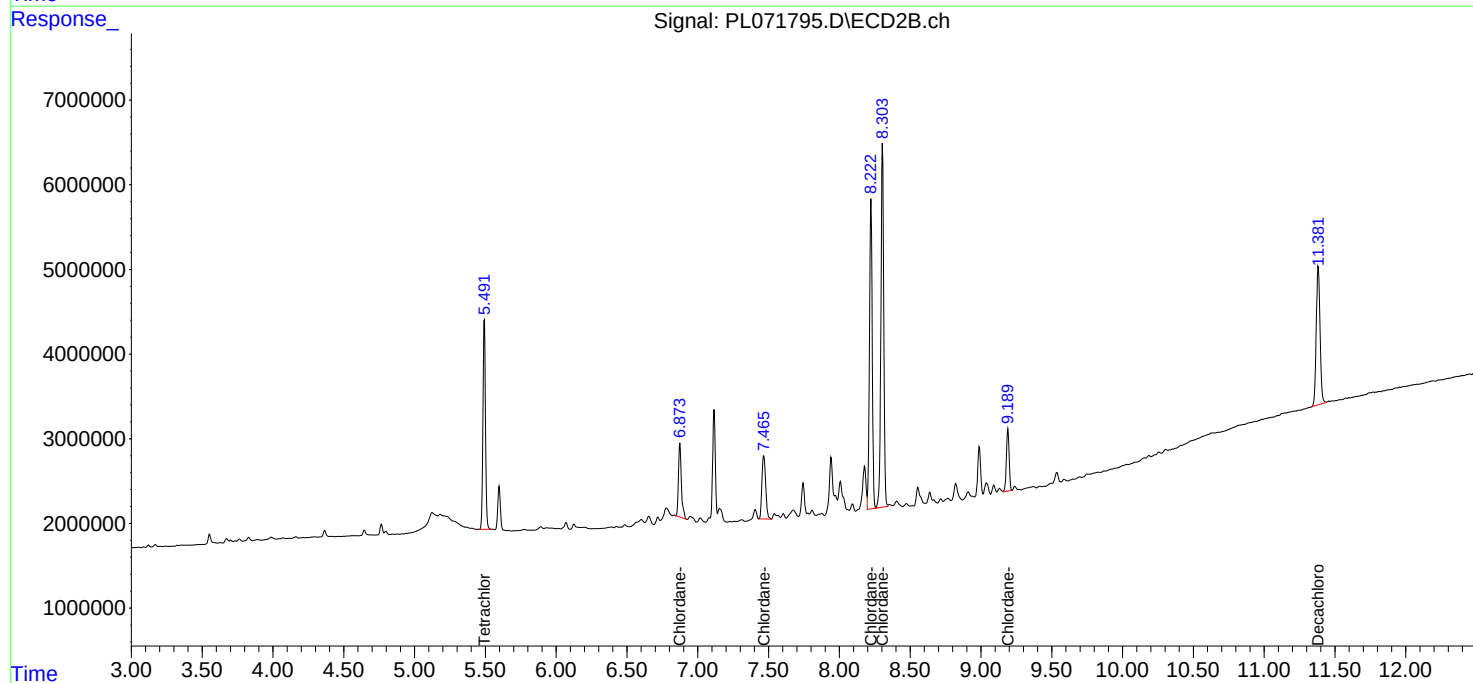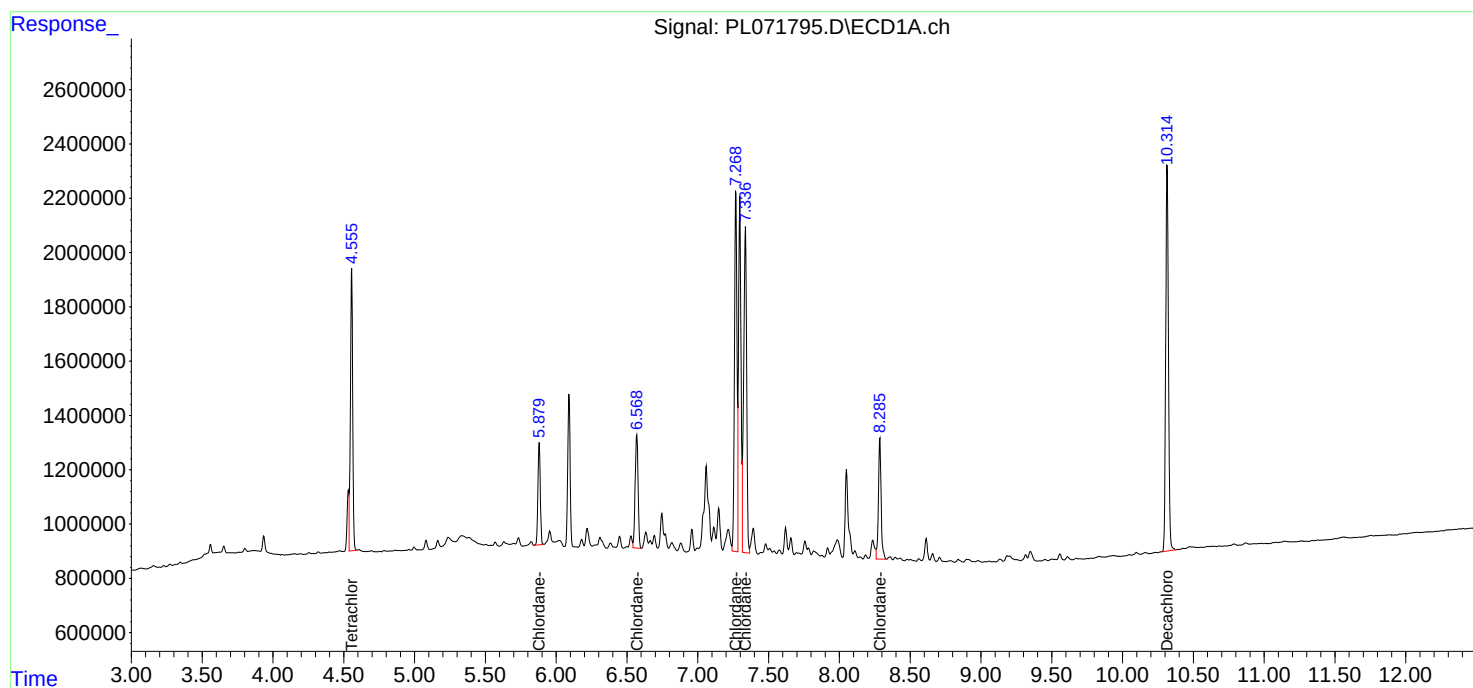


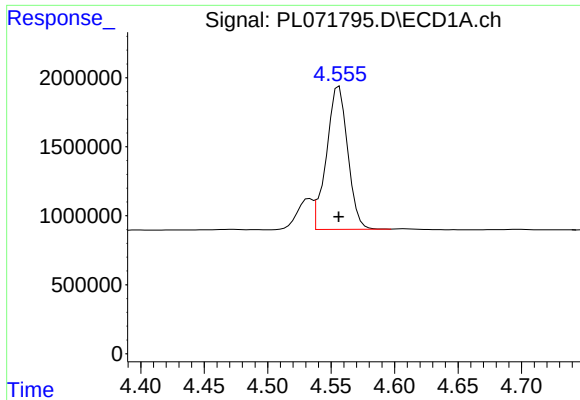

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: 0.000 min
Response: 12124463
Conc: 24.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

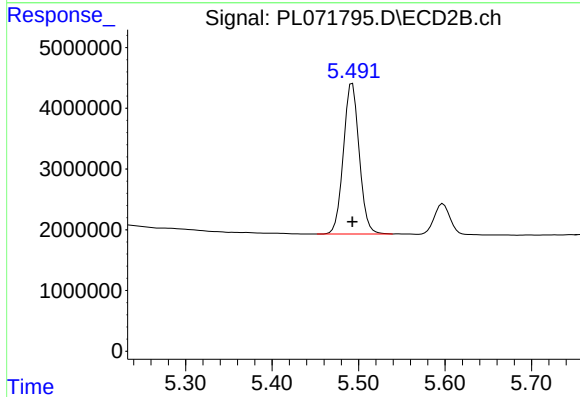


#1 Tetrachloro-m-xylene

R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 31322249
Conc: 24.79 ng/ml

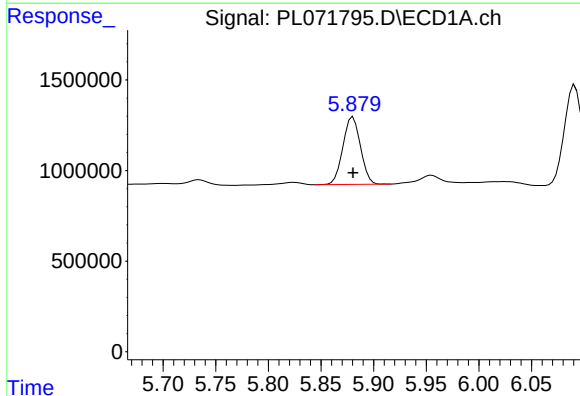


#23 Chlordane-1

R.T.: 5.880 min
Delta R.T.: 0.000 min
Response: 4347051
Conc: 242.29 ng/ml

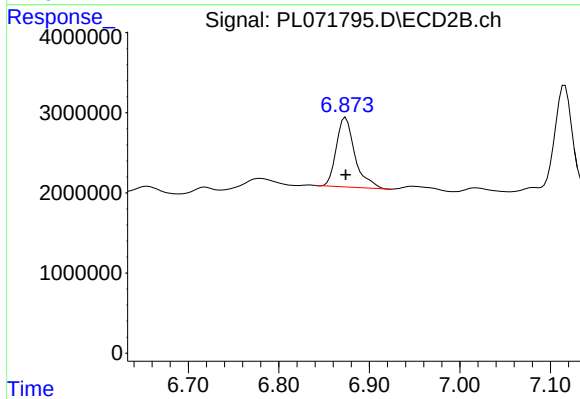

#23 Chlordane-1


R.T.: 6.874 min
Delta R.T.: 0.000 min
Response: 12338289
Conc: 243.11 ng/ml

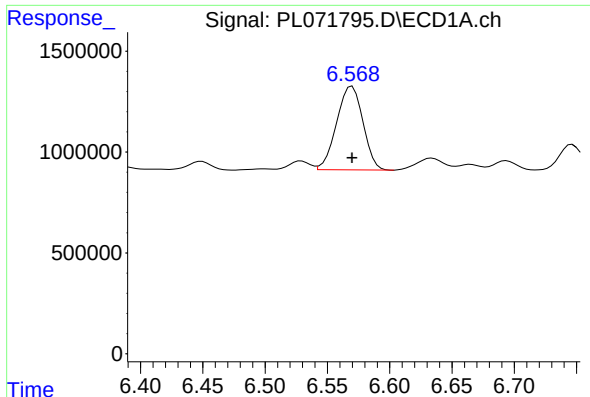

#24 Chlordane-2


R.T.: 6.570 min
Delta R.T.: 0.000 min
Response: 6111499
Conc: 254.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

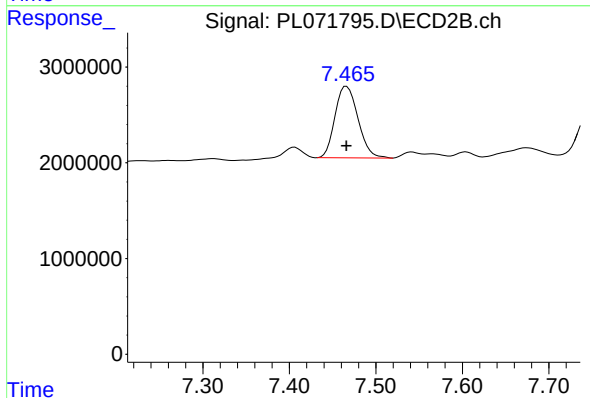


#24 Chlordane-2

R.T.: 7.466 min
Delta R.T.: 0.000 min
Response: 13756955
Conc: 255.70 ng/ml

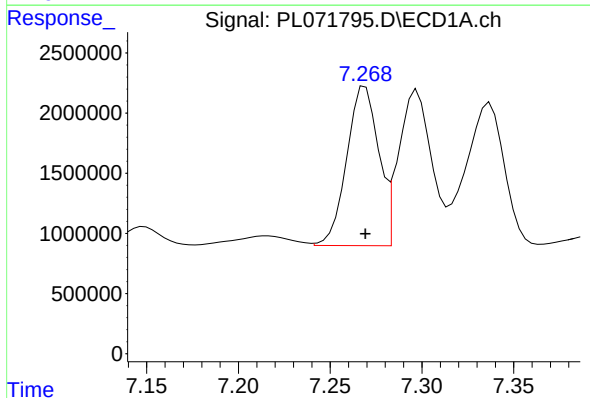


#25 Chlordane-3

R.T.: 7.269 min
Delta R.T.: 0.000 min
Response: 15980953
Conc: 240.87 ng/ml

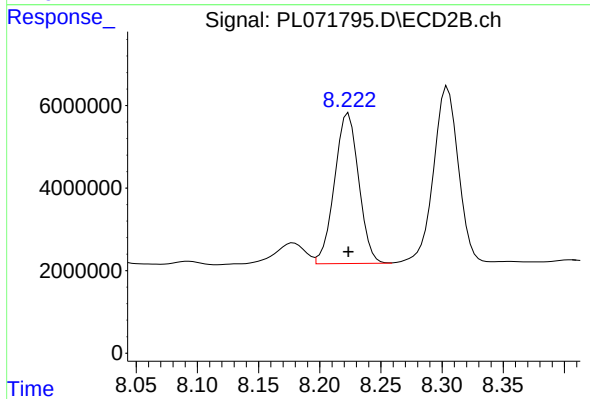

#25 Chlordane-3


R.T.: 8.223 min
Delta R.T.: 0.000 min
Response: 50166947
Conc: 241.56 ng/ml

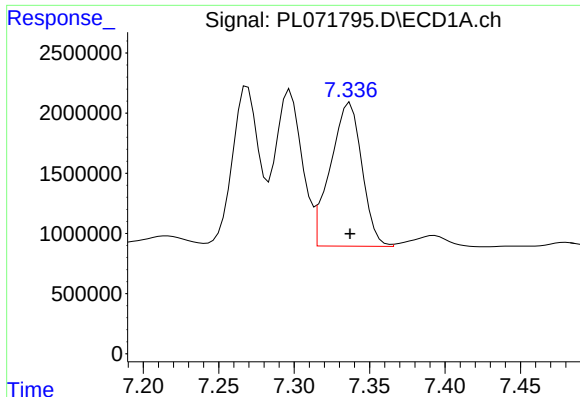

#26 Chlordane-4


R.T.: 7.337 min
Delta R.T.: 0.000 min
Response: 17317629
Conc: 242.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

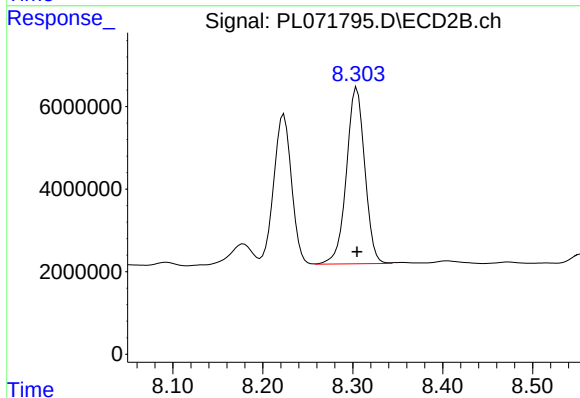


#26 Chlordane-4

R.T.: 8.305 min
Delta R.T.: 0.000 min
Response: 60454529
Conc: 244.79 ng/ml

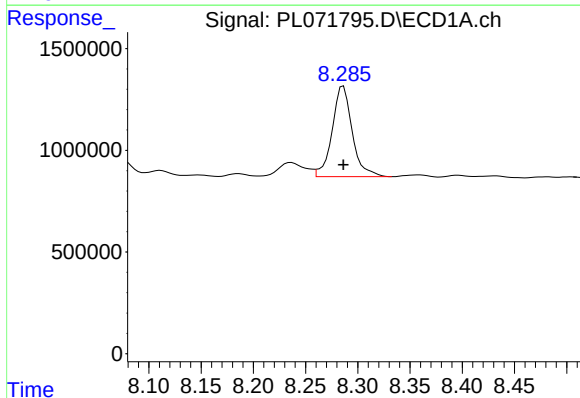


#27 Chlordane-5

R.T.: 8.286 min
Delta R.T.: 0.000 min
Response: 5912531
Conc: 245.68 ng/ml

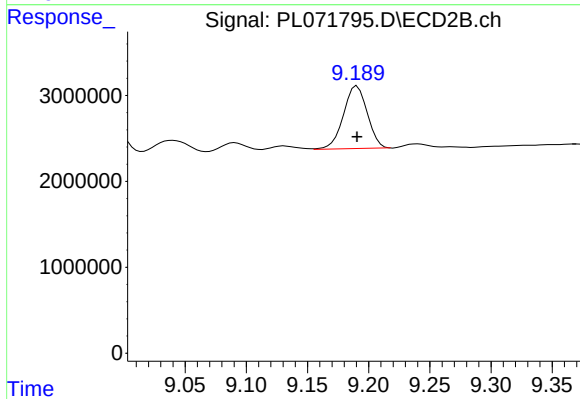

#27 Chlordane-5


R.T.: 9.191 min
Delta R.T.: 0.000 min
Response: 9882825
Conc: 244.20 ng/ml

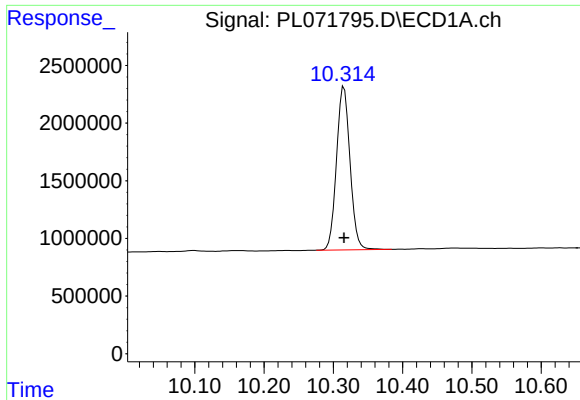

#28 Decachlorobiphenyl

R.T.: 10.315 min
Delta R.T.: 0.000 min
Response: 19143746
Conc: 26.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

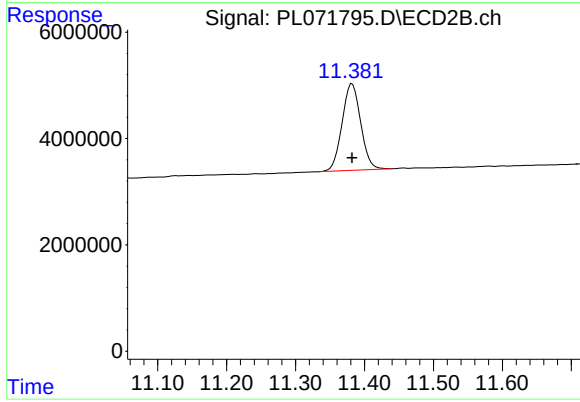

#28 Decachlorobiphenyl

R.T.: 11.382 min
Delta R.T.: 0.000 min
Response: 30587562
Conc: 25.61 ng/ml