

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010423\
 Data File : PL080073.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2023 21:19
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 04:56:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010423.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 05 04:54:57 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.370	2.693	147.7E6	204.8E6	74.107	73.986
28)	SA Decachlor...	8.879	7.848	119.9E6	162.4E6	72.230	71.635
Target Compounds							
23)	Chlordane-1	4.526	3.692	45656386	59301403	739.810	735.047
24)	Chlordane-2	5.057	4.269	52585534	64401306	715.293	719.233
25)	Chlordane-3	5.769	4.901	189.9E6	204.2E6	744.435	747.541
26)	Chlordane-4	5.852	4.963	231.9E6	202.3E6	737.497	739.835
27)	Chlordane-5	6.702	5.631	45133239	54320328	738.364	728.297


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010423\
Data File : PL080073.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2023 21:19
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 04:56:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010423.M
Quant Title : GC Extractables
QLast Update : Thu Jan 05 04:54:57 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

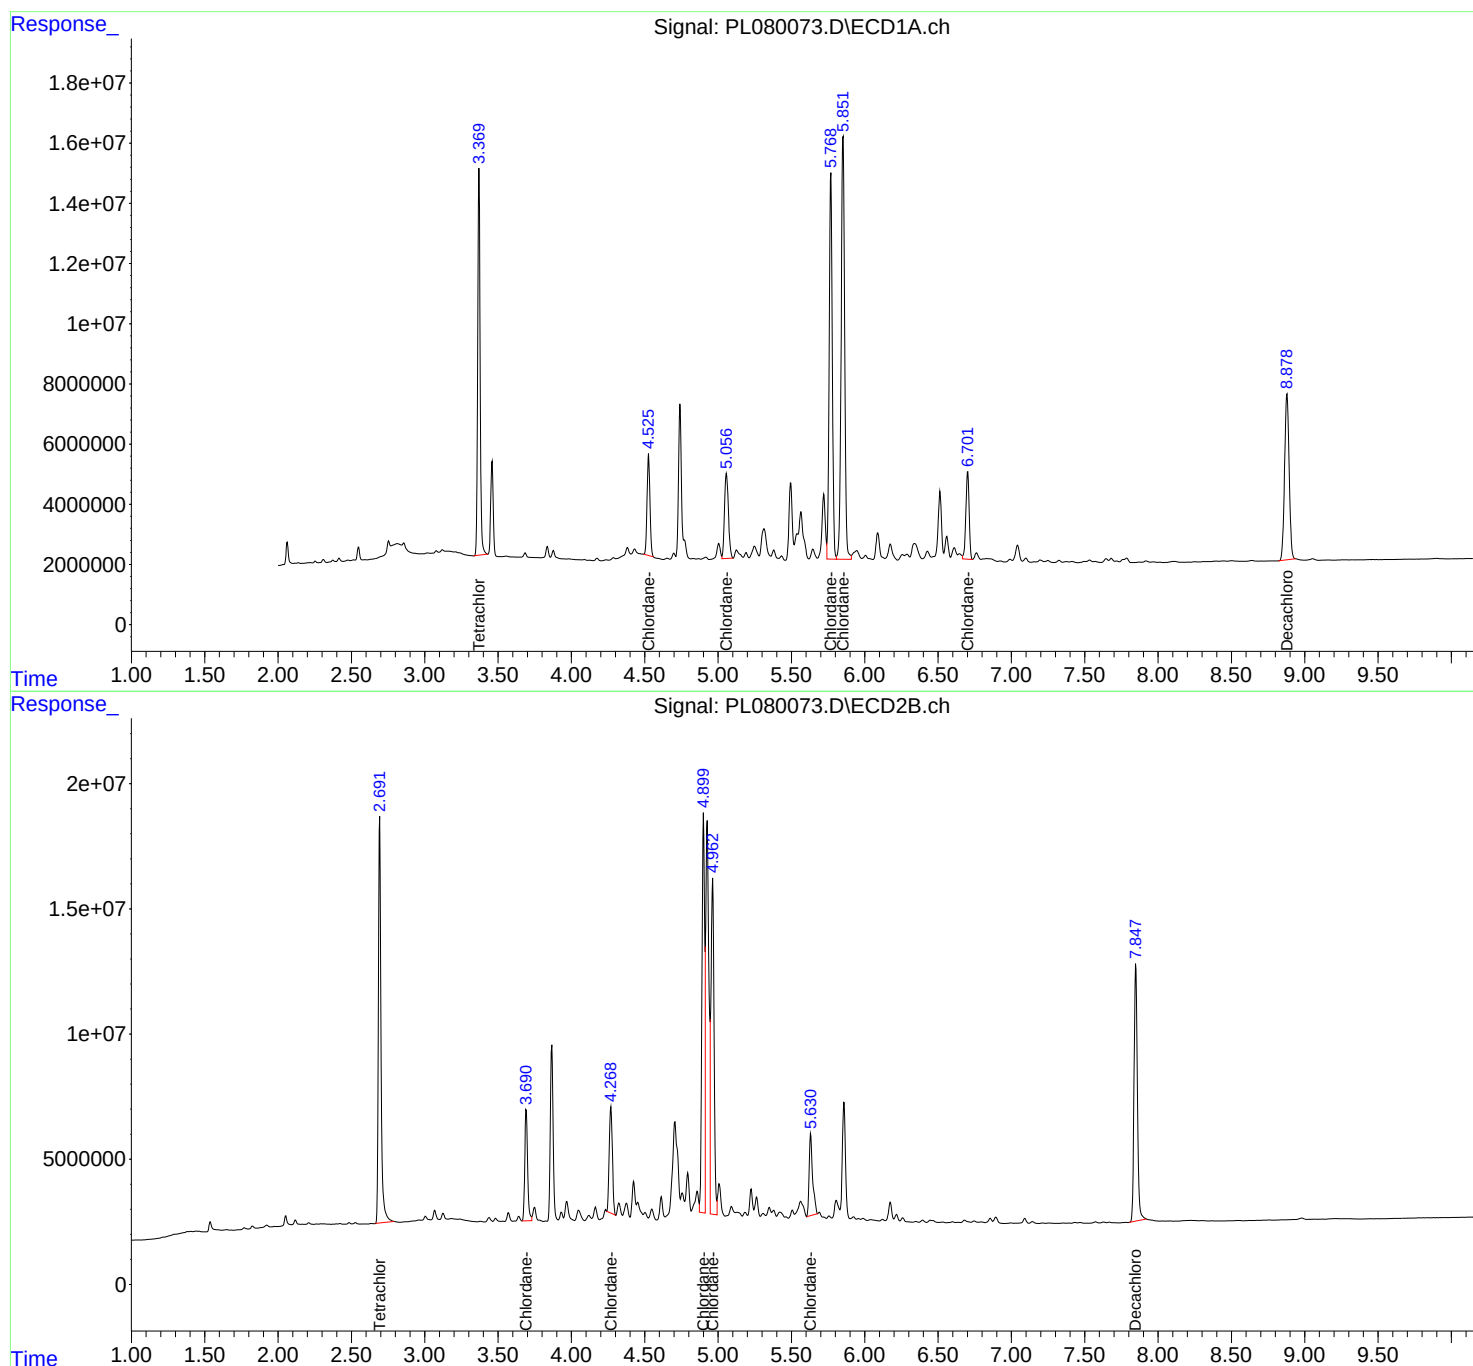


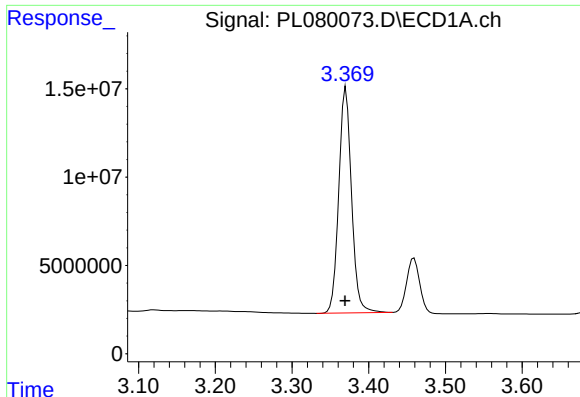

#1 Tetrachloro-m-xylene


R.T.: 3.370 min
Delta R.T.: 0.001 min
Response: 147667515
Conc: 74.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

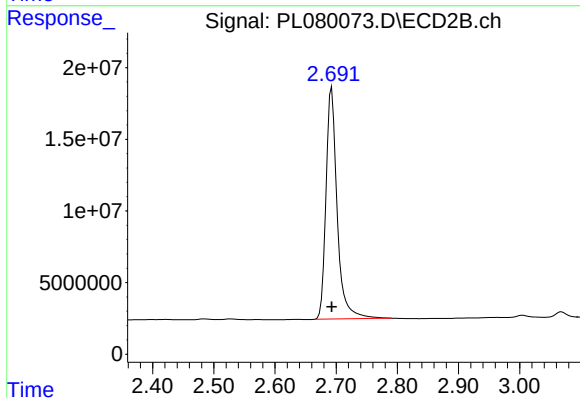


#1 Tetrachloro-m-xylene

R.T.: 2.693 min
Delta R.T.: 0.000 min
Response: 204829073
Conc: 73.99 ng/ml

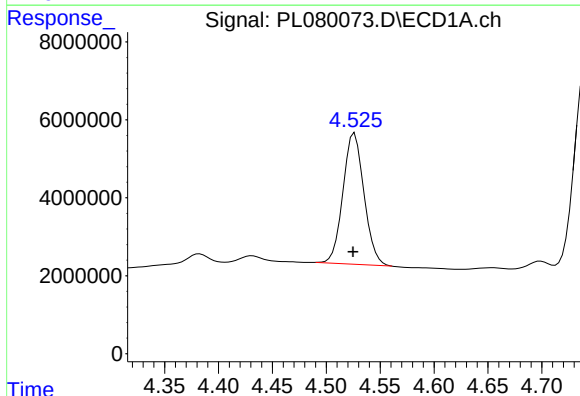


#23 Chlordane-1

R.T.: 4.526 min
Delta R.T.: 0.001 min
Response: 45656386
Conc: 739.81 ng/ml

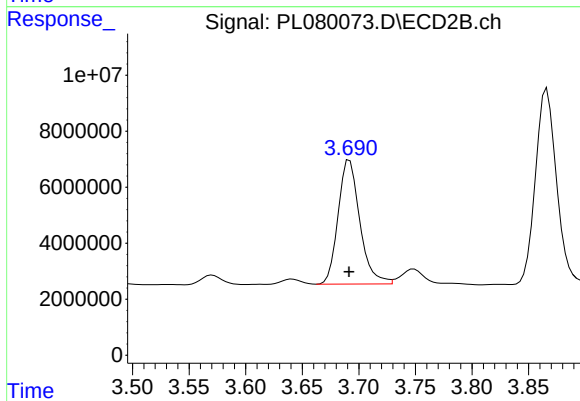

#23 Chlordane-1


R.T.: 3.692 min
Delta R.T.: 0.000 min
Response: 59301403
Conc: 735.05 ng/ml

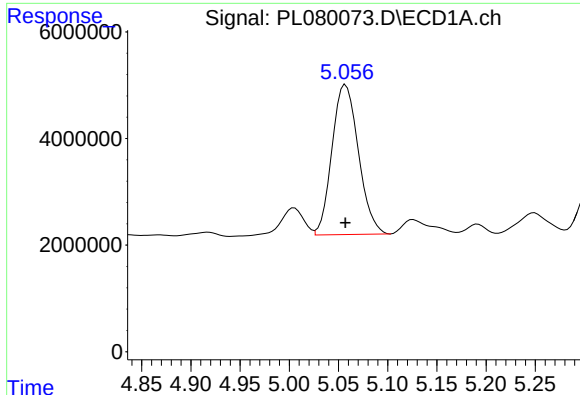

#24 Chlordane-2


R.T.: 5.057 min
Delta R.T.: 0.000 min
Response: 52585534
Conc: 715.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

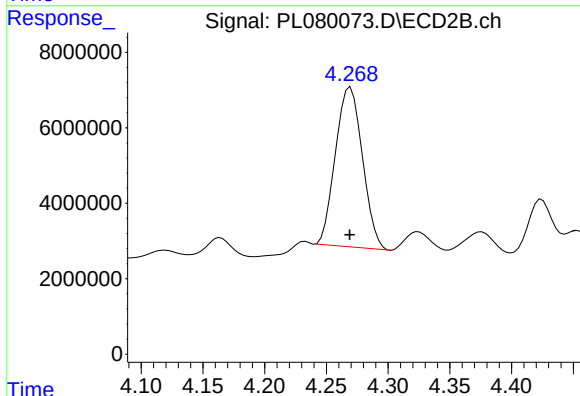


#24 Chlordane-2

R.T.: 4.269 min
Delta R.T.: 0.000 min
Response: 64401306
Conc: 719.23 ng/ml

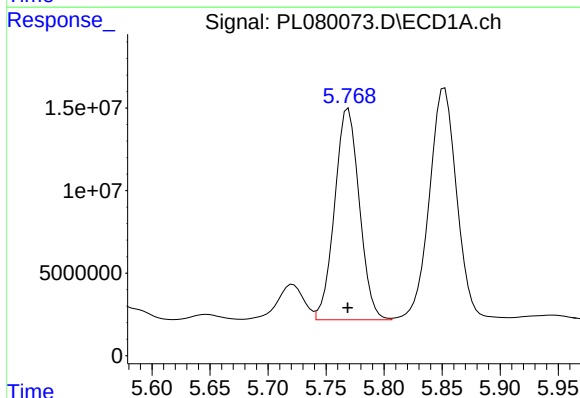


#25 Chlordane-3

R.T.: 5.769 min
Delta R.T.: 0.000 min
Response: 189905228
Conc: 744.43 ng/ml

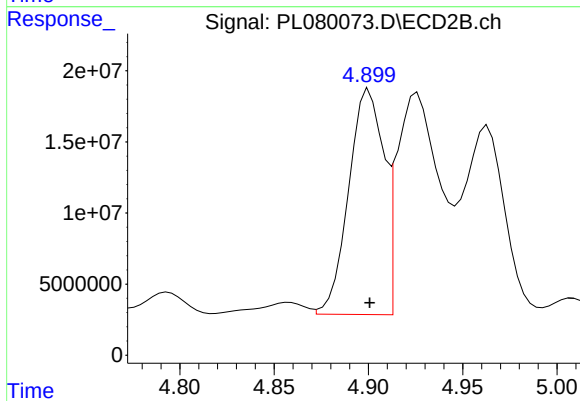

#25 Chlordane-3


R.T.: 4.901 min
Delta R.T.: 0.000 min
Response: 204186295
Conc: 747.54 ng/ml

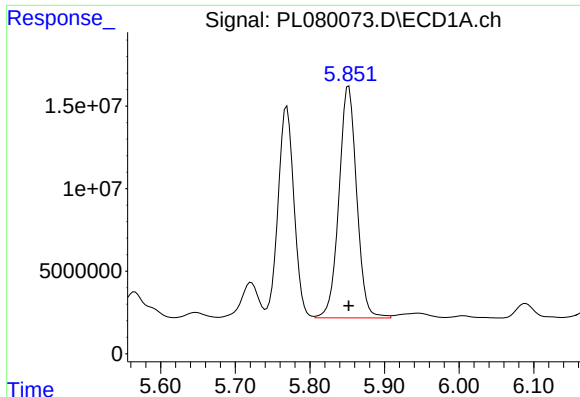

#26 Chlordane-4


R.T.: 5.852 min
Delta R.T.: 0.000 min
Response: 231920618
Conc: 737.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

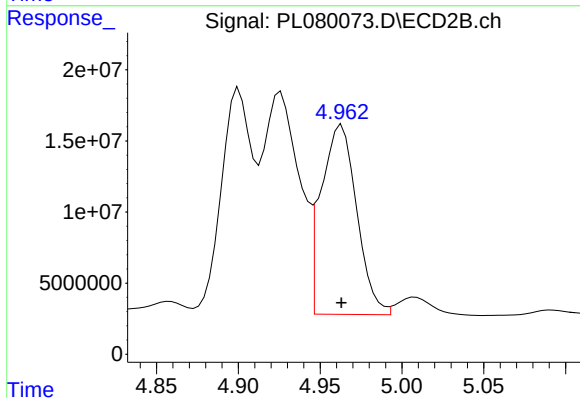


#26 Chlordane-4

R.T.: 4.963 min
Delta R.T.: 0.000 min
Response: 202334451
Conc: 739.83 ng/ml

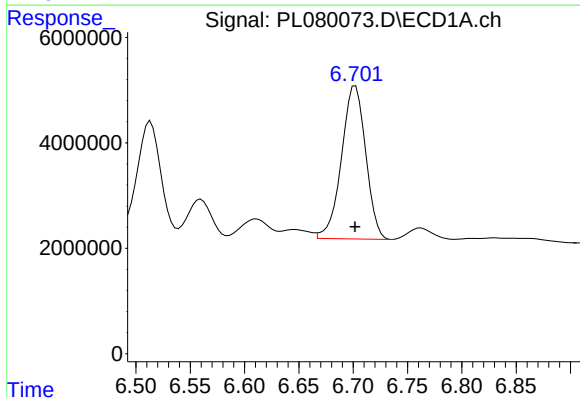


#27 Chlordane-5

R.T.: 6.702 min
Delta R.T.: 0.000 min
Response: 45133239
Conc: 738.36 ng/ml

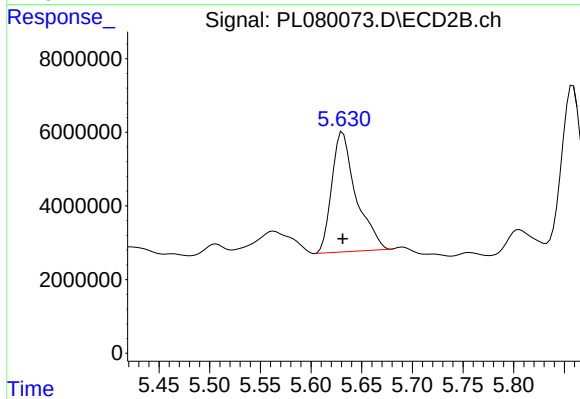

#27 Chlordane-5


R.T.: 5.631 min
Delta R.T.: 0.000 min
Response: 54320328
Conc: 728.30 ng/ml

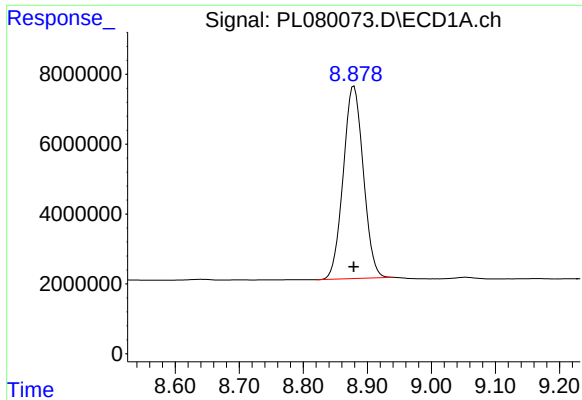

#28 Decachlorobiphenyl

R.T.: 8.879 min
Delta R.T.: 0.000 min
Response: 119874637
Conc: 72.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

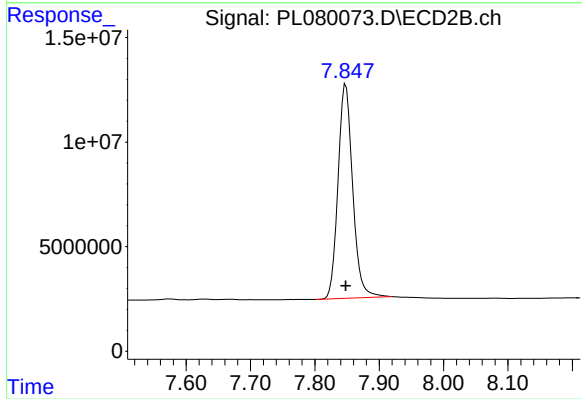

#28 Decachlorobiphenyl

R.T.: 7.848 min
Delta R.T.: 0.000 min
Response: 162405160
Conc: 71.64 ng/ml