

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010423\
 Data File : PL080074.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2023 21:33
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 04:56:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010423.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 05 04:54:57 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.369	2.693	99631452	138.4E6	50.000	50.000
28)	SA Decachlor...	8.879	7.848	82981634	113.4E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.525	3.691	30856831	40338500	500.000	500.000
24)	Chlordane-2	5.057	4.269	36758020	44770804	500.000	500.000
25)	Chlordane-3	5.769	4.901	127.5E6	136.6E6	500.000	500.000
26)	Chlordane-4	5.852	4.963	157.2E6	136.7E6	500.000	500.000
27)	Chlordane-5	6.702	5.631	30562997	37292688	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010423\
Data File : PL080074.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2023 21:33
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 04:56:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010423.M
Quant Title : GC Extractables
QLast Update : Thu Jan 05 04:54:57 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

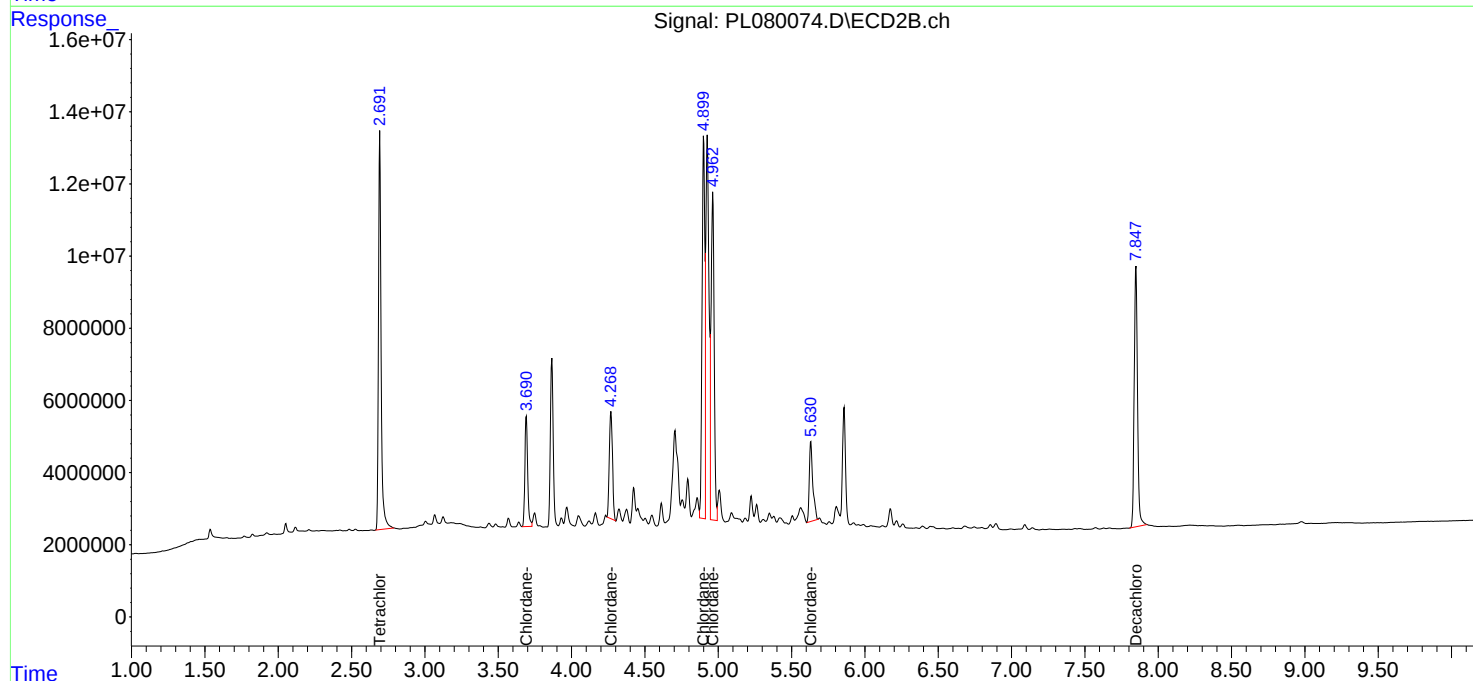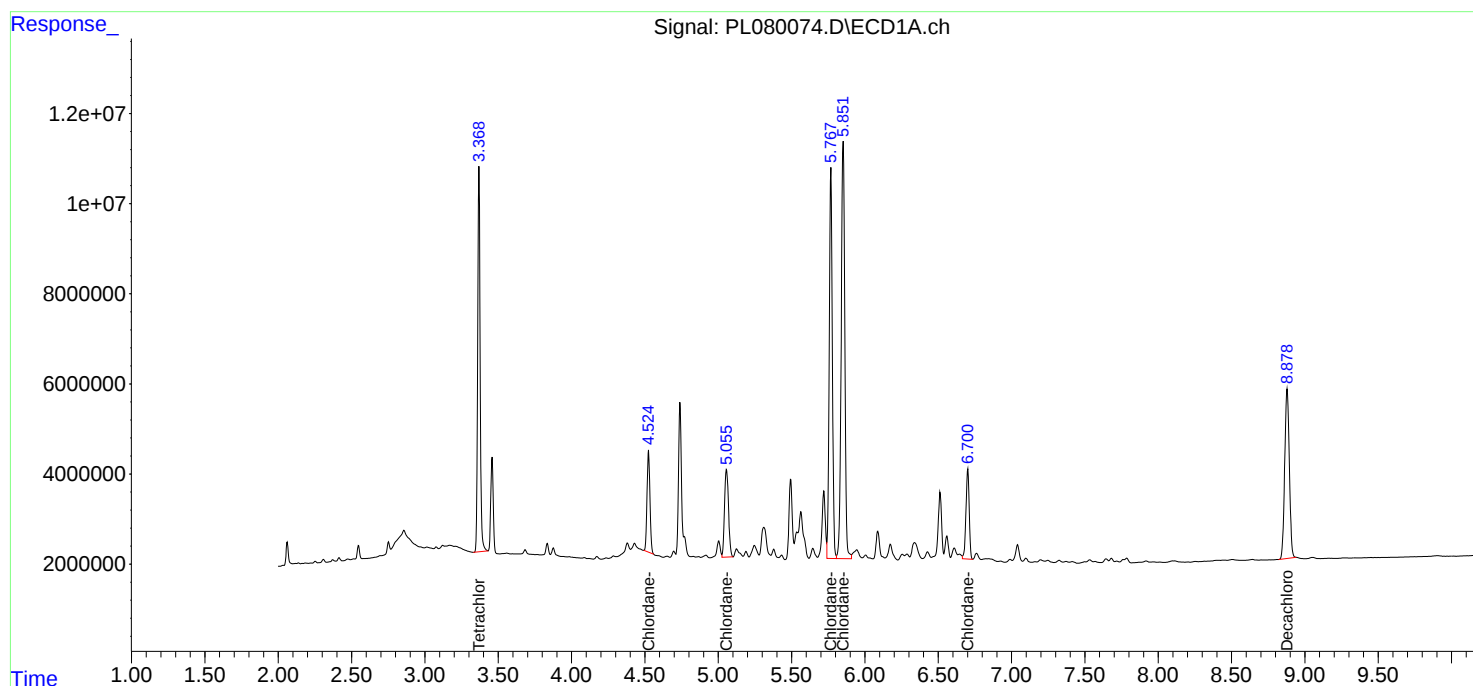


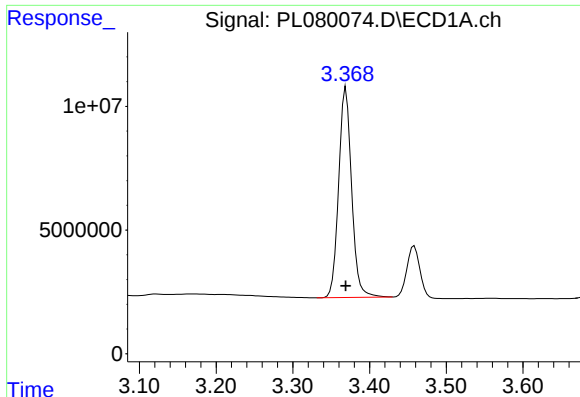

#1 Tetrachloro-m-xylene


R.T.: 3.369 min
Delta R.T.: 0.000 min
Response: 99631452
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

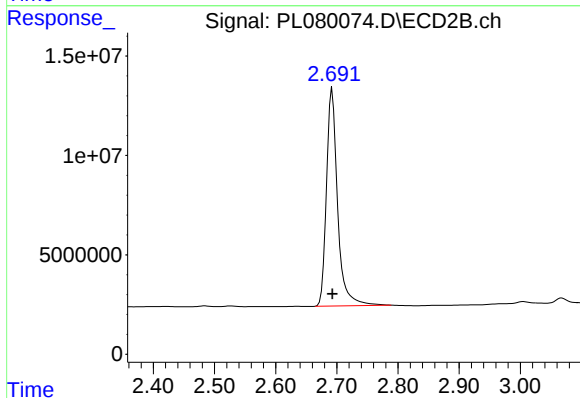


#1 Tetrachloro-m-xylene

R.T.: 2.693 min
Delta R.T.: 0.000 min
Response: 138423738
Conc: 50.00 ng/ml

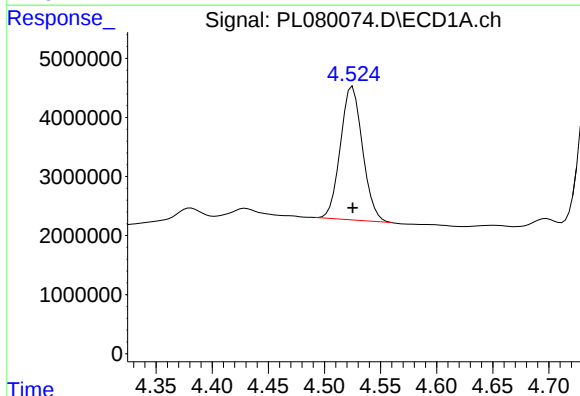


#23 Chlordane-1

R.T.: 4.525 min
Delta R.T.: 0.000 min
Response: 30856831
Conc: 500.00 ng/ml

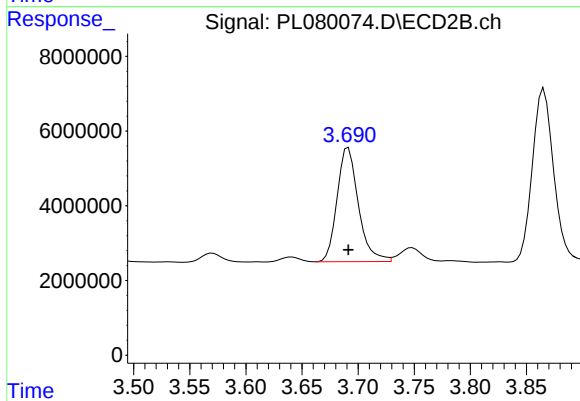

#23 Chlordane-1


R.T.: 3.691 min
Delta R.T.: 0.000 min
Response: 40338500
Conc: 500.00 ng/ml

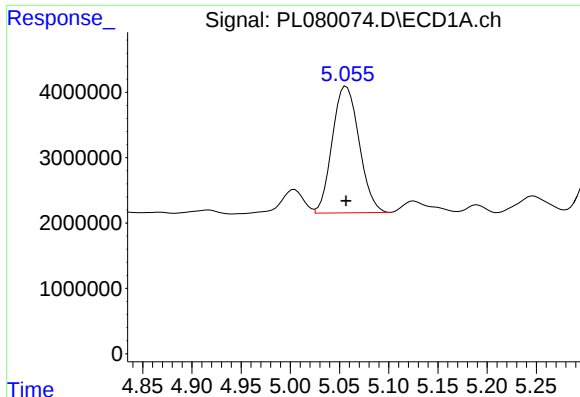

#24 Chlordane-2


R.T.: 5.057 min
Delta R.T.: 0.000 min
Response: 36758020
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

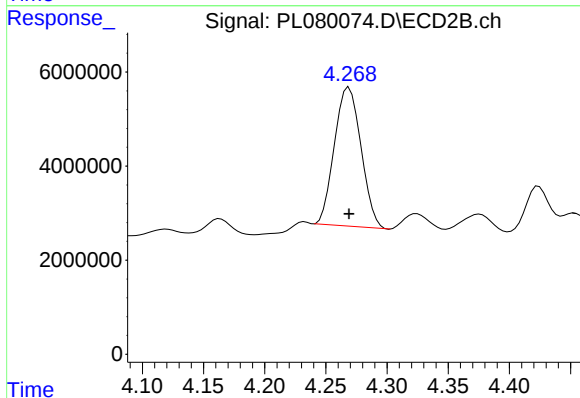


#24 Chlordane-2

R.T.: 4.269 min
Delta R.T.: 0.000 min
Response: 44770804
Conc: 500.00 ng/ml

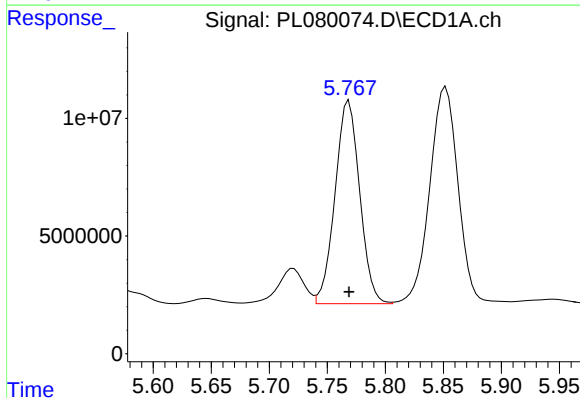


#25 Chlordane-3

R.T.: 5.769 min
Delta R.T.: 0.000 min
Response: 127549975
Conc: 500.00 ng/ml

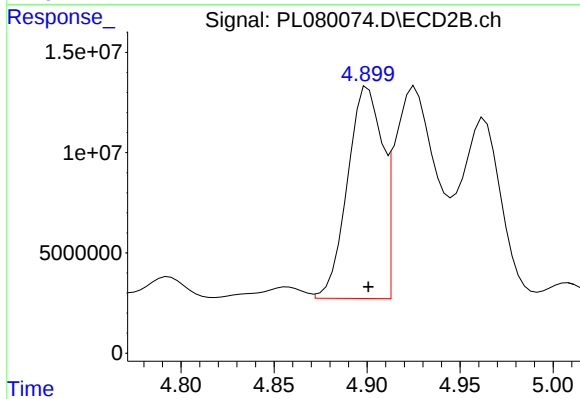

#25 Chlordane-3


R.T.: 4.901 min
Delta R.T.: 0.000 min
Response: 136572024
Conc: 500.00 ng/ml

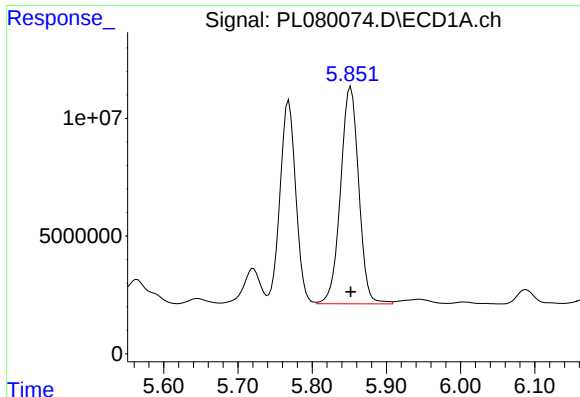

#26 Chlordane-4


R.T.: 5.852 min
Delta R.T.: 0.000 min
Response: 157234875
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

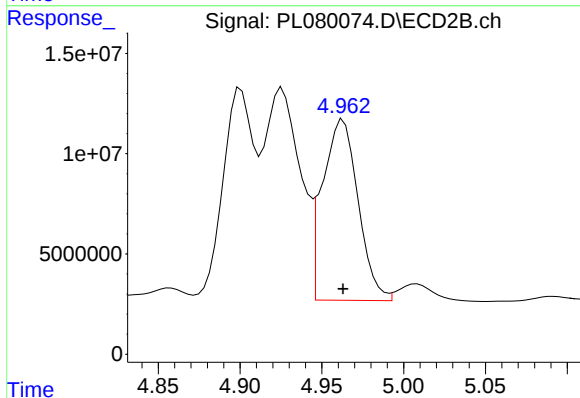


#26 Chlordane-4

R.T.: 4.963 min
Delta R.T.: 0.000 min
Response: 136742960
Conc: 500.00 ng/ml

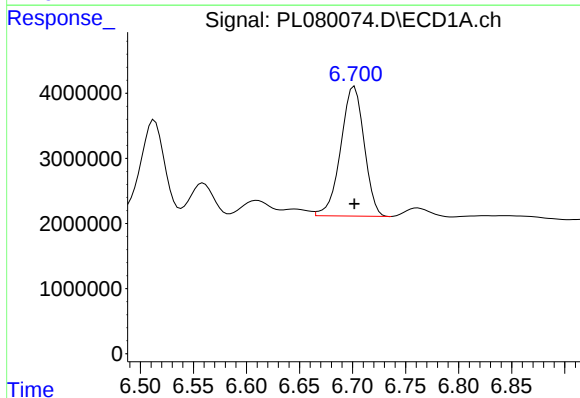


#27 Chlordane-5

R.T.: 6.702 min
Delta R.T.: 0.000 min
Response: 30562997
Conc: 500.00 ng/ml

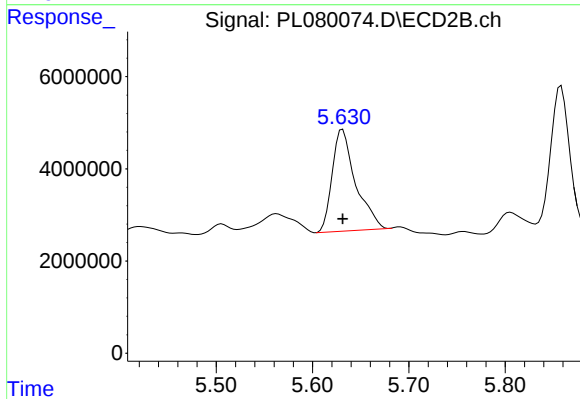

#27 Chlordane-5


R.T.: 5.631 min
Delta R.T.: 0.000 min
Response: 37292688
Conc: 500.00 ng/ml

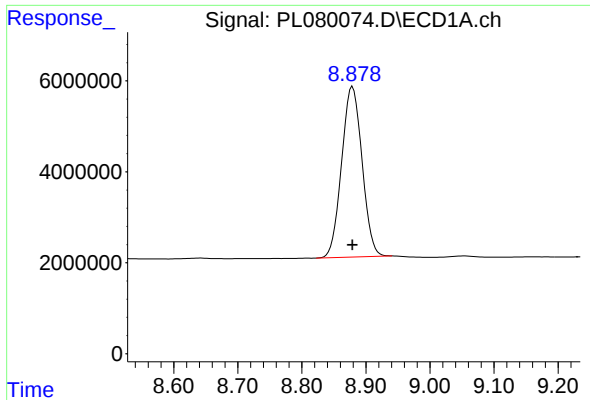

#28 Decachlorobiphenyl

R.T.: 8.879 min
Delta R.T.: 0.000 min
Response: 82981634
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

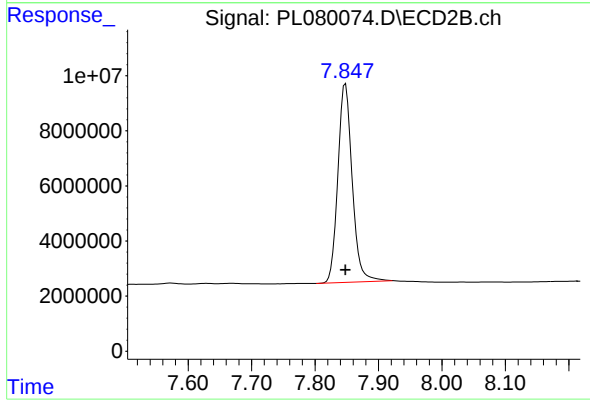

#28 Decachlorobiphenyl

R.T.: 7.848 min
Delta R.T.: 0.000 min
Response: 113355447
Conc: 50.00 ng/ml