

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010423\
 Data File : PL080066.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2023 19:42
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 05:47:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010423.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 05 05:11:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.370	2.693	45240371	50338018	22.743	22.138
28)	SA Decachlor...	8.879	7.848	39917792	51746386	23.266	22.904
Target Compounds							
9)	A Endosulfan I	5.895	5.019	19585547	27629812	11.414	10.667
10)	B gamma-Chl...	5.768	4.900	20868870	30348542	11.567	10.874
12)	B 4,4'-DDE	6.031	5.158	34085632	48774507	21.653	21.021
13)	MA Dieldrin	6.173	5.284	38319517	56210311	22.386	21.491
19)	B Endosulfa...	6.992	6.256	34428081	45288793	21.052	20.384
20)	A Methoxychlor	7.359	6.543	95585930	127.6E6	107.489	111.354
21)	B Endrin ke...	7.477	6.760	40323723	53057753	22.657	21.771


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010423\
Data File : PL080066.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2023 19:42
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 05:47:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010423.M
Quant Title : GC Extractables
QLast Update : Thu Jan 05 05:11:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

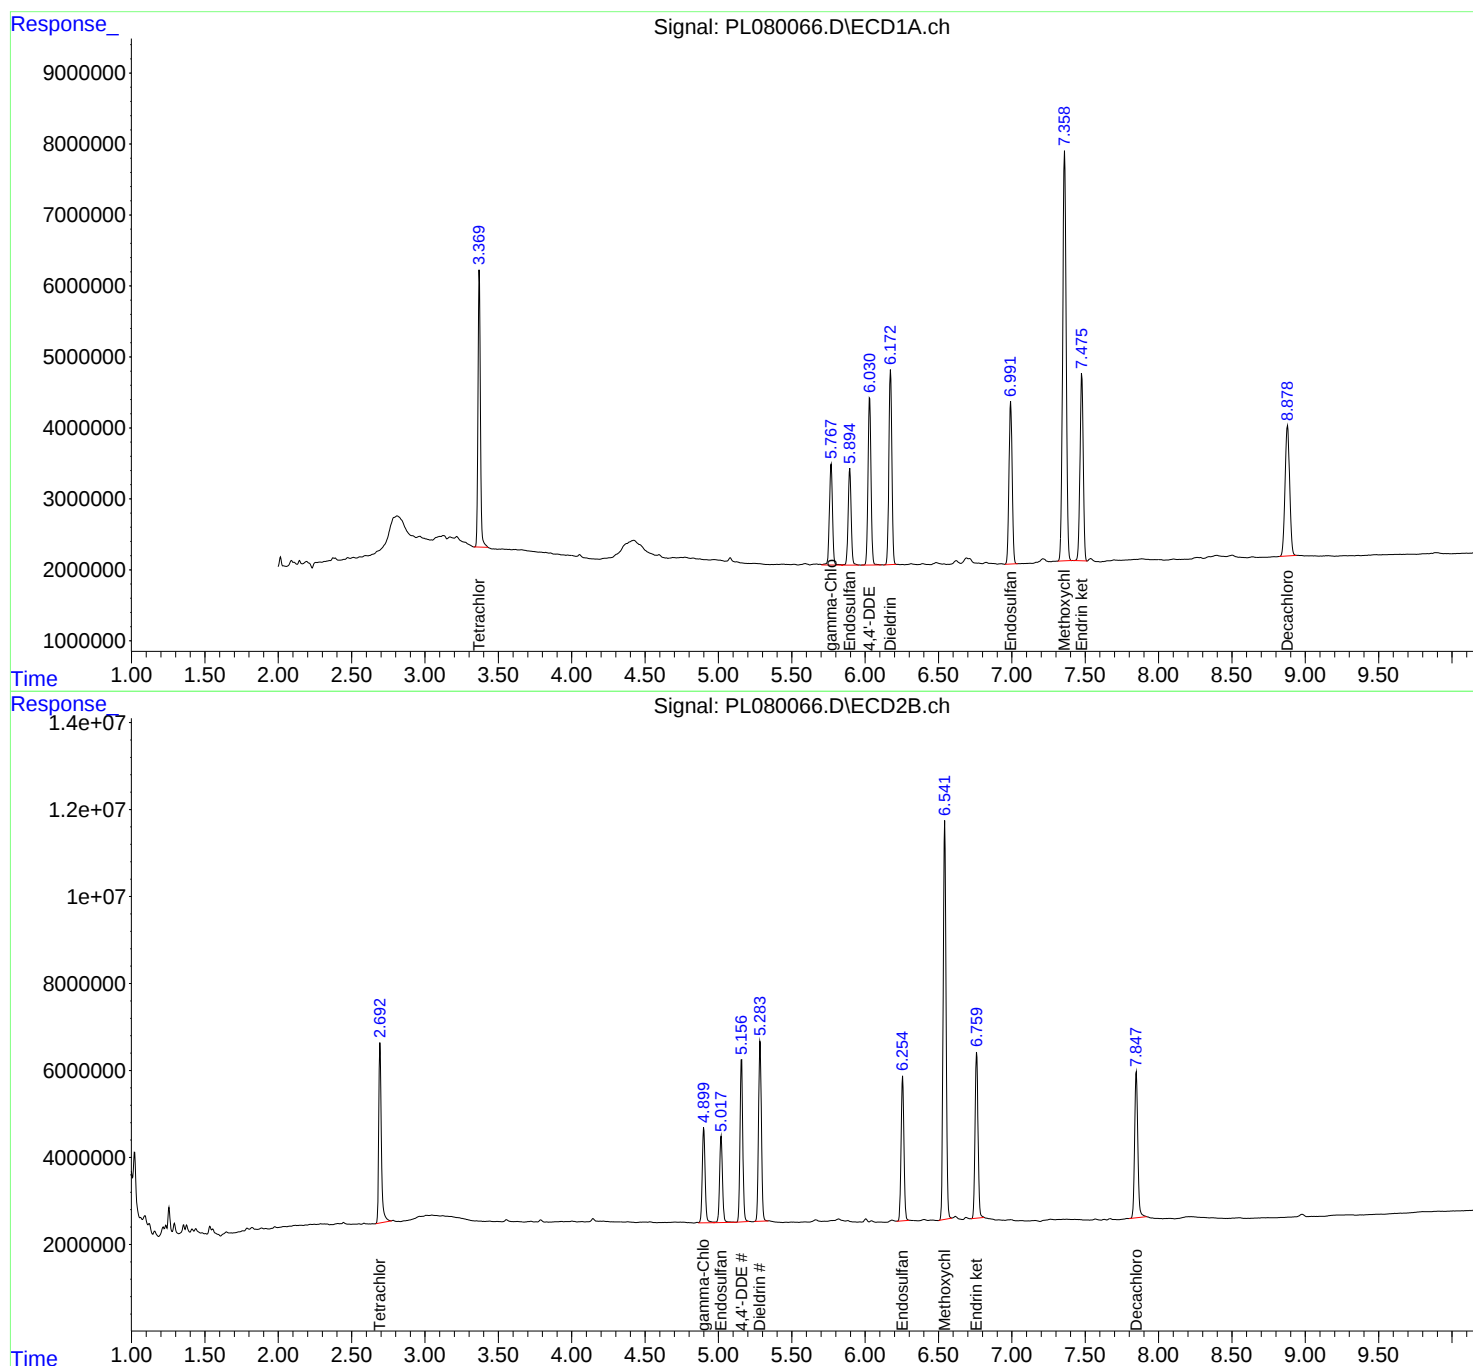


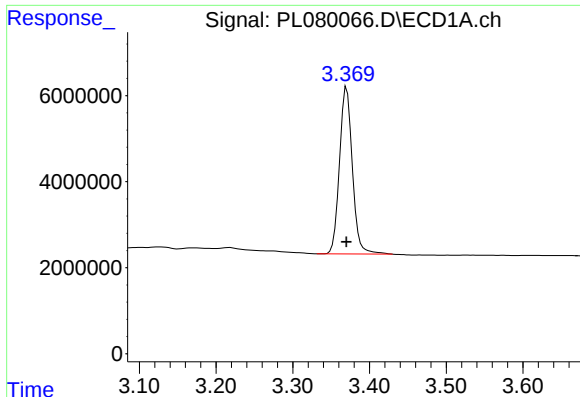

#1 Tetrachloro-m-xylene


R.T.: 3.370 min
Delta R.T.: 0.000 min
Response: 45240371
Conc: 22.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

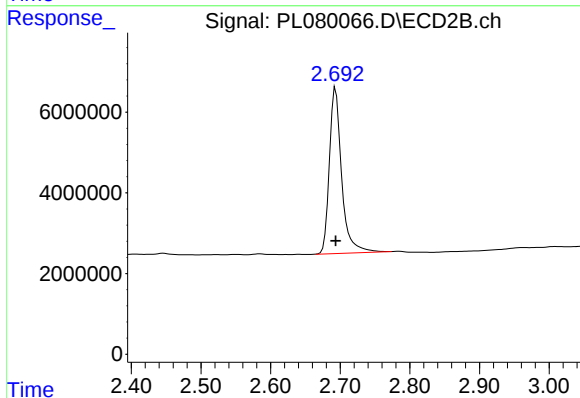


#1 Tetrachloro-m-xylene

R.T.: 2.693 min
Delta R.T.: 0.000 min
Response: 50338018
Conc: 22.14 ng/ml

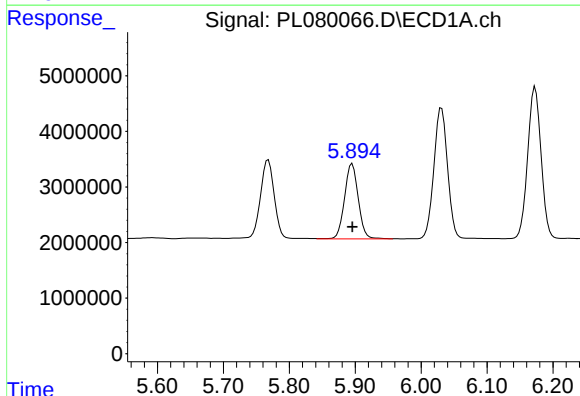


#9 Endosulfan I

R.T.: 5.895 min
Delta R.T.: 0.000 min
Response: 19585547
Conc: 11.41 ng/ml

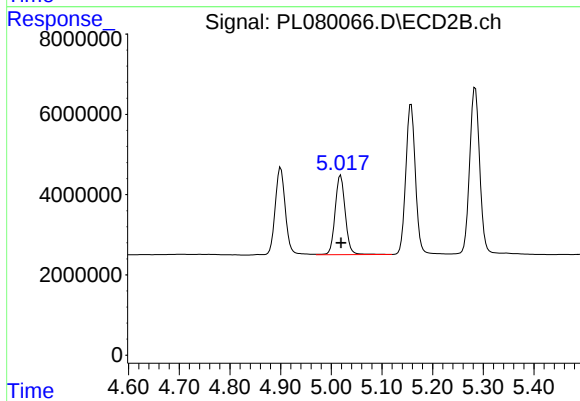

#9 Endosulfan I


R.T.: 5.019 min
Delta R.T.: 0.000 min
Response: 27629812
Conc: 10.67 ng/ml

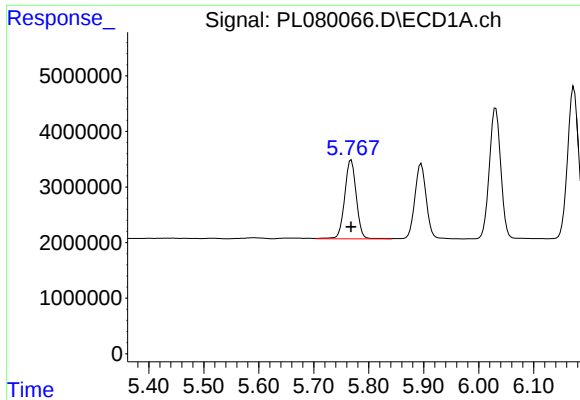

#10 gamma-Chlordane


R.T.: 5.768 min
Delta R.T.: 0.000 min
Response: 20868870
Conc: 11.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

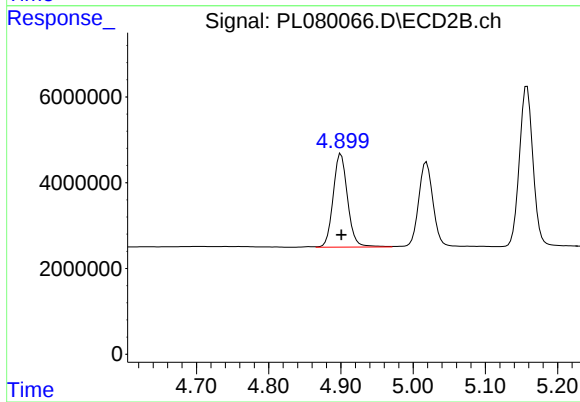


#10 gamma-Chlordane

R.T.: 4.900 min
Delta R.T.: 0.000 min
Response: 30348542
Conc: 10.87 ng/ml

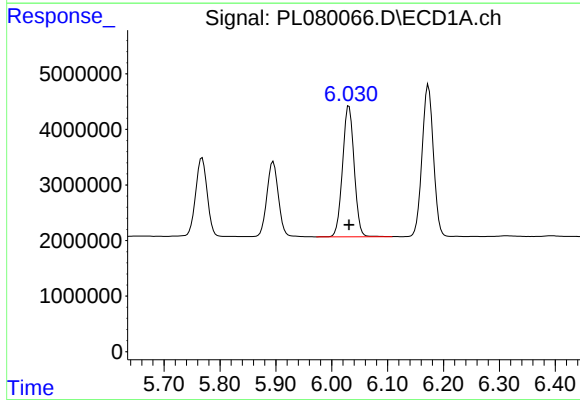


#12 4,4'-DDE

R.T.: 6.031 min
Delta R.T.: 0.000 min
Response: 34085632
Conc: 21.65 ng/ml

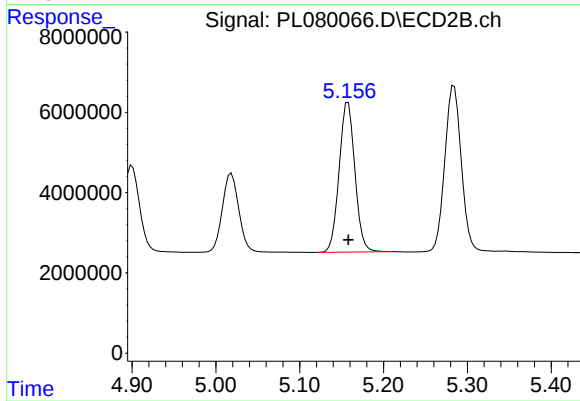

#12 4,4'-DDE


R.T.: 5.158 min
Delta R.T.: 0.000 min
Response: 48774507
Conc: 21.02 ng/ml

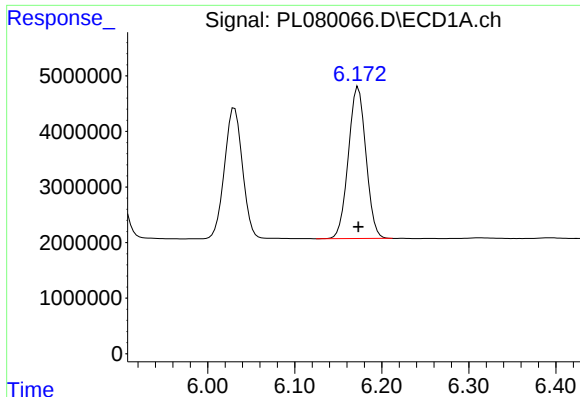

#13 Dieldrin


R.T.: 6.173 min
Delta R.T.: 0.000 min
Response: 38319517
Conc: 22.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

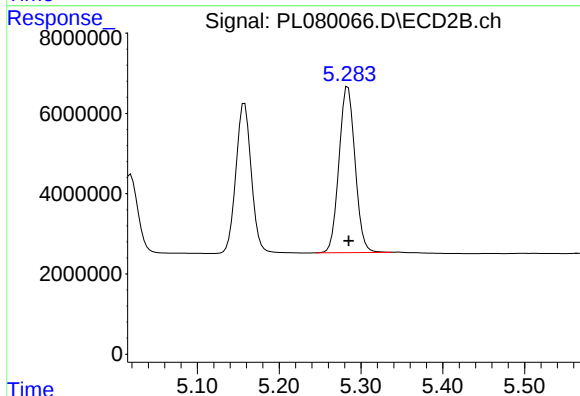


#13 Dieldrin

R.T.: 5.284 min
Delta R.T.: 0.000 min
Response: 56210311
Conc: 21.49 ng/ml

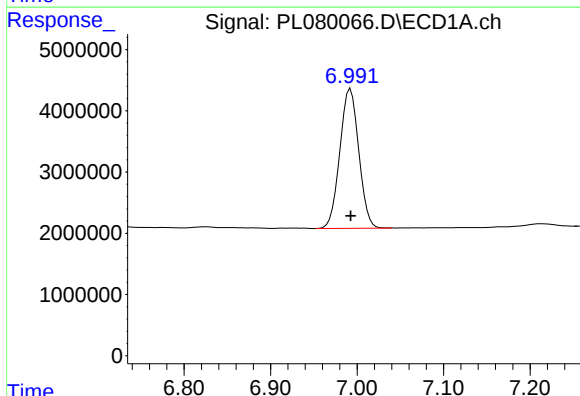


#19 Endosulfan Sulfate

R.T.: 6.992 min
Delta R.T.: 0.000 min
Response: 34428081
Conc: 21.05 ng/ml

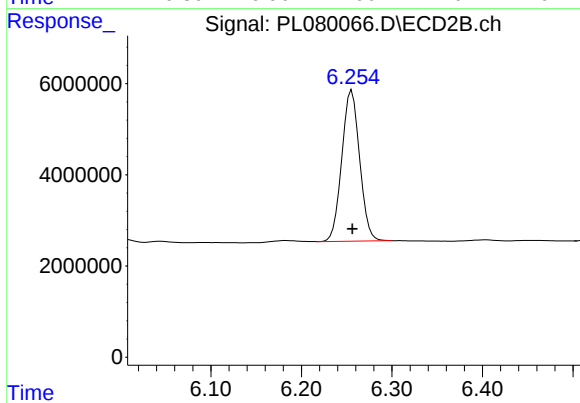

#19 Endosulfan Sulfate


R.T.: 6.256 min
Delta R.T.: 0.000 min
Response: 45288793
Conc: 20.38 ng/ml

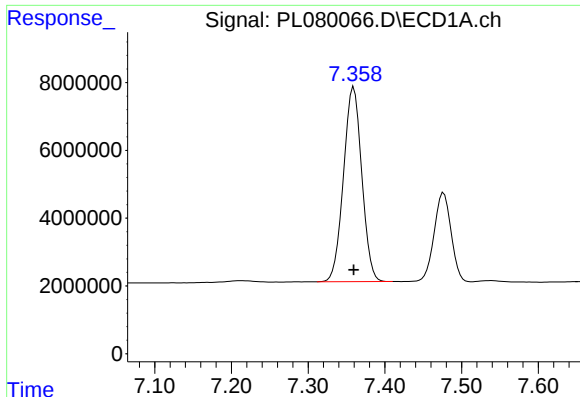

#20 Methoxychlor


R.T.: 7.359 min
Delta R.T.: 0.000 min
Response: 95585930
Conc: 107.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

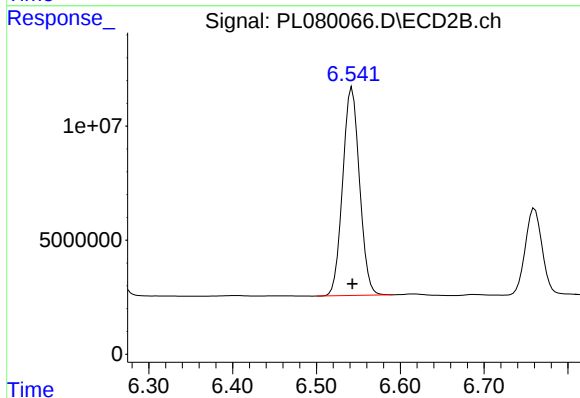


#20 Methoxychlor

R.T.: 6.543 min
Delta R.T.: 0.000 min
Response: 127620016
Conc: 111.35 ng/ml

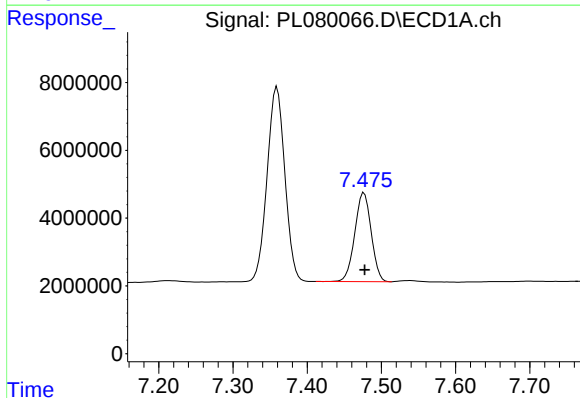


#21 Endrin ketone

R.T.: 7.477 min
Delta R.T.: 0.000 min
Response: 40323723
Conc: 22.66 ng/ml

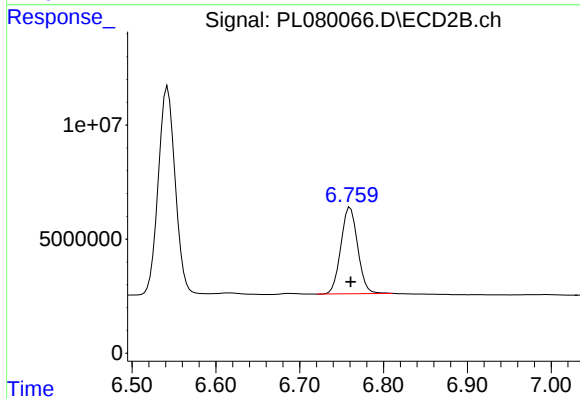

#21 Endrin ketone


R.T.: 6.760 min
Delta R.T.: 0.000 min
Response: 53057753
Conc: 21.77 ng/ml

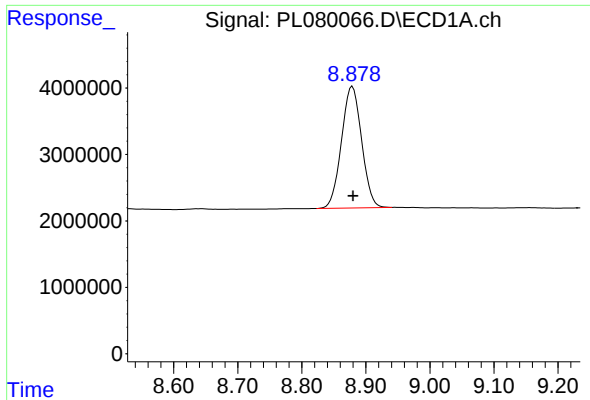

#28 Decachlorobiphenyl

R.T.: 8.879 min
Delta R.T.: 0.000 min
Response: 39917792
Conc: 23.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

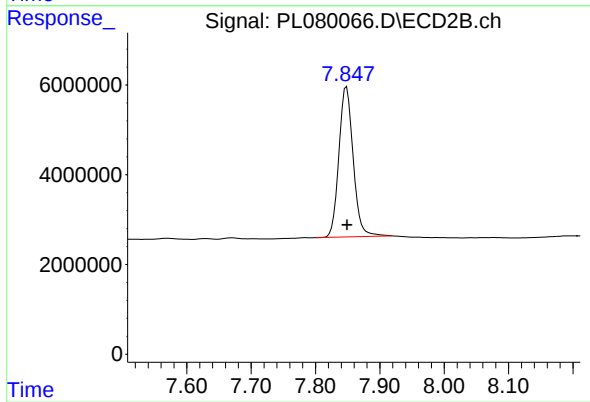

#28 Decachlorobiphenyl

R.T.: 7.848 min
Delta R.T.: 0.000 min
Response: 51746386
Conc: 22.90 ng/ml