

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010423\
 Data File : PL080072.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2023 21:05
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 05:01:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010423.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 05 05:01:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.370	2.693	199.4E6	279.2E6	100.033	100.429
28)	SA Decachlor...	8.880	7.849	156.1E6	216.1E6	96.952	97.604
Target Compounds							
23)	Chlordane-1	4.526	3.692	61485267	80896665	998.146	1001.360
24)	Chlordane-2	5.057	4.270	69883253	85760546	974.667	978.431
25)	Chlordane-3	5.770	4.901	257.6E6	279.7E6	1004.814	1011.914
26)	Chlordane-4	5.852	4.963	312.7E6	280.1E6	997.124	1011.895
27)	Chlordane-5	6.703	5.632	58797196	73275741	980.581	991.143



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010423\
Data File : PL080072.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2023 21:05
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 05:01:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010423.M
Quant Title : GC Extractables
QLast Update : Thu Jan 05 05:01:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

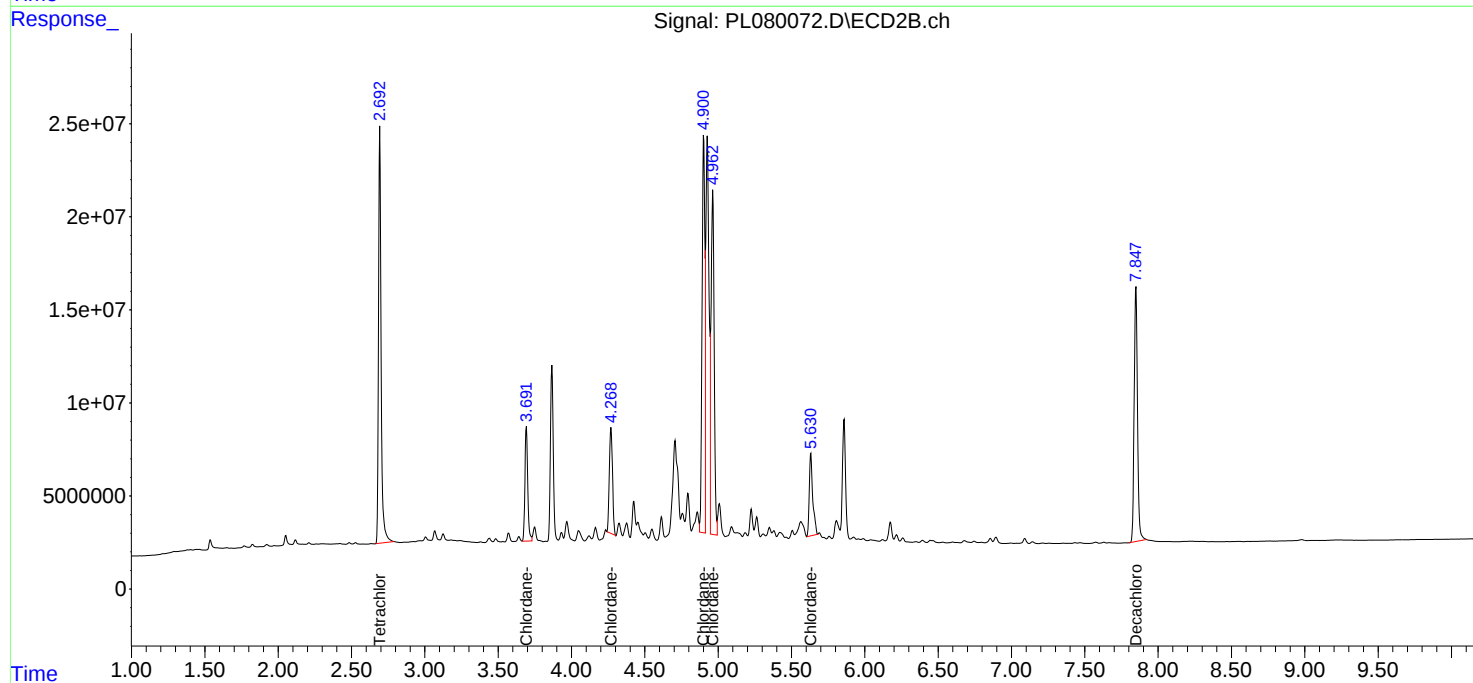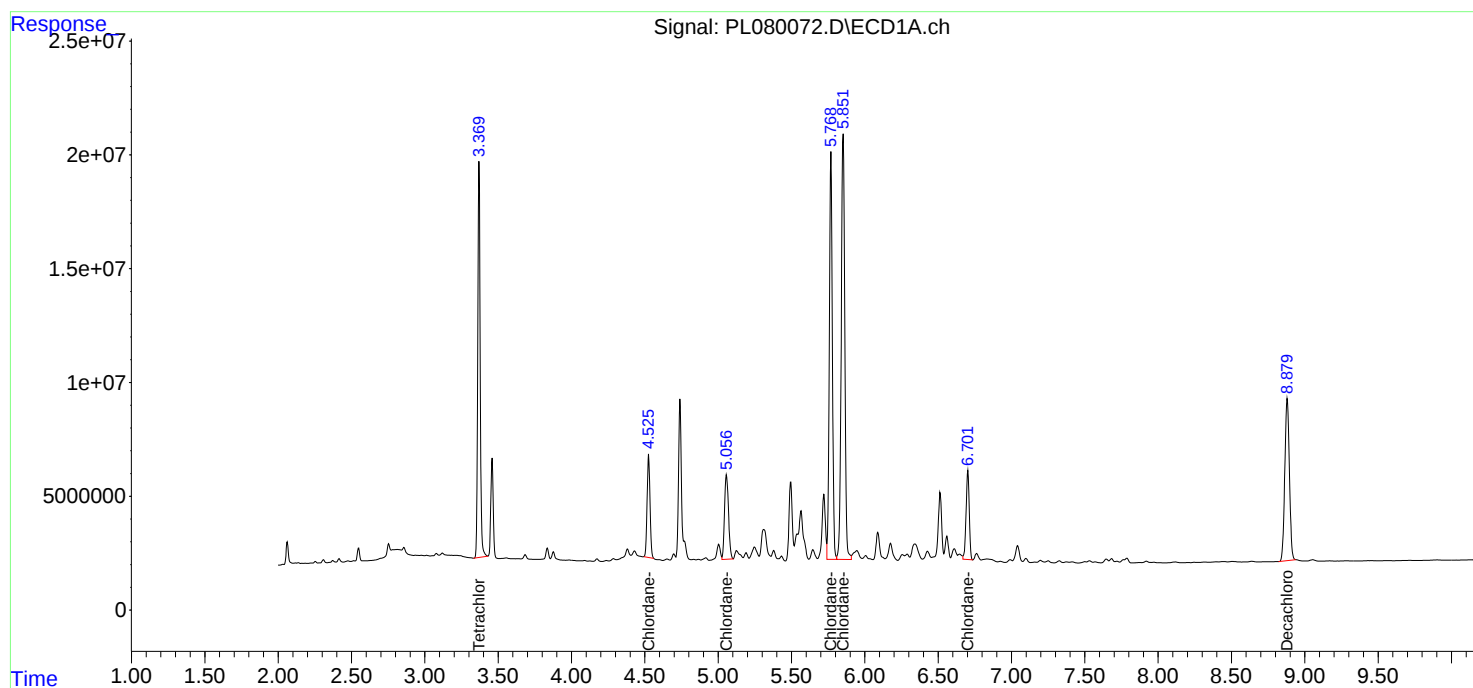


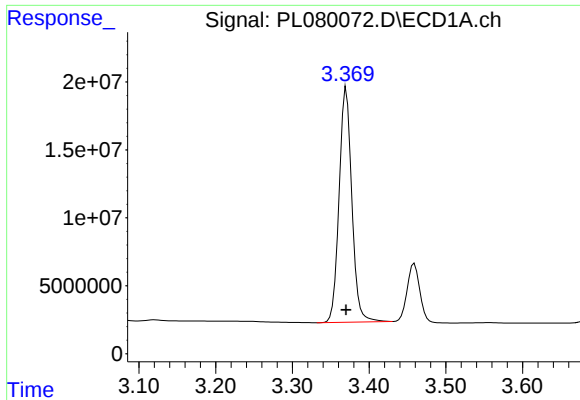

#1 Tetrachloro-m-xylene


R.T.: 3.370 min
Delta R.T.: 0.000 min
Response: 199392982
Conc: 100.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

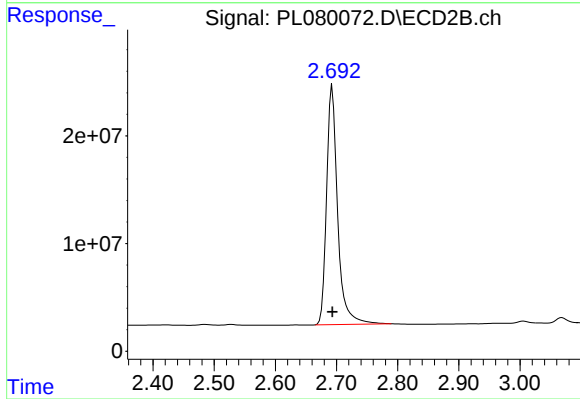


#1 Tetrachloro-m-xylene

R.T.: 2.693 min
Delta R.T.: 0.000 min
Response: 279234476
Conc: 100.43 ng/ml

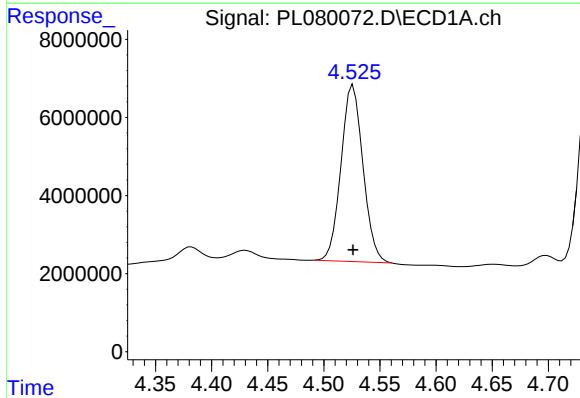


#23 Chlordane-1

R.T.: 4.526 min
Delta R.T.: 0.000 min
Response: 61485267
Conc: 998.15 ng/ml

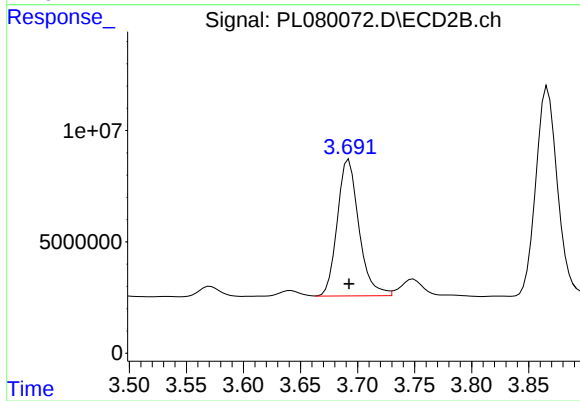

#23 Chlordane-1


R.T.: 3.692 min
Delta R.T.: 0.000 min
Response: 80896665
Conc: 1001.36 ng/ml

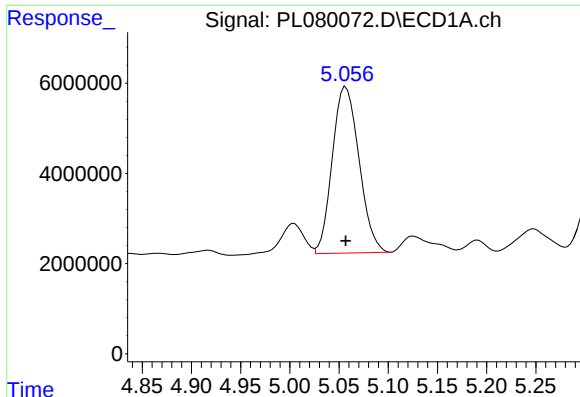

#24 Chlordane-2


R.T.: 5.057 min
Delta R.T.: 0.000 min
Response: 69883253
Conc: 974.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

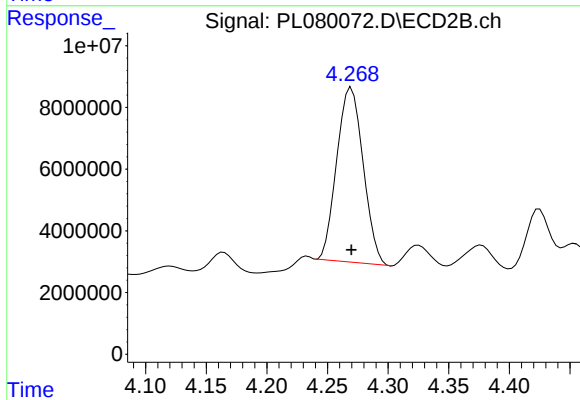


#24 Chlordane-2

R.T.: 4.270 min
Delta R.T.: 0.000 min
Response: 85760546
Conc: 978.43 ng/ml

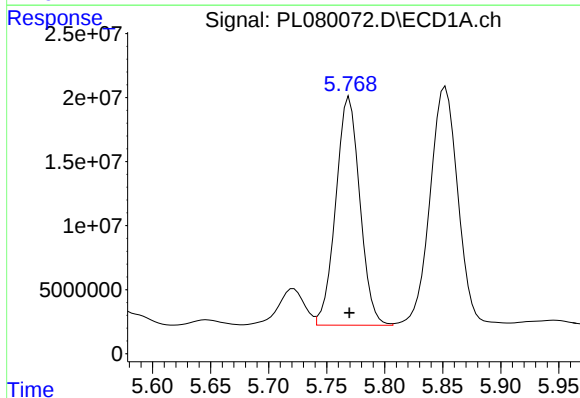


#25 Chlordane-3

R.T.: 5.770 min
Delta R.T.: 0.000 min
Response: 257568037
Conc: 1004.81 ng/ml

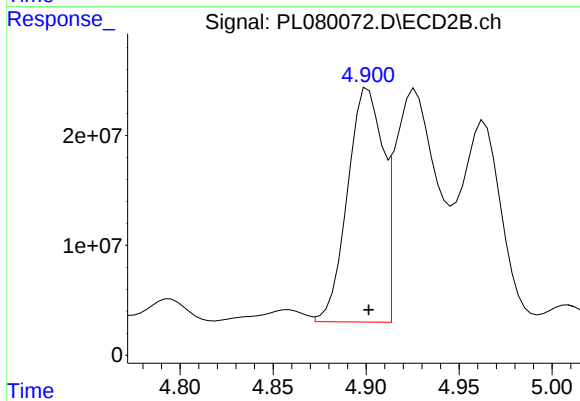

#25 Chlordane-3


R.T.: 4.901 min
Delta R.T.: 0.000 min
Response: 279731070
Conc: 1011.91 ng/ml

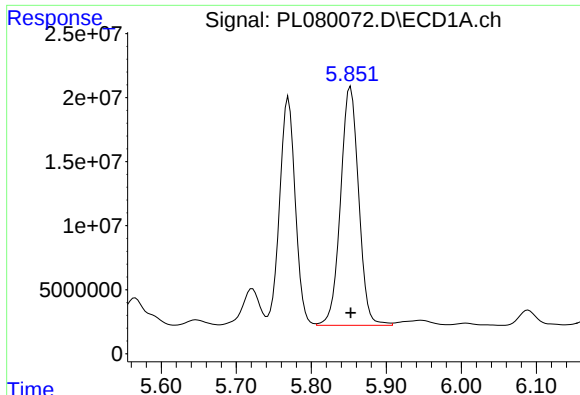

#26 Chlordane-4


R.T.: 5.852 min
Delta R.T.: 0.000 min
Response: 312665883
Conc: 997.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

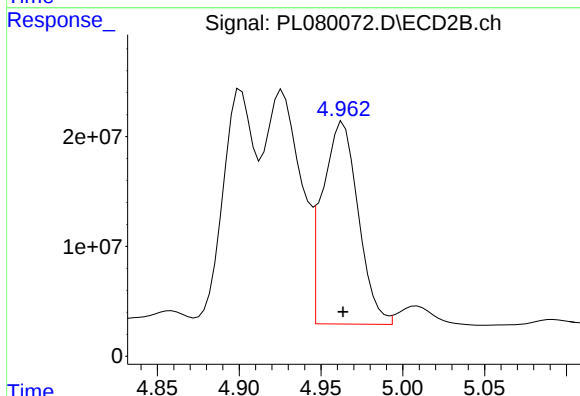


#26 Chlordane-4

R.T.: 4.963 min
Delta R.T.: 0.000 min
Response: 280070574
Conc: 1011.90 ng/ml

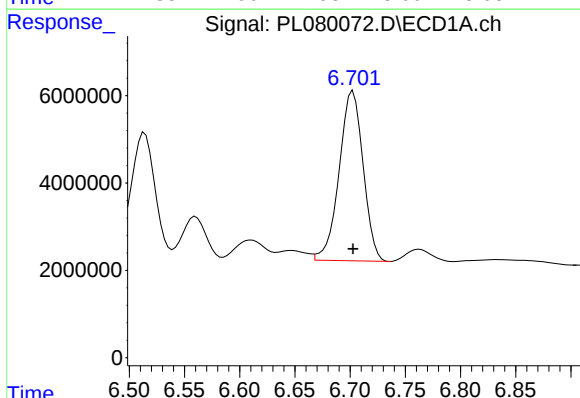


#27 Chlordane-5

R.T.: 6.703 min
Delta R.T.: 0.000 min
Response: 58797196
Conc: 980.58 ng/ml

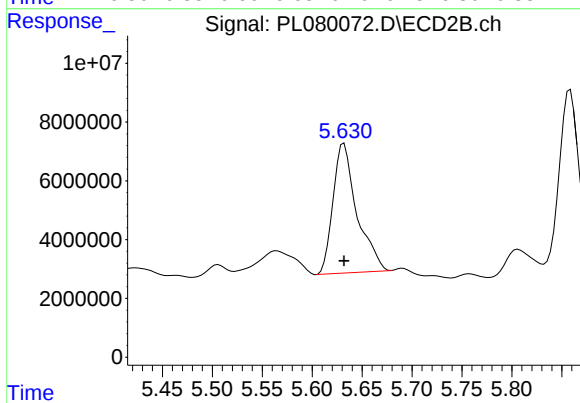

#27 Chlordane-5


R.T.: 5.632 min
Delta R.T.: 0.000 min
Response: 73275741
Conc: 991.14 ng/ml

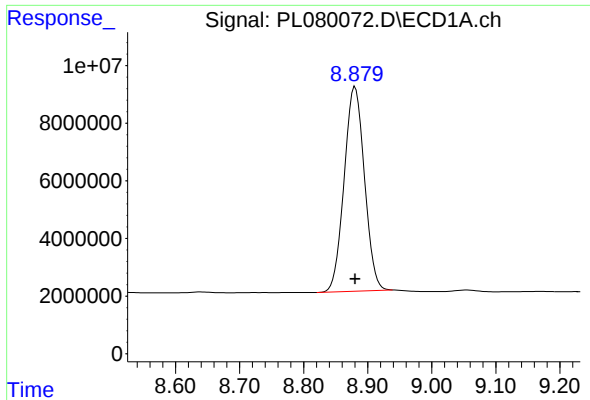

#28 Decachlorobiphenyl

R.T.: 8.880 min
Delta R.T.: 0.000 min
Response: 156144265
Conc: 96.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

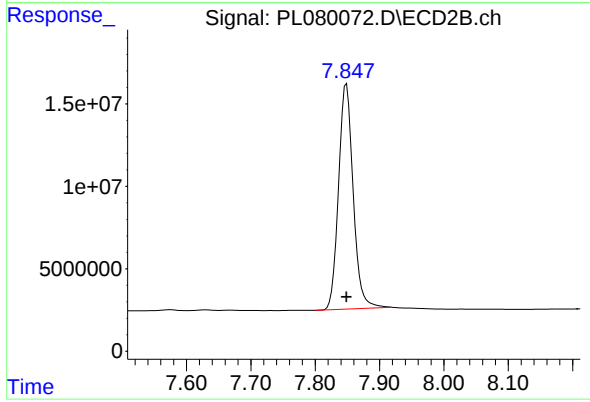

#28 Decachlorobiphenyl

R.T.: 7.849 min
Delta R.T.: 0.000 min
Response: 216099480
Conc: 97.60 ng/ml