

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010423\
 Data File : PL080075.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2023 21:47
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 05:04:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010423.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 05 05:04:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.370	2.693	48925648	65987984	24.733	24.146
28)	SA Decachlor...	8.880	7.848	43462067	58146275	26.510	26.076
Target Compounds							
23)	Chlordane-1	4.525	3.692	15042065	19536482	246.347	245.134
24)	Chlordane-2	5.056	4.269	18661970	22321123	259.049	254.767
25)	Chlordane-3	5.769	4.900	62108637	64221269	244.930	237.415
26)	Chlordane-4	5.852	4.963	77483966	64960849	248.685	239.890
27)	Chlordane-5	6.701	5.632	15837912	18253117	260.222	248.934



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010423\
Data File : PL080075.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2023 21:47
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 05:04:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010423.M
Quant Title : GC Extractables
QLast Update : Thu Jan 05 05:04:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

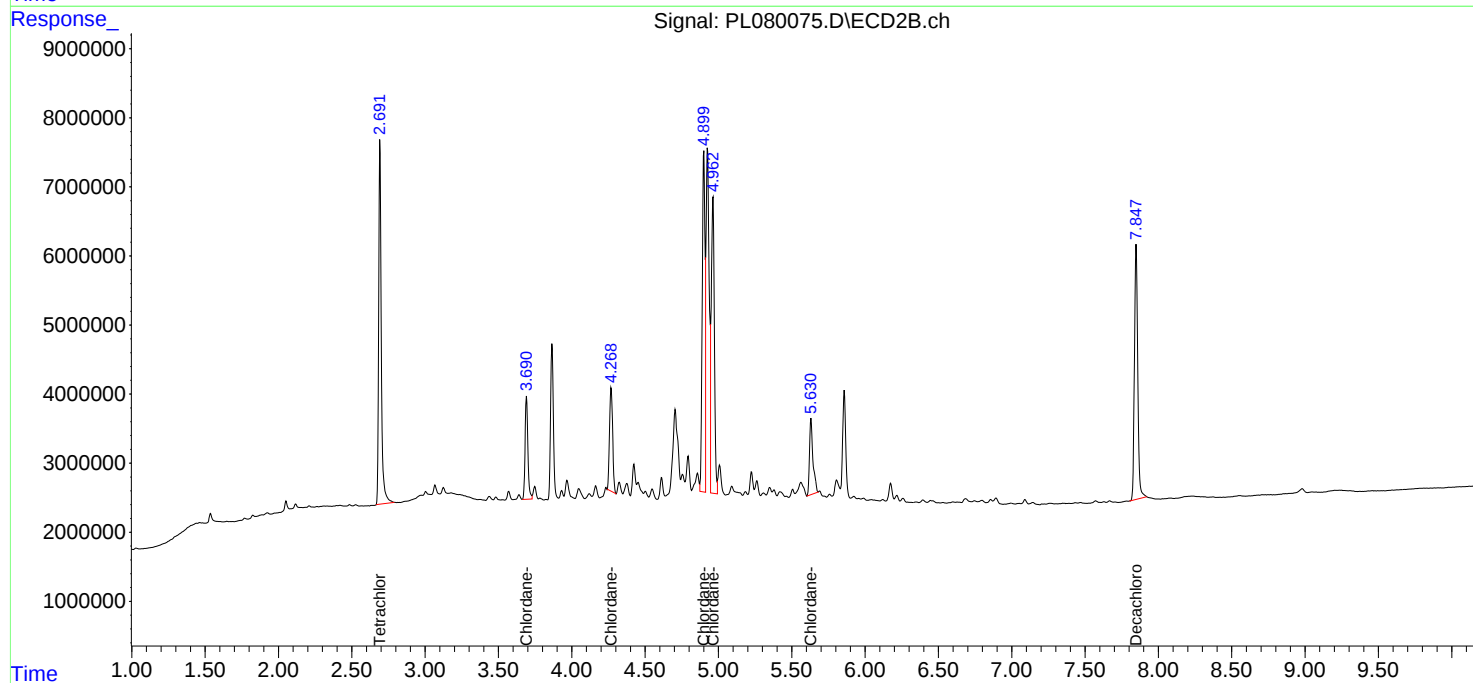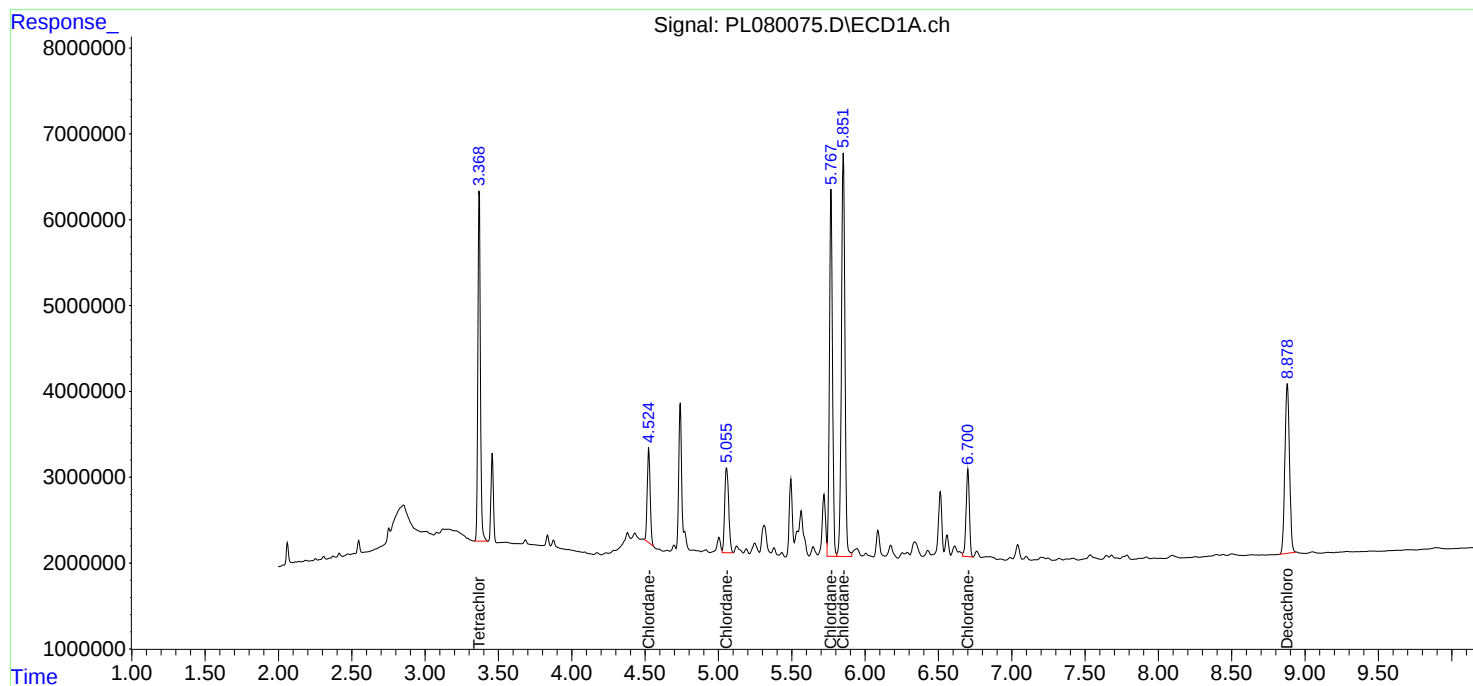


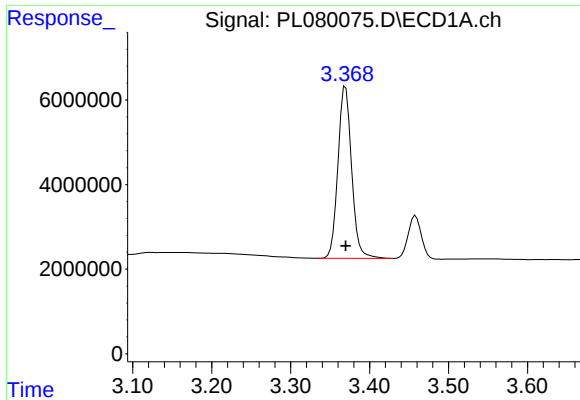

#1 Tetrachloro-m-xylene


R.T.: 3.370 min
Delta R.T.: 0.000 min
Response: 48925648
Conc: 24.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

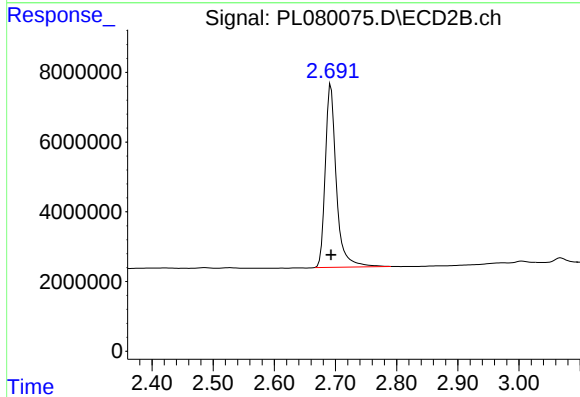


#1 Tetrachloro-m-xylene

R.T.: 2.693 min
Delta R.T.: 0.000 min
Response: 65987984
Conc: 24.15 ng/ml

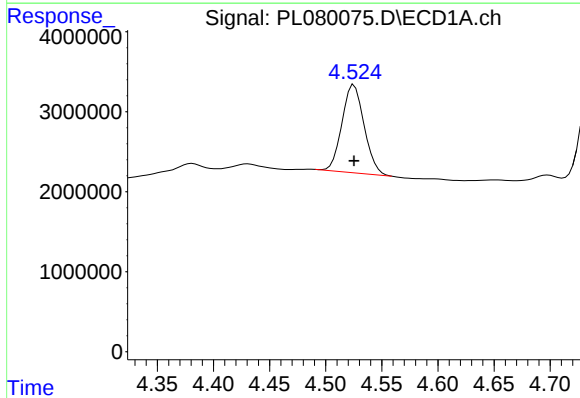


#23 Chlordane-1

R.T.: 4.525 min
Delta R.T.: 0.000 min
Response: 15042065
Conc: 246.35 ng/ml

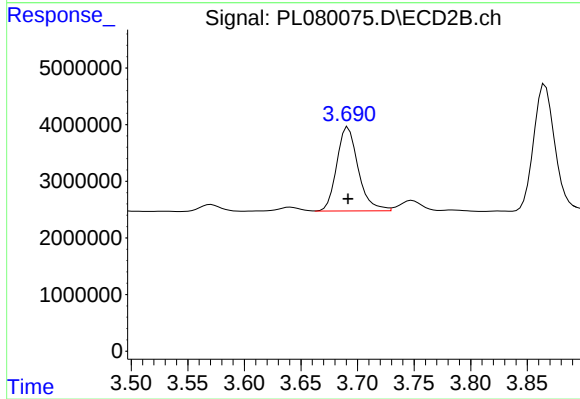

#23 Chlordane-1


R.T.: 3.692 min
Delta R.T.: 0.000 min
Response: 19536482
Conc: 245.13 ng/ml

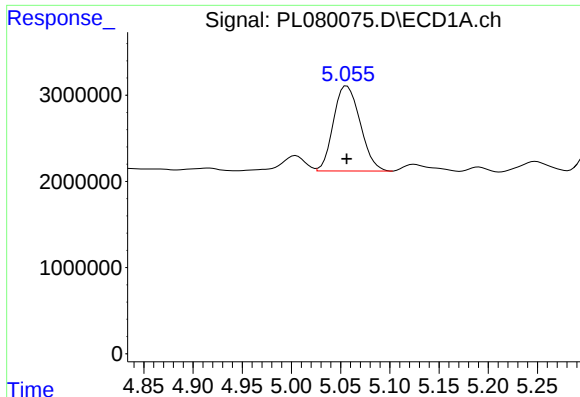

#24 Chlordane-2


R.T.: 5.056 min
Delta R.T.: 0.000 min
Response: 18661970
Conc: 259.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

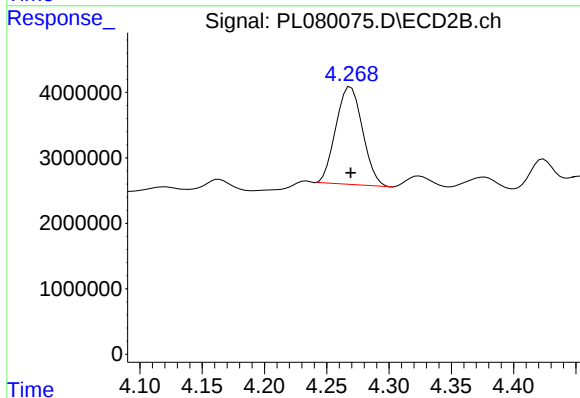


#24 Chlordane-2

R.T.: 4.269 min
Delta R.T.: 0.000 min
Response: 22321123
Conc: 254.77 ng/ml

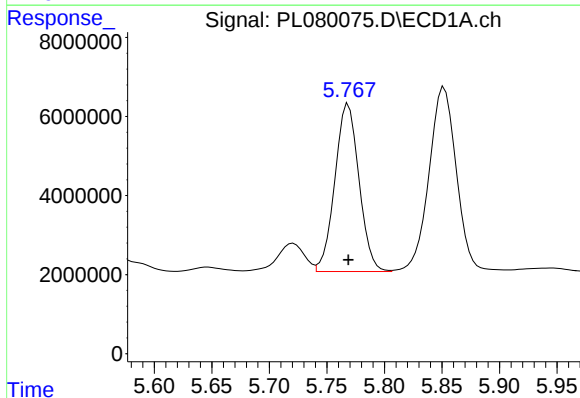


#25 Chlordane-3

R.T.: 5.769 min
Delta R.T.: 0.000 min
Response: 62108637
Conc: 244.93 ng/ml

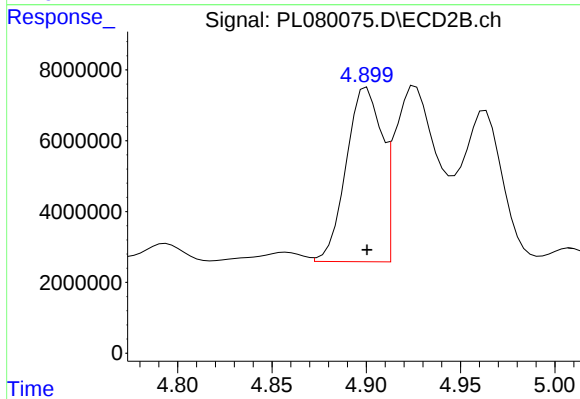

#25 Chlordane-3


R.T.: 4.900 min
Delta R.T.: 0.000 min
Response: 64221269
Conc: 237.42 ng/ml

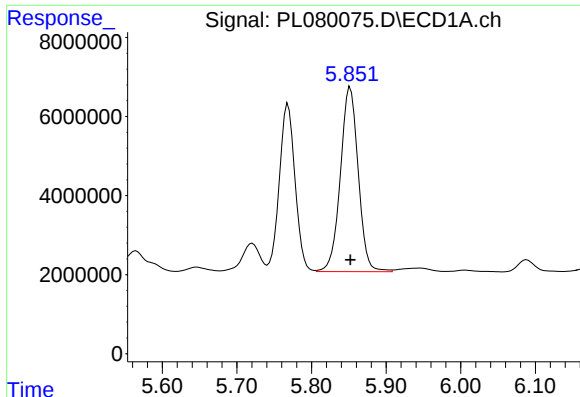

#26 Chlordane-4


R.T.: 5.852 min
Delta R.T.: 0.000 min
Response: 77483966
Conc: 248.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

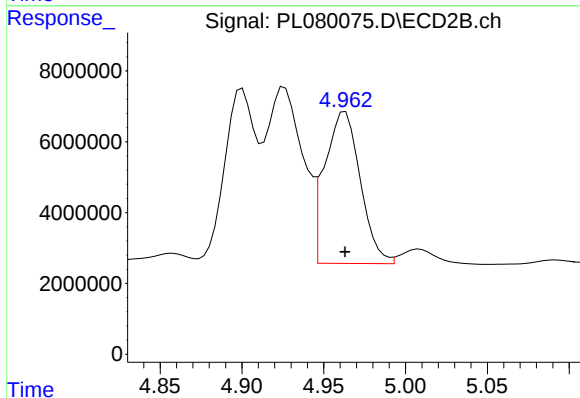


#26 Chlordane-4

R.T.: 4.963 min
Delta R.T.: 0.000 min
Response: 64960849
Conc: 239.89 ng/ml

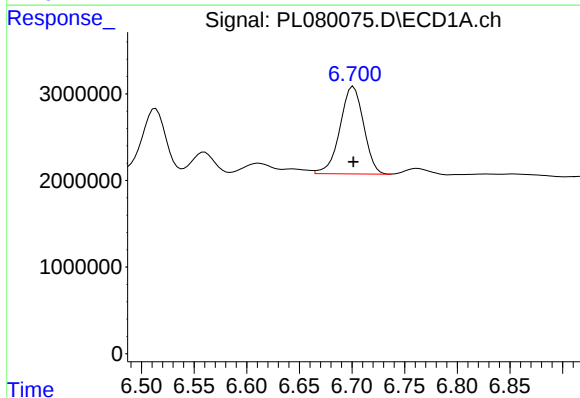


#27 Chlordane-5

R.T.: 6.701 min
Delta R.T.: 0.000 min
Response: 15837912
Conc: 260.22 ng/ml

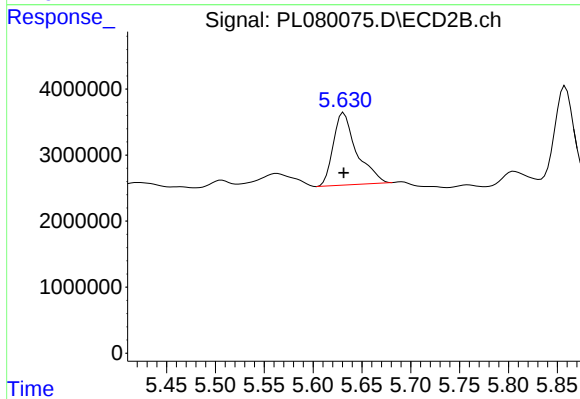

#27 Chlordane-5


R.T.: 5.632 min
Delta R.T.: 0.000 min
Response: 18253117
Conc: 248.93 ng/ml

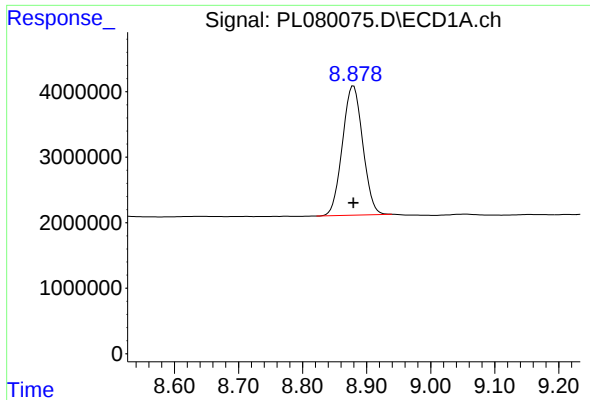

#28 Decachlorobiphenyl

R.T.: 8.880 min
Delta R.T.: 0.000 min
Response: 43462067
Conc: 26.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

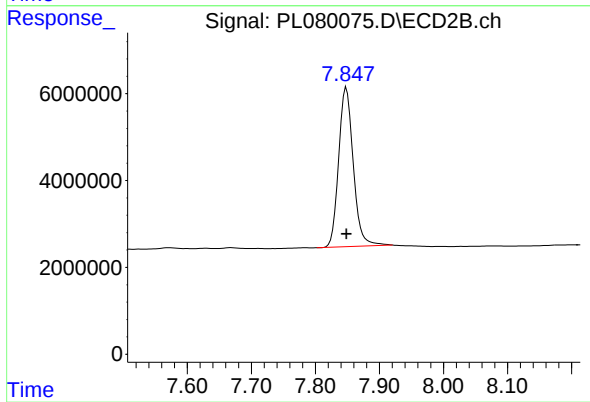

#28 Decachlorobiphenyl

R.T.: 7.848 min
Delta R.T.: 0.000 min
Response: 58146275
Conc: 26.08 ng/ml