

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010423\
 Data File : PL080083.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jan 2023 23:38
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL010423CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 05:07:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010423.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 05 05:06:14 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.371	2.693	103.1E6	140.0E6	52.757	52.709
28)	SA Decachlor...	8.881	7.848	88205614	115.4E6	52.961	51.106
Target Compounds							
23)	Chlordane-1	4.526	3.692	32217748	40795067	540.061	524.044
24)	Chlordane-2	5.058	4.269	38367511	45237623	531.063	519.872
25)	Chlordane-3	5.770	4.901	134.4E6	136.6E6	537.167	522.247
26)	Chlordane-4	5.853	4.963	165.3E6	138.2E6	535.106	524.921
27)	Chlordane-5	6.702	5.632	32383195	37607327	506.228	511.187



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010423\
Data File : PL080083.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jan 2023 23:38
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL010423CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 05:07:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010423.M
Quant Title : GC Extractables
QLast Update : Thu Jan 05 05:06:14 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

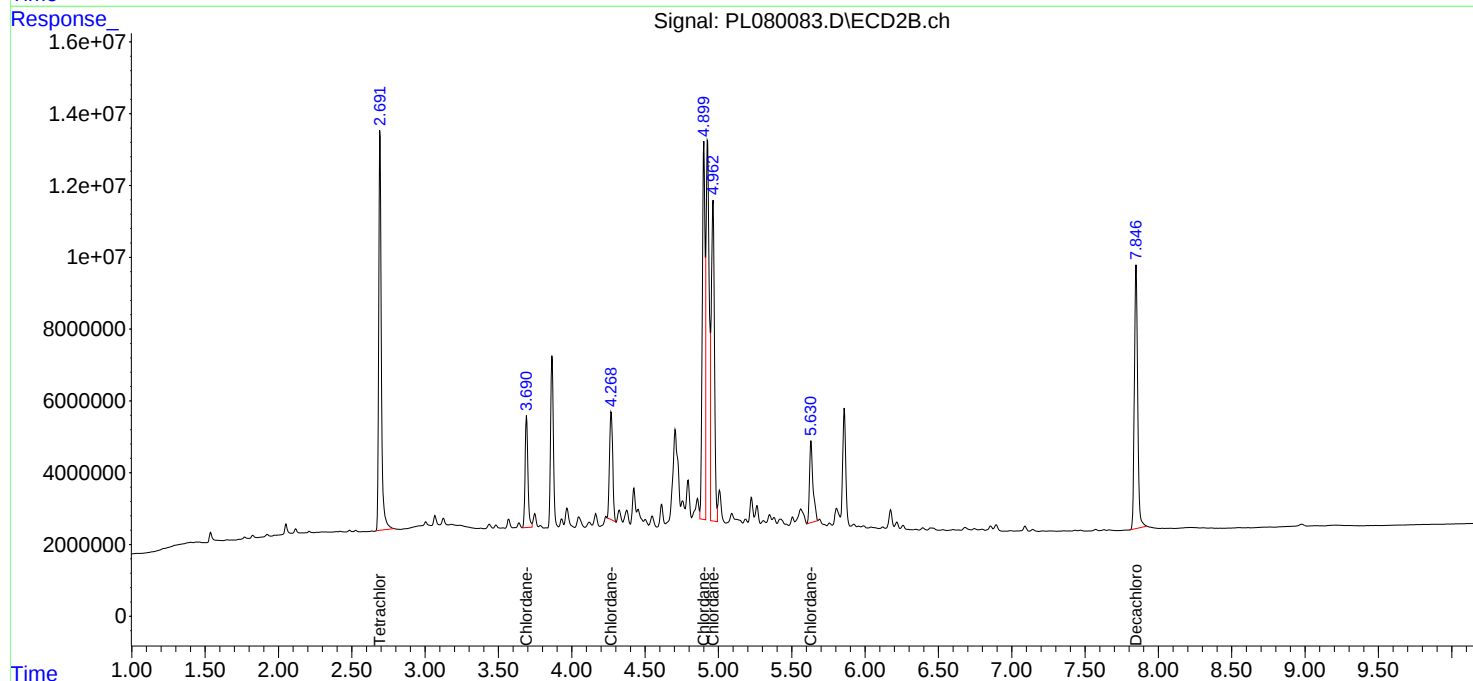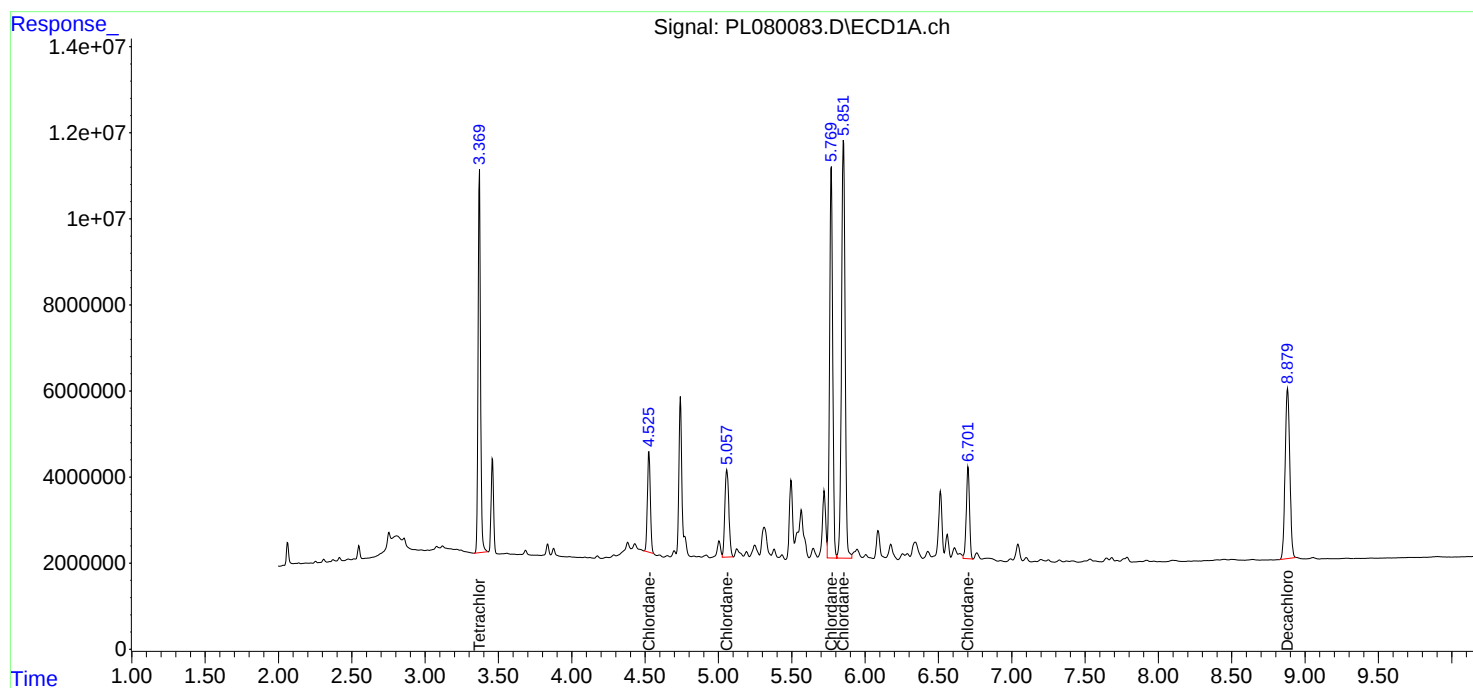


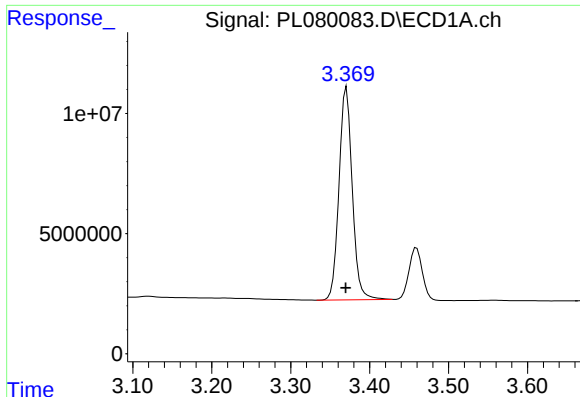

#1 Tetrachloro-m-xylene


R.T.: 3.371 min
Delta R.T.: 0.000 min
Response: 103111843
Conc: 52.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL010423CHLOR

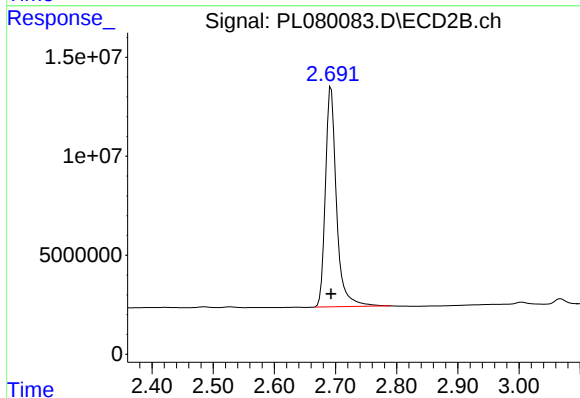


#1 Tetrachloro-m-xylene

R.T.: 2.693 min
Delta R.T.: 0.000 min
Response: 140010856
Conc: 52.71 ng/ml

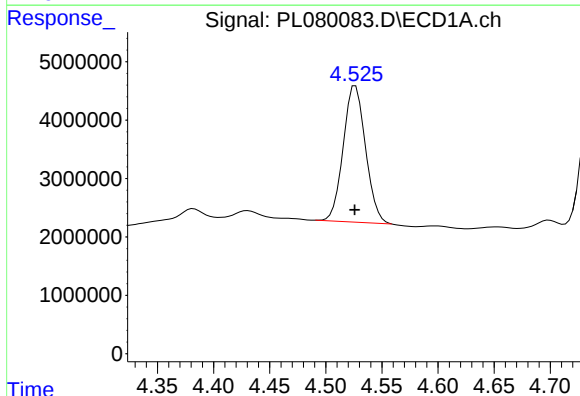


#23 Chlordane-1

R.T.: 4.526 min
Delta R.T.: 0.000 min
Response: 32217748
Conc: 540.06 ng/ml

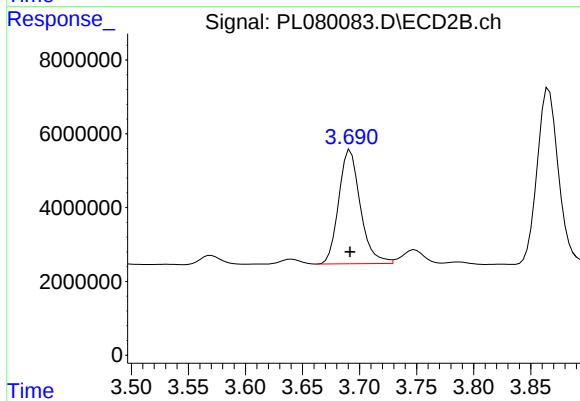

#23 Chlordane-1


R.T.: 3.692 min
Delta R.T.: 0.000 min
Response: 40795067
Conc: 524.04 ng/ml

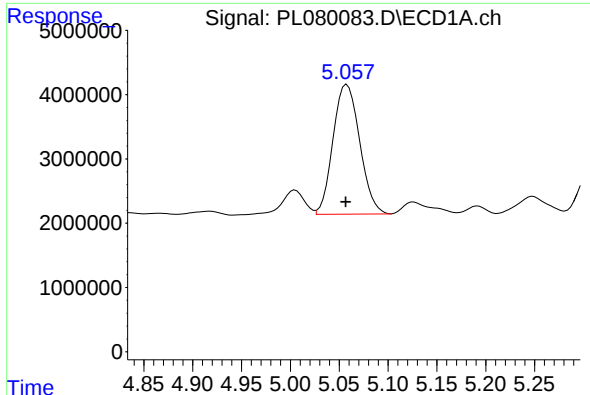

#24 Chlordane-2


R.T.: 5.058 min
Delta R.T.: 0.001 min
Response: 38367511
Conc: 531.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL010423CHLOR

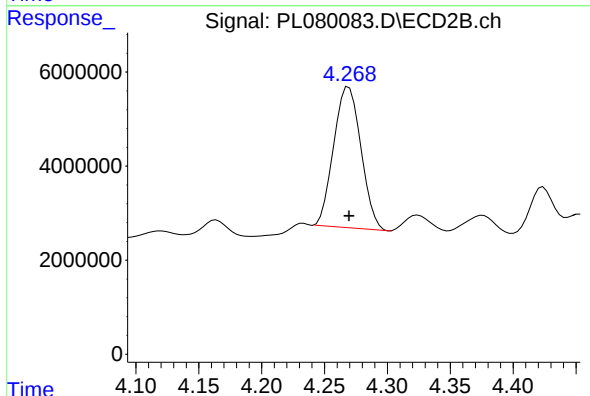


#24 Chlordane-2

R.T.: 4.269 min
Delta R.T.: 0.000 min
Response: 45237623
Conc: 519.87 ng/ml

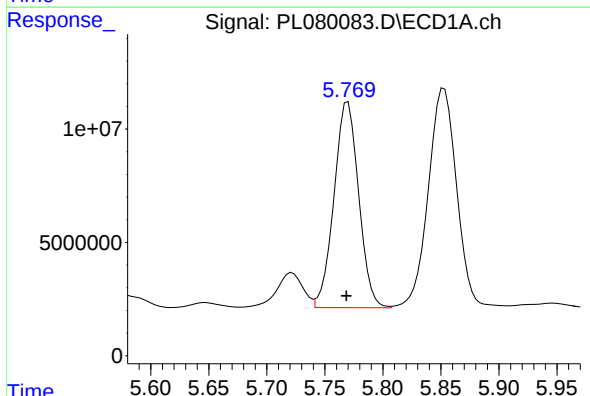


#25 Chlordane-3

R.T.: 5.770 min
Delta R.T.: 0.001 min
Response: 134377754
Conc: 537.17 ng/ml

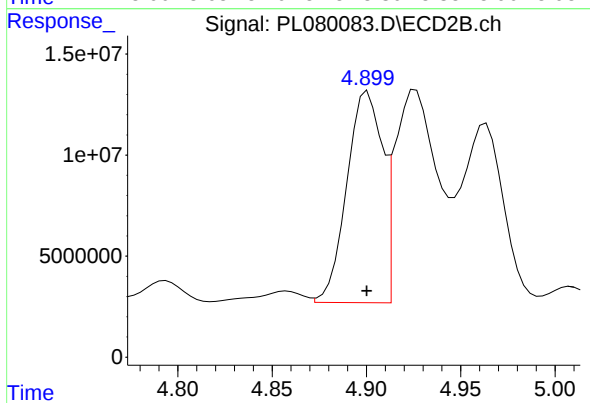

#25 Chlordane-3


R.T.: 4.901 min
Delta R.T.: 0.000 min
Response: 136620355
Conc: 522.25 ng/ml

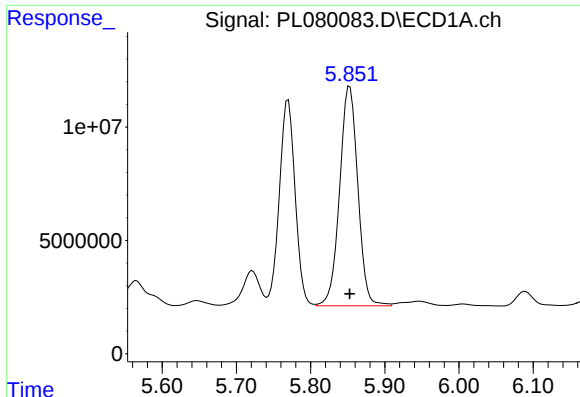

#26 Chlordane-4


R.T.: 5.853 min
Delta R.T.: 0.000 min
Response: 165304335
Conc: 535.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL010423CHLOR

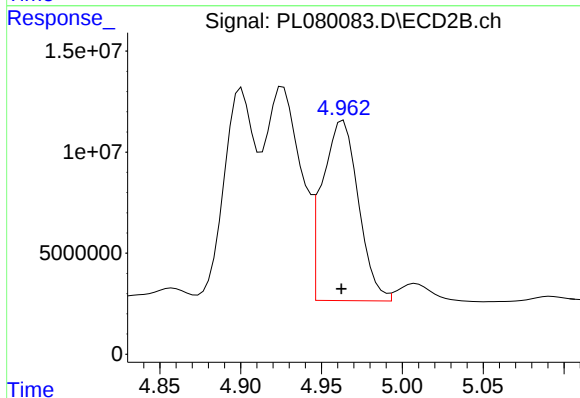


#26 Chlordane-4

R.T.: 4.963 min
Delta R.T.: 0.000 min
Response: 138150177
Conc: 524.92 ng/ml

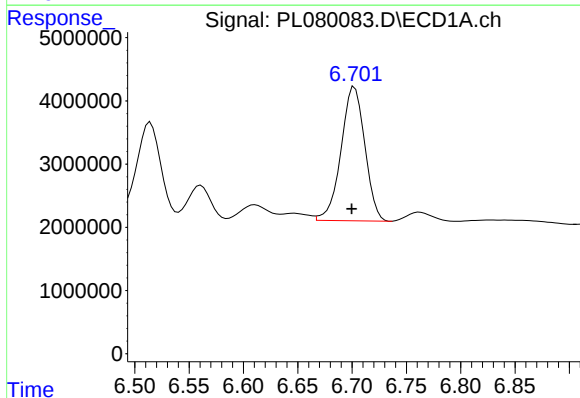


#27 Chlordane-5

R.T.: 6.702 min
Delta R.T.: 0.003 min
Response: 32383195
Conc: 506.23 ng/ml

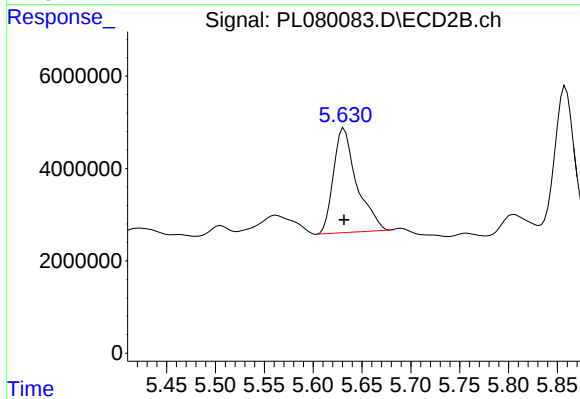

#27 Chlordane-5


R.T.: 5.632 min
Delta R.T.: 0.000 min
Response: 37607327
Conc: 511.19 ng/ml

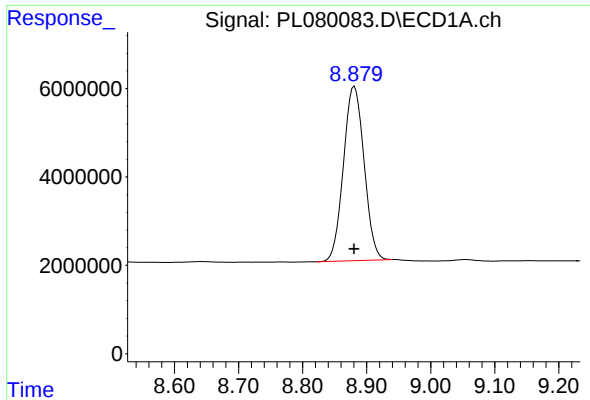

#28 Decachlorobiphenyl

R.T.: 8.881 min
Delta R.T.: 0.000 min
Response: 88205614
Conc: 52.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL010423CHLOR

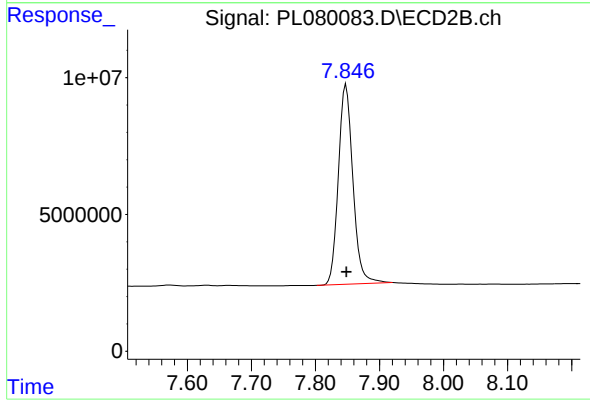

#28 Decachlorobiphenyl

R.T.: 7.848 min
Delta R.T.: 0.000 min
Response: 115366435
Conc: 51.11 ng/ml