

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010423\
 Data File : PL080088.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2023 01:01
 Operator : AR\AJ
 Sample : N6239-01 (Sig #1); N6239-01RE (Sig #2)
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 05:48:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010423.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 05 05:11:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.370	2.693	38262779	41850933	19.236	18.406
28) SA Decachlor...	8.880	7.848	37401619	46976425	21.799	20.793

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010423\
Data File : PL080088.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2023 01:01
Operator : AR\AJ
Sample : N6239-01 (Sig #1); N6239-01RE (Sig #2)
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-1S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 05:48:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010423.M
Quant Title : GC Extractables
QLast Update : Thu Jan 05 05:11:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

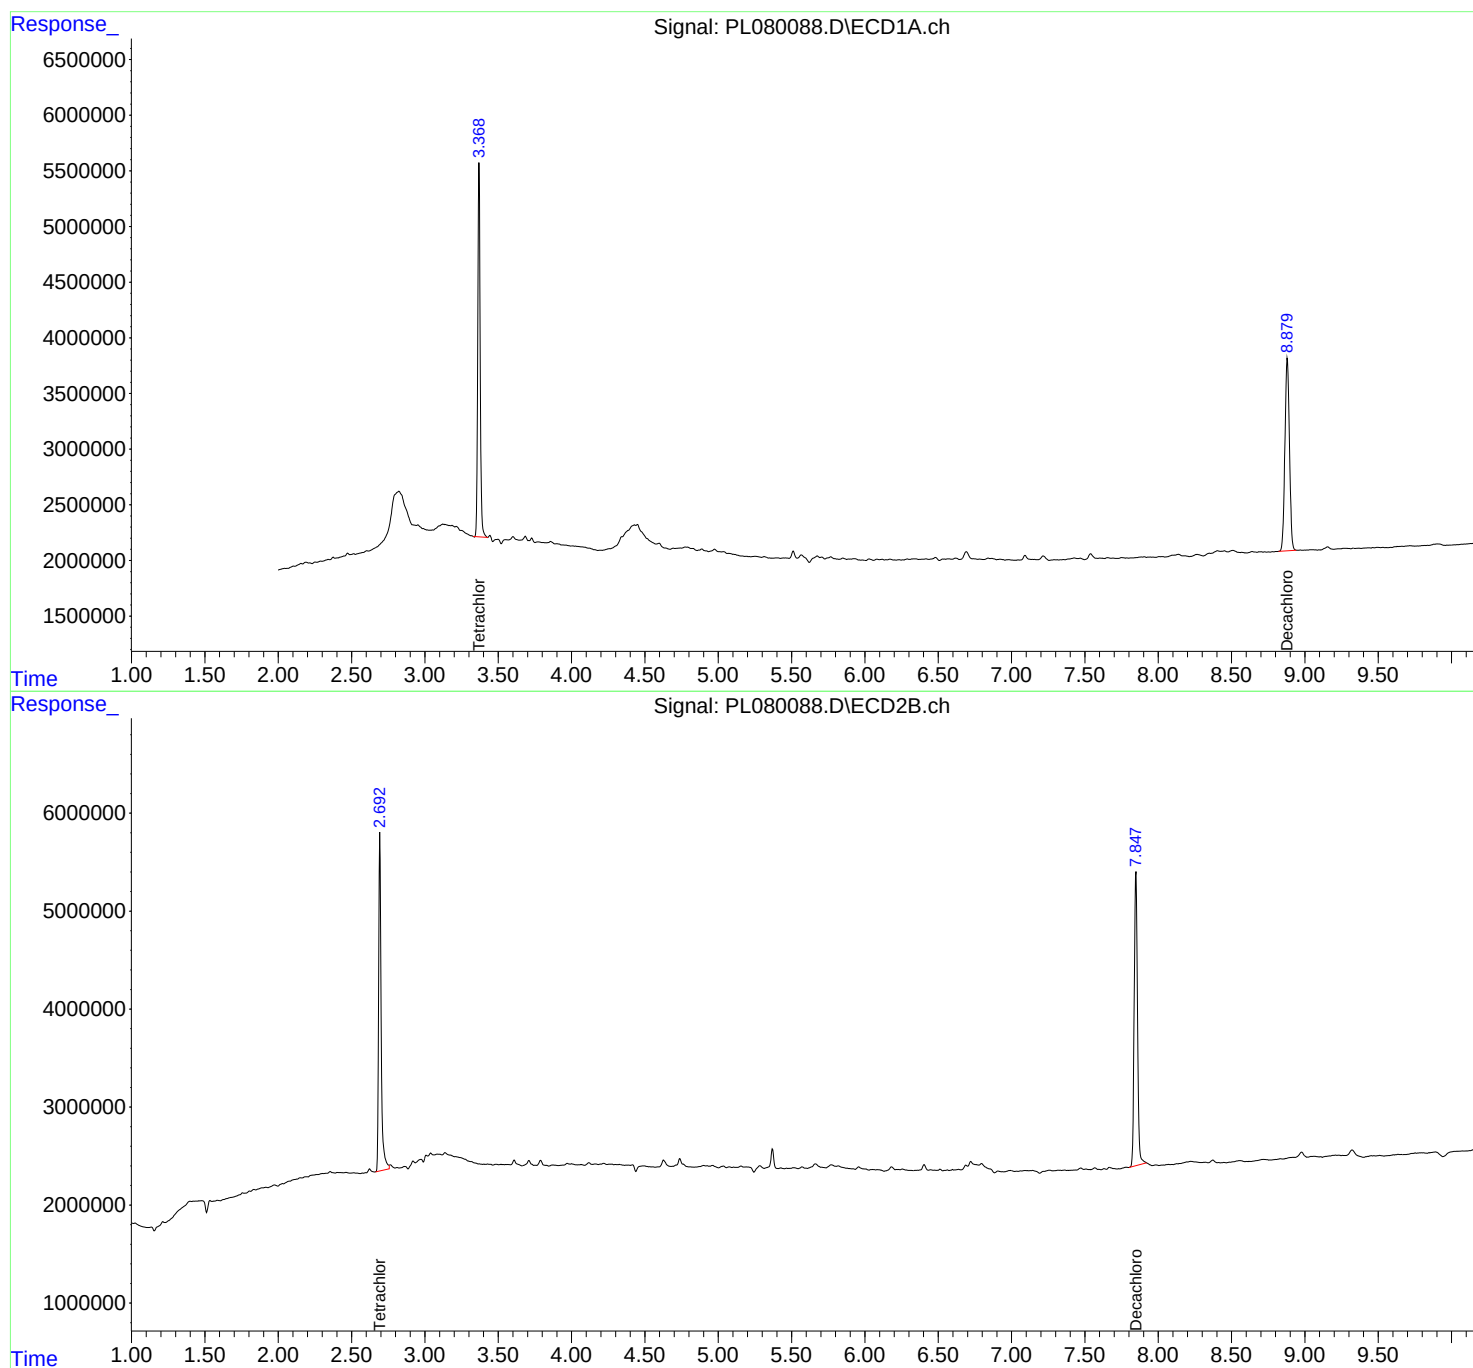


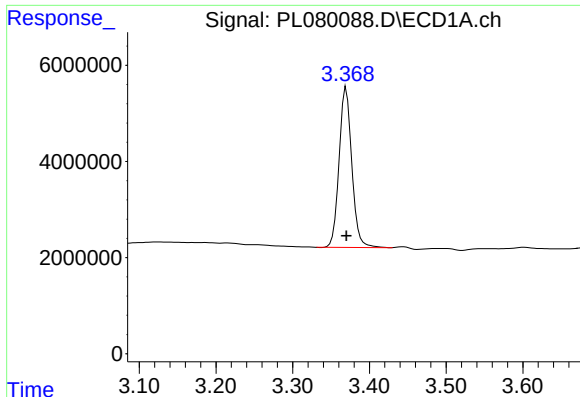

#1 Tetrachloro-m-xylene


R.T.: 3.370 min
Delta R.T.: 0.000 min
Response: 38262779
Conc: 19.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1S

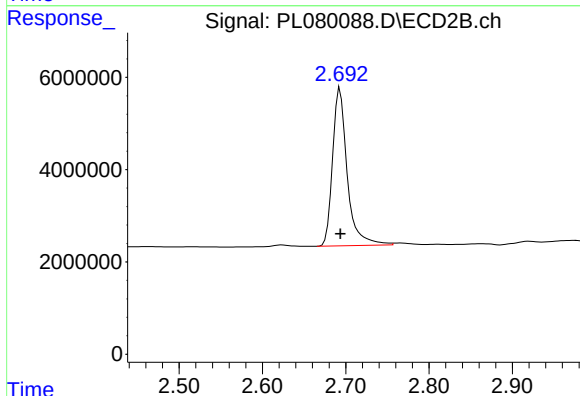


#1 Tetrachloro-m-xylene

R.T.: 2.693 min
Delta R.T.: 0.000 min
Response: 41850933
Conc: 18.41 ng/ml

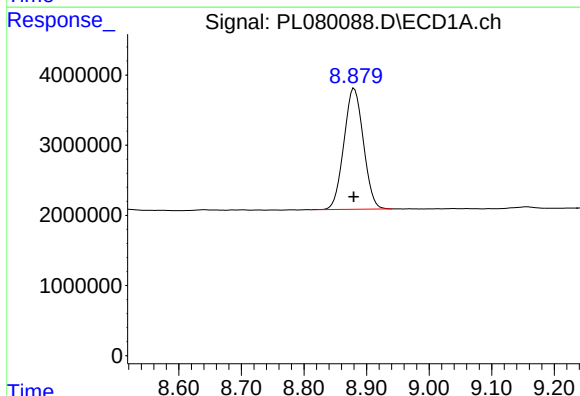

#28 Decachlorobiphenyl

R.T.: 8.880 min
Delta R.T.: 0.000 min
Response: 37401619
Conc: 21.80 ng/ml

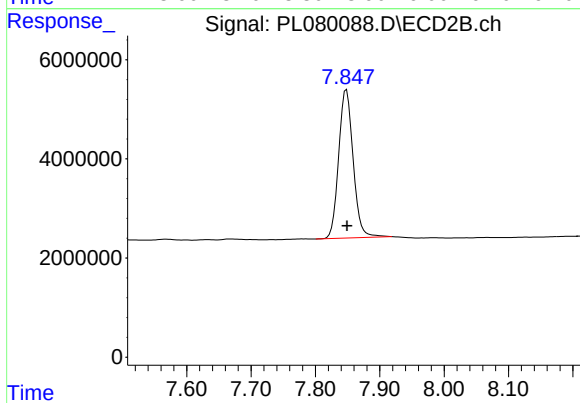

#28 Decachlorobiphenyl

R.T.: 7.848 min
Delta R.T.: 0.000 min
Response: 46976425
Conc: 20.79 ng/ml