

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010521\
 Data File : PL063925.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2021 12:31
 Operator : AR\AJ
 Sample : M1000-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 15:17:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.113	40449717	34131893	13.492	13.369
28)	SA Decachlor...	8.186	9.276	23677454	17353720	8.594	8.802
Target Compounds							
4)	MA Heptachlor	4.445	0.000	2707169	0	0.643	N.D. #
6)	B beta-BHC	0.000	4.996f	0	931768	N.D.	0.531 #
10)	B gamma-Chl...	5.377	6.258	5956270	8148678	1.567	2.945 #
11)	B alpha-Chl...	5.432	6.331	14017617	22911524	3.737	8.301 #
15)	B Endosulfa...	6.264	0.000	3314939	0	1.006	N.D. #
23)	Chlordane-1	4.308	5.126	11716705	4688147	114.330	53.684 #
25)	Chlordane-3	5.377	6.258	5956270	8148678	18.228	23.782 #
26)	Chlordane-4	5.432	6.331	14017617	22911524	52.390	55.741
27)	Chlordane-5	6.264	0.000	3314939	0	30.825	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010521\
Data File : PL063925.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2021 12:31
Operator : AR\AJ
Sample : M1000-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 15:17:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

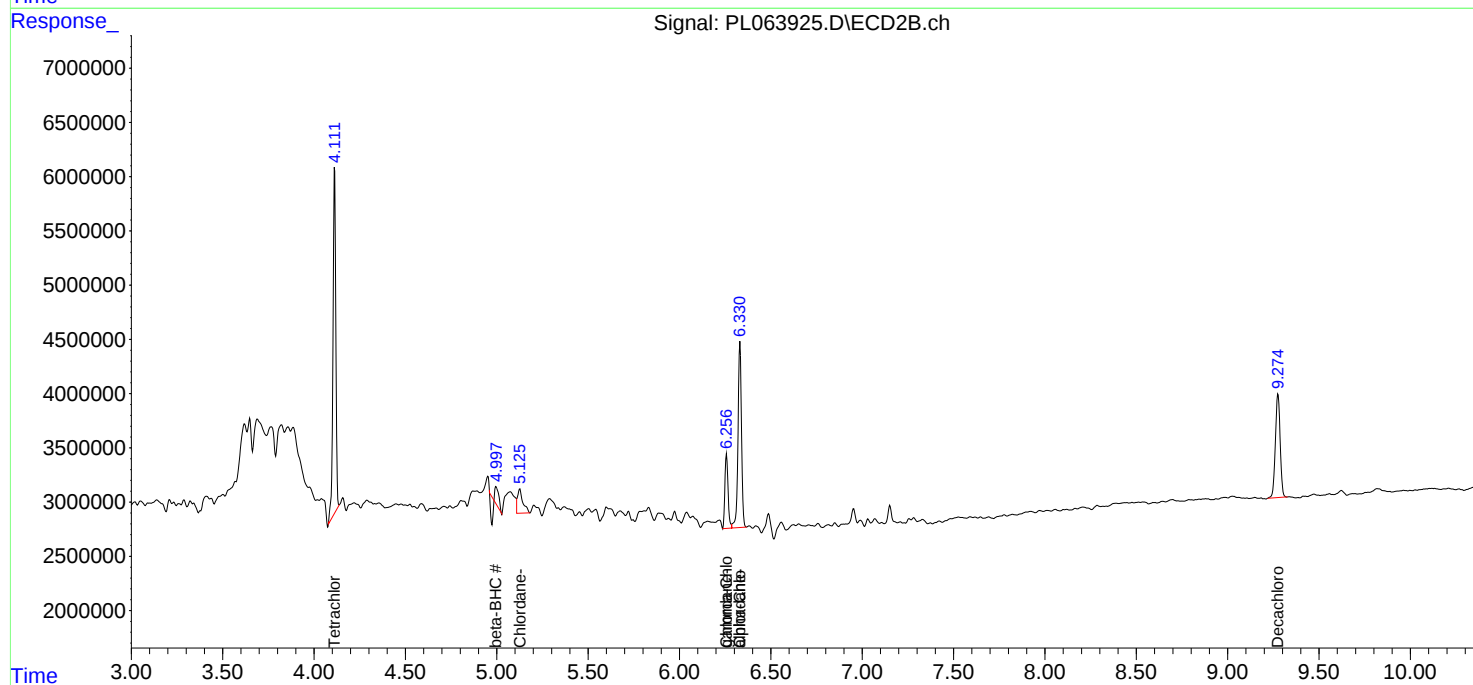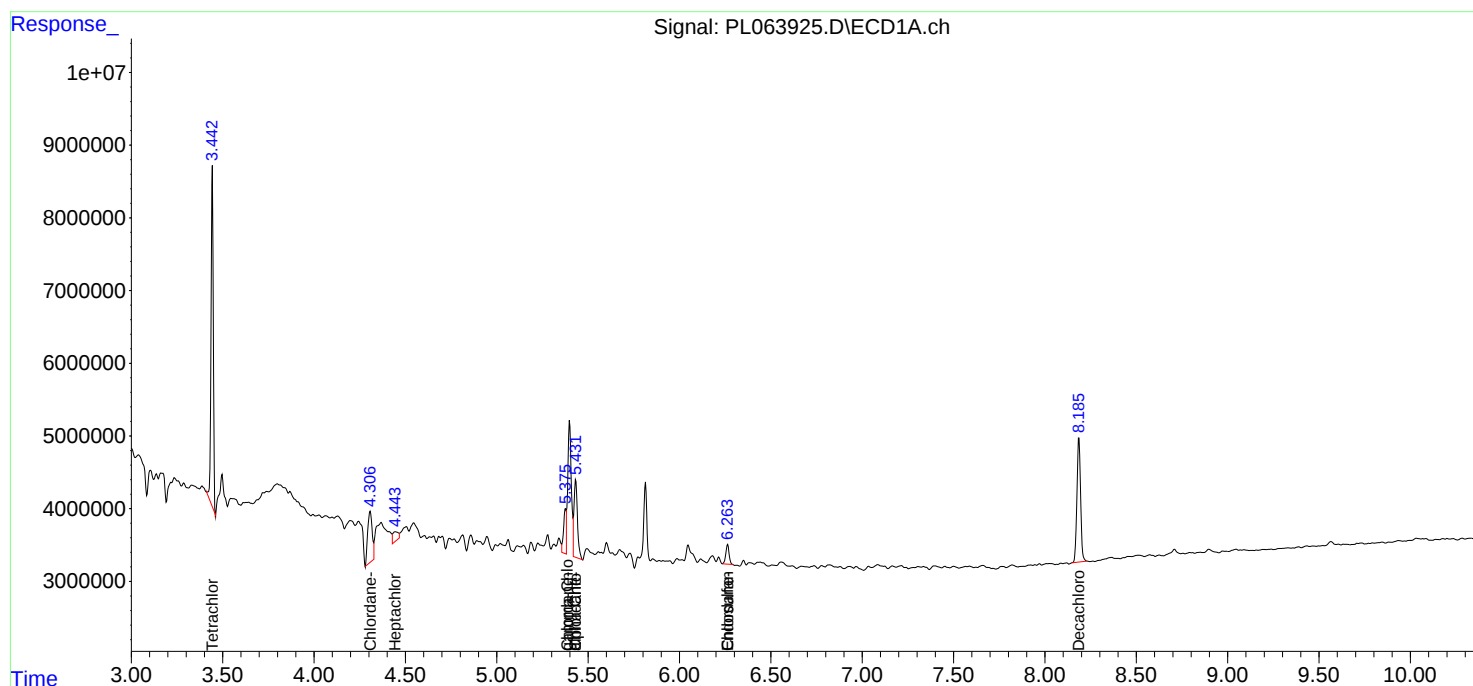


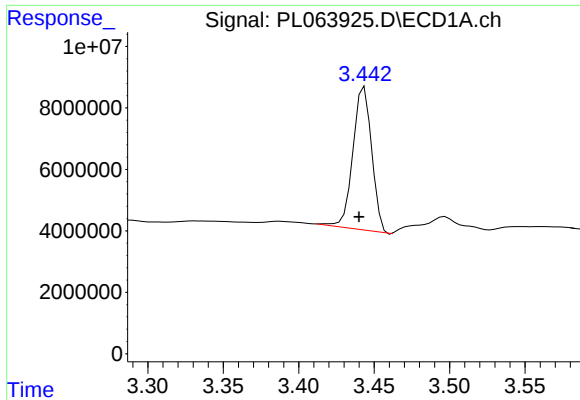

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: 0.004 min
Response: 40449717
Conc: 13.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

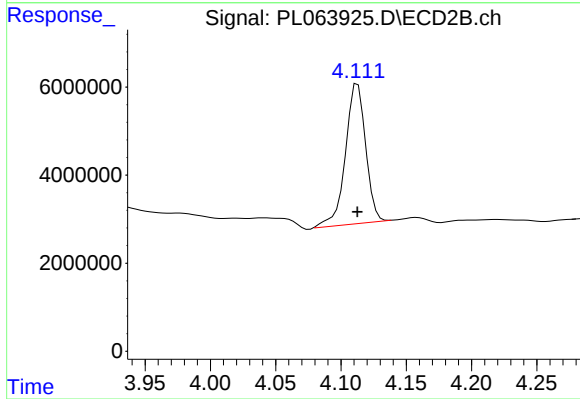


#1 Tetrachloro-m-xylene

R.T.: 4.113 min
Delta R.T.: 0.000 min
Response: 34131893
Conc: 13.37 ng/ml

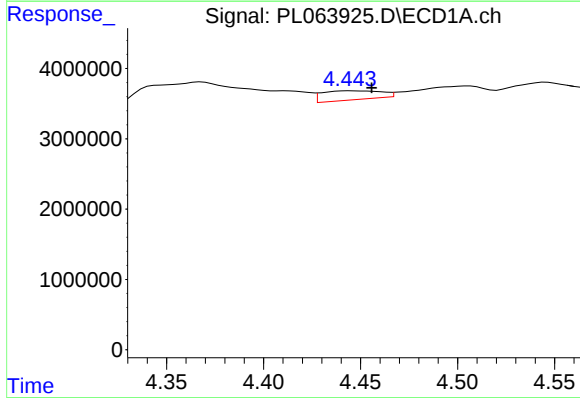


#4 Heptachlor

R.T.: 4.445 min
Delta R.T.: -0.011 min
Response: 2707169
Conc: 0.64 ng/ml

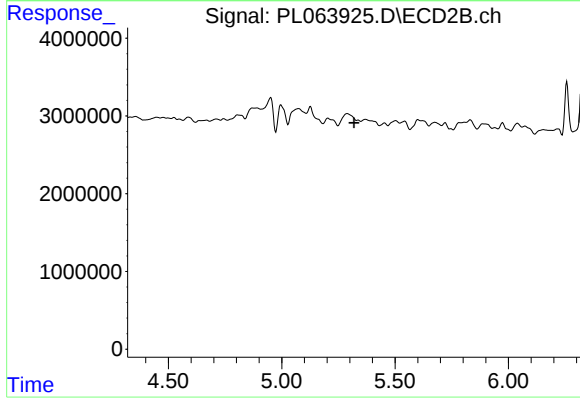

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.319 min
Response: 0
Conc: N.D.

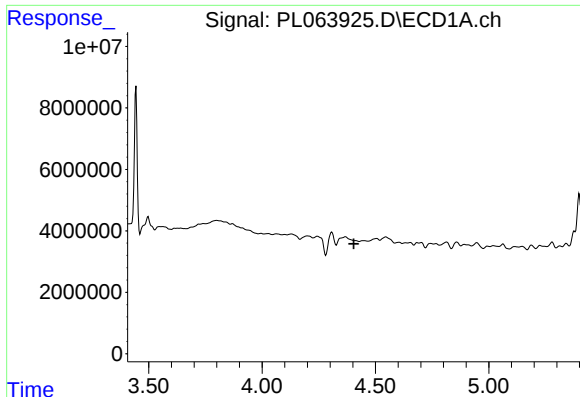

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.404 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

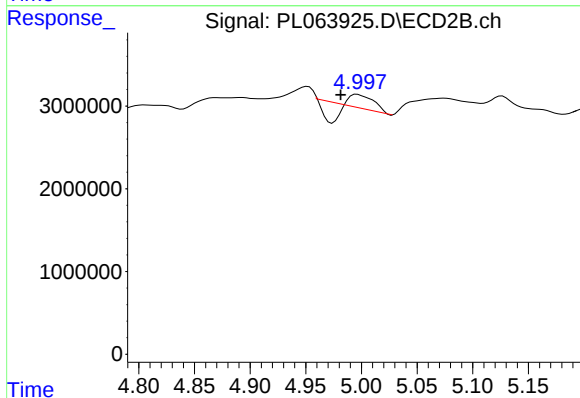


#6 beta-BHC

R.T.: 4.996 min
Delta R.T.: 0.015 min
Response: 931768
Conc: 0.53 ng/ml

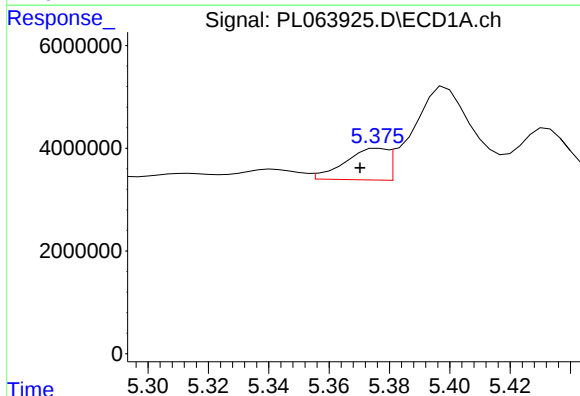


#10 gamma-Chlordane

R.T.: 5.377 min
Delta R.T.: 0.007 min
Response: 5956270
Conc: 1.57 ng/ml

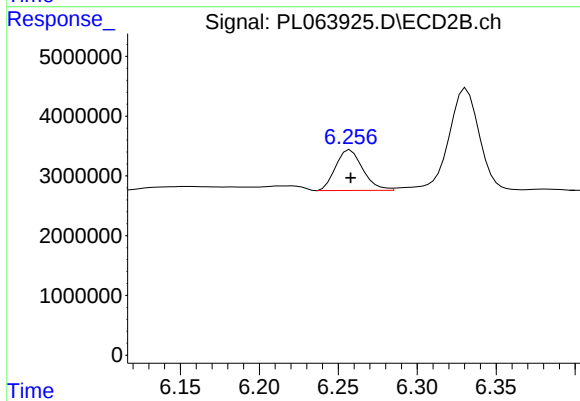

#10 gamma-Chlordane


R.T.: 6.258 min
Delta R.T.: 0.000 min
Response: 8148678
Conc: 2.95 ng/ml

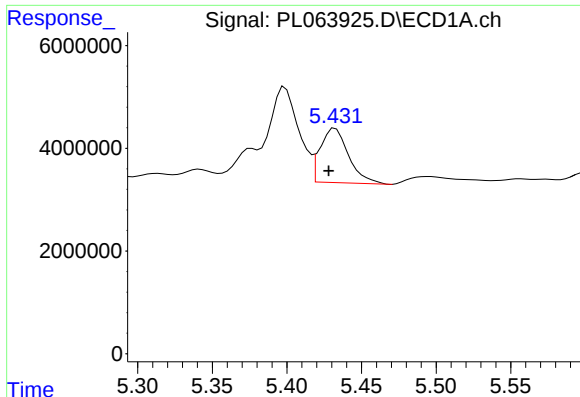

#11 alpha-Chlordane


R.T.: 5.432 min
Delta R.T.: 0.004 min
Response: 14017617
Conc: 3.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

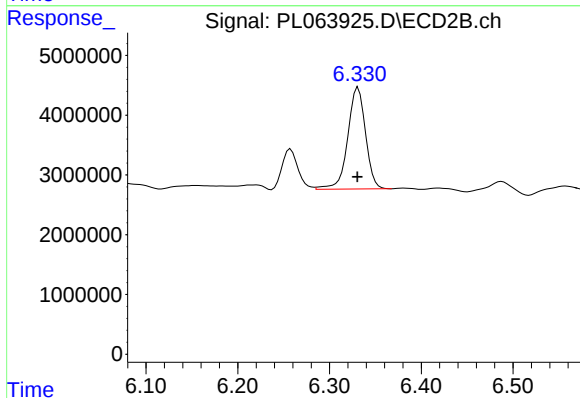


#11 alpha-Chlordane

R.T.: 6.331 min
Delta R.T.: 0.000 min
Response: 22911524
Conc: 8.30 ng/ml

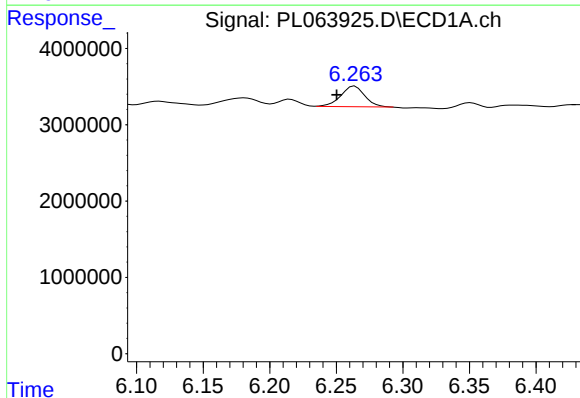


#15 Endosulfan II

R.T.: 6.264 min
Delta R.T.: 0.014 min
Response: 3314939
Conc: 1.01 ng/ml

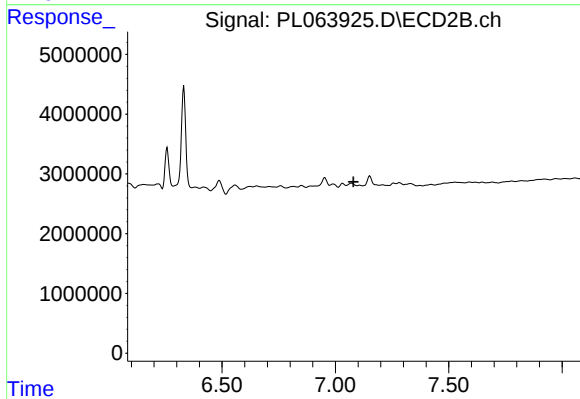

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 7.080 min
Response: 0
Conc: N.D.

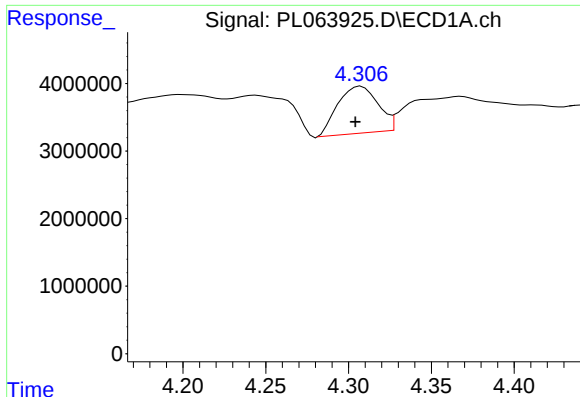

#23 Chlordane-1


R.T.: 4.308 min
Delta R.T.: 0.003 min
Response: 11716705
Conc: 114.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

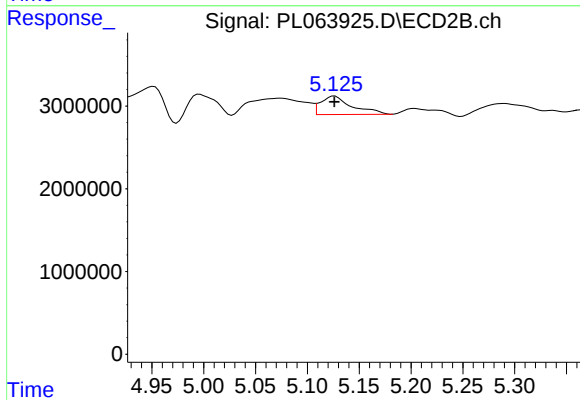


#23 Chlordane-1

R.T.: 5.126 min
Delta R.T.: 0.000 min
Response: 4688147
Conc: 53.68 ng/ml

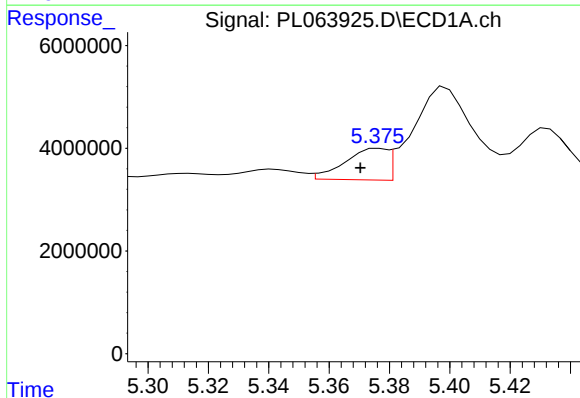


#25 Chlordane-3

R.T.: 5.377 min
Delta R.T.: 0.007 min
Response: 5956270
Conc: 18.23 ng/ml

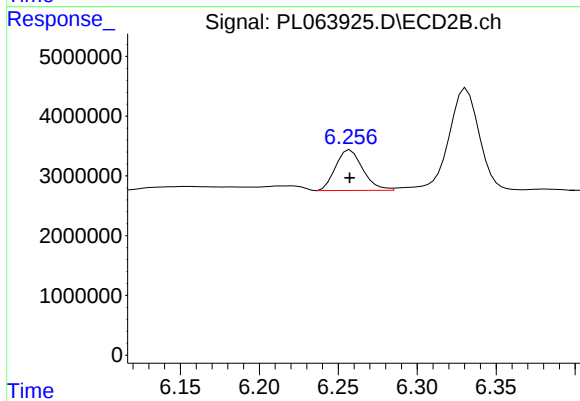

#25 Chlordane-3


R.T.: 6.258 min
Delta R.T.: 0.000 min
Response: 8148678
Conc: 23.78 ng/ml

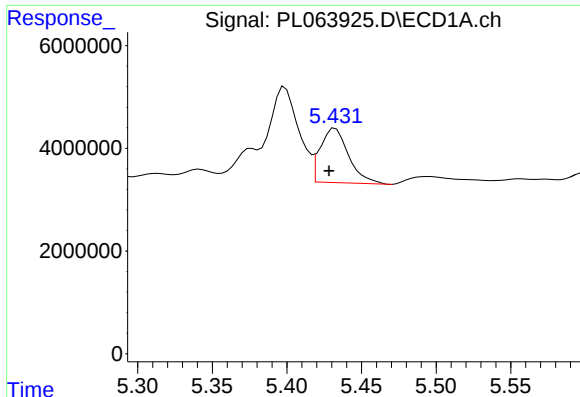

#26 Chlordane-4


R.T.: 5.432 min
Delta R.T.: 0.004 min
Response: 14017617
Conc: 52.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

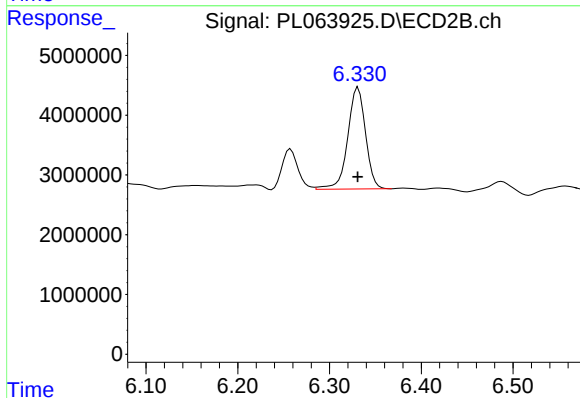


#26 Chlordane-4

R.T.: 6.331 min
Delta R.T.: 0.000 min
Response: 22911524
Conc: 55.74 ng/ml

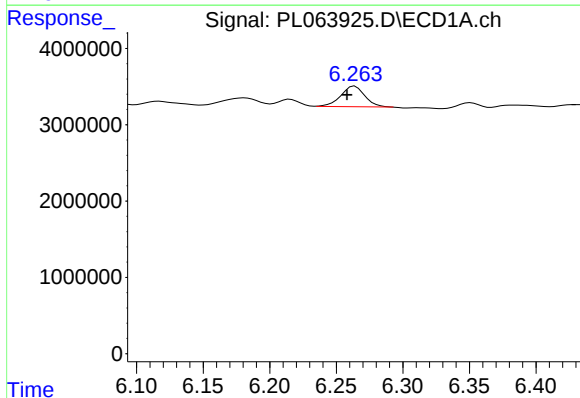


#27 Chlordane-5

R.T.: 6.264 min
Delta R.T.: 0.006 min
Response: 3314939
Conc: 30.83 ng/ml

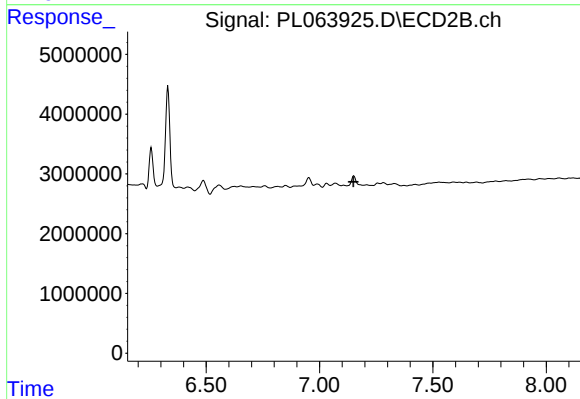

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 7.150 min
Response: 0
Conc: N.D.

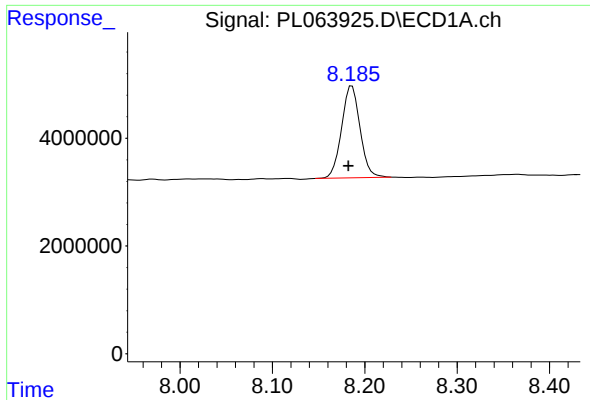

#28 Decachlorobiphenyl

R.T.: 8.186 min
Delta R.T.: 0.004 min
Response: 23677454
Conc: 8.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

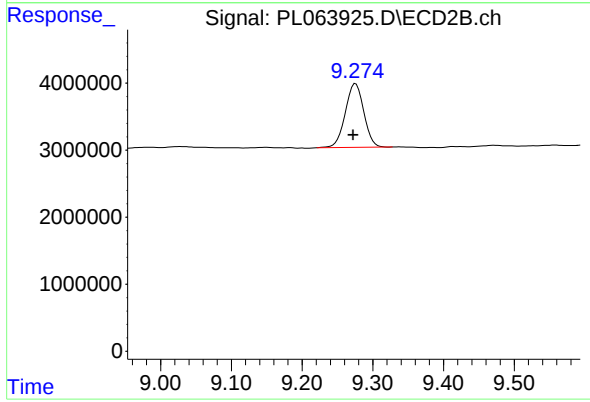

#28 Decachlorobiphenyl

R.T.: 9.276 min
Delta R.T.: 0.004 min
Response: 17353720
Conc: 8.80 ng/ml