

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010521\
 Data File : PL063930.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2021 13:42
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 15:18:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	4.112	59606814	47988519	19.882	18.797
28)	SA Decachlor...	8.177	9.272	47908052	30549918	17.389	15.495
Target Compounds							
6)	B beta-BHC	0.000	4.990	0	3985077	N.D.	2.270 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010521\
Data File : PL063930.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2021 13:42
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 15:18:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

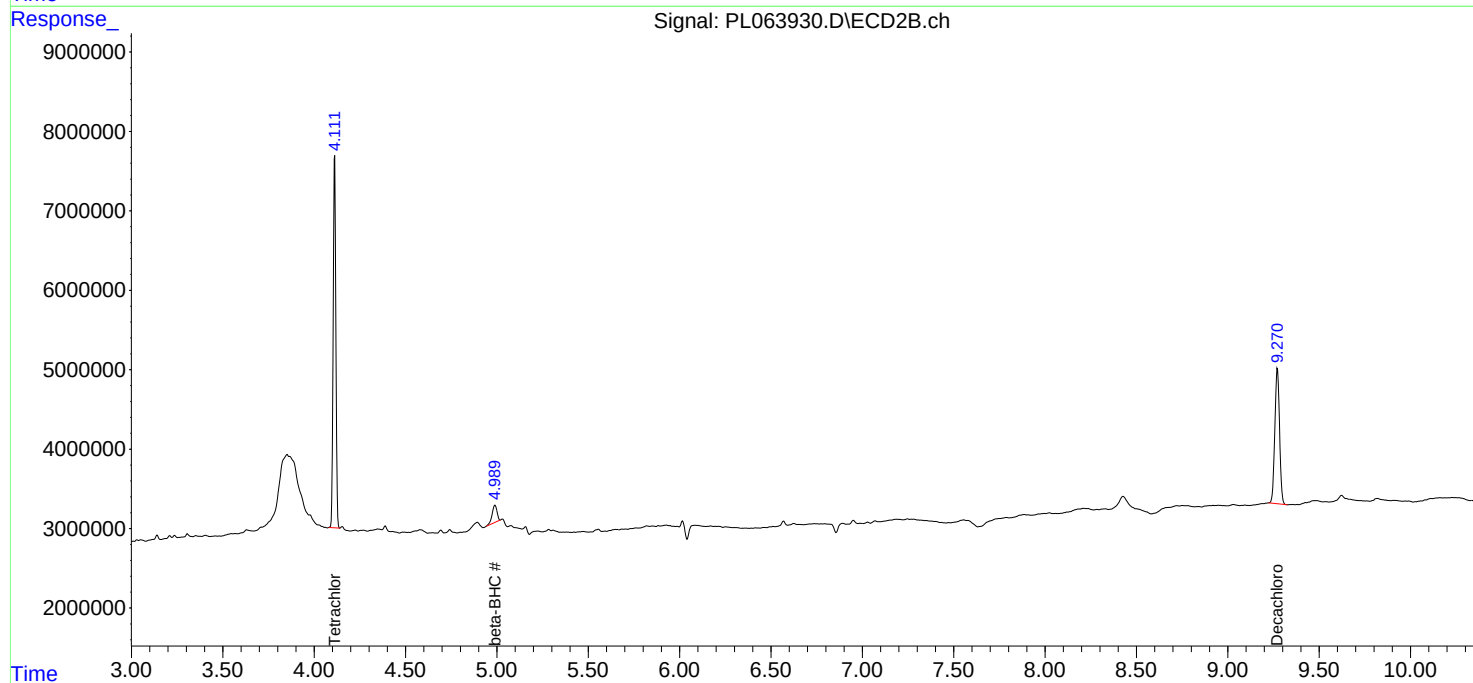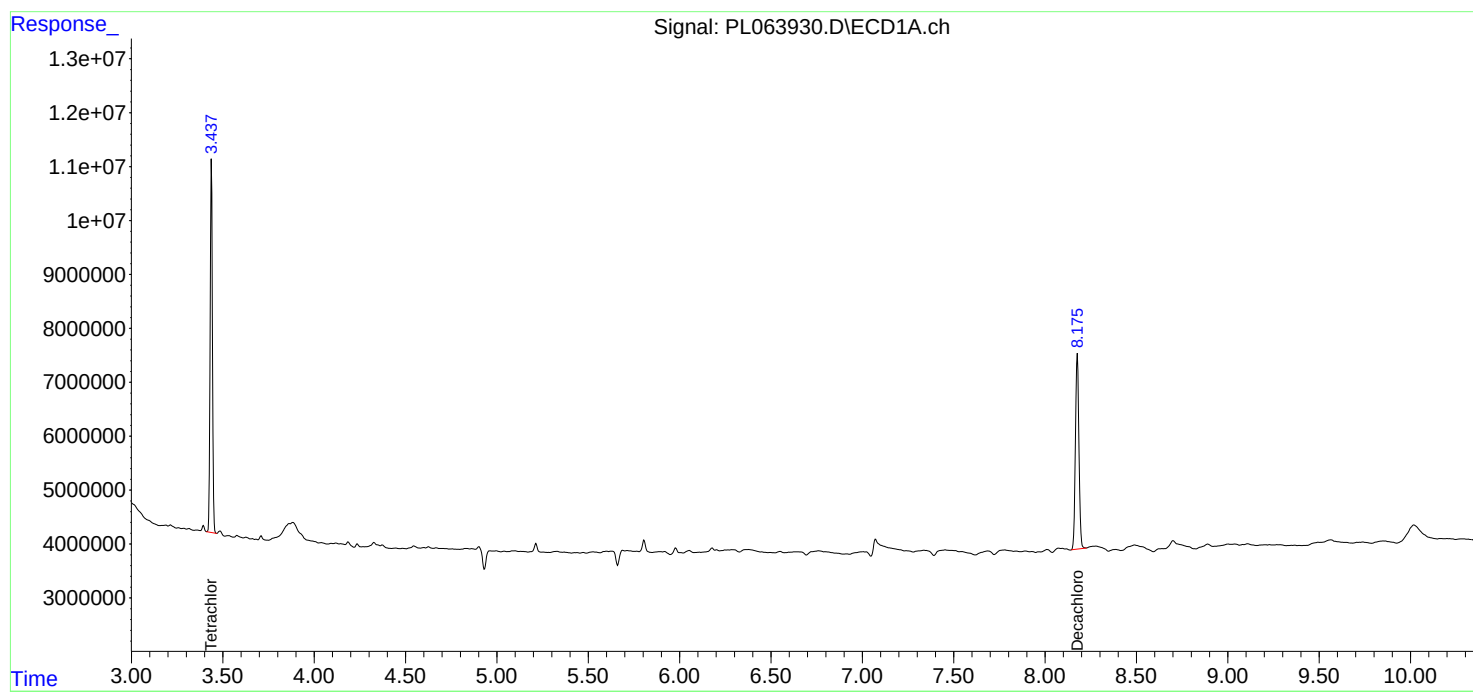


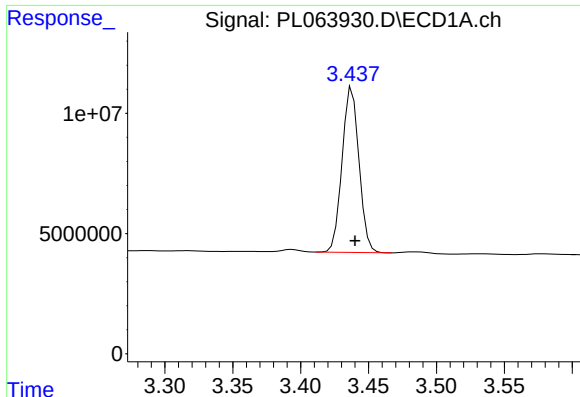

#1 Tetrachloro-m-xylene


R.T.: 3.438 min
Delta R.T.: -0.002 min
Response: 59606814
Conc: 19.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

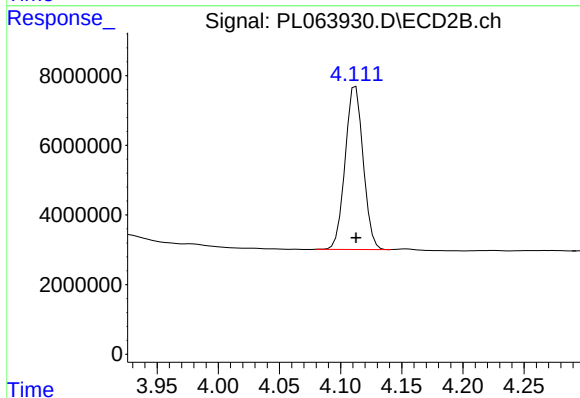


#1 Tetrachloro-m-xylene

R.T.: 4.112 min
Delta R.T.: 0.000 min
Response: 47988519
Conc: 18.80 ng/ml

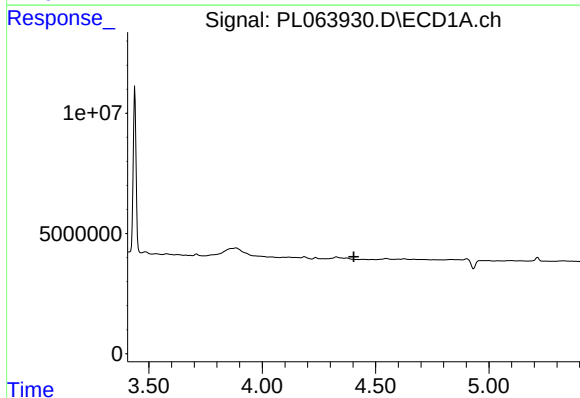


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.404 min
Response: 0
Conc: N.D.

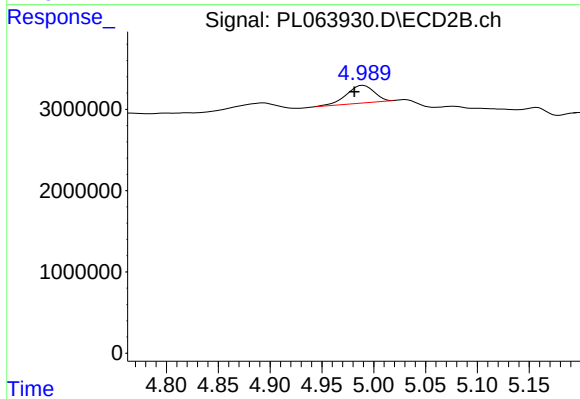

#6 beta-BHC


R.T.: 4.990 min
Delta R.T.: 0.009 min
Response: 3985077
Conc: 2.27 ng/ml

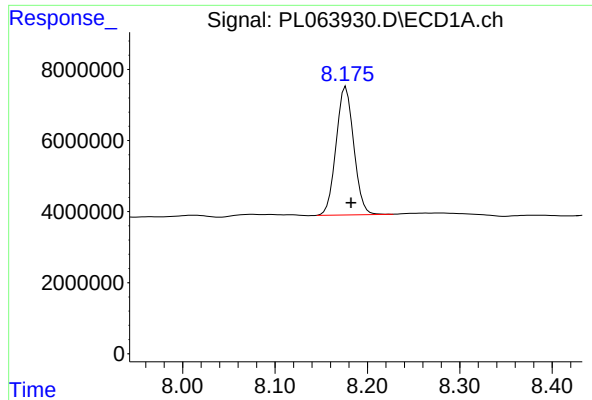

#28 Decachlorobiphenyl

R.T.: 8.177 min
Delta R.T.: -0.006 min
Response: 47908052
Conc: 17.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

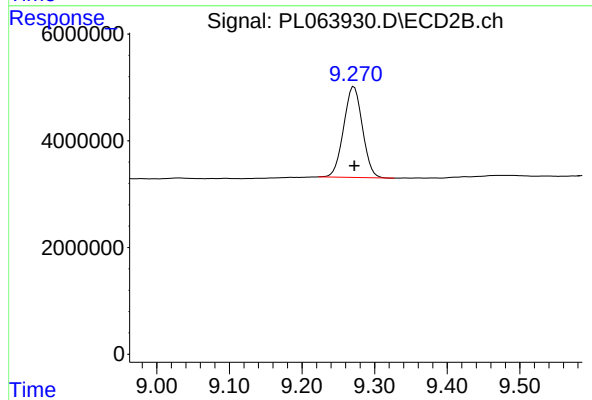

#28 Decachlorobiphenyl

R.T.: 9.272 min
Delta R.T.: 0.000 min
Response: 30549918
Conc: 15.49 ng/ml