

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010521\
 Data File : PL063929.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2021 13:27
 Operator : AR\AJ
 Sample : M1007-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 R-LA-22-1-WC

Manual Integrations
 APPROVED

Ankita
 1/6/2021 10:08:19 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 15:18:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 22 14:02:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	4.111	56169448	43469096	18.736	17.026m
28)	SA Decachlor...	8.177	9.272	21788170	13742237	7.908	6.970

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010521\
Data File : PL063929.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2021 13:27
Operator : AR\AJ
Sample : M1007-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
R-LA-22-1-WC


Manual Integrations
APPROVED

Ankita
1/6/2021 10:08:19 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 15:18:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122220.M
Quant Title : GC Extractables
QLast Update : Tue Dec 22 14:02:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

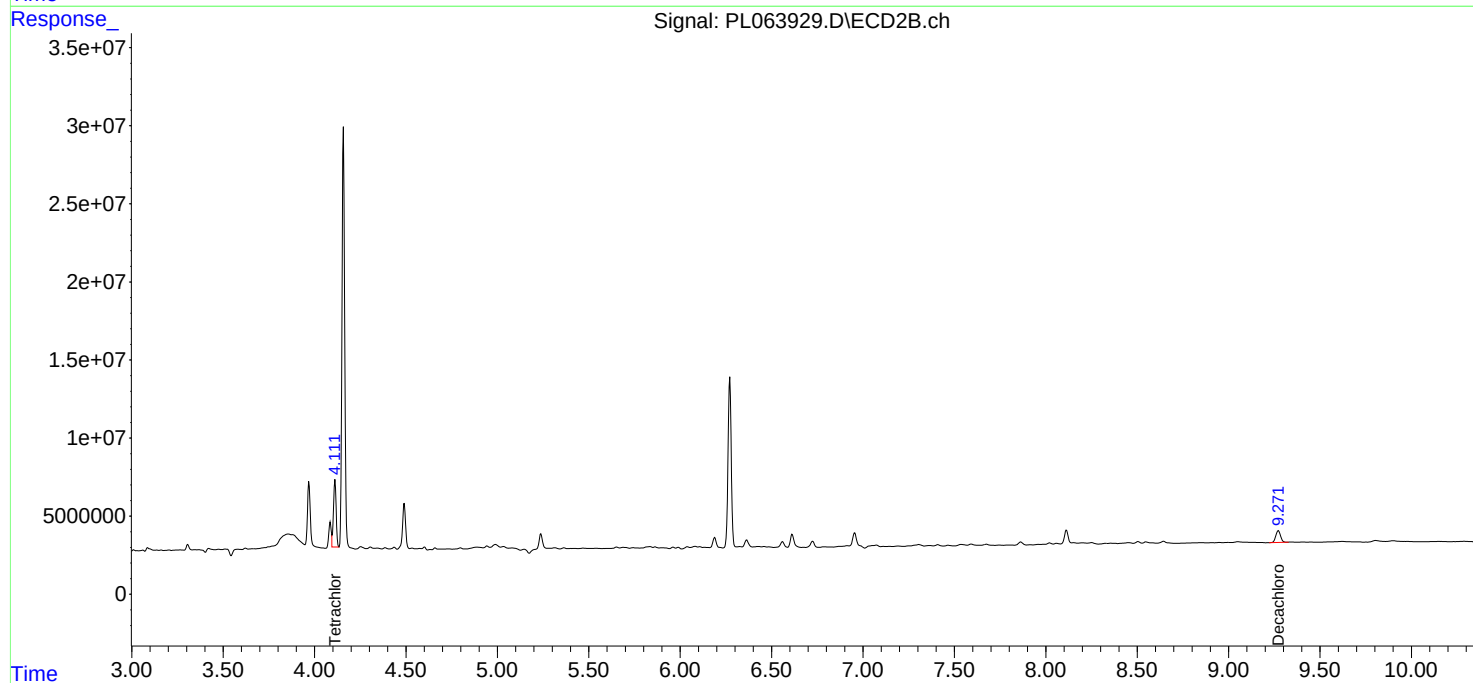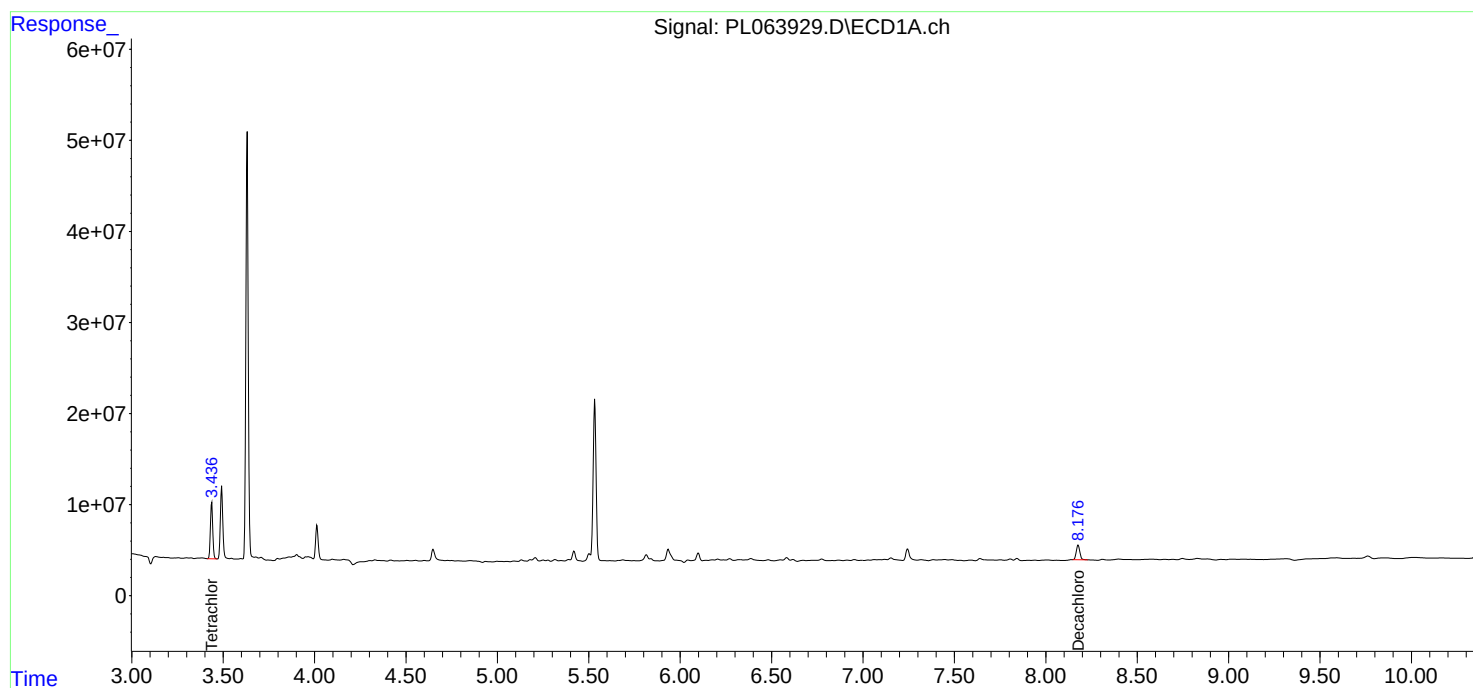

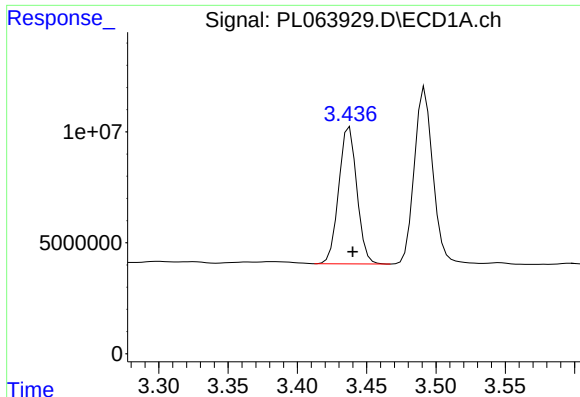


#1 Tetrachloro-m-xylene

R.T.: 3.438 min
Delta R.T.: -0.002 min
Response: 56169448
Conc: 18.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
R-LA-22-1-WC


Manual Integrations
APPROVED

Ankita
1/6/2021 10:08:19 AM

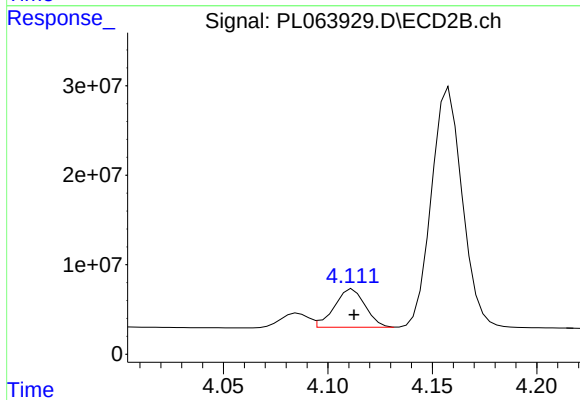


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: -0.002 min
Response: 43469096
Conc: 17.03 ng/ml m

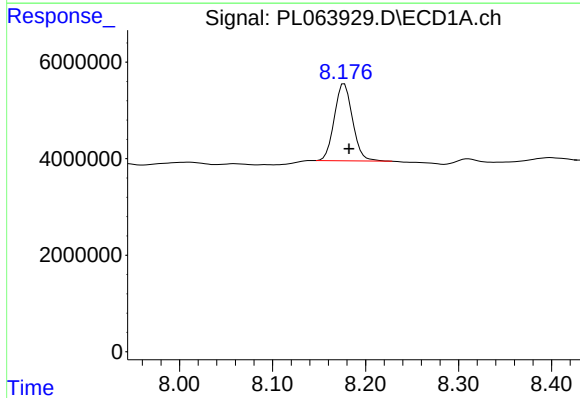

#28 Decachlorobiphenyl

R.T.: 8.177 min
Delta R.T.: -0.005 min
Response: 21788170
Conc: 7.91 ng/ml

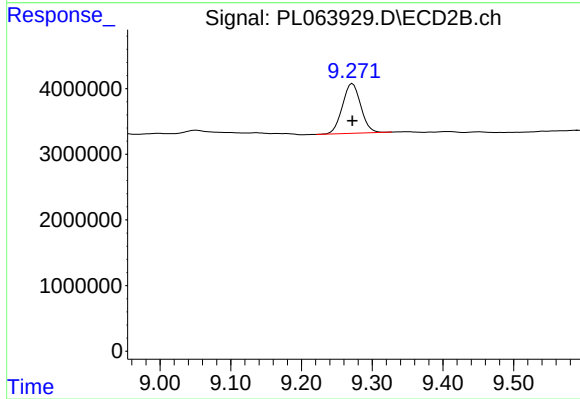

#28 Decachlorobiphenyl

R.T.: 9.272 min
Delta R.T.: 0.000 min
Response: 13742237
Conc: 6.97 ng/ml