

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010522\
 Data File : PL071817.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2022 14:03
 Operator : AR\AJ
 Sample : PB141850BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 06 00:39:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 05 01:51:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.559	5.494	9128528	24961498	19.761	20.316
28)	SA Decachlor...	10.321	11.388	15043980	25076941	20.807	21.162
Target Compounds							
5)	MB Aldrin	0.000	7.466f	0	145142	N.D.	0.094 #
7)	B delta-BHC	0.000	7.019f	0	1855823	N.D.	1.209 #
10)	B gamma-Chl...	0.000	8.211	0	166030	N.D.	0.121 #
11)	B alpha-Chl...	0.000	8.321f	0	92366	N.D.	0.069 #
15)	B Endosulfa...	0.000	9.146f	0	408718	N.D.	0.364 #
19)	B Endosulfa...	0.000	9.496	0	176340	N.D.	0.170 #
24)	Chlordane-2	0.000	7.466	0	145142	N.D.	2.681 #
25)	Chlordane-3	0.000	8.235	0	116985	N.D.	0.573 #
26)	Chlordane-4	0.000	8.321f	0	92366	N.D.	0.379 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010522\
Data File : PL071817.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2022 14:03
Operator : AR\AJ
Sample : PB141850BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 06 00:39:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Wed Jan 05 01:51:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

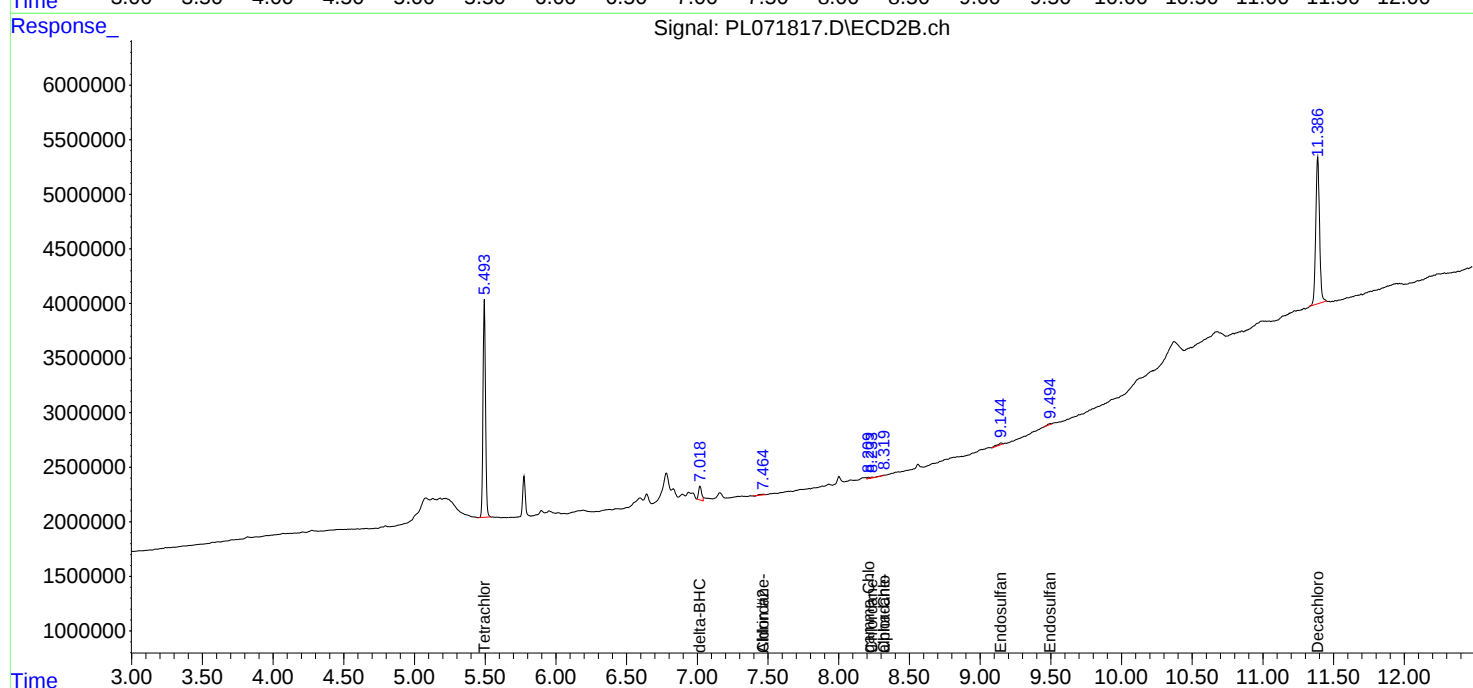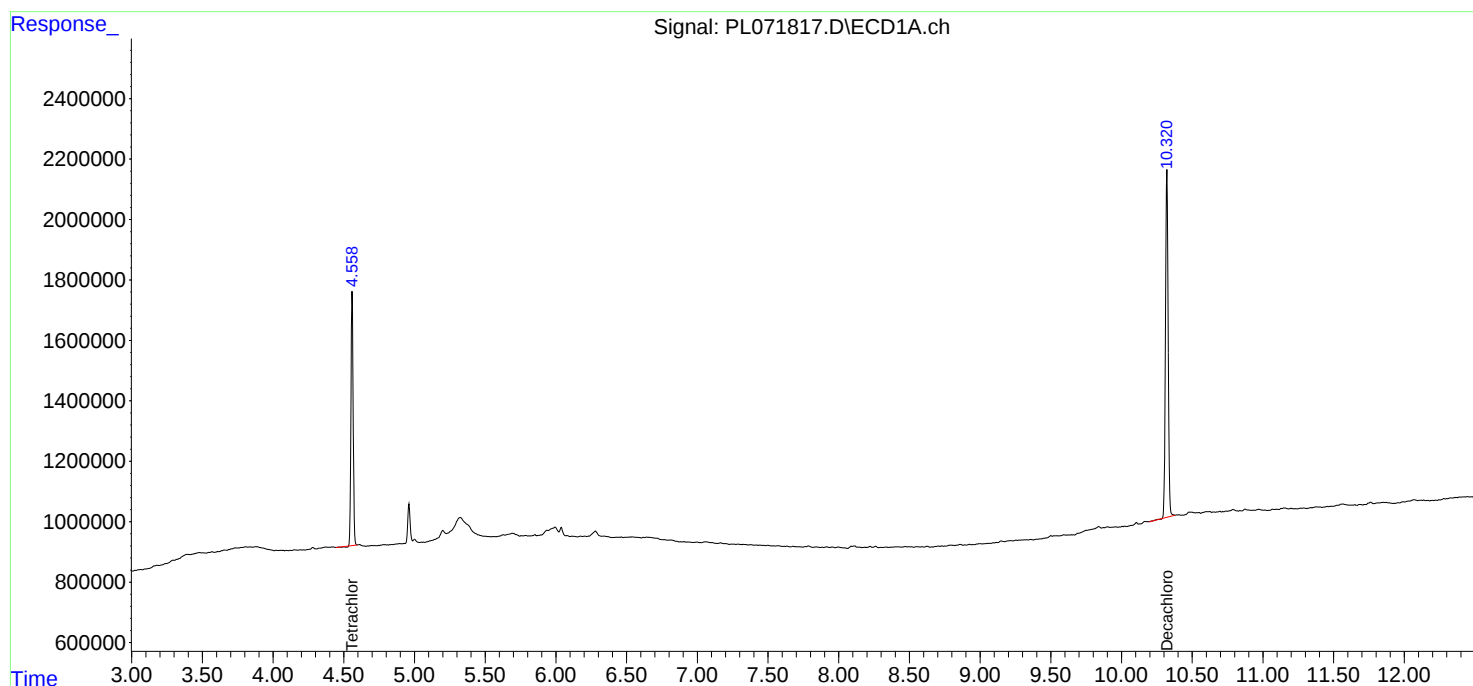


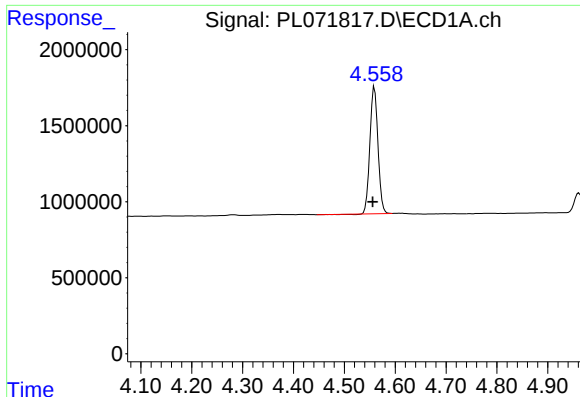

#1 Tetrachloro-m-xylene


R.T.: 4.559 min
Delta R.T.: 0.003 min
Response: 9128528
Conc: 19.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

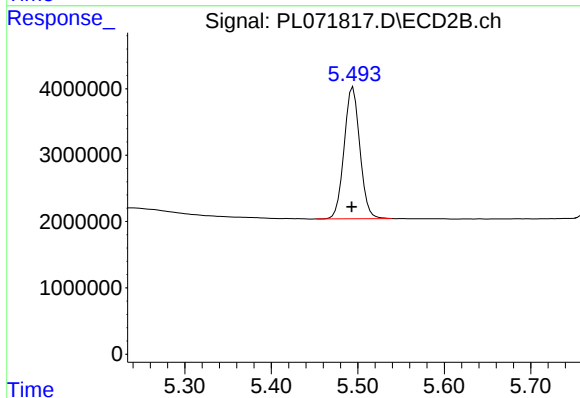


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.001 min
Response: 24961498
Conc: 20.32 ng/ml

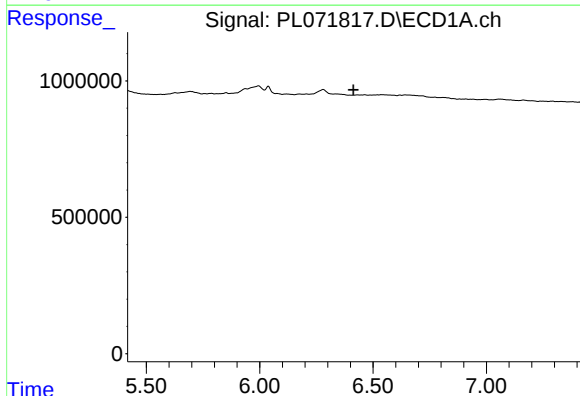


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 6.414 min
Response: 0
Conc: N.D.

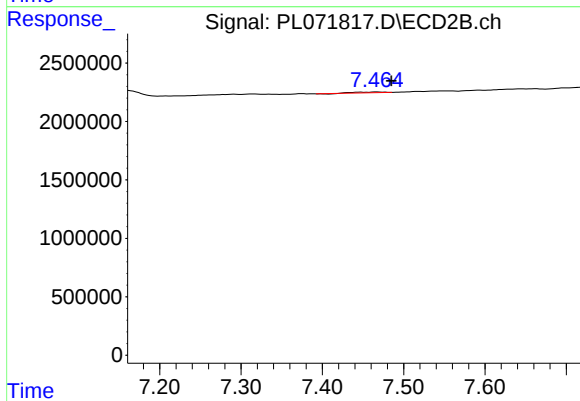

#5 Aldrin


R.T.: 7.466 min
Delta R.T.: -0.019 min
Response: 145142
Conc: 0.09 ng/ml

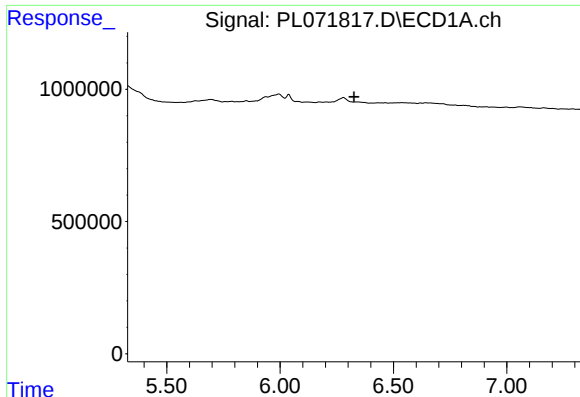

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.327 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

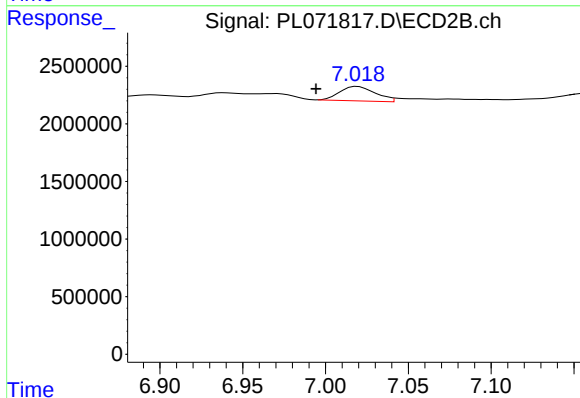


#7 delta-BHC

R.T.: 7.019 min
Delta R.T.: 0.025 min
Response: 1855823
Conc: 1.21 ng/ml

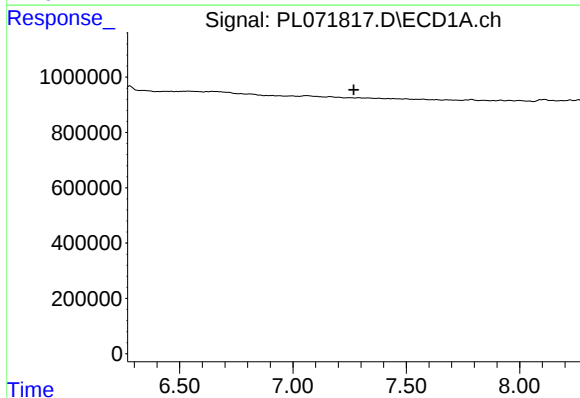


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

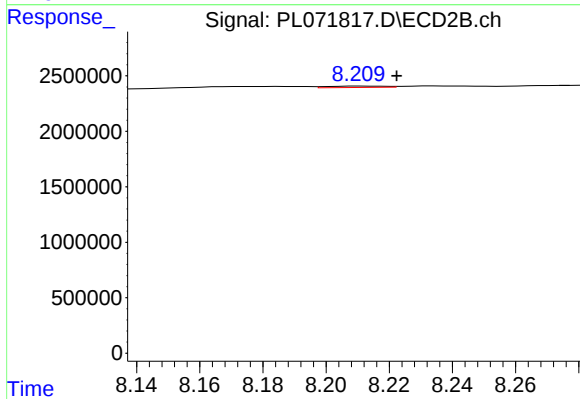

#10 gamma-Chlordane


R.T.: 8.211 min
Delta R.T.: -0.011 min
Response: 166030
Conc: 0.12 ng/ml

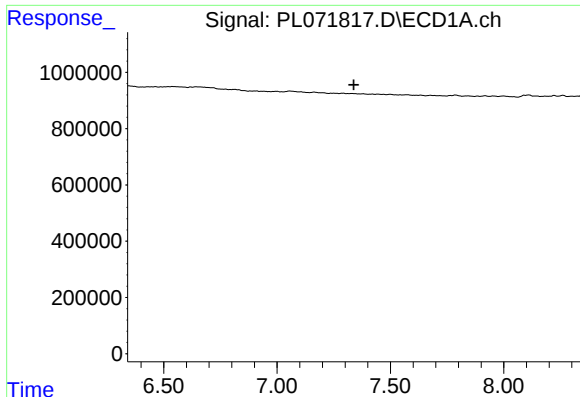

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.338 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

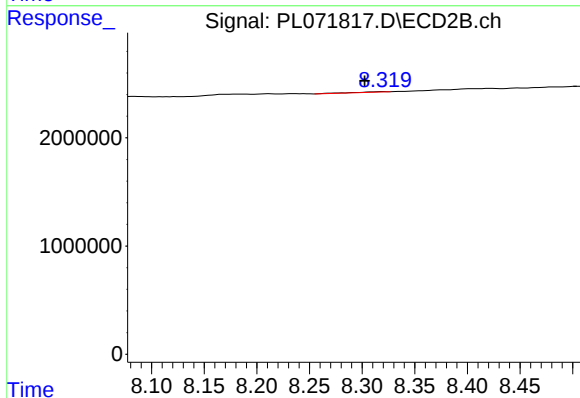


#11 alpha-Chlordane

R.T.: 8.321 min
Delta R.T.: 0.018 min
Response: 92366
Conc: 0.07 ng/ml

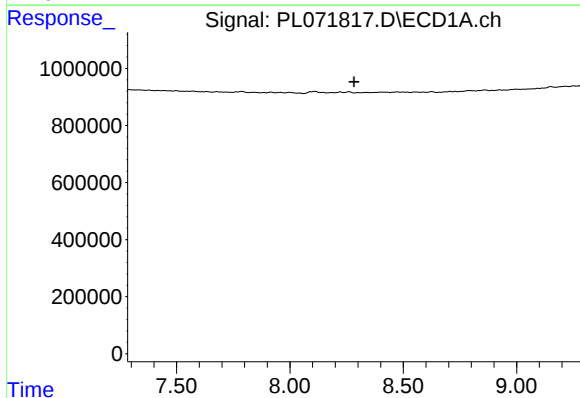


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.283 min
Response: 0
Conc: N.D.

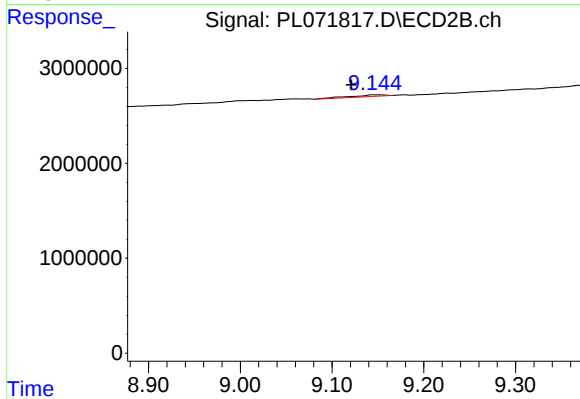

#15 Endosulfan II


R.T.: 9.146 min
Delta R.T.: 0.025 min
Response: 408718
Conc: 0.36 ng/ml

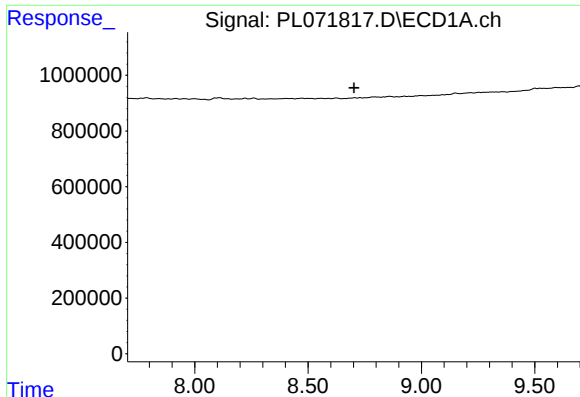

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 8.703 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

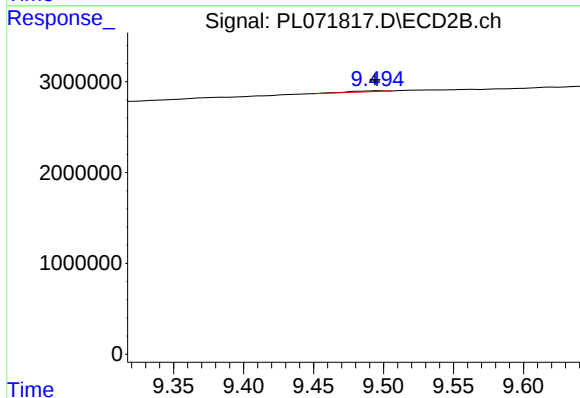


#19 Endosulfan Sulfate

R.T.: 9.496 min
Delta R.T.: 0.002 min
Response: 176340
Conc: 0.17 ng/ml

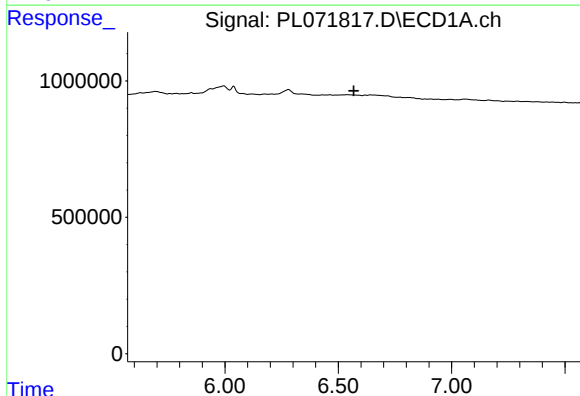


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 6.569 min
Response: 0
Conc: N.D.

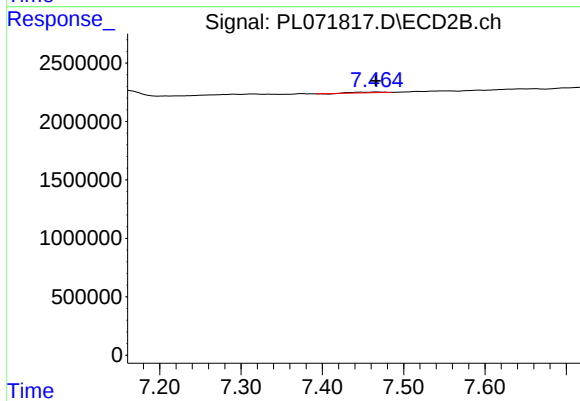

#24 Chlordane-2


R.T.: 7.466 min
Delta R.T.: 0.000 min
Response: 145142
Conc: 2.68 ng/ml

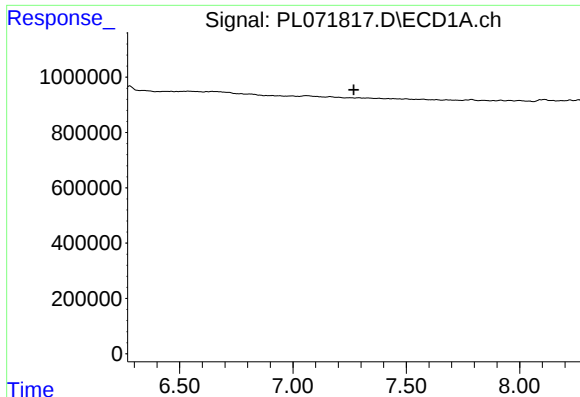

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

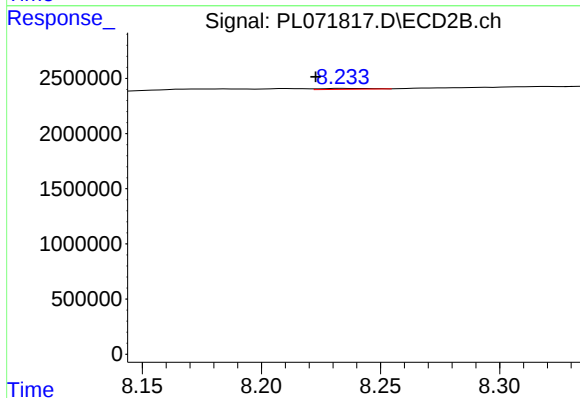


#25 Chlordane-3

R.T.: 8.235 min
Delta R.T.: 0.012 min
Response: 116985
Conc: 0.57 ng/ml

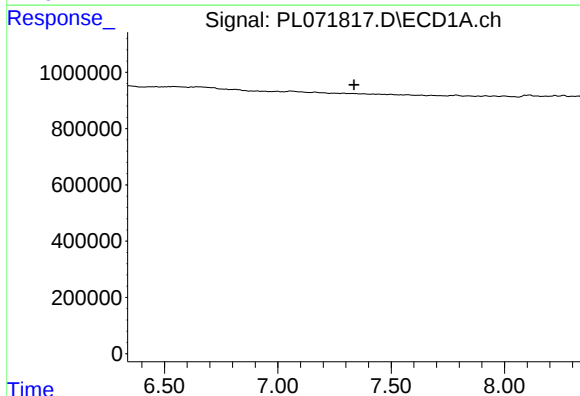


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.337 min
Response: 0
Conc: N.D.

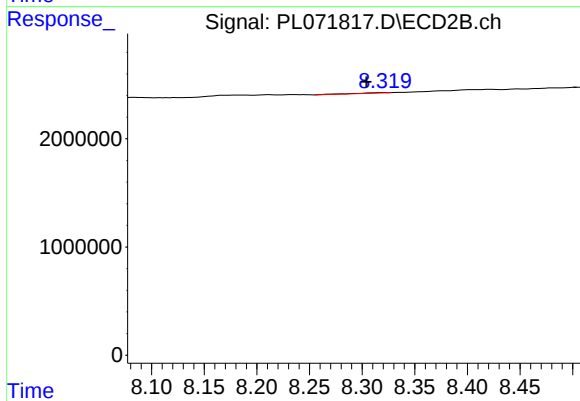

#26 Chlordane-4


R.T.: 8.321 min
Delta R.T.: 0.016 min
Response: 92366
Conc: 0.38 ng/ml

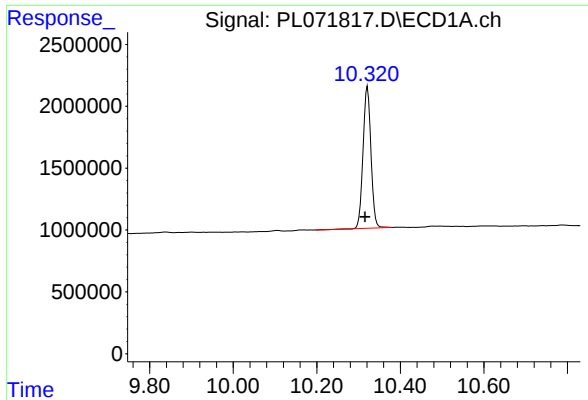

#28 Decachlorobiphenyl

R.T.: 10.321 min
Delta R.T.: 0.006 min
Response: 15043980
Conc: 20.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

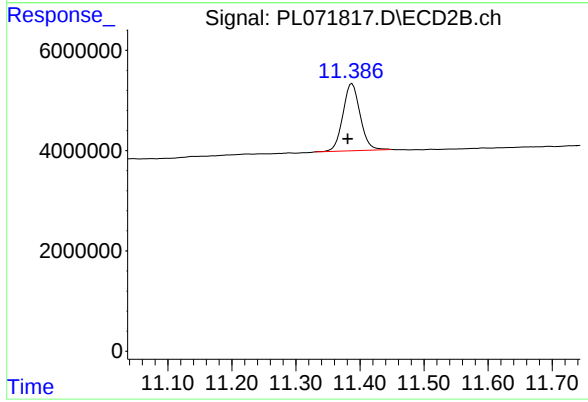

#28 Decachlorobiphenyl

R.T.: 11.388 min
Delta R.T.: 0.007 min
Response: 25076941
Conc: 21.16 ng/ml