

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010522\
 Data File : PL071826.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2022 17:21
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 06 00:41:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 05 01:51:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.557	5.494	9536299	25171364	20.644	20.487
28)	SA Decachlor...	10.318	11.386	14736645	24035152	20.382	20.283
Target Compounds							
8)	B Heptachlo...	0.000	7.963	0	9573028	N.D.	6.851 #
9)	A Endosulfan I	0.000	8.383f	0	851014	N.D.	0.687 #
10)	B gamma-Chl...	0.000	8.222	0	3948672	N.D.	2.888 #
11)	B alpha-Chl...	0.000	8.323f	0	2288756	N.D.	1.720 #
13)	MA Dieldrin	7.696f	0.000	1401741	0	2.324	N.D. #
14)	MA Endrin	7.999f	0.000	1153003	0	2.182	N.D. #
15)	B Endosulfa...	0.000	9.102f	0	270200	N.D.	0.241 #
16)	A 4,4'-DDD	0.000	9.047	0	86309	N.D.	0.090 #
17)	MA 4,4'-DDT	0.000	9.370f	0	964297	N.D.	1.023 #
18)	B Endrin al...	0.000	9.284f	0	472387	N.D.	0.557 #
25)	Chlordane-3	0.000	8.222	0	3948672	N.D.	19.346 #
26)	Chlordane-4	0.000	8.323f	0	2288756	N.D.	9.403 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010522\
Data File : PL071826.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2022 17:21
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 06 00:41:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Wed Jan 05 01:51:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

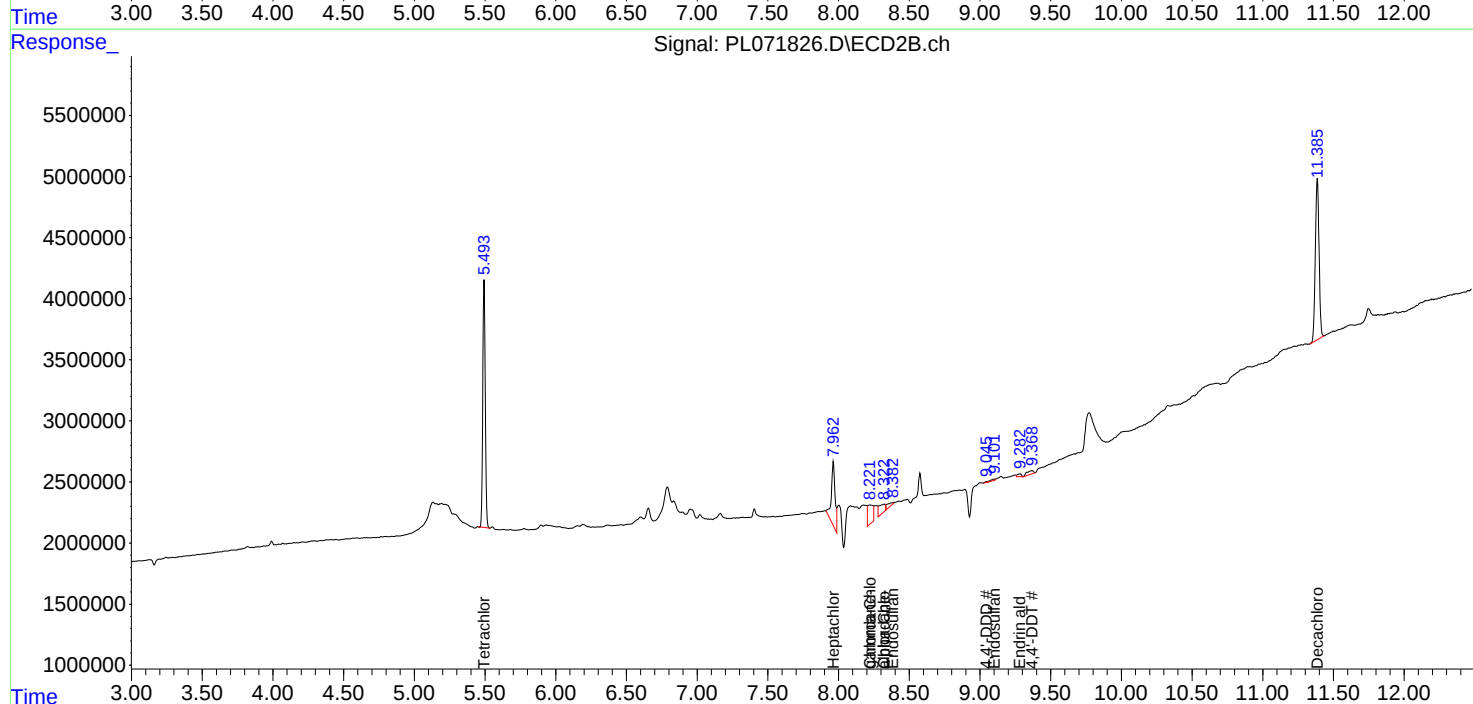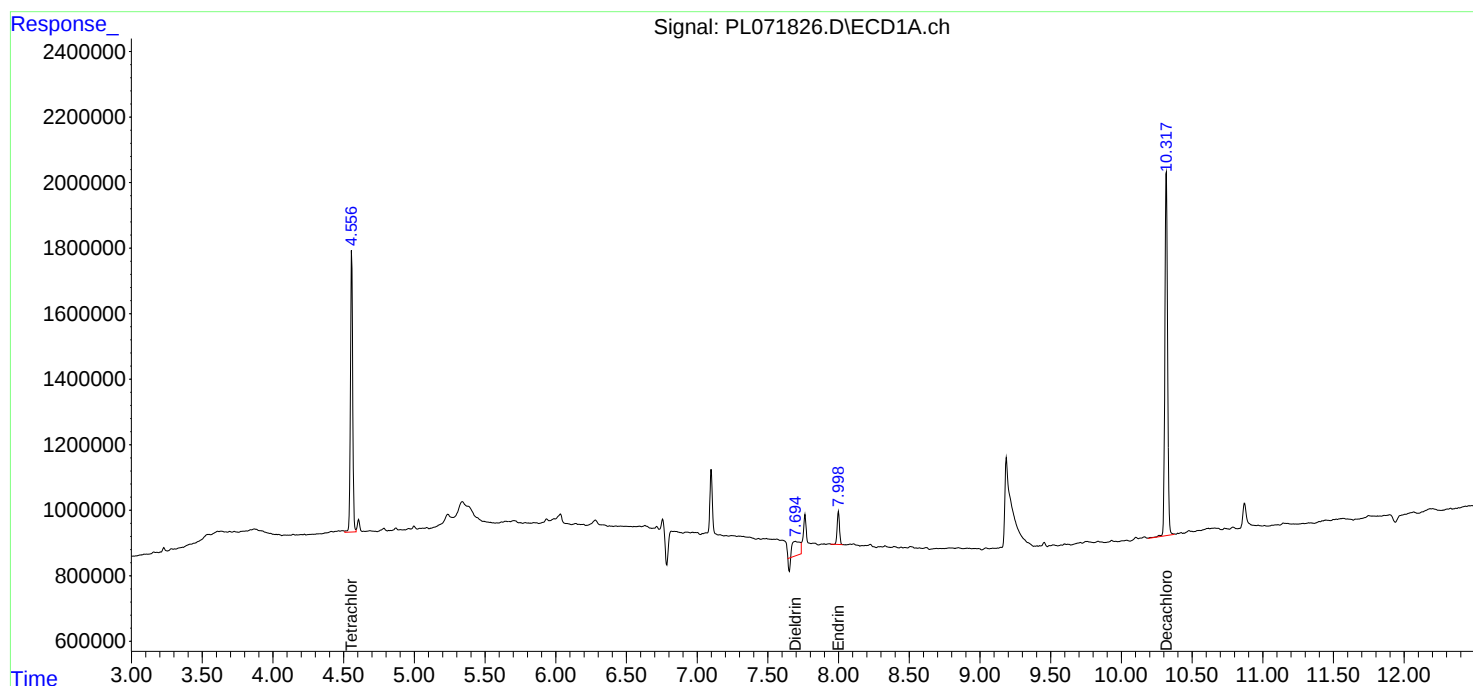


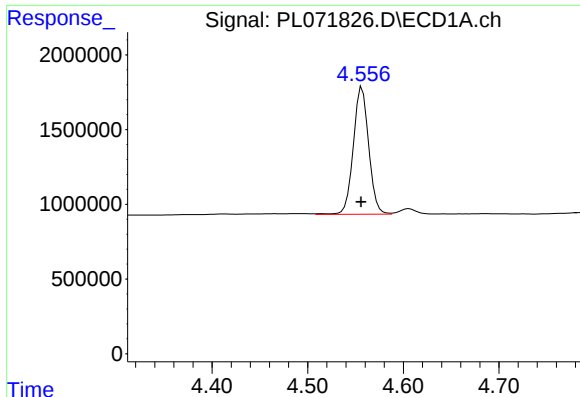

#1 Tetrachloro-m-xylene


R.T.: 4.557 min
Delta R.T.: 0.001 min
Response: 9536299
Conc: 20.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

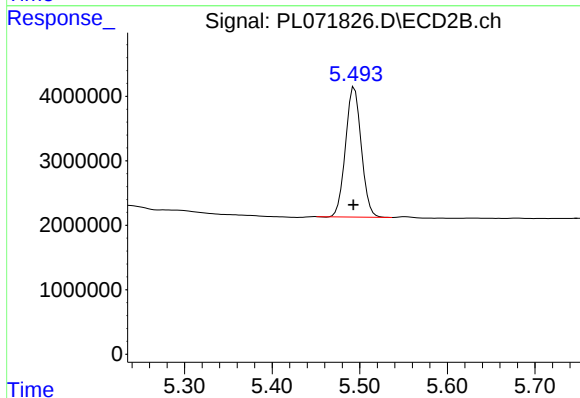


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.000 min
Response: 25171364
Conc: 20.49 ng/ml

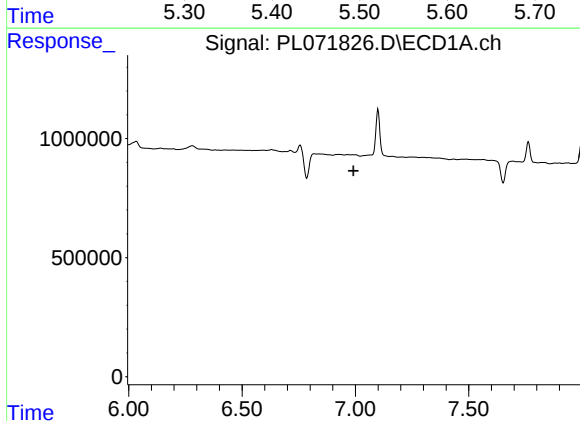


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 6.992 min
Response: 0
Conc: N.D.

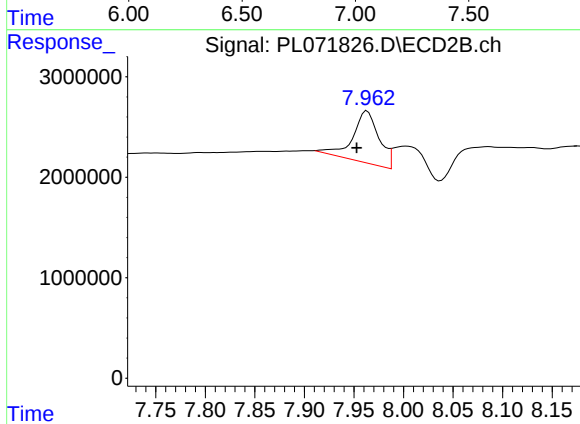

#8 Heptachlor epoxide


R.T.: 7.963 min
Delta R.T.: 0.011 min
Response: 9573028
Conc: 6.85 ng/ml

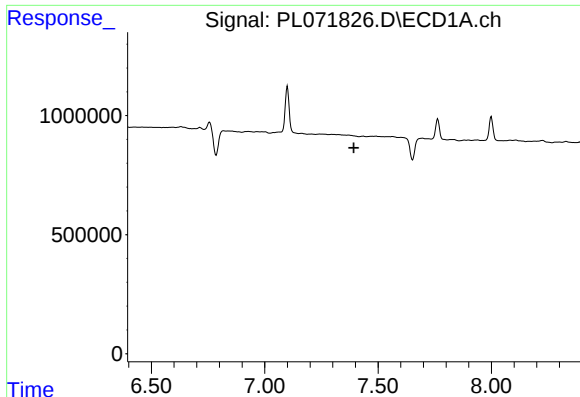

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.394 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

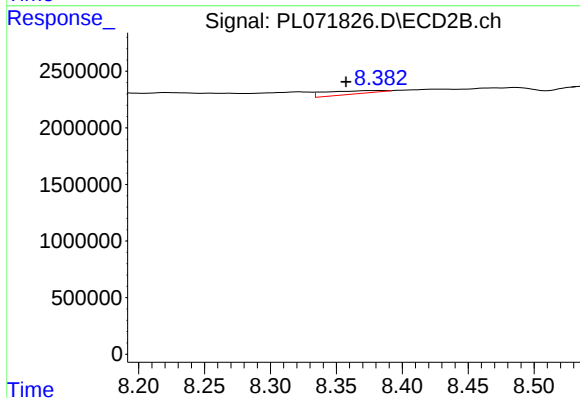


#9 Endosulfan I

R.T.: 8.383 min
Delta R.T.: 0.026 min
Response: 851014
Conc: 0.69 ng/ml

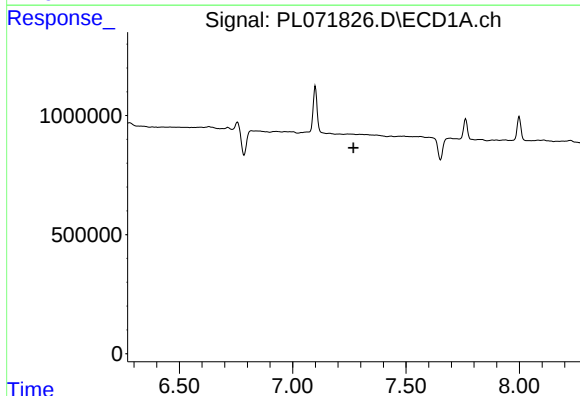


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

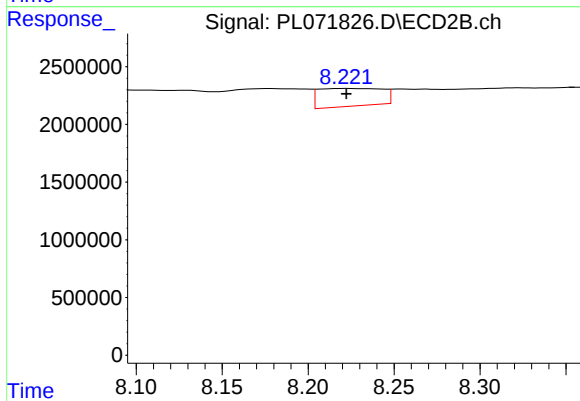

#10 gamma-Chlordane


R.T.: 8.222 min
Delta R.T.: 0.000 min
Response: 3948672
Conc: 2.89 ng/ml

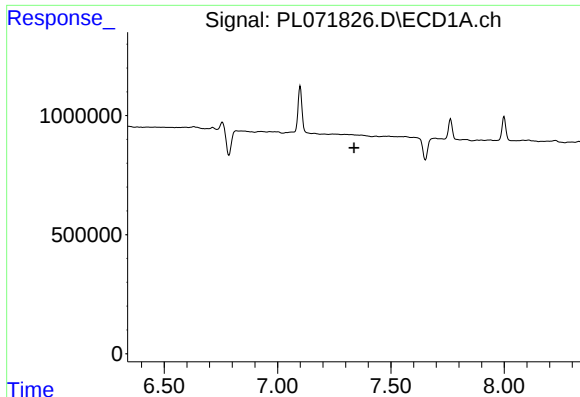

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.338 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

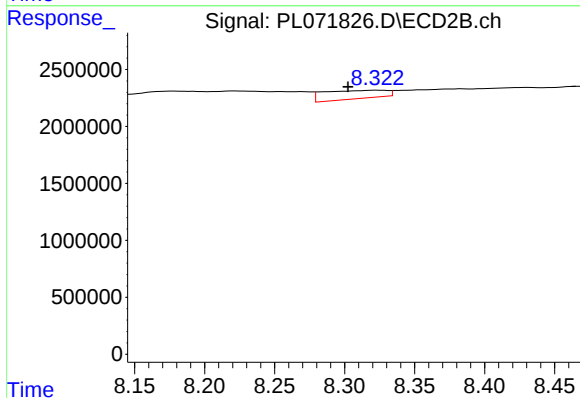


#11 alpha-Chlordane

R.T.: 8.323 min
Delta R.T.: 0.020 min
Response: 2288756
Conc: 1.72 ng/ml

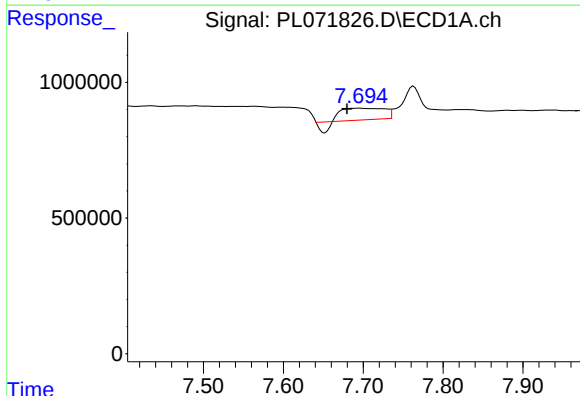


#13 Dieldrin

R.T.: 7.696 min
Delta R.T.: 0.016 min
Response: 1401741
Conc: 2.32 ng/ml

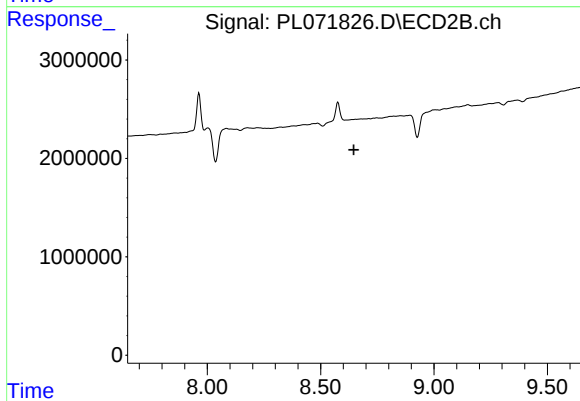

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.646 min
Response: 0
Conc: N.D.

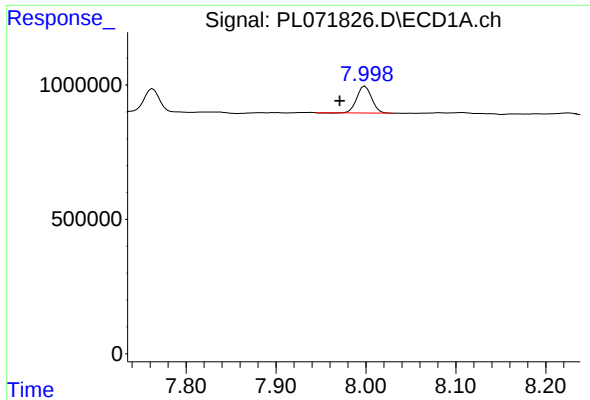

#14 Endrin


R.T.: 7.999 min
Delta R.T.: 0.028 min
Response: 1153003
Conc: 2.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

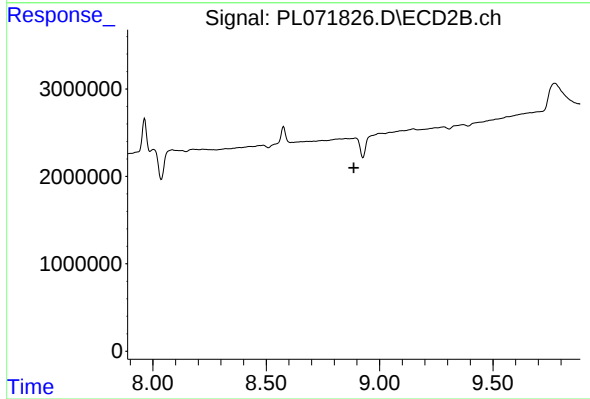


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.886 min
Response: 0
Conc: N.D.

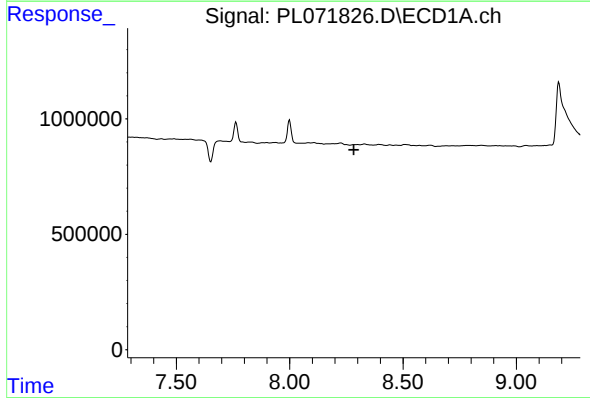


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.283 min
Response: 0
Conc: N.D.

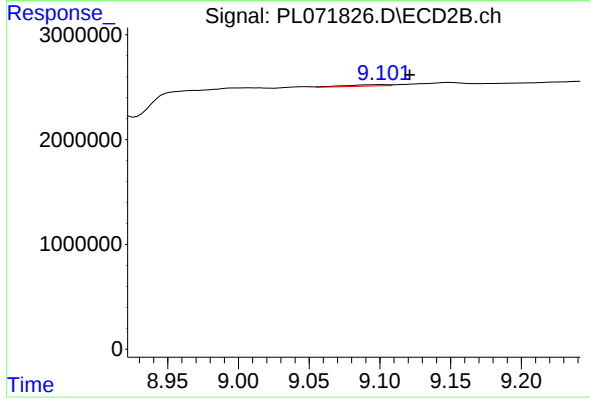

#15 Endosulfan II


R.T.: 9.102 min
Delta R.T.: -0.019 min
Response: 270200
Conc: 0.24 ng/ml

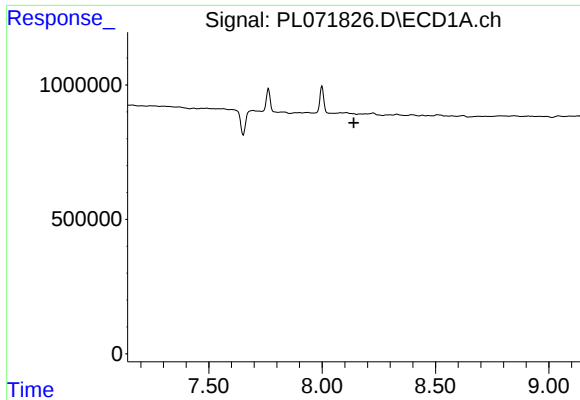

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.139 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

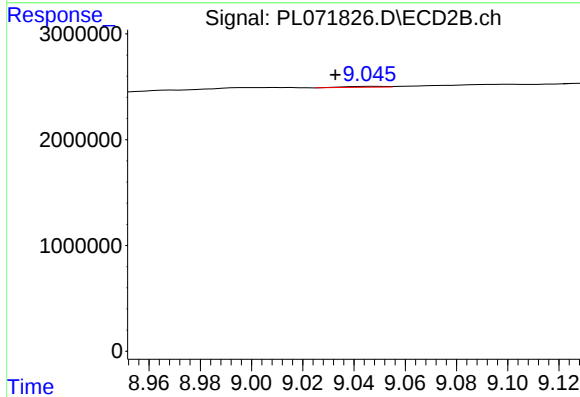


#16 4,4'-DDD

R.T.: 9.047 min
Delta R.T.: 0.014 min
Response: 86309
Conc: 0.09 ng/ml

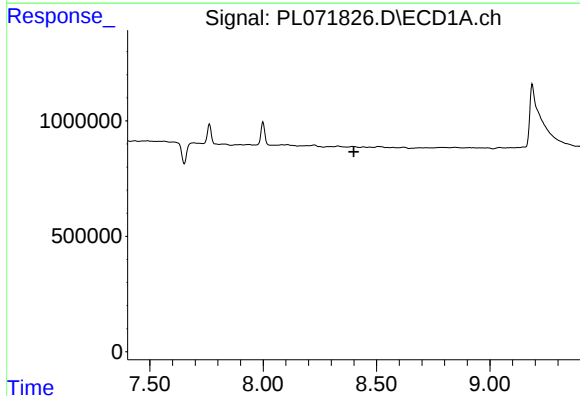


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.399 min
Response: 0
Conc: N.D.

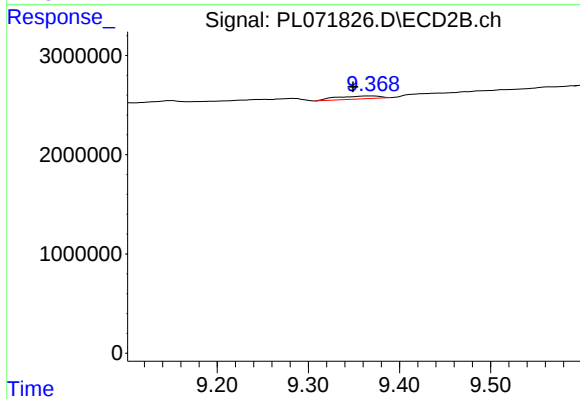

#17 4,4'-DDT


R.T.: 9.370 min
Delta R.T.: 0.020 min
Response: 964297
Conc: 1.02 ng/ml

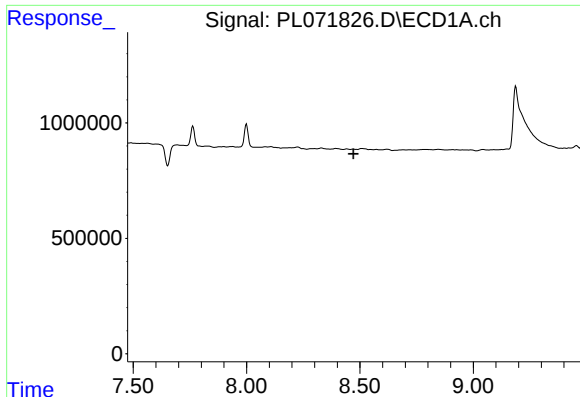

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 8.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

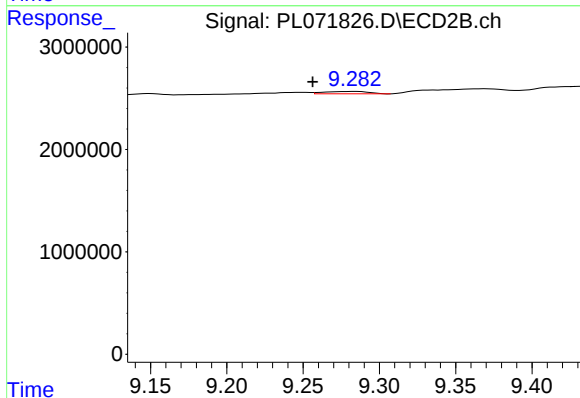


#18 Endrin aldehyde

R.T.: 9.284 min
Delta R.T.: 0.027 min
Response: 472387
Conc: 0.56 ng/ml

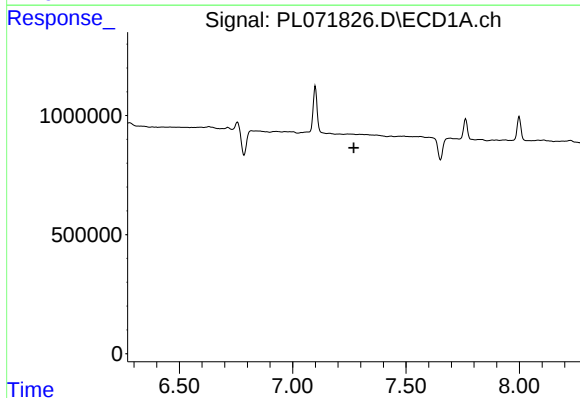


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

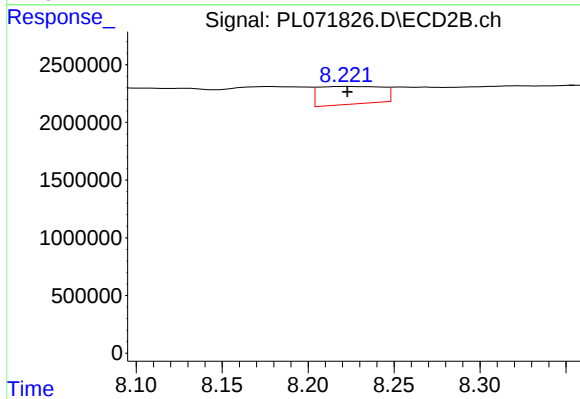

#25 Chlordane-3


R.T.: 8.222 min
Delta R.T.: -0.001 min
Response: 3948672
Conc: 19.35 ng/ml

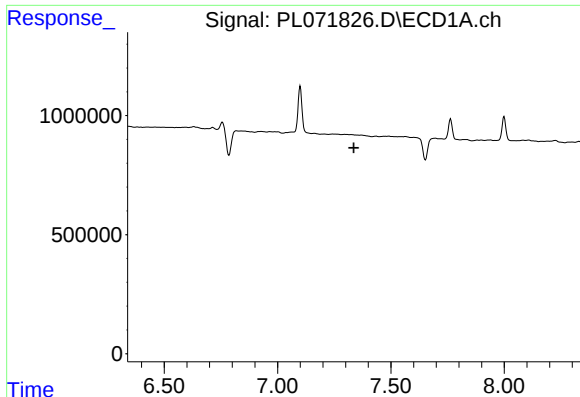

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.337 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

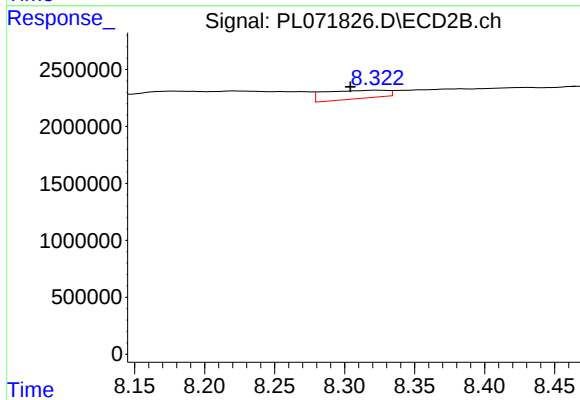


#26 Chlordane-4

R.T.: 8.323 min
Delta R.T.: 0.019 min
Response: 2288756
Conc: 9.40 ng/ml

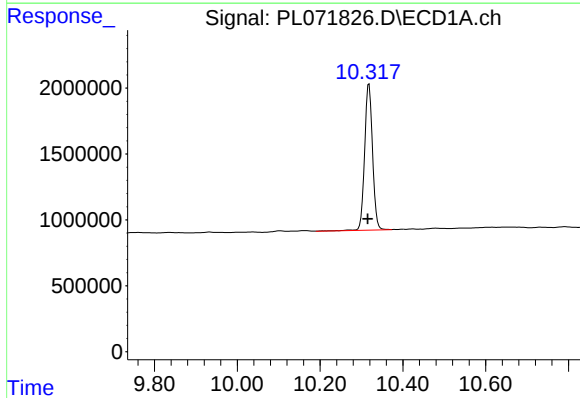

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: 0.003 min
Response: 14736645
Conc: 20.38 ng/ml

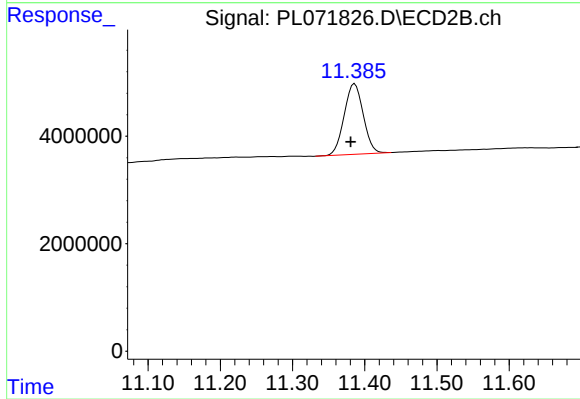

#28 Decachlorobiphenyl

R.T.: 11.386 min
Delta R.T.: 0.005 min
Response: 24035152
Conc: 20.28 ng/ml