

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010522\
 Data File : PL071805.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2022 09:35
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 06 00:35:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 05 01:51:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	10.320	11.385	31726	98766	0.044	0.083 #
Target Compounds							
6)	B beta-BHC	6.041f	0.000	292726	0	1.082	N.D. #
7)	B delta-BHC	0.000	6.996	0	368329	N.D.	0.240 #
8)	B Heptachlo...	0.000	7.955	0	1647398	N.D.	1.179 #
9)	A Endosulfan I	0.000	8.346	0	327230	N.D.	0.264 #
10)	B gamma-Chl...	0.000	8.215	0	1479202	N.D.	1.082 #
11)	B alpha-Chl...	0.000	8.309	0	596133	N.D.	0.448 #
13)	MA Dieldrin	7.704f	0.000	215263	0	0.357	N.D. #
16)	A 4,4'-DDD	0.000	9.019	0	134927	N.D.	0.140 #
17)	MA 4,4'-DDT	0.000	9.323f	0	185188	N.D.	0.196 #
21)	B Endrin ke...	0.000	10.017f	0	97277	N.D.	0.086 #
25)	Chlordane-3	0.000	8.215	0	1479202	N.D.	7.247 #
26)	Chlordane-4	0.000	8.309	0	596133	N.D.	2.449 #
27)	Chlordane-5	0.000	9.176	0	75967	N.D.	1.897 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010522\
Data File : PL071805.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2022 09:35
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 06 00:35:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Wed Jan 05 01:51:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

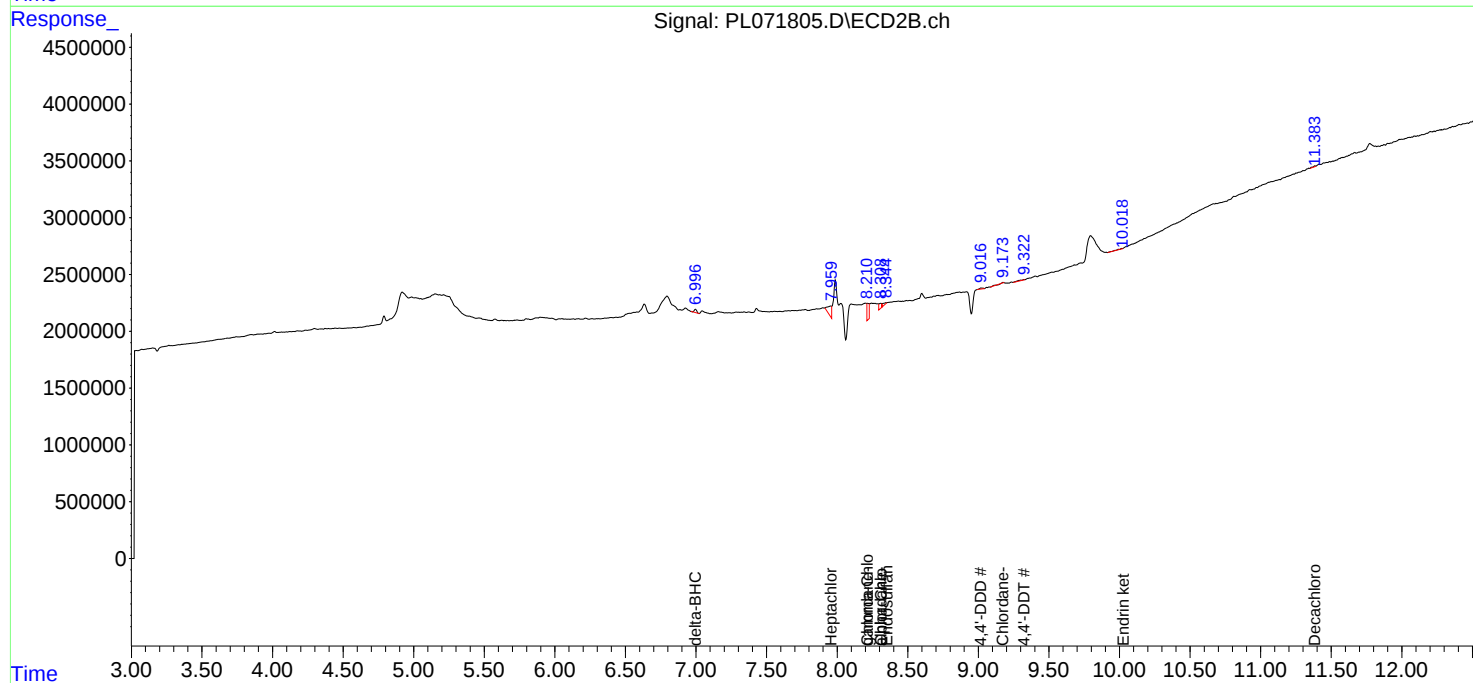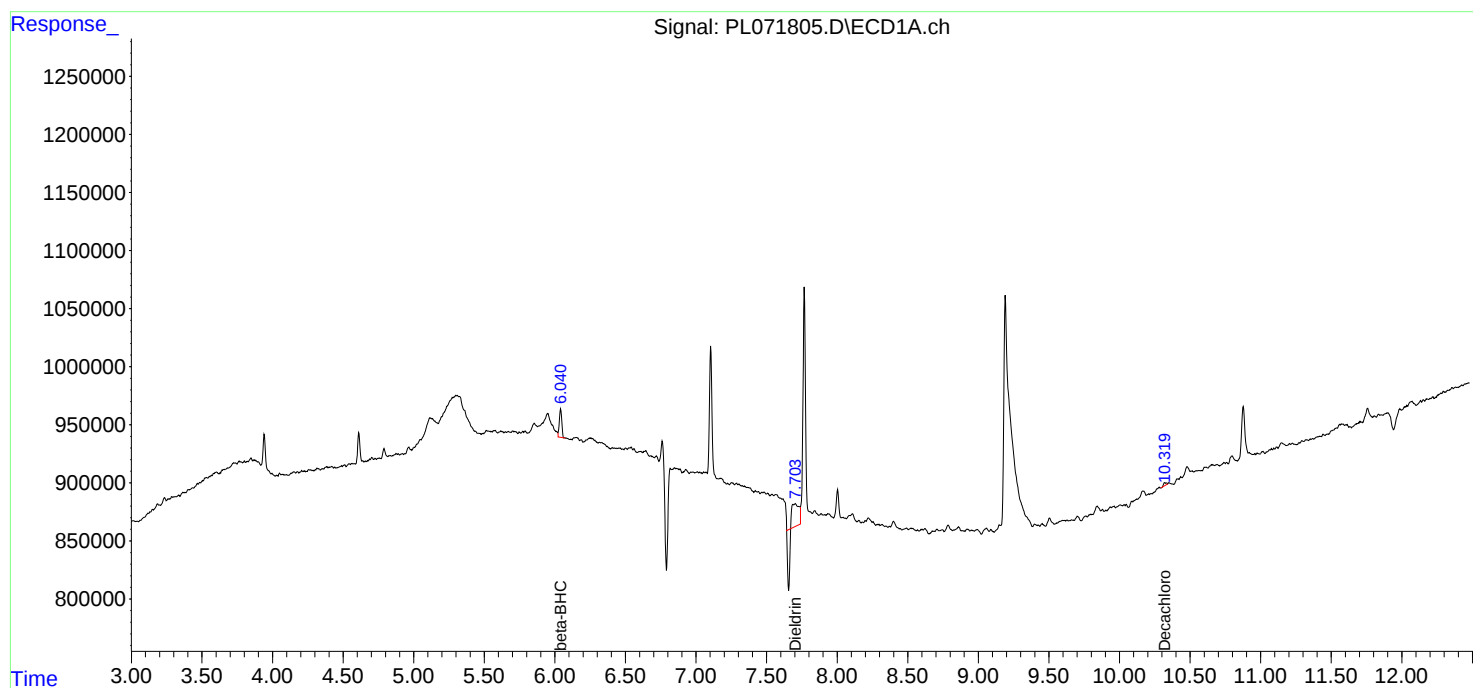


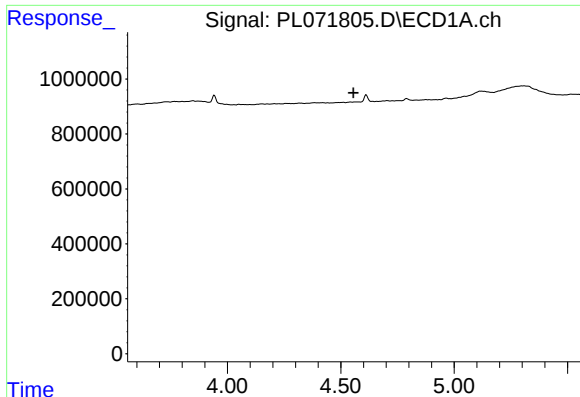

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 4.556 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

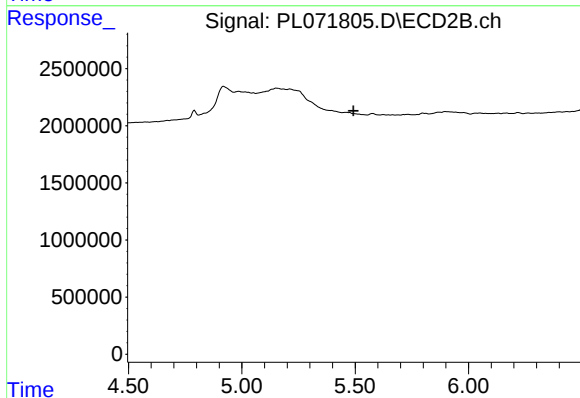


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 5.493 min
Response: 0
Conc: N.D.

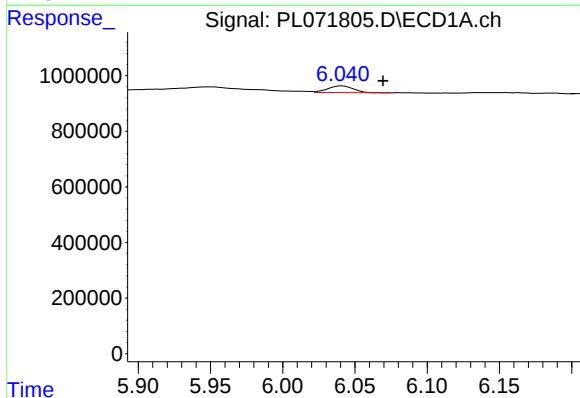


#6 beta-BHC

R.T.: 6.041 min
Delta R.T.: -0.028 min
Response: 292726
Conc: 1.08 ng/ml

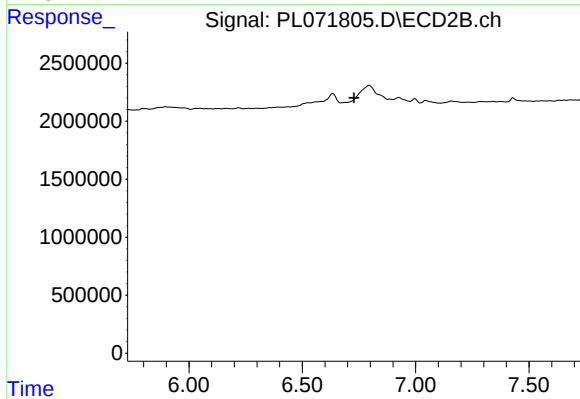

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.729 min
Response: 0
Conc: N.D.

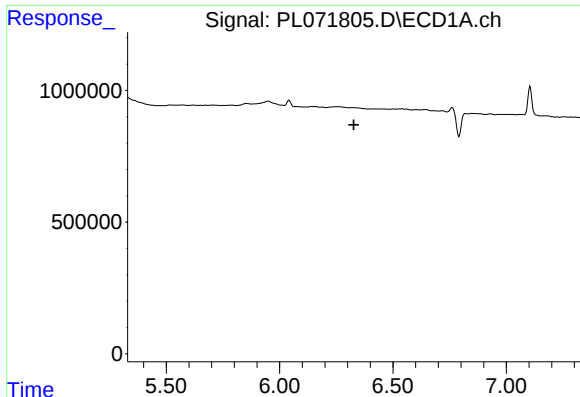

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.327 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

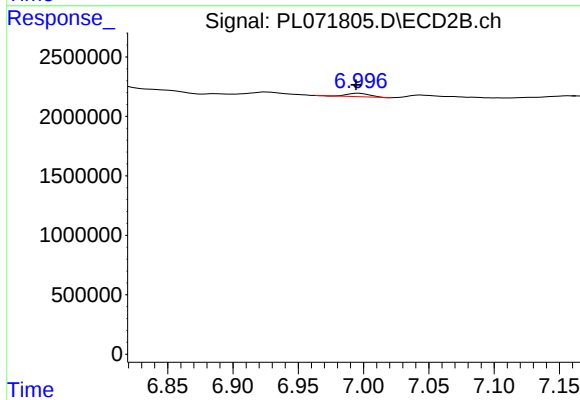


#7 delta-BHC

R.T.: 6.996 min
Delta R.T.: 0.002 min
Response: 368329
Conc: 0.24 ng/ml

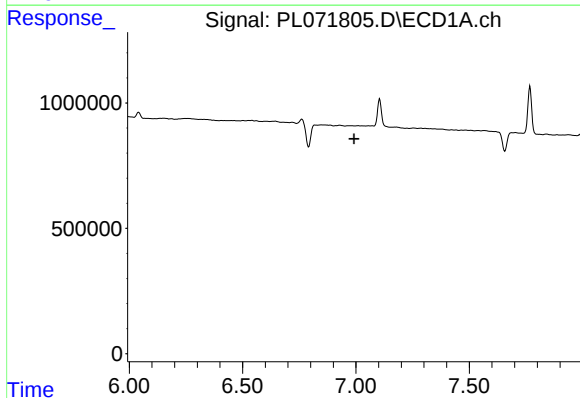


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 6.992 min
Response: 0
Conc: N.D.

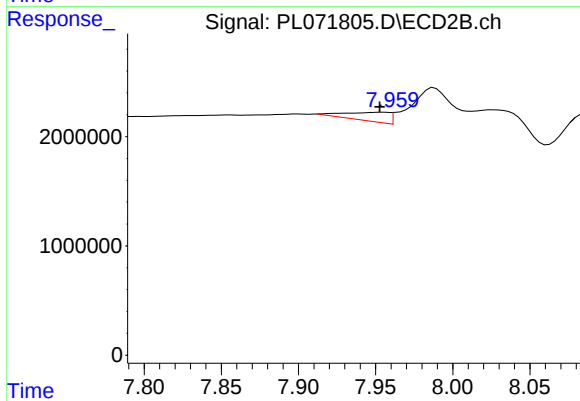

#8 Heptachlor epoxide


R.T.: 7.955 min
Delta R.T.: 0.003 min
Response: 1647398
Conc: 1.18 ng/ml

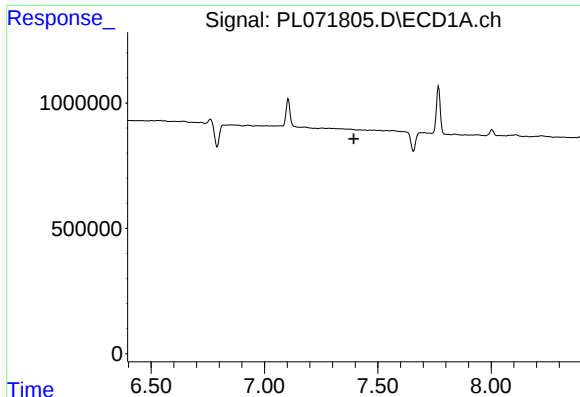

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.394 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

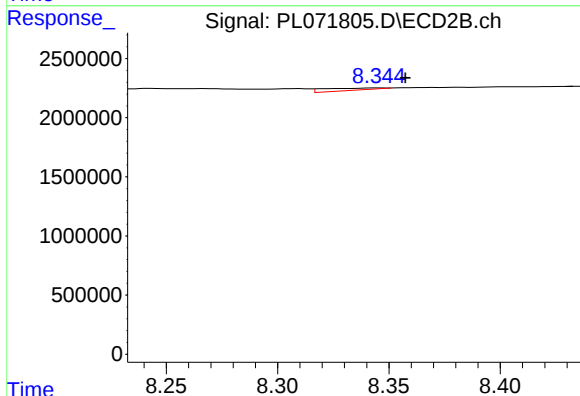


#9 Endosulfan I

R.T.: 8.346 min
Delta R.T.: -0.012 min
Response: 327230
Conc: 0.26 ng/ml

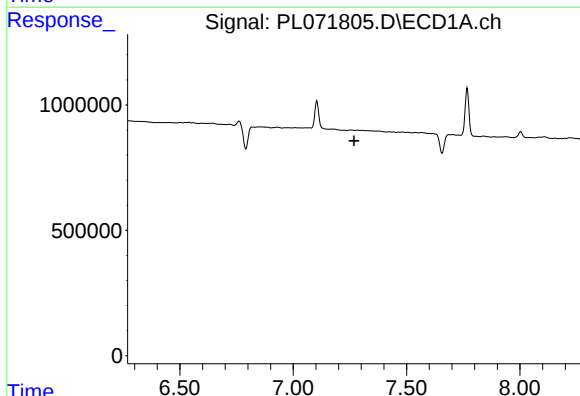


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

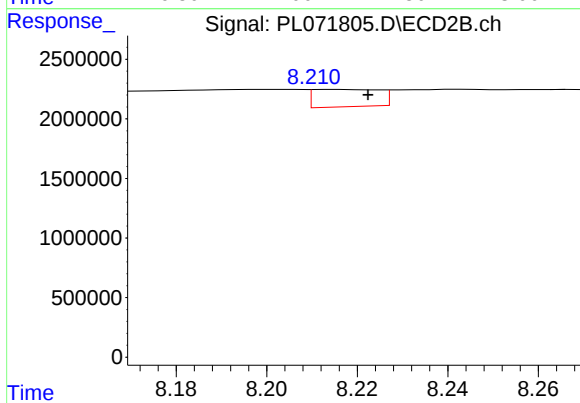

#10 gamma-Chlordane


R.T.: 8.215 min
Delta R.T.: -0.008 min
Response: 1479202
Conc: 1.08 ng/ml

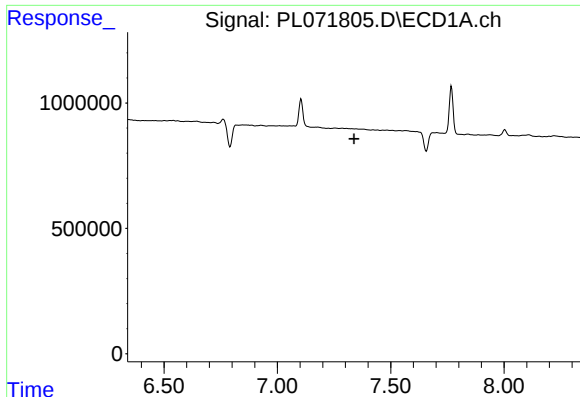

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.338 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

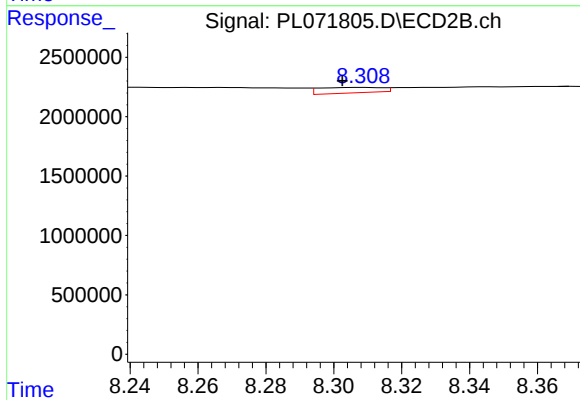


#11 alpha-Chlordane

R.T.: 8.309 min
Delta R.T.: 0.006 min
Response: 596133
Conc: 0.45 ng/ml

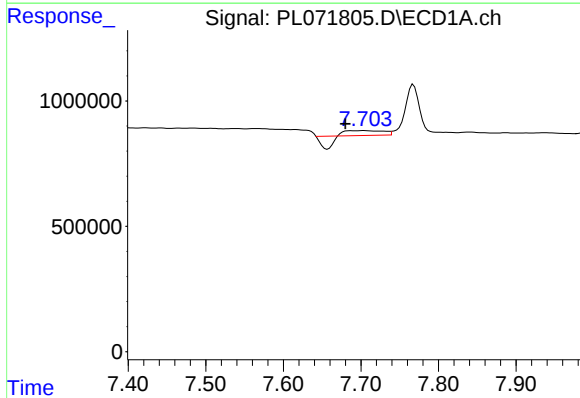


#13 Dieldrin

R.T.: 7.704 min
Delta R.T.: 0.024 min
Response: 215263
Conc: 0.36 ng/ml

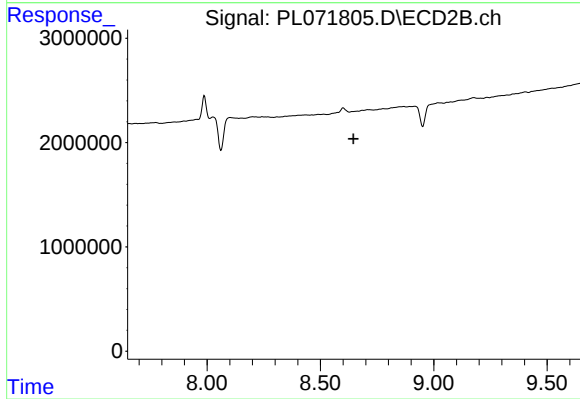

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.646 min
Response: 0
Conc: N.D.

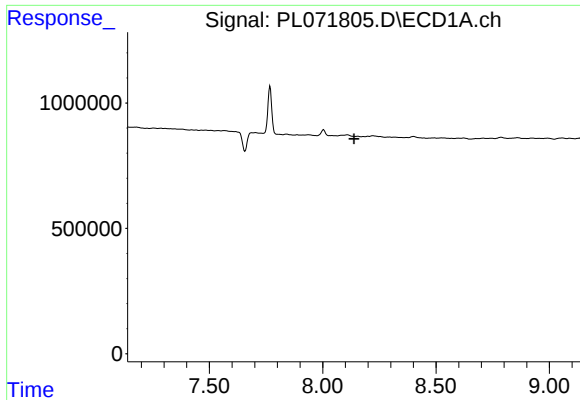

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.139 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

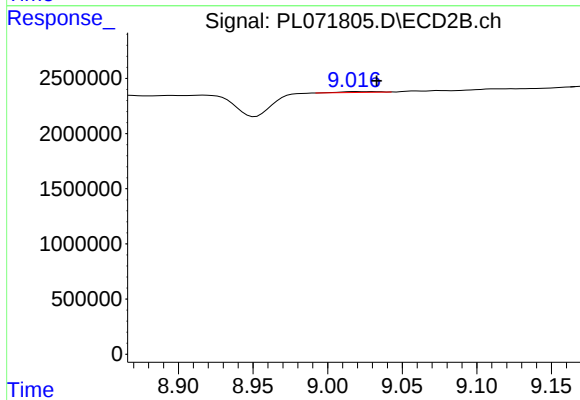


#16 4,4'-DDD

R.T.: 9.019 min
Delta R.T.: -0.014 min
Response: 134927
Conc: 0.14 ng/ml

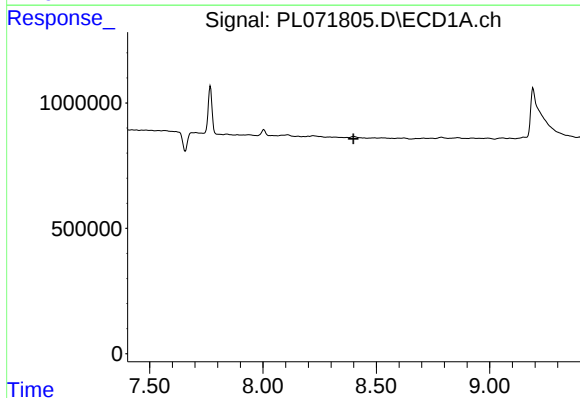


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.399 min
Response: 0
Conc: N.D.

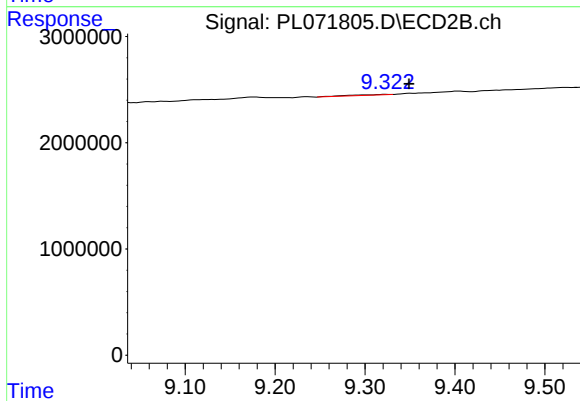

#17 4,4'-DDT


R.T.: 9.323 min
Delta R.T.: -0.026 min
Response: 185188
Conc: 0.20 ng/ml

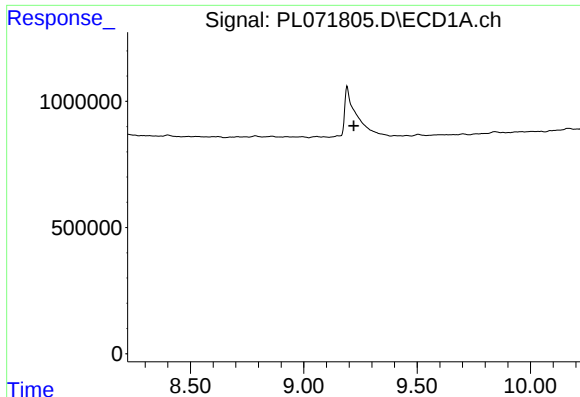

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

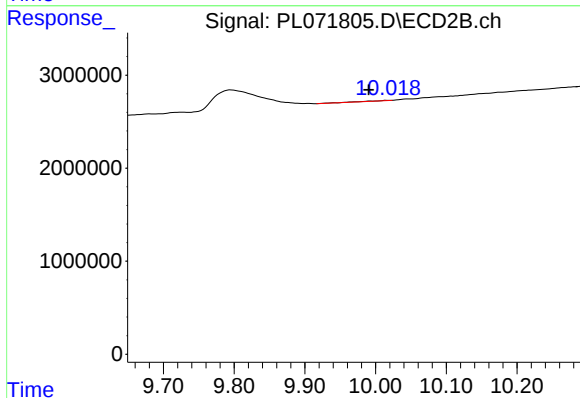


#21 Endrin ketone

R.T.: 10.017 min
Delta R.T.: 0.027 min
Response: 97277
Conc: 0.09 ng/ml

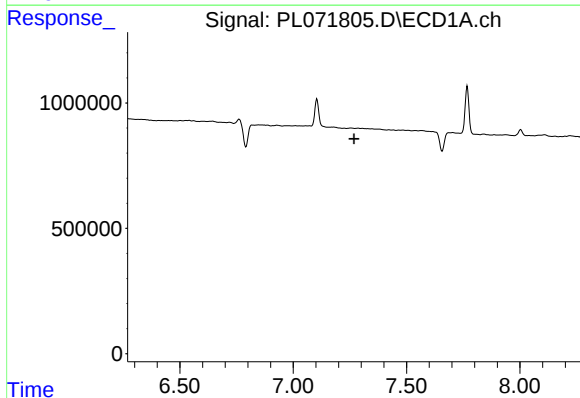


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

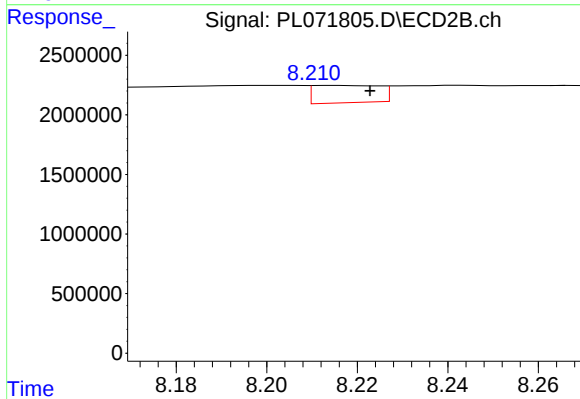

#25 Chlordane-3


R.T.: 8.215 min
Delta R.T.: -0.008 min
Response: 1479202
Conc: 7.25 ng/ml

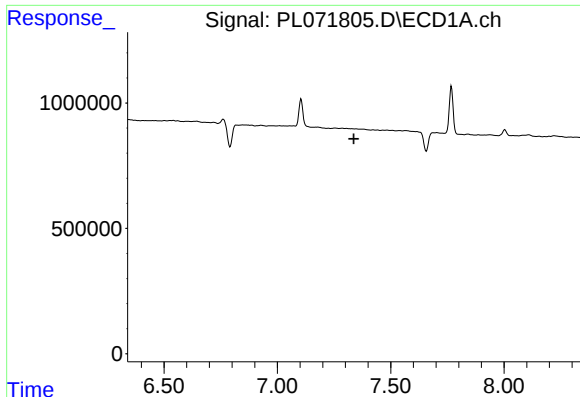

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.337 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

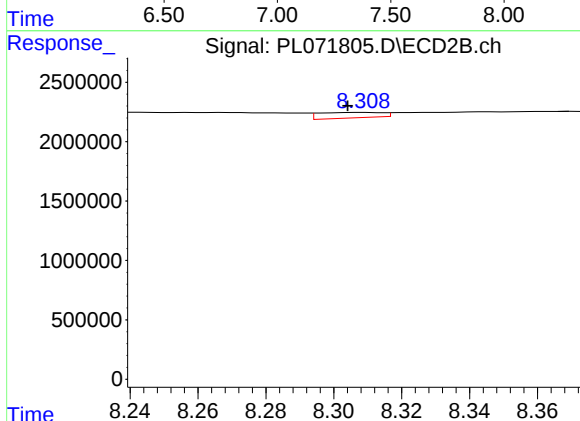


#26 Chlordane-4

R.T.: 8.309 min
Delta R.T.: 0.005 min
Response: 596133
Conc: 2.45 ng/ml

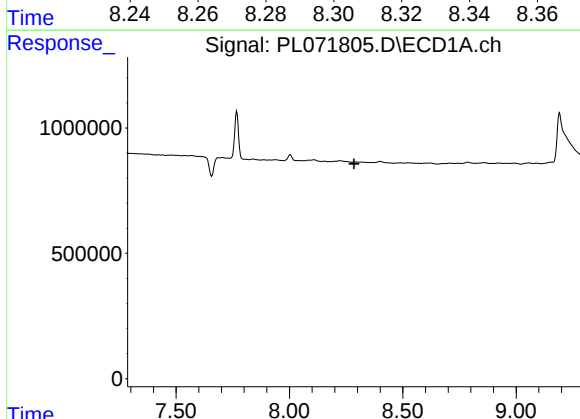


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.286 min
Response: 0
Conc: N.D.

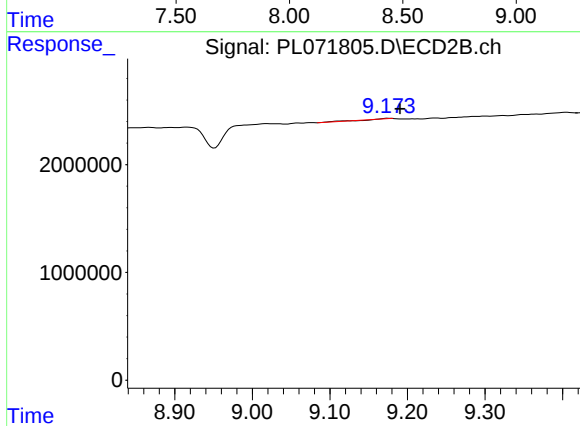

#27 Chlordane-5


R.T.: 9.176 min
Delta R.T.: -0.014 min
Response: 75967
Conc: 1.90 ng/ml

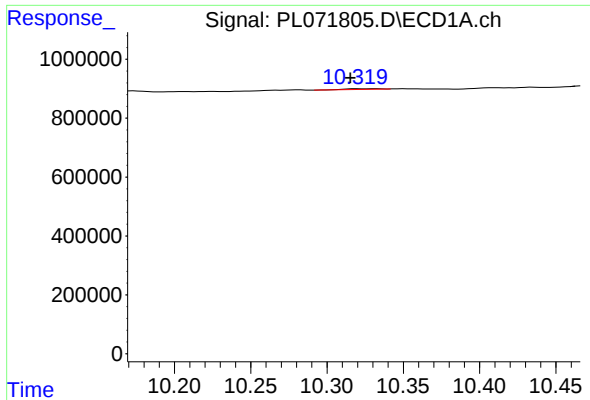

#28 Decachlorobiphenyl

R.T.: 10.320 min
Delta R.T.: 0.005 min
Response: 31726
Conc: 0.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

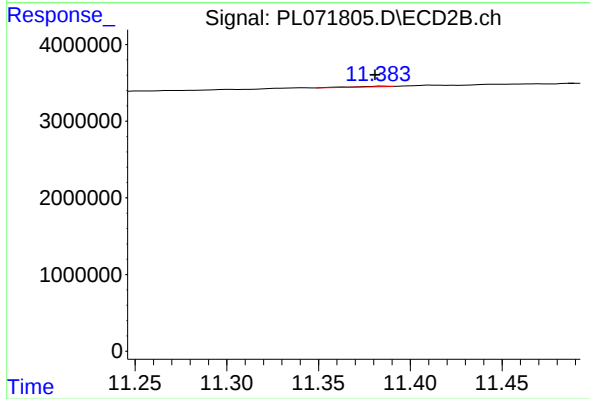

#28 Decachlorobiphenyl

R.T.: 11.385 min
Delta R.T.: 0.004 min
Response: 98766
Conc: 0.08 ng/ml