

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010522\
 Data File : PL071822.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2022 16:14
 Operator : AR\AJ
 Sample : N1018-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DUP-01-010422

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/06/2022
 Supervised By :Ankita Jodhani 01/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 06 00:40:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 05 01:51:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.557	5.494	6070466	16306288	13.141	13.272
28) SA Decachlor...	10.317	11.384	10497848	22934284	14.519m	19.354m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010522\
Data File : PL071822.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2022 16:14
Operator : AR\AJ
Sample : N1018-04
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
DUP-01-010422


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/06/2022
Supervised By :Ankita Jodhani 01/06/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 06 00:40:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Wed Jan 05 01:51:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

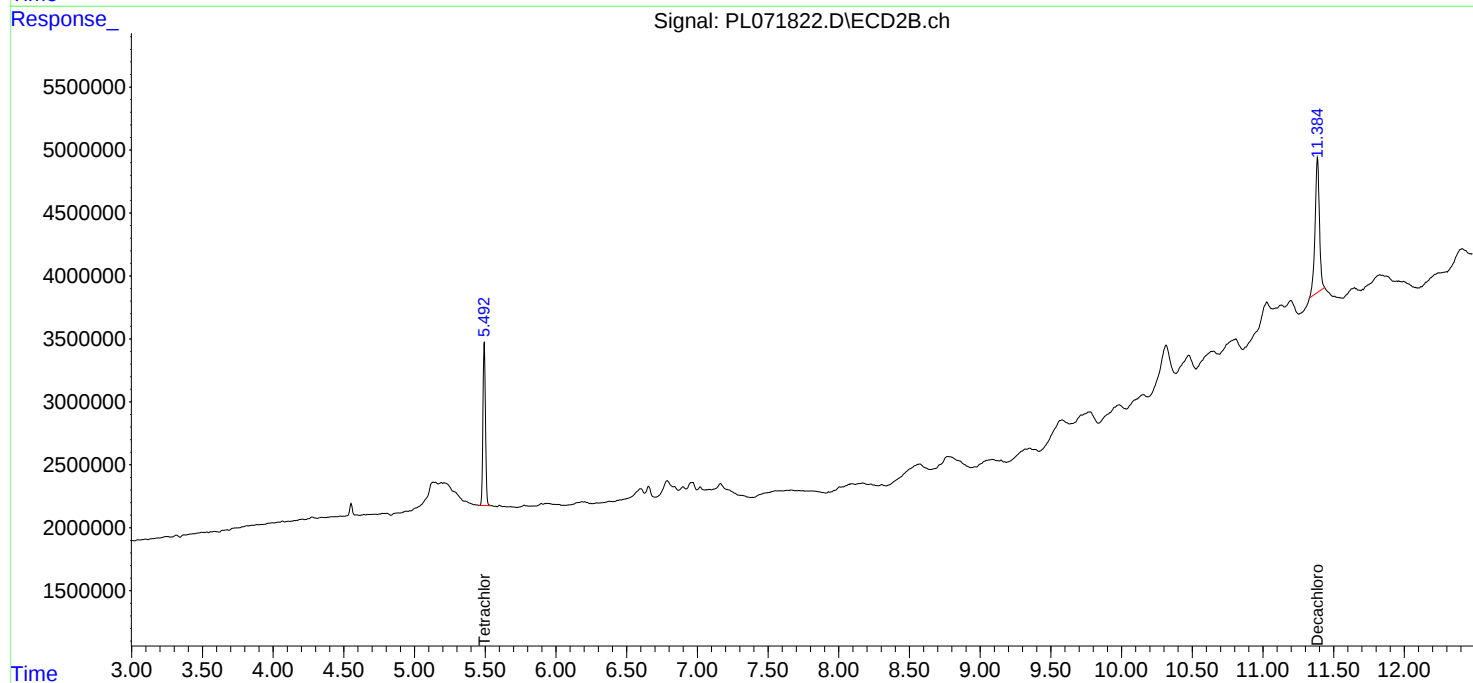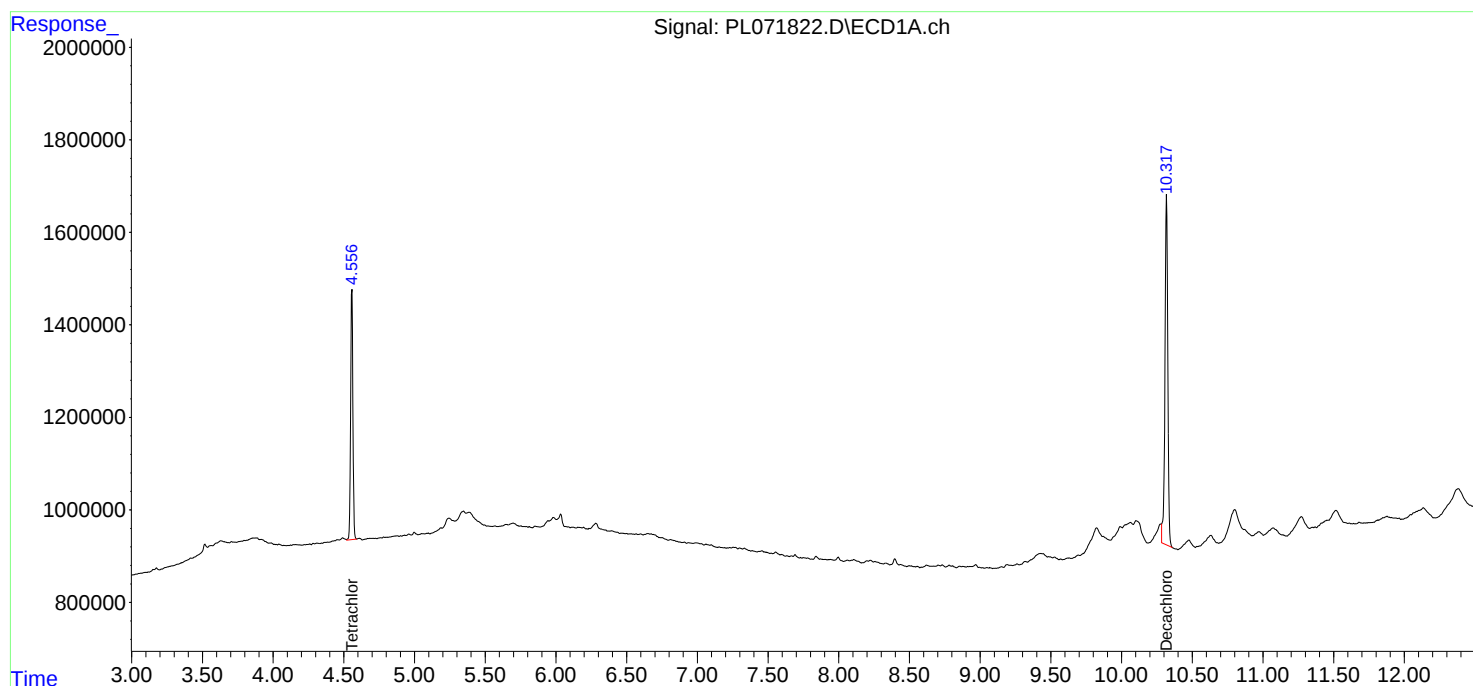

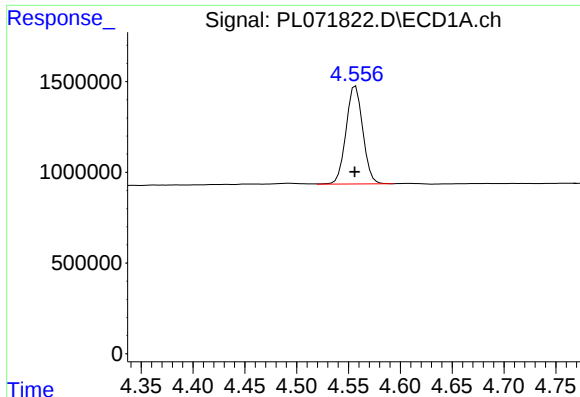


#1 Tetrachloro-m-xylene

R.T.: 4.557 min
Delta R.T.: 0.000 min
Response: 6070466
Conc: 13.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
DUP-01-010422


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/06/2022
Supervised By :Ankita Jodhani 01/06/2022

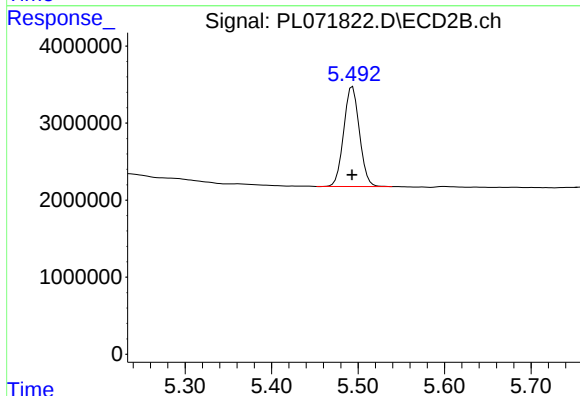


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.000 min
Response: 16306288
Conc: 13.27 ng/ml

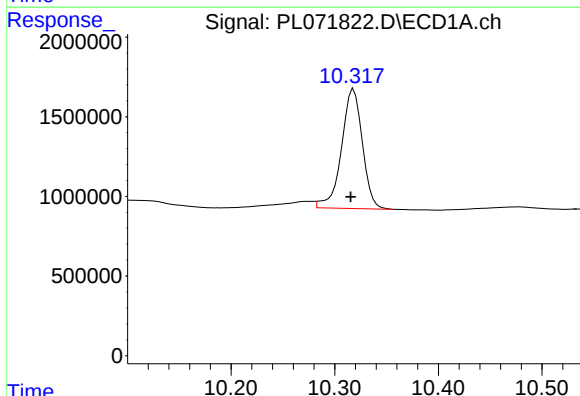

#28 Decachlorobiphenyl

R.T.: 10.317 min
Delta R.T.: 0.002 min
Response: 10497848
Conc: 14.52 ng/ml m

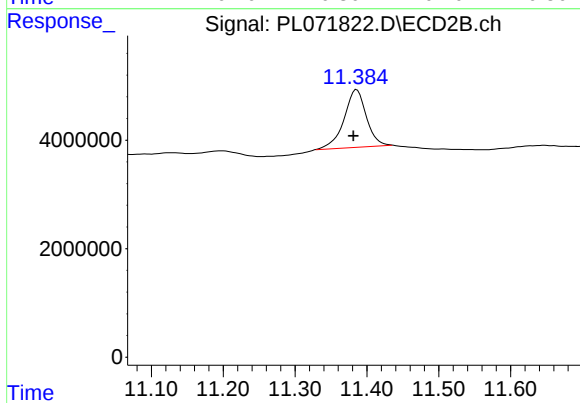

#28 Decachlorobiphenyl

R.T.: 11.384 min
Delta R.T.: 0.004 min
Response: 22934284
Conc: 19.35 ng/ml m