

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010524\
 Data File : PL087643.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2024 12:02
 Operator : AR\AJ
 Sample : PB158243BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB158243BL

Manual Integrations APPROVED

Reviewed By :Abdul
 Mirza

01/08/2024
 Supervised By :Ankita
 Jodhani

01/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 20:13:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 29 03:17:47 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.420	2.675	42856745	17445812	14.315	14.402
28) SA Decachlor...	8.978	7.861	45376522	22509249	15.933	17.768m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010524\
Data File : PL087643.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2024 12:02
Operator : AR\AJ
Sample : PB158243BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB158243BL

Manual Integrations
APPROVED



Reviewed By :Abdul
Mirza


01/08/2024
Supervised By :Ankita
Jodhani

01/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 20:13:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 03:17:47 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

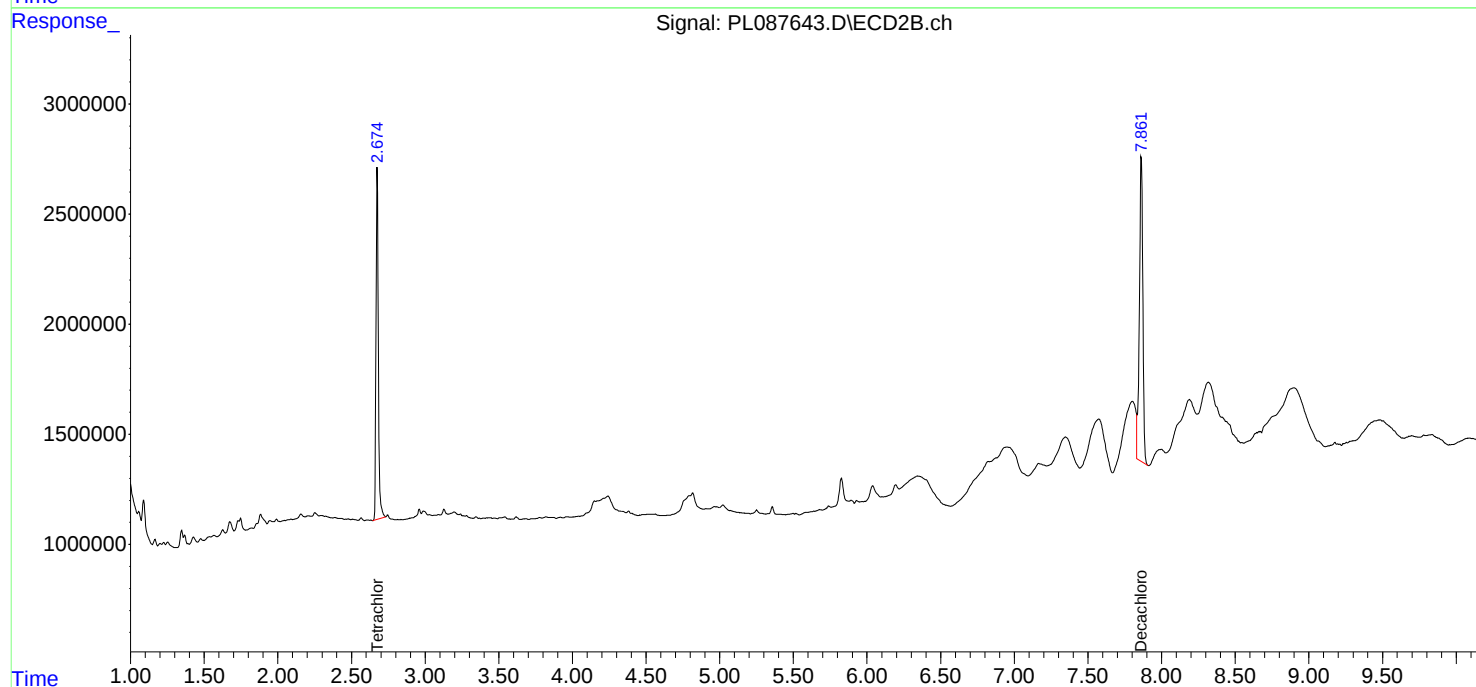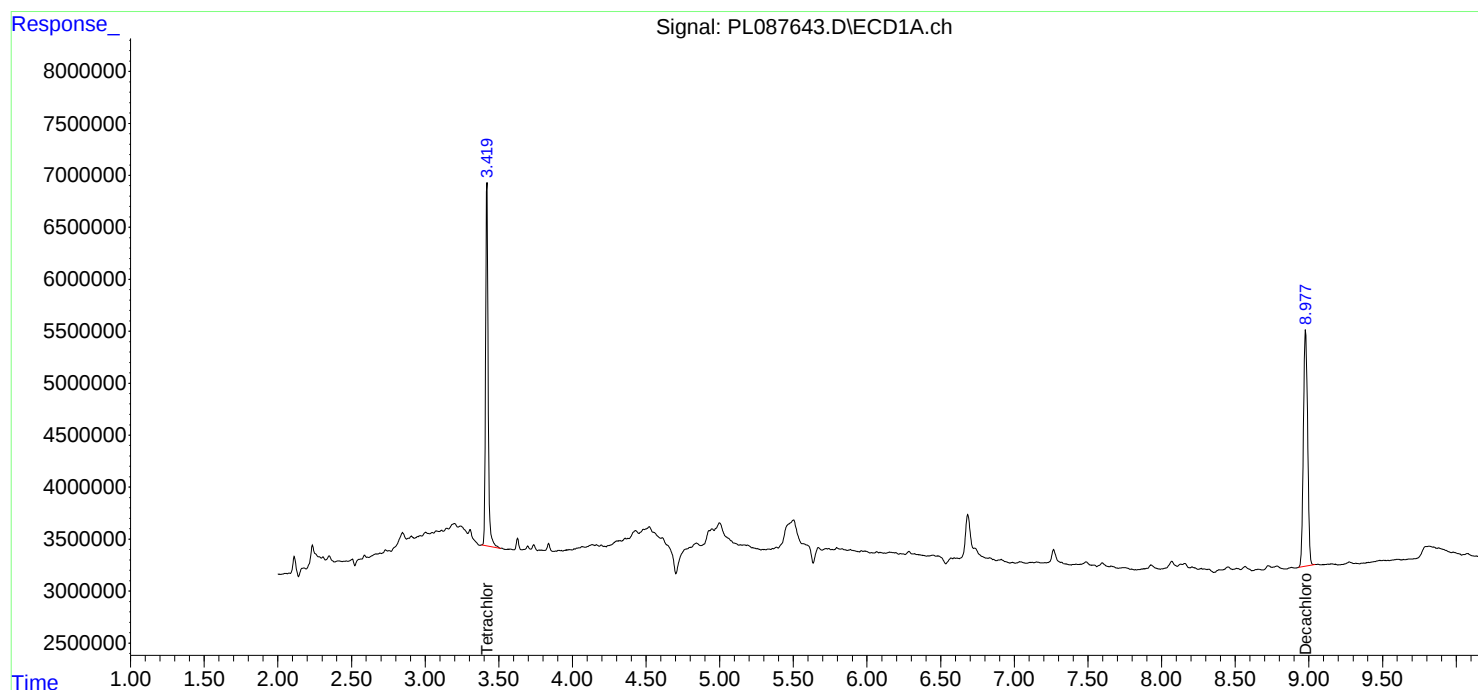

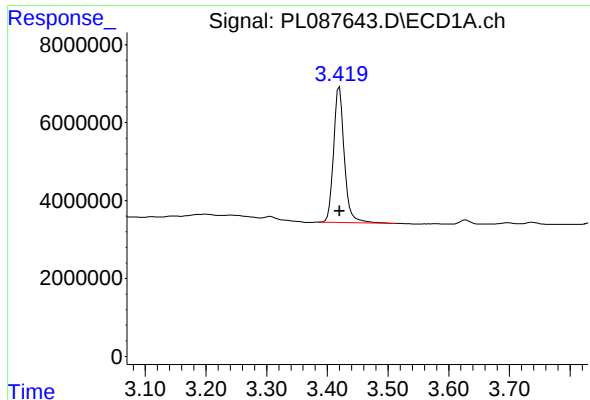

#1 Tetrachloro-m-xylene

R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 42856745
Conc: 14.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB158243BL


Manual Integrations
APPROVED

Reviewed By :Abdul
Mirza

01/08/2024


Supervised By :Ankita
Jodhani

01/08/2024

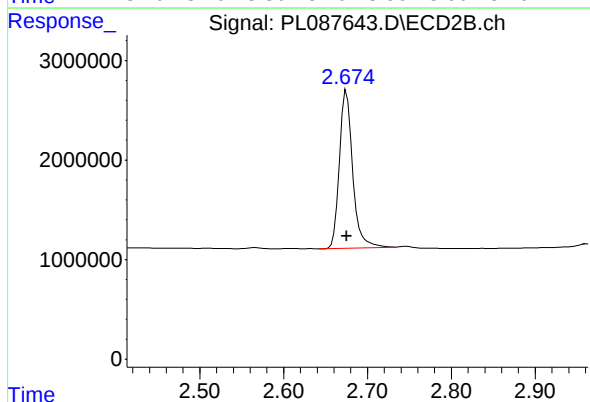


#1 Tetrachloro-m-xylene

R.T.: 2.675 min
Delta R.T.: 0.000 min
Response: 17445812
Conc: 14.40 ng/ml

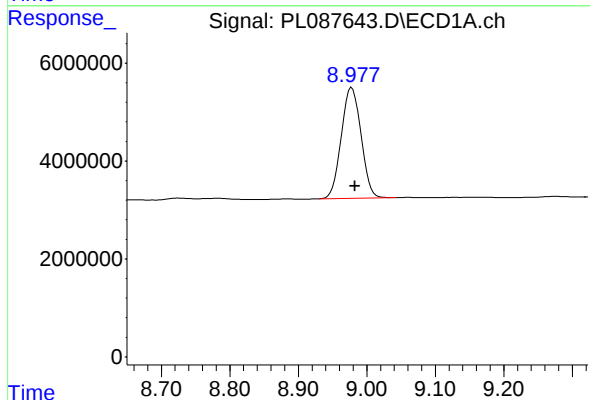

#28 Decachlorobiphenyl

R.T.: 8.978 min
Delta R.T.: -0.005 min
Response: 45376522
Conc: 15.93 ng/ml

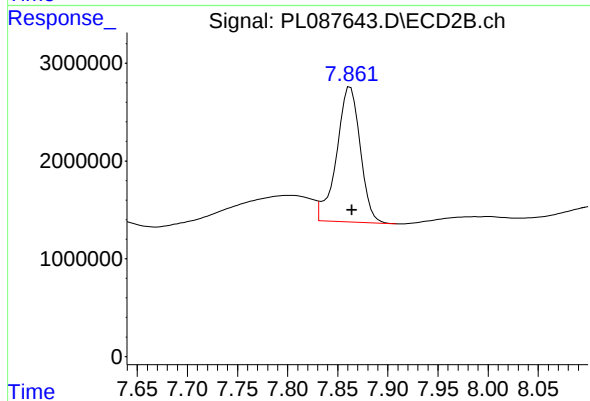

#28 Decachlorobiphenyl

R.T.: 7.861 min
Delta R.T.: -0.003 min
Response: 22509249
Conc: 17.77 ng/ml m