

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010524\
 Data File : PL087646.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2024 13:15
 Operator : AR\AJ
 Sample : P1012-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BI-WEEKLY-DECANT

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/08/2024
 Supervised By :Ankita Jodhani 01/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 20:16:34 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 29 03:17:47 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.421	2.676	51442156	20401473	17.183	16.842
28) SA Decachlor...	8.979	7.860	42612575	15879762	14.962m	12.535m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010524\
Data File : PL087646.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2024 13:15
Operator : AR\AJ
Sample : P1012-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/08/2024
Supervised By :Ankita Jodhani 01/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 20:16:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122823.M
Quant Title : GC Extractables
QLast Update : Fri Dec 29 03:17:47 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

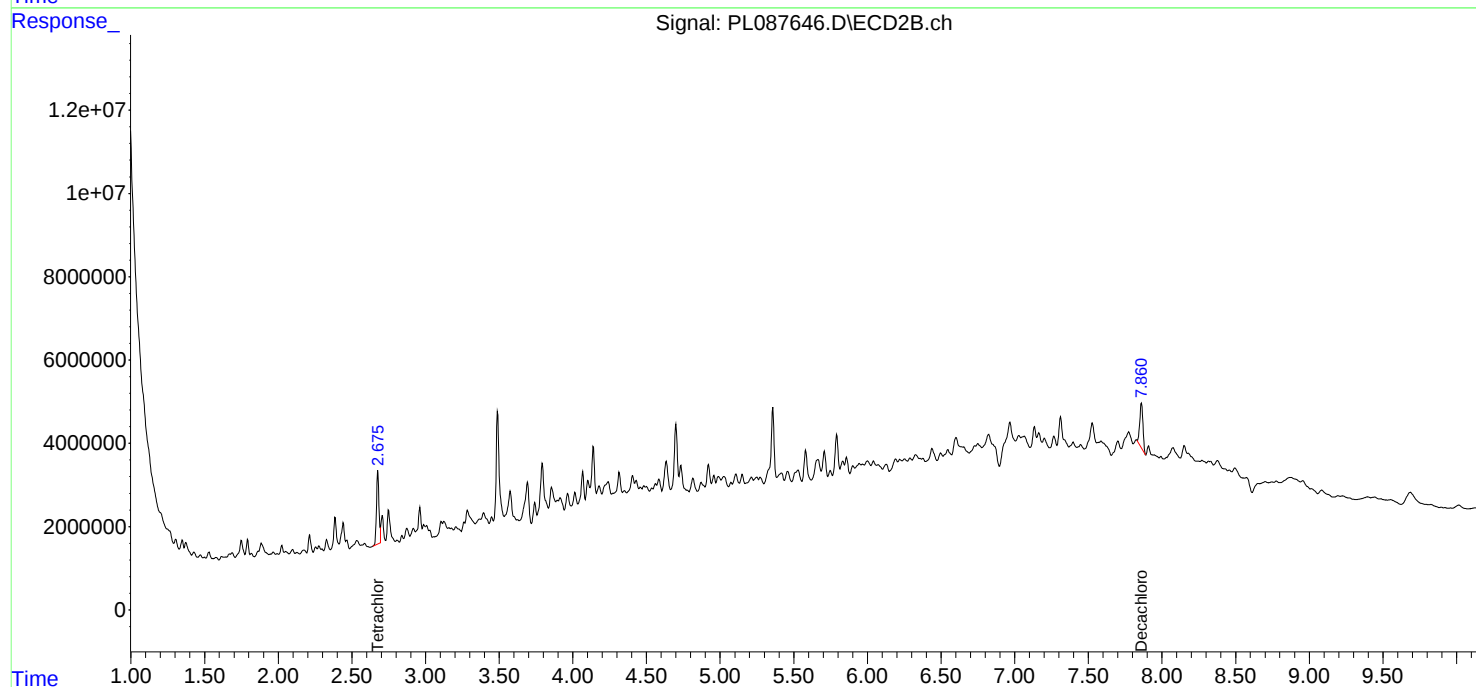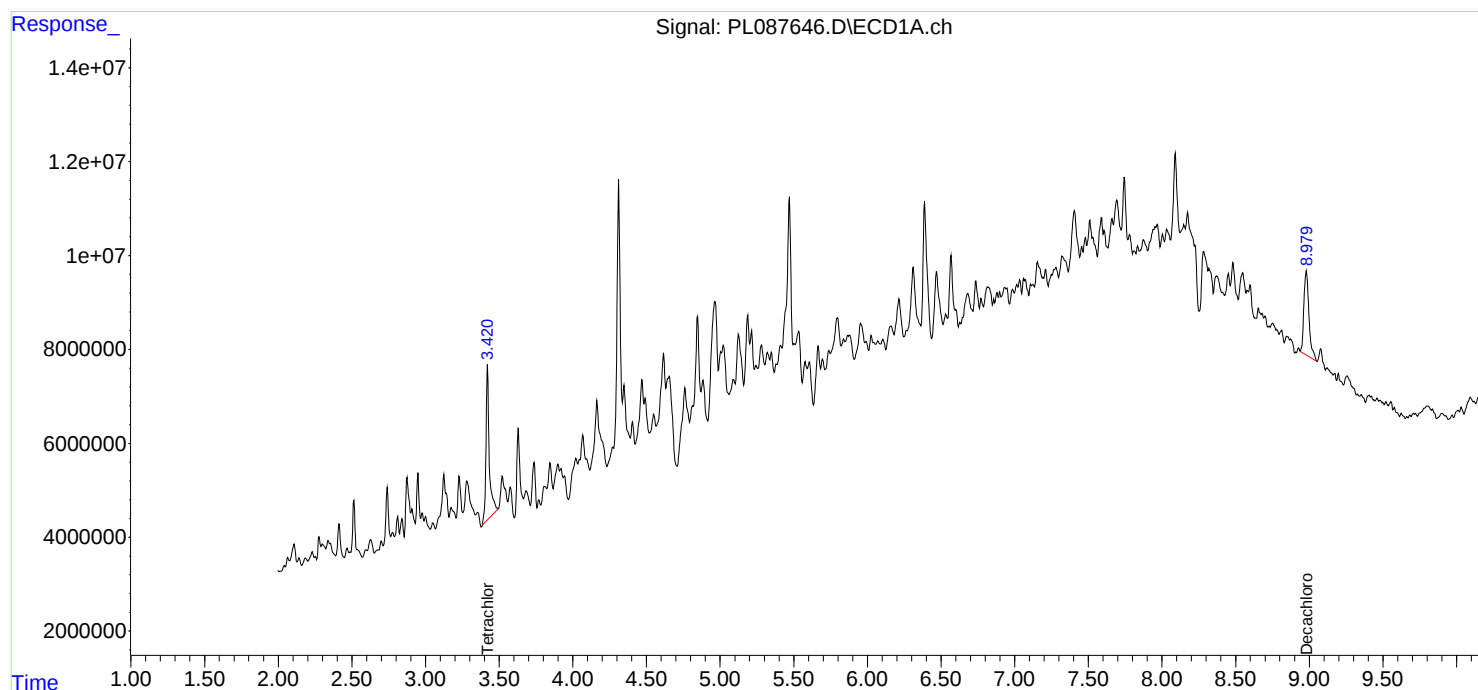

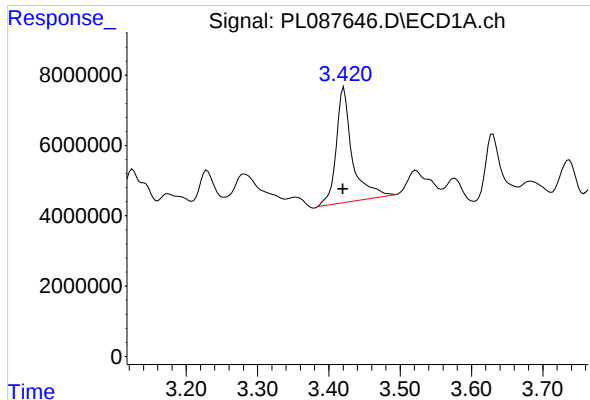


#1 Tetrachloro-m-xylene

R.T.: 3.421 min
Delta R.T.: 0.001 min
Response: 51442156
Conc: 17.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/08/2024
Supervised By :Ankita Jodhani 01/08/2024

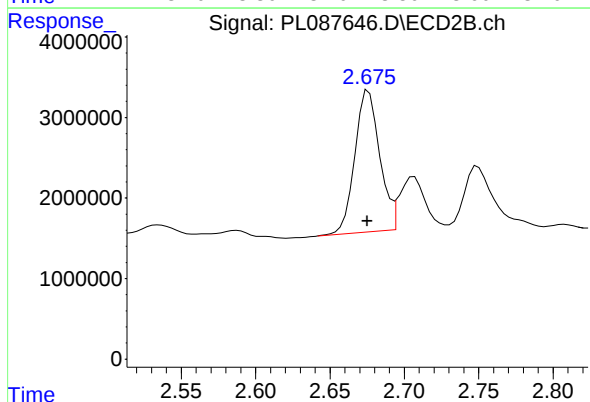


#1 Tetrachloro-m-xylene

R.T.: 2.676 min
Delta R.T.: 0.000 min
Response: 20401473
Conc: 16.84 ng/ml

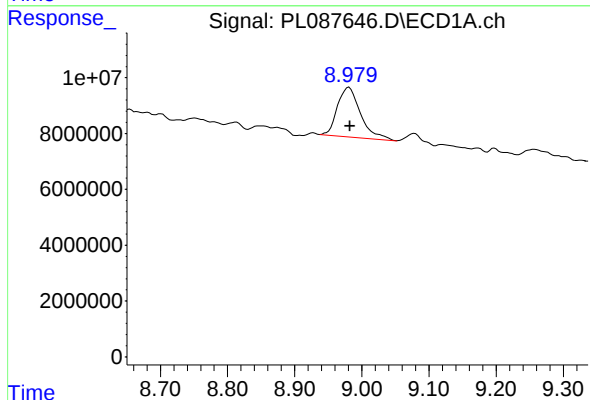

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: -0.003 min
Response: 42612575
Conc: 14.96 ng/ml m

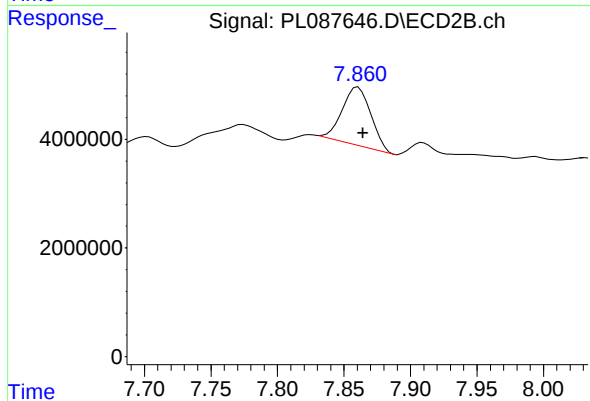

#28 Decachlorobiphenyl

R.T.: 7.860 min
Delta R.T.: -0.004 min
Response: 15879762
Conc: 12.54 ng/ml m