

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010622\
 Data File : PL071828.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jan 2022 08:58
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 00:02:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	10.289f	0.000	104317	0	0.144	N.D. #
Target Compounds							
5)	MB Aldrin	0.000	7.473	0	78259	N.D.	0.051 #
6)	B beta-BHC	6.045f	0.000	65240	0	0.241	N.D. #
7)	B delta-BHC	6.353f	7.023f	61327	414843	0.098	0.270 #
10)	B gamma-Chl...	0.000	8.229	0	99671	N.D.	0.073 #
13)	MA Dieldrin	0.000	8.638	0	134121	N.D.	0.102 #
14)	MA Endrin	0.000	8.910f	0	478851	N.D.	0.463 #
15)	B Endosulfa...	0.000	9.108	0	166569	N.D.	0.148 #
17)	MA 4,4'-DDT	0.000	9.373f	0	941851	N.D.	0.999 #
18)	B Endrin al...	0.000	9.252	0	227336	N.D.	0.268 #
20)	A Methoxychlor	9.000	9.819f	269407	891464	0.870	1.810 #
22)	Mirex	9.379f	10.455	421650	1233450	0.703	1.436 #
24)	Chlordane-2	0.000	7.473	0	78259	N.D.	1.446 #
25)	Chlordane-3	0.000	8.229	0	99671	N.D.	0.488 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010622\
Data File : PL071828.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jan 2022 08:58
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 00:02:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

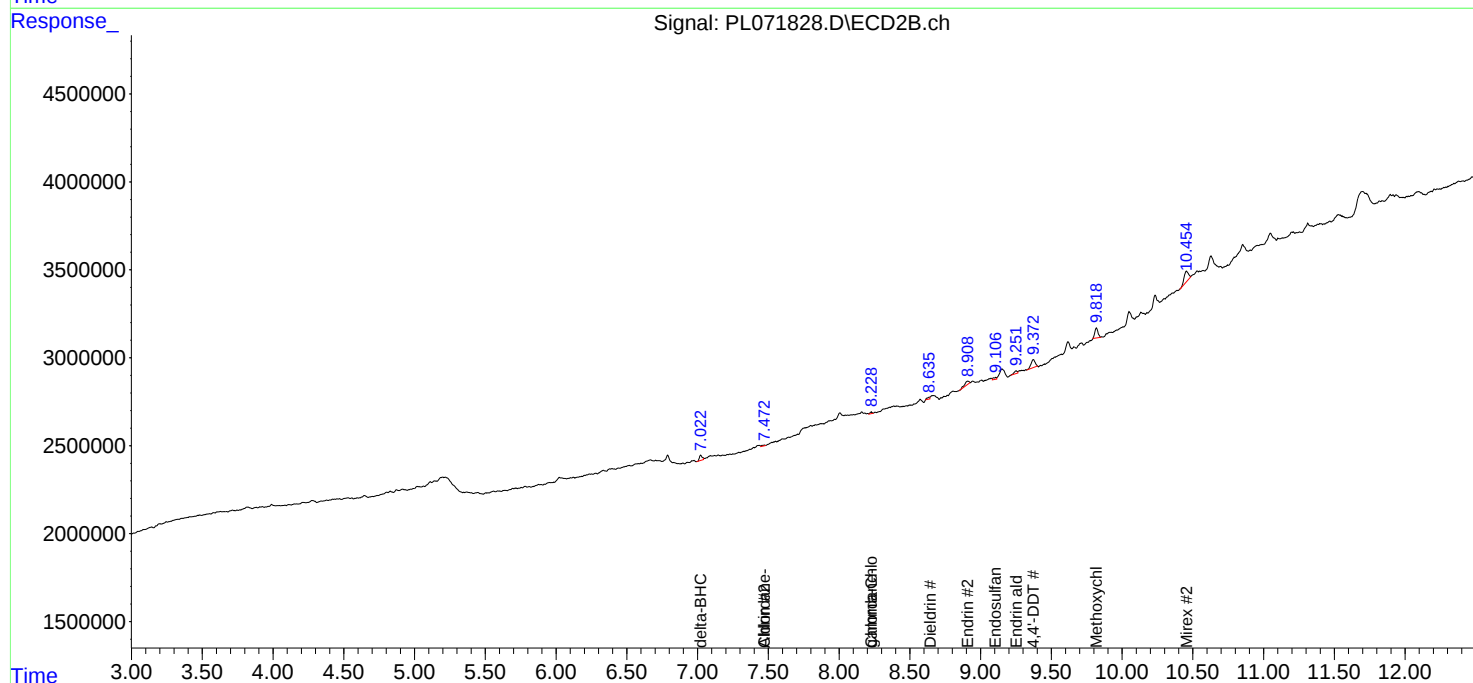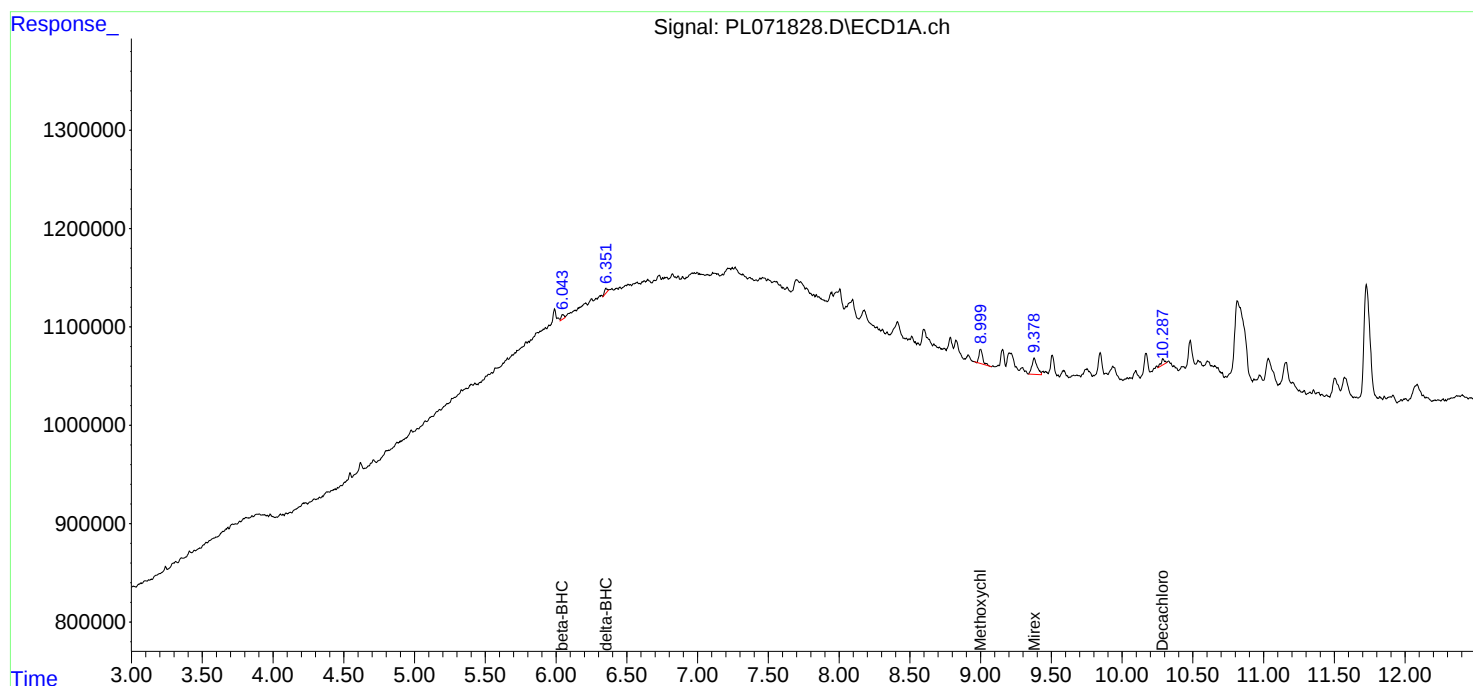


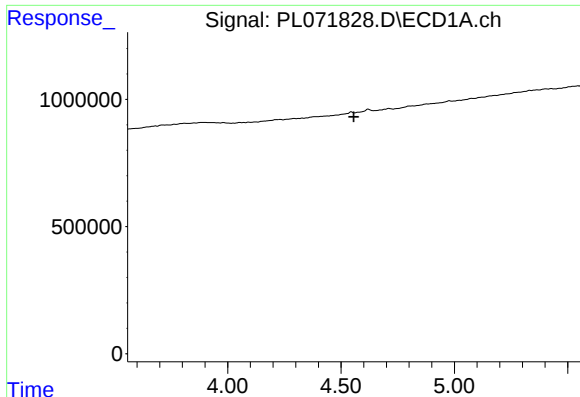

#1 Tetrachloro-m-xylene


R.T.: 4.545 min
Delta R.T.: -0.011 min
Response: -41872
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

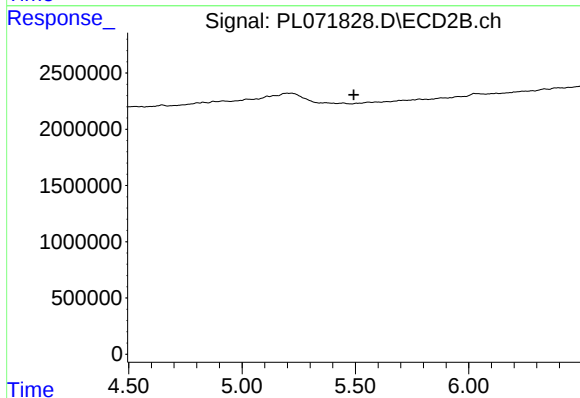


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.492 min
Response: 0
Conc: N.D.

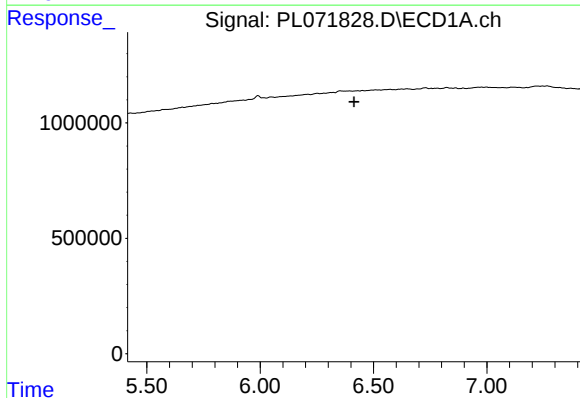


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 6.414 min
Response: 0
Conc: N.D.

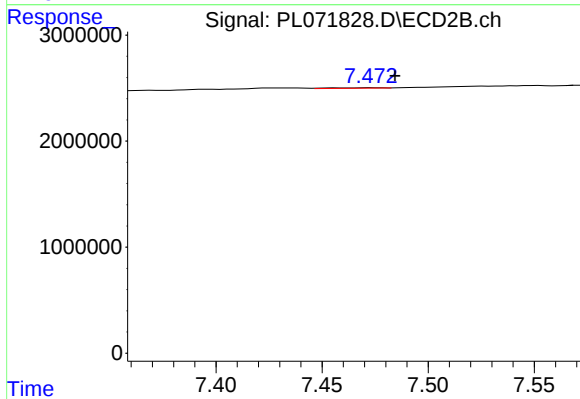

#5 Aldrin


R.T.: 7.473 min
Delta R.T.: -0.011 min
Response: 78259
Conc: 0.05 ng/ml

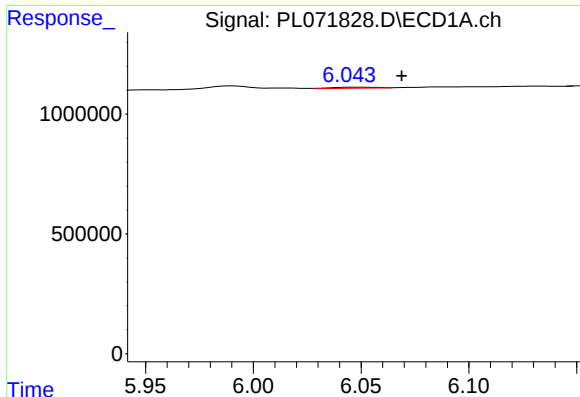

#6 beta-BHC


R.T.: 6.045 min
Delta R.T.: -0.024 min
Response: 65240
Conc: 0.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

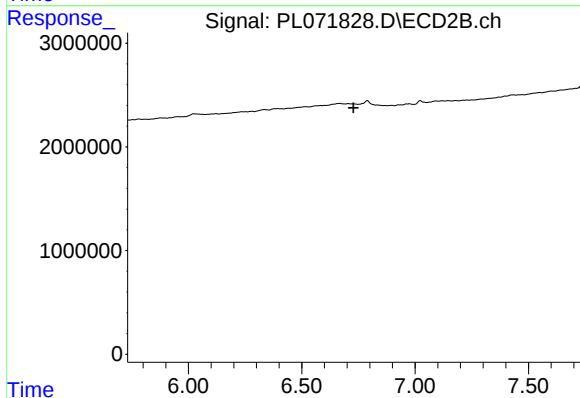


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.729 min
Response: 0
Conc: N.D.

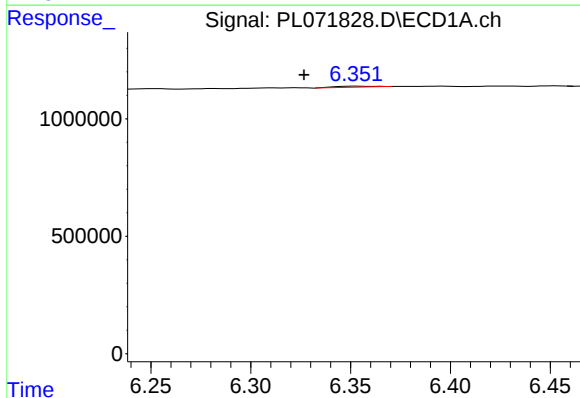


#7 delta-BHC

R.T.: 6.353 min
Delta R.T.: 0.026 min
Response: 61327
Conc: 0.10 ng/ml

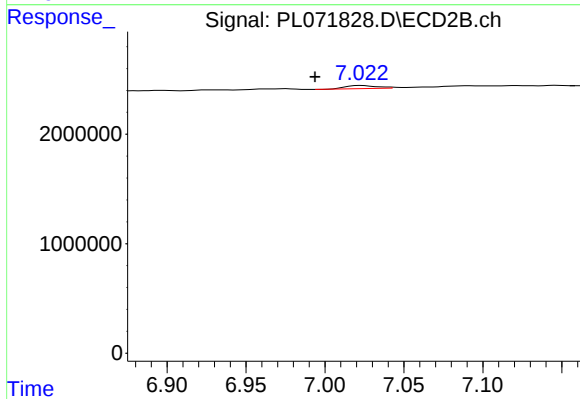

#7 delta-BHC


R.T.: 7.023 min
Delta R.T.: 0.029 min
Response: 414843
Conc: 0.27 ng/ml

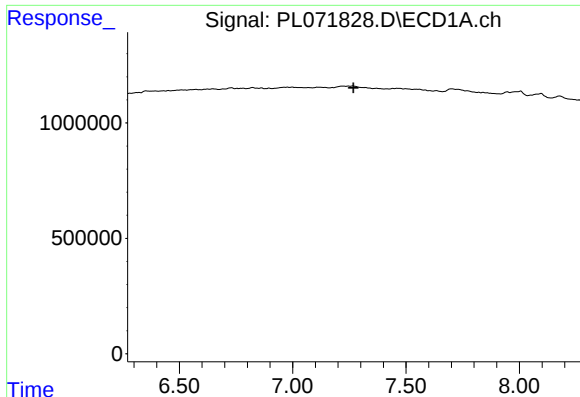

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

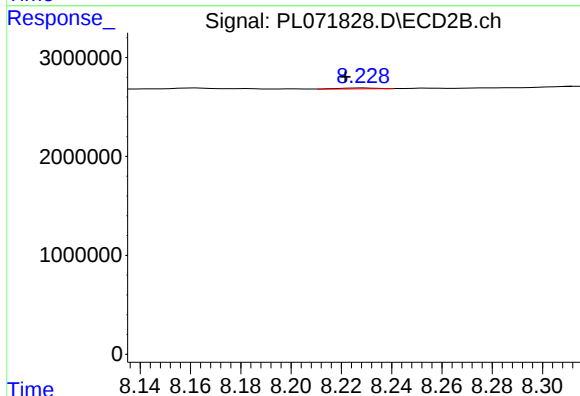


#10 gamma-Chlordane

R.T.: 8.229 min
Delta R.T.: 0.007 min
Response: 99671
Conc: 0.07 ng/ml

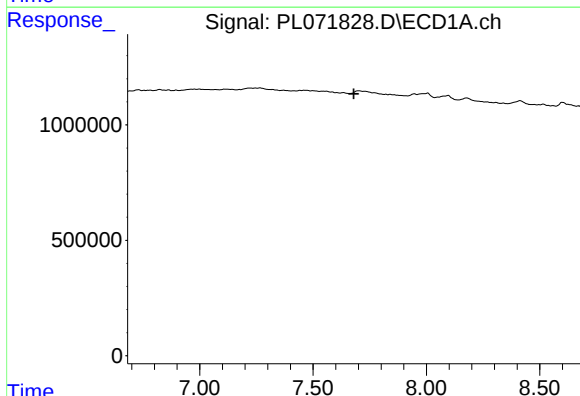


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 7.680 min
Response: 0
Conc: N.D.

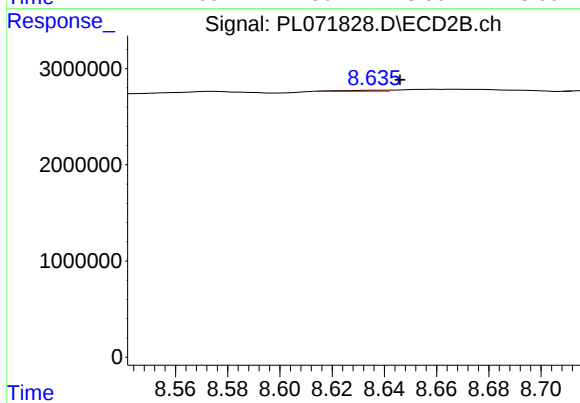

#13 Dieldrin


R.T.: 8.638 min
Delta R.T.: -0.008 min
Response: 134121
Conc: 0.10 ng/ml

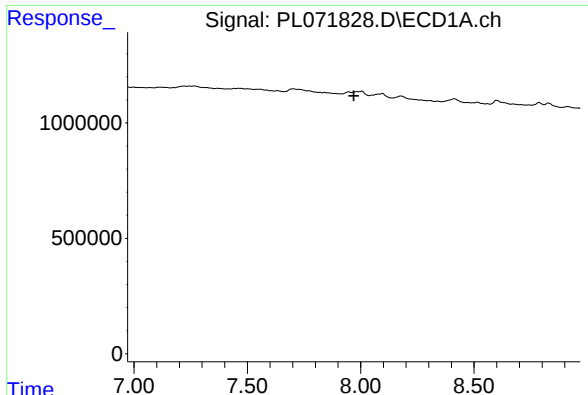

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 7.970 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

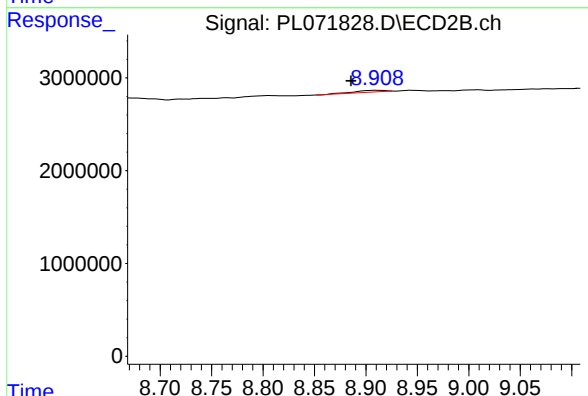


#14 Endrin

R.T.: 8.910 min
Delta R.T.: 0.024 min
Response: 478851
Conc: 0.46 ng/ml

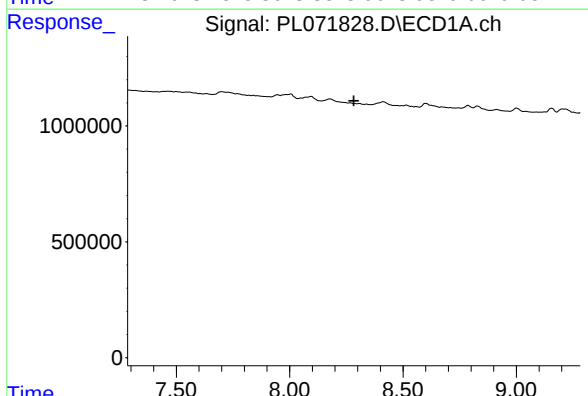


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.283 min
Response: 0
Conc: N.D.

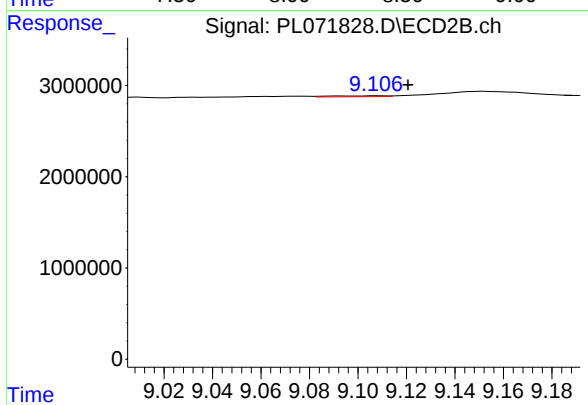

#15 Endosulfan II


R.T.: 9.108 min
Delta R.T.: -0.012 min
Response: 166569
Conc: 0.15 ng/ml

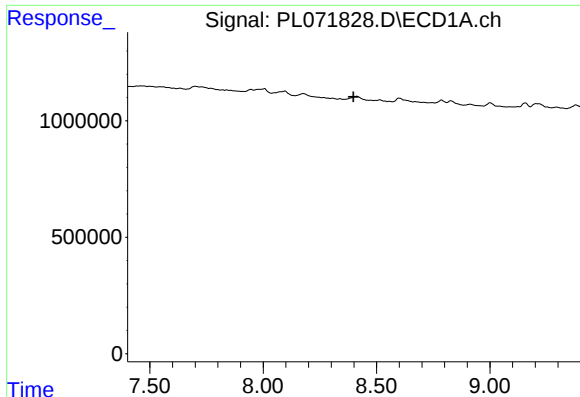

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

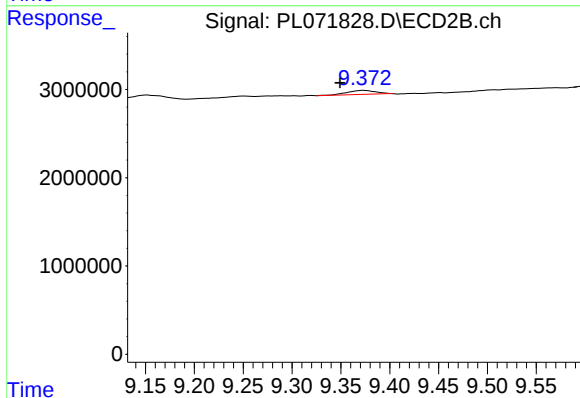


#17 4,4'-DDT

R.T.: 9.373 min
Delta R.T.: 0.024 min
Response: 941851
Conc: 1.00 ng/ml

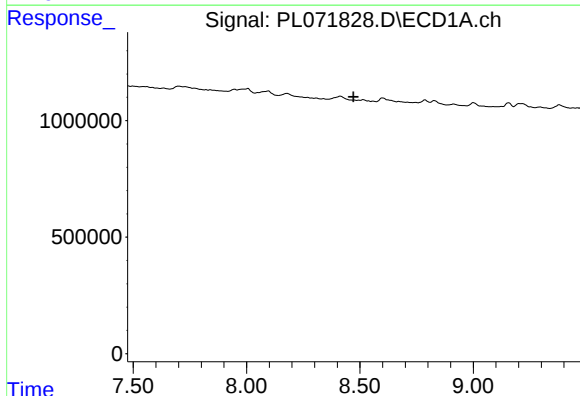


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 8.472 min
Response: 0
Conc: N.D.

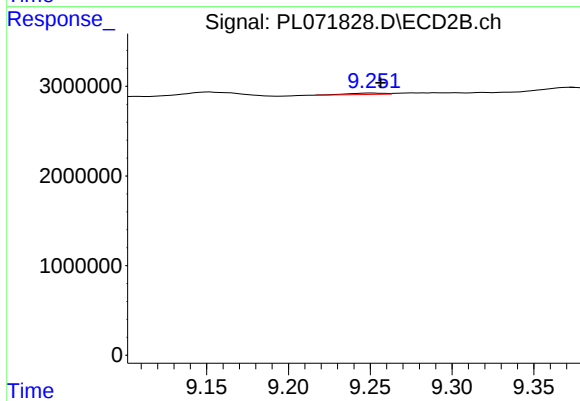

#18 Endrin aldehyde


R.T.: 9.252 min
Delta R.T.: -0.005 min
Response: 227336
Conc: 0.27 ng/ml

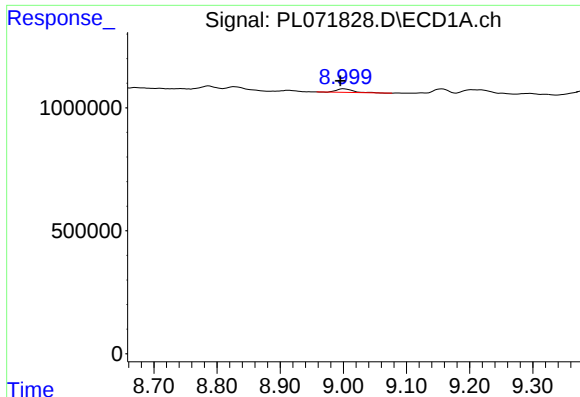

#20 Methoxychlor


R.T.: 9.000 min
Delta R.T.: 0.005 min
Response: 269407
Conc: 0.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

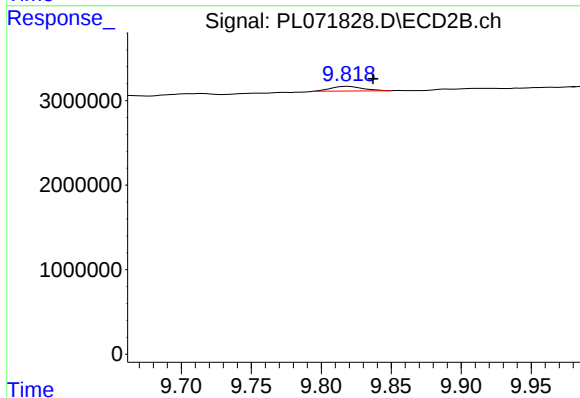


#20 Methoxychlor

R.T.: 9.819 min
Delta R.T.: -0.018 min
Response: 891464
Conc: 1.81 ng/ml

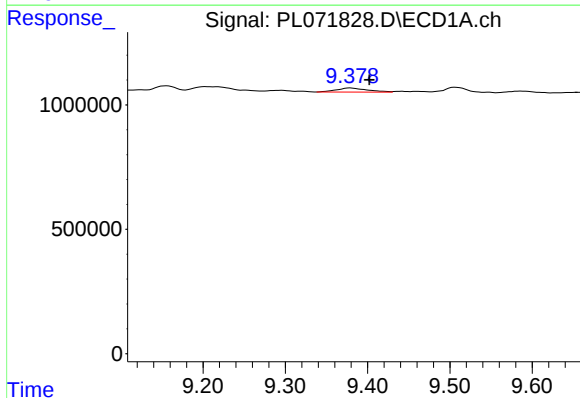


#22 Mirex

R.T.: 9.379 min
Delta R.T.: -0.023 min
Response: 421650
Conc: 0.70 ng/ml

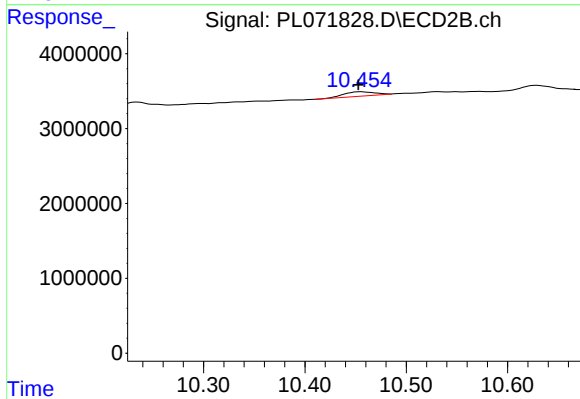

#22 Mirex


R.T.: 10.455 min
Delta R.T.: 0.002 min
Response: 1233450
Conc: 1.44 ng/ml

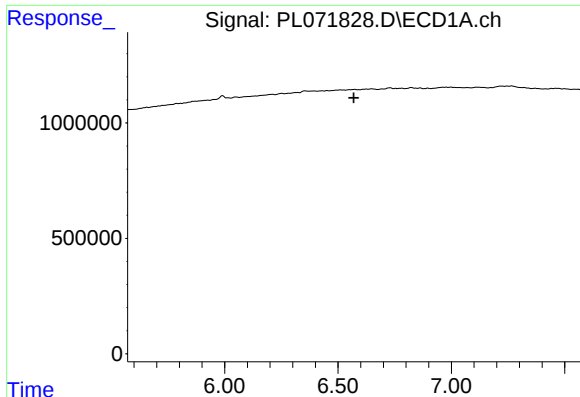

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 6.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

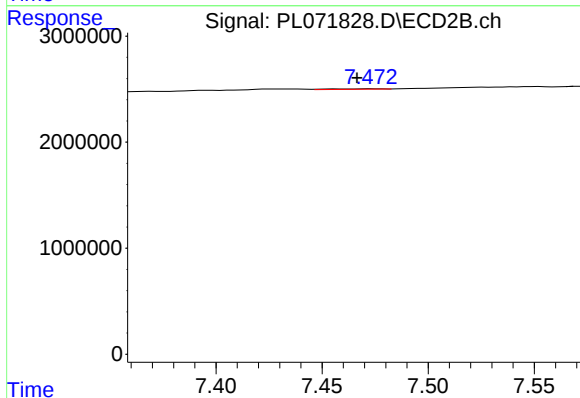


#24 Chlordane-2

R.T.: 7.473 min
Delta R.T.: 0.007 min
Response: 78259
Conc: 1.45 ng/ml

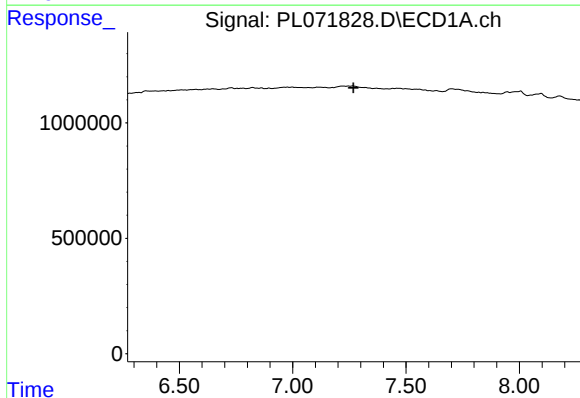


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

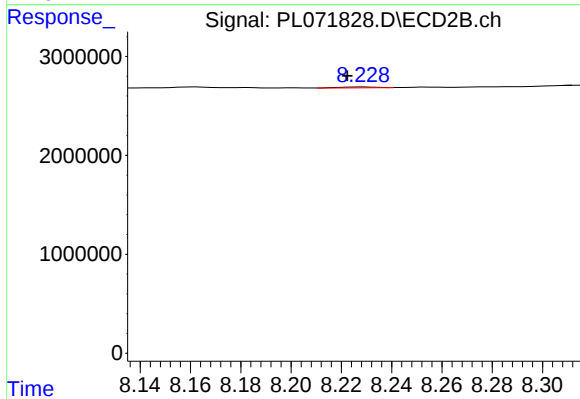

#25 Chlordane-3


R.T.: 8.229 min
Delta R.T.: 0.006 min
Response: 99671
Conc: 0.49 ng/ml

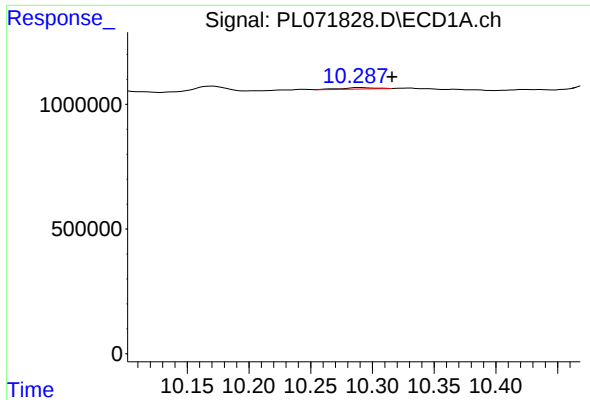

#28 Decachlorobiphenyl

R.T.: 10.289 min
Delta R.T.: -0.027 min
Response: 104317
Conc: 0.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

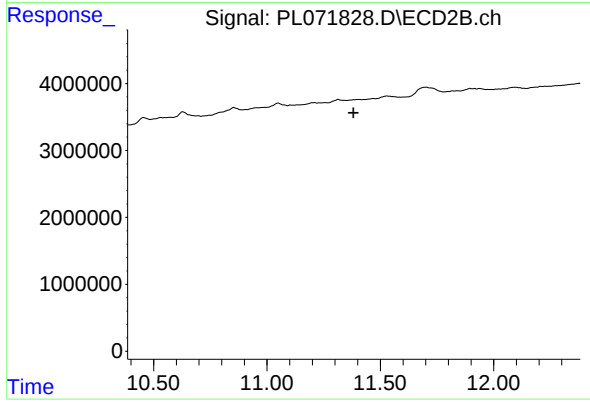

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.382 min
Response: 0
Conc: N.D.