

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010622\
 Data File : PL071832.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jan 2022 10:30
 Operator : AR\AJ
 Sample : PB141873BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 00:03:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.558	5.494	9006407	23423586	19.497	19.065
28)	SA Decachlor...	10.319	11.386	14481869	23646578	20.030	19.955
Target Compounds							
2)	A alpha-BHC	5.259	0.000	358452	0	0.581	N.D. #
7)	B delta-BHC	0.000	7.019f	0	1499841	N.D.	0.977 #
9)	A Endosulfan I	0.000	8.334f	0	171555	N.D.	0.139 #
10)	B gamma-Chl...	0.000	8.225	0	149553	N.D.	0.109 #
15)	B Endosulfa...	0.000	9.150f	0	639285	N.D.	0.569 #
16)	A 4,4'-DDD	0.000	9.003f	0	227127	N.D.	0.236 #
19)	B Endosulfa...	0.000	9.517f	0	81236	N.D.	0.078 #
25)	Chlordane-3	0.000	8.225	0	149553	N.D.	0.733 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010622\
Data File : PL071832.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jan 2022 10:30
Operator : AR\AJ
Sample : PB141873BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 00:03:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

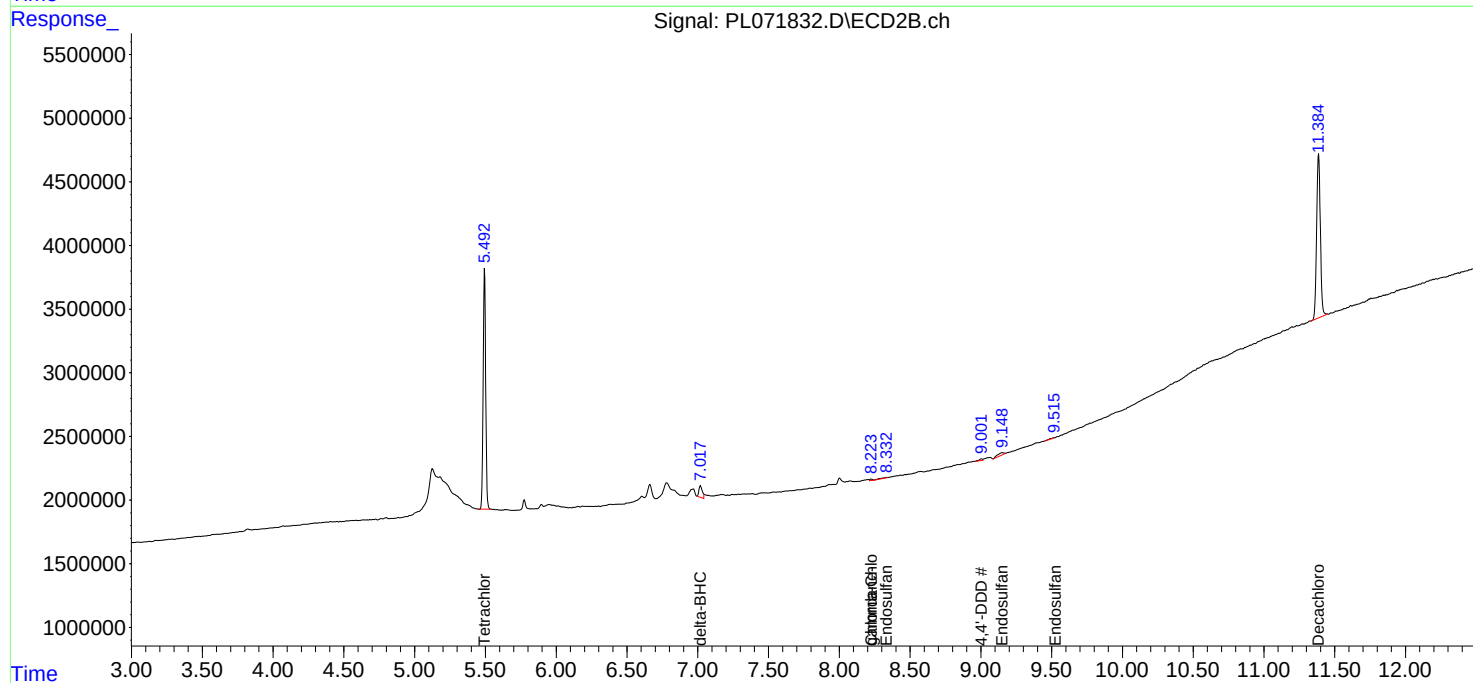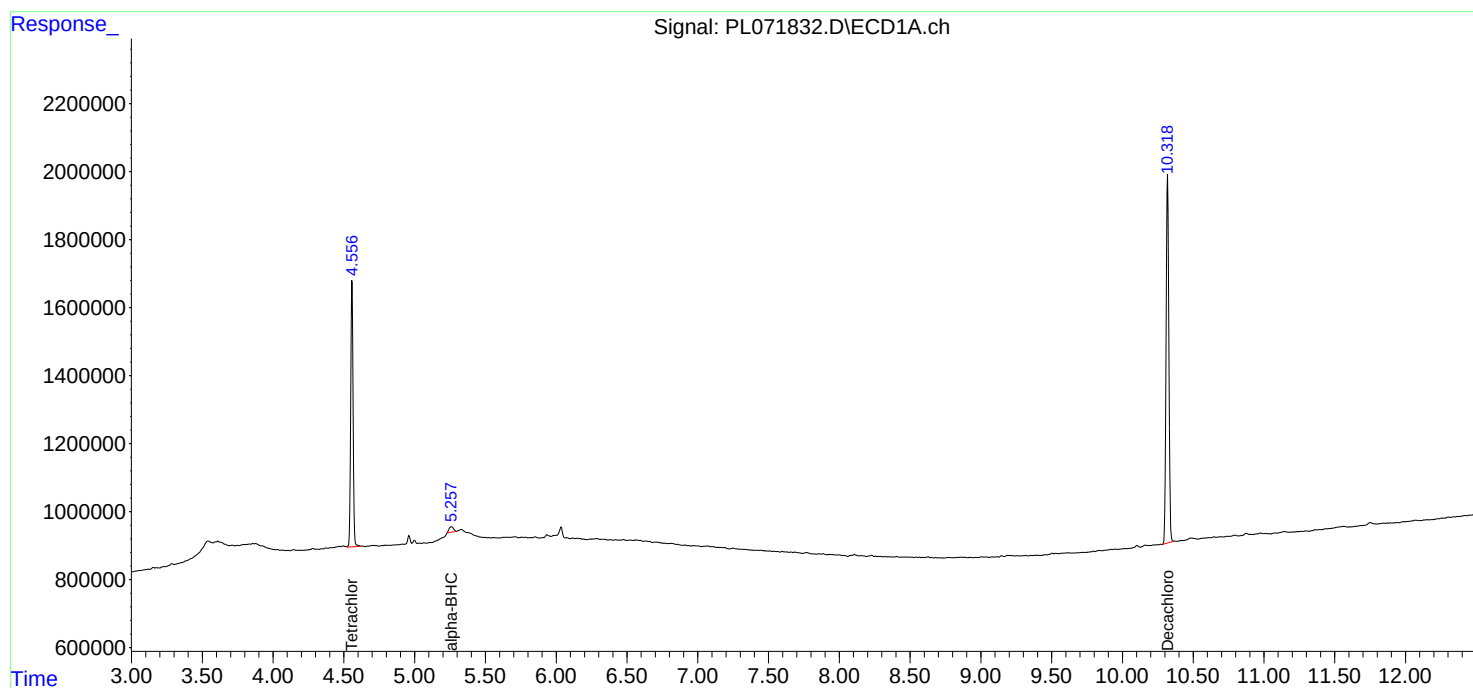


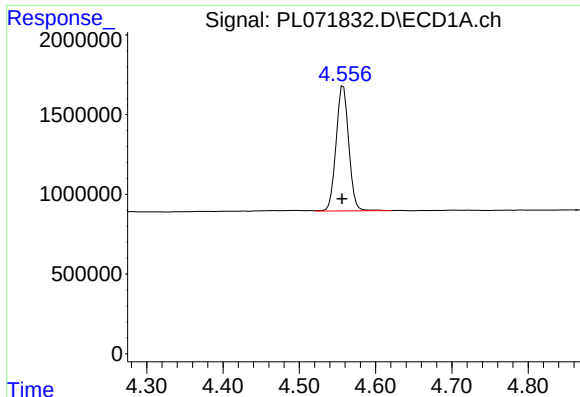

#1 Tetrachloro-m-xylene


R.T.: 4.558 min
Delta R.T.: 0.002 min
Response: 9006407
Conc: 19.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

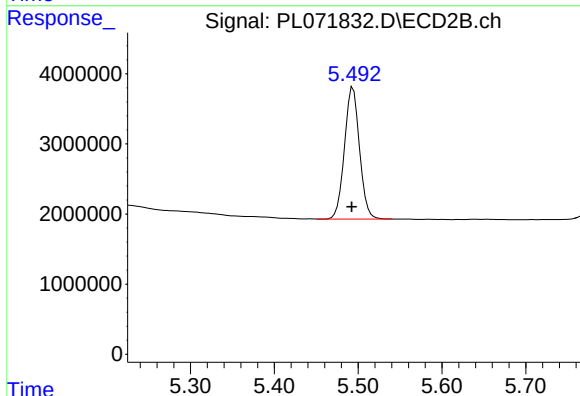


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.001 min
Response: 23423586
Conc: 19.06 ng/ml

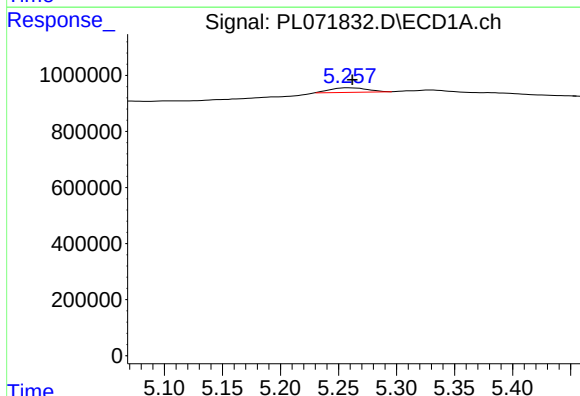


#2 alpha-BHC

R.T.: 5.259 min
Delta R.T.: -0.003 min
Response: 358452
Conc: 0.58 ng/ml

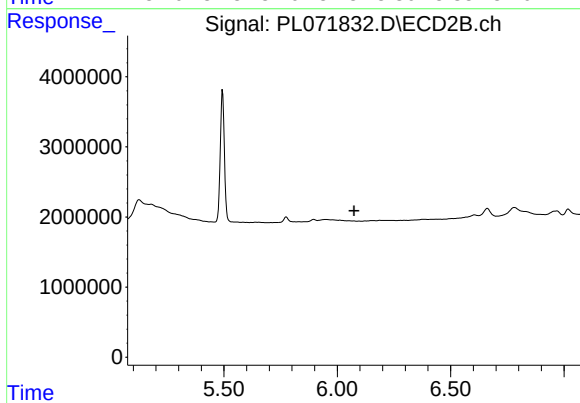

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.074 min
Response: 0
Conc: N.D.

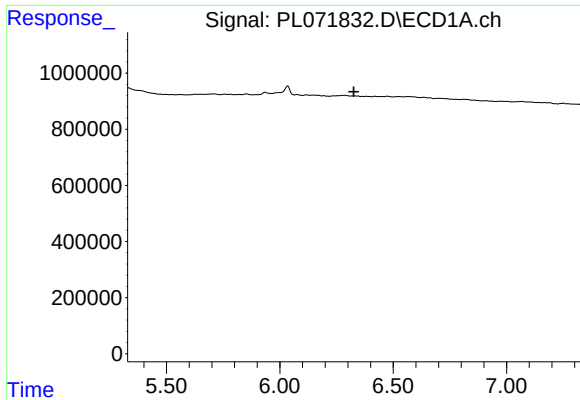

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.327 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

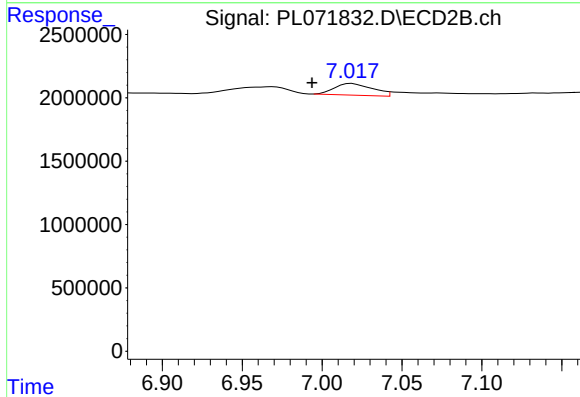


#7 delta-BHC

R.T.: 7.019 min
Delta R.T.: 0.025 min
Response: 1499841
Conc: 0.98 ng/ml

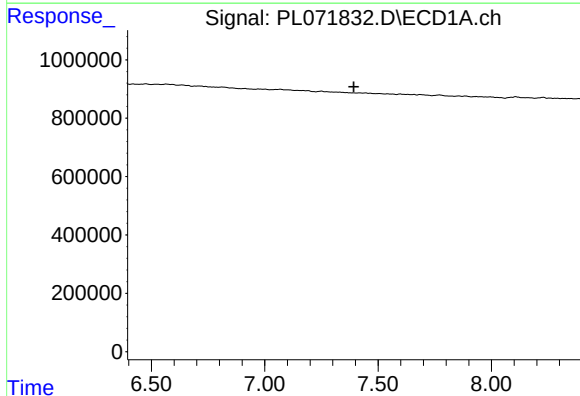


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.393 min
Response: 0
Conc: N.D.

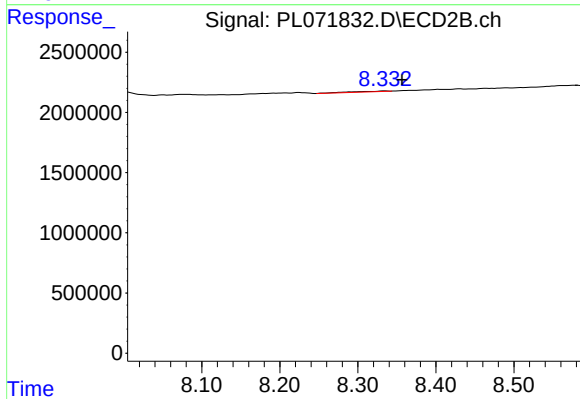

#9 Endosulfan I


R.T.: 8.334 min
Delta R.T.: -0.023 min
Response: 171555
Conc: 0.14 ng/ml

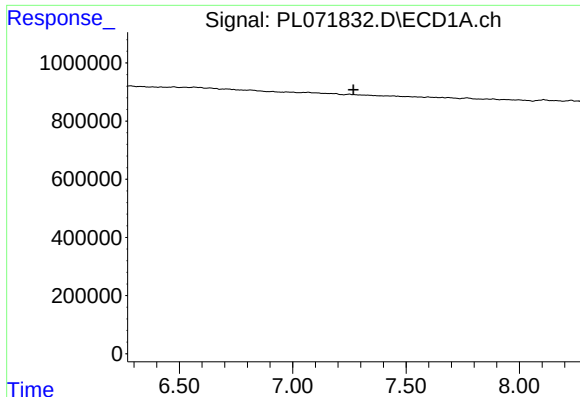

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

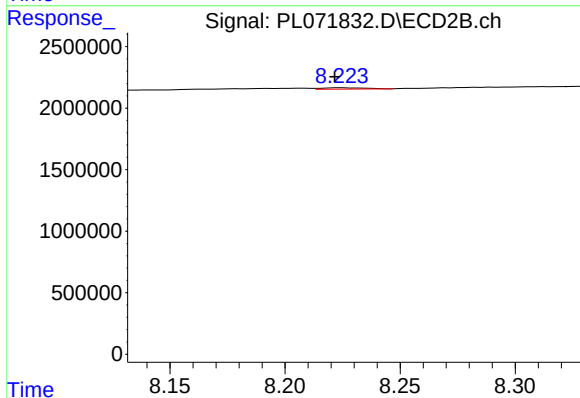


#10 gamma-Chlordane

R.T.: 8.225 min
Delta R.T.: 0.003 min
Response: 149553
Conc: 0.11 ng/ml

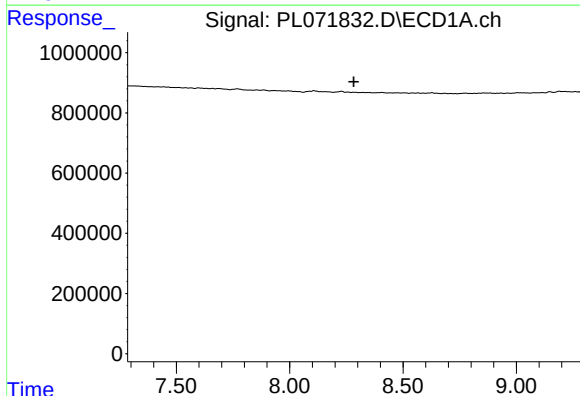


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.283 min
Response: 0
Conc: N.D.

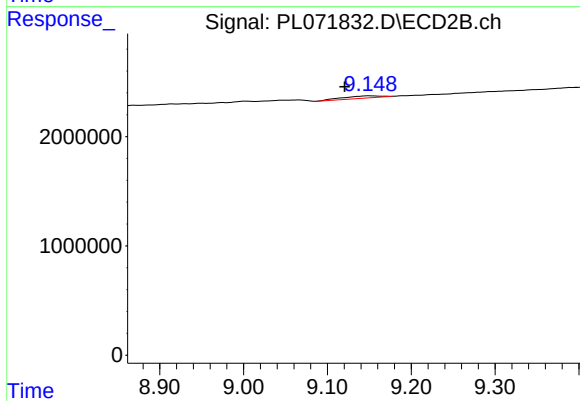

#15 Endosulfan II


R.T.: 9.150 min
Delta R.T.: 0.030 min
Response: 639285
Conc: 0.57 ng/ml

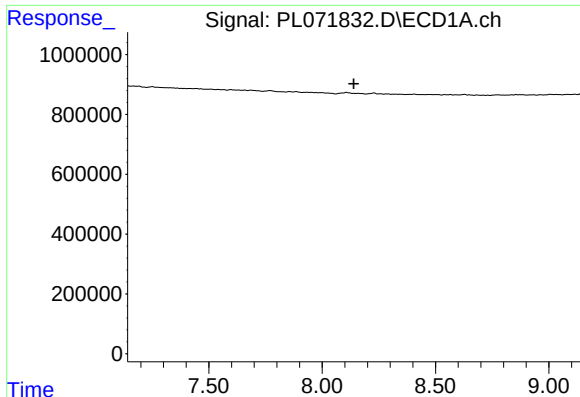

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.139 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

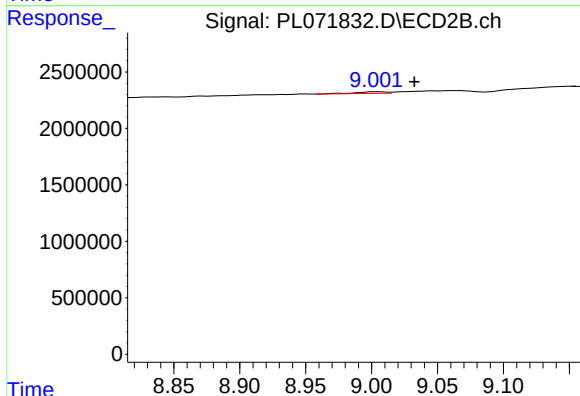


#16 4,4'-DDD

R.T.: 9.003 min
Delta R.T.: -0.029 min
Response: 227127
Conc: 0.24 ng/ml

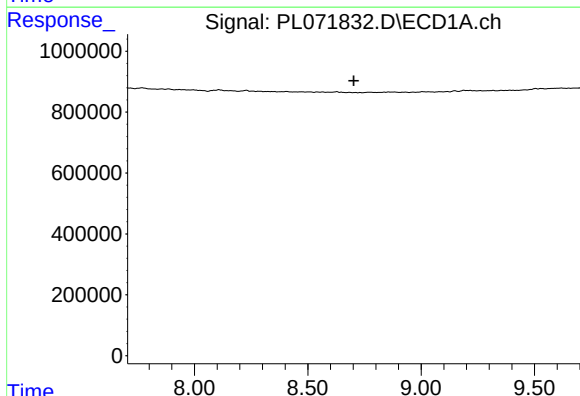


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.703 min
Response: 0
Conc: N.D.

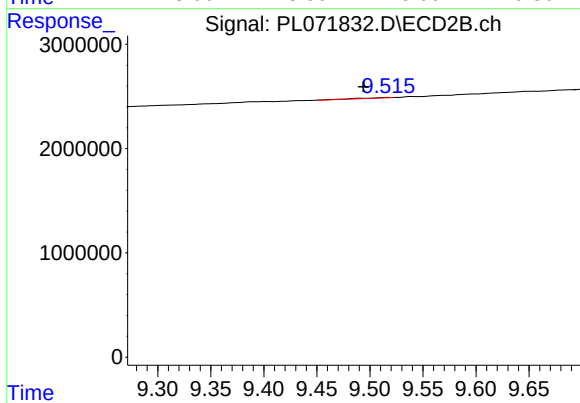

#19 Endosulfan Sulfate


R.T.: 9.517 min
Delta R.T.: 0.023 min
Response: 81236
Conc: 0.08 ng/ml

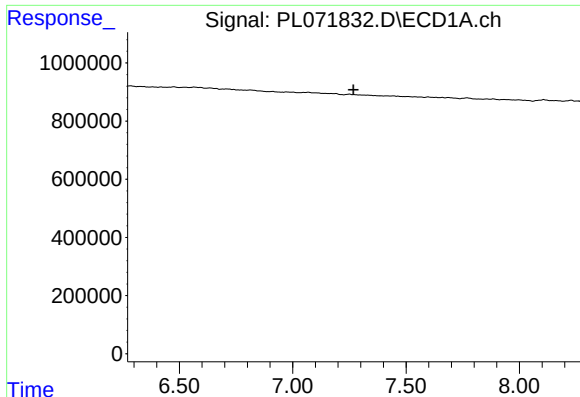

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

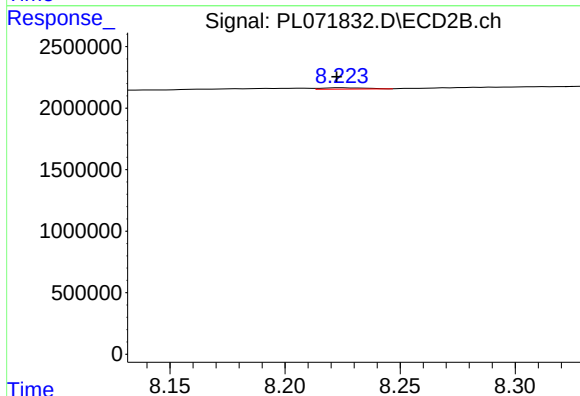


#25 Chlordane-3

R.T.: 8.225 min
Delta R.T.: 0.002 min
Response: 149553
Conc: 0.73 ng/ml

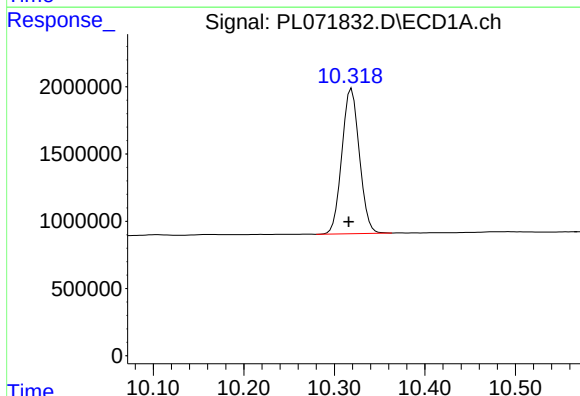

#28 Decachlorobiphenyl

R.T.: 10.319 min
Delta R.T.: 0.003 min
Response: 14481869
Conc: 20.03 ng/ml

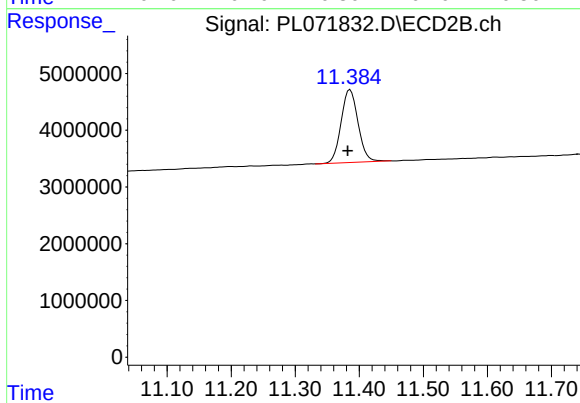

#28 Decachlorobiphenyl

R.T.: 11.386 min
Delta R.T.: 0.004 min
Response: 23646578
Conc: 19.95 ng/ml