

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010622\
 Data File : PL071834.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jan 2022 11:12
 Operator : AR\AJ
 Sample : PB141830TB
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 00:04:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.563	5.494	8811576	23184565	19.075	18.870
28)	SA Decachlor...	10.324	11.388	14471409	23793200	20.015	20.078
Target Compounds							
4)	MA Heptachlor	0.000	7.124	0	818517	N.D.	0.511 #
6)	B beta-BHC	6.042f	6.733	390764	5851092	1.444	8.189 #
7)	B delta-BHC	0.000	6.973f	0	422106	N.D.	0.275 #
10)	B gamma-Chl...	0.000	8.228	0	181778	N.D.	0.133 #
11)	B alpha-Chl...	0.000	8.298	0	54389	N.D.	0.041 #
18)	B Endrin al...	0.000	9.255	0	36511	N.D.	0.043 #
20)	A Methoxychlor	0.000	9.820f	0	36205	N.D.	0.074 #
23)	Chlordane-1	5.898f	6.865	393341	236603	21.899	4.777 #
25)	Chlordane-3	0.000	8.228	0	181778	N.D.	0.891 #
26)	Chlordane-4	0.000	8.298	0	54389	N.D.	0.223 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010622\
Data File : PL071834.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jan 2022 11:12
Operator : AR\AJ
Sample : PB141830TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 00:04:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

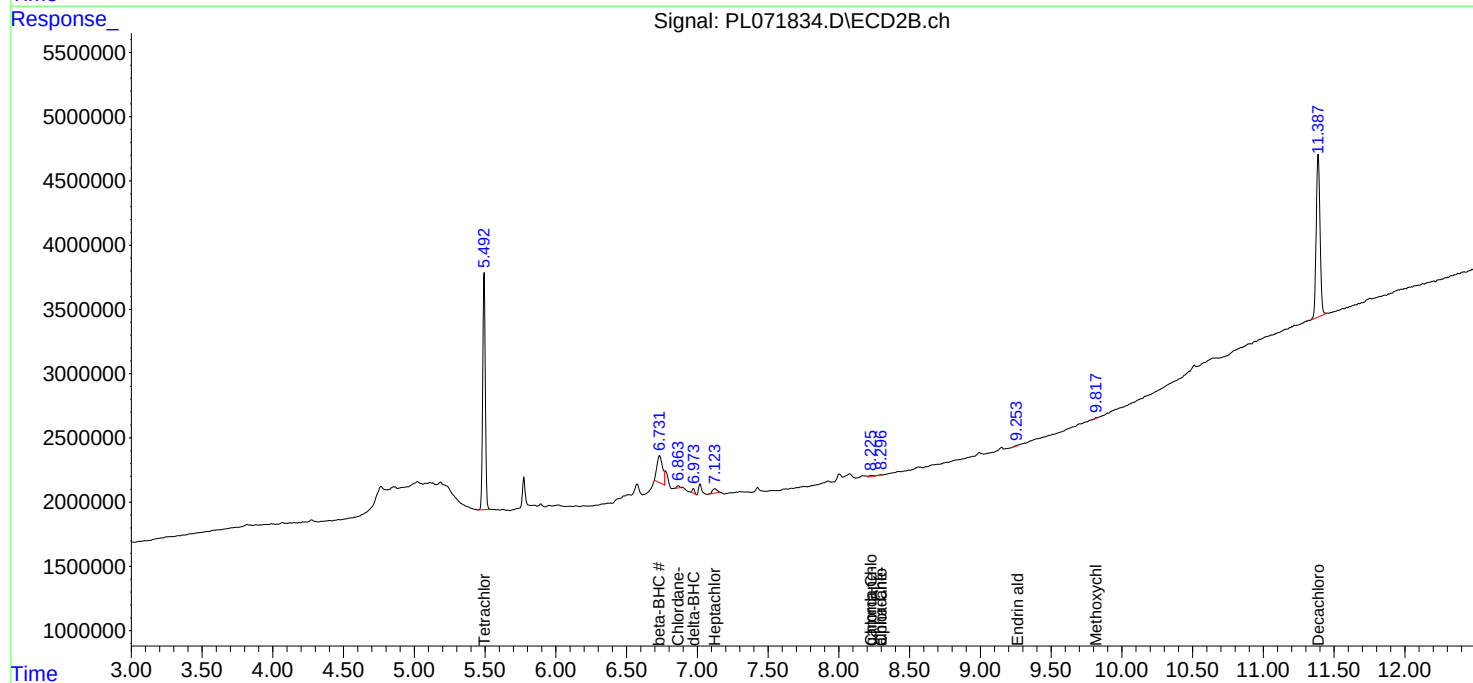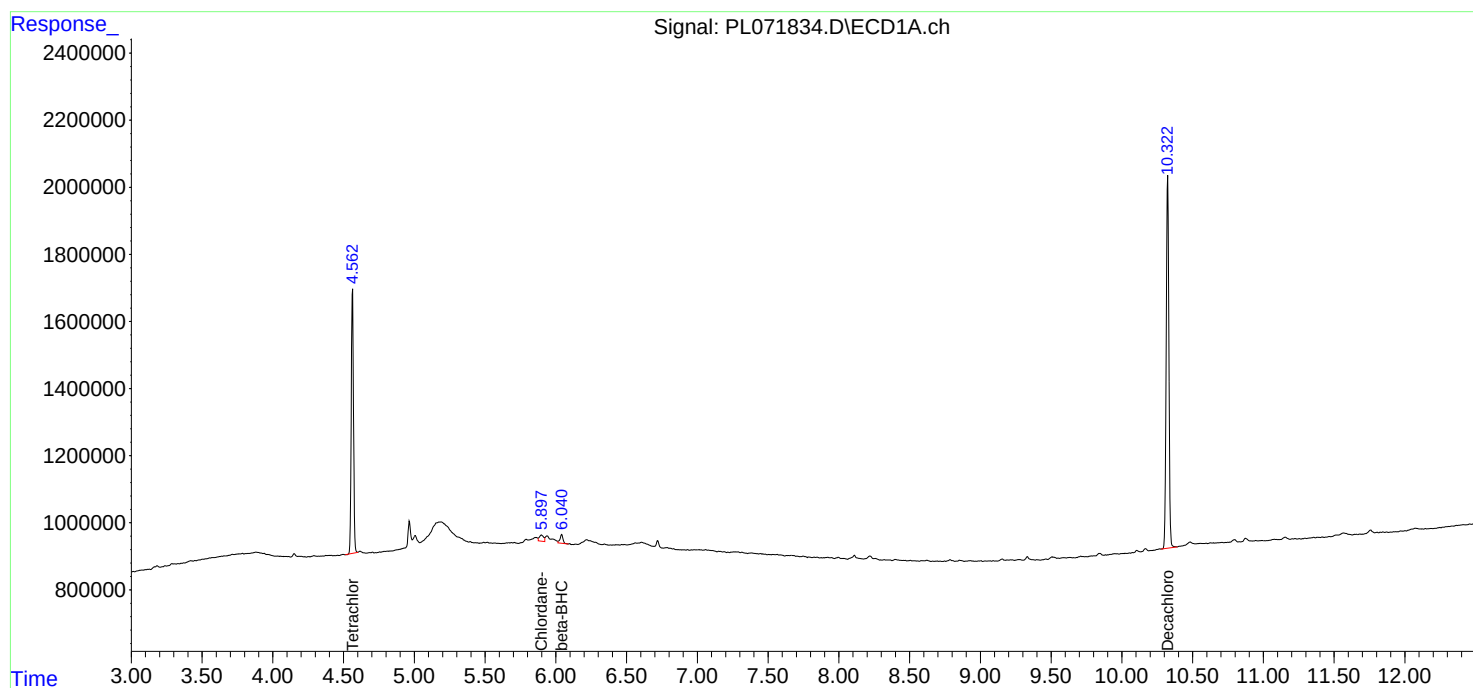


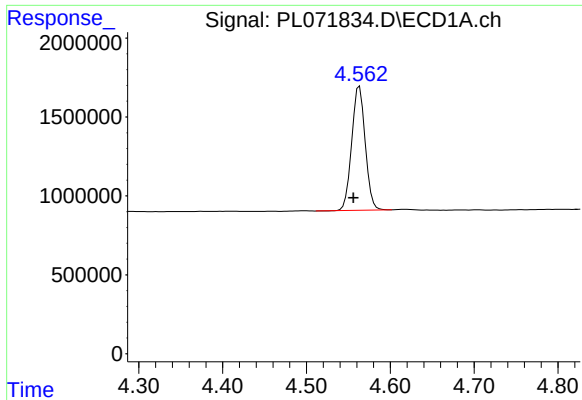

#1 Tetrachloro-m-xylene


R.T.: 4.563 min
Delta R.T.: 0.007 min
Response: 8811576
Conc: 19.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

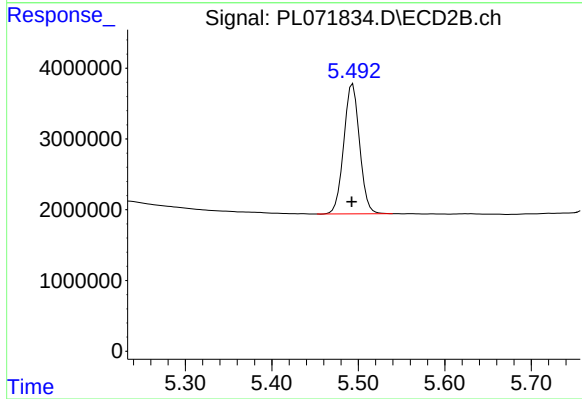


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.001 min
Response: 23184565
Conc: 18.87 ng/ml

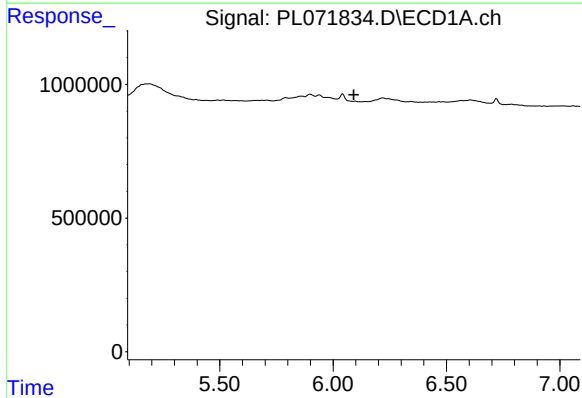


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 6.091 min
Response: 0
Conc: N.D.

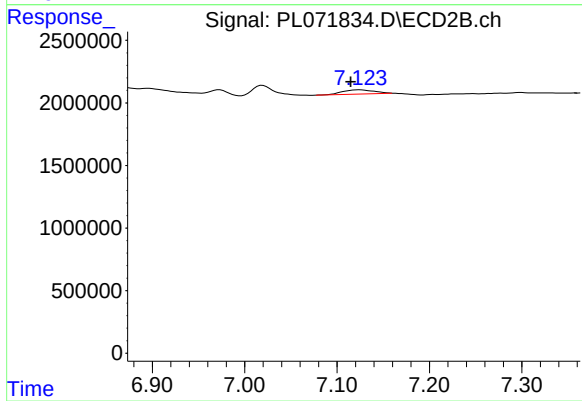

#4 Heptachlor


R.T.: 7.124 min
Delta R.T.: 0.009 min
Response: 818517
Conc: 0.51 ng/ml

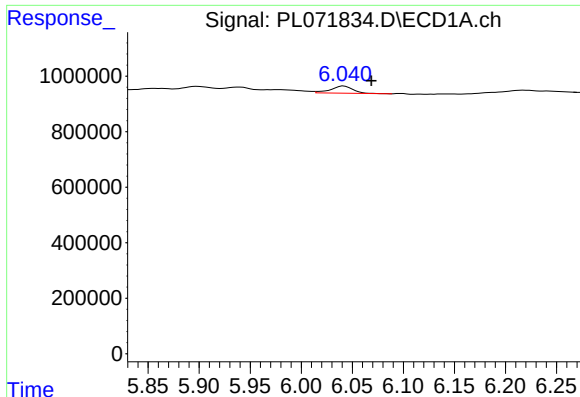

#6 beta-BHC


R.T.: 6.042 min
Delta R.T.: -0.027 min
Response: 390764
Conc: 1.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

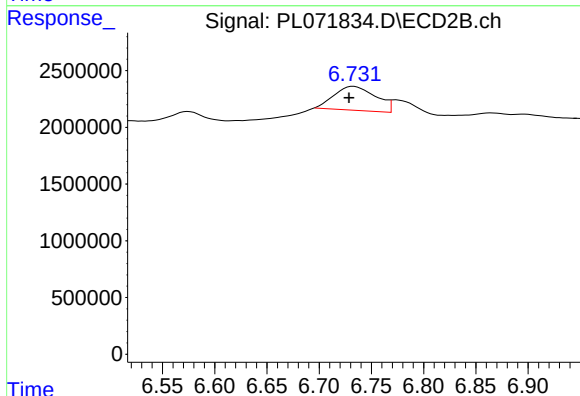


#6 beta-BHC

R.T.: 6.733 min
Delta R.T.: 0.004 min
Response: 5851092
Conc: 8.19 ng/ml

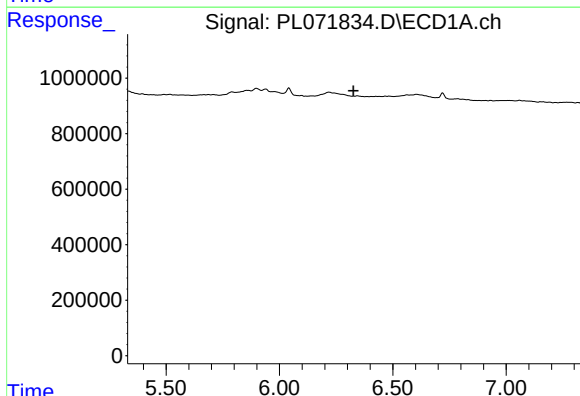


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.327 min
Response: 0
Conc: N.D.

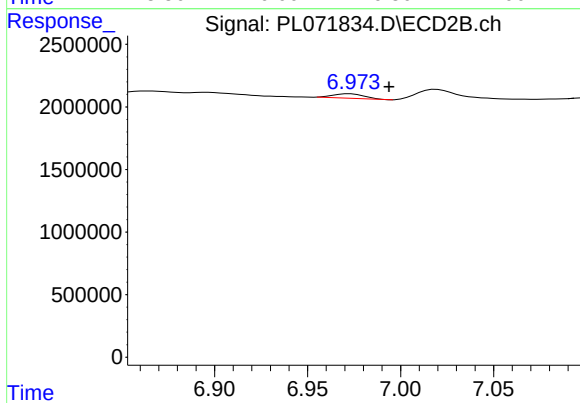

#7 delta-BHC


R.T.: 6.973 min
Delta R.T.: -0.021 min
Response: 422106
Conc: 0.27 ng/ml

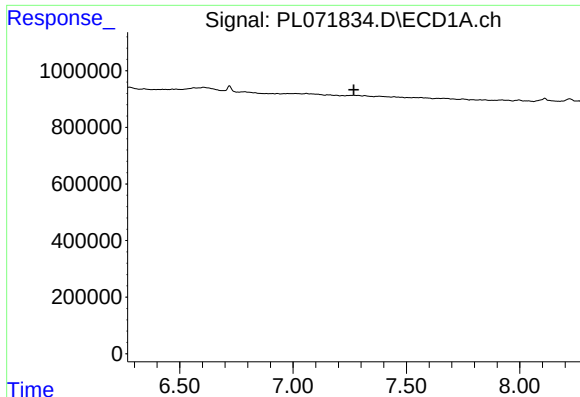

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

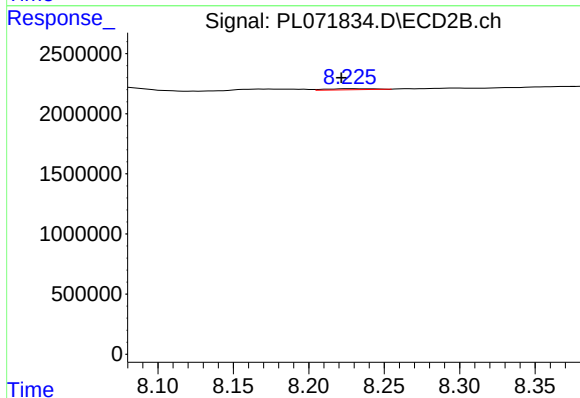


#10 gamma-Chlordane

R.T.: 8.228 min
Delta R.T.: 0.006 min
Response: 181778
Conc: 0.13 ng/ml

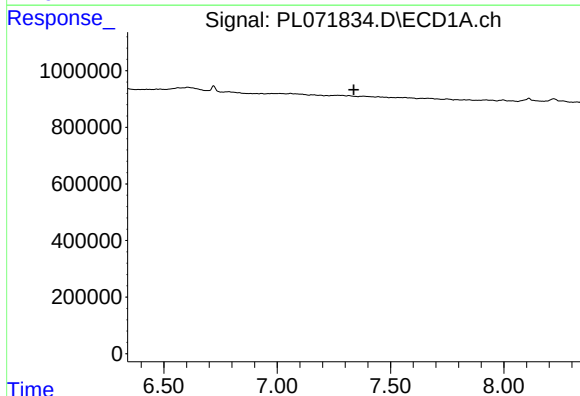


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.338 min
Response: 0
Conc: N.D.

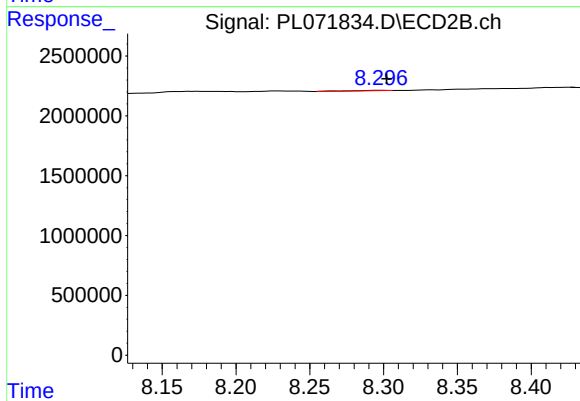

#11 alpha-Chlordane


R.T.: 8.298 min
Delta R.T.: -0.004 min
Response: 54389
Conc: 0.04 ng/ml

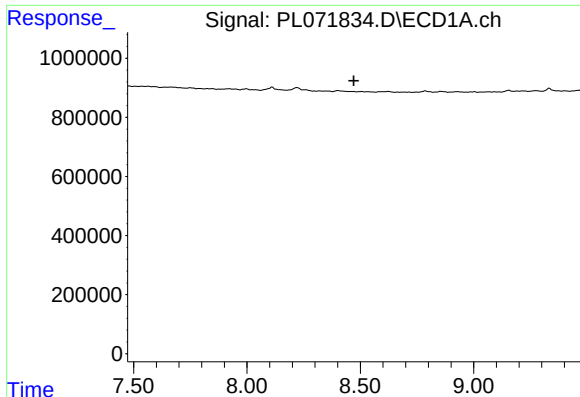

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 8.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

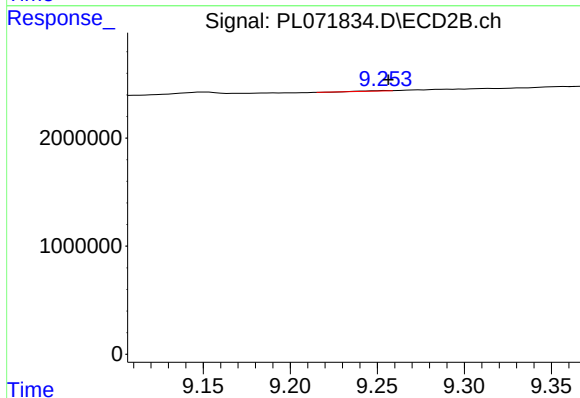


#18 Endrin aldehyde

R.T.: 9.255 min
Delta R.T.: -0.001 min
Response: 36511
Conc: 0.04 ng/ml

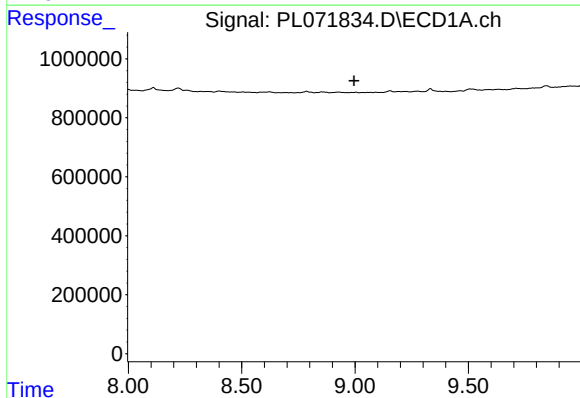


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 8.995 min
Response: 0
Conc: N.D.

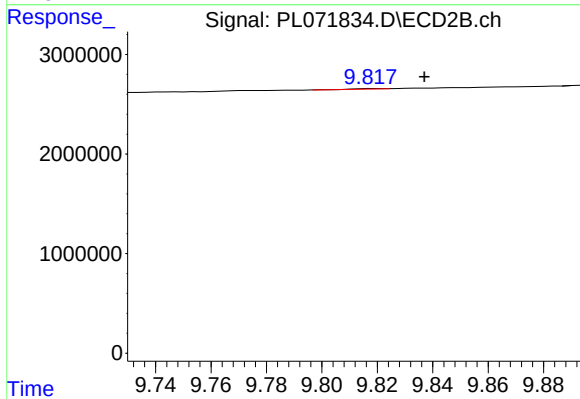

#20 Methoxychlor


R.T.: 9.820 min
Delta R.T.: -0.017 min
Response: 36205
Conc: 0.07 ng/ml

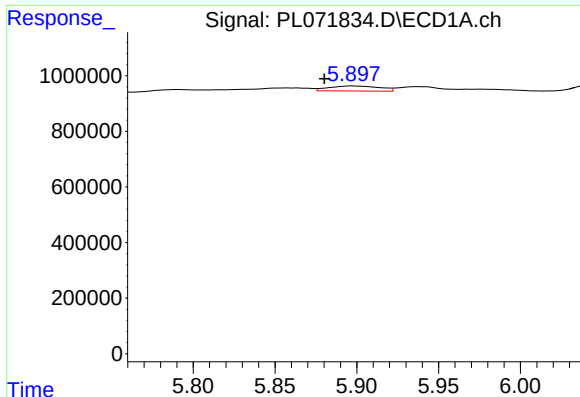

#23 Chlordane-1


R.T.: 5.898 min
Delta R.T.: 0.018 min
Response: 393341
Conc: 21.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

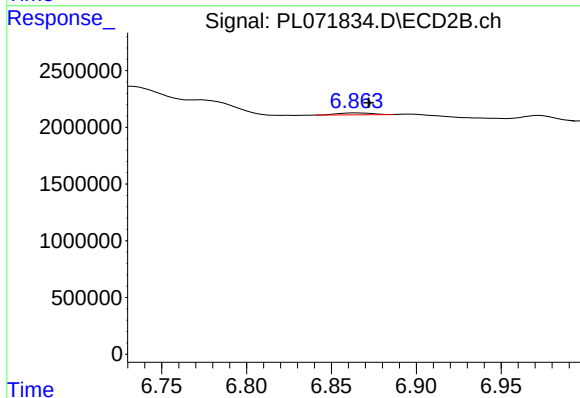


#23 Chlordane-1

R.T.: 6.865 min
Delta R.T.: -0.007 min
Response: 236603
Conc: 4.78 ng/ml

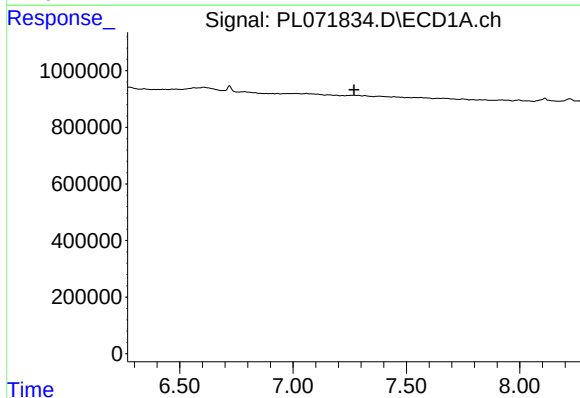


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.269 min
Response: 0
Conc: N.D.

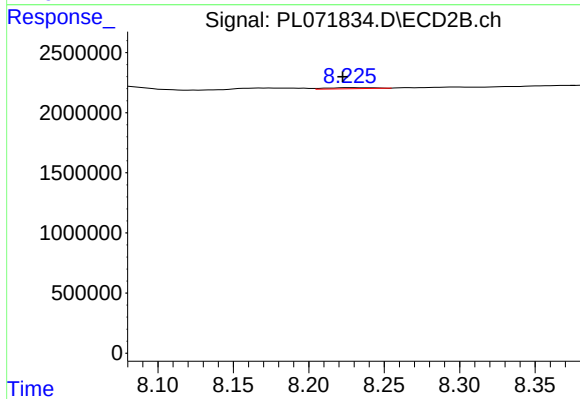

#25 Chlordane-3


R.T.: 8.228 min
Delta R.T.: 0.006 min
Response: 181778
Conc: 0.89 ng/ml

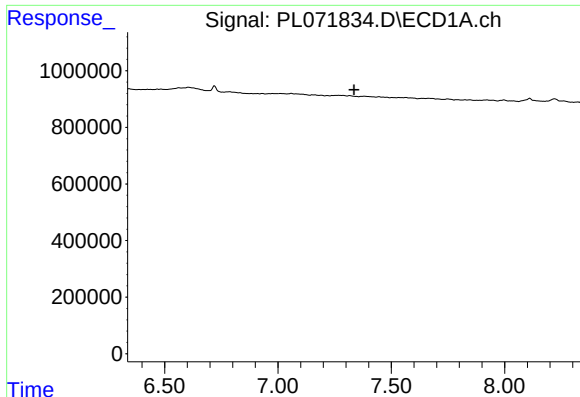

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.336 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

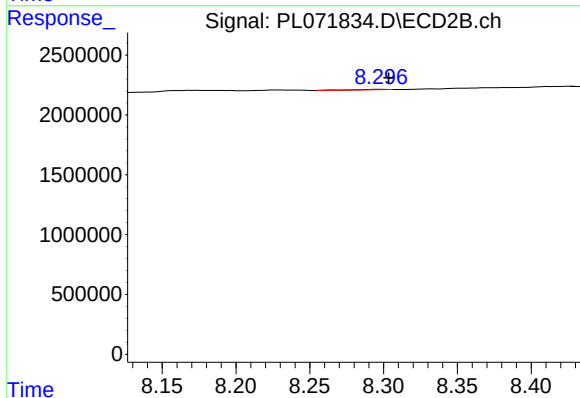


#26 Chlordane-4

R.T.: 8.298 min
Delta R.T.: -0.006 min
Response: 54389
Conc: 0.22 ng/ml

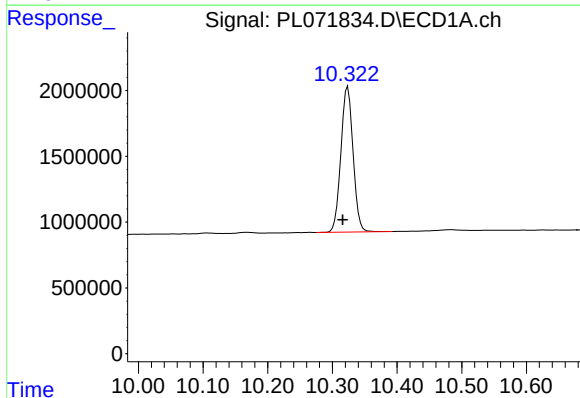

#28 Decachlorobiphenyl

R.T.: 10.324 min
Delta R.T.: 0.008 min
Response: 14471409
Conc: 20.02 ng/ml

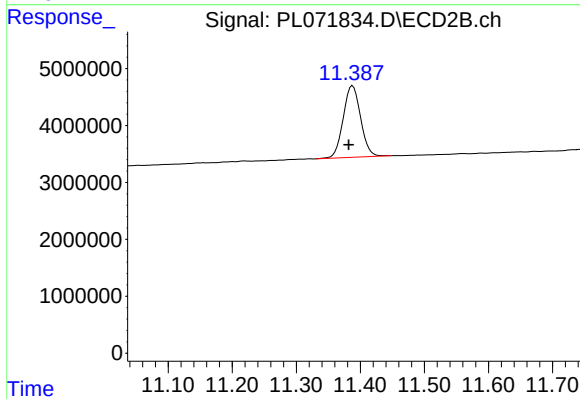

#28 Decachlorobiphenyl

R.T.: 11.388 min
Delta R.T.: 0.006 min
Response: 23793200
Conc: 20.08 ng/ml