

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010622\
 Data File : PL071835.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jan 2022 11:28
 Operator : AR\AJ
 Sample : N1014-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 00:04:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.558	5.494	9903439	25869500	21.438	21.055
28)	SA Decachlor...	10.320	11.387	15570999	25320465	21.536	21.367
Target Compounds							
7)	B delta-BHC	0.000	6.973f	0	1734607	N.D.	1.130 #
10)	B gamma-Chl...	0.000	8.220	0	325187	N.D.	0.238 #
11)	B alpha-Chl...	0.000	8.293	0	78264	N.D.	0.059 #
13)	MA Dieldrin	0.000	8.674f	0	180388	N.D.	0.137 #
15)	B Endosulfa...	0.000	9.150f	0	378831	N.D.	0.337 #
16)	A 4,4'-DDD	0.000	9.036	0	62922	N.D.	0.065 #
19)	B Endosulfa...	0.000	9.499	0	214084	N.D.	0.206 #
20)	A Methoxychlor	0.000	9.841	0	114143	N.D.	0.232 #
25)	Chlordane-3	0.000	8.220	0	325187	N.D.	1.593 #
26)	Chlordane-4	0.000	8.293	0	78264	N.D.	0.322 #
27)	Chlordane-5	0.000	9.176	0	13353	N.D.	0.333 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010622\
Data File : PL071835.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jan 2022 11:28
Operator : AR\AJ
Sample : N1014-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 00:04:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

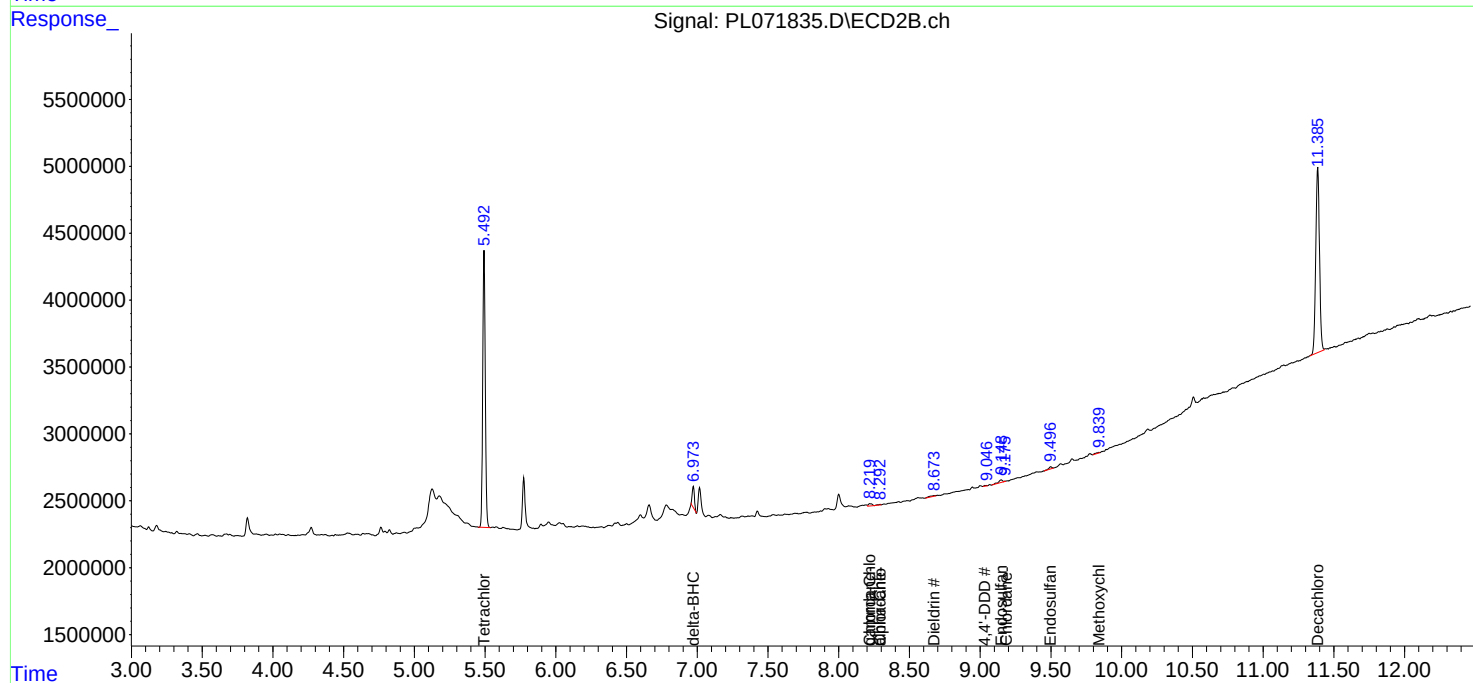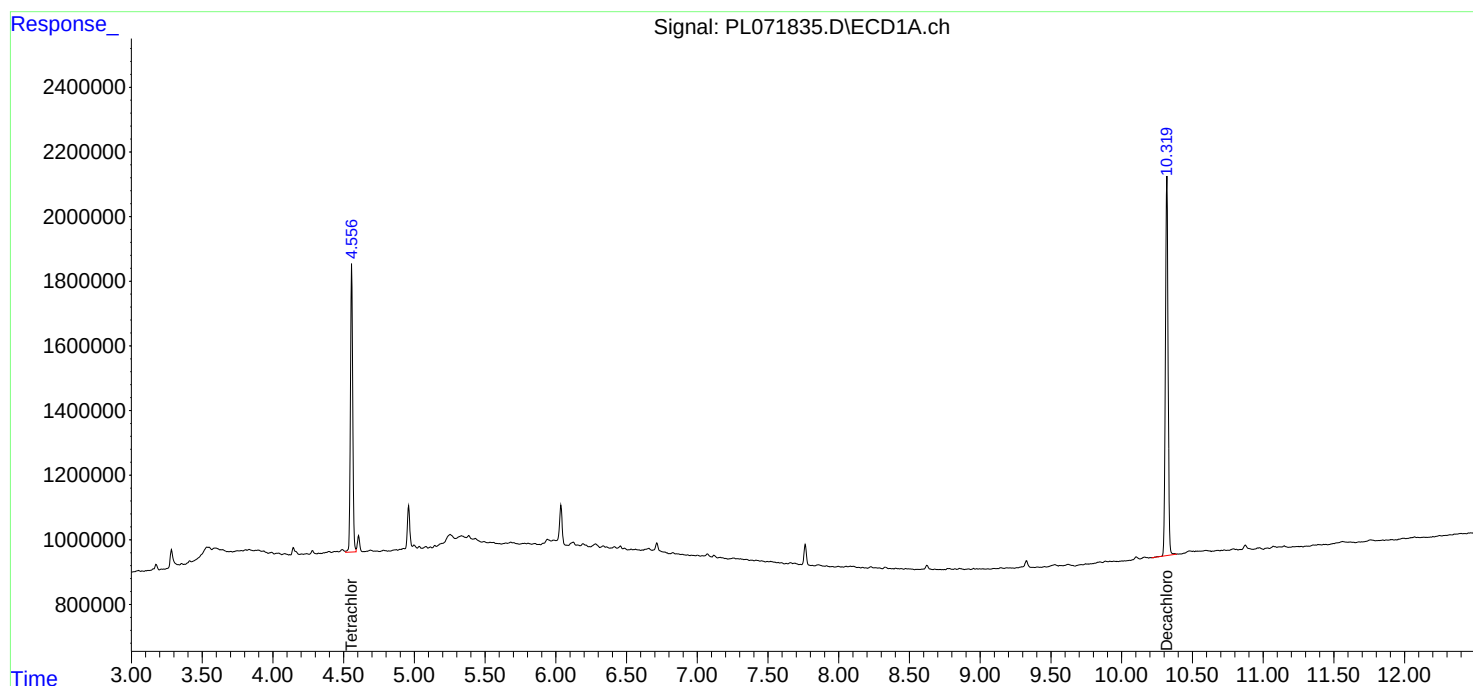


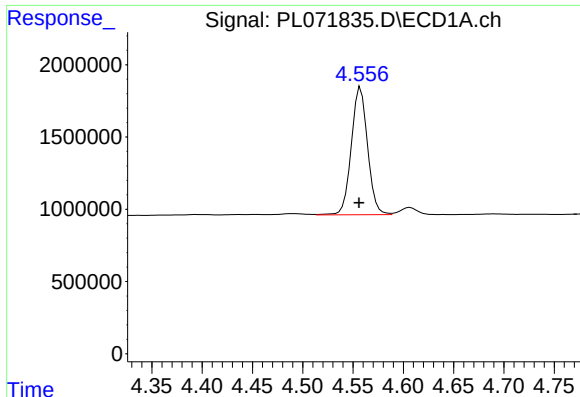

#1 Tetrachloro-m-xylene


R.T.: 4.558 min
Delta R.T.: 0.002 min
Response: 9903439
Conc: 21.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

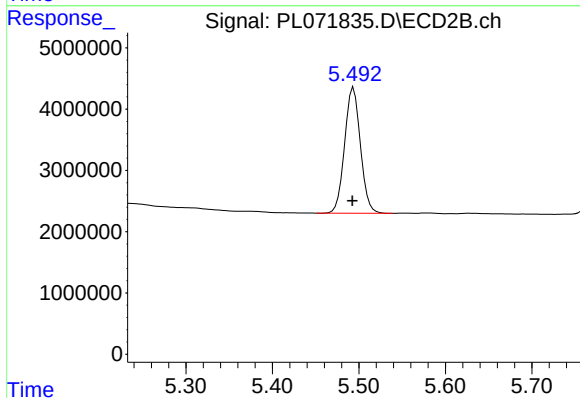


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.001 min
Response: 25869500
Conc: 21.06 ng/ml

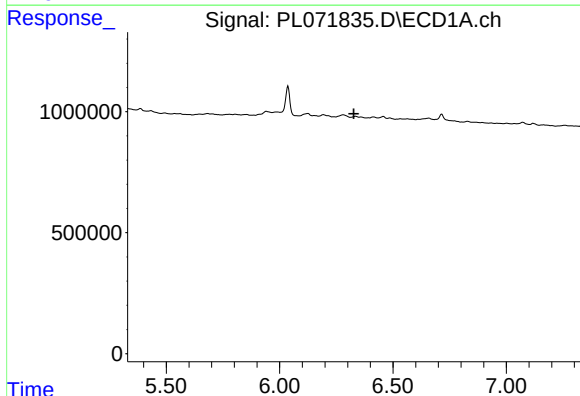


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.327 min
Response: 0
Conc: N.D.

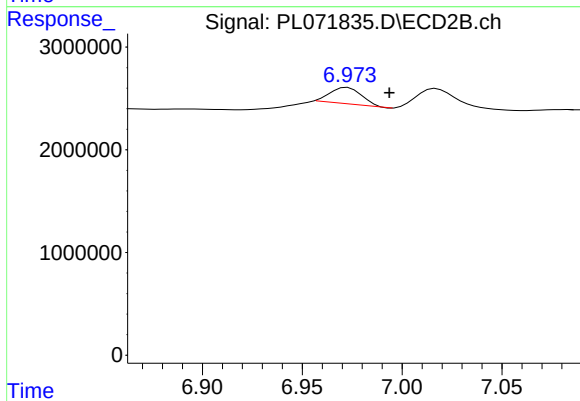

#7 delta-BHC


R.T.: 6.973 min
Delta R.T.: -0.021 min
Response: 1734607
Conc: 1.13 ng/ml

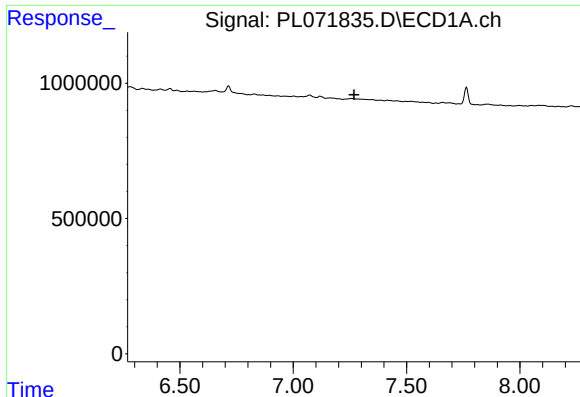

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

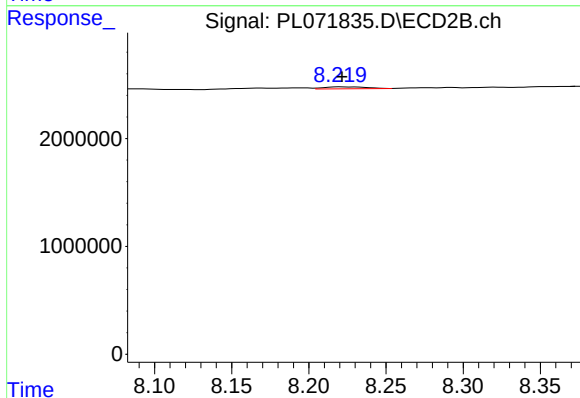


#10 gamma-Chlordane

R.T.: 8.220 min
Delta R.T.: -0.002 min
Response: 325187
Conc: 0.24 ng/ml

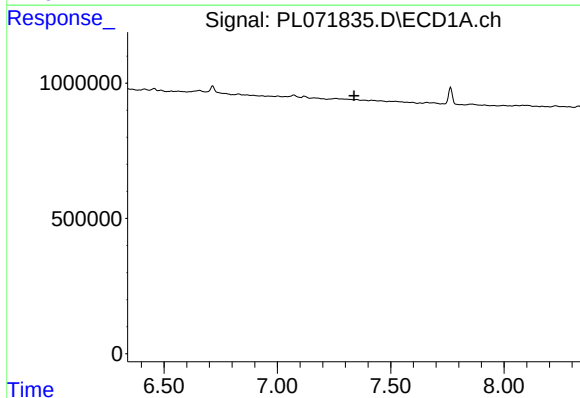


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.338 min
Response: 0
Conc: N.D.

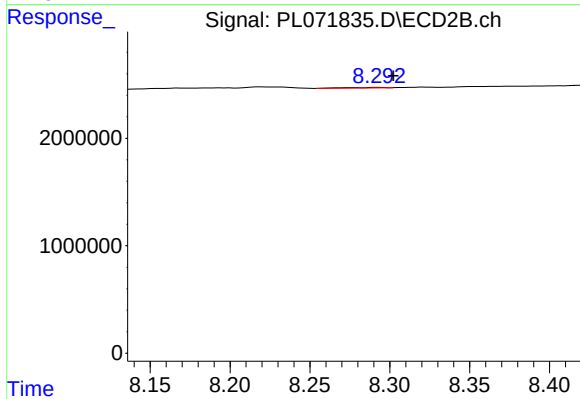

#11 alpha-Chlordane


R.T.: 8.293 min
Delta R.T.: -0.009 min
Response: 78264
Conc: 0.06 ng/ml

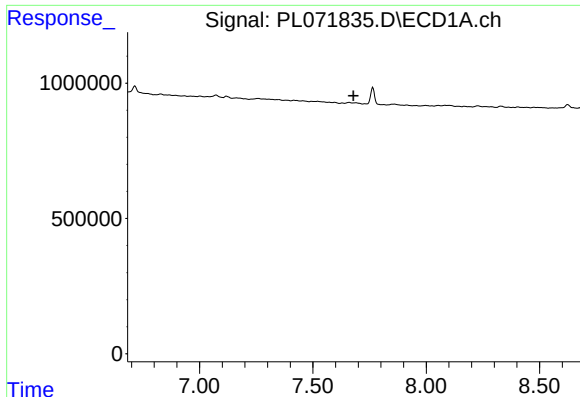

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 7.680 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

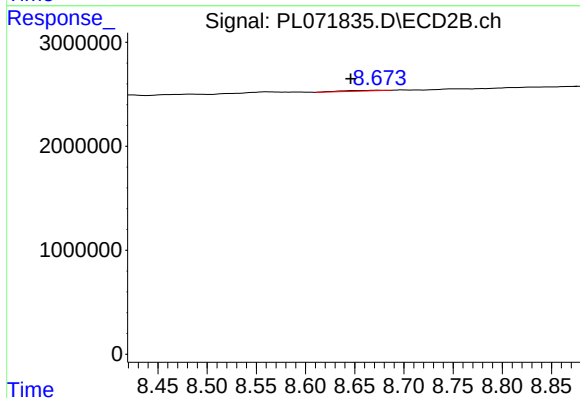


#13 Dieldrin

R.T.: 8.674 min
Delta R.T.: 0.028 min
Response: 180388
Conc: 0.14 ng/ml

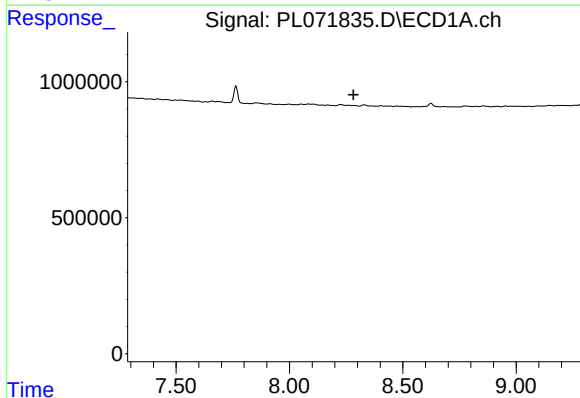


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.283 min
Response: 0
Conc: N.D.

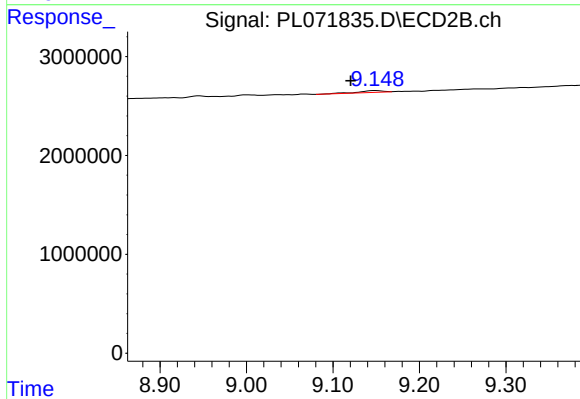

#15 Endosulfan II


R.T.: 9.150 min
Delta R.T.: 0.029 min
Response: 378831
Conc: 0.34 ng/ml

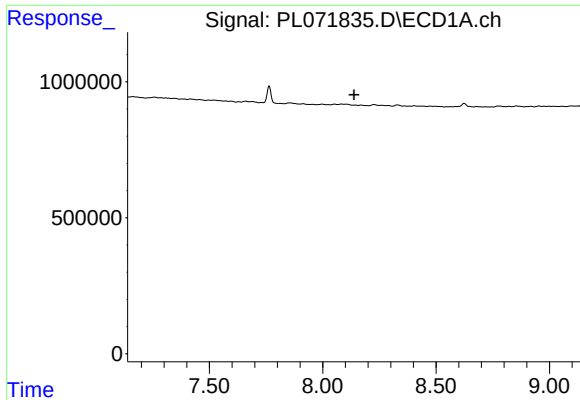

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.139 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

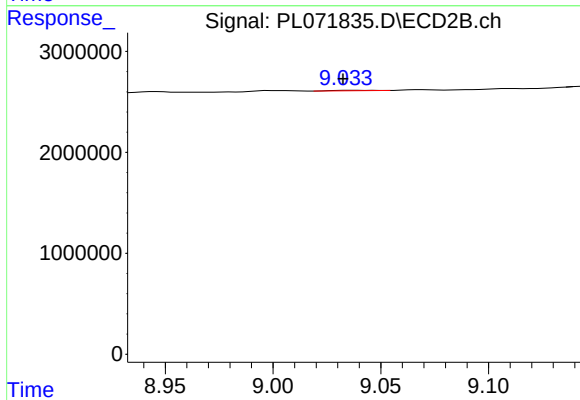


#16 4,4'-DDD

R.T.: 9.036 min
Delta R.T.: 0.003 min
Response: 62922
Conc: 0.07 ng/ml

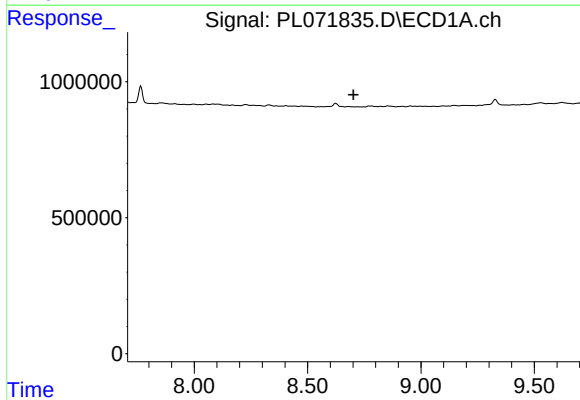


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.703 min
Response: 0
Conc: N.D.

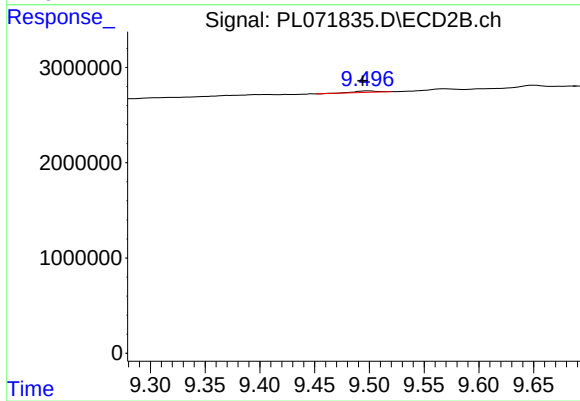

#19 Endosulfan Sulfate


R.T.: 9.499 min
Delta R.T.: 0.005 min
Response: 214084
Conc: 0.21 ng/ml

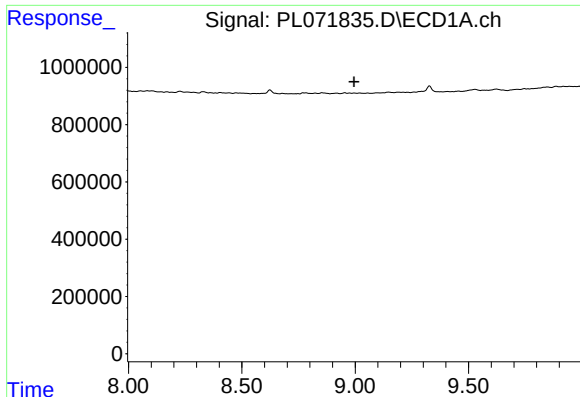

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 8.995 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

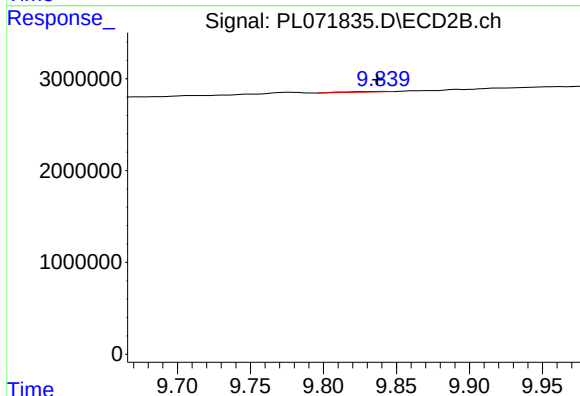


#20 Methoxychlor

R.T.: 9.841 min
Delta R.T.: 0.004 min
Response: 114143
Conc: 0.23 ng/ml

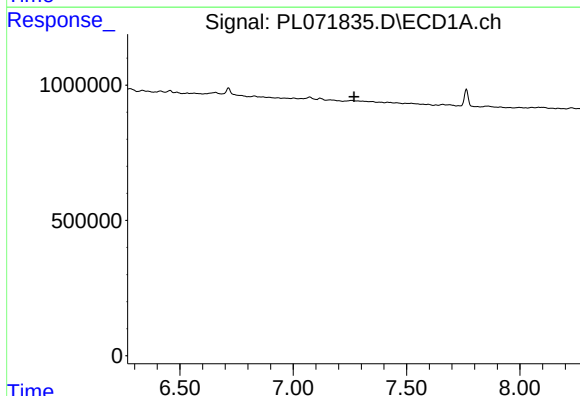


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

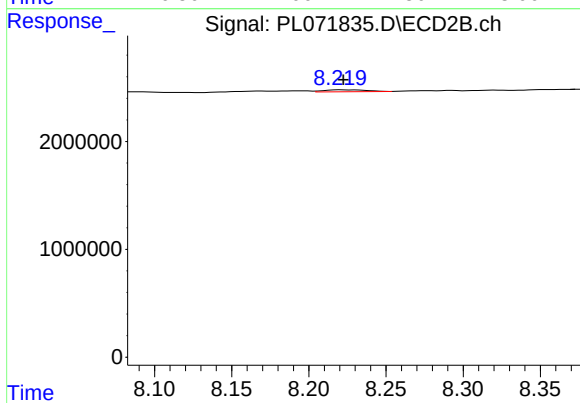

#25 Chlordane-3


R.T.: 8.220 min
Delta R.T.: -0.002 min
Response: 325187
Conc: 1.59 ng/ml

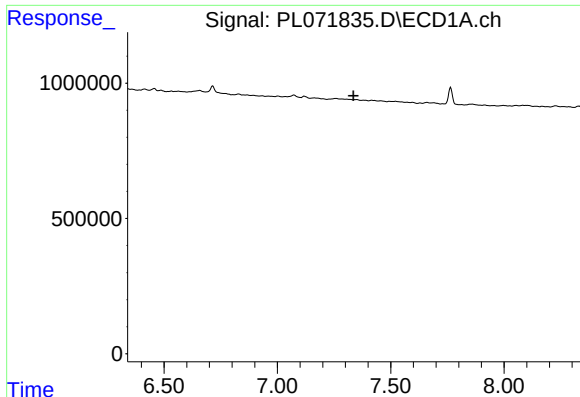

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.336 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

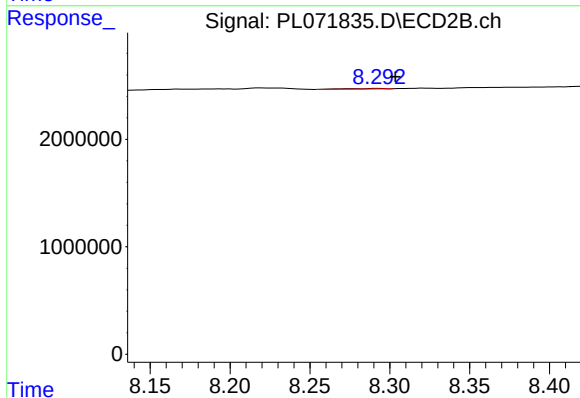


#26 Chlordane-4

R.T.: 8.293 min
Delta R.T.: -0.011 min
Response: 78264
Conc: 0.32 ng/ml

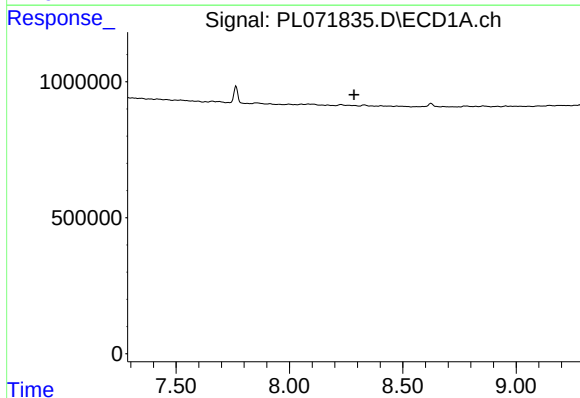


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.286 min
Response: 0
Conc: N.D.

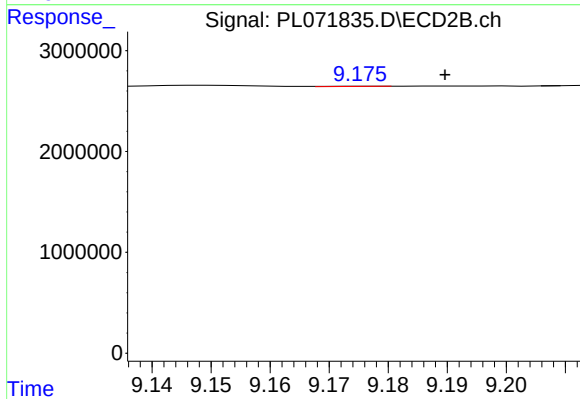

#27 Chlordane-5


R.T.: 9.176 min
Delta R.T.: -0.013 min
Response: 13353
Conc: 0.33 ng/ml

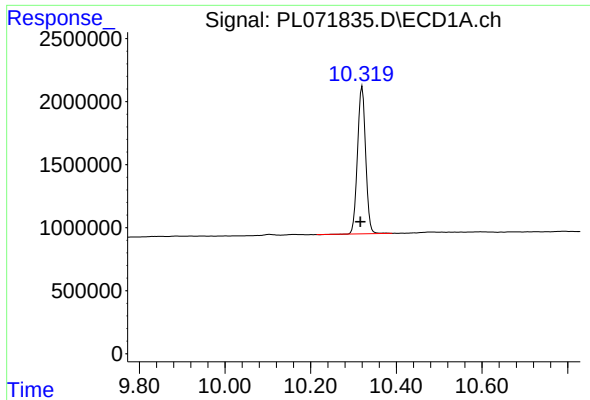

#28 Decachlorobiphenyl

R.T.: 10.320 min
Delta R.T.: 0.004 min
Response: 15570999
Conc: 21.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

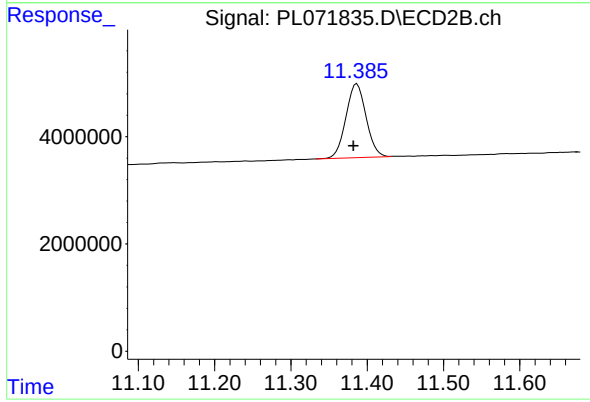

#28 Decachlorobiphenyl

R.T.: 11.387 min
Delta R.T.: 0.005 min
Response: 25320465
Conc: 21.37 ng/ml