

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010622\
 Data File : PL071849.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jan 2022 15:22
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 00:08:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.558	5.494	9126672	25025129	19.757	20.368
28)	SA Decachlor...	10.322	11.389	14851293	24268050	20.540	20.479
Target Compounds							
6)	B beta-BHC	0.000	6.736	0	51676	N.D.	0.072 #
7)	B delta-BHC	0.000	6.974f	0	590483	N.D.	0.385 #
9)	A Endosulfan I	0.000	8.365	0	24100	N.D.	0.019 #
10)	B gamma-Chl...	0.000	8.236	0	235775	N.D.	0.172 #
15)	B Endosulfa...	0.000	9.147f	0	471815	N.D.	0.420 #
16)	A 4,4'-DDD	0.000	9.005f	0	22014	N.D.	0.023 #
17)	MA 4,4'-DDT	0.000	9.330f	0	43243	N.D.	0.046 #
19)	B Endosulfa...	0.000	9.501	0	79249	N.D.	0.076 #
25)	Chlordane-3	0.000	8.236	0	235775	N.D.	1.155 #
27)	Chlordane-5	0.000	9.188	0	85830	N.D.	2.143 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010622\
Data File : PL071849.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jan 2022 15:22
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 00:08:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

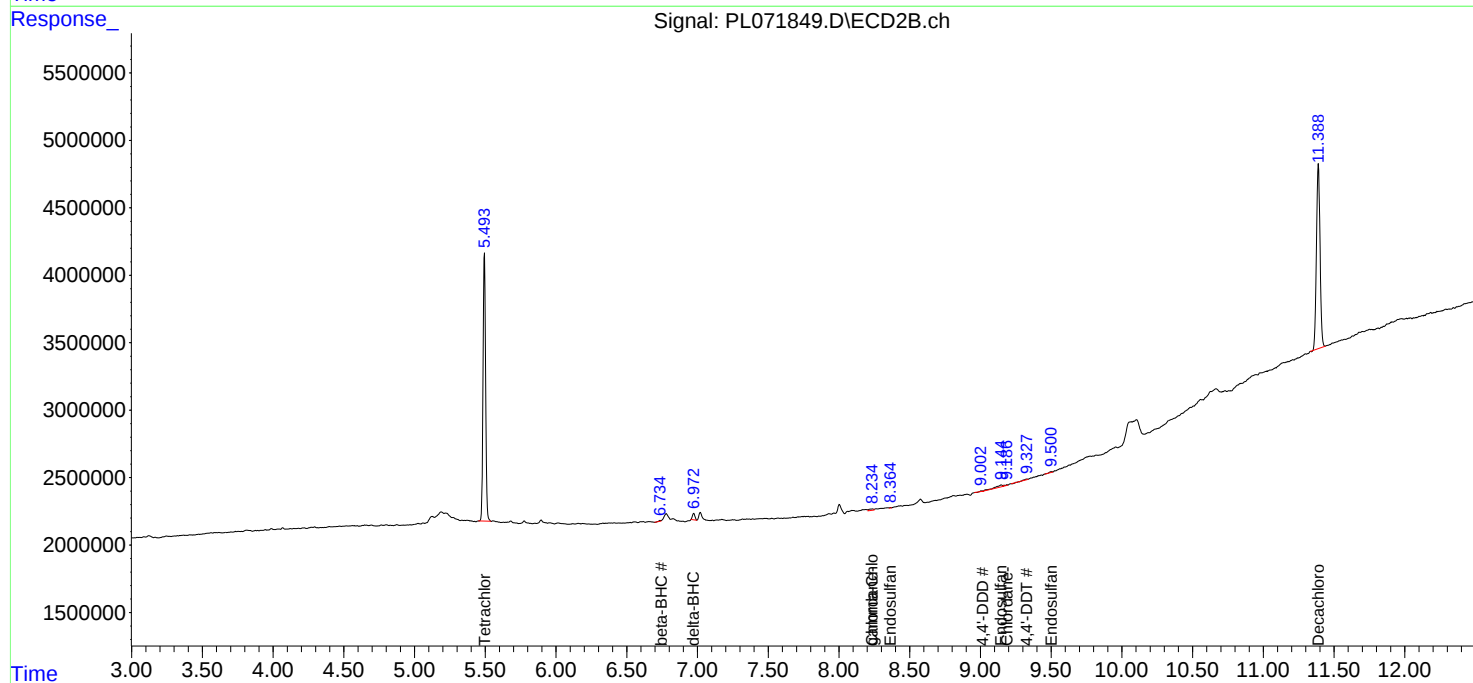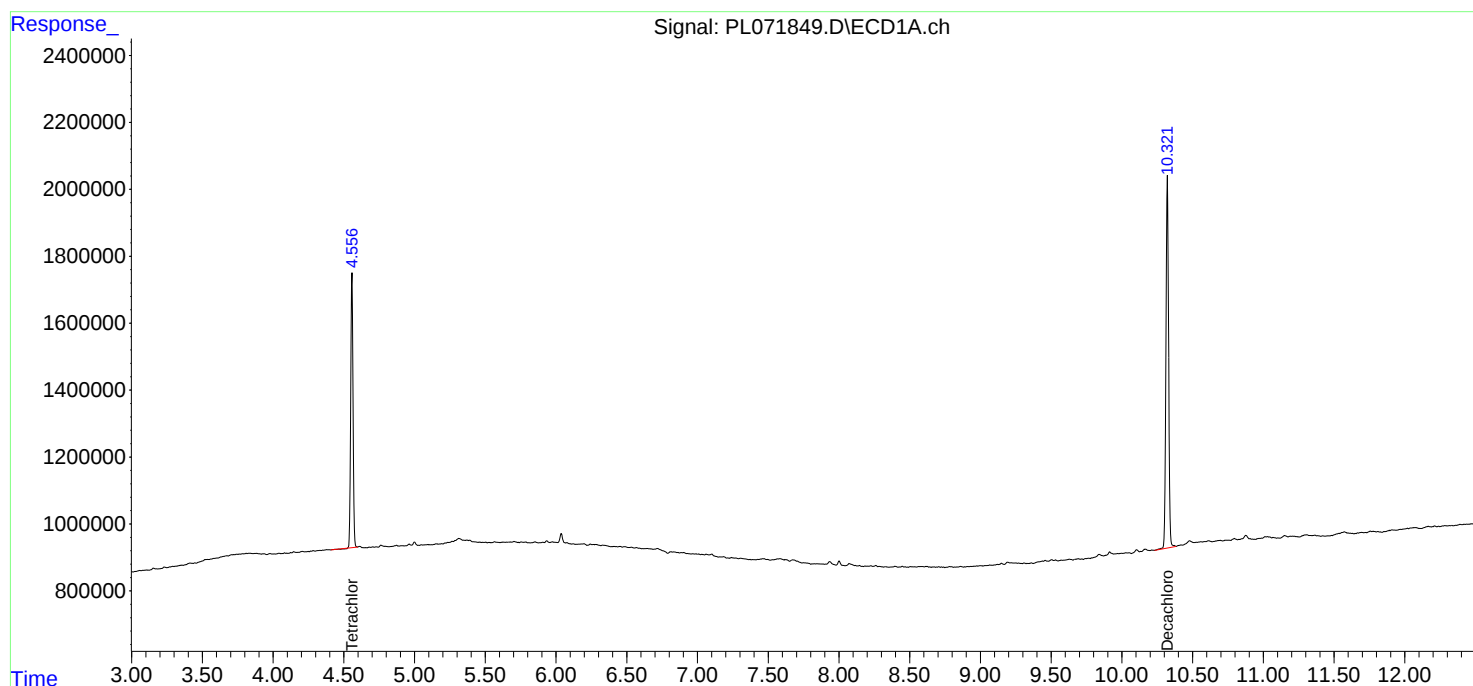


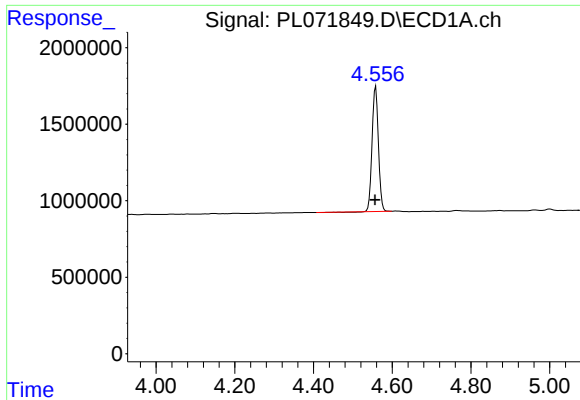

#1 Tetrachloro-m-xylene


R.T.: 4.558 min
Delta R.T.: 0.002 min
Response: 9126672
Conc: 19.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

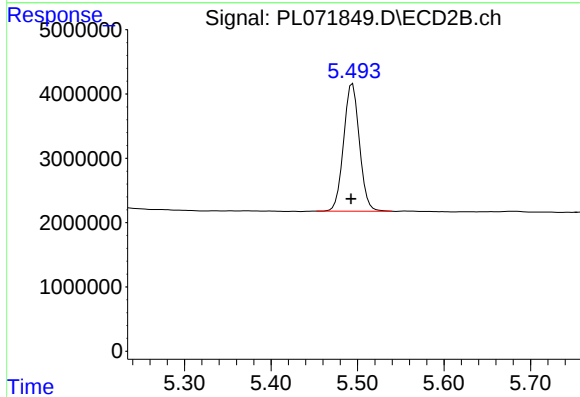


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.002 min
Response: 25025129
Conc: 20.37 ng/ml

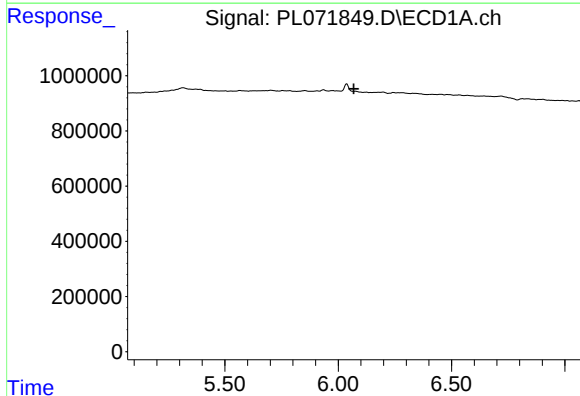


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.069 min
Response: 0
Conc: N.D.

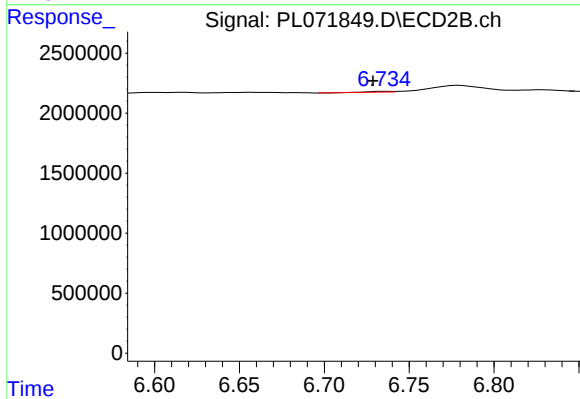

#6 beta-BHC


R.T.: 6.736 min
Delta R.T.: 0.007 min
Response: 51676
Conc: 0.07 ng/ml

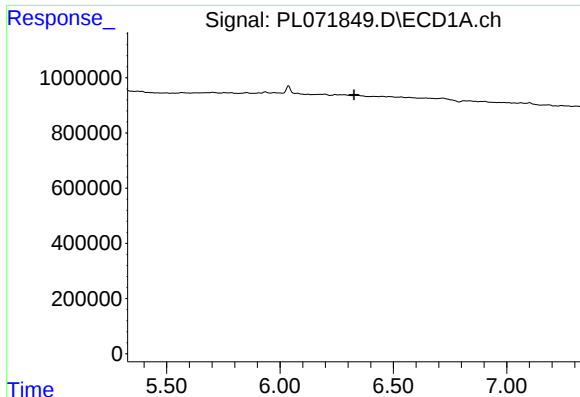

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.327 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

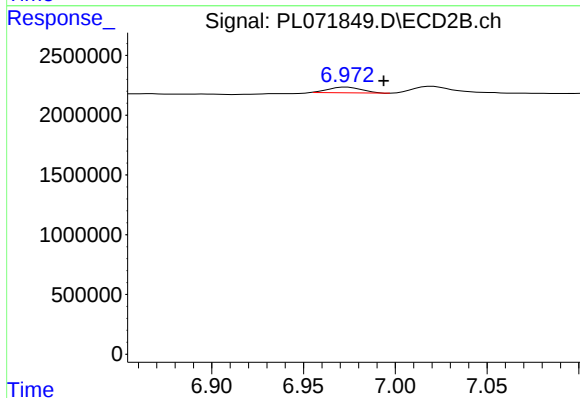


#7 delta-BHC

R.T.: 6.974 min
Delta R.T.: -0.020 min
Response: 590483
Conc: 0.38 ng/ml

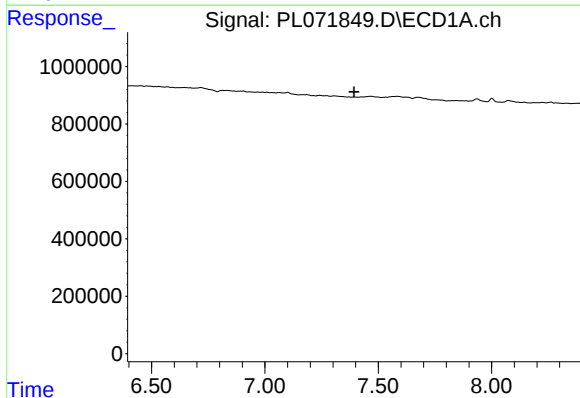


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.393 min
Response: 0
Conc: N.D.

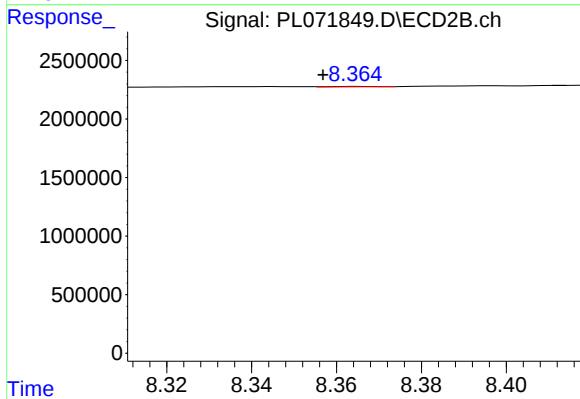

#9 Endosulfan I


R.T.: 8.365 min
Delta R.T.: 0.008 min
Response: 24100
Conc: 0.02 ng/ml

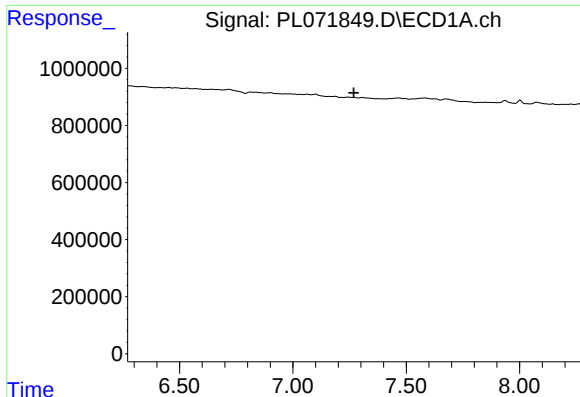

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

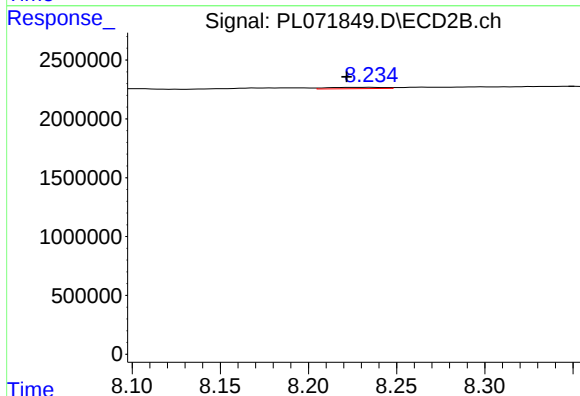


#10 gamma-Chlordane

R.T.: 8.236 min
Delta R.T.: 0.015 min
Response: 235775
Conc: 0.17 ng/ml

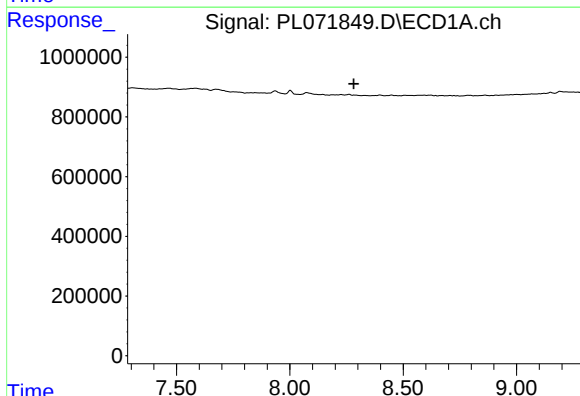


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.283 min
Response: 0
Conc: N.D.

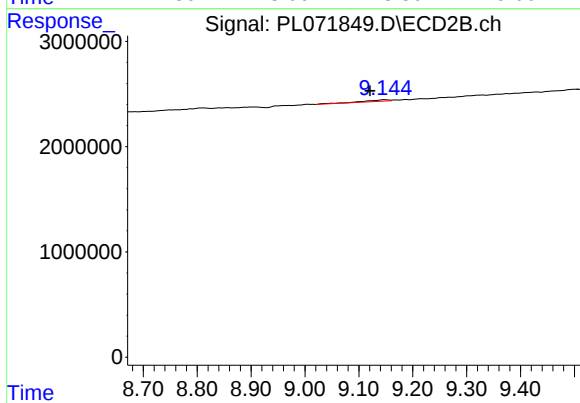

#15 Endosulfan II


R.T.: 9.147 min
Delta R.T.: 0.026 min
Response: 471815
Conc: 0.42 ng/ml

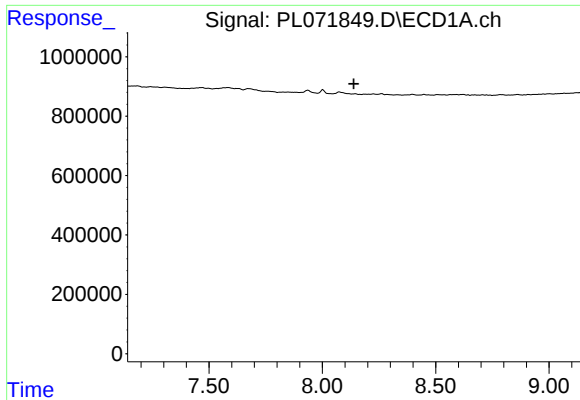

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.139 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

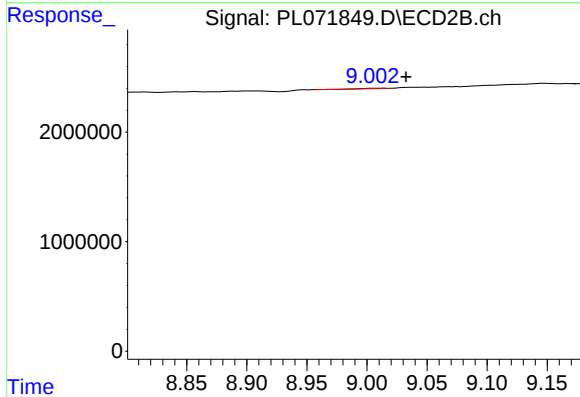


#16 4,4'-DDD

R.T.: 9.005 min
Delta R.T.: -0.027 min
Response: 22014
Conc: 0.02 ng/ml

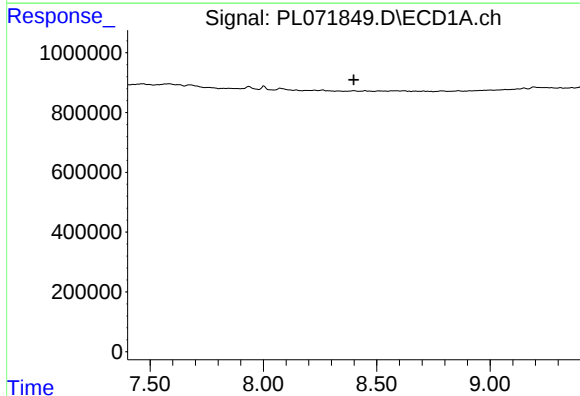


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

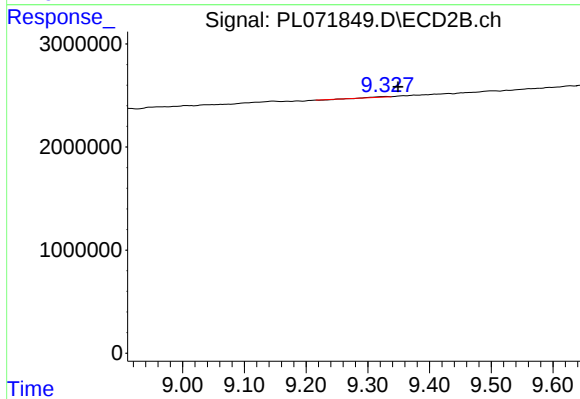

#17 4,4'-DDT


R.T.: 9.330 min
Delta R.T.: -0.019 min
Response: 43243
Conc: 0.05 ng/ml

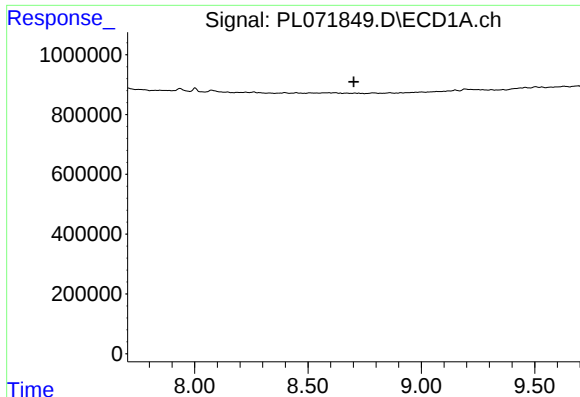

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 8.703 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

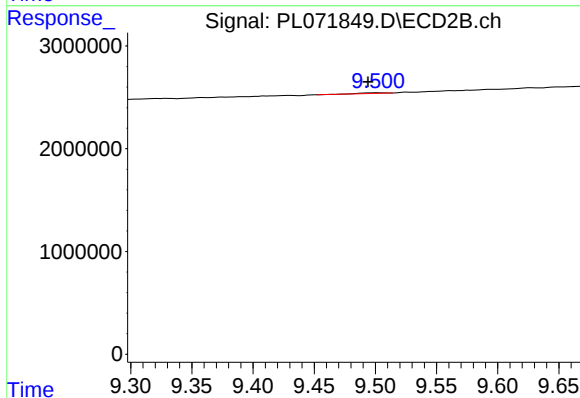


#19 Endosulfan Sulfate

R.T.: 9.501 min
Delta R.T.: 0.008 min
Response: 79249
Conc: 0.08 ng/ml

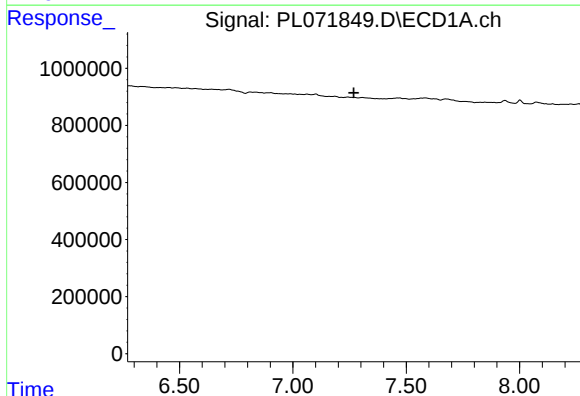


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

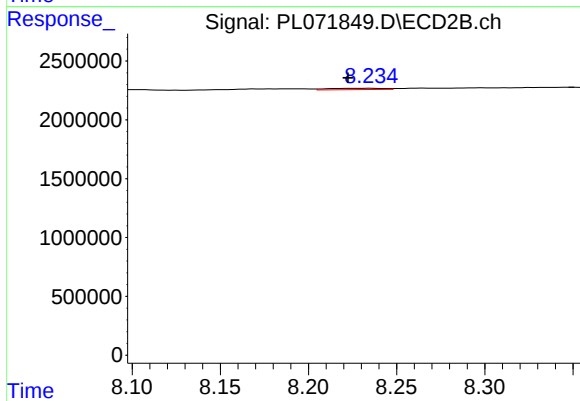

#25 Chlordane-3


R.T.: 8.236 min
Delta R.T.: 0.014 min
Response: 235775
Conc: 1.16 ng/ml

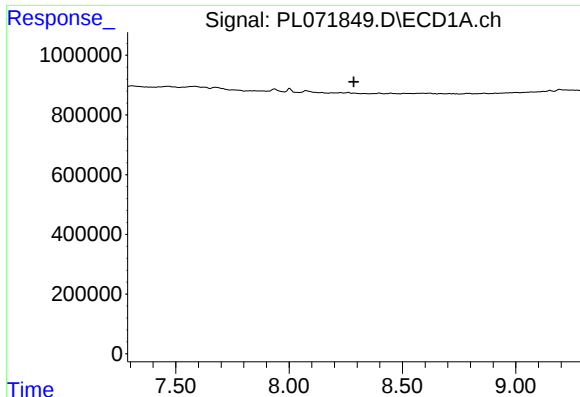

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.286 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

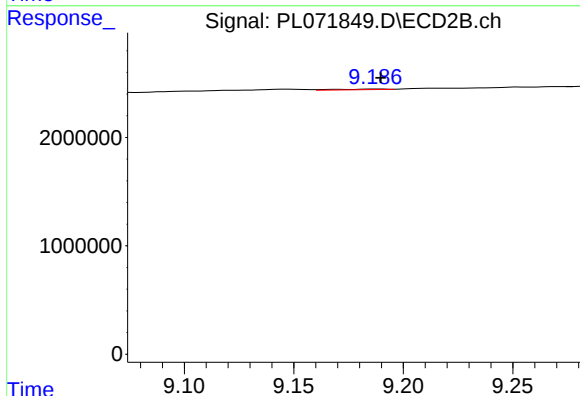


#27 Chlordane-5

R.T.: 9.188 min
Delta R.T.: -0.002 min
Response: 85830
Conc: 2.14 ng/ml

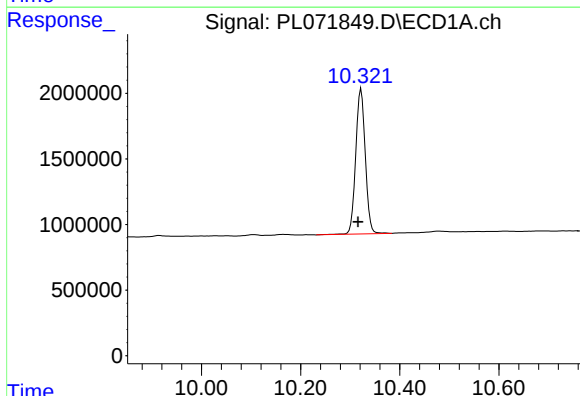

#28 Decachlorobiphenyl

R.T.: 10.322 min
Delta R.T.: 0.006 min
Response: 14851293
Conc: 20.54 ng/ml

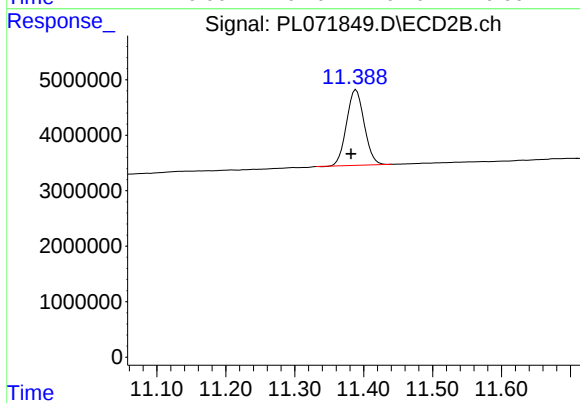

#28 Decachlorobiphenyl

R.T.: 11.389 min
Delta R.T.: 0.007 min
Response: 24268050
Conc: 20.48 ng/ml