

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010622\
 Data File : PL071855.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jan 2022 17:20
 Operator : AR\AJ
 Sample : N1047-05
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 00:09:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.558	5.494	10550503	28882562	22.839	23.508
28)	SA Decachlor...	10.322	11.388	12385050	20682241	17.129	17.453
Target Compounds							
5)	MB Aldrin	0.000	7.461f	0	389232	N.D.	0.253 #
7)	B delta-BHC	0.000	6.972f	0	495600	N.D.	0.323 #
9)	A Endosulfan I	0.000	8.328f	0	24829	N.D.	0.020 #
10)	B gamma-Chl...	0.000	8.227	0	169343	N.D.	0.124 #
11)	B alpha-Chl...	0.000	8.303	0	34243	N.D.	0.026 #
13)	MA Dieldrin	0.000	8.671f	0	69267	N.D.	0.053 #
15)	B Endosulfa...	0.000	9.148f	0	339203	N.D.	0.302 #
19)	B Endosulfa...	0.000	9.500	0	123119	N.D.	0.119 #
21)	B Endrin ke...	0.000	9.975	0	43919	N.D.	0.039 #
24)	Chlordane-2	0.000	7.461	0	389232	N.D.	7.191 #
25)	Chlordane-3	0.000	8.227	0	169343	N.D.	0.830 #
26)	Chlordane-4	0.000	8.303	0	34243	N.D.	0.141 #
27)	Chlordane-5	0.000	9.199	0	23604	N.D.	0.589 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010622\
Data File : PL071855.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jan 2022 17:20
Operator : AR\AJ
Sample : N1047-05
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 00:09:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

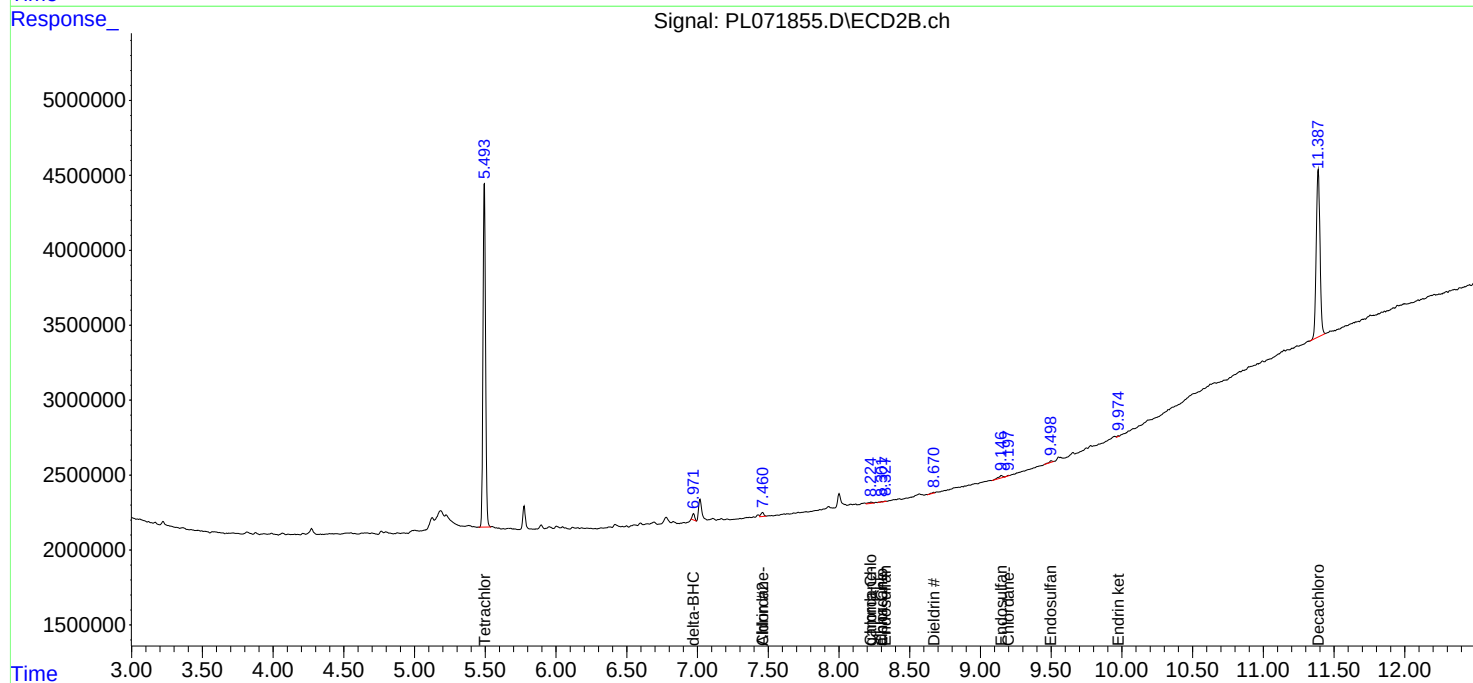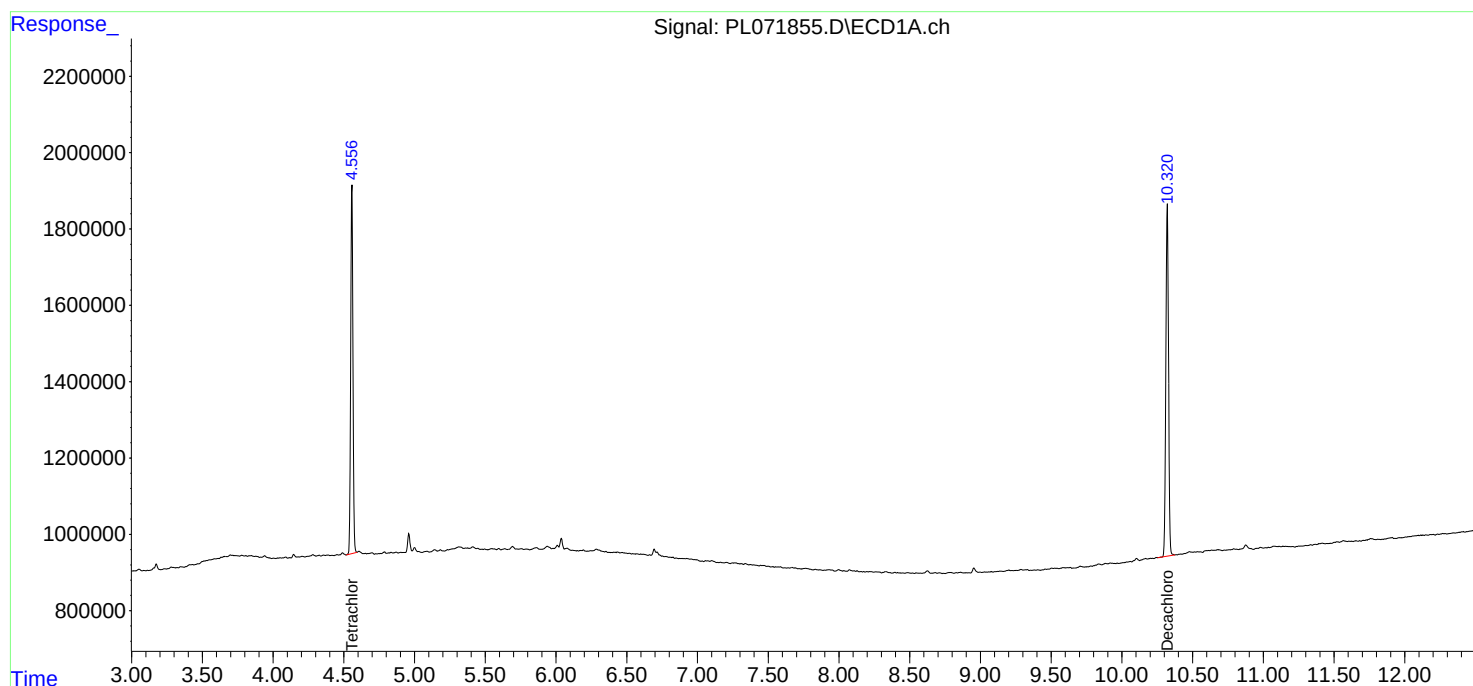


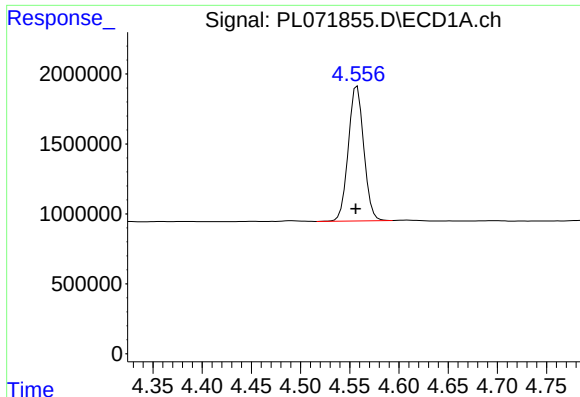

#1 Tetrachloro-m-xylene


R.T.: 4.558 min
Delta R.T.: 0.002 min
Response: 10550503
Conc: 22.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

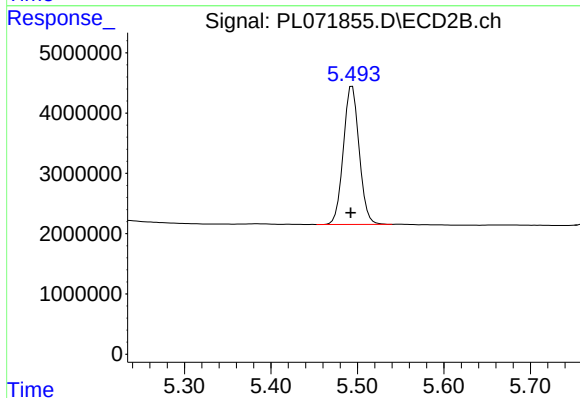


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.002 min
Response: 28882562
Conc: 23.51 ng/ml

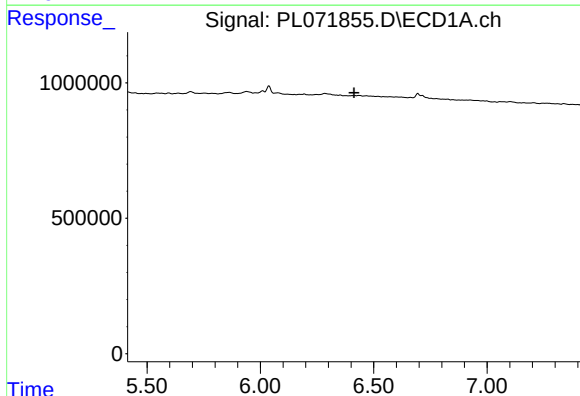


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 6.414 min
Response: 0
Conc: N.D.

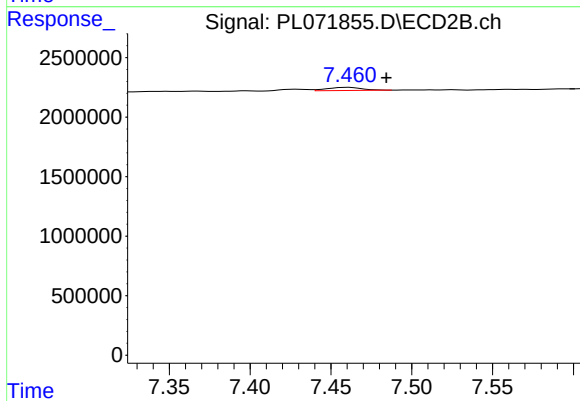

#5 Aldrin


R.T.: 7.461 min
Delta R.T.: -0.023 min
Response: 389232
Conc: 0.25 ng/ml

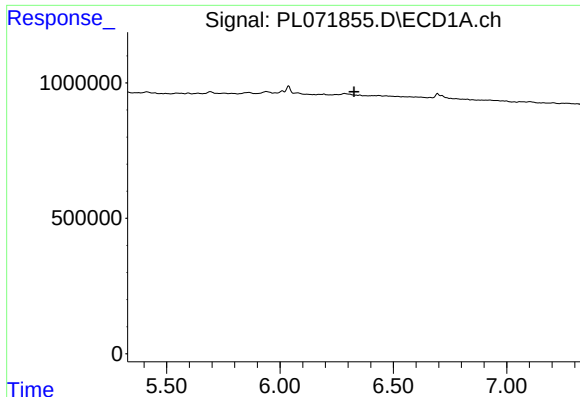

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.327 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

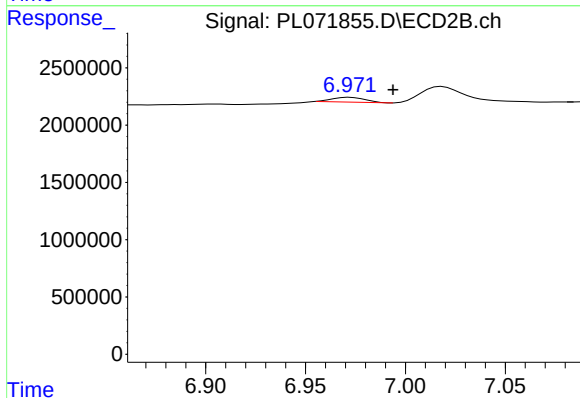


#7 delta-BHC

R.T.: 6.972 min
Delta R.T.: -0.022 min
Response: 495600
Conc: 0.32 ng/ml

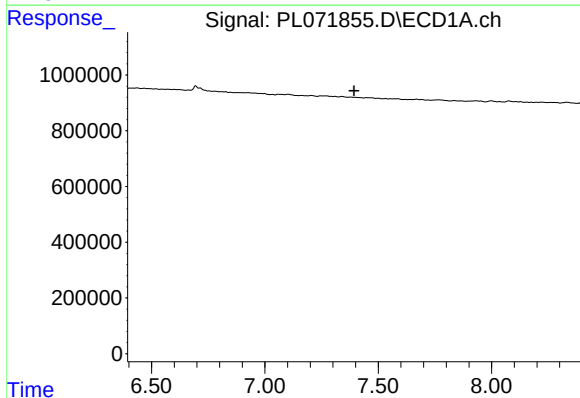


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.393 min
Response: 0
Conc: N.D.

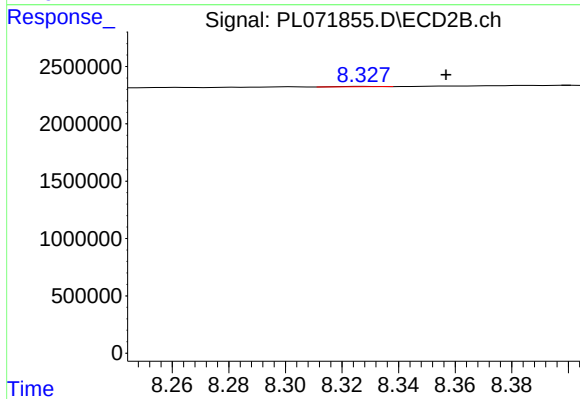

#9 Endosulfan I


R.T.: 8.328 min
Delta R.T.: -0.029 min
Response: 24829
Conc: 0.02 ng/ml

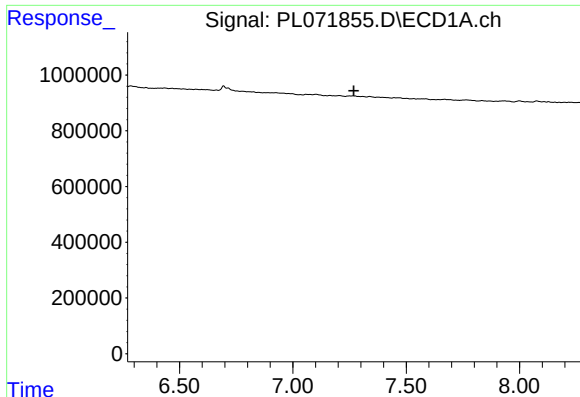

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

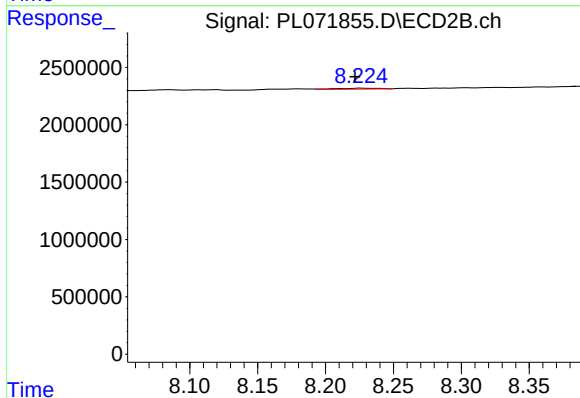


#10 gamma-Chlordane

R.T.: 8.227 min
Delta R.T.: 0.005 min
Response: 169343
Conc: 0.12 ng/ml

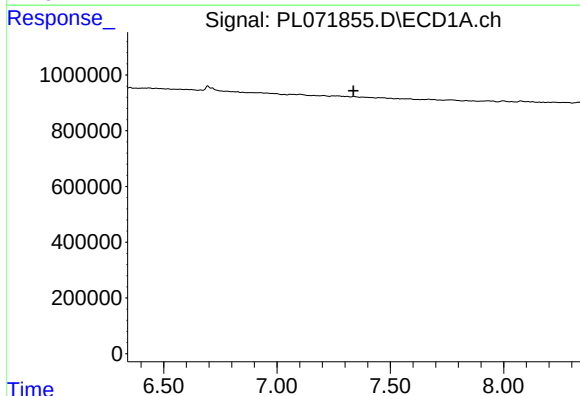


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.338 min
Response: 0
Conc: N.D.

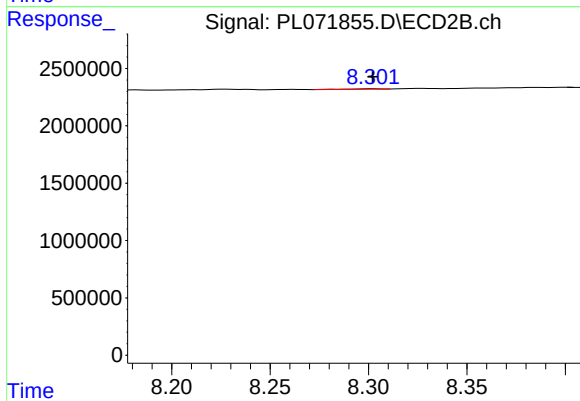

#11 alpha-Chlordane


R.T.: 8.303 min
Delta R.T.: 0.001 min
Response: 34243
Conc: 0.03 ng/ml

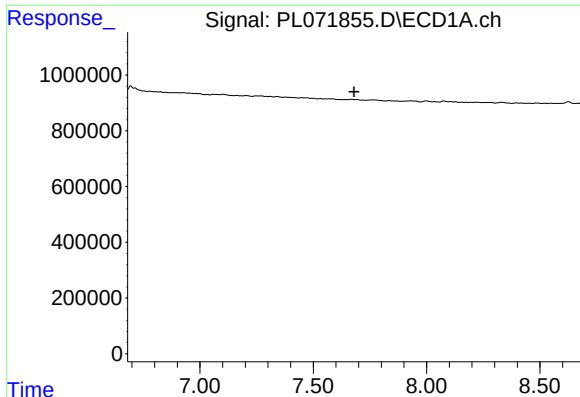

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 7.680 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

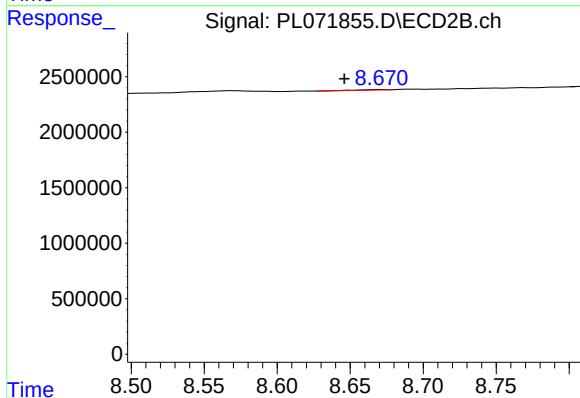


#13 Dieldrin

R.T.: 8.671 min
Delta R.T.: 0.025 min
Response: 69267
Conc: 0.05 ng/ml

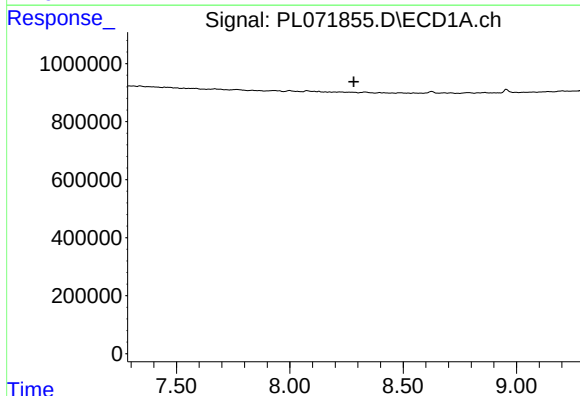


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.283 min
Response: 0
Conc: N.D.

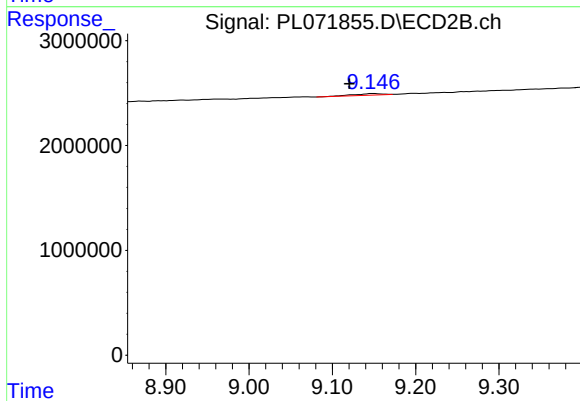

#15 Endosulfan II


R.T.: 9.148 min
Delta R.T.: 0.027 min
Response: 339203
Conc: 0.30 ng/ml

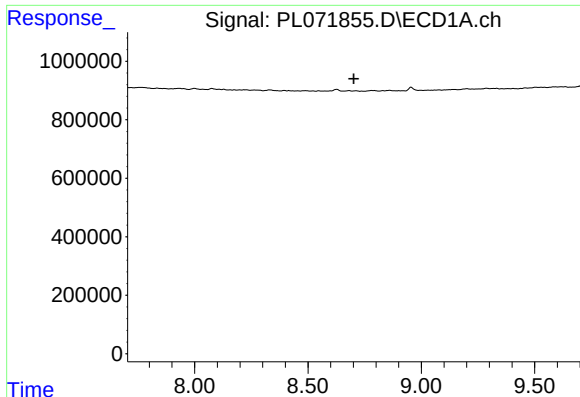

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 8.703 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

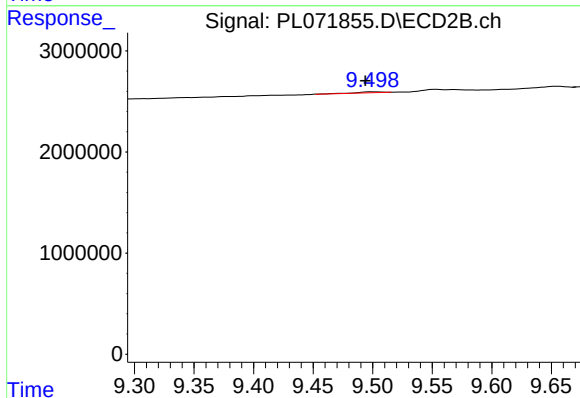


#19 Endosulfan Sulfate

R.T.: 9.500 min
Delta R.T.: 0.006 min
Response: 123119
Conc: 0.12 ng/ml

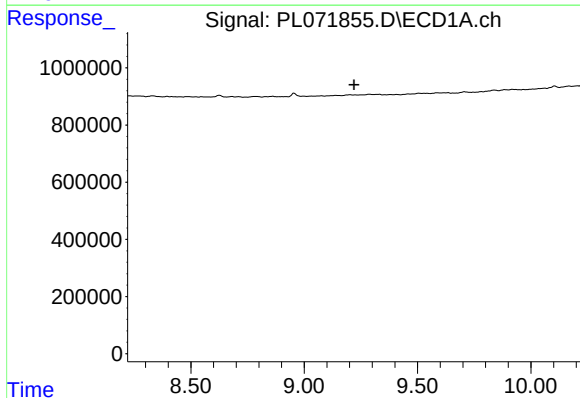


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.220 min
Response: 0
Conc: N.D.

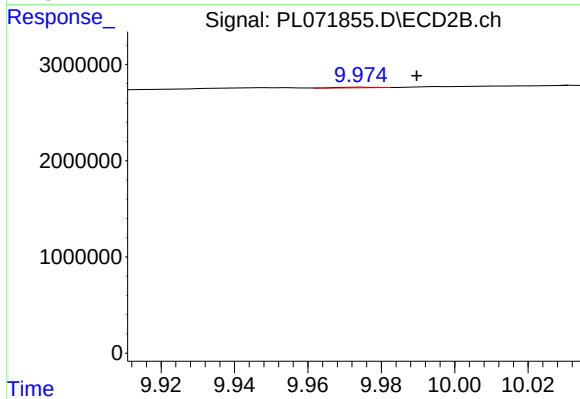

#21 Endrin ketone


R.T.: 9.975 min
Delta R.T.: -0.015 min
Response: 43919
Conc: 0.04 ng/ml

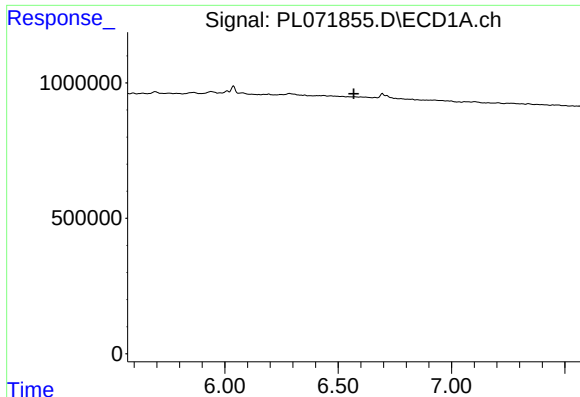

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 6.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

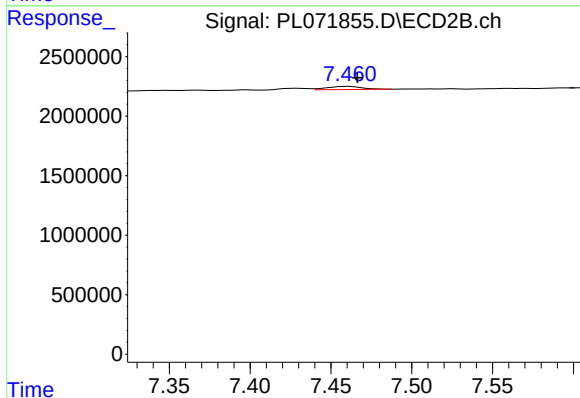


#24 Chlordane-2

R.T.: 7.461 min
Delta R.T.: -0.005 min
Response: 389232
Conc: 7.19 ng/ml

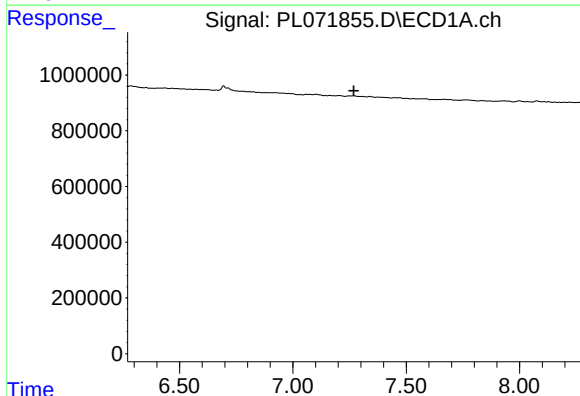


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

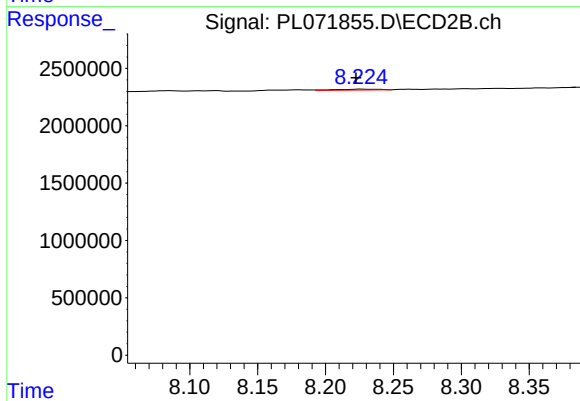

#25 Chlordane-3


R.T.: 8.227 min
Delta R.T.: 0.004 min
Response: 169343
Conc: 0.83 ng/ml

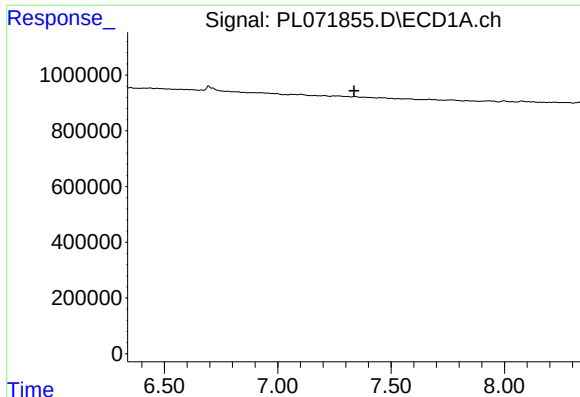

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.336 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

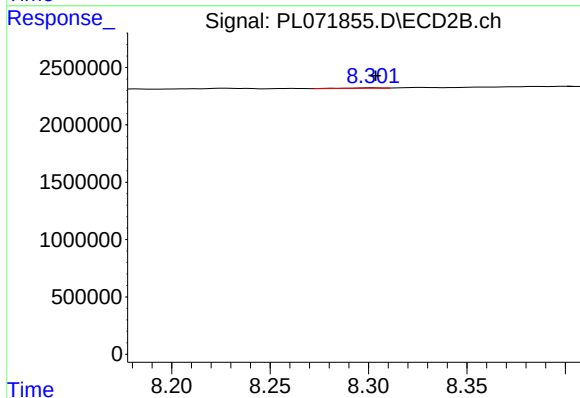


#26 Chlordane-4

R.T.: 8.303 min
Delta R.T.: 0.000 min
Response: 34243
Conc: 0.14 ng/ml

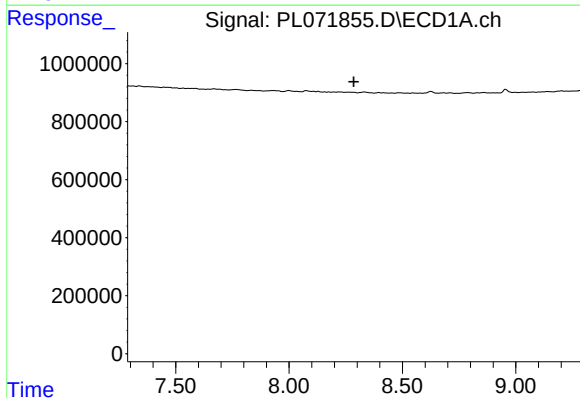


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.286 min
Response: 0
Conc: N.D.

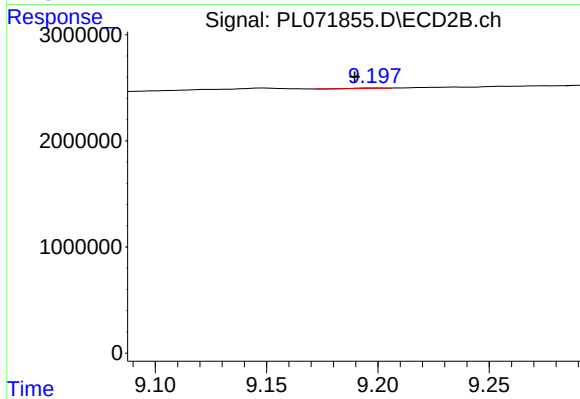

#27 Chlordane-5


R.T.: 9.199 min
Delta R.T.: 0.009 min
Response: 23604
Conc: 0.59 ng/ml

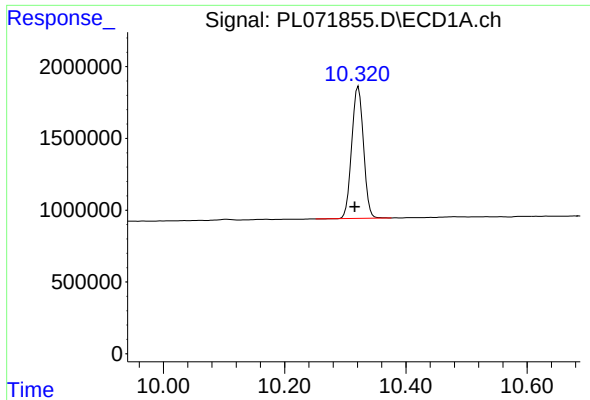

#28 Decachlorobiphenyl

R.T.: 10.322 min
Delta R.T.: 0.006 min
Response: 12385050
Conc: 17.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

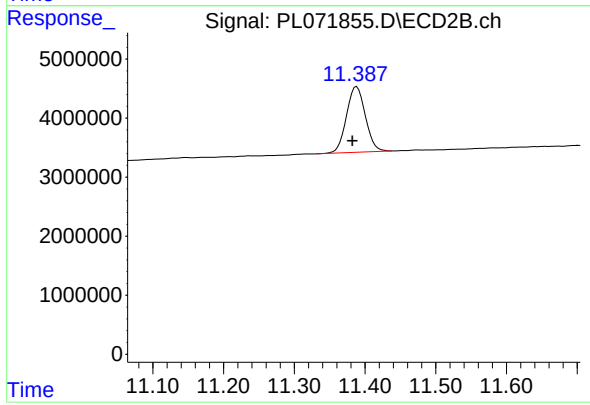

#28 Decachlorobiphenyl

R.T.: 11.388 min
Delta R.T.: 0.006 min
Response: 20682241
Conc: 17.45 ng/ml